

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112918\
 Data File : PL042617.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2018 21:14
 Operator : AJ\SJ
 Sample : J5767-20
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 00:01:30 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.102	107.4E6	56370370	18.254	19.599
28)	SA Decachlor...	8.204	9.233	105.5E6	41869586	16.740	17.360
Target Compounds							
3)	MA gamma-BHC...	4.197	4.824f	3875849	2980674	0.470	0.754 #
6)	B beta-BHC	4.401f	4.906f	10082477	1086141	2.846	0.688 #
8)	B Heptachlo...	0.000	5.997	0	2333837	N.D.	0.651 #
15)	B Endosulfa...	6.298	0.000	2715671	0	0.434	N.D. #
23)	Chlordane-1	4.349	0.000	5476776	0	19.809	N.D. #
27)	Chlordane-5	6.298	0.000	2715671	0	9.114	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112918\
Data File : PL042617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2018 21:14
Operator : AJ\SJ
Sample : J5767-20
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 00:01:30 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

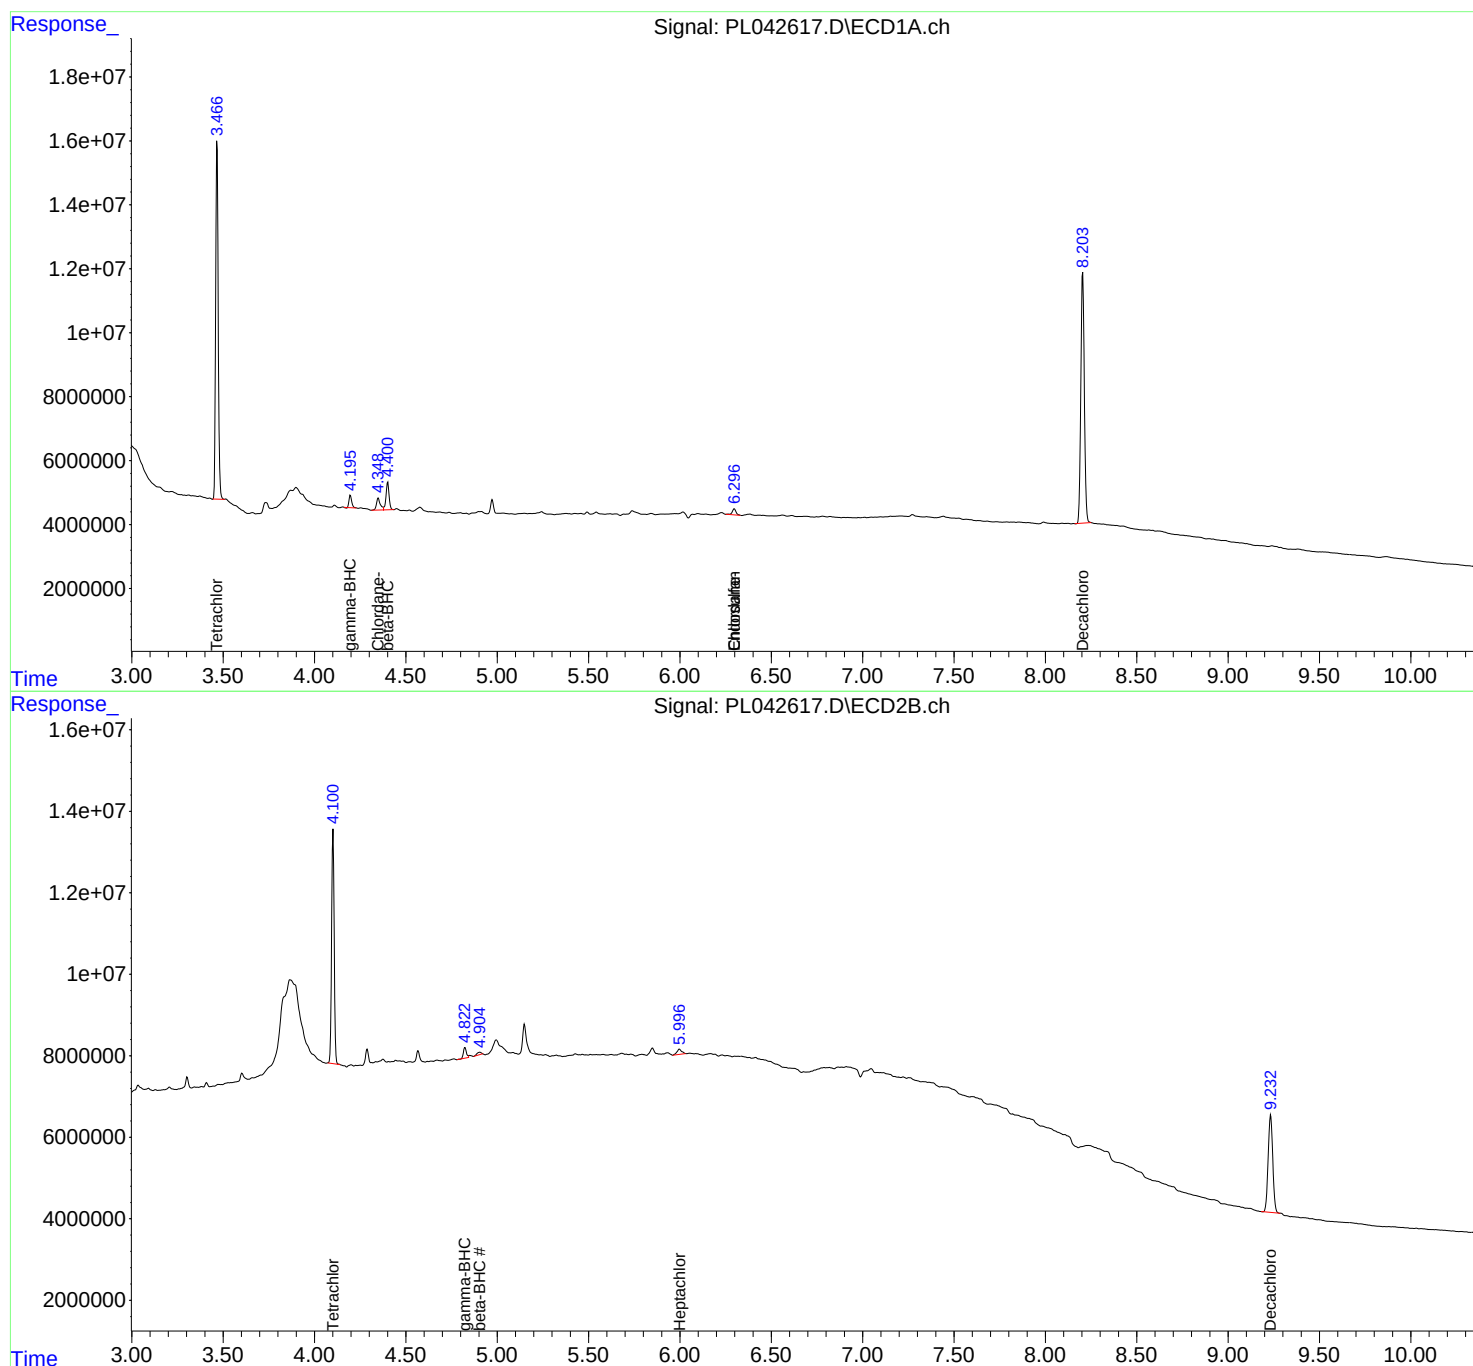


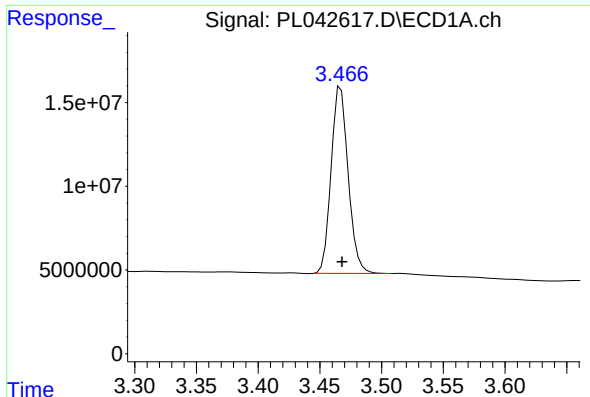

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: -0.001 min
Response: 107398871
Conc: 18.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

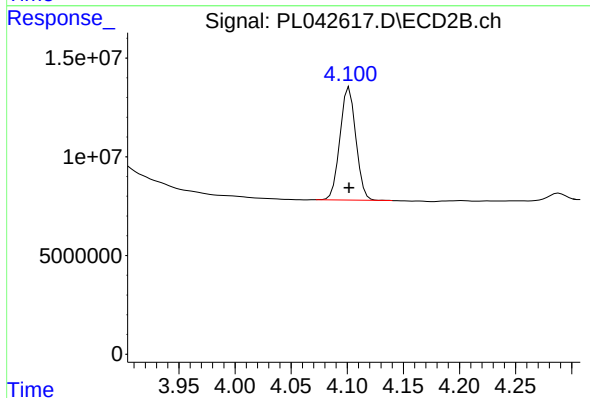


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 56370370
Conc: 19.60 ng/ml

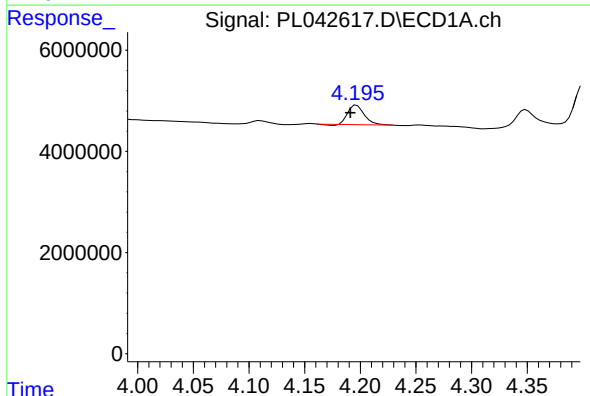


#3 gamma-BHC (Lindane)

R.T.: 4.197 min
Delta R.T.: 0.006 min
Response: 3875849
Conc: 0.47 ng/ml

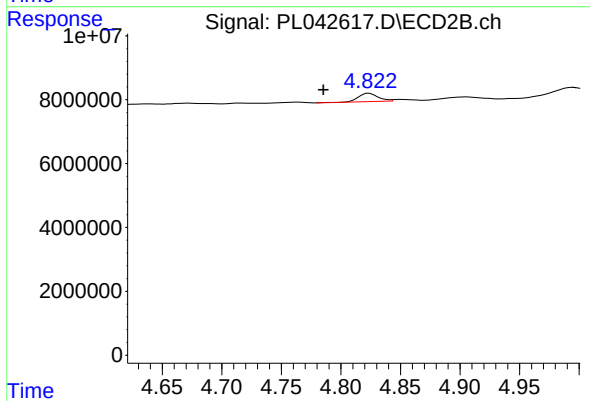

#3 gamma-BHC (Lindane)


R.T.: 4.824 min
Delta R.T.: 0.039 min
Response: 2980674
Conc: 0.75 ng/ml

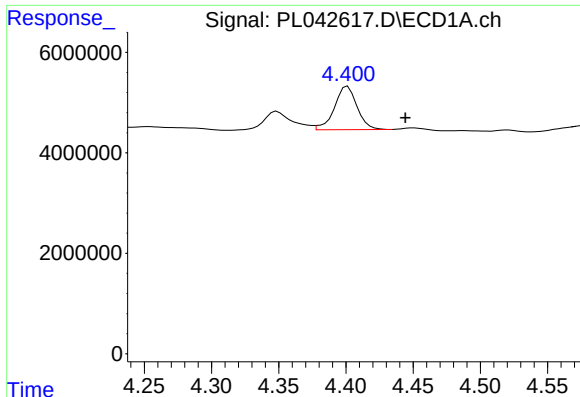

#6 beta-BHC


R.T.: 4.401 min
Delta R.T.: -0.043 min
Response: 10082477
Conc: 2.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

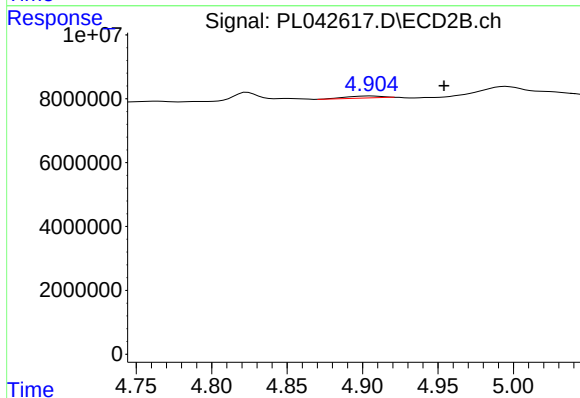


#6 beta-BHC

R.T.: 4.906 min
Delta R.T.: -0.048 min
Response: 1086141
Conc: 0.69 ng/ml

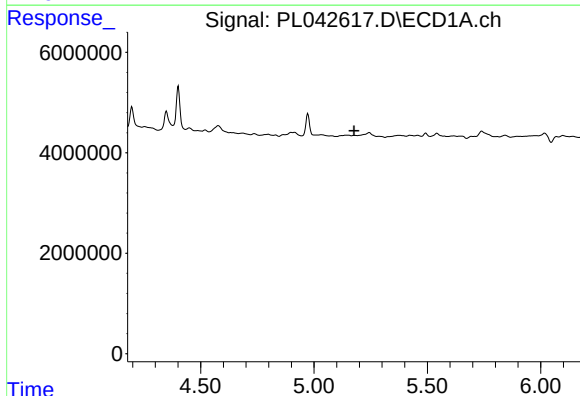


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.177 min
Response: 0
Conc: N.D.

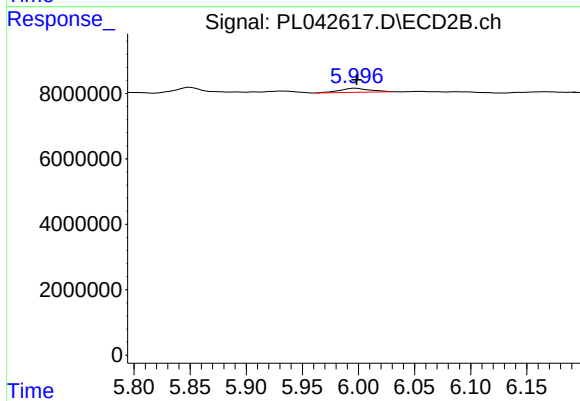

#8 Heptachlor epoxide


R.T.: 5.997 min
Delta R.T.: 0.000 min
Response: 2333837
Conc: 0.65 ng/ml

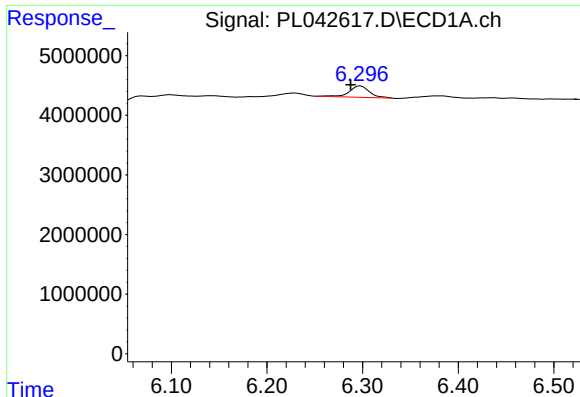

#15 Endosulfan II


R.T.: 6.298 min
Delta R.T.: 0.010 min
Response: 2715671
Conc: 0.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

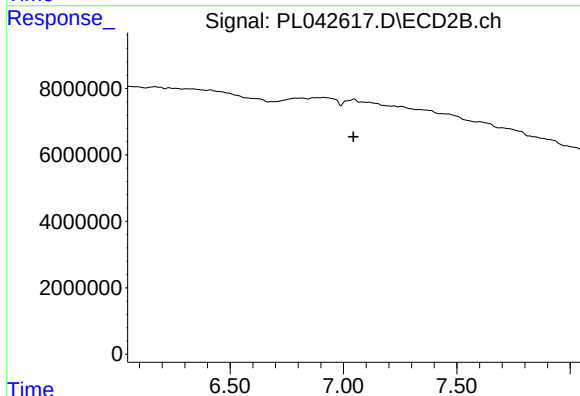


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.044 min
Response: 0
Conc: N.D.

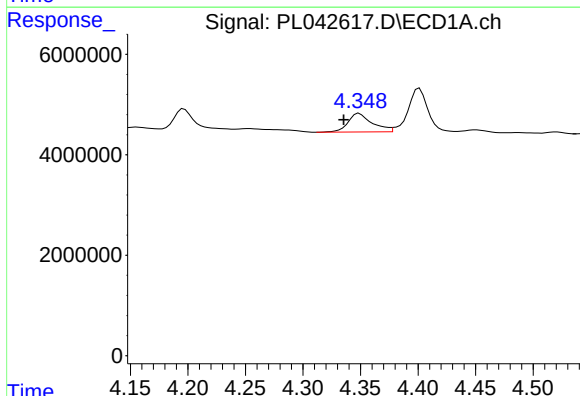


#23 Chlordane-1

R.T.: 4.349 min
Delta R.T.: 0.014 min
Response: 5476776
Conc: 19.81 ng/ml

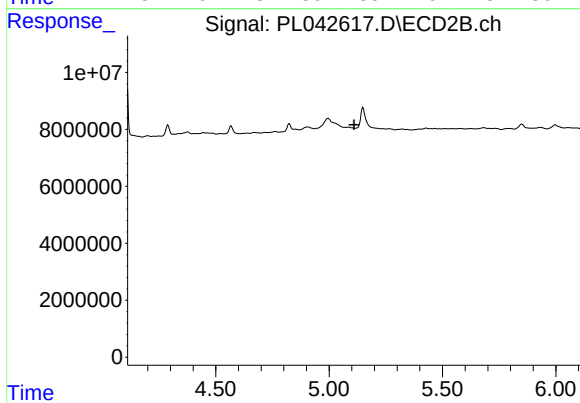

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

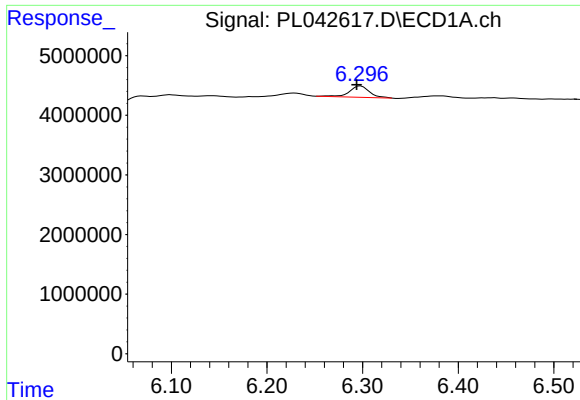

#27 Chlordane-5


R.T.: 6.298 min
Delta R.T.: 0.004 min
Response: 2715671
Conc: 9.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

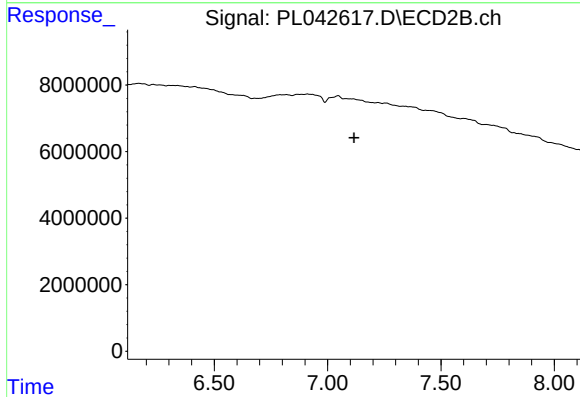


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

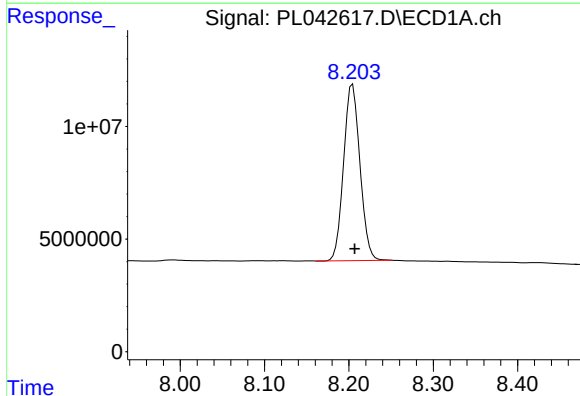

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.003 min
Response: 105497749
Conc: 16.74 ng/ml

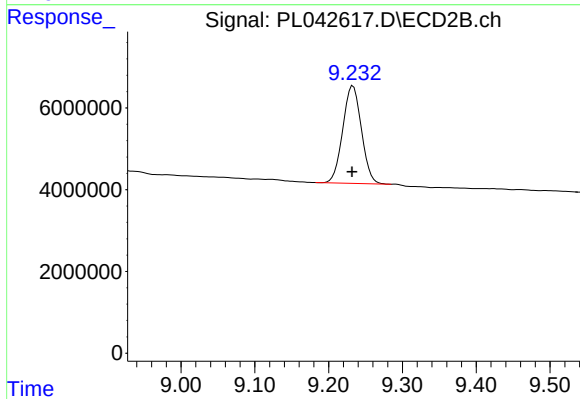

#28 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: 0.002 min
Response: 41869586
Conc: 17.36 ng/ml