

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112918\
 Data File : PL042618.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2018 21:29
 Operator : AJ\SJ
 Sample : J5767-18
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 00:01:36 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.102	111.8E6	59328036	18.999	20.628
28)	SA Decachlor...	8.205	9.234	110.6E6	44177349	17.545	18.317
Target Compounds							
3)	MA gamma-BHC...	4.198	4.767	8361370	1350564	1.014	0.342 #
6)	B beta-BHC	4.402f	4.906f	11388158	845761	3.214	0.536 #
8)	B Heptachlo...	5.243f	0.000	5039719	0	0.665	N.D. #
9)	A Endosulfan I	5.542	0.000	1316313	0	0.190	N.D. #
13)	MA Dieldrin	5.741	0.000	4376208	0	0.595	N.D. #
14)	MA Endrin	6.016	0.000	2092636	0	0.320	N.D. #
15)	B Endosulfa...	6.297	0.000	3162707	0	0.506	N.D. #
23)	Chlordane-1	4.348	0.000	2541608	0	9.193	N.D. #
27)	Chlordane-5	6.297	0.000	3162707	0	10.614	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112918\
Data File : PL042618.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2018 21:29
Operator : AJ\SJ
Sample : J5767-18
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 00:01:36 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

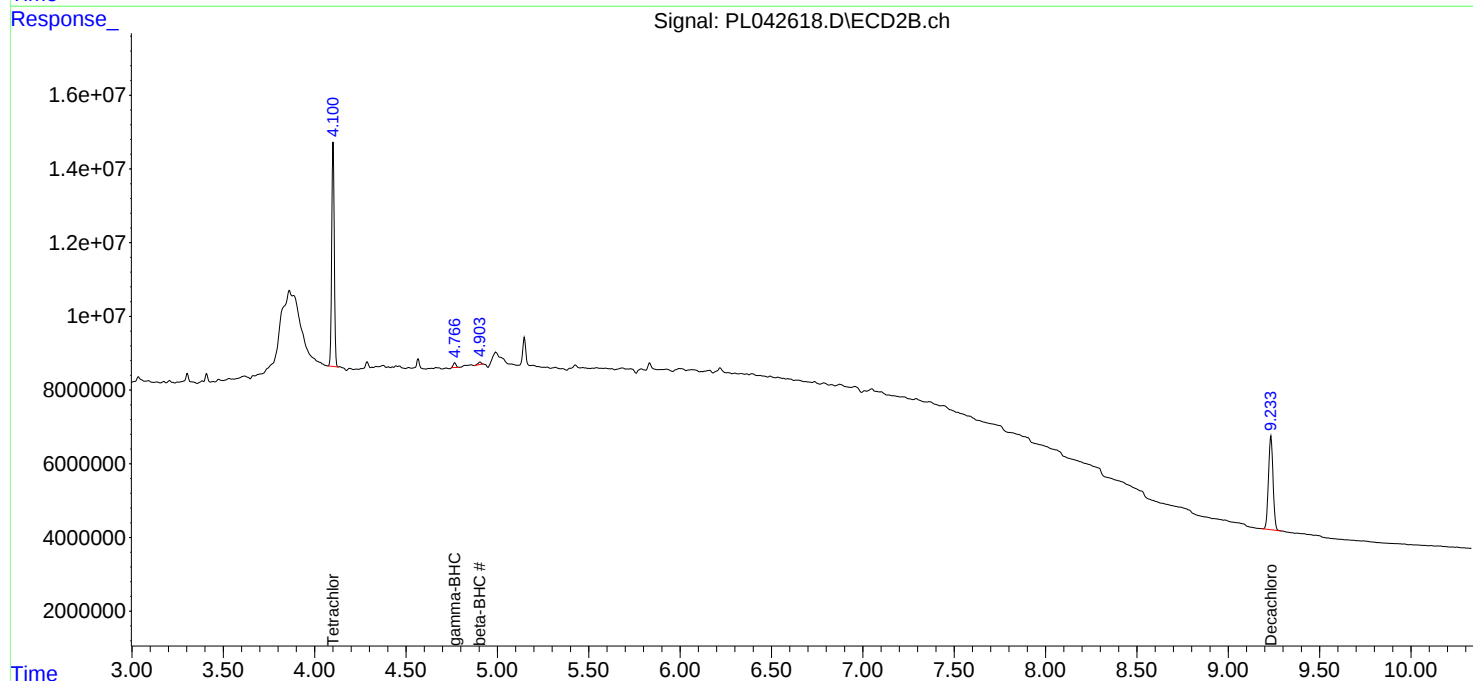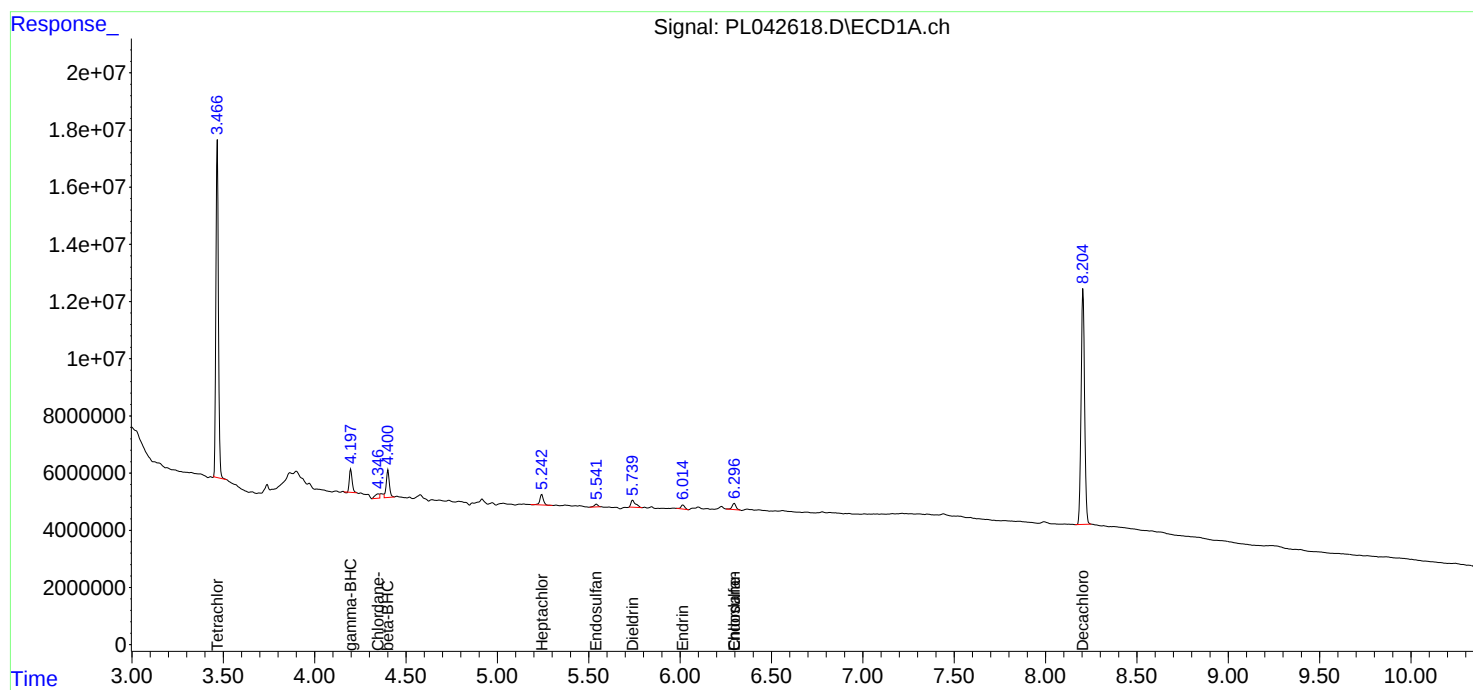


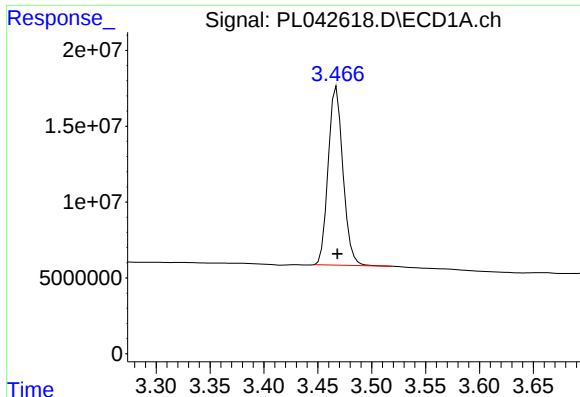

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 111779396
Conc: 19.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

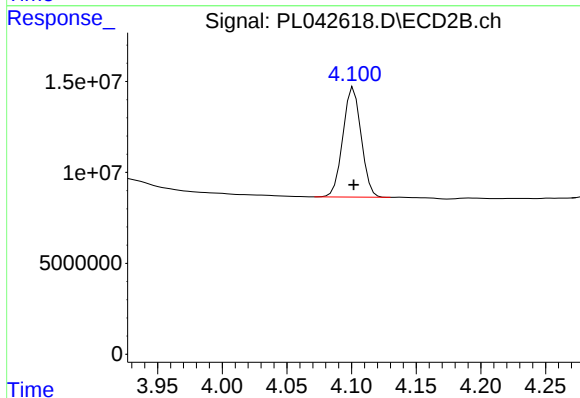


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 59328036
Conc: 20.63 ng/ml

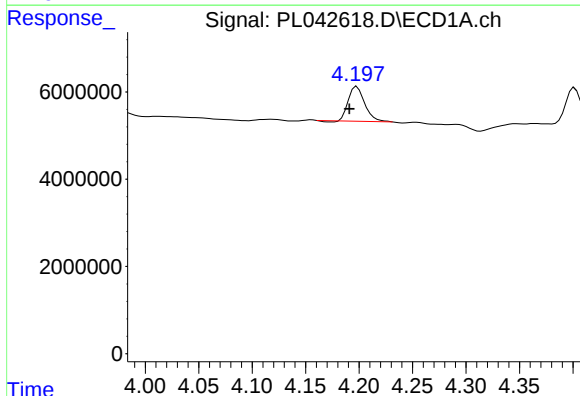


#3 gamma-BHC (Lindane)

R.T.: 4.198 min
Delta R.T.: 0.007 min
Response: 8361370
Conc: 1.01 ng/ml

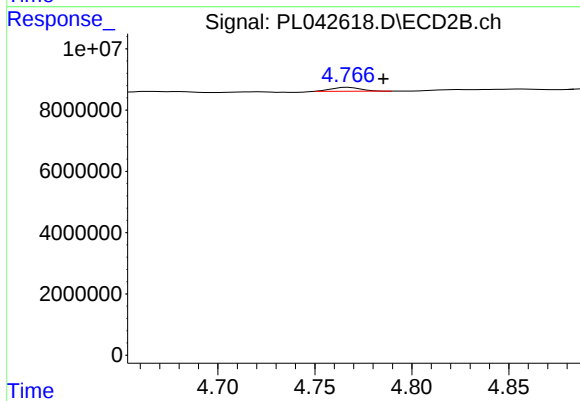

#3 gamma-BHC (Lindane)


R.T.: 4.767 min
Delta R.T.: -0.018 min
Response: 1350564
Conc: 0.34 ng/ml

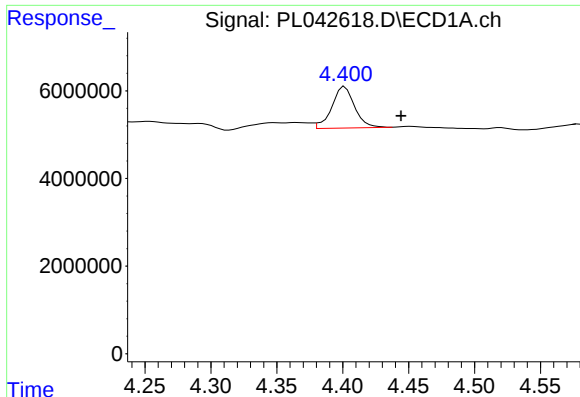

#6 beta-BHC


R.T.: 4.402 min
Delta R.T.: -0.043 min
Response: 11388158
Conc: 3.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

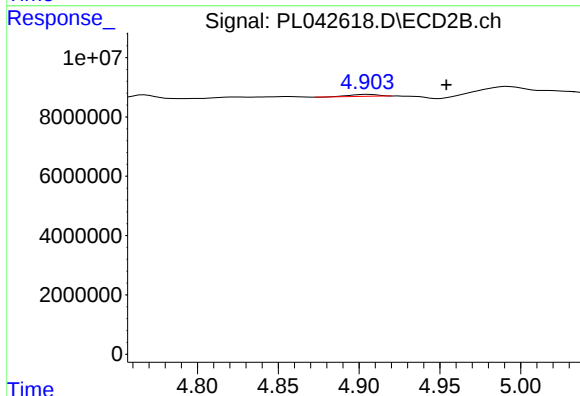


#6 beta-BHC

R.T.: 4.906 min
Delta R.T.: -0.048 min
Response: 845761
Conc: 0.54 ng/ml

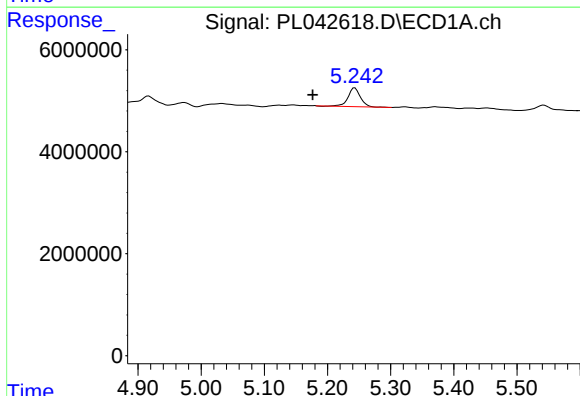


#8 Heptachlor epoxide

R.T.: 5.243 min
Delta R.T.: 0.067 min
Response: 5039719
Conc: 0.66 ng/ml

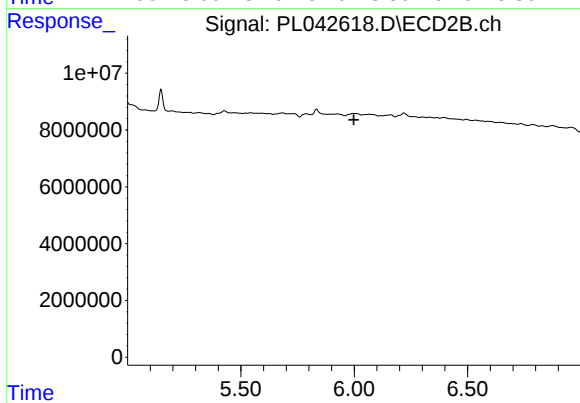

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.998 min
Response: 0
Conc: N.D.

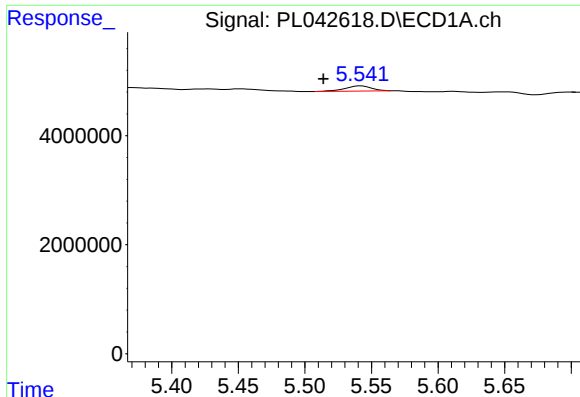

#9 Endosulfan I


R.T.: 5.542 min
Delta R.T.: 0.029 min
Response: 1316313
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

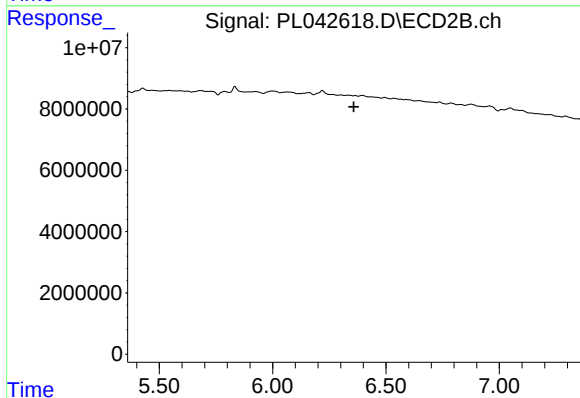


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.358 min
Response: 0
Conc: N.D.

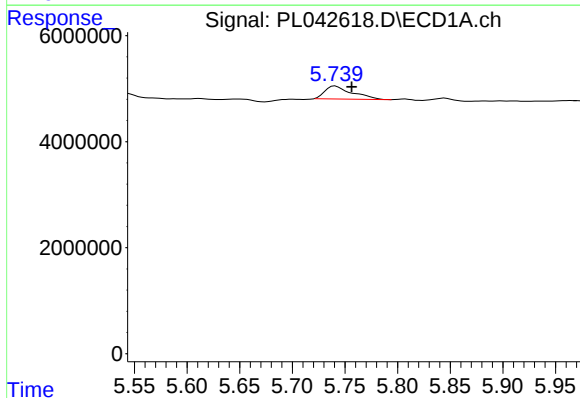


#13 Dieldrin

R.T.: 5.741 min
Delta R.T.: -0.016 min
Response: 4376208
Conc: 0.59 ng/ml

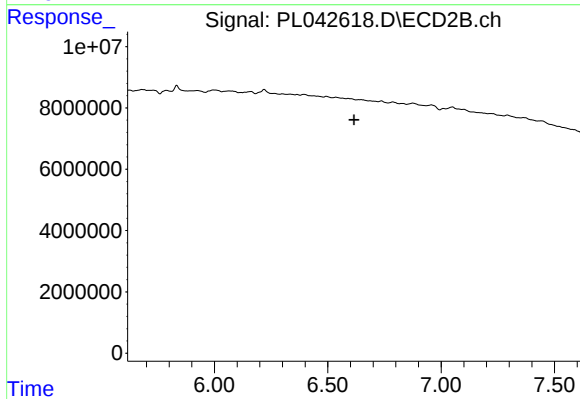

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.617 min
Response: 0
Conc: N.D.

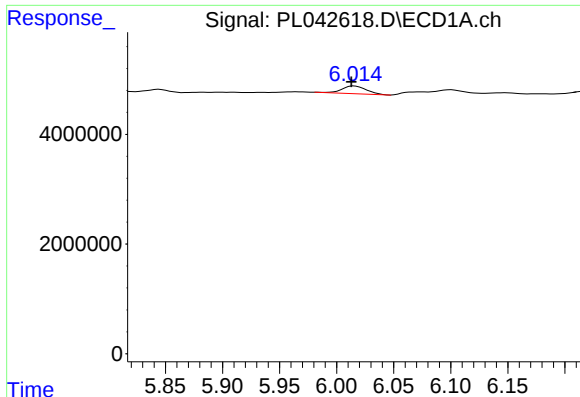

#14 Endrin


R.T.: 6.016 min
Delta R.T.: 0.002 min
Response: 2092636
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

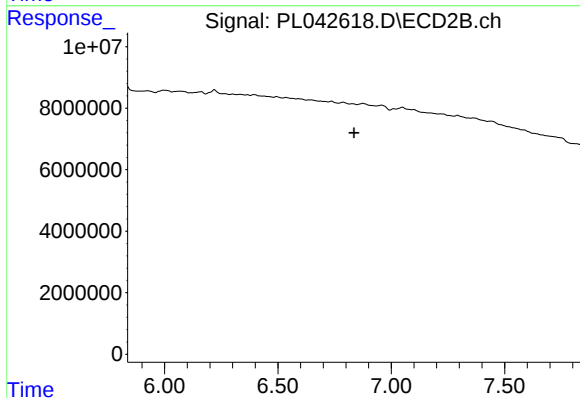


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.836 min
Response: 0
Conc: N.D.

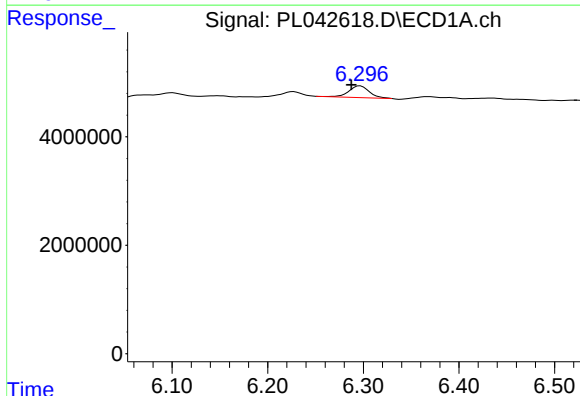


#15 Endosulfan II

R.T.: 6.297 min
Delta R.T.: 0.009 min
Response: 3162707
Conc: 0.51 ng/ml

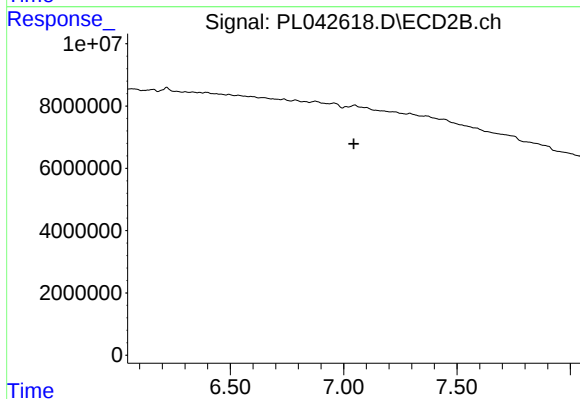

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.044 min
Response: 0
Conc: N.D.

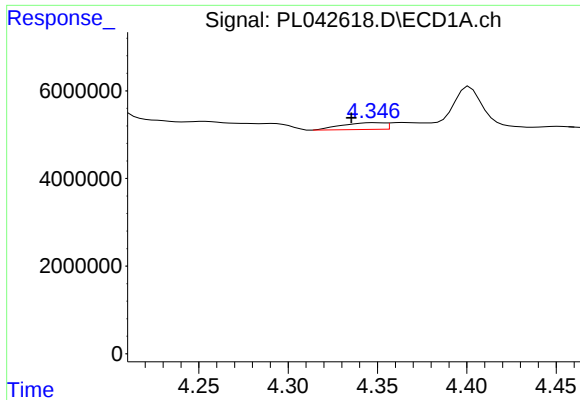

#23 Chlordane-1


R.T.: 4.348 min
Delta R.T.: 0.012 min
Response: 2541608
Conc: 9.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

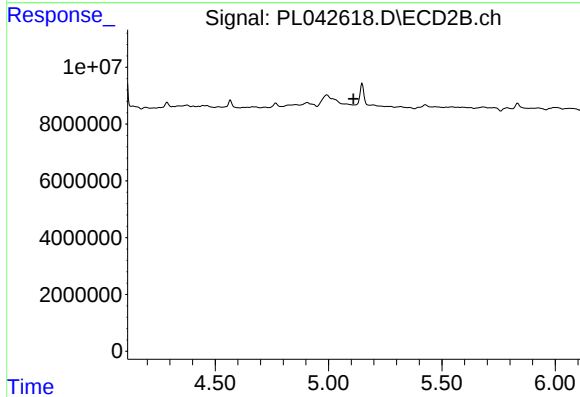


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

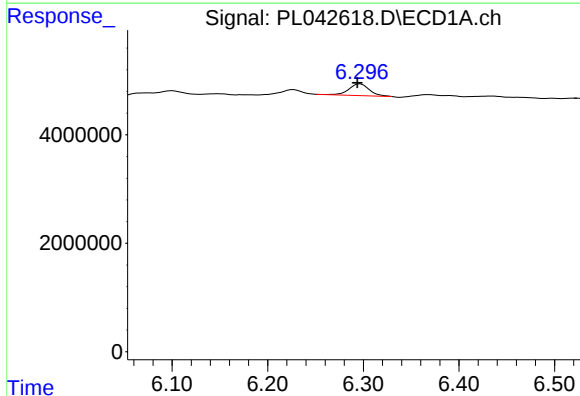


#27 Chlordane-5

R.T.: 6.297 min
Delta R.T.: 0.003 min
Response: 3162707
Conc: 10.61 ng/ml

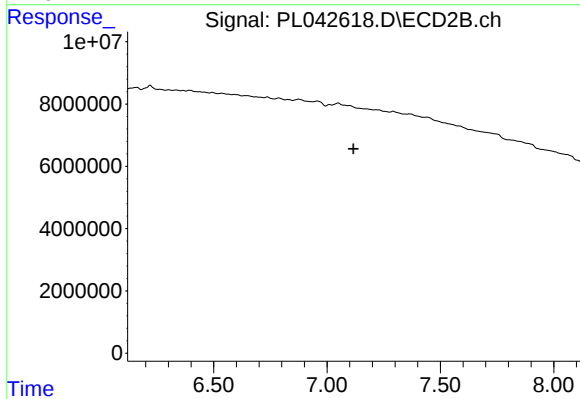

#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

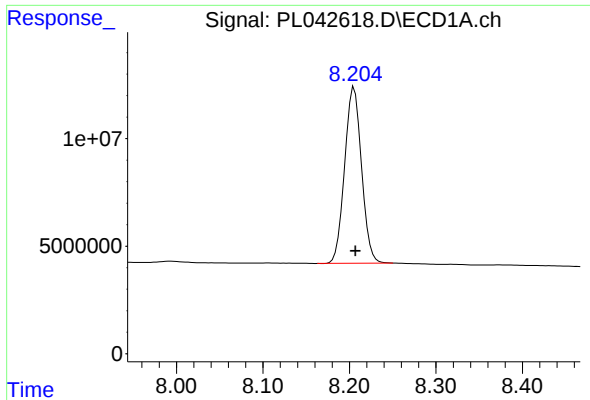

#28 Decachlorobiphenyl


R.T.: 8.205 min

Delta R.T.: -0.002 min

Response: 110568947

Conc: 17.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

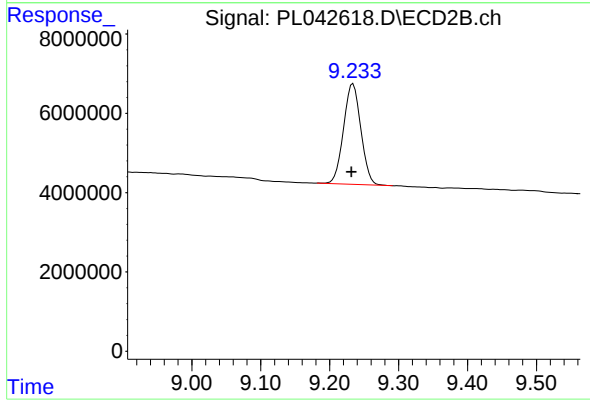

#28 Decachlorobiphenyl

R.T.: 9.234 min

Delta R.T.: 0.002 min

Response: 44177349

Conc: 18.32 ng/ml