

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112923\
 Data File : PL086859.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2023 03:49
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 04:46:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112923.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 29 04:42:22 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.343	2.610	312.7E6	109.8E6	99.114	101.380
28)	SA Decachlor...	8.843	7.761	246.4E6	102.6E6	94.050	94.092
Target Compounds							
23)	Chlordane-1	4.500	3.598	135.4E6	35136298	990.691	990.263
24)	Chlordane-2	5.033	4.176	138.3E6	41658854	949.085	970.574
25)	Chlordane-3	5.745	4.805	570.3E6	121.0E6	1019.073	1039.673
26)	Chlordane-4	5.828	4.866	698.1E6	136.1E6	998.268	1014.184
27)	Chlordane-5	6.675	5.537	103.4E6	32965221	996.149	999.927



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112923\
Data File : PL086859.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2023 03:49
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 04:46:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112923.M
Quant Title : GC Extractables
QLast Update : Wed Nov 29 04:42:22 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

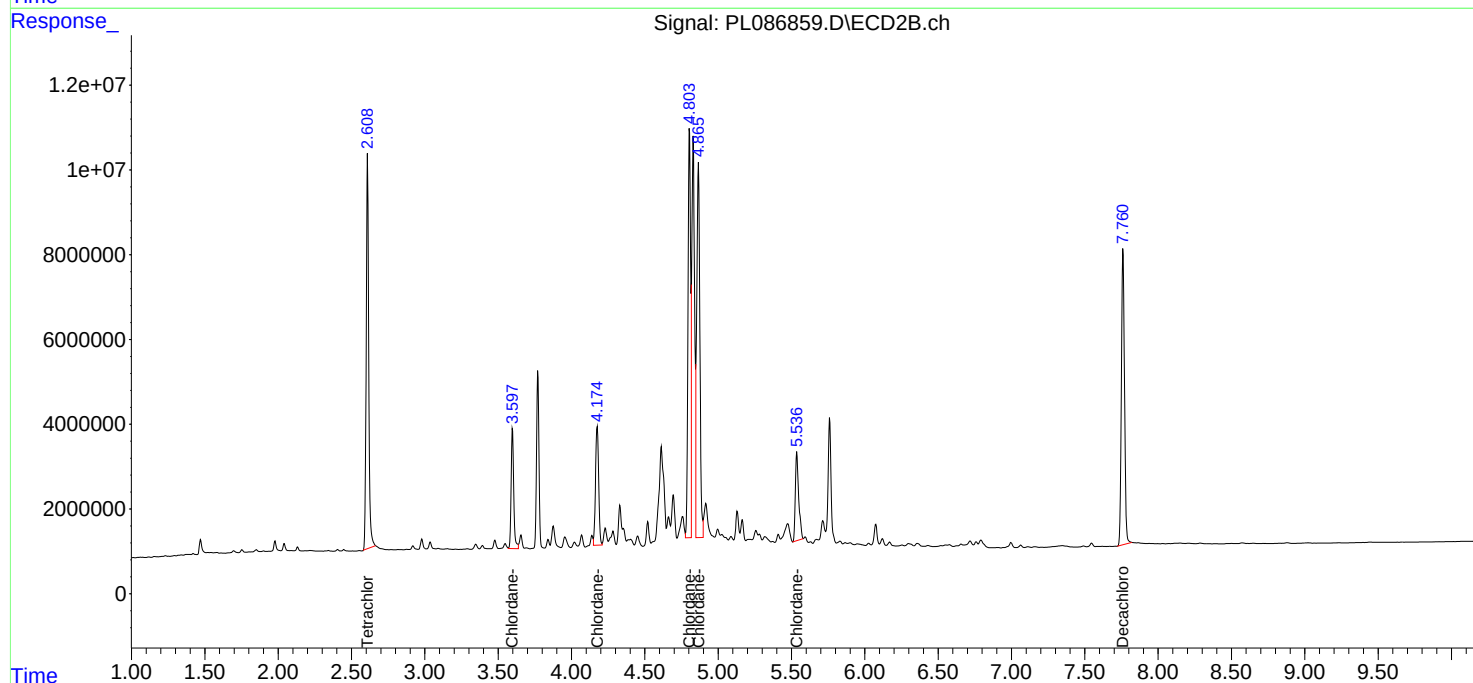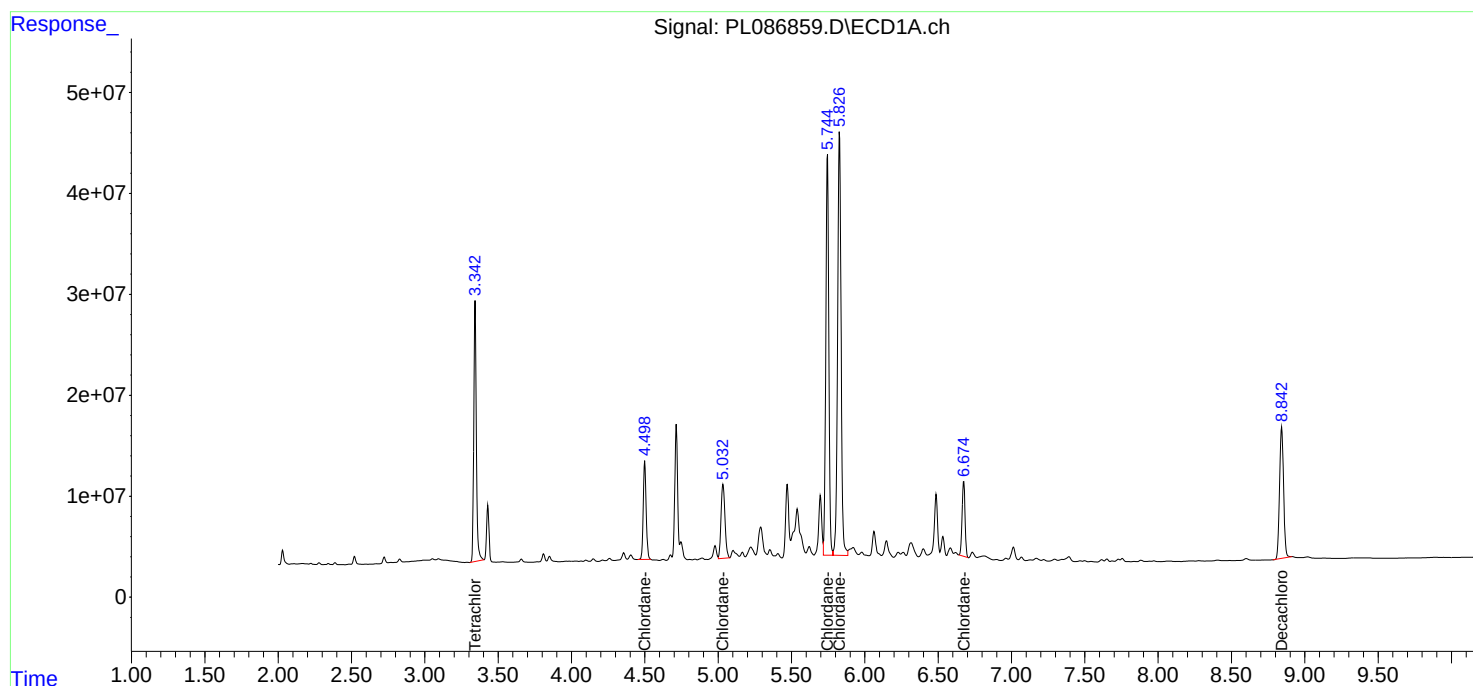


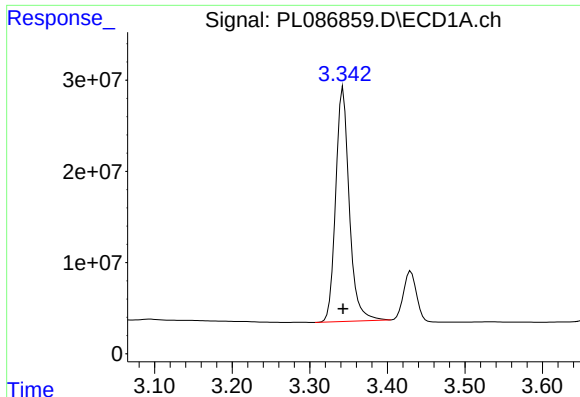

#1 Tetrachloro-m-xylene


R.T.: 3.343 min
Delta R.T.: 0.000 min
Response: 312662911
Conc: 99.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

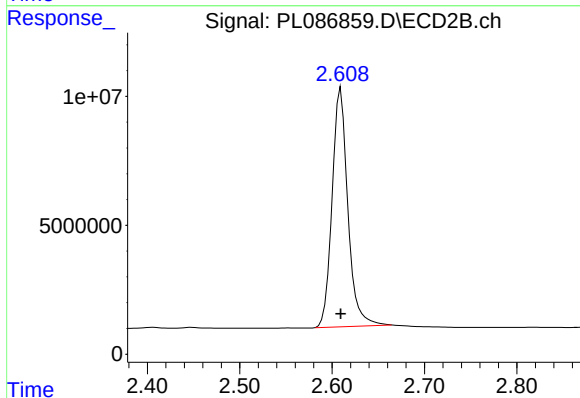


#1 Tetrachloro-m-xylene

R.T.: 2.610 min
Delta R.T.: 0.000 min
Response: 109768582
Conc: 101.38 ng/ml

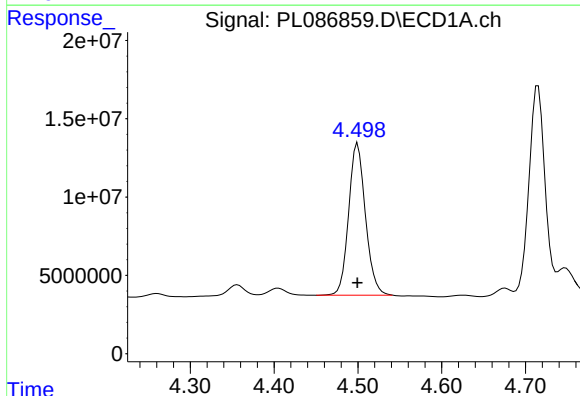


#23 Chlordane-1

R.T.: 4.500 min
Delta R.T.: 0.000 min
Response: 135442054
Conc: 990.69 ng/ml

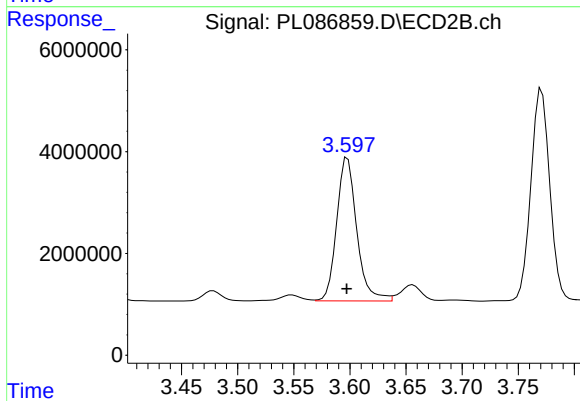

#23 Chlordane-1


R.T.: 3.598 min
Delta R.T.: 0.000 min
Response: 35136298
Conc: 990.26 ng/ml

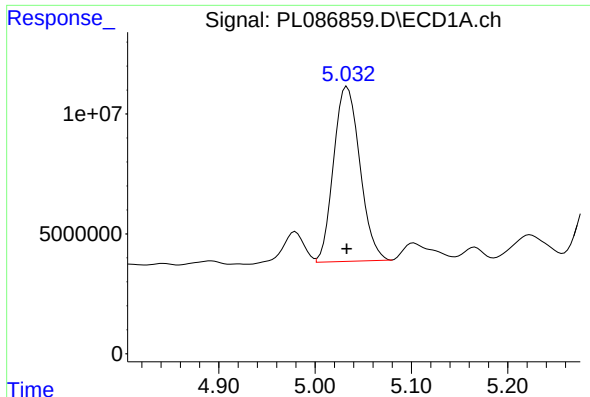

#24 Chlordane-2


R.T.: 5.033 min
Delta R.T.: 0.000 min
Response: 138323888
Conc: 949.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

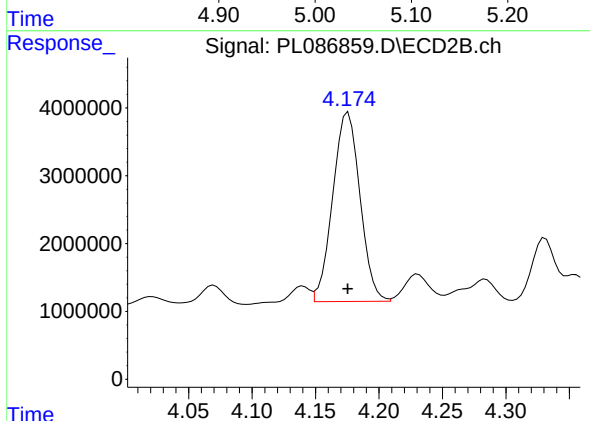


#24 Chlordane-2

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 41658854
Conc: 970.57 ng/ml

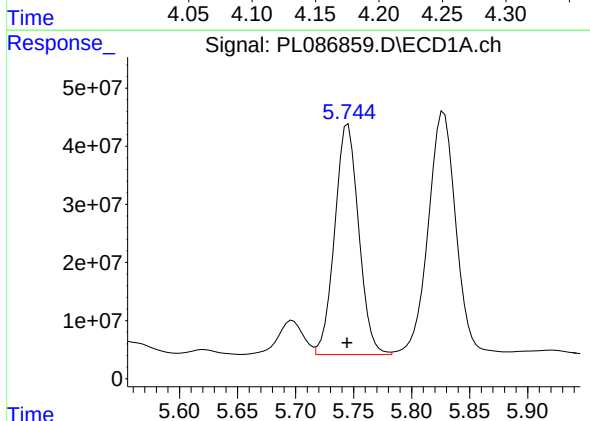


#25 Chlordane-3

R.T.: 5.745 min
Delta R.T.: 0.001 min
Response: 570254181
Conc: 1019.07 ng/ml

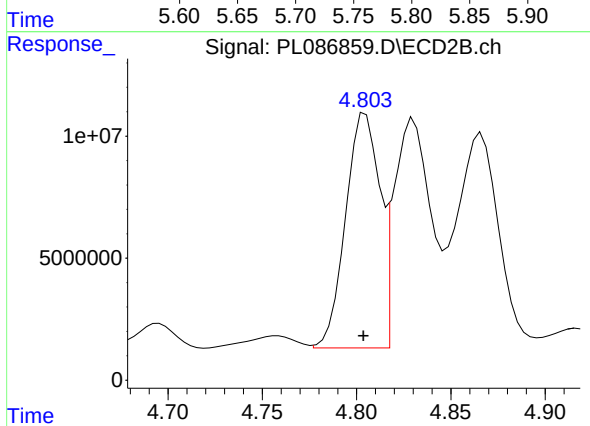

#25 Chlordane-3


R.T.: 4.805 min
Delta R.T.: 0.001 min
Response: 121016011
Conc: 1039.67 ng/ml

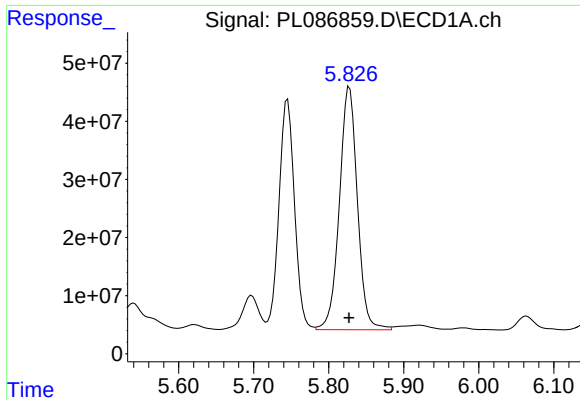

#26 Chlordane-4


R.T.: 5.828 min
Delta R.T.: 0.000 min
Response: 698126166
Conc: 998.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

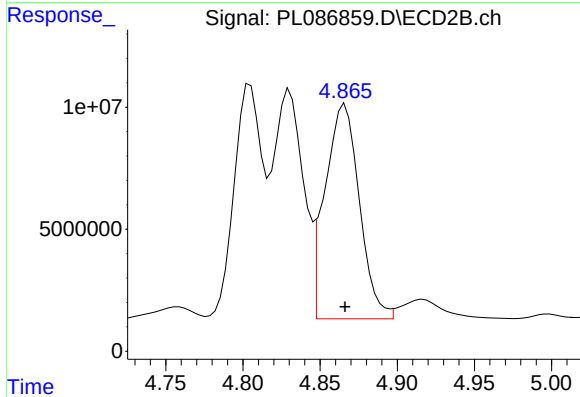


#26 Chlordane-4

R.T.: 4.866 min
Delta R.T.: 0.000 min
Response: 136144933
Conc: 1014.18 ng/ml

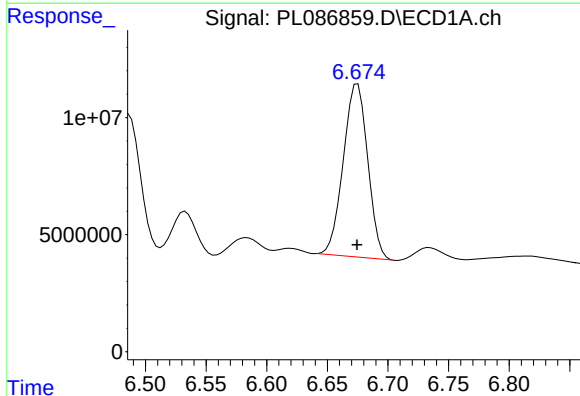


#27 Chlordane-5

R.T.: 6.675 min
Delta R.T.: 0.000 min
Response: 103409615
Conc: 996.15 ng/ml

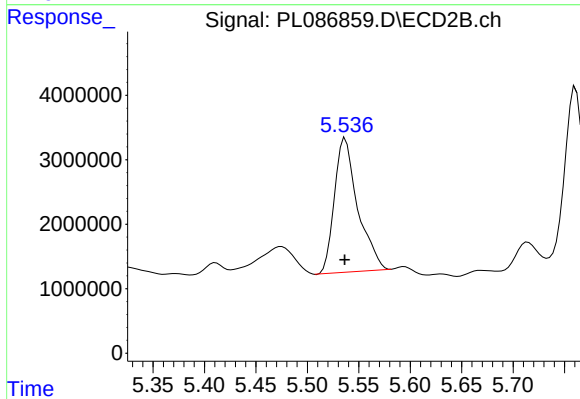

#27 Chlordane-5


R.T.: 5.537 min
Delta R.T.: 0.000 min
Response: 32965221
Conc: 999.93 ng/ml

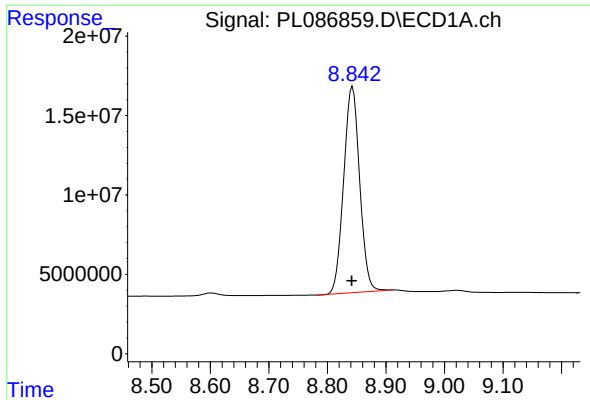

#28 Decachlorobiphenyl

R.T.: 8.843 min
Delta R.T.: 0.001 min
Response: 246406359
Conc: 94.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

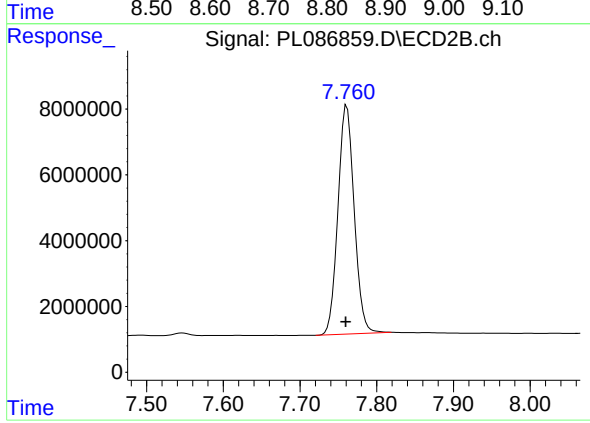

#28 Decachlorobiphenyl

R.T.: 7.761 min
Delta R.T.: 0.001 min
Response: 102641618
Conc: 94.09 ng/ml