

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112923\
 Data File : PL086860.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2023 04:03
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 04:46:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112923.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 29 04:42:22 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.343	2.630f	235.1E6	78274266	74.525	72.292
28)	SA Decachlor...	8.843	7.780f	189.6E6	77623687	72.379	71.158
Target Compounds							
23)	Chlordane-1	4.500	3.618f	101.5E6	25753949	742.634	725.836
24)	Chlordane-2	5.032	4.160f	105.7E6	1911339	725.111	44.531 #
25)	Chlordane-3	5.745	4.824f	424.1E6	88736555	757.967	762.354
26)	Chlordane-4	5.827	4.851f	523.1E6	94067074	747.933	700.734
27)	Chlordane-5	6.675	5.557f	77562518	10830793	747.163	328.528 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112923\
Data File : PL086860.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2023 04:03
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 04:46:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112923.M
Quant Title : GC Extractables
QLast Update : Wed Nov 29 04:42:22 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

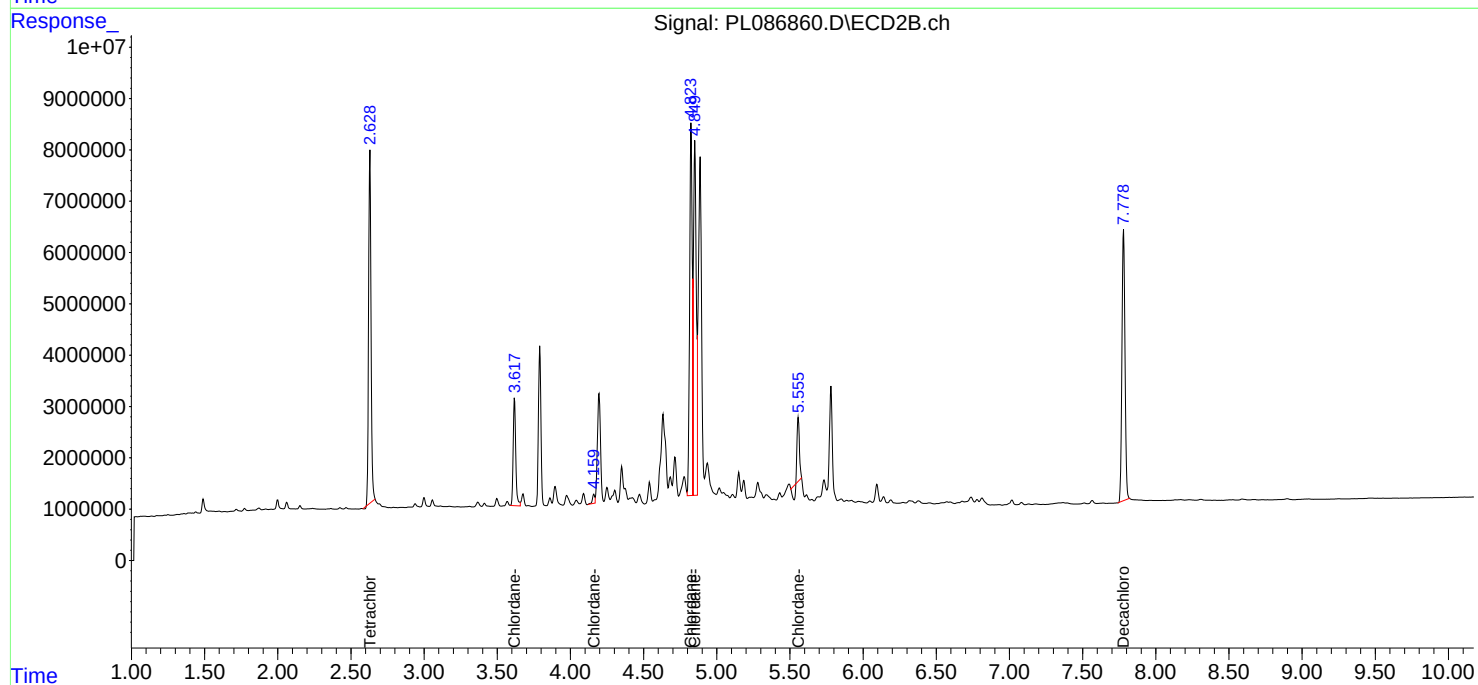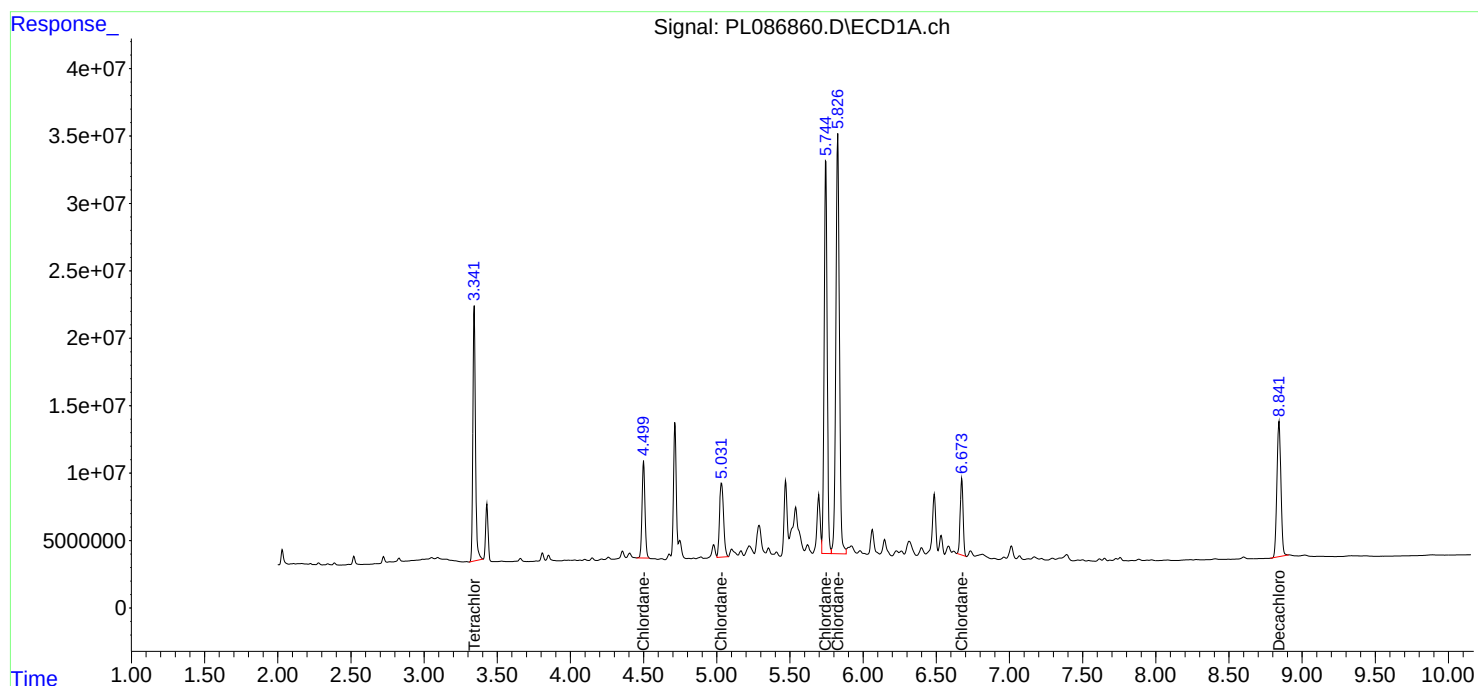


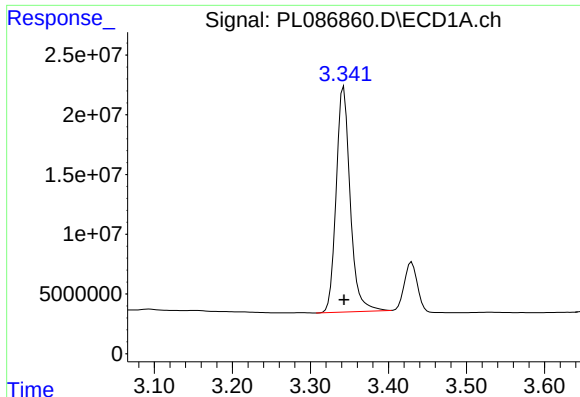

#1 Tetrachloro-m-xylene


R.T.: 3.343 min
Delta R.T.: 0.000 min
Response: 235094785
Conc: 74.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

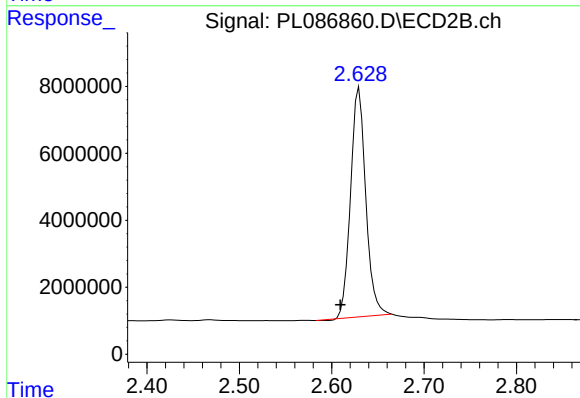


#1 Tetrachloro-m-xylene

R.T.: 2.630 min
Delta R.T.: 0.020 min
Response: 78274266
Conc: 72.29 ng/ml

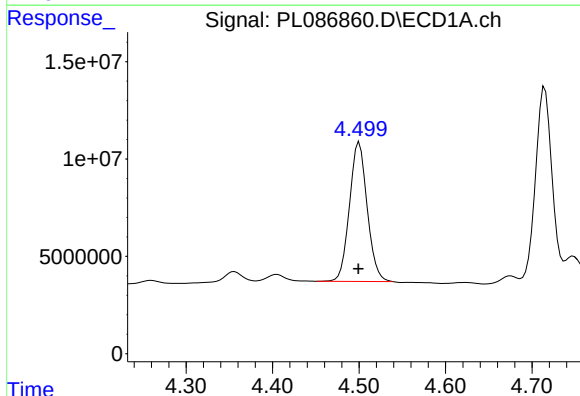


#23 Chlordane-1

R.T.: 4.500 min
Delta R.T.: 0.001 min
Response: 101529061
Conc: 742.63 ng/ml

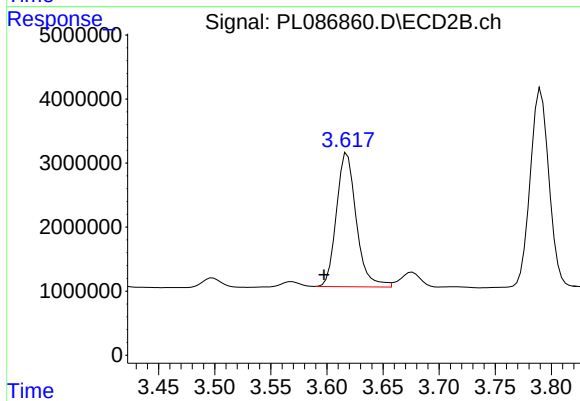

#23 Chlordane-1


R.T.: 3.618 min
Delta R.T.: 0.021 min
Response: 25753949
Conc: 725.84 ng/ml

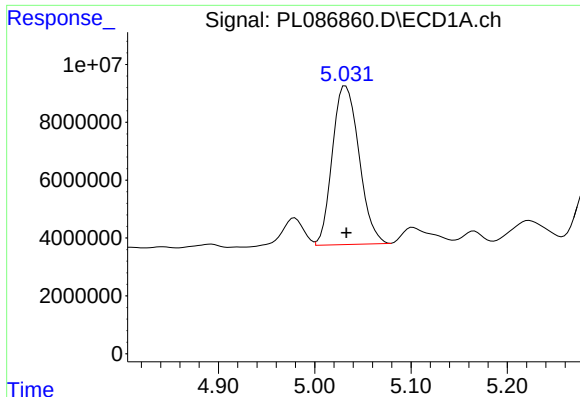

#24 Chlordane-2


R.T.: 5.032 min
Delta R.T.: 0.000 min
Response: 105680865
Conc: 725.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

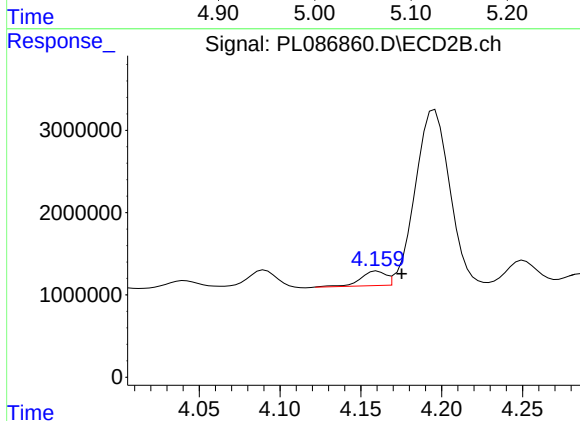


#24 Chlordane-2

R.T.: 4.160 min
Delta R.T.: -0.015 min
Response: 1911339
Conc: 44.53 ng/ml

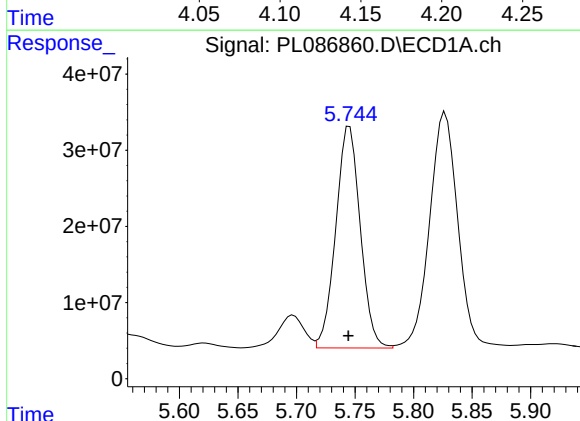


#25 Chlordane-3

R.T.: 5.745 min
Delta R.T.: 0.001 min
Response: 424144208
Conc: 757.97 ng/ml

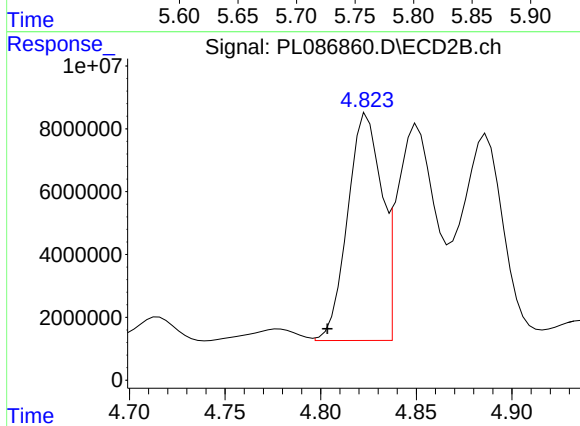

#25 Chlordane-3


R.T.: 4.824 min
Delta R.T.: 0.021 min
Response: 88736555
Conc: 762.35 ng/ml

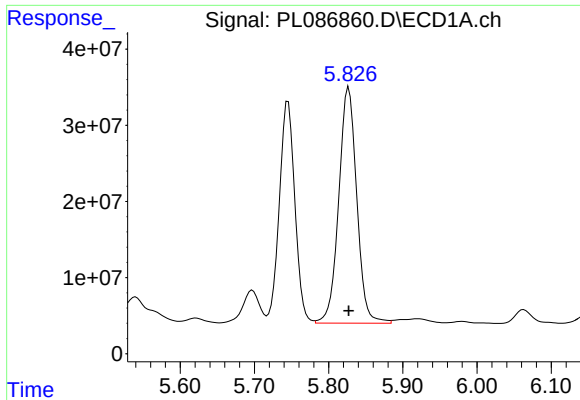

#26 Chlordane-4


R.T.: 5.827 min
Delta R.T.: 0.000 min
Response: 523057512
Conc: 747.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

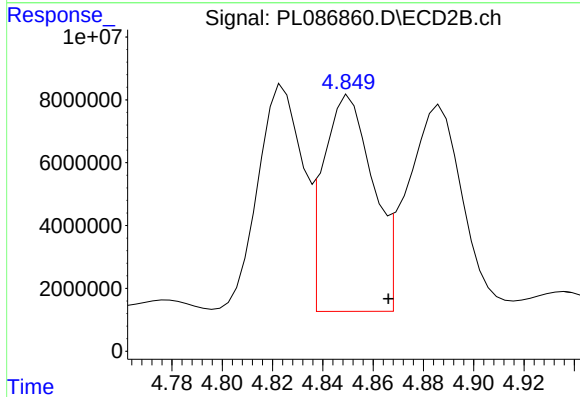


#26 Chlordane-4

R.T.: 4.851 min
Delta R.T.: -0.015 min
Response: 94067074
Conc: 700.73 ng/ml

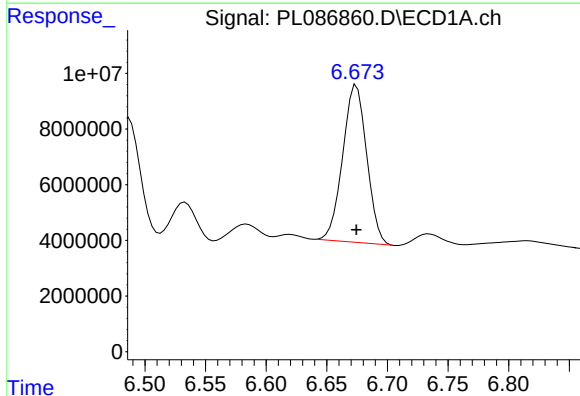


#27 Chlordane-5

R.T.: 6.675 min
Delta R.T.: 0.000 min
Response: 77562518
Conc: 747.16 ng/ml

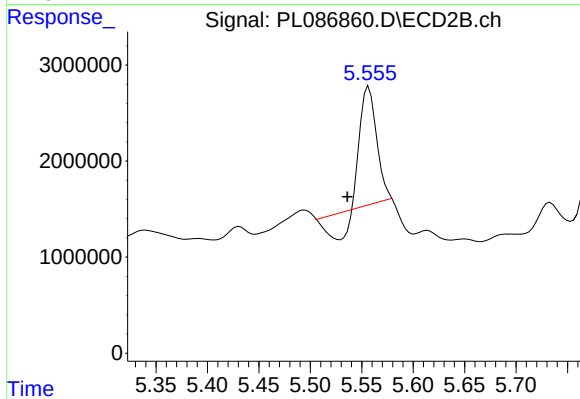

#27 Chlordane-5


R.T.: 5.557 min
Delta R.T.: 0.021 min
Response: 10830793
Conc: 328.53 ng/ml

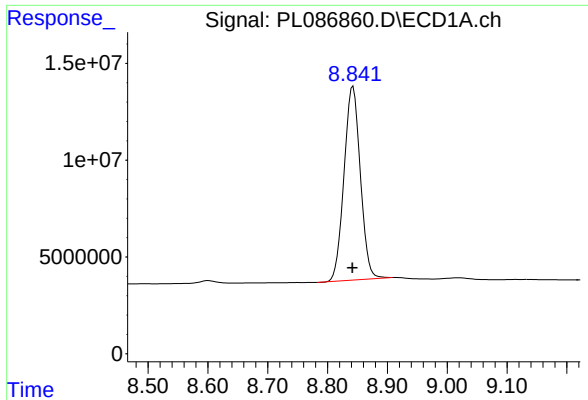

#28 Decachlorobiphenyl

R.T.: 8.843 min
Delta R.T.: 0.001 min
Response: 189628691
Conc: 72.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

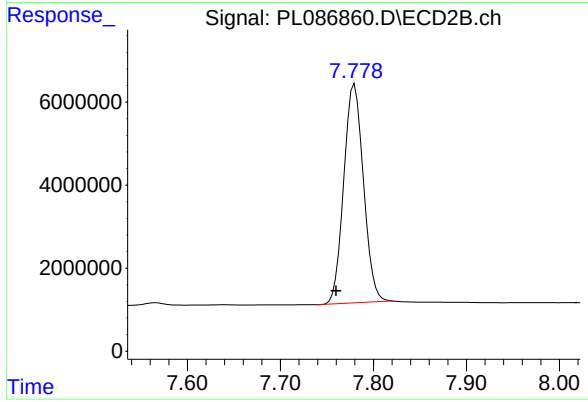

#28 Decachlorobiphenyl

R.T.: 7.780 min
Delta R.T.: 0.020 min
Response: 77623687
Conc: 71.16 ng/ml