

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112923\
 Data File : PL086863.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2023 04:44
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 05:00:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112923.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 29 04:58:49 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.343	2.609f	12885122	4107743	4.126	3.807
28)	SA Decachlor...	8.843	7.760f	12382044	5107762	4.799	4.764
Target Compounds							
23)	Chlordane-1	4.499	3.597f	5271576	2017266	38.980	57.258 #
24)	Chlordane-2	5.033	4.175f	6613783	1795665	46.163	42.393
25)	Chlordane-3	5.744	4.830	20900764	4684390	37.522	40.243
26)	Chlordane-4	5.827	4.868f	28159654	7080892	40.658	53.502 #
27)	Chlordane-5	6.674	5.536f	4269682	1235407	41.395	37.823



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112923\
Data File : PL086863.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2023 04:44
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 05:00:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112923.M
Quant Title : GC Extractables
QLast Update : Wed Nov 29 04:58:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

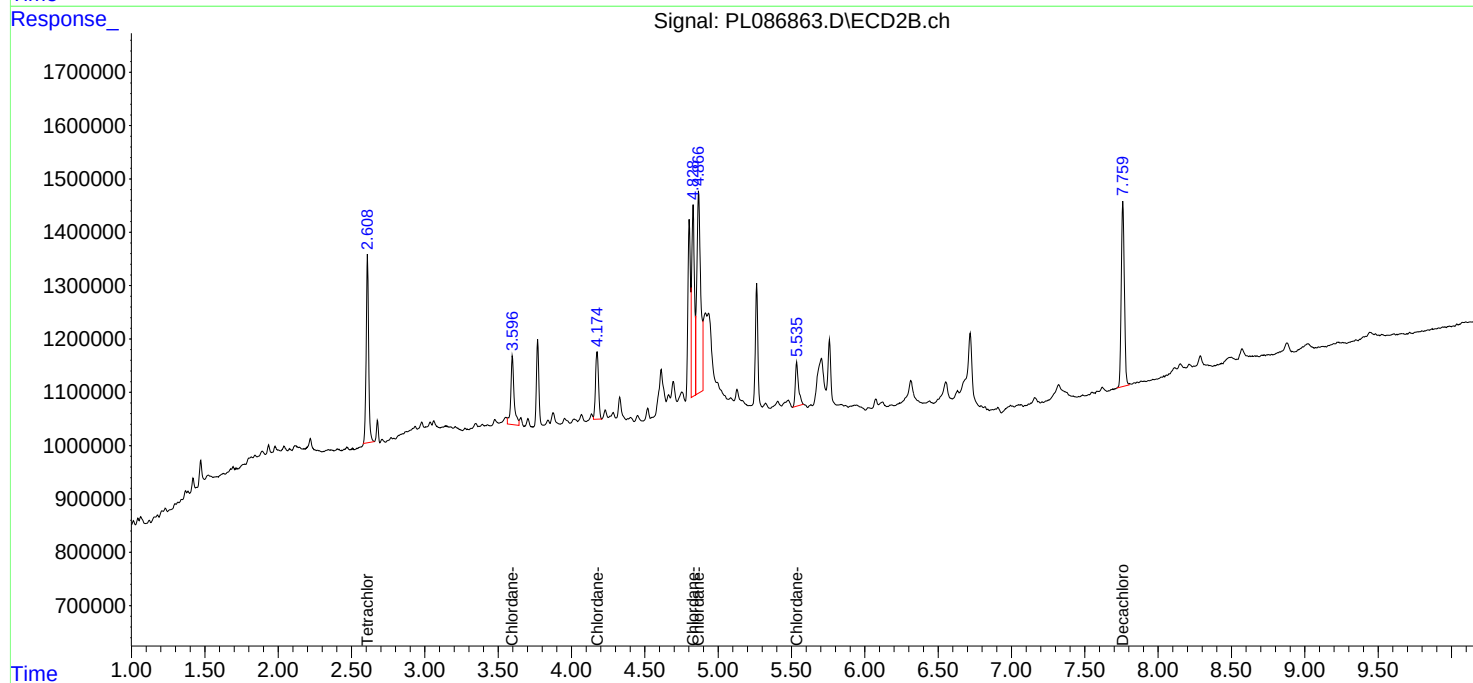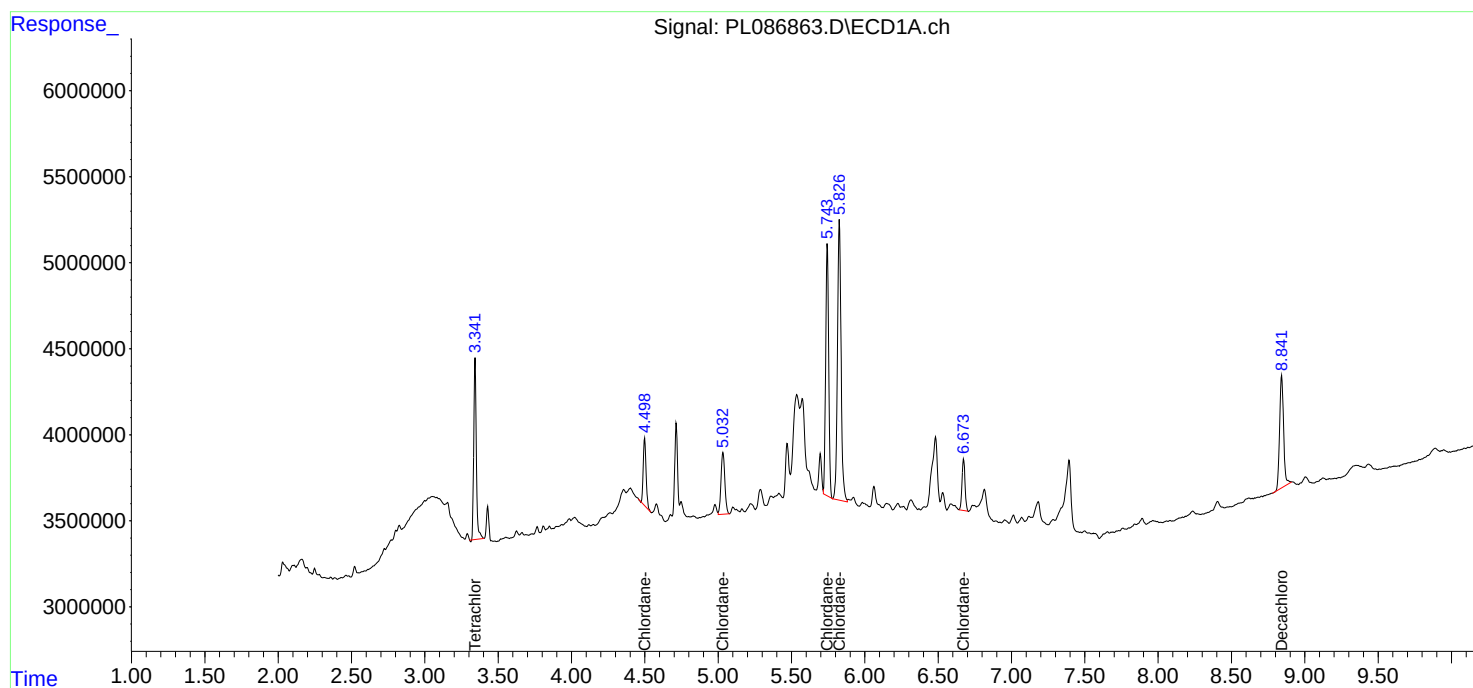


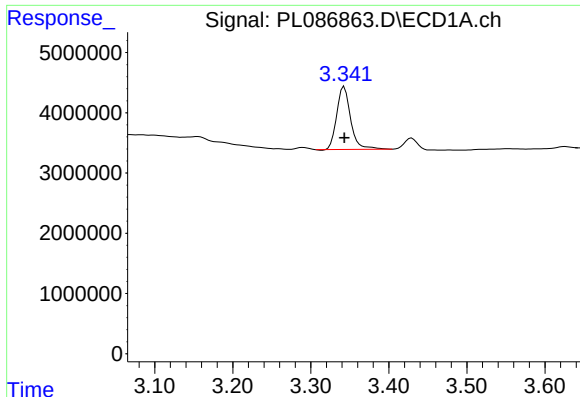

#1 Tetrachloro-m-xylene


R.T.: 3.343 min
Delta R.T.: 0.000 min
Response: 12885122
Conc: 4.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

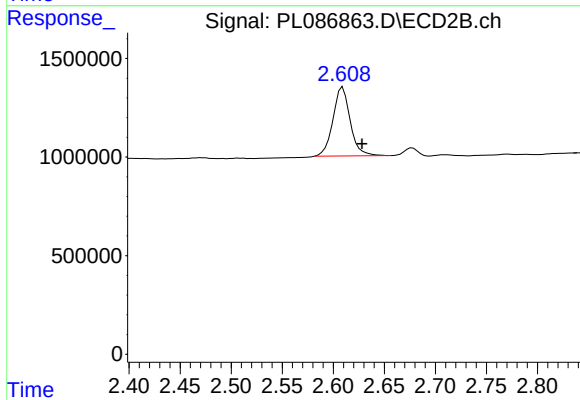


#1 Tetrachloro-m-xylene

R.T.: 2.609 min
Delta R.T.: -0.019 min
Response: 4107743
Conc: 3.81 ng/ml

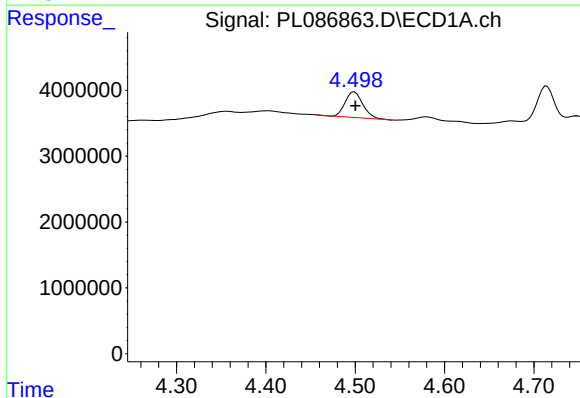


#23 Chlordane-1

R.T.: 4.499 min
Delta R.T.: -0.001 min
Response: 5271576
Conc: 38.98 ng/ml

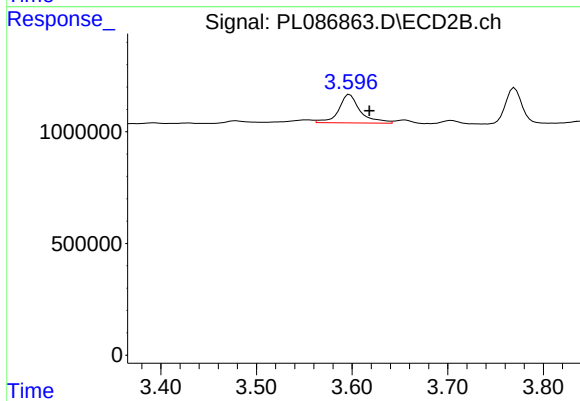

#23 Chlordane-1


R.T.: 3.597 min
Delta R.T.: -0.021 min
Response: 2017266
Conc: 57.26 ng/ml

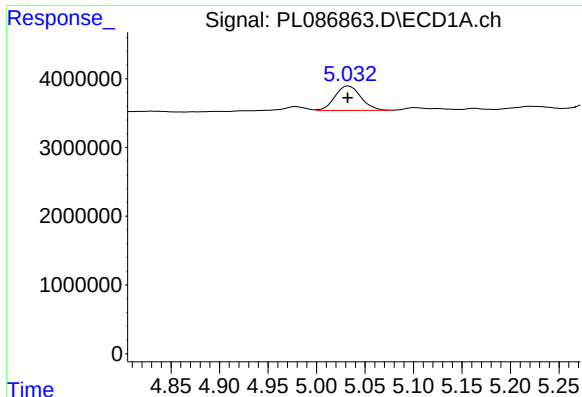

#24 Chlordane-2


R.T.: 5.033 min
Delta R.T.: 0.001 min
Response: 6613783
Conc: 46.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

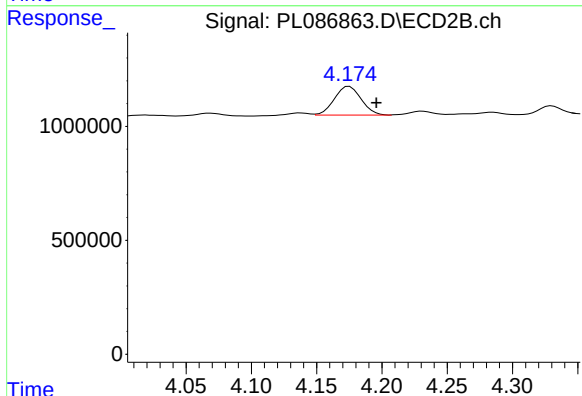


#24 Chlordane-2

R.T.: 4.175 min
Delta R.T.: -0.021 min
Response: 1795665
Conc: 42.39 ng/ml

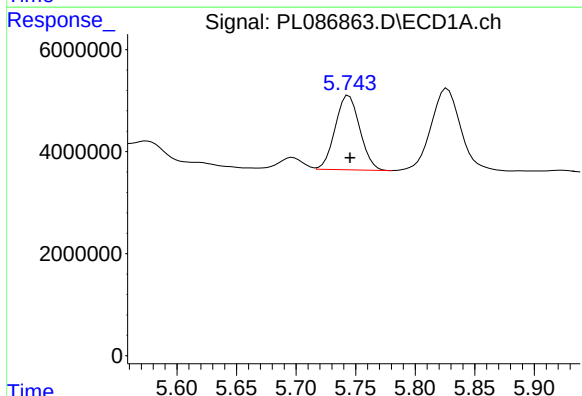


#25 Chlordane-3

R.T.: 5.744 min
Delta R.T.: -0.001 min
Response: 20900764
Conc: 37.52 ng/ml

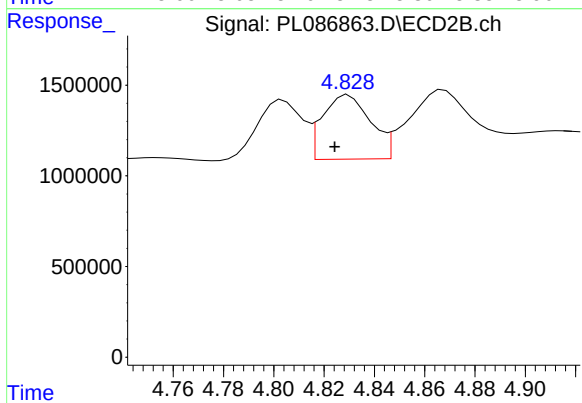

#25 Chlordane-3


R.T.: 4.830 min
Delta R.T.: 0.006 min
Response: 4684390
Conc: 40.24 ng/ml

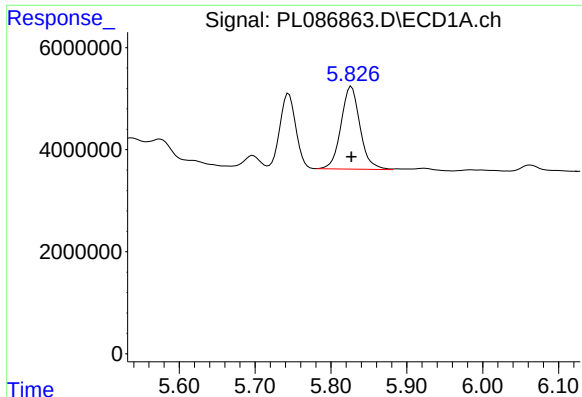

#26 Chlordane-4


R.T.: 5.827 min
Delta R.T.: 0.000 min
Response: 28159654
Conc: 40.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

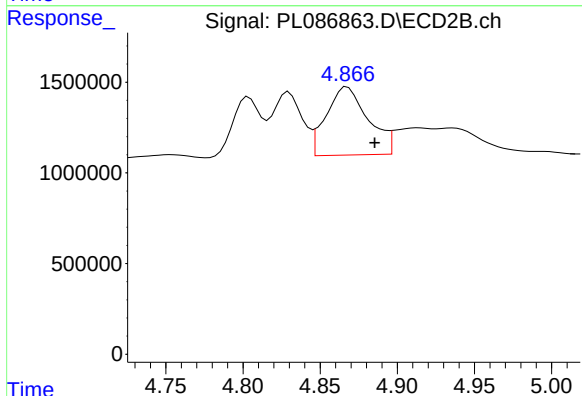


#26 Chlordane-4

R.T.: 4.868 min
Delta R.T.: -0.018 min
Response: 7080892
Conc: 53.50 ng/ml

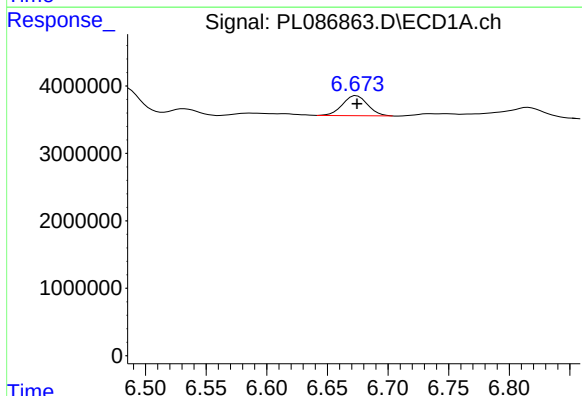


#27 Chlordane-5

R.T.: 6.674 min
Delta R.T.: 0.000 min
Response: 4269682
Conc: 41.40 ng/ml

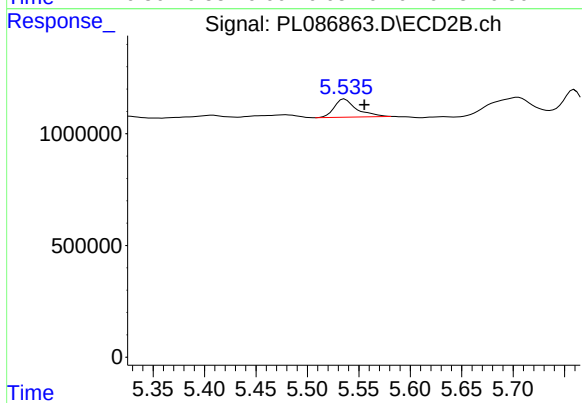

#27 Chlordane-5


R.T.: 5.536 min
Delta R.T.: -0.019 min
Response: 1235407
Conc: 37.82 ng/ml

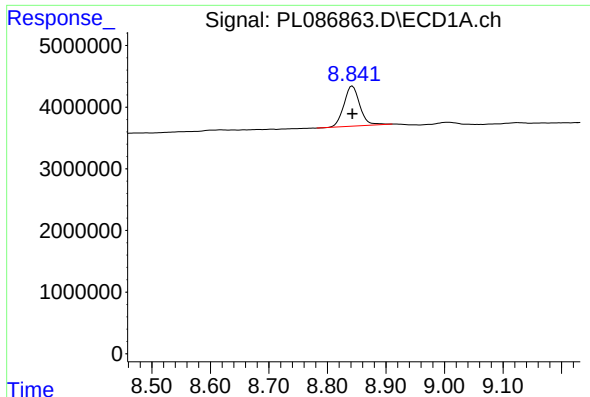

#28 Decachlorobiphenyl

R.T.: 8.843 min
Delta R.T.: 0.000 min
Response: 12382044
Conc: 4.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

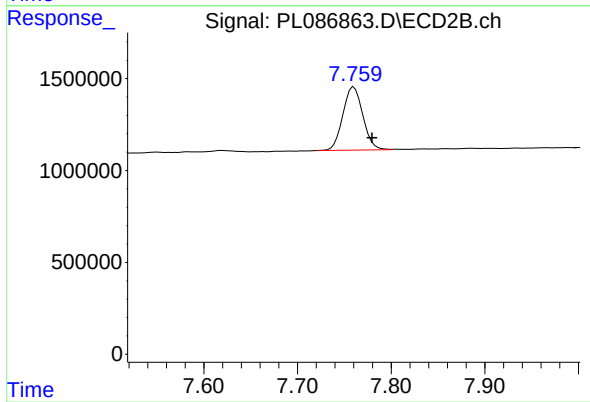

#28 Decachlorobiphenyl

R.T.: 7.760 min
Delta R.T.: -0.020 min
Response: 5107762
Conc: 4.76 ng/ml