

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112923\
 Data File : PL086861.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2023 04:17
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 04:47:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112923.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 29 04:42:22 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.343	2.609	157.7E6	54137210	50.000	50.000
28)	SA Decachlor...	8.841	7.760	131.0E6	54543482	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.499	3.597	68357391	17740896	500.000	500.000
24)	Chlordane-2	5.033	4.175	72872207	21460933	500.000	500.000
25)	Chlordane-3	5.744	4.804	279.8E6	58199074	500.000	500.000
26)	Chlordane-4	5.827	4.866	349.7E6	67120412	500.000	500.000
27)	Chlordane-5	6.675	5.536	51904674	16483818	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112923\
Data File : PL086861.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2023 04:17
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 04:47:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112923.M
Quant Title : GC Extractables
QLast Update : Wed Nov 29 04:42:22 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

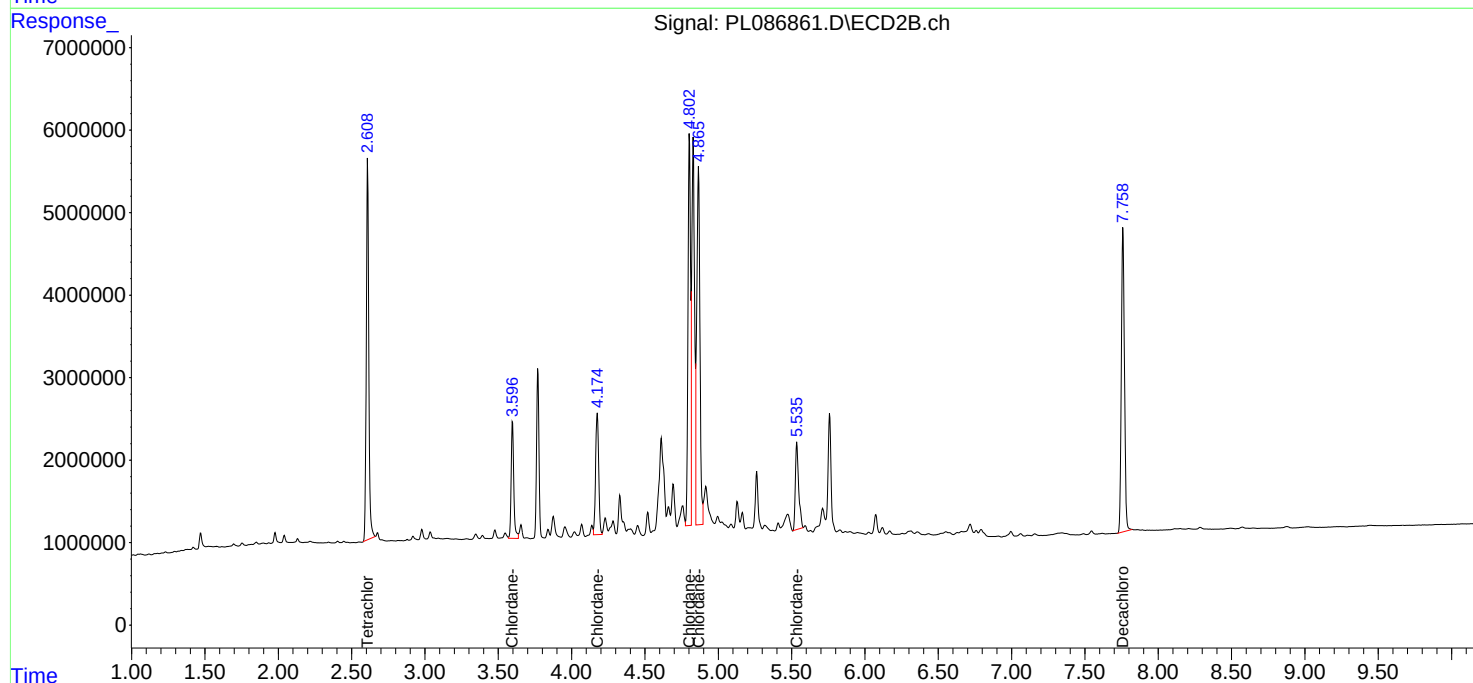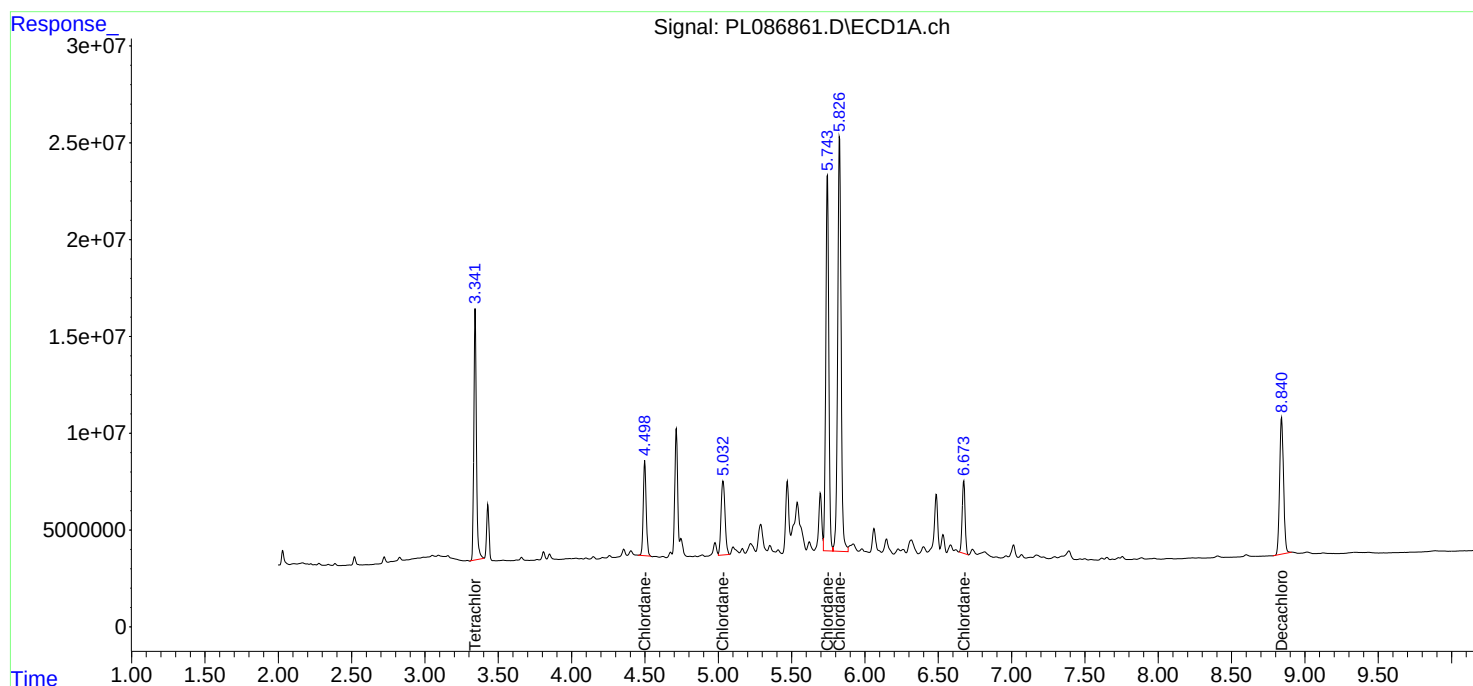


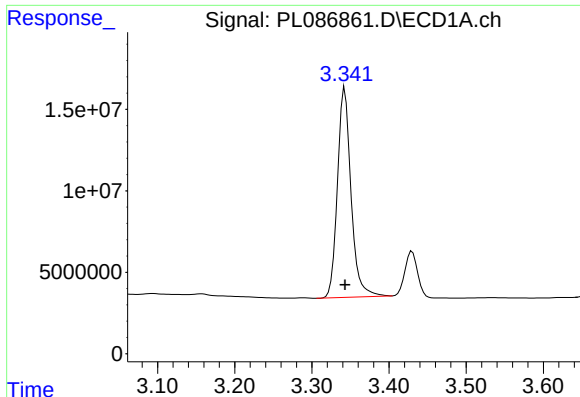

#1 Tetrachloro-m-xylene


R.T.: 3.343 min
Delta R.T.: 0.000 min
Response: 157728521
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

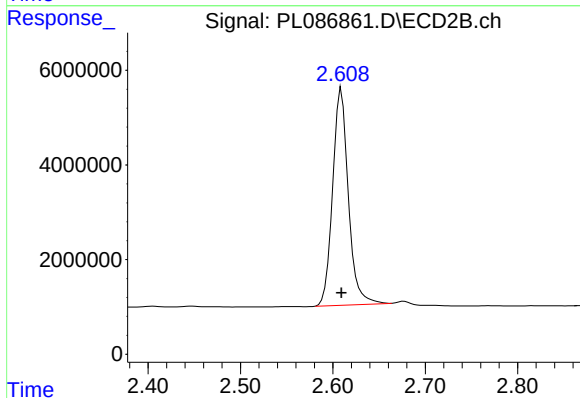


#1 Tetrachloro-m-xylene

R.T.: 2.609 min
Delta R.T.: 0.000 min
Response: 54137210
Conc: 50.00 ng/ml

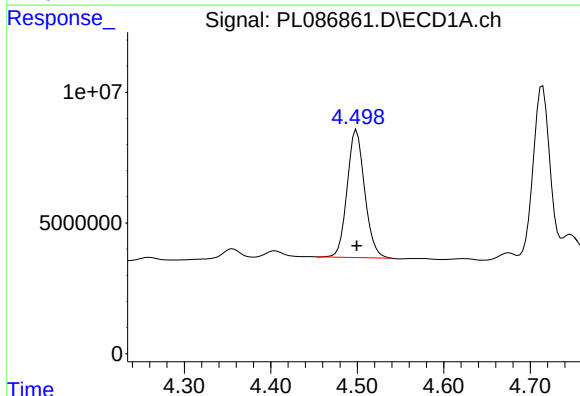


#23 Chlordane-1

R.T.: 4.499 min
Delta R.T.: 0.000 min
Response: 68357391
Conc: 500.00 ng/ml

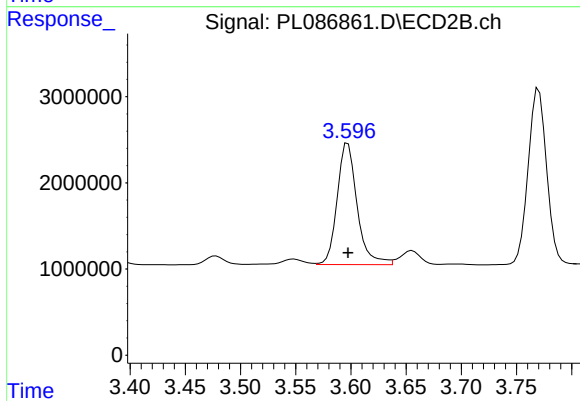

#23 Chlordane-1


R.T.: 3.597 min
Delta R.T.: 0.000 min
Response: 17740896
Conc: 500.00 ng/ml

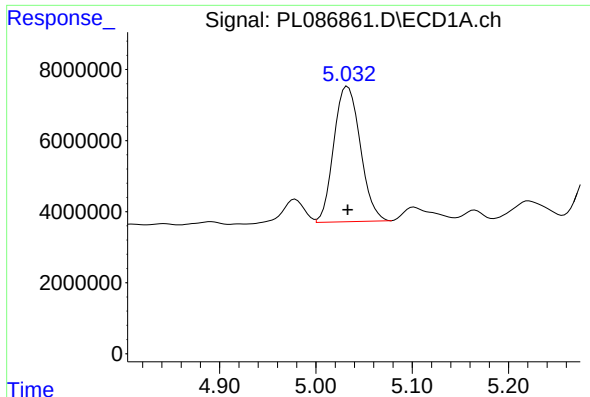

#24 Chlordane-2


R.T.: 5.033 min
Delta R.T.: 0.000 min
Response: 72872207
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

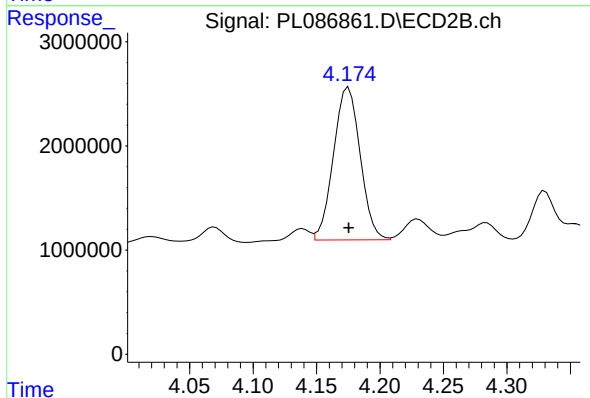


#24 Chlordane-2

R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 21460933
Conc: 500.00 ng/ml

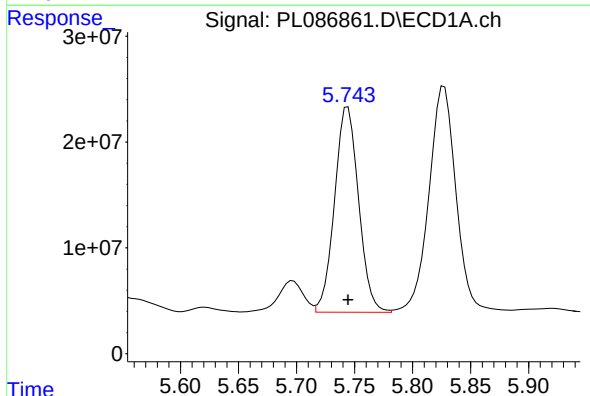


#25 Chlordane-3

R.T.: 5.744 min
Delta R.T.: 0.000 min
Response: 279790582
Conc: 500.00 ng/ml

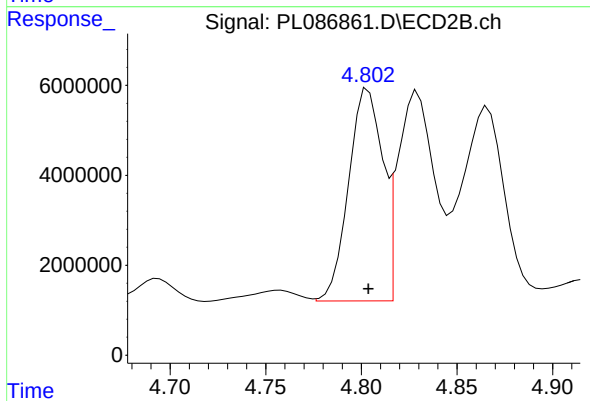

#25 Chlordane-3


R.T.: 4.804 min
Delta R.T.: 0.000 min
Response: 58199074
Conc: 500.00 ng/ml

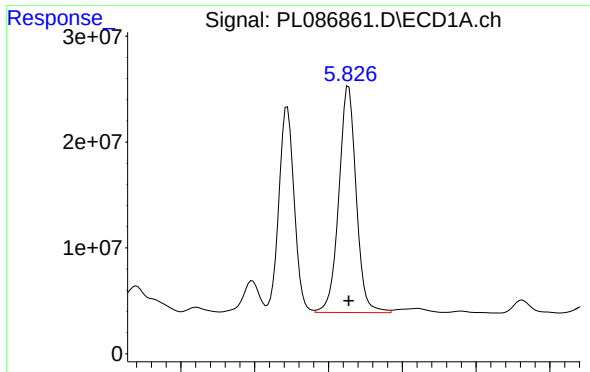

#26 Chlordane-4


R.T.: 5.827 min
Delta R.T.: 0.000 min
Response: 349668620
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

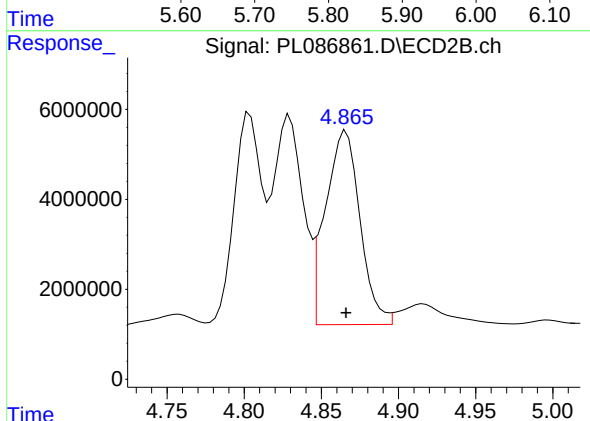


#26 Chlordane-4

R.T.: 4.866 min
Delta R.T.: 0.000 min
Response: 67120412
Conc: 500.00 ng/ml

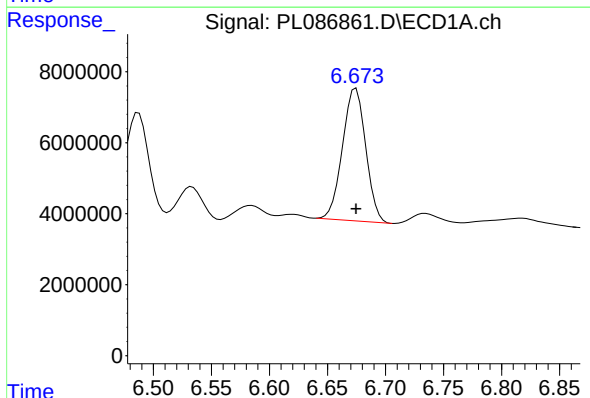


#27 Chlordane-5

R.T.: 6.675 min
Delta R.T.: 0.000 min
Response: 51904674
Conc: 500.00 ng/ml

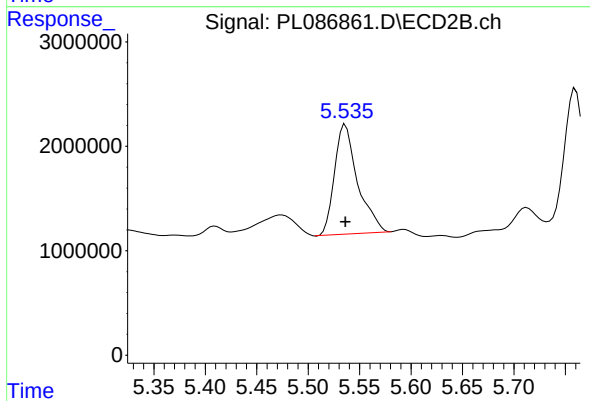

#27 Chlordane-5

R.T.: 5.536 min
Delta R.T.: 0.000 min
Response: 16483818
Conc: 500.00 ng/ml

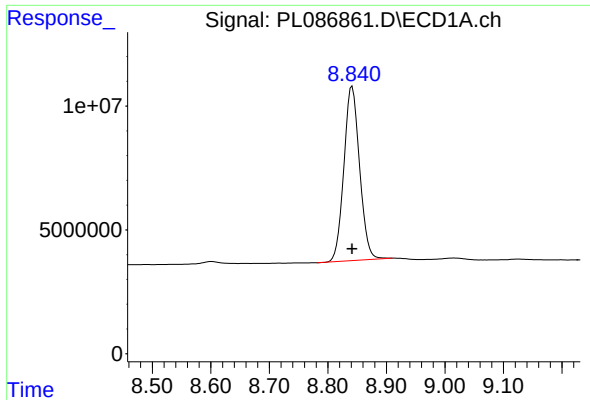

#28 Decachlorobiphenyl


R.T.: 8.841 min

Delta R.T.: 0.000 min

Response: 130996944

Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

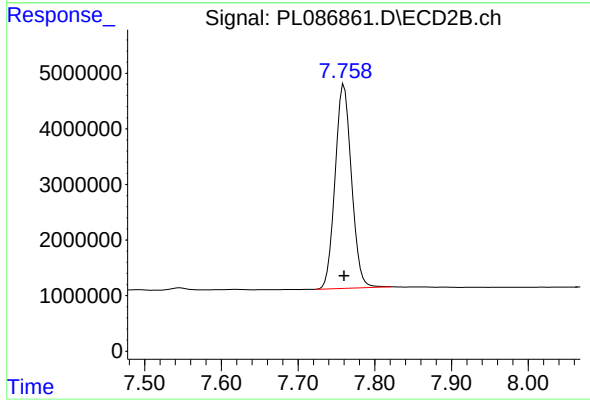

#28 Decachlorobiphenyl

R.T.: 7.760 min

Delta R.T.: 0.000 min

Response: 54543482

Conc: 50.00 ng/ml