

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112923\
 Data File : PL086862.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2023 04:31
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 04:57:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112923.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 29 04:57:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.342	2.609	76868957	26127749	24.617	24.480
28)	SA Decachlor...	8.843	7.761	67715294	28405942	26.244	26.430
Target Compounds							
23)	Chlordane-1	4.499	3.597	33356815	8991748	246.651	255.223
24)	Chlordane-2	5.032	4.175	37026650	10857157	258.438	256.460
25)	Chlordane-3	5.745	4.804	133.2E6	27469786	239.093	235.990
26)	Chlordane-4	5.827	4.866	168.9E6	32996098	243.830	250.069
27)	Chlordane-5	6.674	5.537	25485460	7901511	247.085	242.715



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112923\
Data File : PL086862.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2023 04:31
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 04:57:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112923.M
Quant Title : GC Extractables
QLast Update : Wed Nov 29 04:57:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

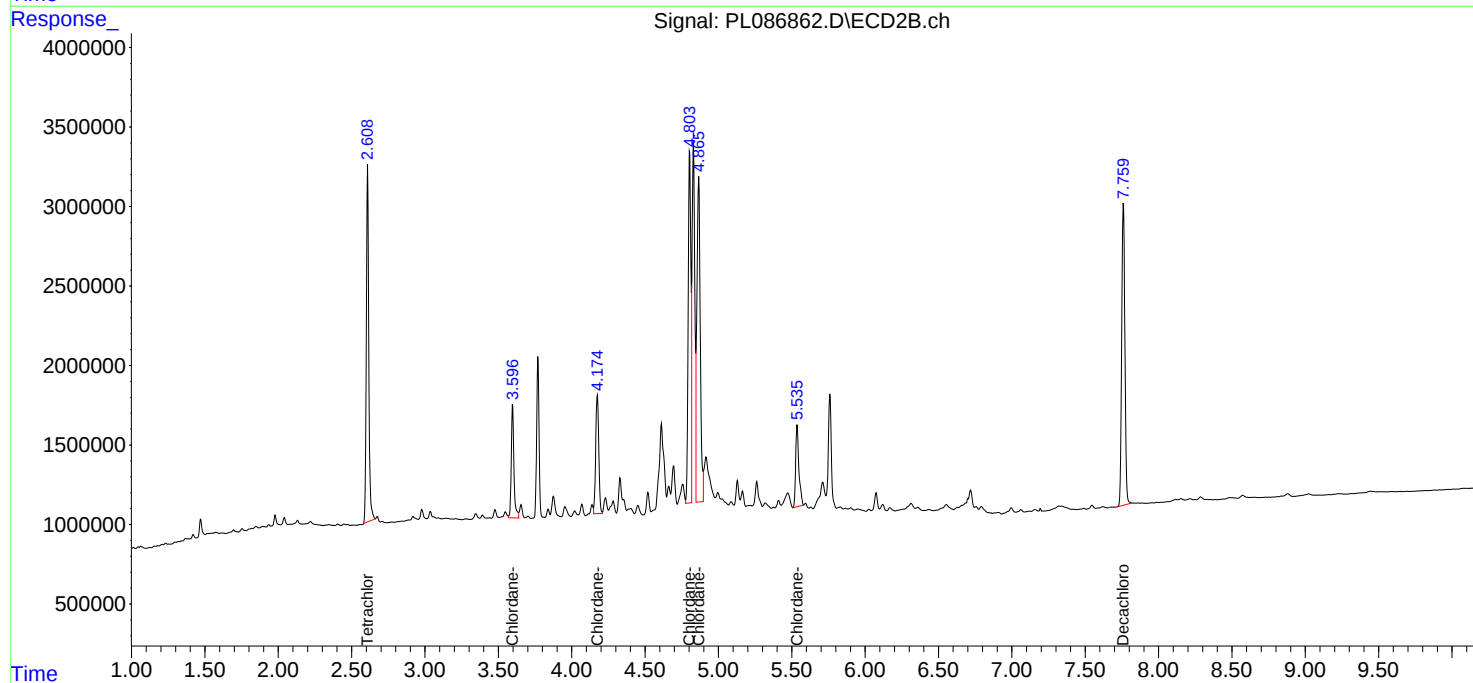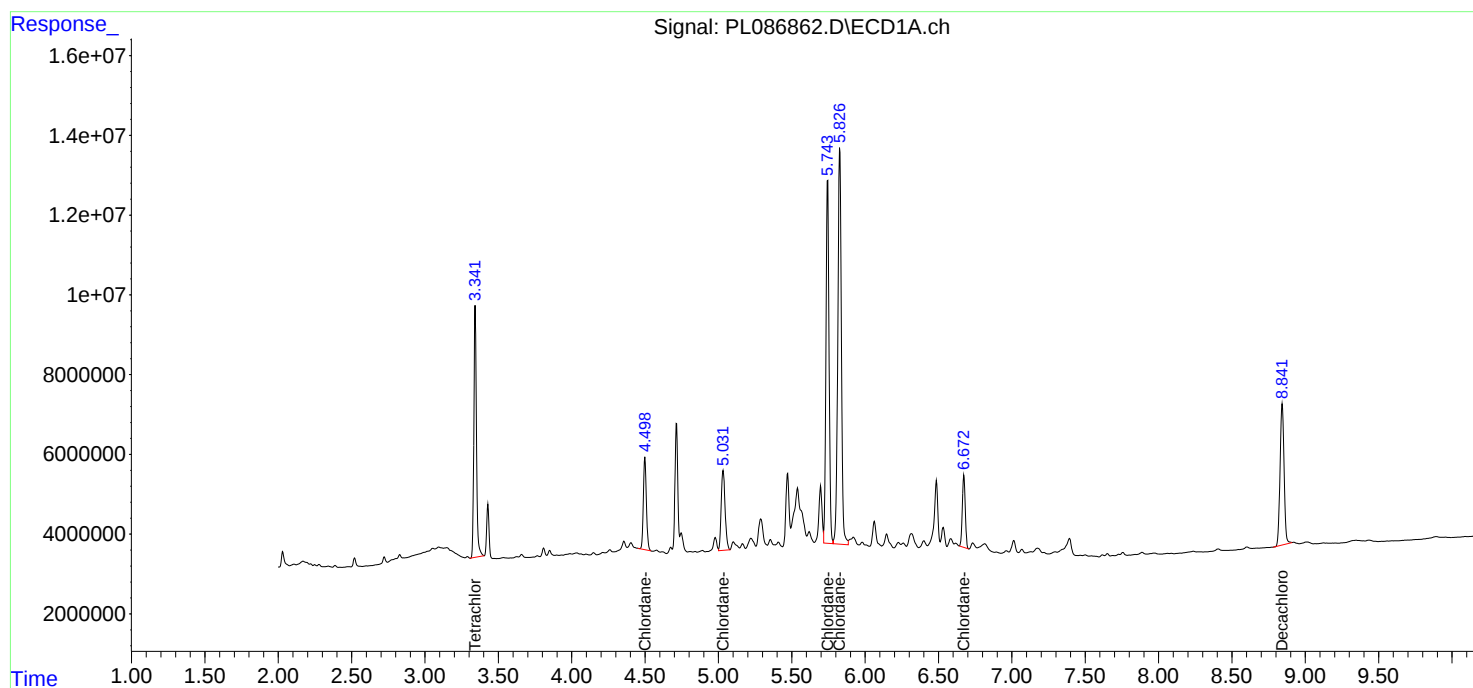


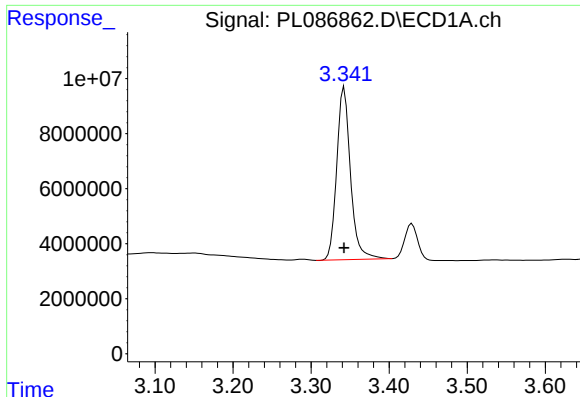

#1 Tetrachloro-m-xylene


R.T.: 3.342 min
Delta R.T.: 0.000 min
Response: 76868957
Conc: 24.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

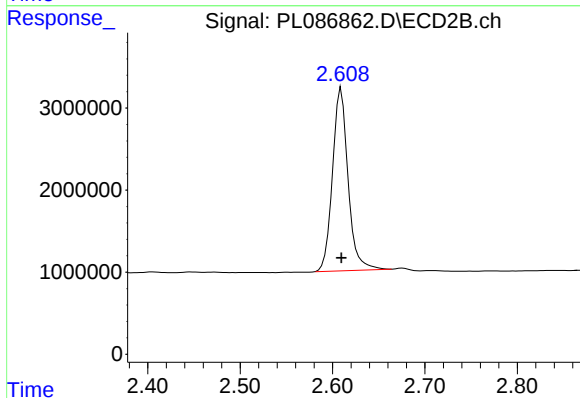


#1 Tetrachloro-m-xylene

R.T.: 2.609 min
Delta R.T.: 0.000 min
Response: 26127749
Conc: 24.48 ng/ml

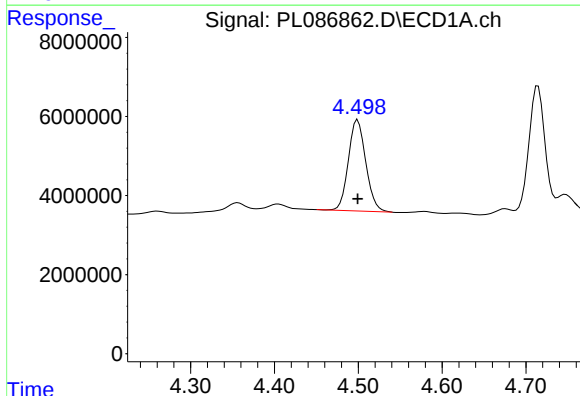


#23 Chlordane-1

R.T.: 4.499 min
Delta R.T.: 0.000 min
Response: 33356815
Conc: 246.65 ng/ml

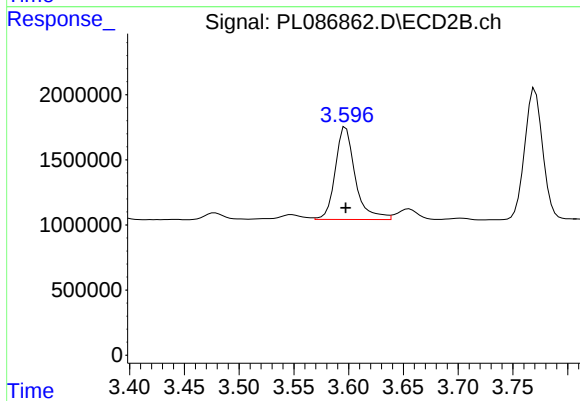

#23 Chlordane-1


R.T.: 3.597 min
Delta R.T.: 0.000 min
Response: 8991748
Conc: 255.22 ng/ml

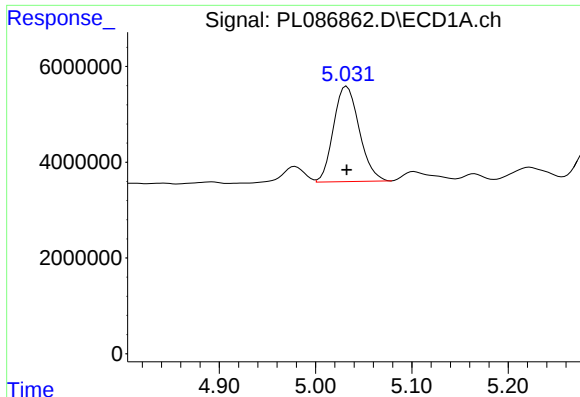

#24 Chlordane-2


R.T.: 5.032 min
Delta R.T.: 0.000 min
Response: 37026650
Conc: 258.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

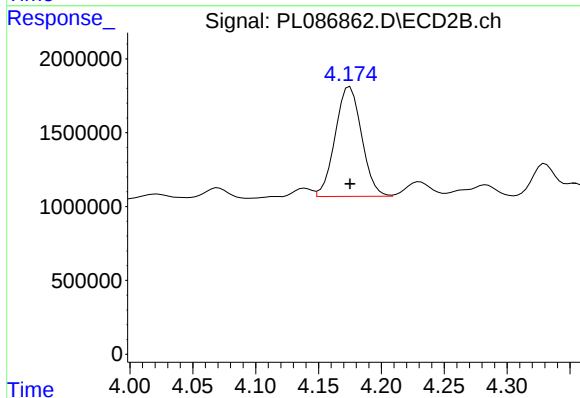


#24 Chlordane-2

R.T.: 4.175 min
Delta R.T.: 0.000 min
Response: 10857157
Conc: 256.46 ng/ml

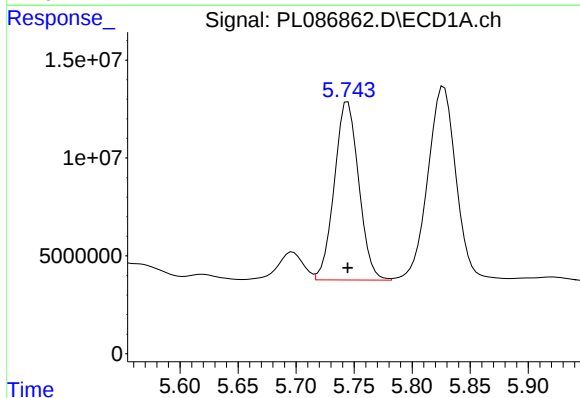


#25 Chlordane-3

R.T.: 5.745 min
Delta R.T.: 0.000 min
Response: 133179567
Conc: 239.09 ng/ml

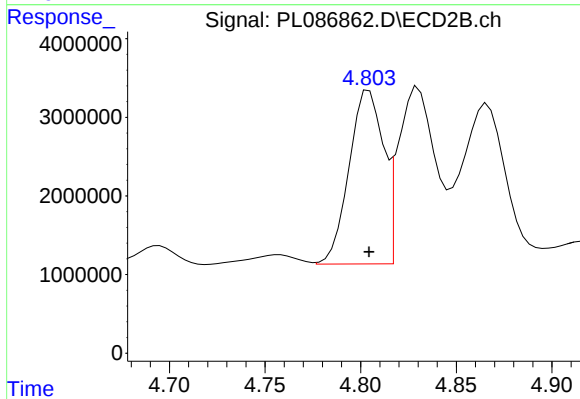

#25 Chlordane-3


R.T.: 4.804 min
Delta R.T.: 0.000 min
Response: 27469786
Conc: 235.99 ng/ml

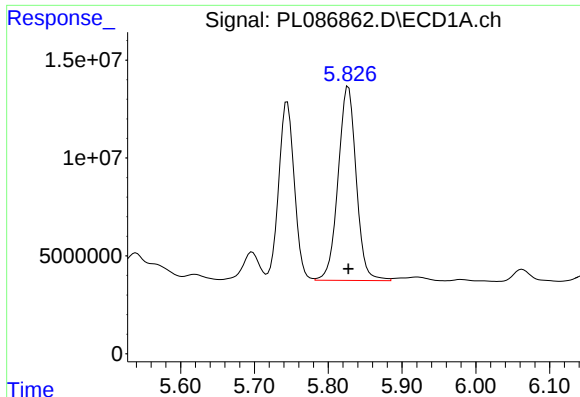

#26 Chlordane-4


R.T.: 5.827 min
Delta R.T.: 0.000 min
Response: 168875321
Conc: 243.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

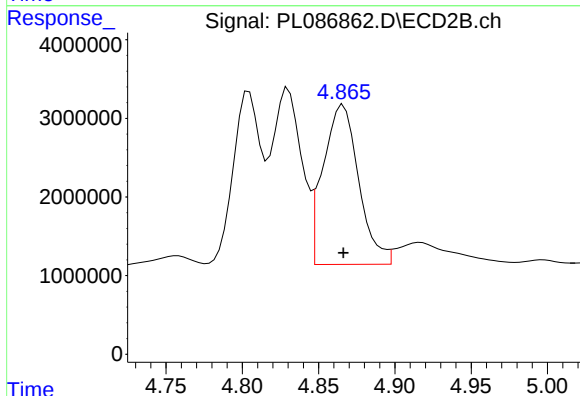


#26 Chlordane-4

R.T.: 4.866 min
Delta R.T.: 0.000 min
Response: 32996098
Conc: 250.07 ng/ml

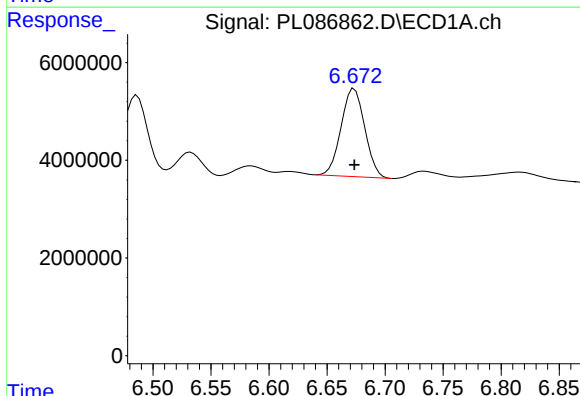


#27 Chlordane-5

R.T.: 6.674 min
Delta R.T.: 0.000 min
Response: 25485460
Conc: 247.09 ng/ml

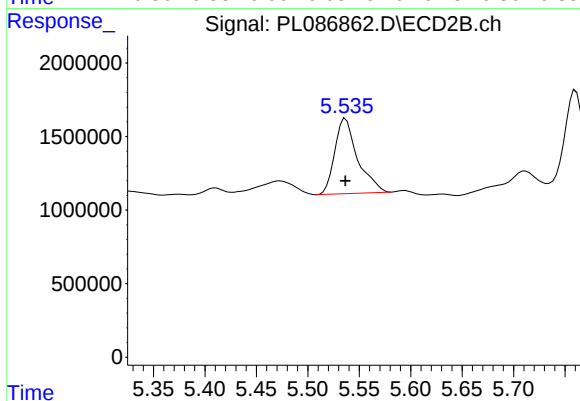

#27 Chlordane-5


R.T.: 5.537 min
Delta R.T.: 0.000 min
Response: 7901511
Conc: 242.71 ng/ml

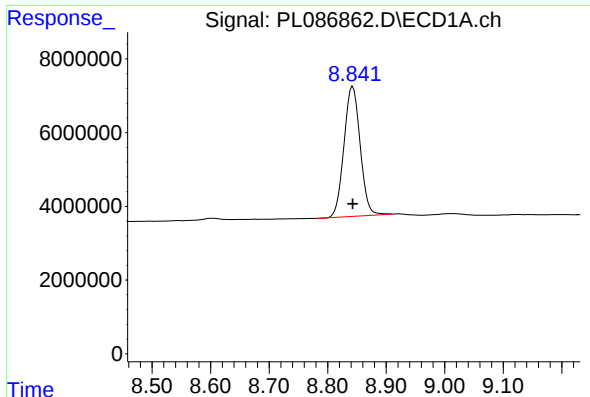

#28 Decachlorobiphenyl

R.T.: 8.843 min
Delta R.T.: 0.000 min
Response: 67715294
Conc: 26.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

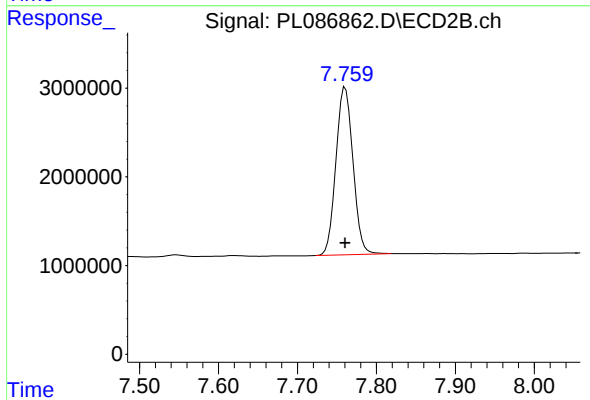

#28 Decachlorobiphenyl

R.T.: 7.761 min
Delta R.T.: 0.000 min
Response: 28405942
Conc: 26.43 ng/ml