

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL113018\
 Data File : PL042626.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2018 15:35
 Operator : AJ\SJ
 Sample : PB115197BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 00:09:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	4.100	104.7E6	49098395	17.792	17.071
28)	SA Decachlor...	8.215	9.237	106.7E6	41362572	16.927	17.150
Target Compounds							
6)	B beta-BHC	4.411f	0.000	6053653	0	1.709	N.D. #
9)	A Endosulfan I	0.000	6.317f	0	14680881	N.D.	4.649 #
10)	B gamma-Chl...	0.000	6.183f	0	9919046	N.D.	2.914 #
11)	B alpha-Chl...	0.000	6.317	0	14680881	N.D.	4.390 #
18)	B Endrin al...	0.000	7.123f	0	1358069	N.D.	0.592 #
19)	B Endosulfa...	6.695	0.000	1570289	0	0.252	N.D. #
25)	Chlordane-3	0.000	6.183	0	9919046	N.D.	21.108 #
26)	Chlordane-4	0.000	6.317	0	14680881	N.D.	26.831 #
27)	Chlordane-5	0.000	7.123	0	1358069	N.D.	14.118 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL113018\
Data File : PL042626.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2018 15:35
Operator : AJ\SJ
Sample : PB115197BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 00:09:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

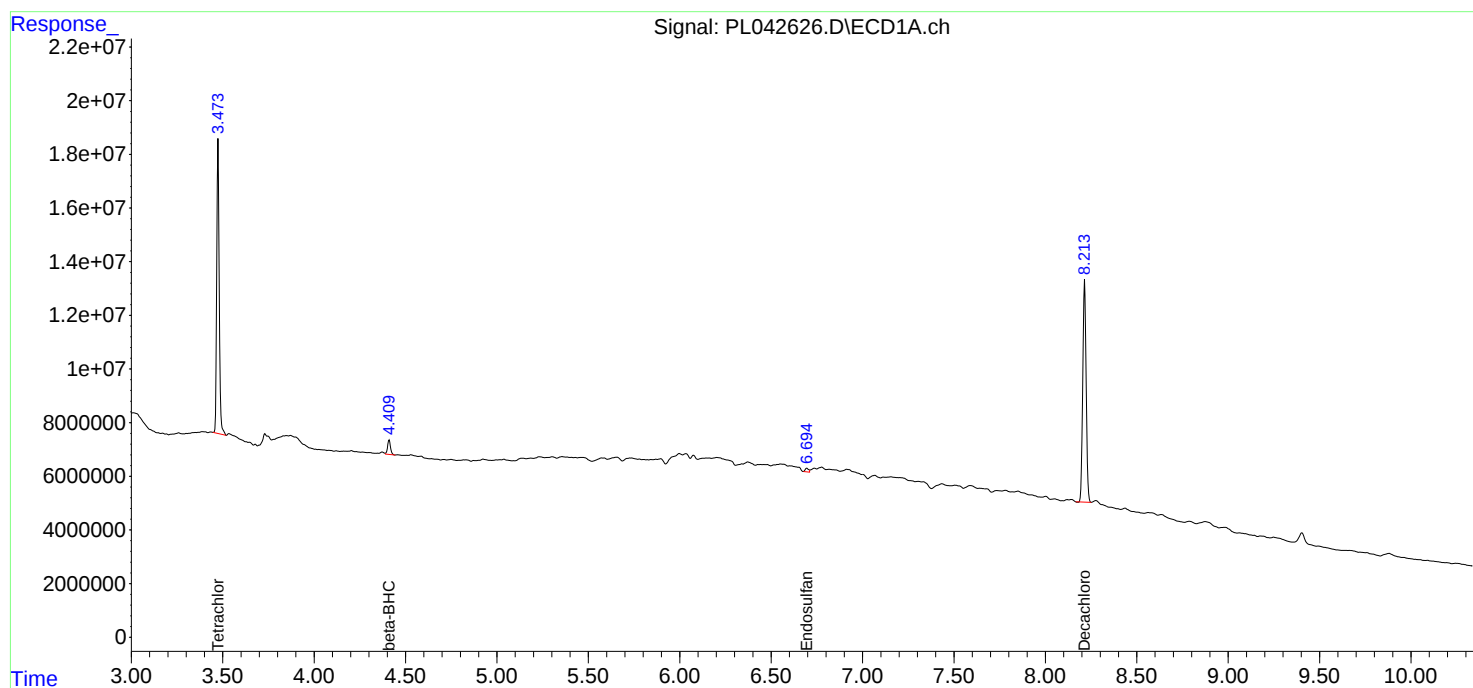


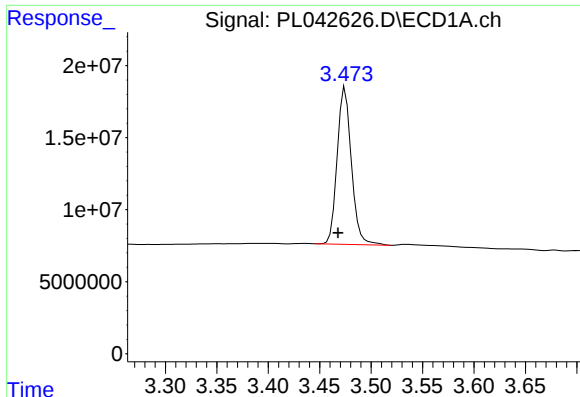

#1 Tetrachloro-m-xylene


R.T.: 3.475 min
Delta R.T.: 0.007 min
Response: 104678424
Conc: 17.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

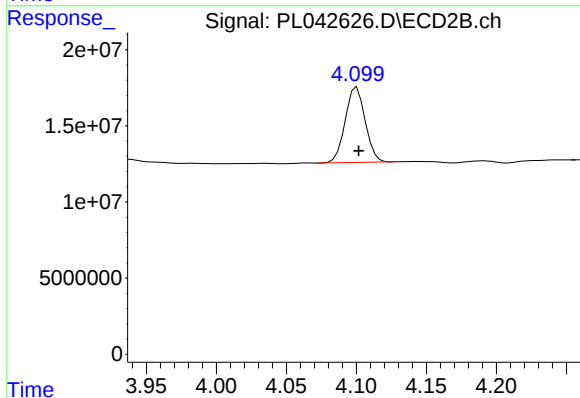


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: -0.001 min
Response: 49098395
Conc: 17.07 ng/ml

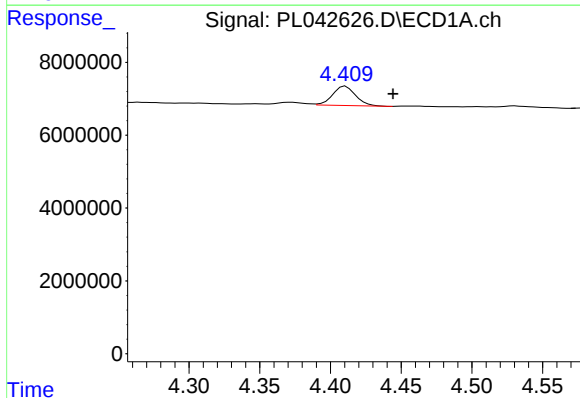


#6 beta-BHC

R.T.: 4.411 min
Delta R.T.: -0.034 min
Response: 6053653
Conc: 1.71 ng/ml

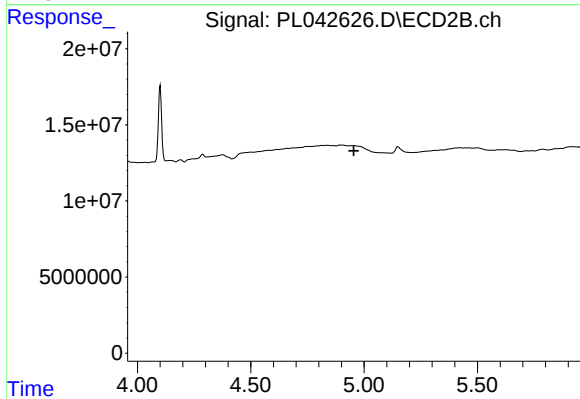

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

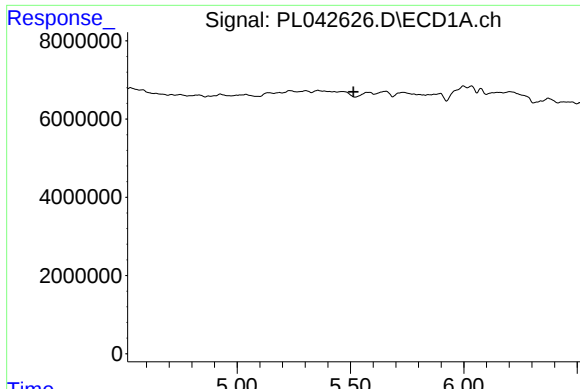

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.514 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

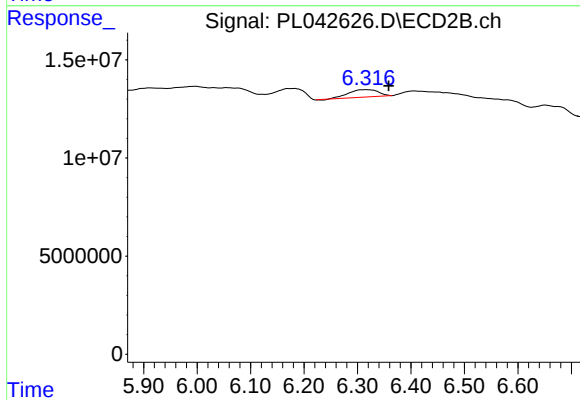


#9 Endosulfan I

R.T.: 6.317 min
Delta R.T.: -0.041 min
Response: 14680881
Conc: 4.65 ng/ml

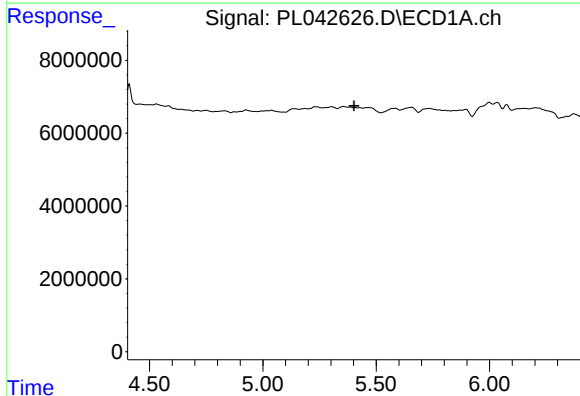


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

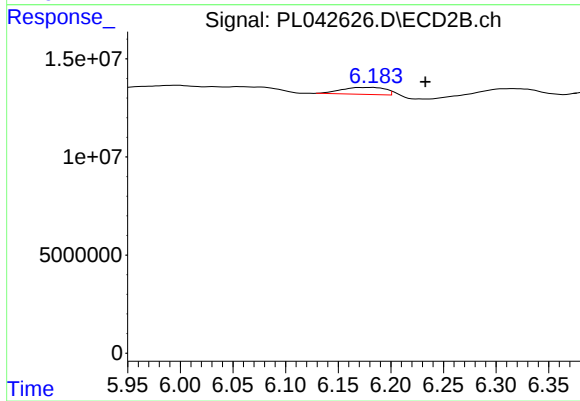

#10 gamma-Chlordane


R.T.: 6.183 min
Delta R.T.: -0.050 min
Response: 9919046
Conc: 2.91 ng/ml

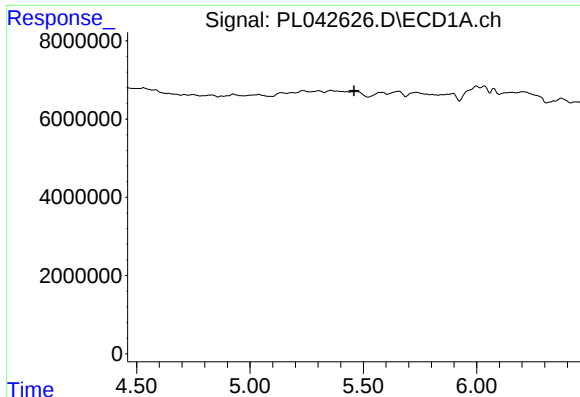

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

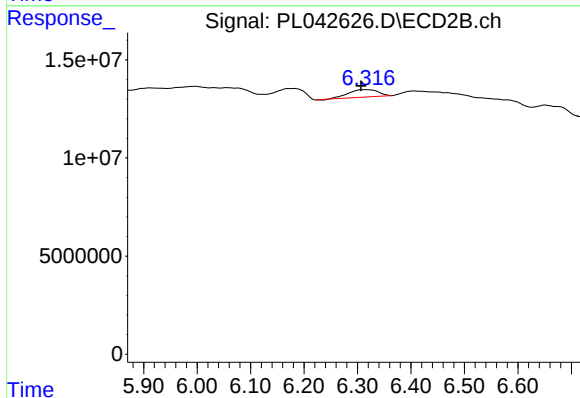


#11 alpha-Chlordane

R.T.: 6.317 min
Delta R.T.: 0.010 min
Response: 14680881
Conc: 4.39 ng/ml

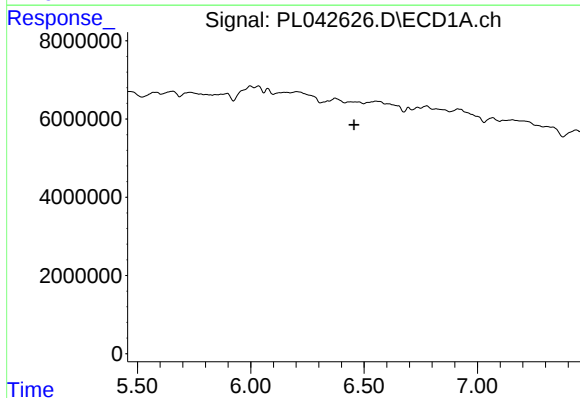


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.456 min
Response: 0
Conc: N.D.

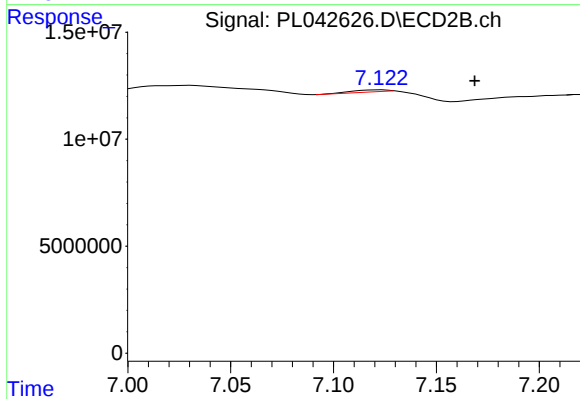

#18 Endrin aldehyde


R.T.: 7.123 min
Delta R.T.: -0.045 min
Response: 1358069
Conc: 0.59 ng/ml

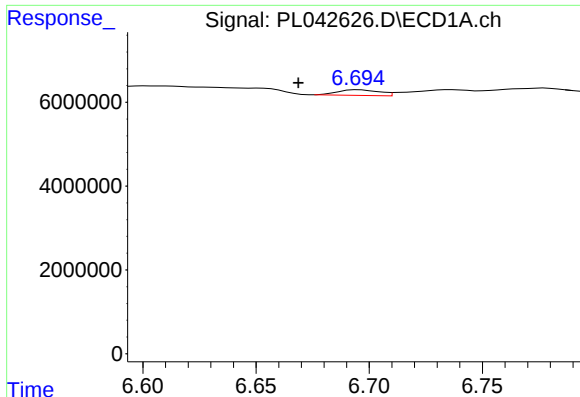

#19 Endosulfan Sulfate


R.T.: 6.695 min
Delta R.T.: 0.027 min
Response: 1570289
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

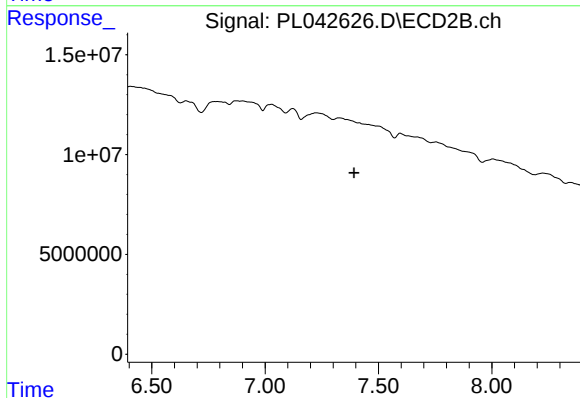


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

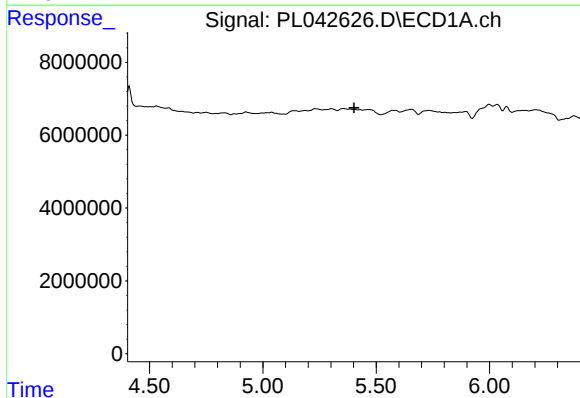


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

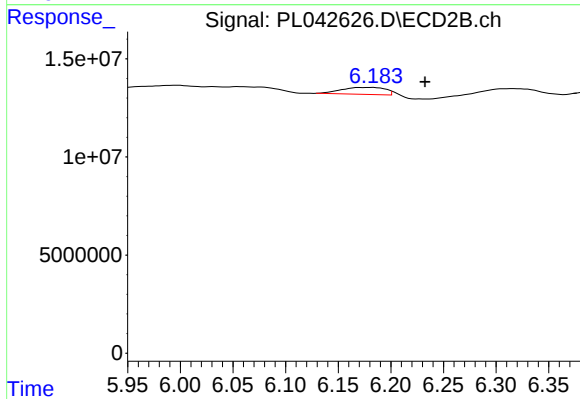

#25 Chlordane-3


R.T.: 6.183 min
Delta R.T.: -0.049 min
Response: 9919046
Conc: 21.11 ng/ml

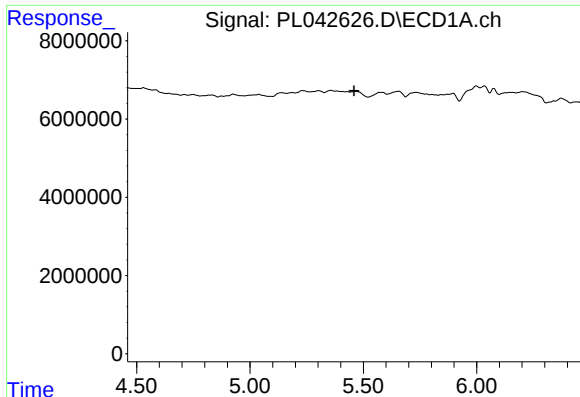

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

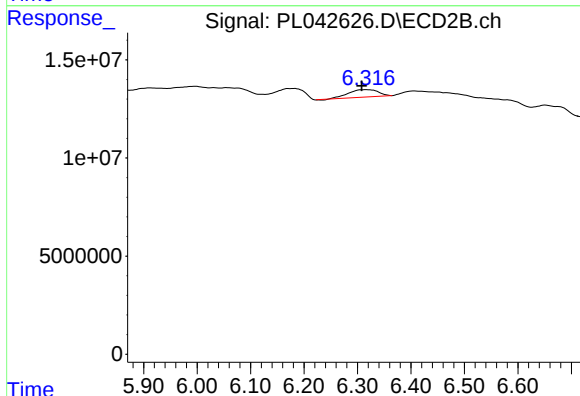


#26 Chlordane-4

R.T.: 6.317 min
Delta R.T.: 0.009 min
Response: 14680881
Conc: 26.83 ng/ml

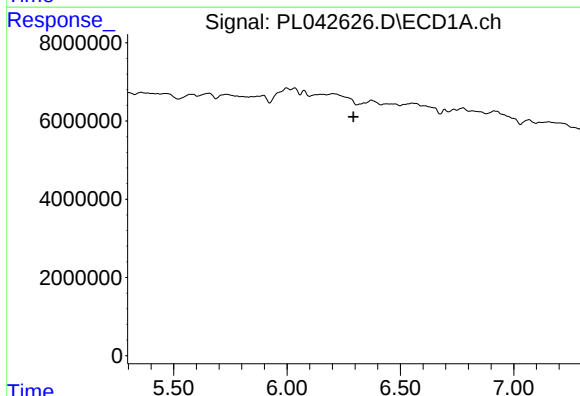


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.294 min
Response: 0
Conc: N.D.

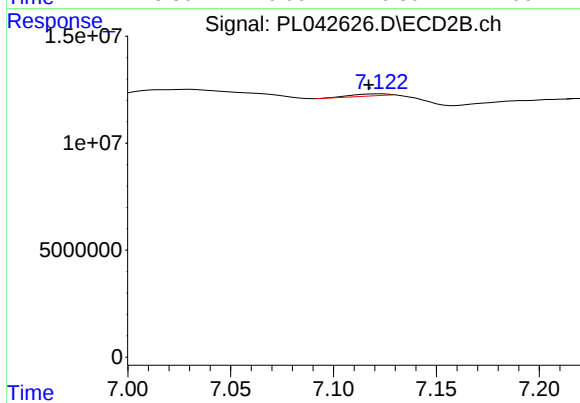

#27 Chlordane-5


R.T.: 7.123 min
Delta R.T.: 0.006 min
Response: 1358069
Conc: 14.12 ng/ml

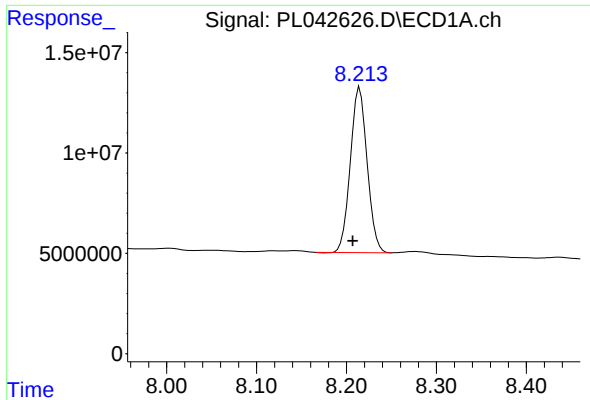

#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: 0.008 min
Response: 106672995
Conc: 16.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

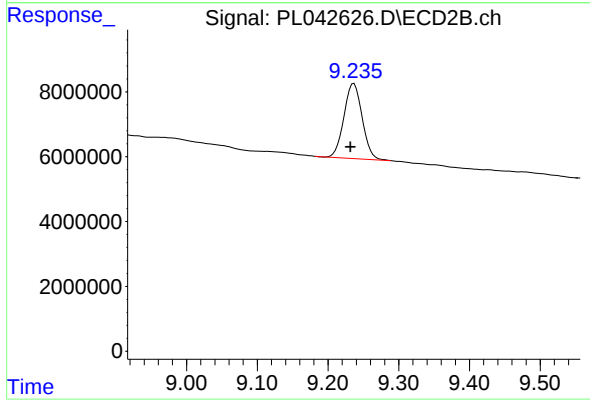

#28 Decachlorobiphenyl

R.T.: 9.237 min
Delta R.T.: 0.005 min
Response: 41362572
Conc: 17.15 ng/ml