

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL113018\
 Data File : PL042630.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2018 16:32
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 00:09:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.466	4.101	127.8E6	65465574	21.729	22.762
28)	SA Decachlor...	8.204	9.232	118.4E6	47421584	18.790	19.662
Target Compounds							
9)	A Endosulfan I	5.514	0.000	14906597	0	2.154	N.D. #
10)	B gamma-Chl...	5.464f	0.000	35508545	0	4.657	N.D. #
11)	B alpha-Chl...	5.464	0.000	35508545	0	4.730	N.D. #
20)	A Methoxychlor	0.000	7.727	0	2490041	N.D.	1.826 #
25)	Chlordane-3	5.464	0.000	35508545	0	40.508	N.D. #
26)	Chlordane-4	5.464	0.000	35508545	0	46.788	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL113018\
Data File : PL042630.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2018 16:32
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 00:09:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

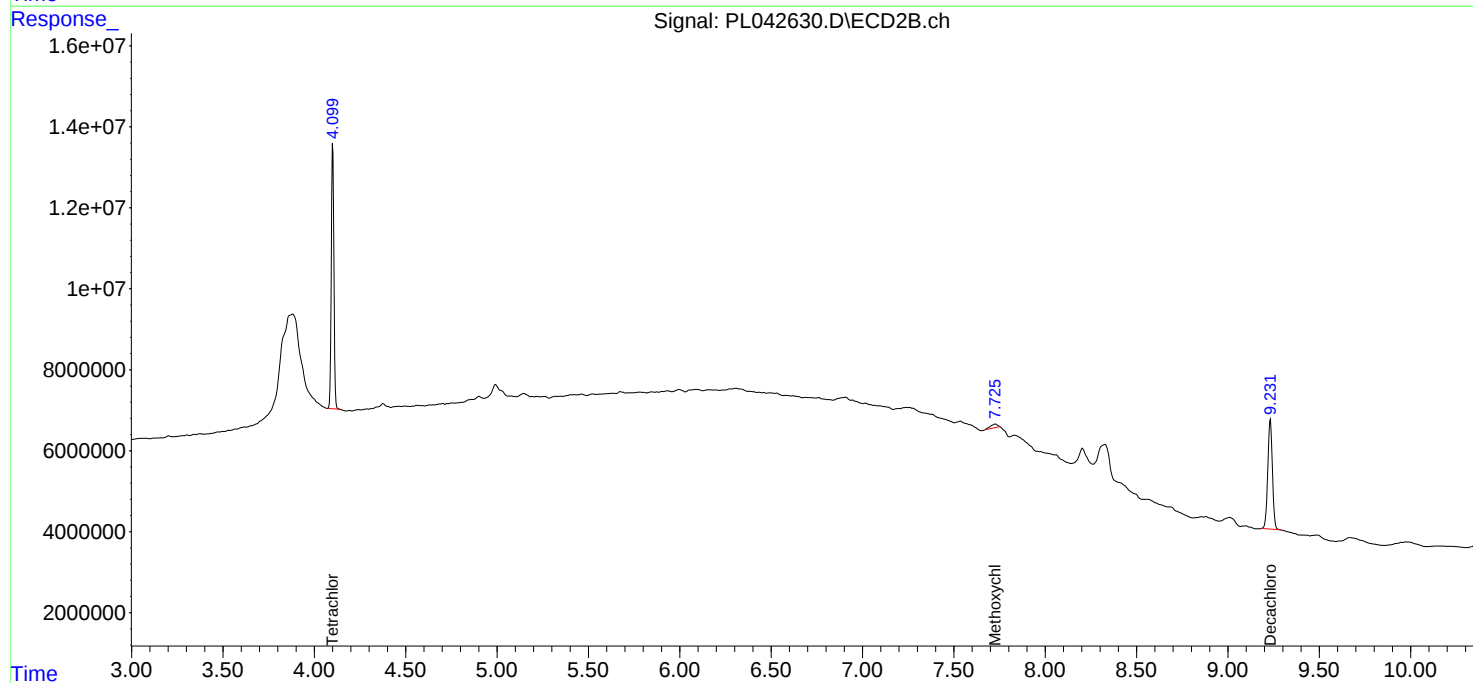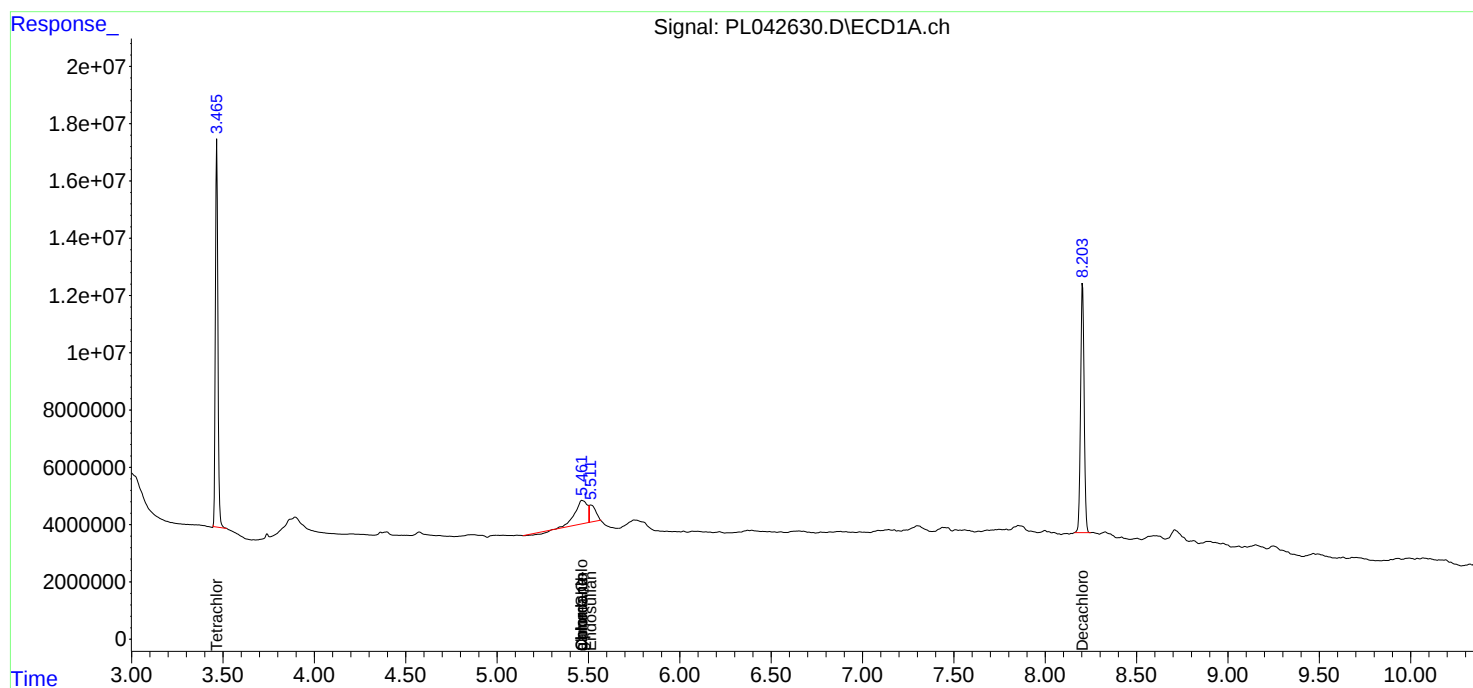


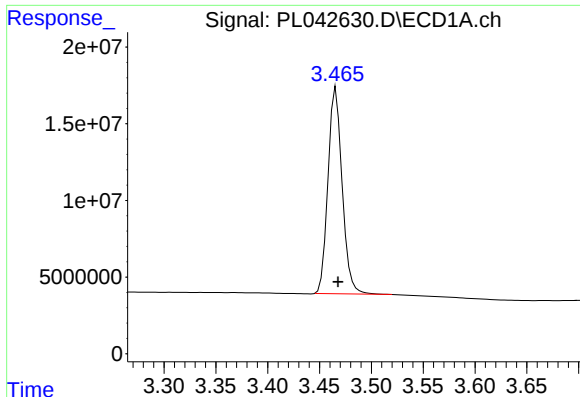

#1 Tetrachloro-m-xylene


R.T.: 3.466 min
Delta R.T.: -0.002 min
Response: 127839957
Conc: 21.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

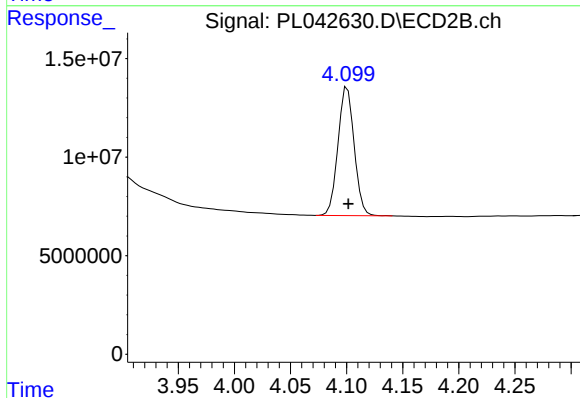


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 65465574
Conc: 22.76 ng/ml

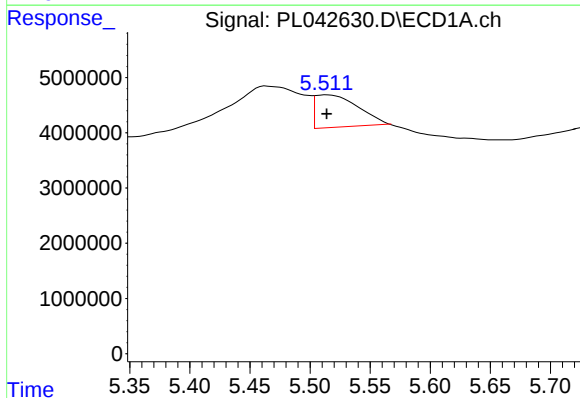


#9 Endosulfan I

R.T.: 5.514 min
Delta R.T.: 0.000 min
Response: 14906597
Conc: 2.15 ng/ml

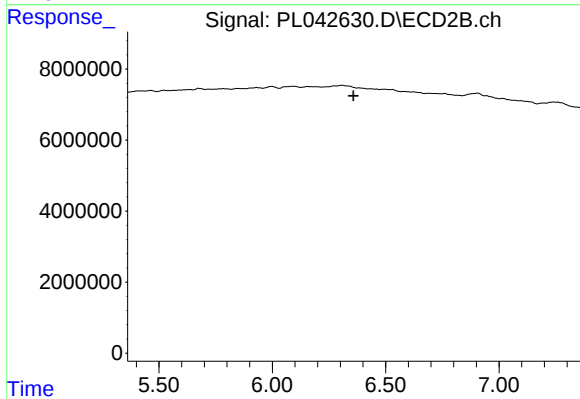

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.358 min
Response: 0
Conc: N.D.

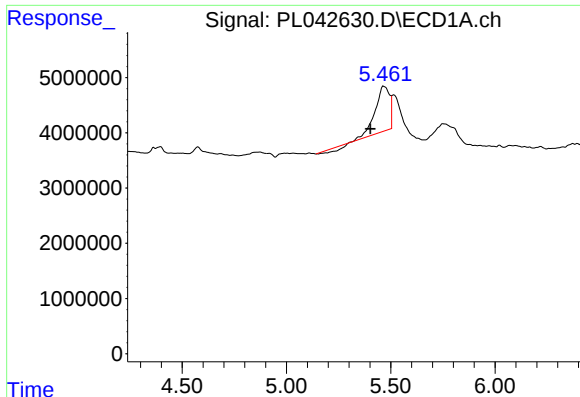

#10 gamma-Chlordane


R.T.: 5.464 min
Delta R.T.: 0.062 min
Response: 35508545
Conc: 4.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

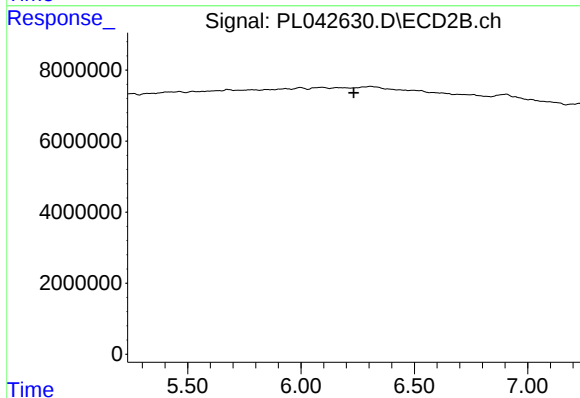


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.233 min
Response: 0
Conc: N.D.

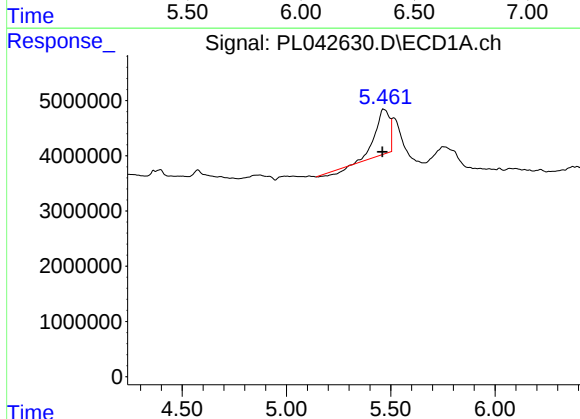


#11 alpha-Chlordane

R.T.: 5.464 min
Delta R.T.: 0.004 min
Response: 35508545
Conc: 4.73 ng/ml

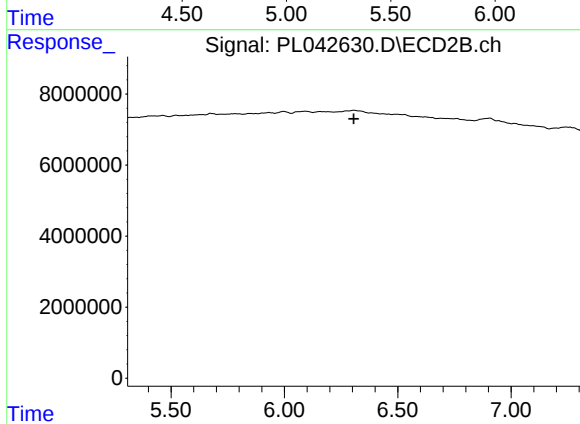

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.307 min
Response: 0
Conc: N.D.

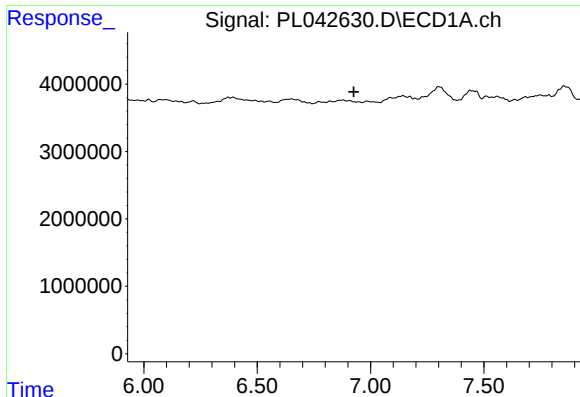

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.926 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

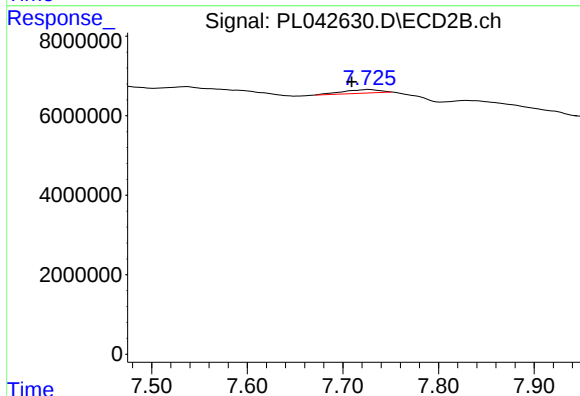


#20 Methoxychlor

R.T.: 7.727 min
Delta R.T.: 0.018 min
Response: 2490041
Conc: 1.83 ng/ml

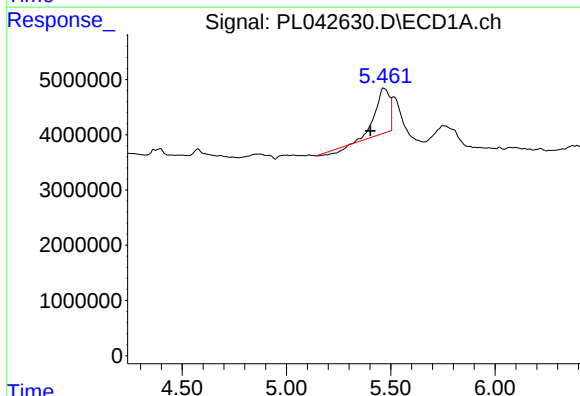


#25 Chlordane-3

R.T.: 5.464 min
Delta R.T.: 0.061 min
Response: 35508545
Conc: 40.51 ng/ml

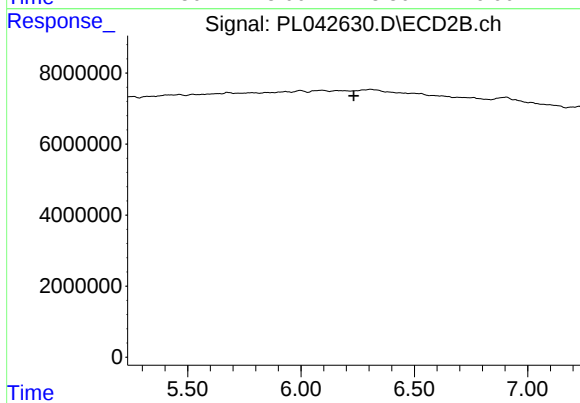

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.233 min
Response: 0
Conc: N.D.

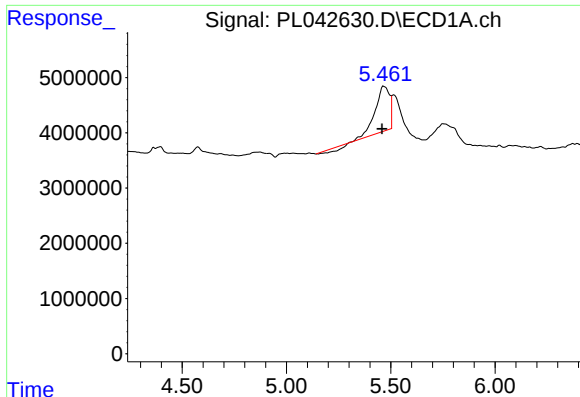

#26 Chlordane-4


R.T.: 5.464 min
Delta R.T.: 0.005 min
Response: 35508545
Conc: 46.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

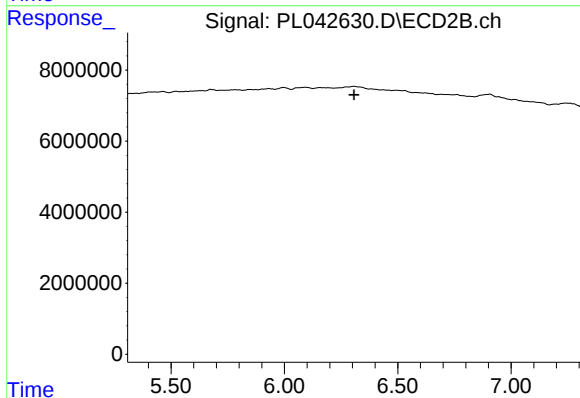


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.308 min
Response: 0
Conc: N.D.

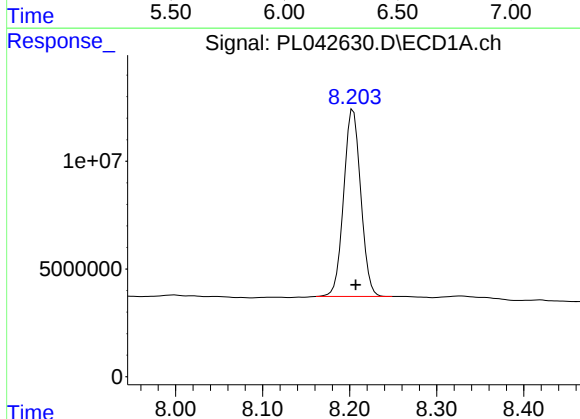

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.003 min
Response: 118418622
Conc: 18.79 ng/ml

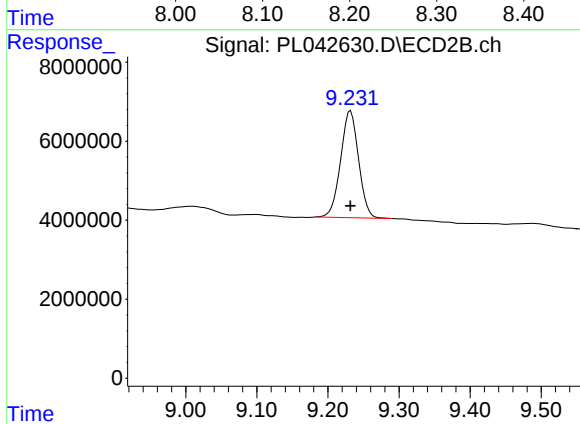

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.000 min
Response: 47421584
Conc: 19.66 ng/ml