

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL113018\
 Data File : PL042656.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2018 22:39
 Operator : AJ\SJ
 Sample : J5770-14
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 00:15:06 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.101	116.5E6	60591683	19.809	21.067
28)	SA Decachlor...	8.203	9.233	102.7E6	42903466	16.289	17.789
Target Compounds							
6)	B beta-BHC	4.401f	0.000	12748170	0	3.598	N.D. #
8)	B Heptachlo...	0.000	5.996	0	5213829	N.D.	1.454 #
9)	A Endosulfan I	5.490	6.334	8454707	3633167	1.222	1.150
10)	B gamma-Chl...	0.000	6.266	0	3547532	N.D.	1.042 #
11)	B alpha-Chl...	5.490	6.334	8454707	3633167	1.126	1.087
23)	Chlordane-1	4.364	0.000	1289610	0	4.665	N.D. #
24)	Chlordane-2	4.837	0.000	1690383	0	6.015	N.D. #
25)	Chlordane-3	0.000	6.266	0	3547532	N.D.	7.549 #
26)	Chlordane-4	5.490	6.334	8454707	3633167	11.140	6.640 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL113018\
Data File : PL042656.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2018 22:39
Operator : AJ\SJ
Sample : J5770-14
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 00:15:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

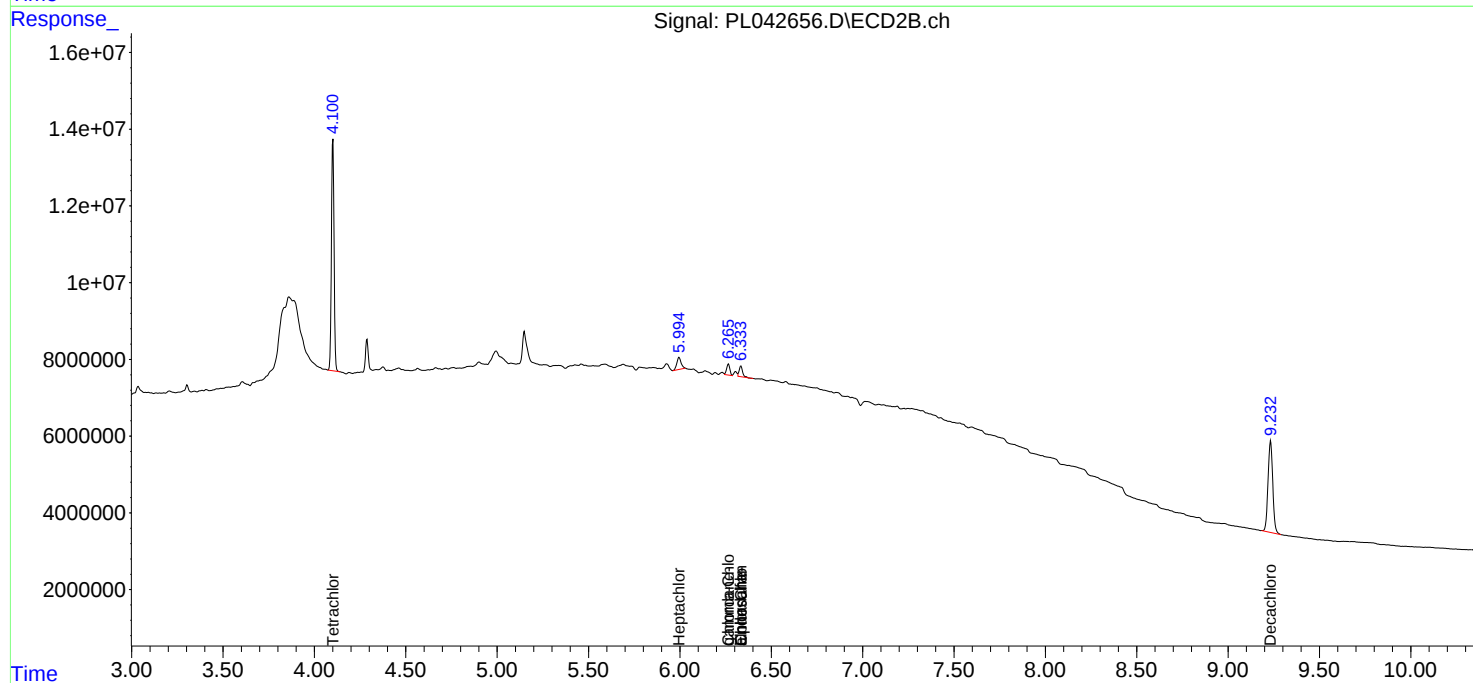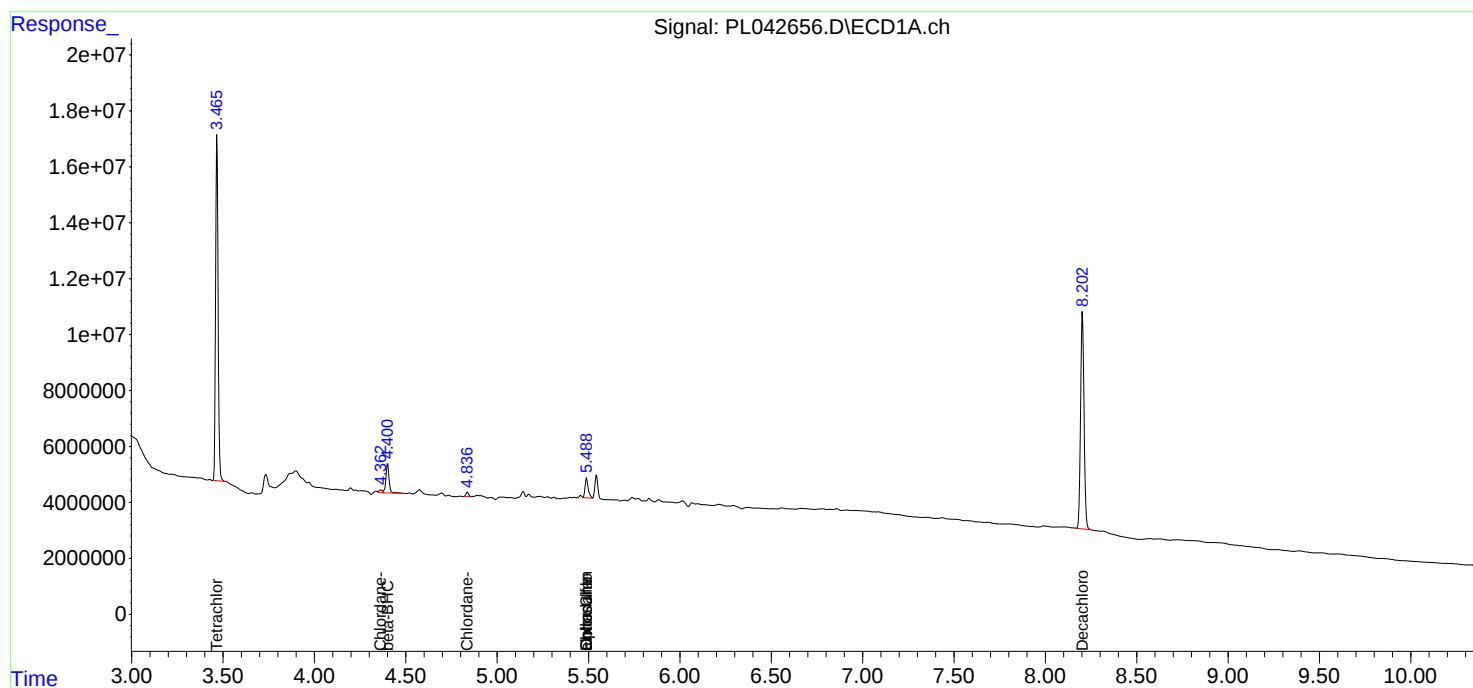


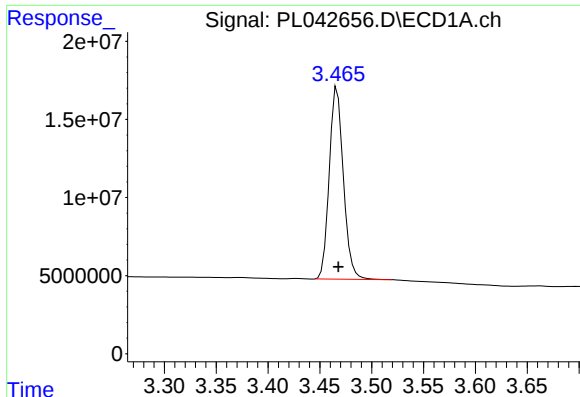

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: -0.001 min
Response: 116546426
Conc: 19.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

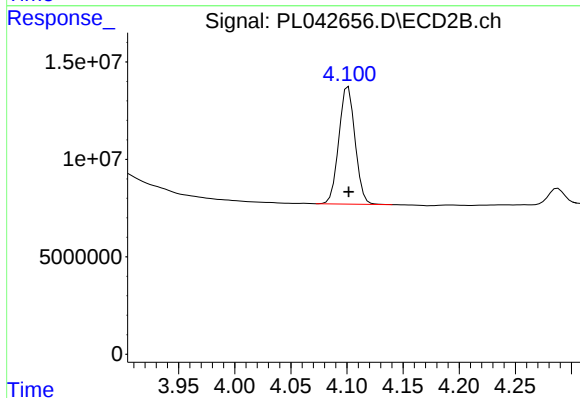


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 60591683
Conc: 21.07 ng/ml

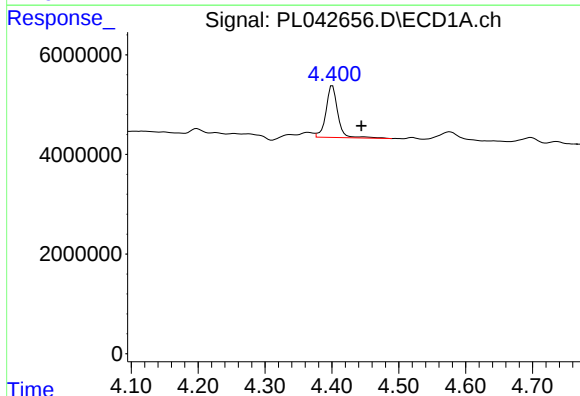


#6 beta-BHC

R.T.: 4.401 min
Delta R.T.: -0.043 min
Response: 12748170
Conc: 3.60 ng/ml

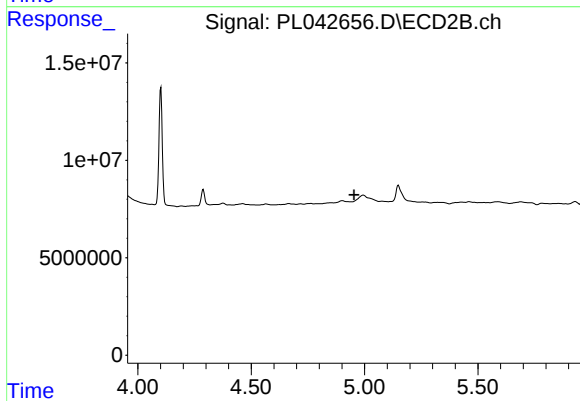

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

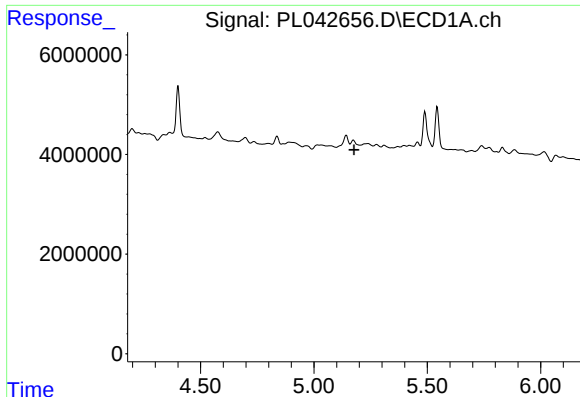

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

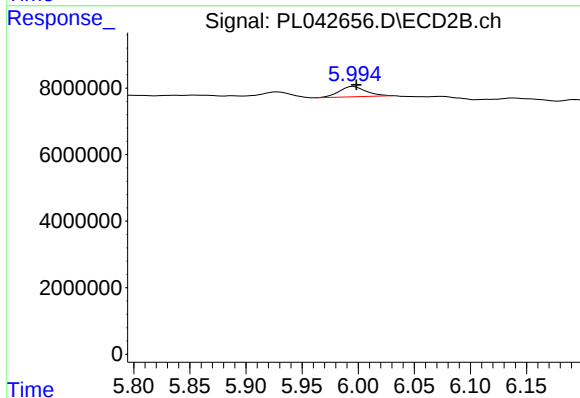


#8 Heptachlor epoxide

R.T.: 5.996 min
Delta R.T.: -0.003 min
Response: 5213829
Conc: 1.45 ng/ml

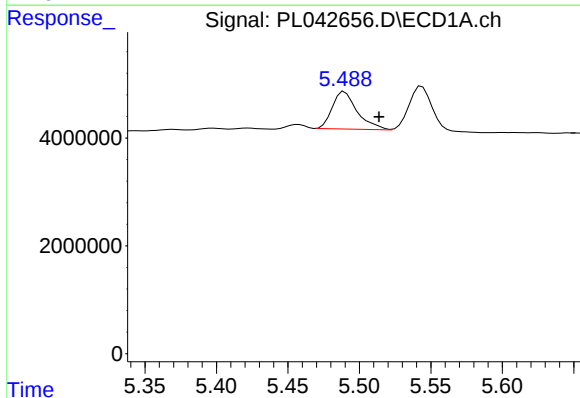


#9 Endosulfan I

R.T.: 5.490 min
Delta R.T.: -0.024 min
Response: 8454707
Conc: 1.22 ng/ml

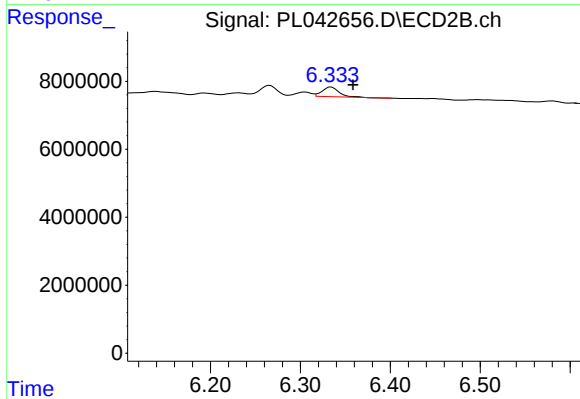

#9 Endosulfan I


R.T.: 6.334 min
Delta R.T.: -0.024 min
Response: 3633167
Conc: 1.15 ng/ml

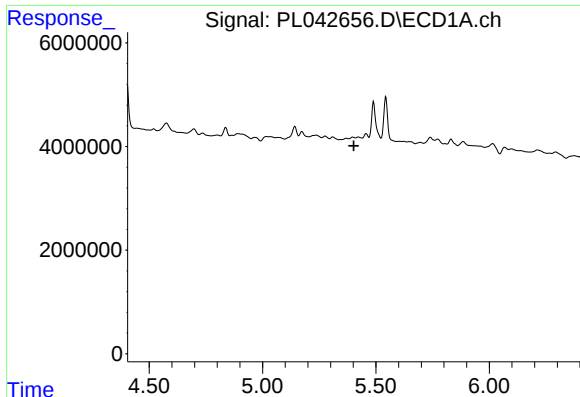

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

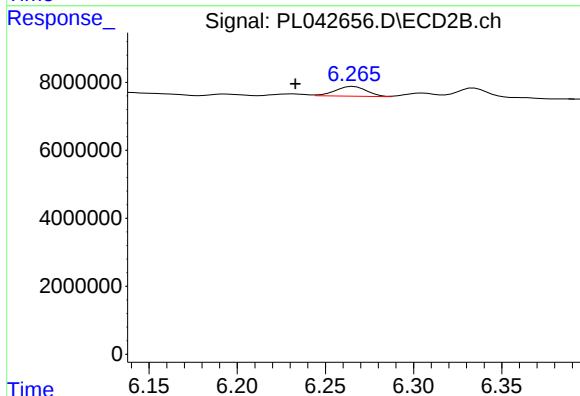


#10 gamma-Chlordane

R.T.: 6.266 min
Delta R.T.: 0.033 min
Response: 3547532
Conc: 1.04 ng/ml

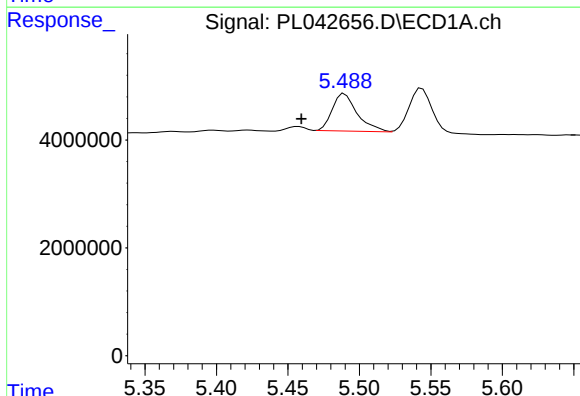


#11 alpha-Chlordane

R.T.: 5.490 min
Delta R.T.: 0.030 min
Response: 8454707
Conc: 1.13 ng/ml

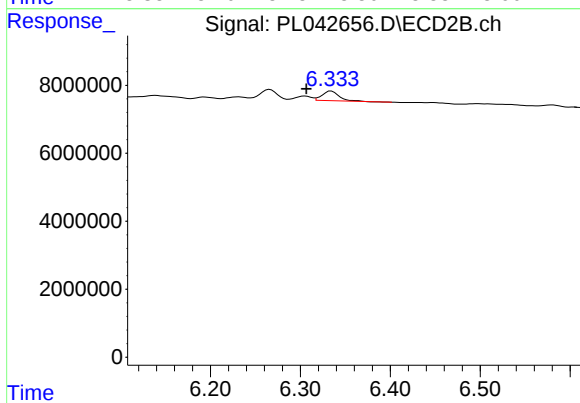

#11 alpha-Chlordane


R.T.: 6.334 min
Delta R.T.: 0.028 min
Response: 3633167
Conc: 1.09 ng/ml

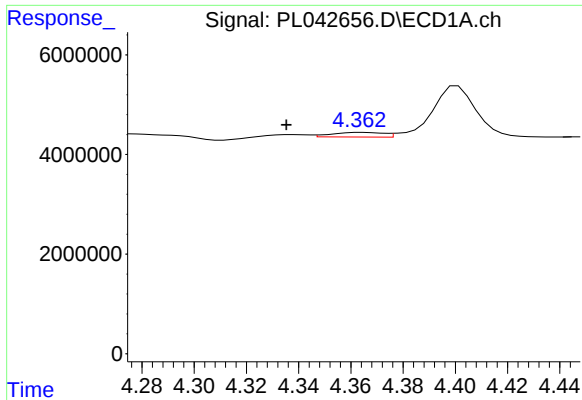

#23 Chlordane-1


R.T.: 4.364 min
Delta R.T.: 0.029 min
Response: 1289610
Conc: 4.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

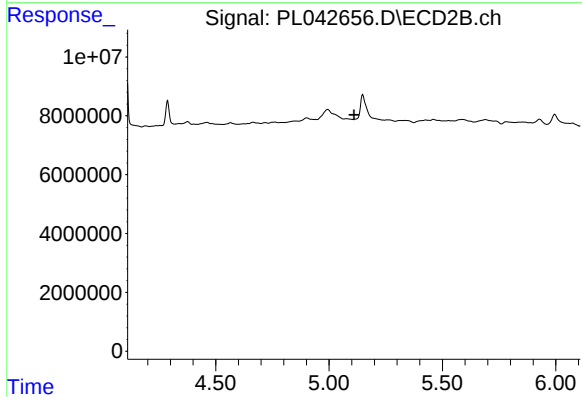


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

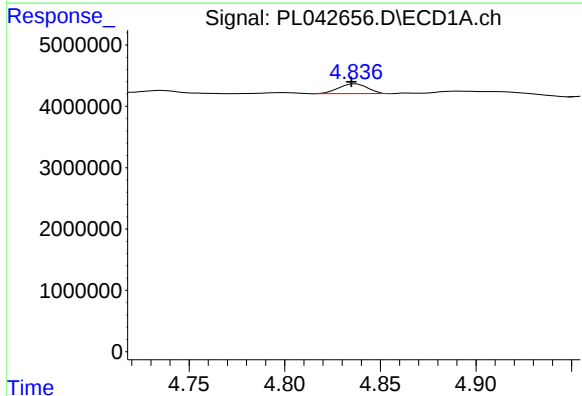


#24 Chlordane-2

R.T.: 4.837 min
Delta R.T.: 0.002 min
Response: 1690383
Conc: 6.02 ng/ml

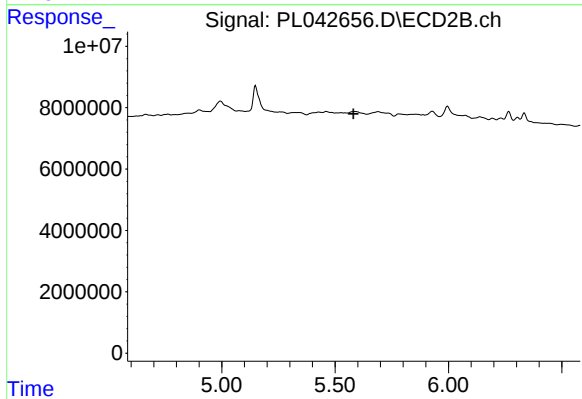

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.582 min
Response: 0
Conc: N.D.

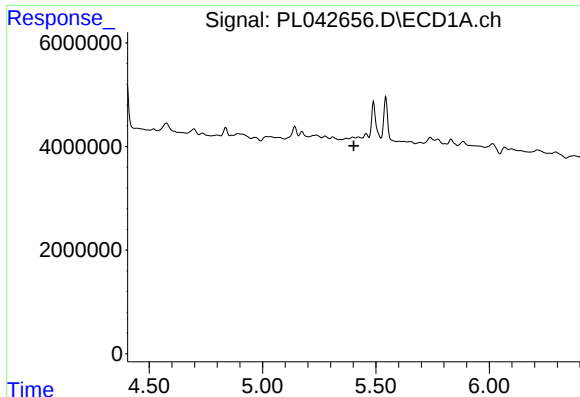

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

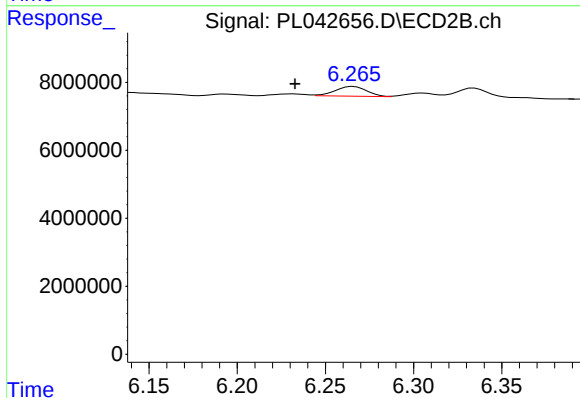


#25 Chlordane-3

R.T.: 6.266 min
Delta R.T.: 0.033 min
Response: 3547532
Conc: 7.55 ng/ml

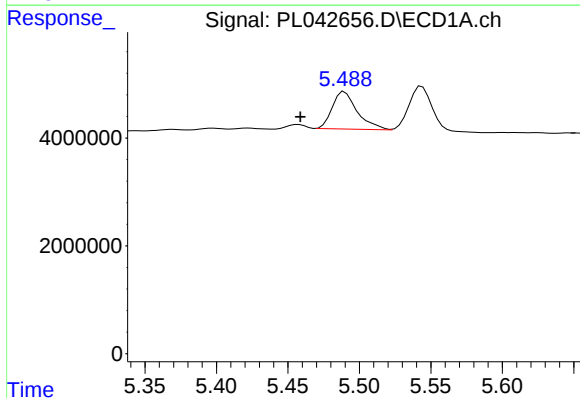


#26 Chlordane-4

R.T.: 5.490 min
Delta R.T.: 0.031 min
Response: 8454707
Conc: 11.14 ng/ml

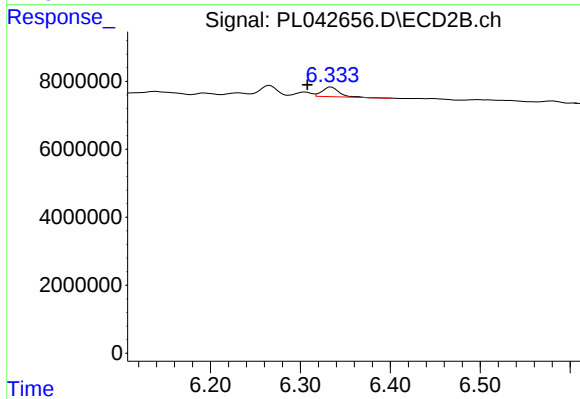

#26 Chlordane-4

R.T.: 6.334 min
Delta R.T.: 0.027 min
Response: 3633167
Conc: 6.64 ng/ml

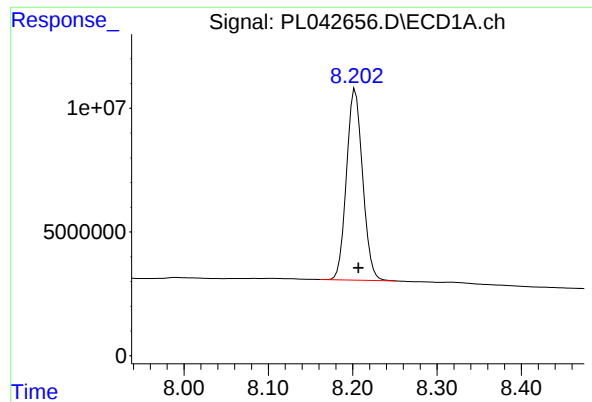

#28 Decachlorobiphenyl


R.T.: 8.203 min

Delta R.T.: -0.004 min

Response: 102657540

Conc: 16.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

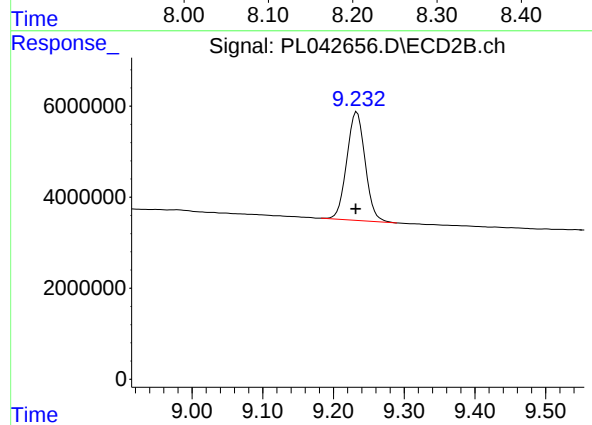

#28 Decachlorobiphenyl

R.T.: 9.233 min

Delta R.T.: 0.002 min

Response: 42903466

Conc: 17.79 ng/ml