

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL113021\
 Data File : PL071188.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2021 10:34
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 16:31:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

6) B	beta-BHC	0.000	6.726	0	21142804	N.D.	24.023 #
7) B	delta-BHC	0.000	7.023f	0	1744520	N.D.	1.026 #
8) B	Heptachlo...	7.015	0.000	170005	0	0.273	N.D. #
10) B	gamma-Chl...	0.000	8.222	0	1807962	N.D.	1.131 #
14) MA	Endrin	7.984	0.000	793014	0	1.402	N.D. #
15) B	Endosulfa...	8.269f	9.099f	8104831	9826291	13.881	7.293 #
17) MA	4,4'-DDT	0.000	9.338f	0	930195	N.D.	0.669 #
21) B	Endrin ke...	9.202f	0.000	2241875	0	3.146	N.D. #
25)	Chlordane-3	0.000	8.222	0	1807962	N.D.	8.222 #
27)	Chlordane-5	8.269f	0.000	8104831	0	339.542	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL113021\
Data File : PL071188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2021 10:34
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 16:31:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

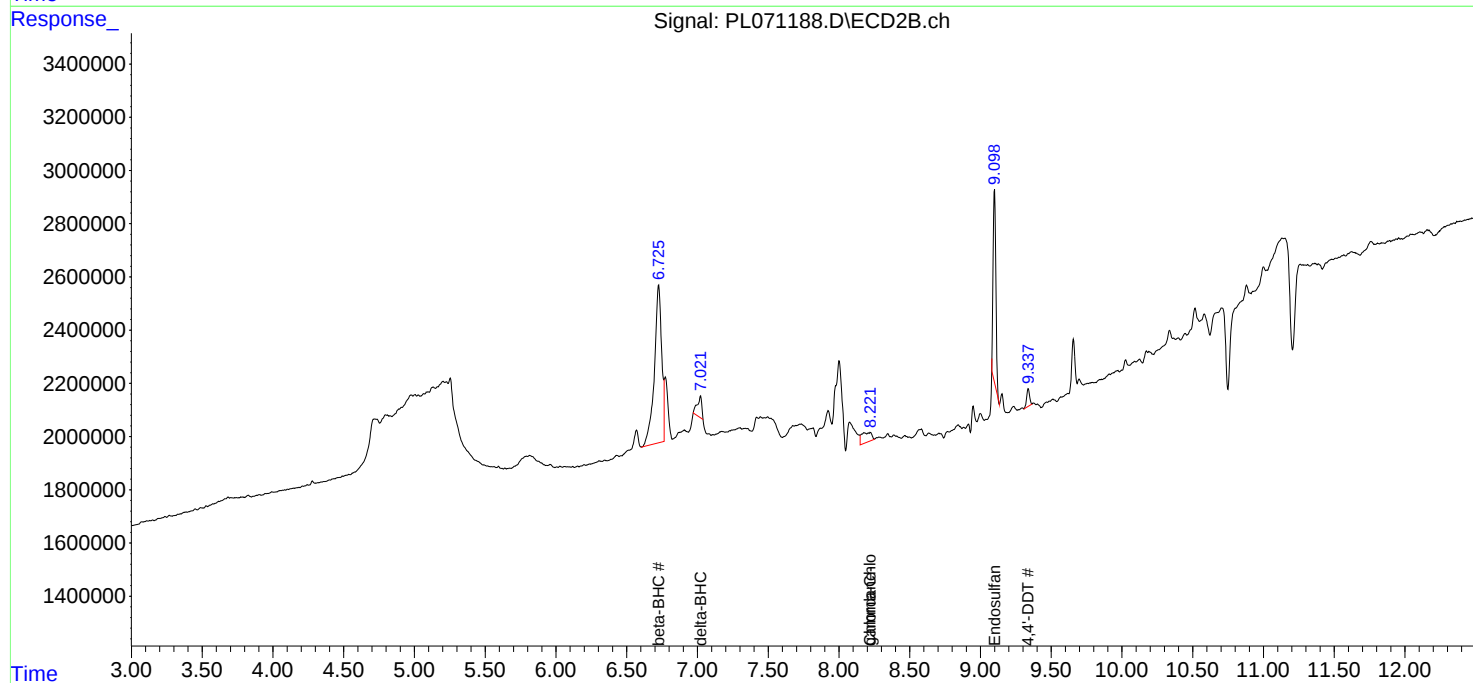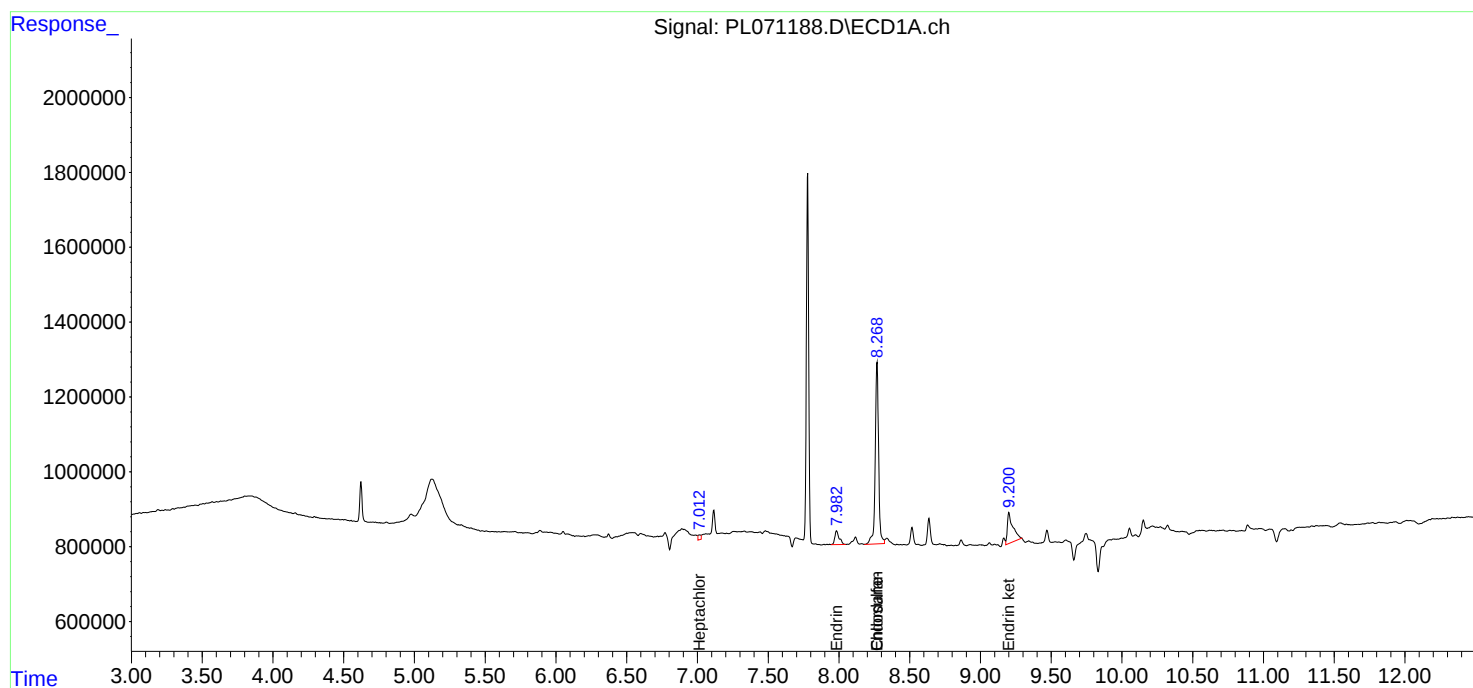


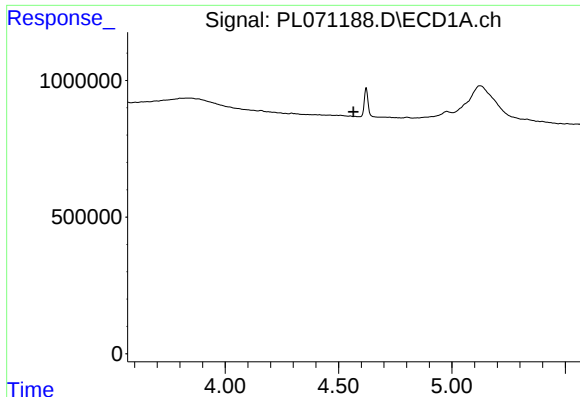

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

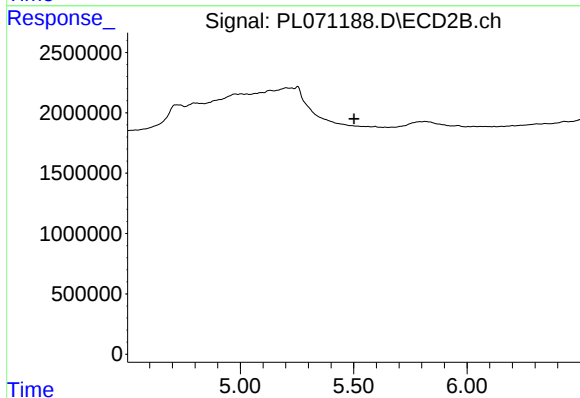


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.502 min
Response: 0
Conc: N.D.

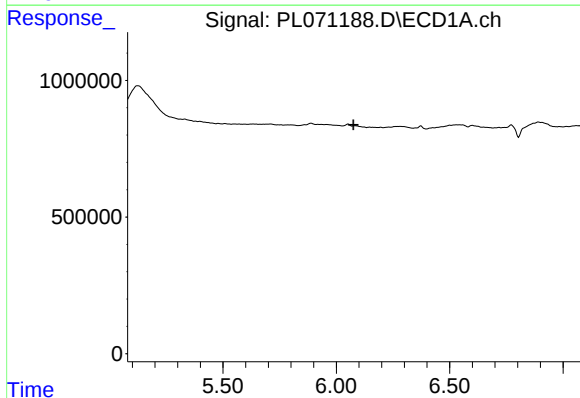


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.076 min
Response: 0
Conc: N.D.

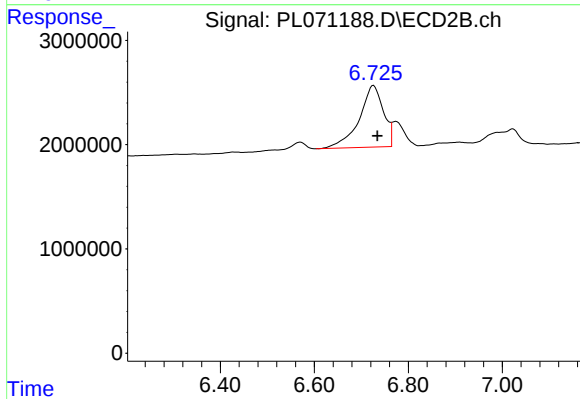

#6 beta-BHC


R.T.: 6.726 min
Delta R.T.: -0.008 min
Response: 21142804
Conc: 24.02 ng/ml

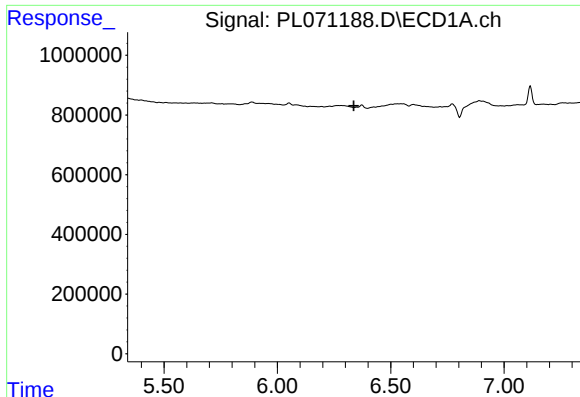

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.337 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

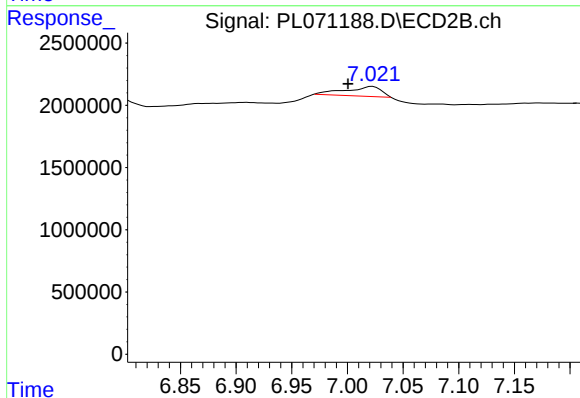


#7 delta-BHC

R.T.: 7.023 min
Delta R.T.: 0.022 min
Response: 1744520
Conc: 1.03 ng/ml

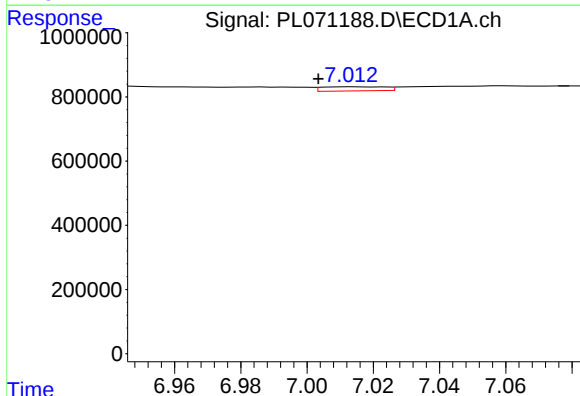


#8 Heptachlor epoxide

R.T.: 7.015 min
Delta R.T.: 0.012 min
Response: 170005
Conc: 0.27 ng/ml

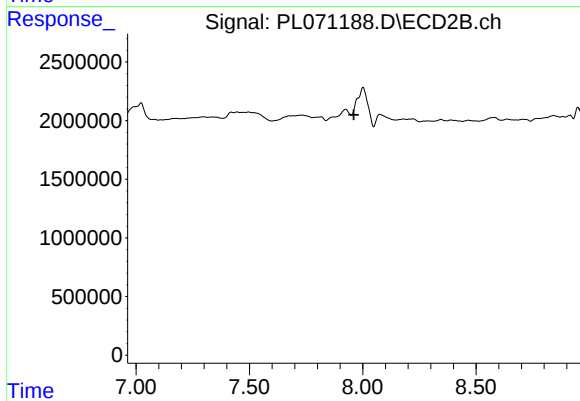

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 7.961 min
Response: 0
Conc: N.D.

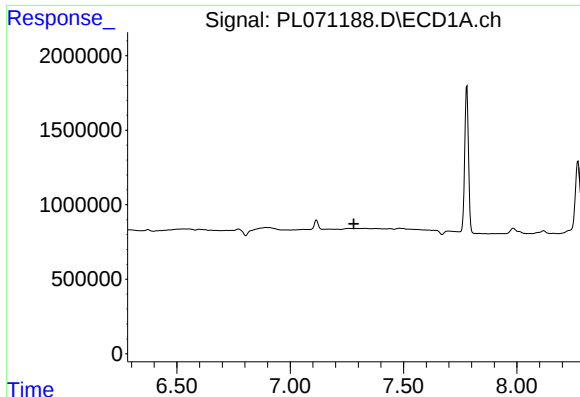

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.281 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

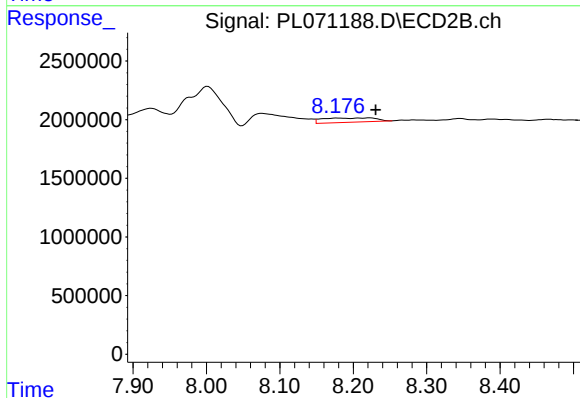


#10 gamma-Chlordane

R.T.: 8.222 min
Delta R.T.: -0.008 min
Response: 1807962
Conc: 1.13 ng/ml

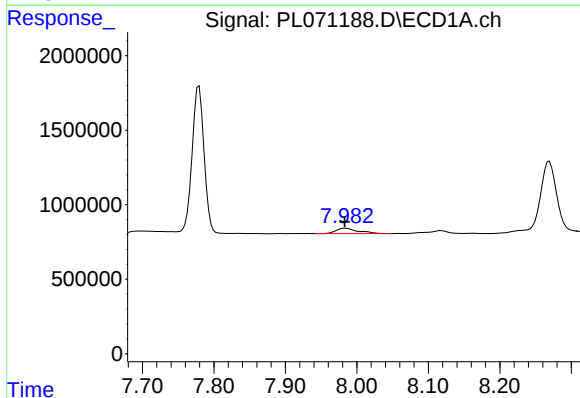


#14 Endrin

R.T.: 7.984 min
Delta R.T.: 0.000 min
Response: 793014
Conc: 1.40 ng/ml

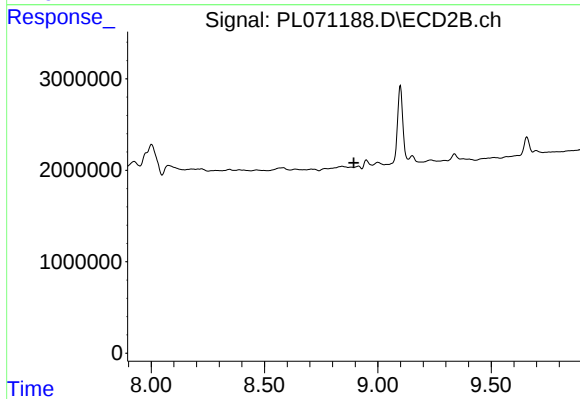

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.893 min
Response: 0
Conc: N.D.

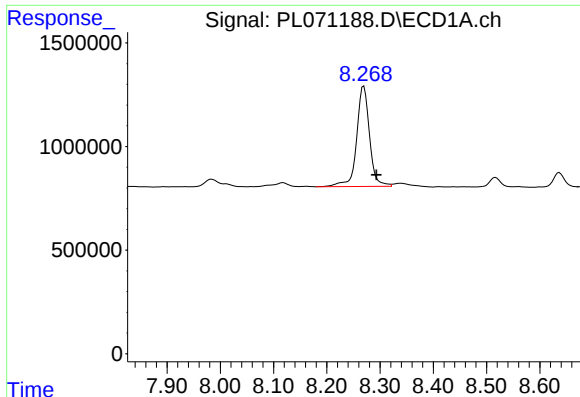

#15 Endosulfan II


R.T.: 8.269 min
Delta R.T.: -0.023 min
Response: 8104831
Conc: 13.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

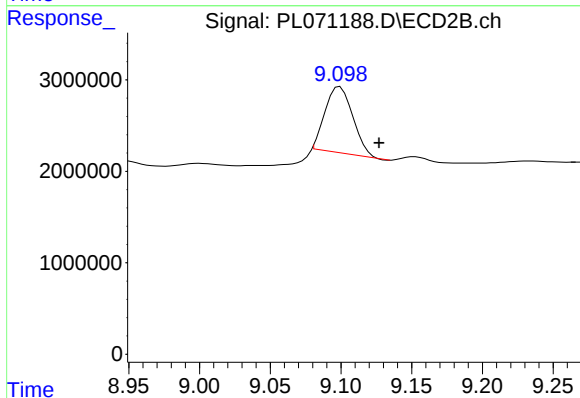


#15 Endosulfan II

R.T.: 9.099 min
Delta R.T.: -0.028 min
Response: 9826291
Conc: 7.29 ng/ml

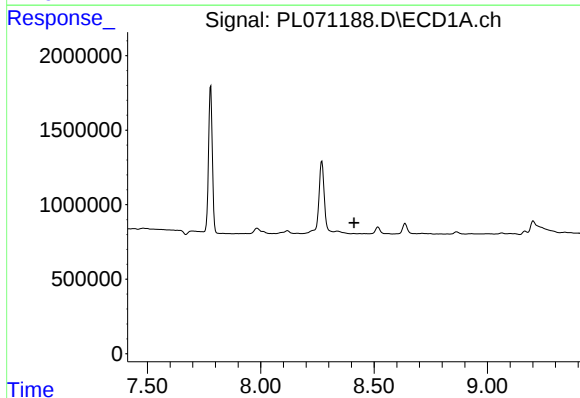


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 8.411 min
Response: 0
Conc: N.D.

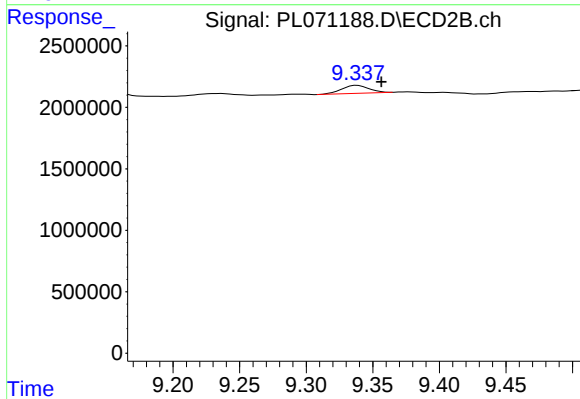

#17 4,4'-DDT


R.T.: 9.338 min
Delta R.T.: -0.018 min
Response: 930195
Conc: 0.67 ng/ml

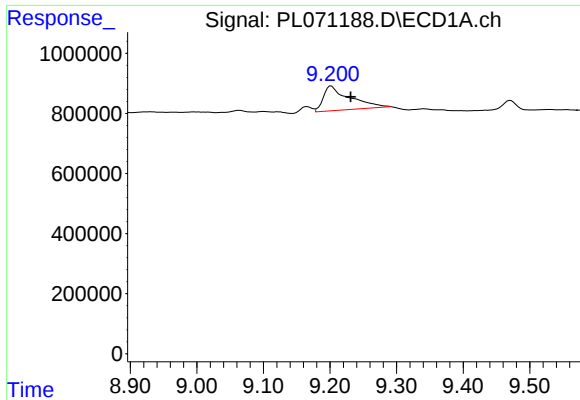

#21 Endrin ketone


R.T.: 9.202 min
Delta R.T.: -0.030 min
Response: 2241875
Conc: 3.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

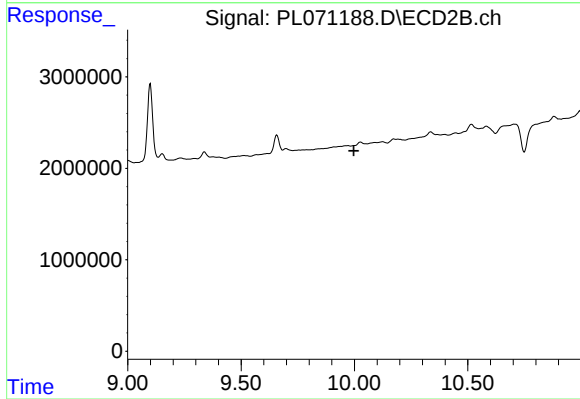


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.997 min
Response: 0
Conc: N.D.

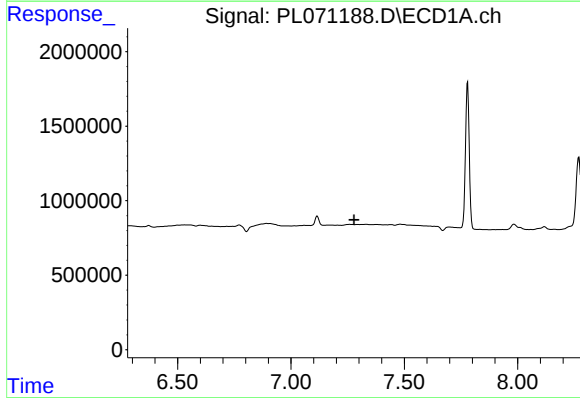


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.278 min
Response: 0
Conc: N.D.

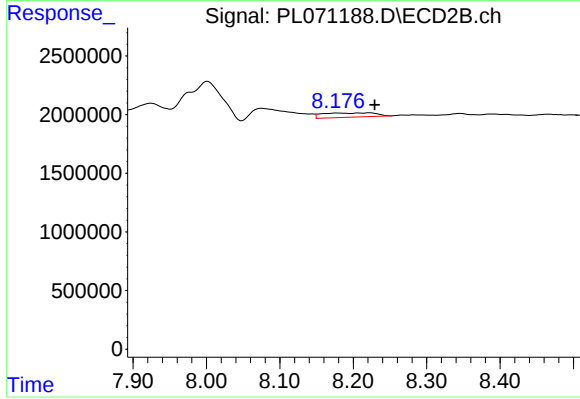

#25 Chlordane-3


R.T.: 8.222 min
Delta R.T.: -0.007 min
Response: 1807962
Conc: 8.22 ng/ml

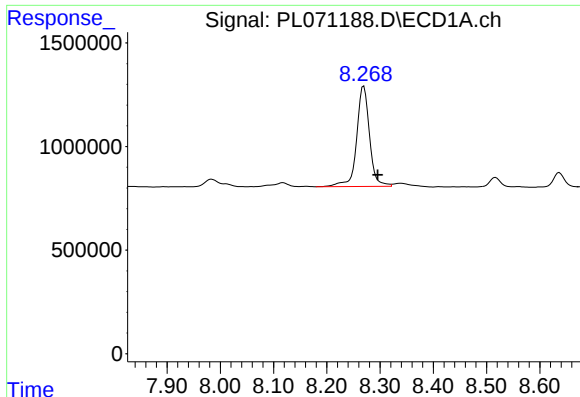

#27 Chlordane-5


R.T.: 8.269 min
Delta R.T.: -0.027 min
Response: 8104831
Conc: 339.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

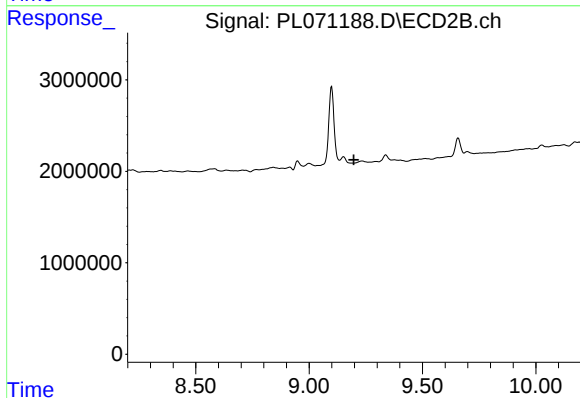


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.197 min
Response: 0
Conc: N.D.

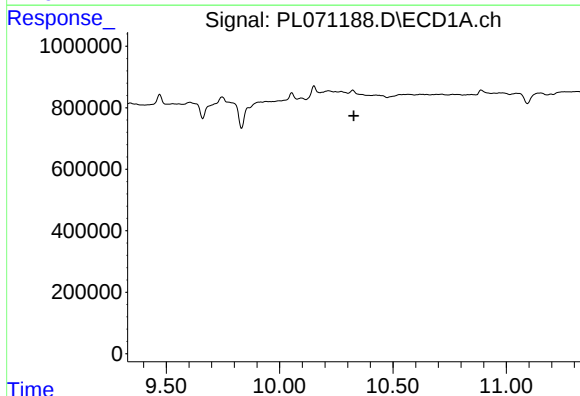

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.328 min
Response: 0
Conc: N.D.

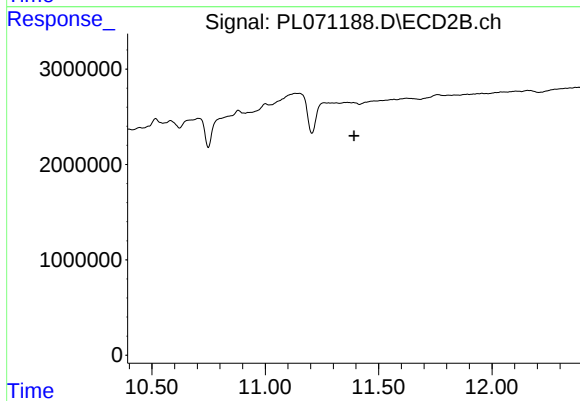

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.392 min
Response: 0
Conc: N.D.