

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL113021\
 Data File : PL071220.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2021 19:26
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 21:39:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.564	5.500	9659232	26239232	20.565	20.909
28)	SA Decachlor...	10.327	11.391	13327730	27968625	18.406	20.121
Target Compounds							
2)	A alpha-BHC	0.000	6.056f	0	631518	N.D.	0.341 #
7)	B delta-BHC	0.000	7.020f	0	2585343	N.D.	1.521 #
13)	MA Dieldrin	7.690	0.000	147262	0	0.244	N.D. #
14)	MA Endrin	8.006f	0.000	248132	0	0.439	N.D. #
15)	B Endosulfa...	8.268f	0.000	203953	0	0.349	N.D. #
16)	A 4,4'-DDD	0.000	9.047	0	1018094	N.D.	0.878 #
18)	B Endrin al...	0.000	9.284f	0	923817	N.D.	0.894 #
21)	B Endrin ke...	9.261f	10.025f	178689	384254	0.251	0.262
27)	Chlordane-5	8.268f	0.000	203953	0	8.544	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL113021\
Data File : PL071220.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2021 19:26
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 21:39:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

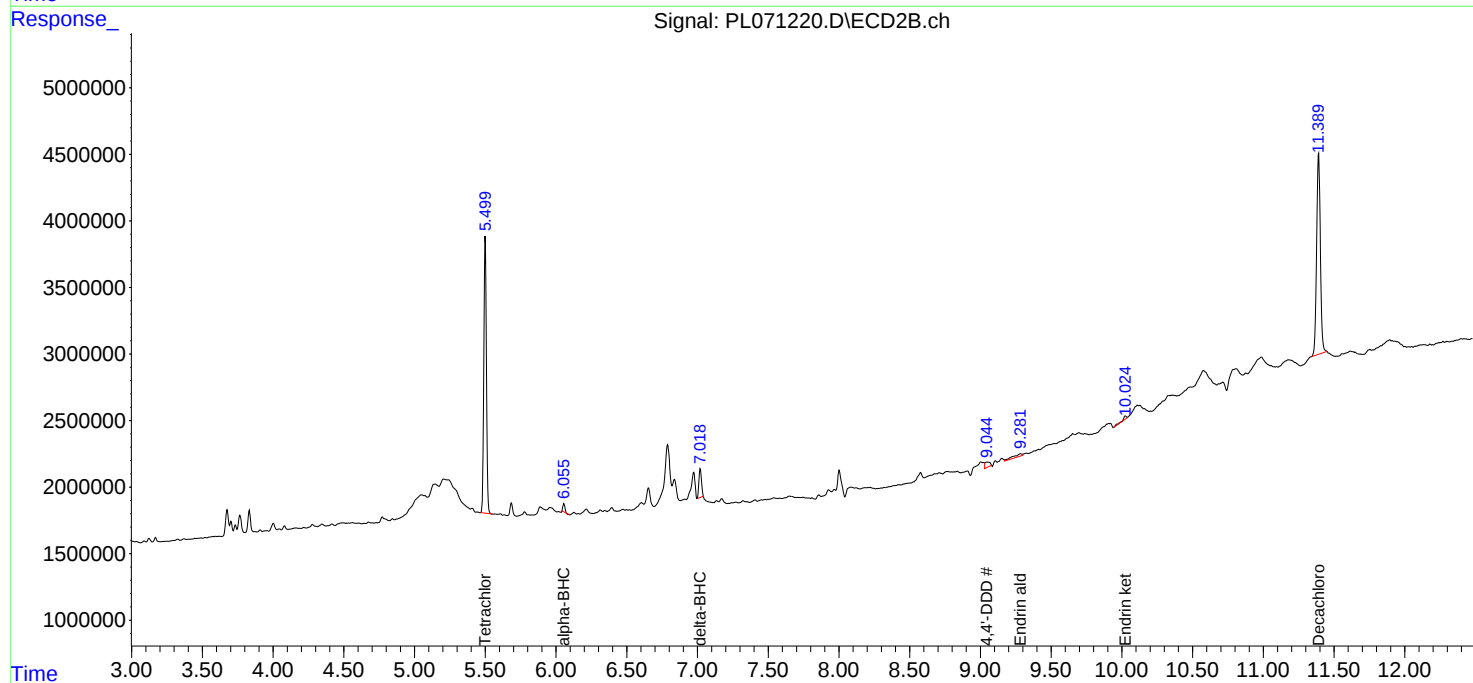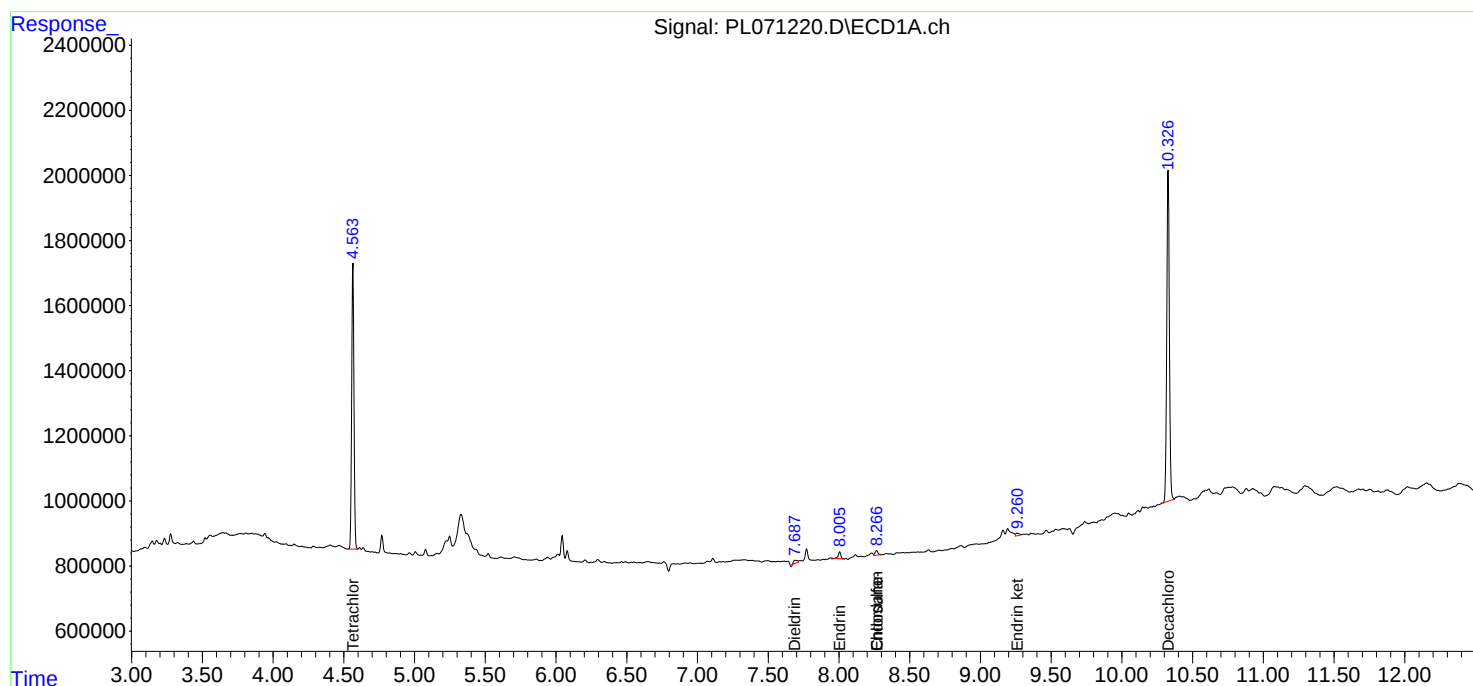


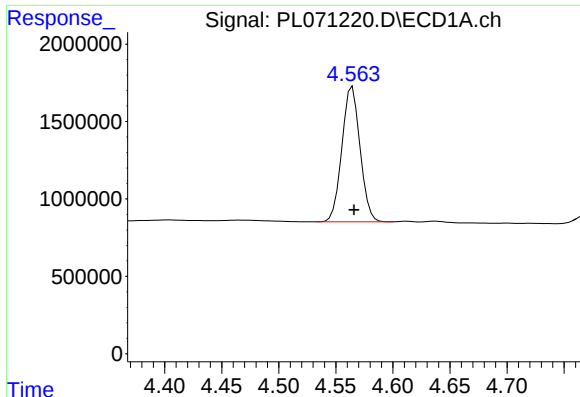

#1 Tetrachloro-m-xylene


R.T.: 4.564 min
Delta R.T.: -0.002 min
Response: 9659232
Conc: 20.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

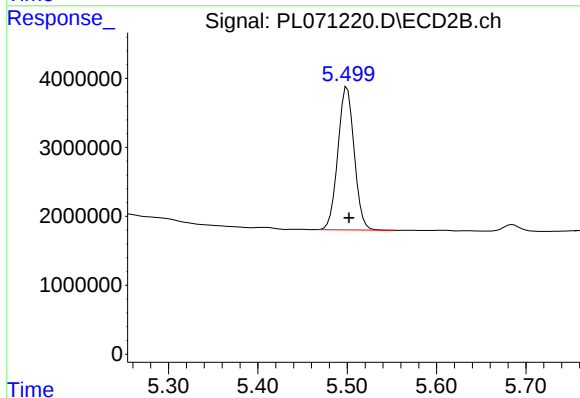


#1 Tetrachloro-m-xylene

R.T.: 5.500 min
Delta R.T.: -0.002 min
Response: 26239232
Conc: 20.91 ng/ml

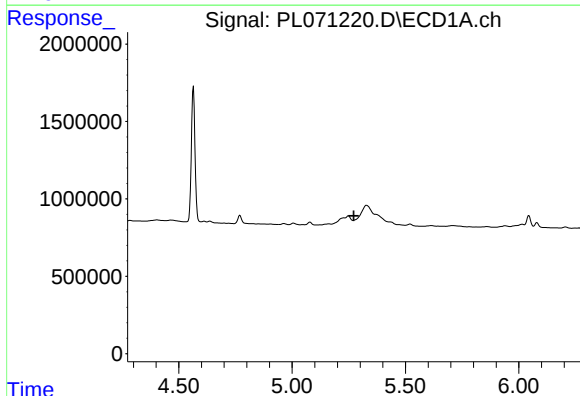


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.273 min
Response: 0
Conc: N.D.

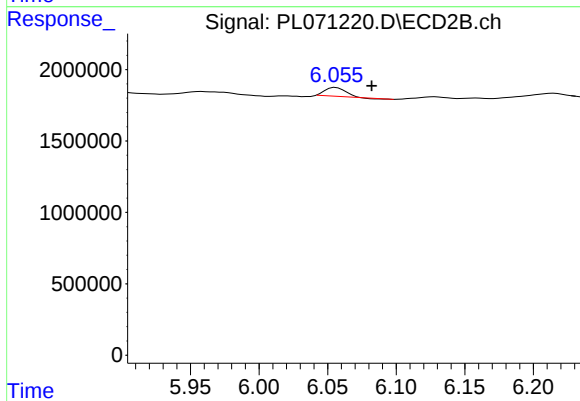

#2 alpha-BHC


R.T.: 6.056 min
Delta R.T.: -0.026 min
Response: 631518
Conc: 0.34 ng/ml

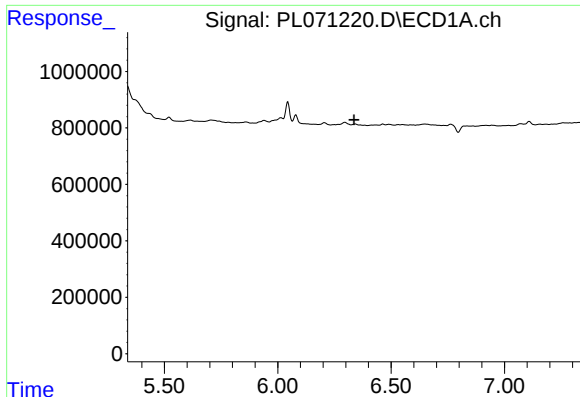

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.337 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

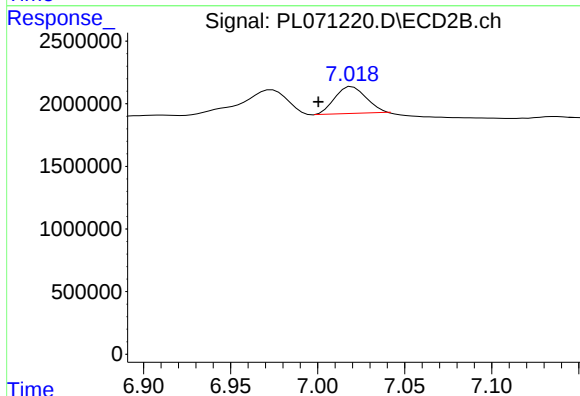


#7 delta-BHC

R.T.: 7.020 min
Delta R.T.: 0.019 min
Response: 2585343
Conc: 1.52 ng/ml

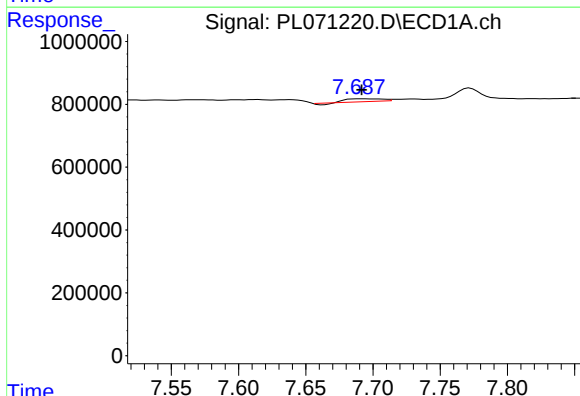


#13 Dieldrin

R.T.: 7.690 min
Delta R.T.: -0.001 min
Response: 147262
Conc: 0.24 ng/ml

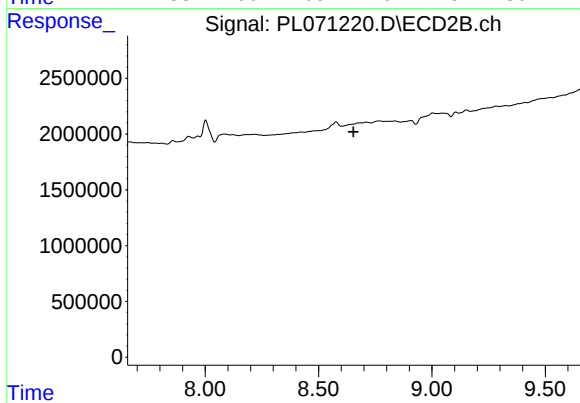

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 8.655 min
Response: 0
Conc: N.D.

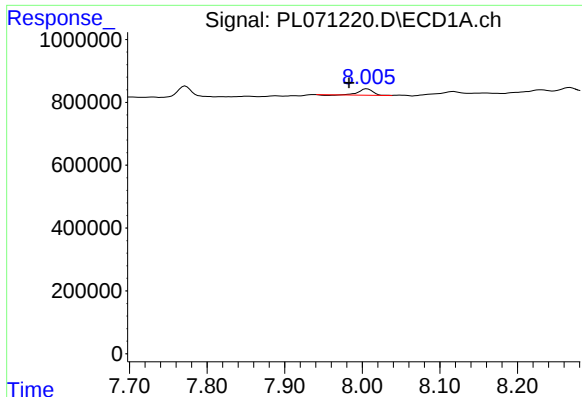

#14 Endrin


R.T.: 8.006 min
Delta R.T.: 0.023 min
Response: 248132
Conc: 0.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

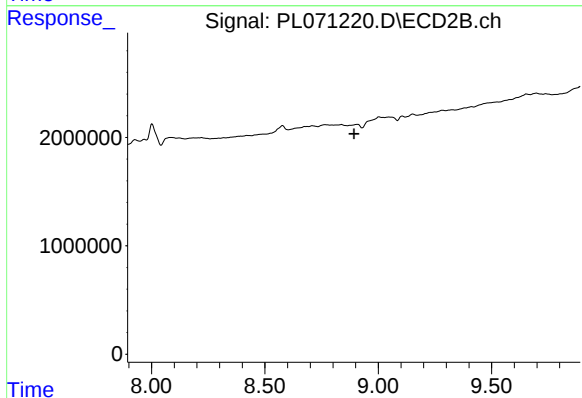


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.893 min
Response: 0
Conc: N.D.

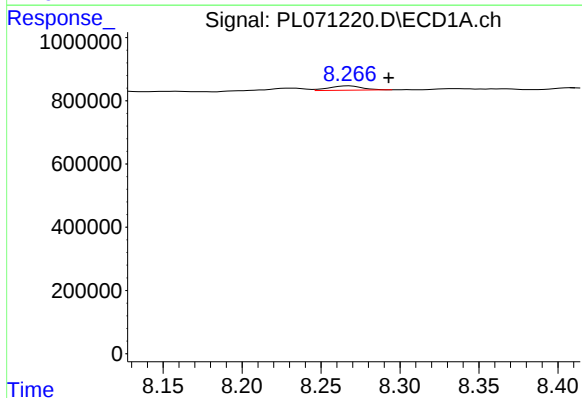


#15 Endosulfan II

R.T.: 8.268 min
Delta R.T.: -0.025 min
Response: 203953
Conc: 0.35 ng/ml

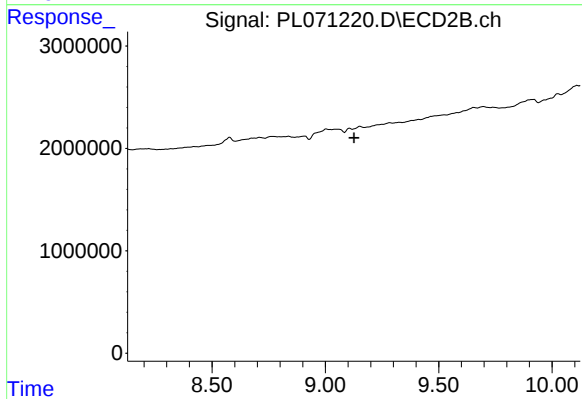

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 9.127 min
Response: 0
Conc: N.D.

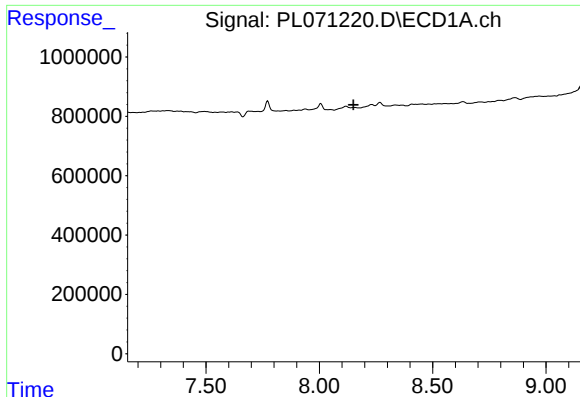

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

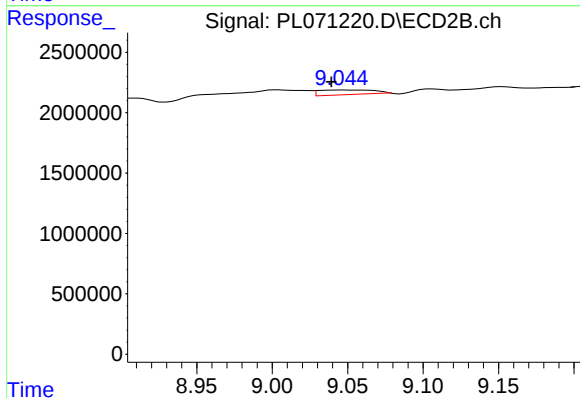


#16 4,4'-DDD

R.T.: 9.047 min
Delta R.T.: 0.008 min
Response: 1018094
Conc: 0.88 ng/ml

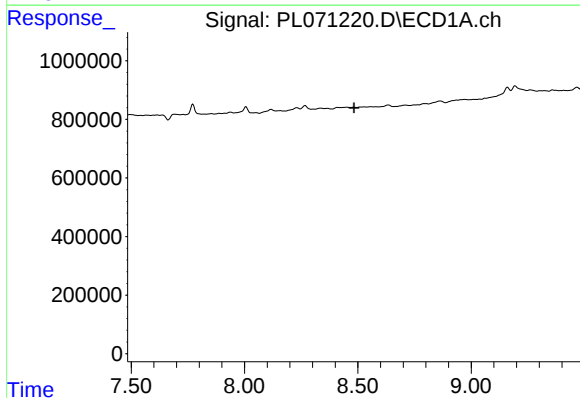


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 8.483 min
Response: 0
Conc: N.D.

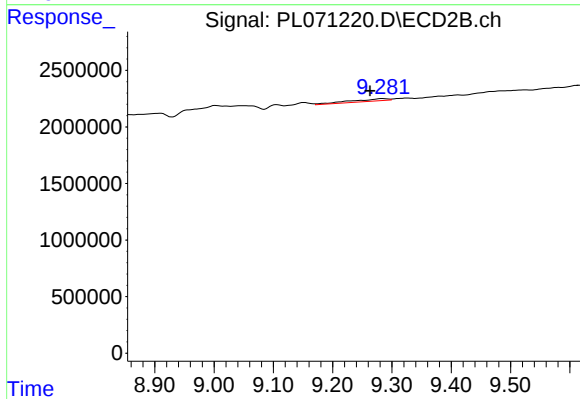

#18 Endrin aldehyde


R.T.: 9.284 min
Delta R.T.: 0.021 min
Response: 923817
Conc: 0.89 ng/ml

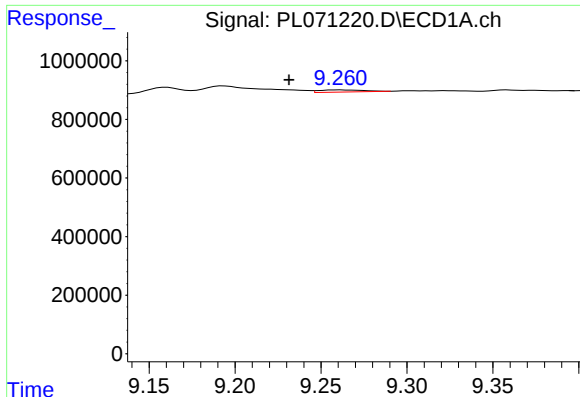

#21 Endrin ketone


R.T.: 9.261 min
Delta R.T.: 0.030 min
Response: 178689
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

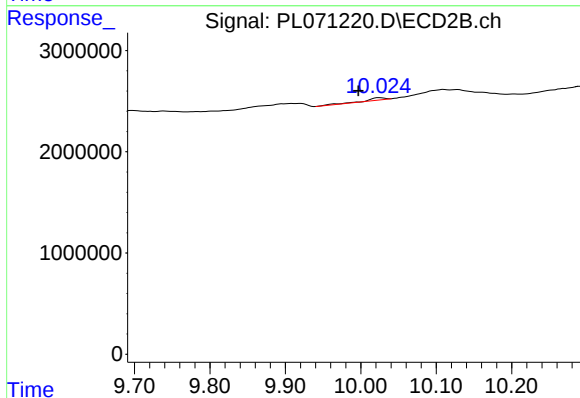


#21 Endrin ketone

R.T.: 10.025 min
Delta R.T.: 0.029 min
Response: 384254
Conc: 0.26 ng/ml

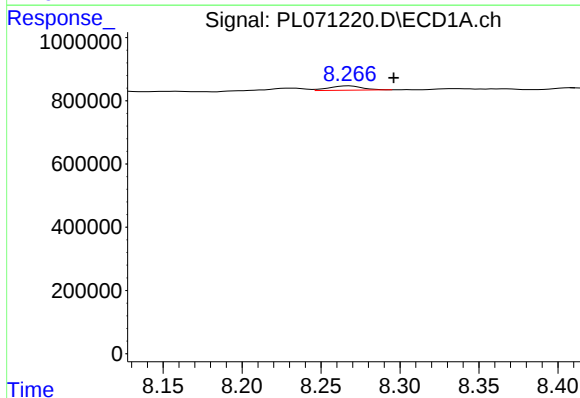


#27 Chlordane-5

R.T.: 8.268 min
Delta R.T.: -0.028 min
Response: 203953
Conc: 8.54 ng/ml

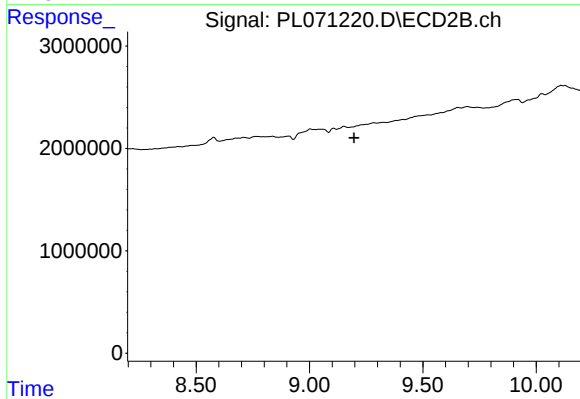

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.197 min
Response: 0
Conc: N.D.

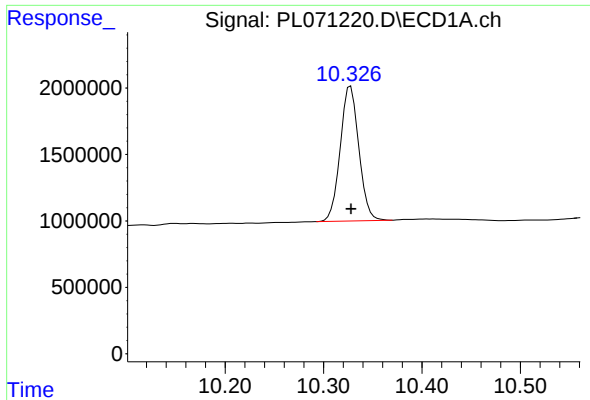

#28 Decachlorobiphenyl

R.T.: 10.327 min
Delta R.T.: 0.000 min
Response: 13327730
Conc: 18.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

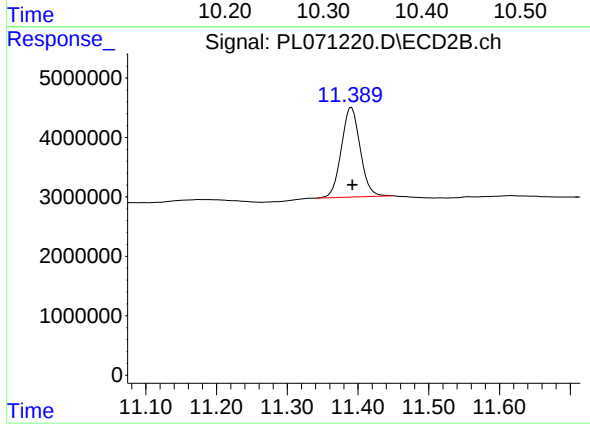

#28 Decachlorobiphenyl

R.T.: 11.391 min
Delta R.T.: -0.001 min
Response: 27968625
Conc: 20.12 ng/ml