

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL113021\
 Data File : PL071197.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2021 13:04
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 14:36:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 14:36:25 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.564	5.500	49334735	126.5E6	99.335	97.565
28)	SA Decachlor...	10.326	11.390	66491510	136.2E6	91.922	94.069
Target Compounds							
23)	Chlordane-1	5.890	6.881	16366490	50829938	998.981	974.153
24)	Chlordane-2	6.579	7.473	21181368	53474974	943.976	952.419
25)	Chlordane-3	7.279	8.230	61226854	221.0E6	1003.696	996.742
26)	Chlordane-4	7.347	8.311	65463767	263.1E6	998.945	981.823
27)	Chlordane-5	8.296	9.197	22966536	47281736	976.046	999.388



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL113021\
Data File : PL071197.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2021 13:04
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 14:36:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 14:36:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

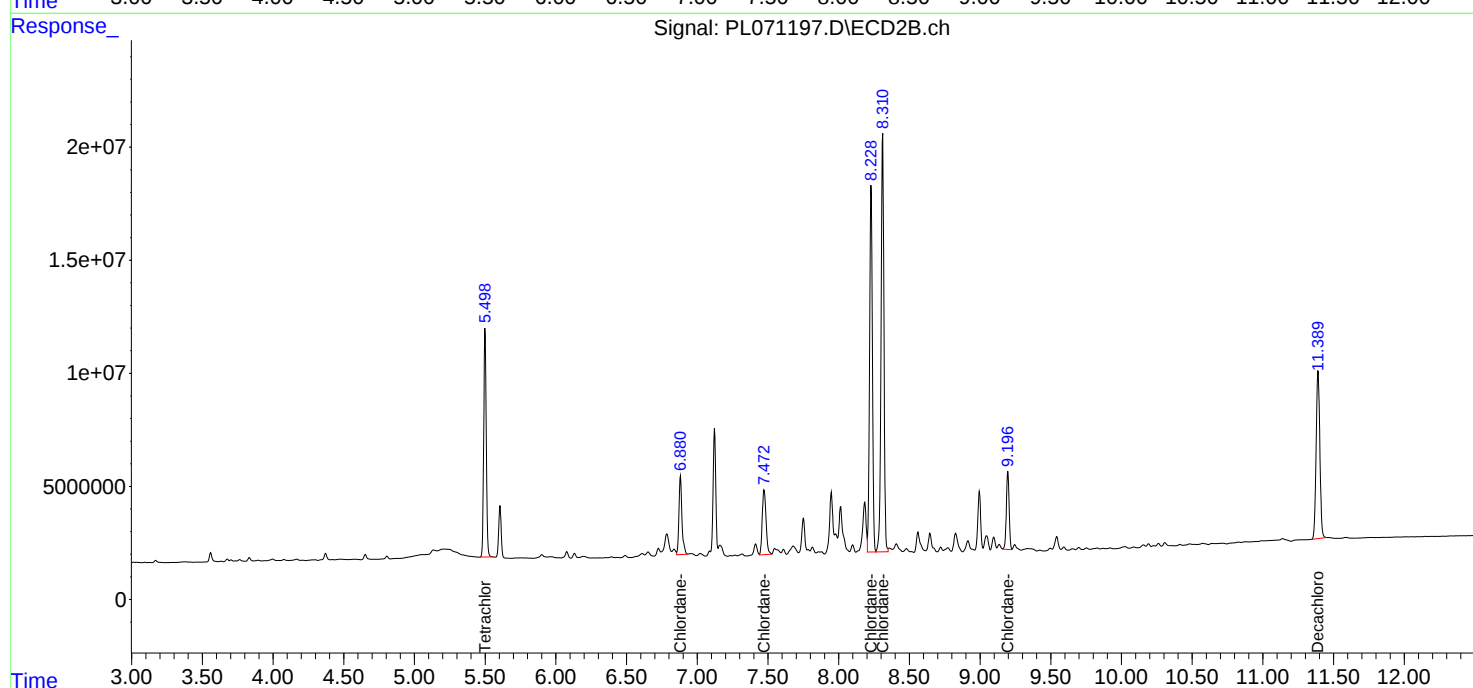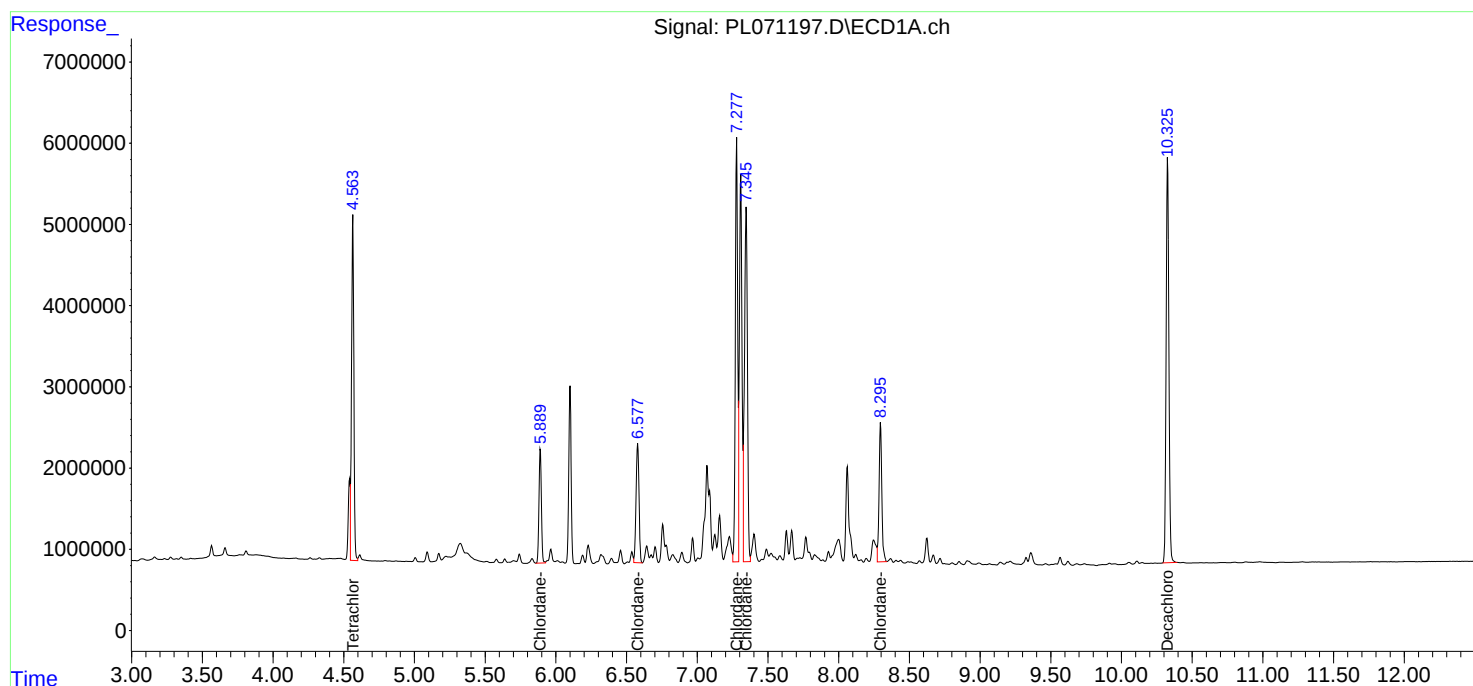


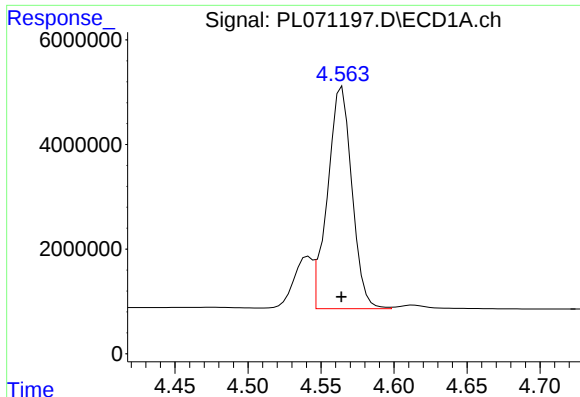

#1 Tetrachloro-m-xylene


R.T.: 4.564 min
Delta R.T.: 0.000 min
Response: 49334735
Conc: 99.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

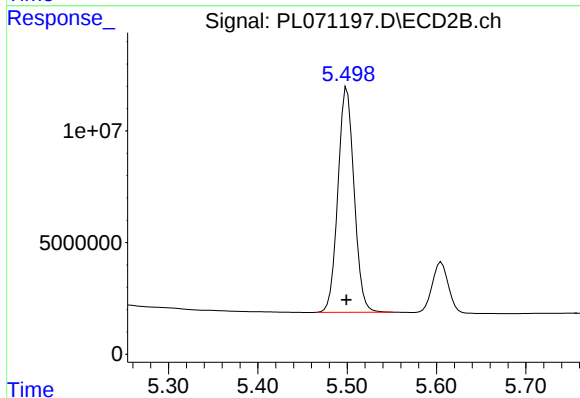


#1 Tetrachloro-m-xylene

R.T.: 5.500 min
Delta R.T.: 0.000 min
Response: 126530149
Conc: 97.56 ng/ml

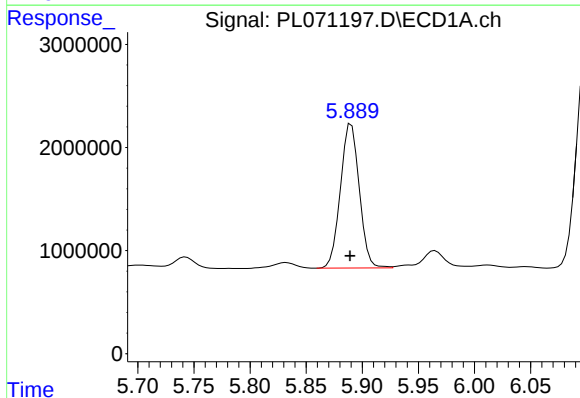


#23 Chlordane-1

R.T.: 5.890 min
Delta R.T.: 0.000 min
Response: 16366490
Conc: 998.98 ng/ml

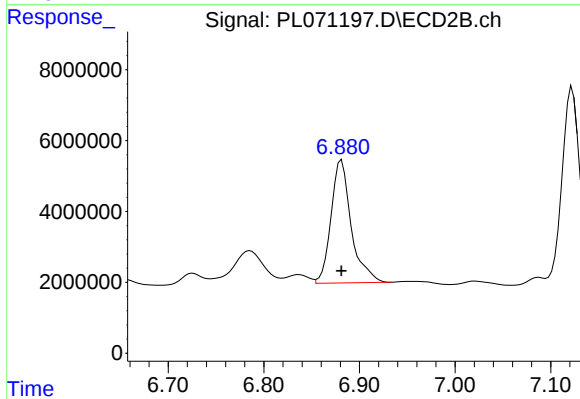

#23 Chlordane-1


R.T.: 6.881 min
Delta R.T.: 0.000 min
Response: 50829938
Conc: 974.15 ng/ml

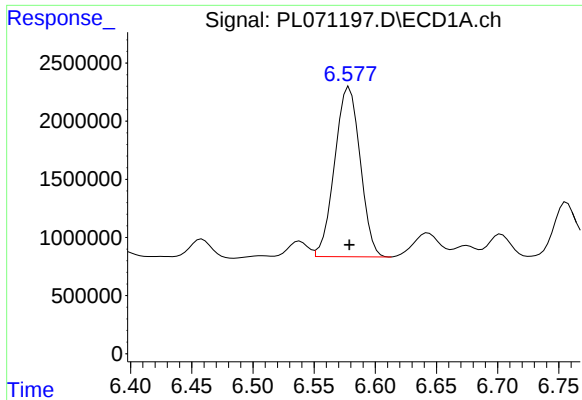

#24 Chlordane-2


R.T.: 6.579 min
Delta R.T.: 0.000 min
Response: 21181368
Conc: 943.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

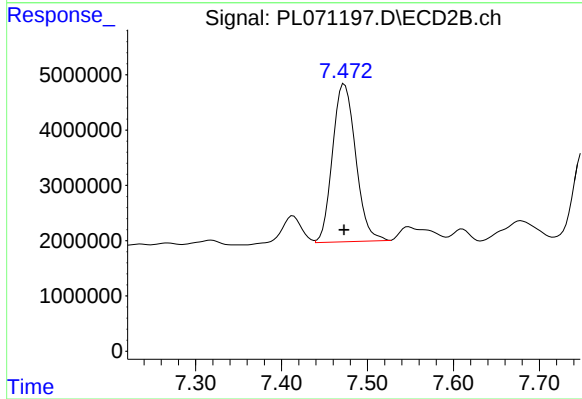


#24 Chlordane-2

R.T.: 7.473 min
Delta R.T.: 0.000 min
Response: 53474974
Conc: 952.42 ng/ml

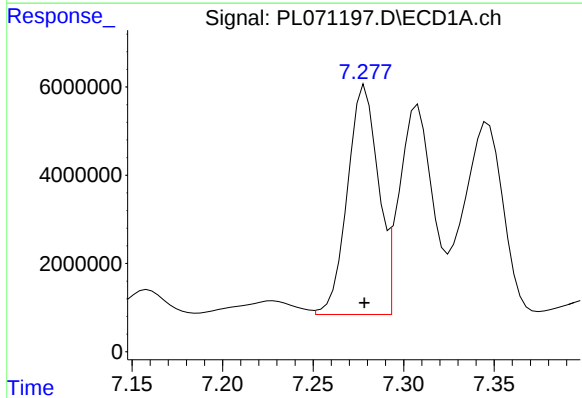


#25 Chlordane-3

R.T.: 7.279 min
Delta R.T.: 0.000 min
Response: 61226854
Conc: 1003.70 ng/ml

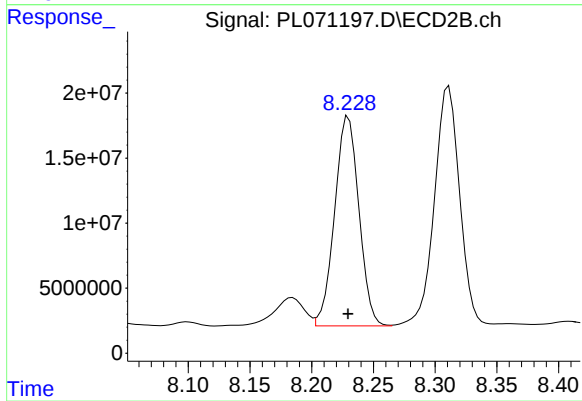

#25 Chlordane-3


R.T.: 8.230 min
Delta R.T.: 0.000 min
Response: 220975158
Conc: 996.74 ng/ml

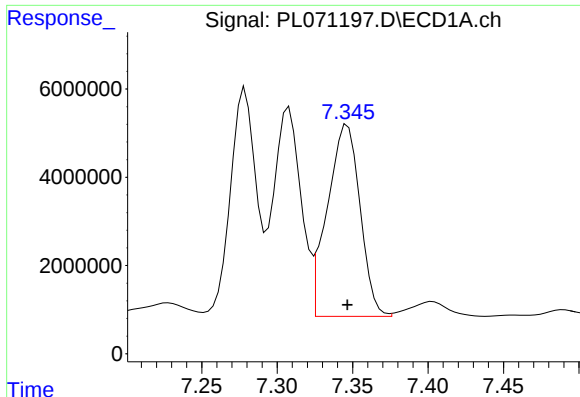

#26 Chlordane-4


R.T.: 7.347 min
Delta R.T.: 0.000 min
Response: 65463767
Conc: 998.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

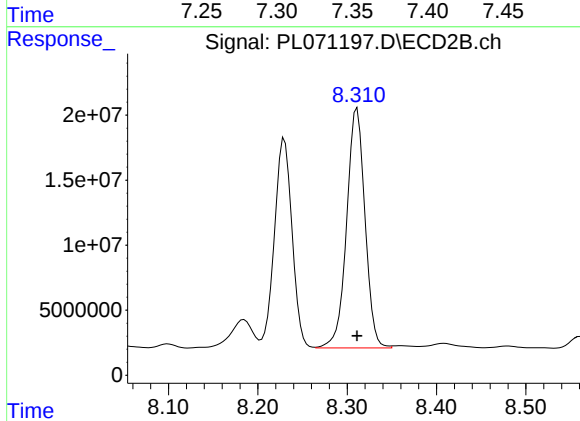


#26 Chlordane-4

R.T.: 8.311 min
Delta R.T.: 0.000 min
Response: 263109570
Conc: 981.82 ng/ml

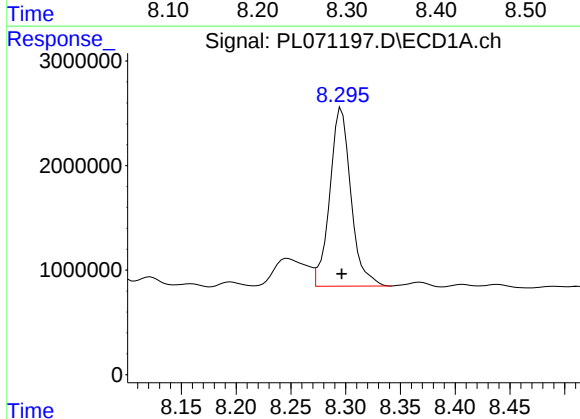


#27 Chlordane-5

R.T.: 8.296 min
Delta R.T.: 0.000 min
Response: 22966536
Conc: 976.05 ng/ml

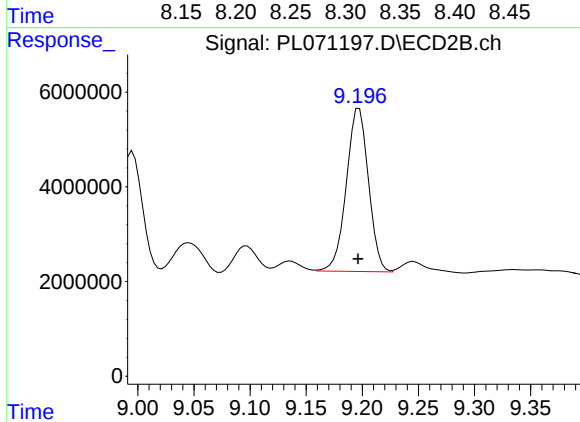

#27 Chlordane-5


R.T.: 9.197 min
Delta R.T.: 0.000 min
Response: 47281736
Conc: 999.39 ng/ml

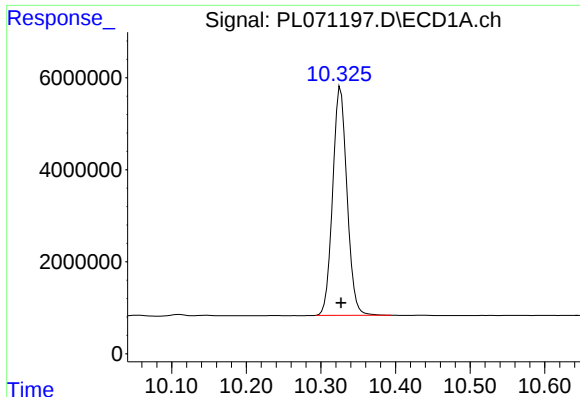

#28 Decachlorobiphenyl

R.T.: 10.326 min
Delta R.T.: 0.000 min
Response: 66491510
Conc: 91.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

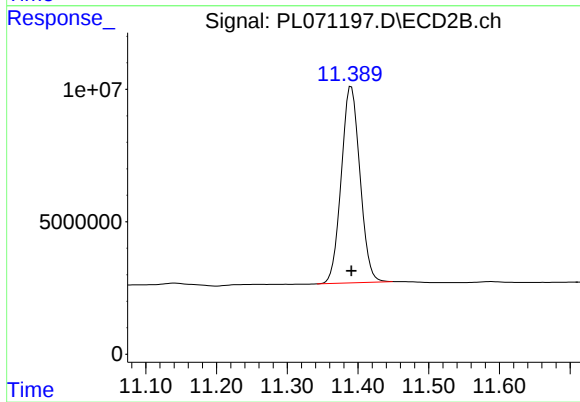

#28 Decachlorobiphenyl

R.T.: 11.390 min
Delta R.T.: 0.000 min
Response: 136171524
Conc: 94.07 ng/ml