

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL113021\
 Data File : PL071198.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2021 13:20
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 14:37:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 14:36:25 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.564	5.500	37985044	98787988	76.483	76.173
28)	SA Decachlor...	10.327	11.390	51757803	105.2E6	71.553	72.651
Target Compounds							
23)	Chlordane-1	5.890	6.881	12602976	40080311	769.263	768.137
24)	Chlordane-2	6.579	7.472	16562647	41541900	738.137	739.884
25)	Chlordane-3	7.279	8.229	46381611	168.5E6	760.337	760.241
26)	Chlordane-4	7.347	8.311	49711188	201.7E6	758.569	752.710
27)	Chlordane-5	8.297	9.197	17498579	35389957	743.665	748.033



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL113021\
Data File : PL071198.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2021 13:20
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 14:37:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 14:36:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

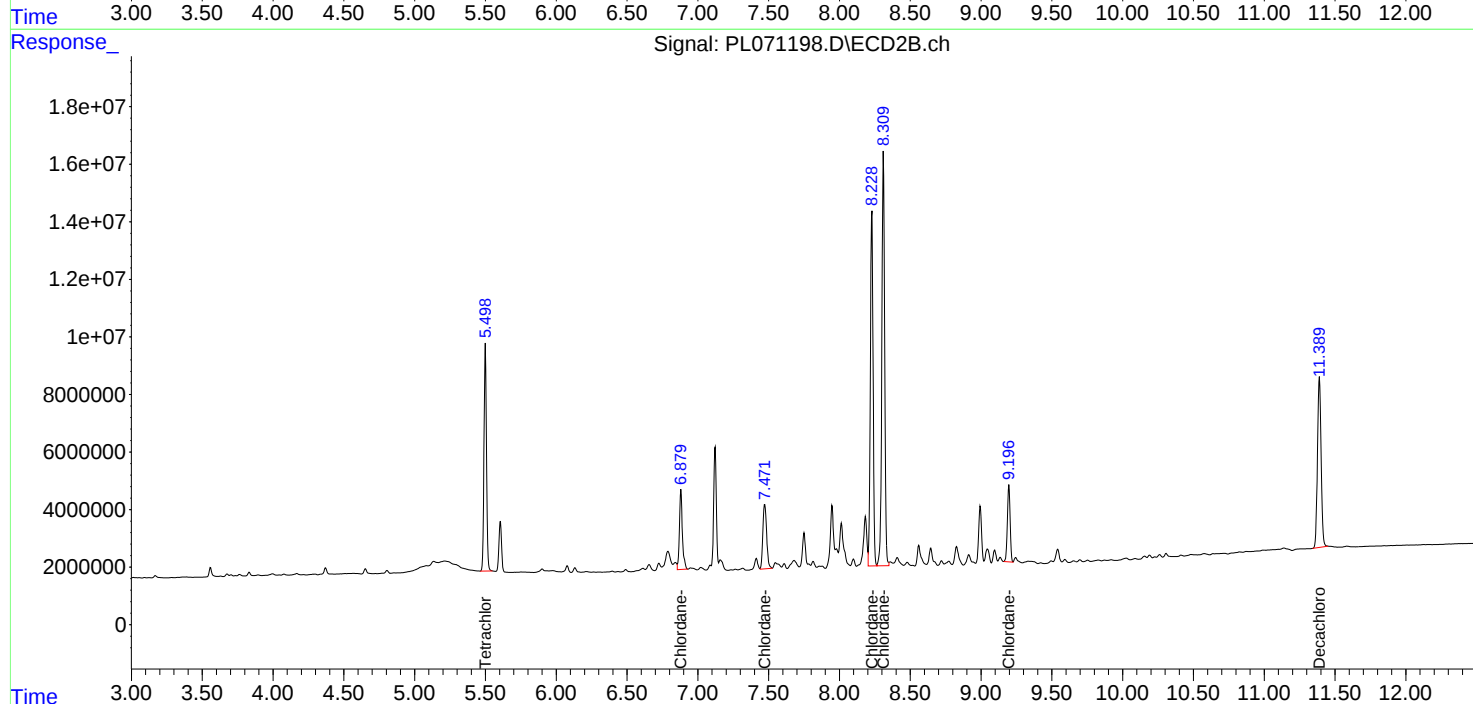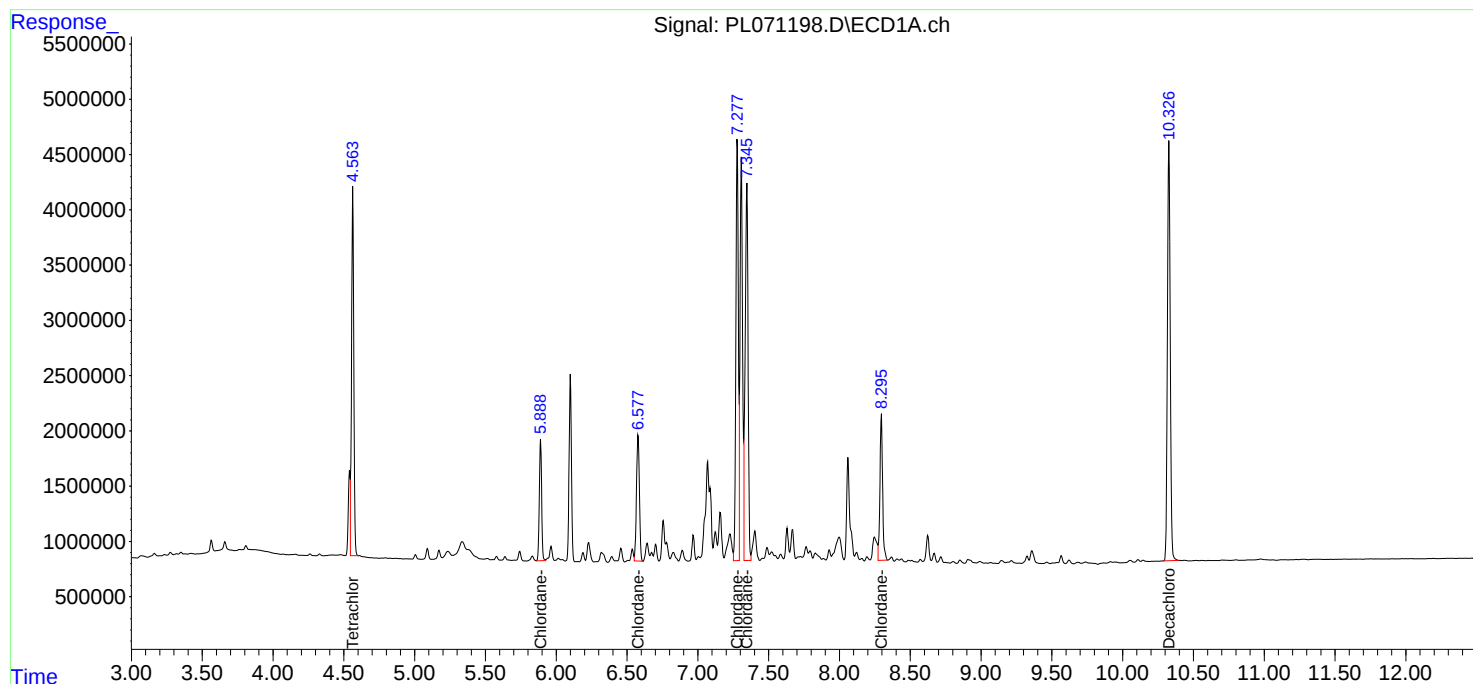


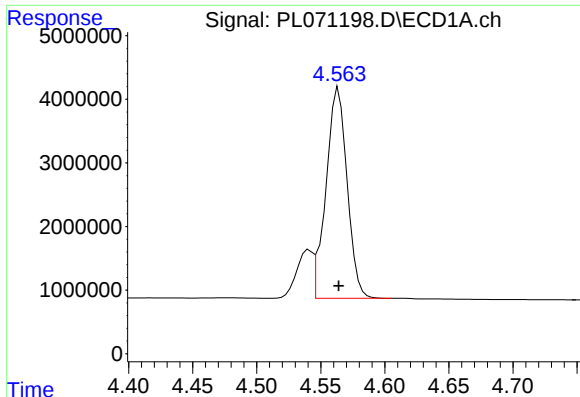

#1 Tetrachloro-m-xylene


R.T.: 4.564 min
Delta R.T.: 0.000 min
Response: 37985044
Conc: 76.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

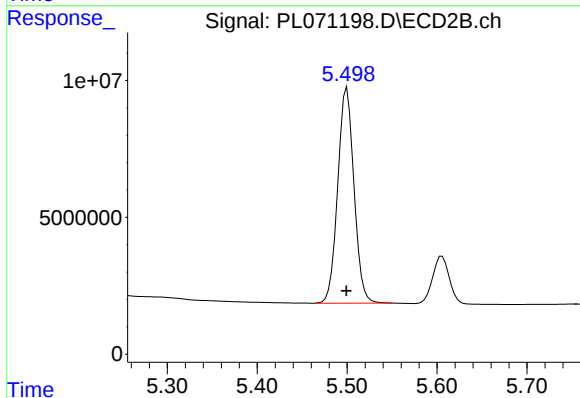


#1 Tetrachloro-m-xylene

R.T.: 5.500 min
Delta R.T.: 0.000 min
Response: 98787988
Conc: 76.17 ng/ml

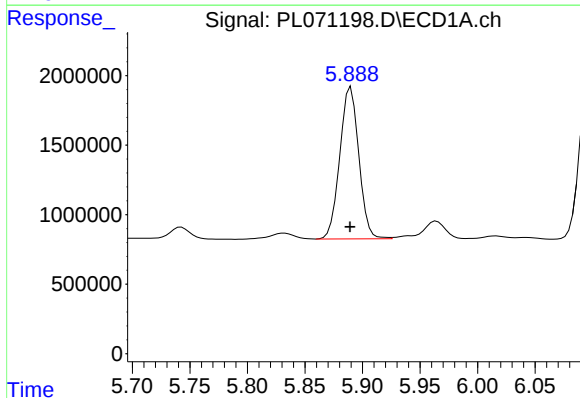


#23 Chlordane-1

R.T.: 5.890 min
Delta R.T.: 0.000 min
Response: 12602976
Conc: 769.26 ng/ml

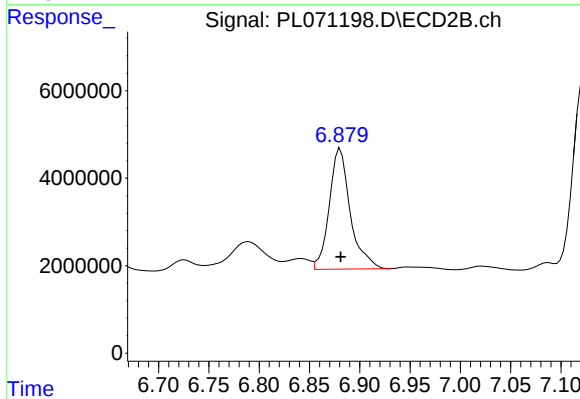

#23 Chlordane-1


R.T.: 6.881 min
Delta R.T.: 0.000 min
Response: 40080311
Conc: 768.14 ng/ml

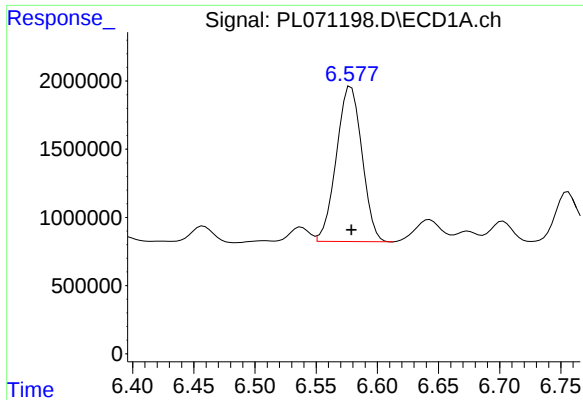

#24 Chlordane-2


R.T.: 6.579 min
Delta R.T.: 0.000 min
Response: 16562647
Conc: 738.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

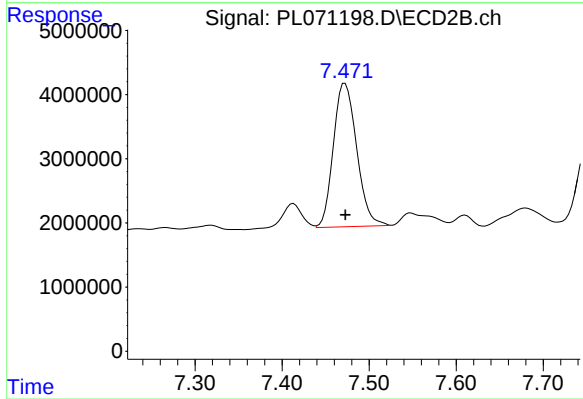


#24 Chlordane-2

R.T.: 7.472 min
Delta R.T.: 0.000 min
Response: 41541900
Conc: 739.88 ng/ml

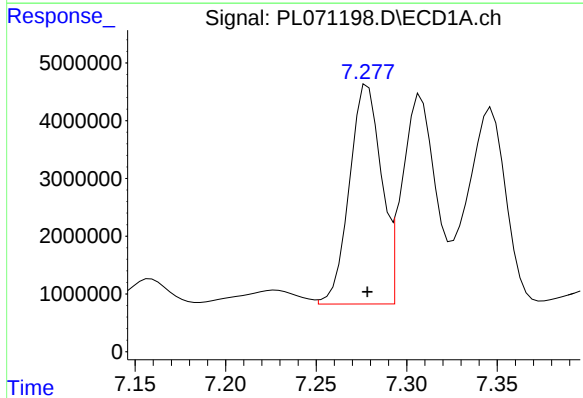


#25 Chlordane-3

R.T.: 7.279 min
Delta R.T.: 0.000 min
Response: 46381611
Conc: 760.34 ng/ml

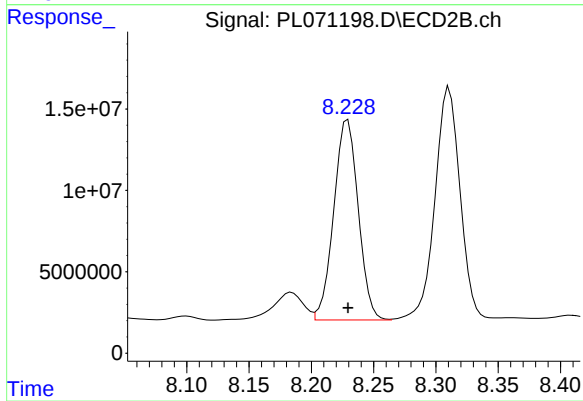

#25 Chlordane-3


R.T.: 8.229 min
Delta R.T.: 0.000 min
Response: 168543639
Conc: 760.24 ng/ml

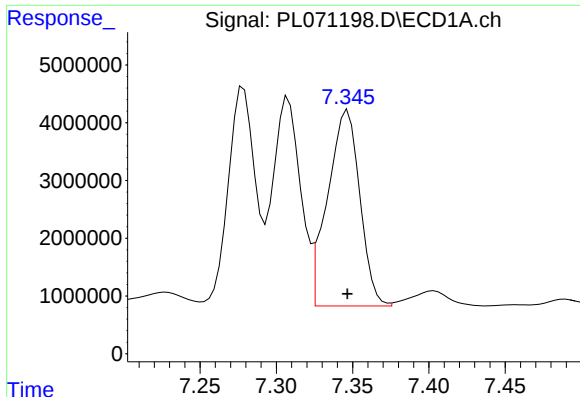

#26 Chlordane-4


R.T.: 7.347 min
Delta R.T.: 0.000 min
Response: 49711188
Conc: 758.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

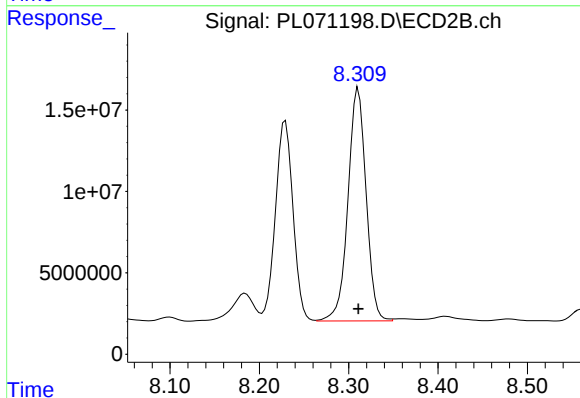


#26 Chlordane-4

R.T.: 8.311 min
Delta R.T.: 0.000 min
Response: 201711758
Conc: 752.71 ng/ml

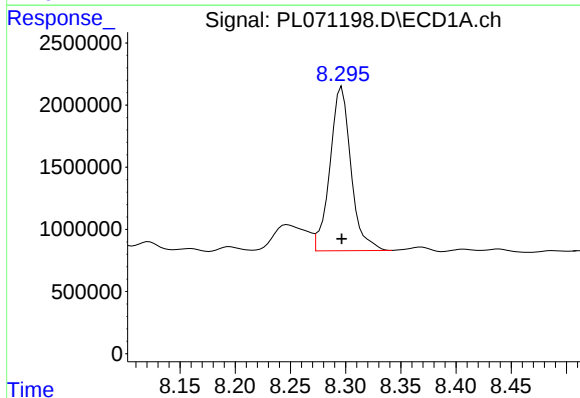


#27 Chlordane-5

R.T.: 8.297 min
Delta R.T.: 0.000 min
Response: 17498579
Conc: 743.67 ng/ml

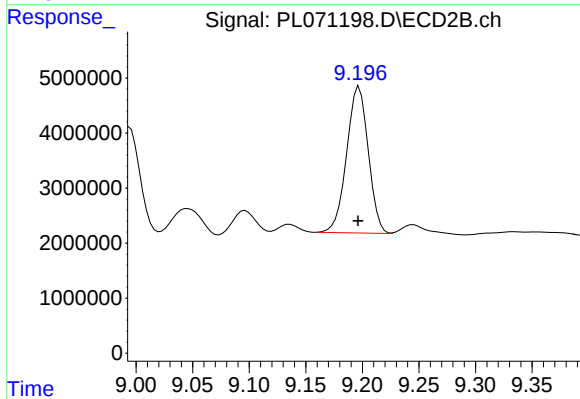

#27 Chlordane-5


R.T.: 9.197 min
Delta R.T.: 0.000 min
Response: 35389957
Conc: 748.03 ng/ml

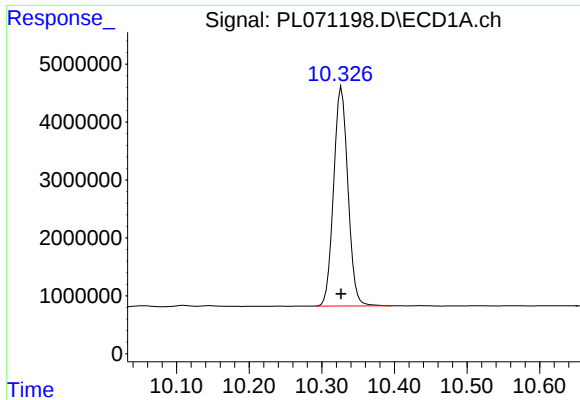

#28 Decachlorobiphenyl

R.T.: 10.327 min
Delta R.T.: 0.000 min
Response: 51757803
Conc: 71.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

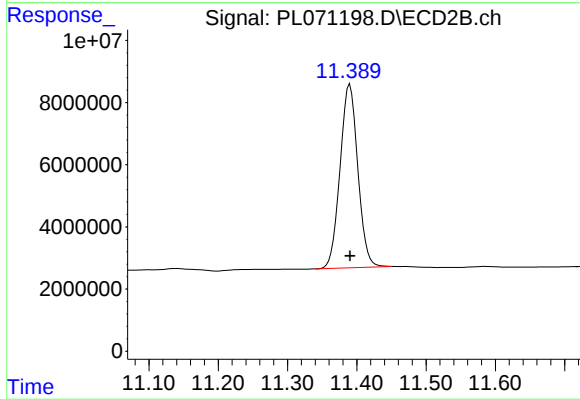

#28 Decachlorobiphenyl

R.T.: 11.390 min
Delta R.T.: 0.000 min
Response: 105167168
Conc: 72.65 ng/ml