

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL113021\
 Data File : PL071201.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2021 14:10
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 14:57:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 14:36:25 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.564	5.499	2710653	6841143	5.458	5.275
28)	SA Decachlor...	10.328	11.390	4555412	7718919	6.298	5.332
Target Compounds							
23)	Chlordane-1	5.889	6.880	900464	2700422	54.963	51.753
24)	Chlordane-2	6.578	7.472	1430528	3218250	63.753	57.319
25)	Chlordane-3	7.278	8.229	3340464	10931005	54.760	49.306
26)	Chlordane-4	7.347	8.311	3527303	13304424	53.825	49.647
27)	Chlordane-5	8.296	9.197	1306220	2344287	55.513	49.551



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL113021\
Data File : PL071201.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2021 14:10
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 14:57:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 14:36:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

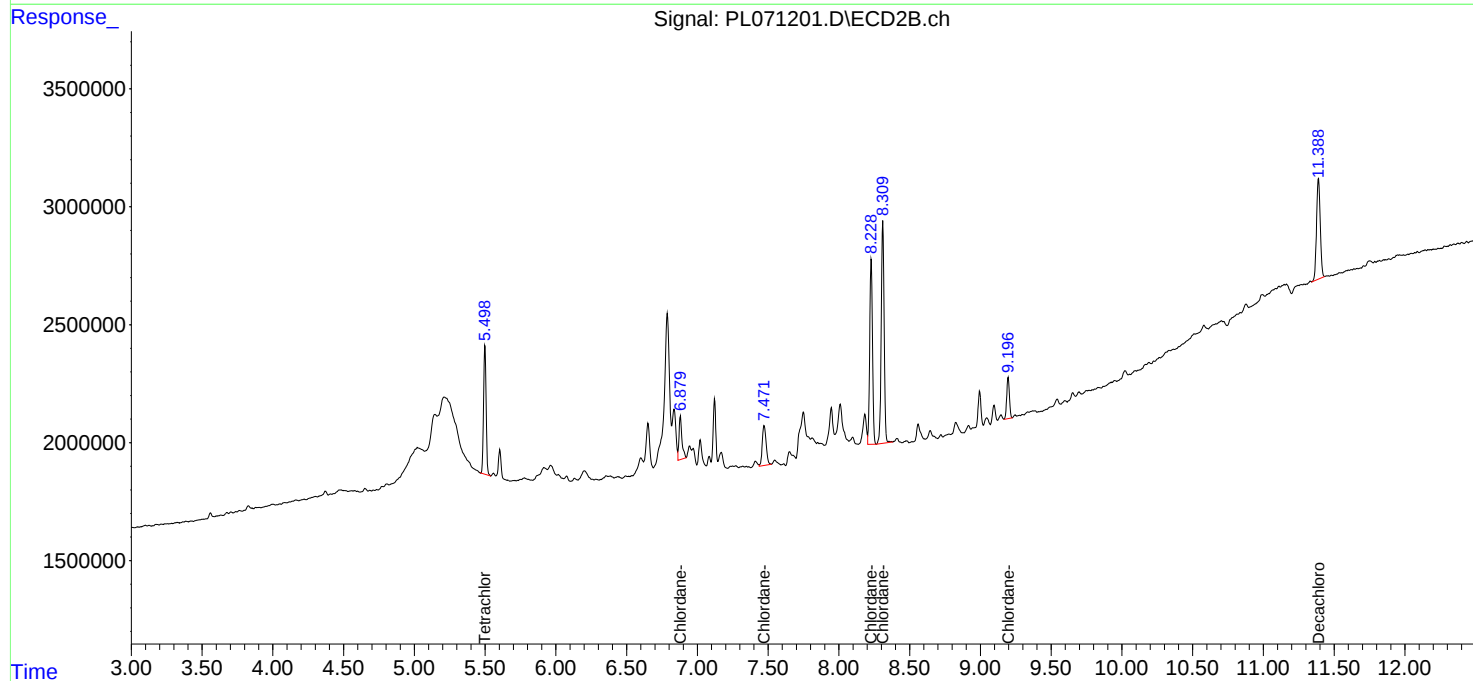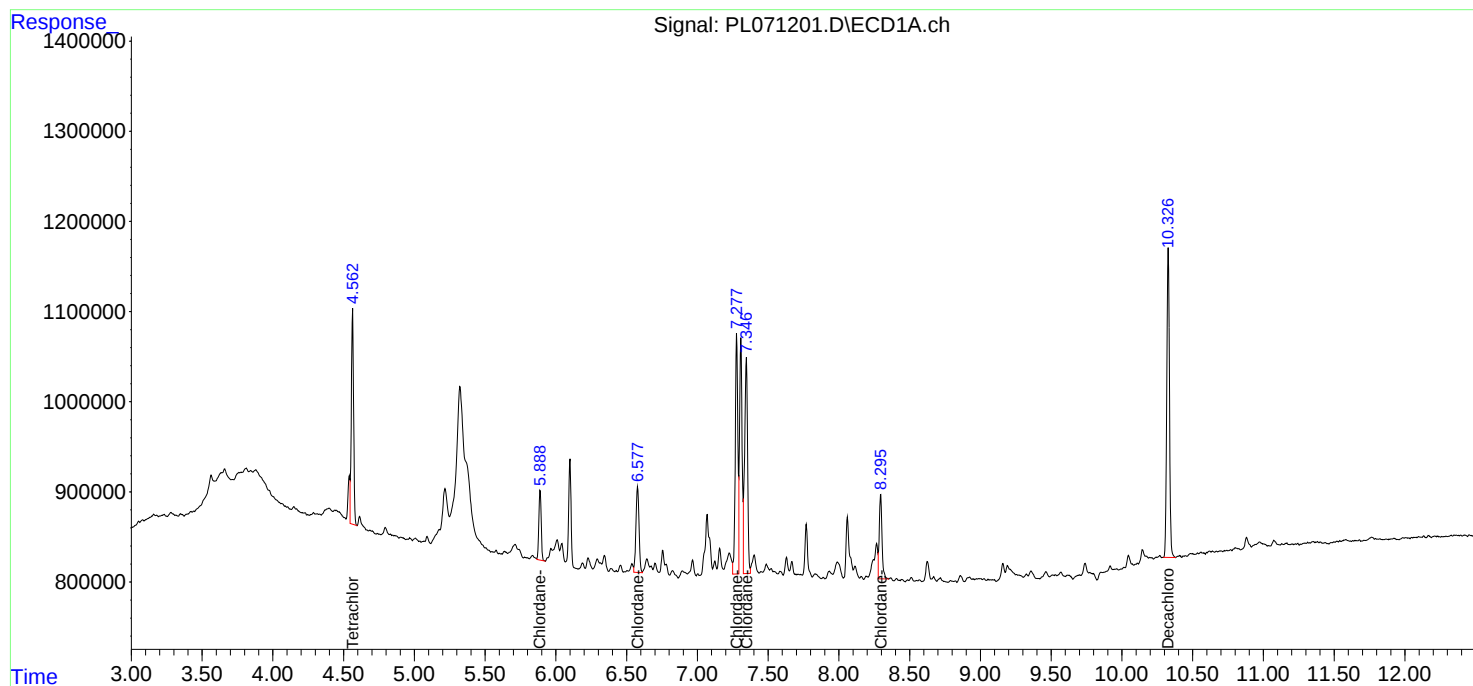


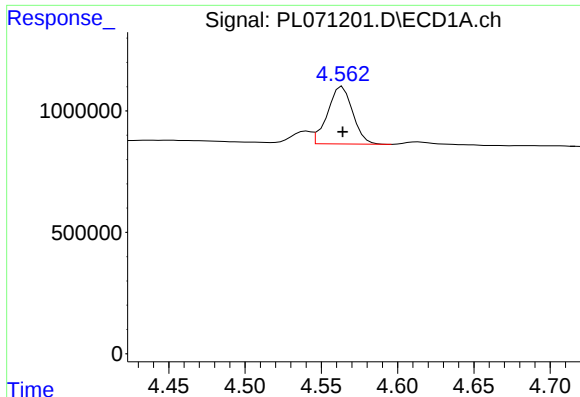

#1 Tetrachloro-m-xylene


R.T.: 4.564 min
Delta R.T.: 0.000 min
Response: 2710653
Conc: 5.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

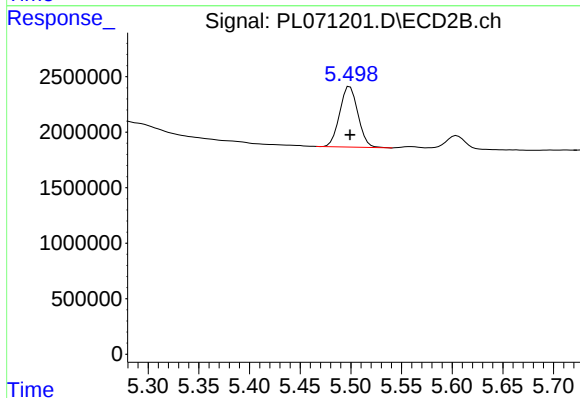


#1 Tetrachloro-m-xylene

R.T.: 5.499 min
Delta R.T.: 0.000 min
Response: 6841143
Conc: 5.28 ng/ml

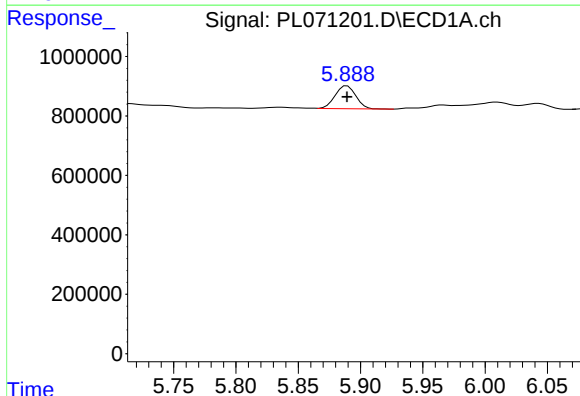


#23 Chlordane-1

R.T.: 5.889 min
Delta R.T.: 0.000 min
Response: 900464
Conc: 54.96 ng/ml

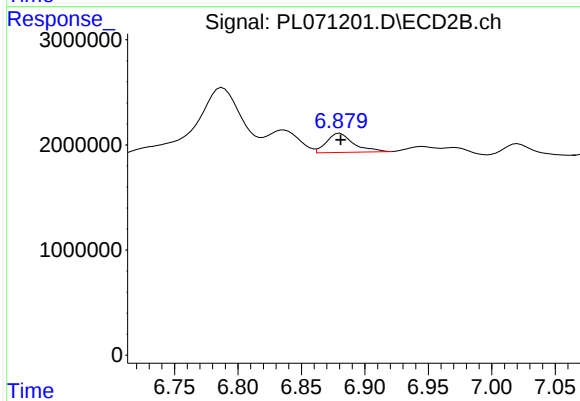

#23 Chlordane-1


R.T.: 6.880 min
Delta R.T.: 0.000 min
Response: 2700422
Conc: 51.75 ng/ml

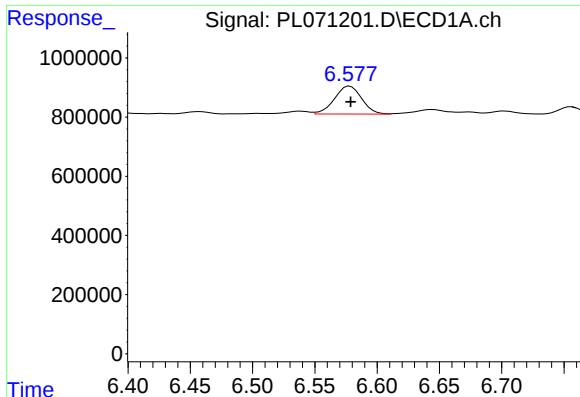

#24 Chlordane-2


R.T.: 6.578 min
Delta R.T.: 0.000 min
Response: 1430528
Conc: 63.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

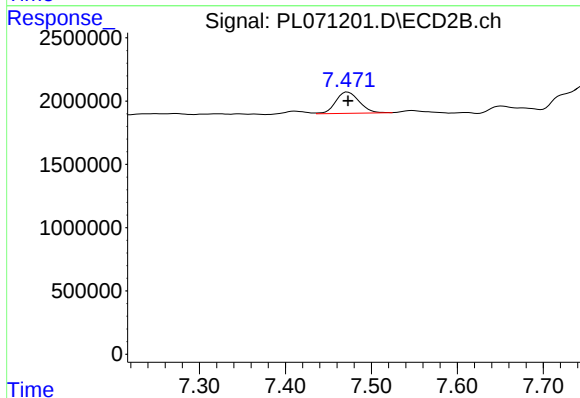


#24 Chlordane-2

R.T.: 7.472 min
Delta R.T.: 0.000 min
Response: 3218250
Conc: 57.32 ng/ml

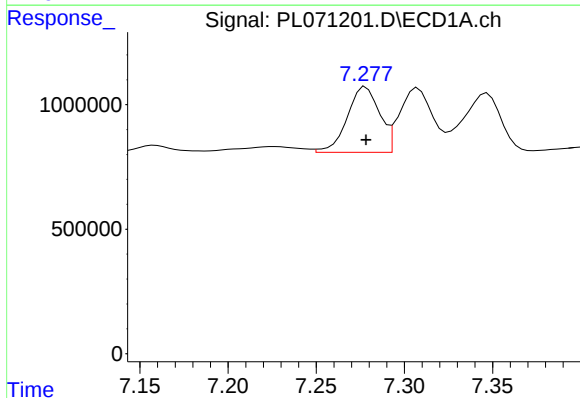


#25 Chlordane-3

R.T.: 7.278 min
Delta R.T.: 0.000 min
Response: 3340464
Conc: 54.76 ng/ml

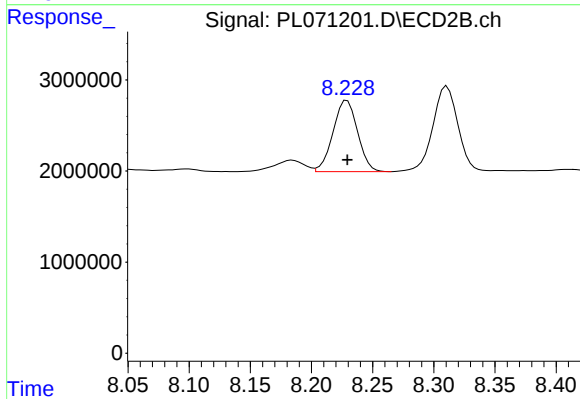

#25 Chlordane-3


R.T.: 8.229 min
Delta R.T.: 0.000 min
Response: 10931005
Conc: 49.31 ng/ml

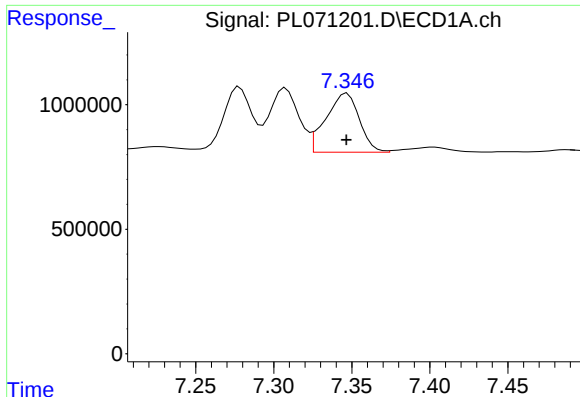

#26 Chlordane-4


R.T.: 7.347 min
Delta R.T.: 0.000 min
Response: 3527303
Conc: 53.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

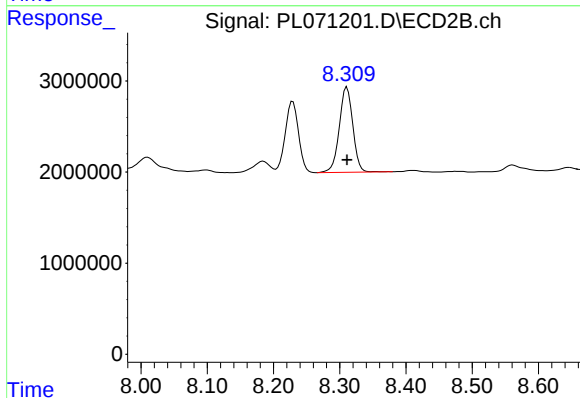


#26 Chlordane-4

R.T.: 8.311 min
Delta R.T.: 0.000 min
Response: 13304424
Conc: 49.65 ng/ml

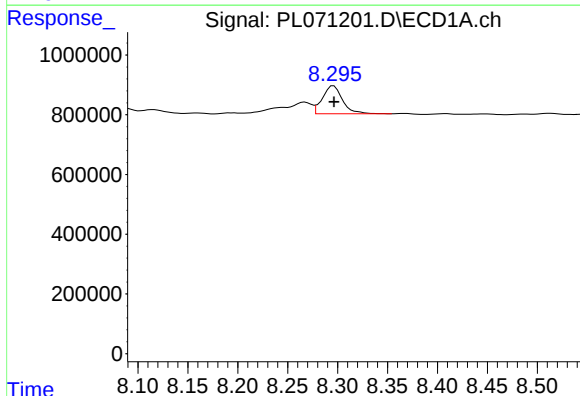


#27 Chlordane-5

R.T.: 8.296 min
Delta R.T.: 0.000 min
Response: 1306220
Conc: 55.51 ng/ml

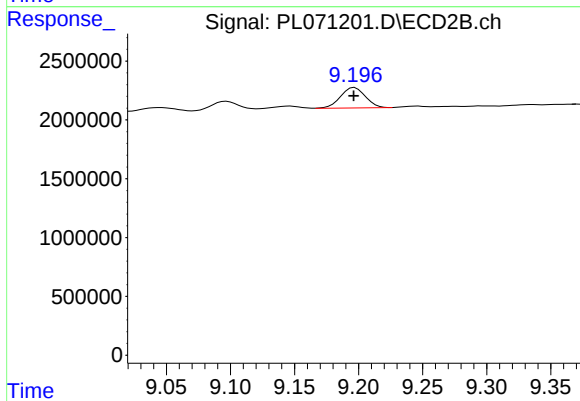

#27 Chlordane-5


R.T.: 9.197 min
Delta R.T.: 0.000 min
Response: 2344287
Conc: 49.55 ng/ml

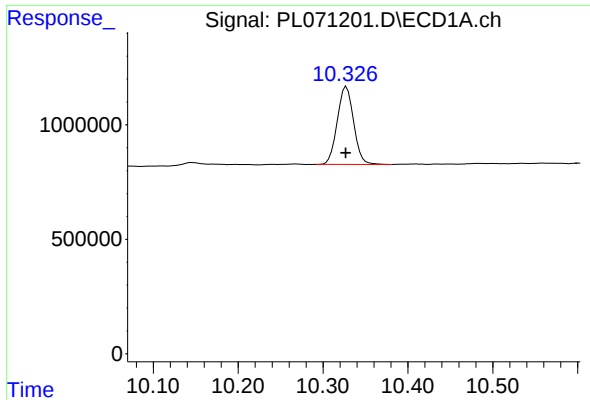

#28 Decachlorobiphenyl

R.T.: 10.328 min
Delta R.T.: 0.000 min
Response: 4555412
Conc: 6.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

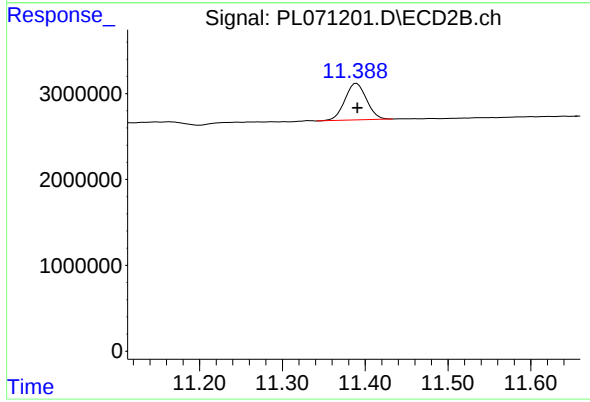

#28 Decachlorobiphenyl

R.T.: 11.390 min
Delta R.T.: 0.000 min
Response: 7718919
Conc: 5.33 ng/ml