

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL113021\
 Data File : PL071208.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2021 16:07
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL113021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 16:23:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 15:05:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.564	5.499	26522398	69352519	52.063	53.031
28)	SA Decachlor...	10.327	11.390	37032211	75299105	49.334	52.158
Target Compounds							
23)	Chlordane-1	5.890	6.880	8765417	28249539	521.305	532.384
24)	Chlordane-2	6.579	7.473	11778671	29648552	502.002	517.711
25)	Chlordane-3	7.279	8.229	31970475	116.4E6	515.491	529.225
26)	Chlordane-4	7.347	8.311	34330275	140.3E6	517.599	528.602
27)	Chlordane-5	8.296	9.197	12093246	24774960	506.631	525.516



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL113021\
Data File : PL071208.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2021 16:07
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL113021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 16:23:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 15:05:02 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

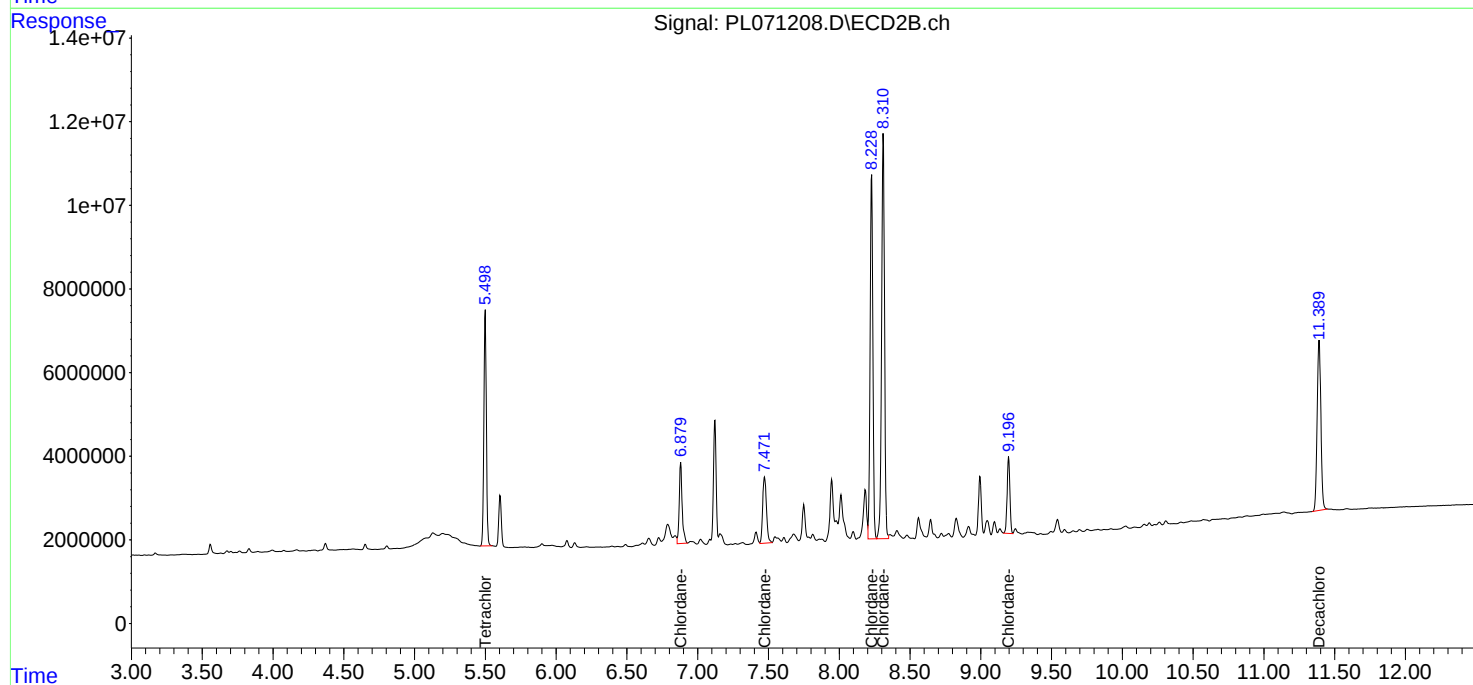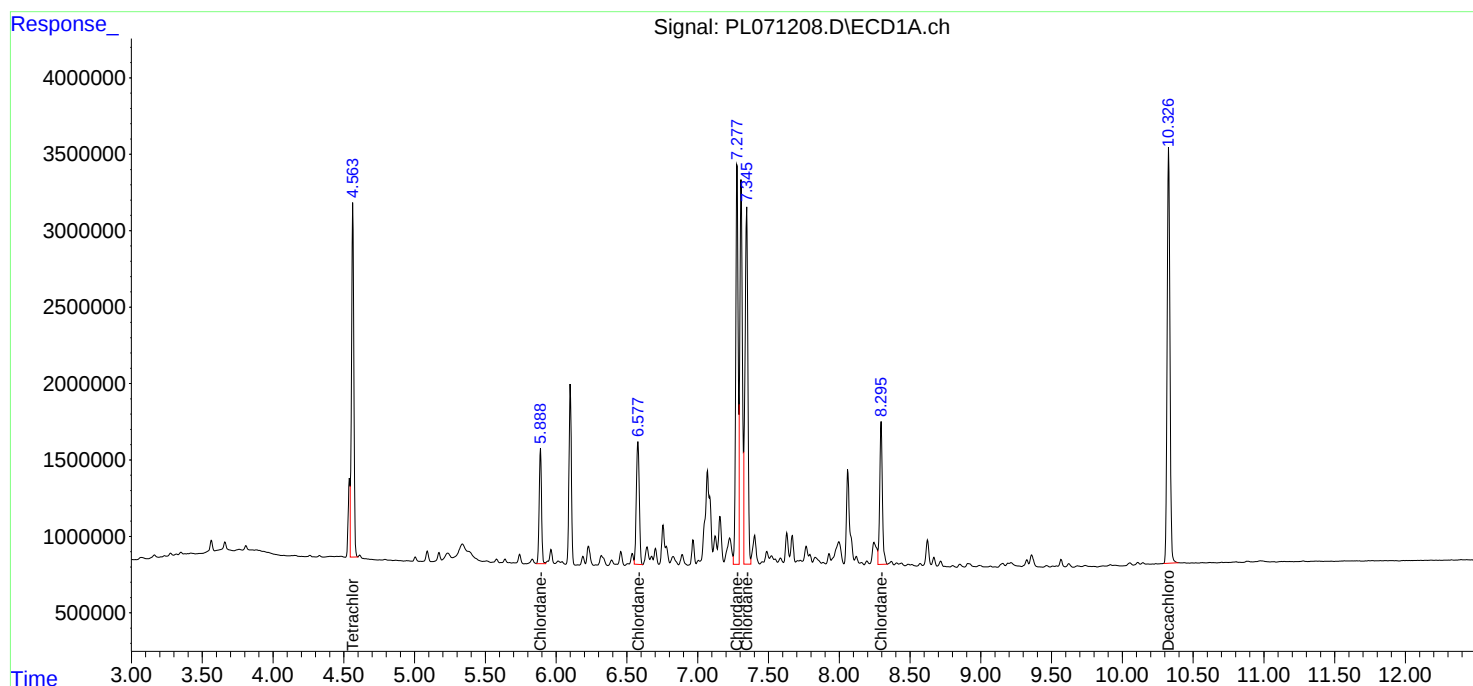


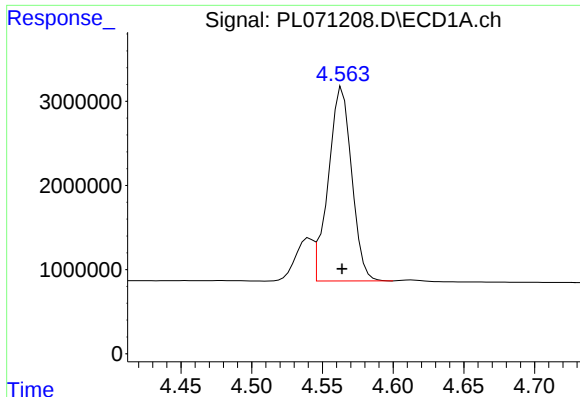

#1 Tetrachloro-m-xylene


R.T.: 4.564 min
Delta R.T.: 0.000 min
Response: 26522398
Conc: 52.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL113021

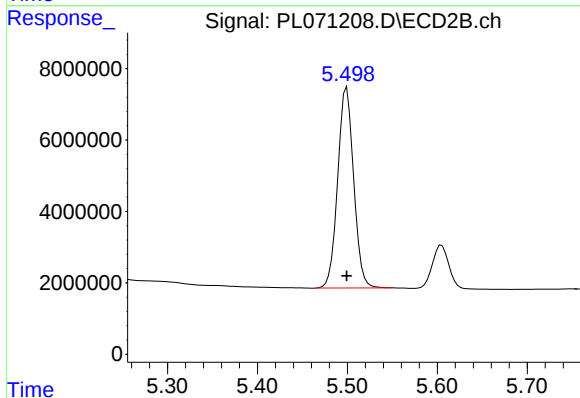


#1 Tetrachloro-m-xylene

R.T.: 5.499 min
Delta R.T.: 0.000 min
Response: 69352519
Conc: 53.03 ng/ml

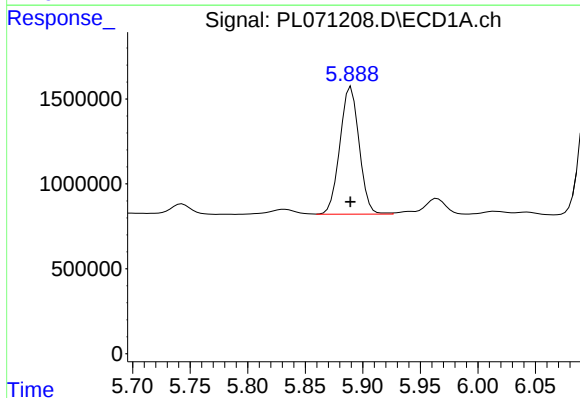


#23 Chlordane-1

R.T.: 5.890 min
Delta R.T.: 0.000 min
Response: 8765417
Conc: 521.31 ng/ml

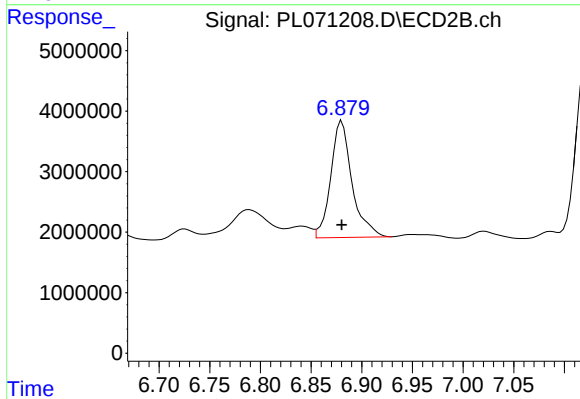

#23 Chlordane-1


R.T.: 6.880 min
Delta R.T.: 0.000 min
Response: 28249539
Conc: 532.38 ng/ml

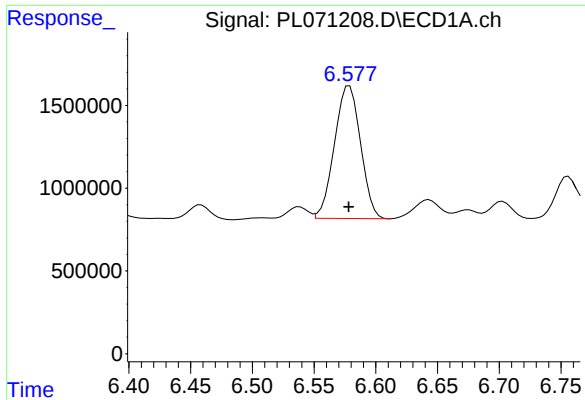

#24 Chlordane-2


R.T.: 6.579 min
Delta R.T.: 0.000 min
Response: 11778671
Conc: 502.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL113021

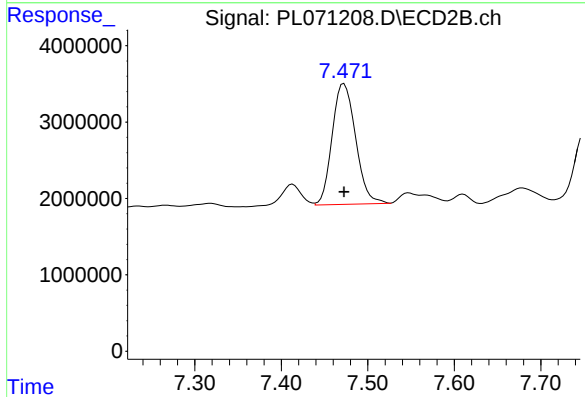


#24 Chlordane-2

R.T.: 7.473 min
Delta R.T.: 0.000 min
Response: 29648552
Conc: 517.71 ng/ml

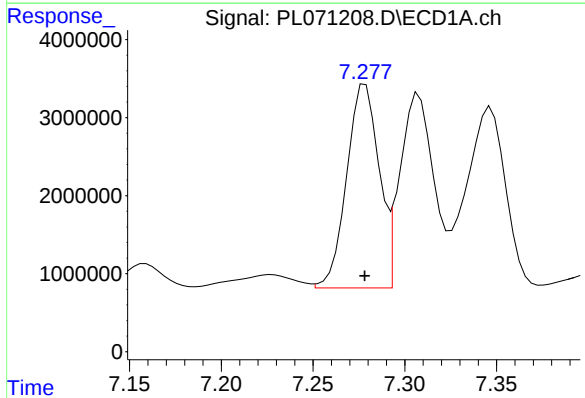


#25 Chlordane-3

R.T.: 7.279 min
Delta R.T.: 0.000 min
Response: 31970475
Conc: 515.49 ng/ml

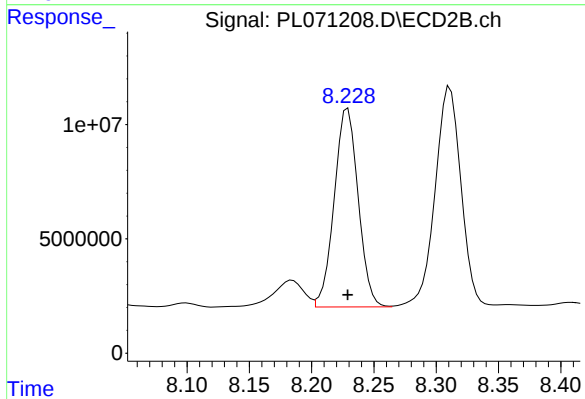

#25 Chlordane-3


R.T.: 8.229 min
Delta R.T.: 0.000 min
Response: 116371318
Conc: 529.22 ng/ml

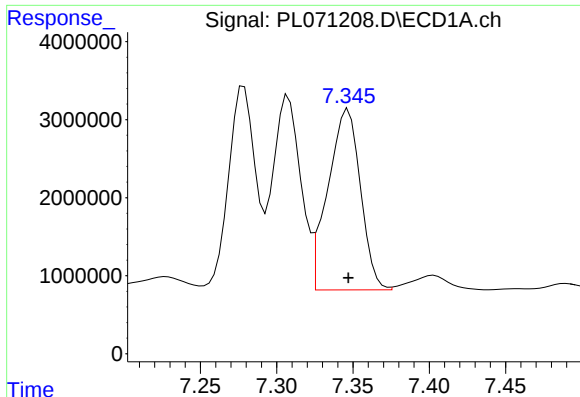

#26 Chlordane-4


R.T.: 7.347 min
Delta R.T.: 0.000 min
Response: 34330275
Conc: 517.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL113021

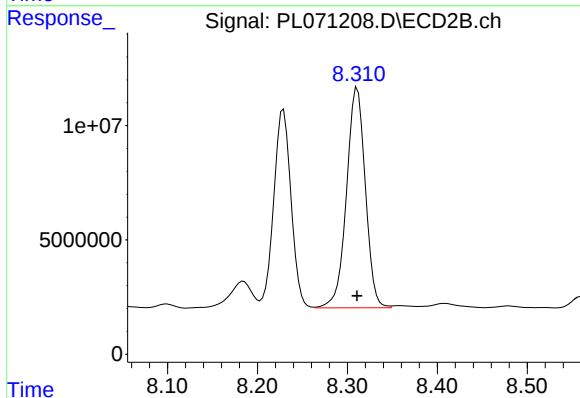


#26 Chlordane-4

R.T.: 8.311 min
Delta R.T.: 0.000 min
Response: 140258288
Conc: 528.60 ng/ml

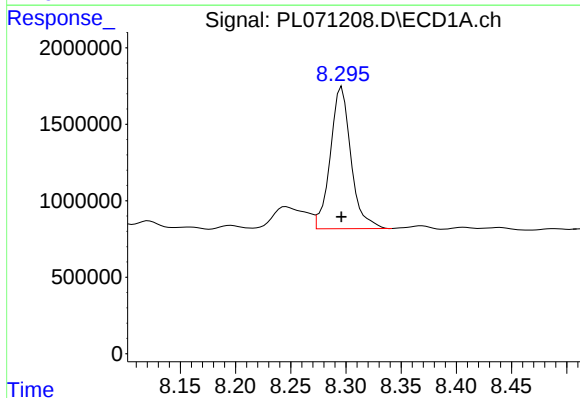


#27 Chlordane-5

R.T.: 8.296 min
Delta R.T.: 0.000 min
Response: 12093246
Conc: 506.63 ng/ml

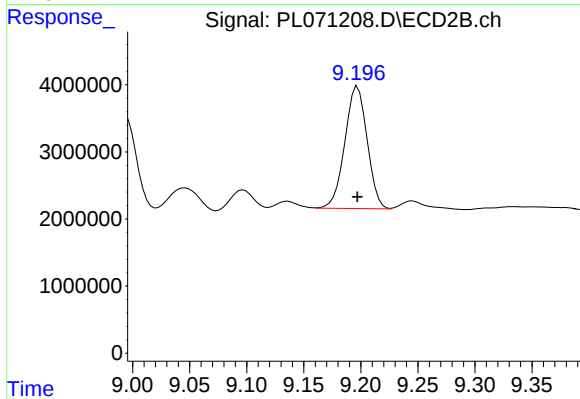

#27 Chlordane-5


R.T.: 9.197 min
Delta R.T.: 0.000 min
Response: 24774960
Conc: 525.52 ng/ml

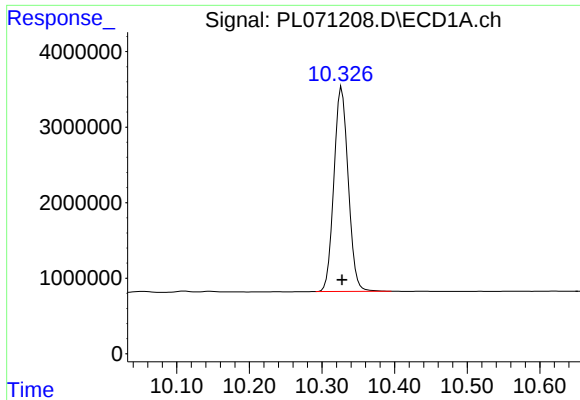

#28 Decachlorobiphenyl

R.T.: 10.327 min
Delta R.T.: 0.000 min
Response: 37032211
Conc: 49.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL113021

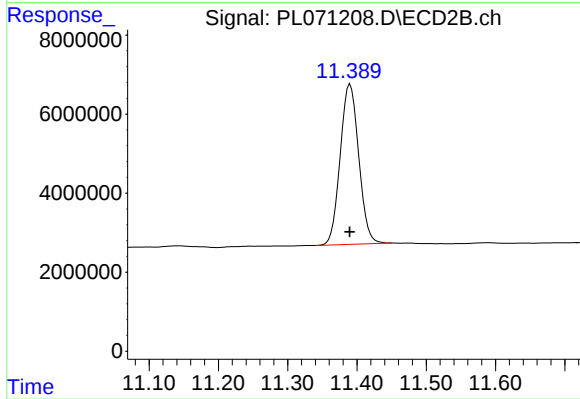

#28 Decachlorobiphenyl

R.T.: 11.390 min
Delta R.T.: 0.000 min
Response: 75299105
Conc: 52.16 ng/ml