

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120121\
 Data File : PL071222.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2021 08:45
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 23:37:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) B	Heptachlo...	6.998	7.971	1191252	7948340	1.911 5.003 #
10) B	gamma-Chl...	7.271	0.000	796845	0	1.255 N.D. #
11) B	alpha-Chl...	0.000	8.298	0	234123	N.D. 0.147 #
12) B	4,4'-DDE	7.560	0.000	144646	0	0.256 N.D. #
13) MA	Dieldrin	7.701	0.000	70118	0	0.116 N.D. #
19) B	Endosulfa...	0.000	9.491	0	1211510	N.D. 0.927 #
20) A	Methoxychlor	8.994	0.000	1378038	0	3.814 N.D. #
21) B	Endrin ke...	9.203f	0.000	3867750	0	5.427 N.D. #
23)	Chlordane-1	5.879	0.000	189939	0	11.296 N.D. #
25)	Chlordane-3	7.271	0.000	796845	0	12.848 N.D. #
26)	Chlordane-4	0.000	8.298	0	234123	N.D. 0.882 #
27)	Chlordane-5	0.000	9.208	0	3435423	N.D. 72.871 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120121\
Data File : PL071222.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2021 08:45
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 23:37:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

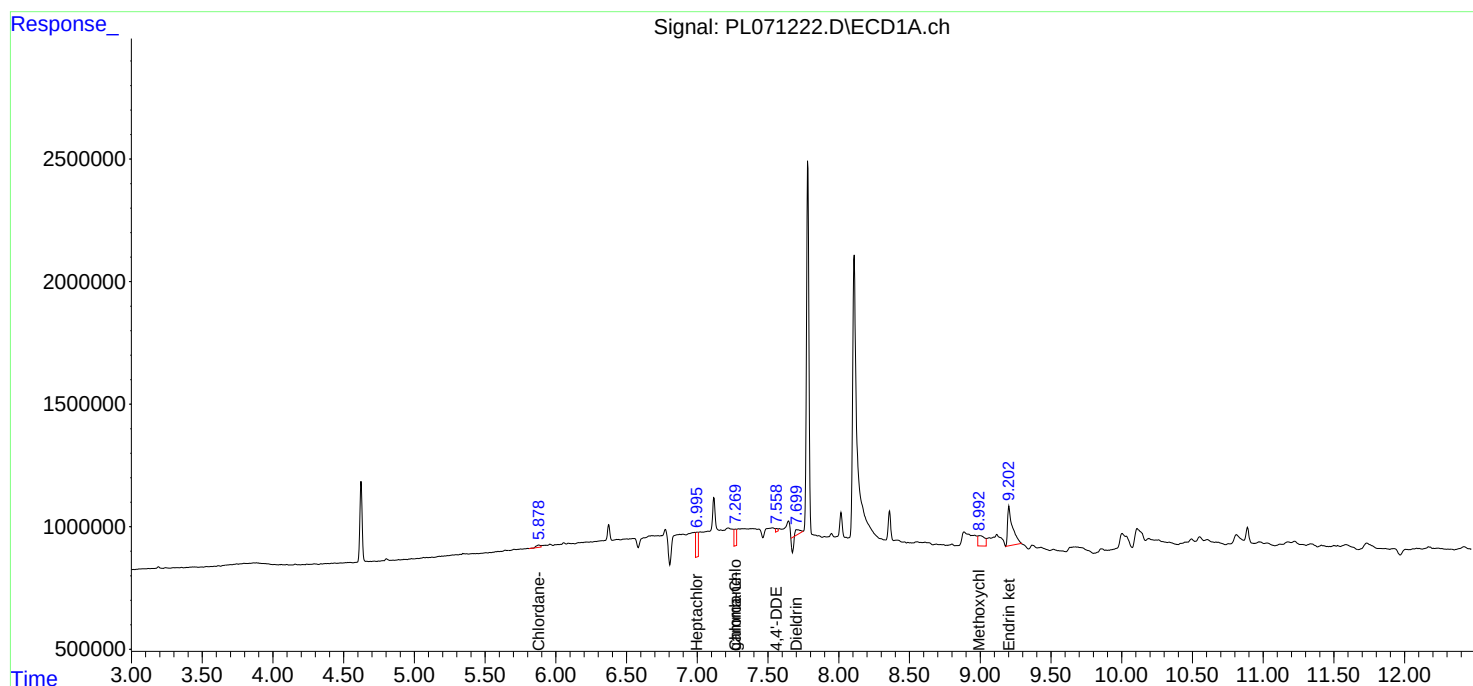


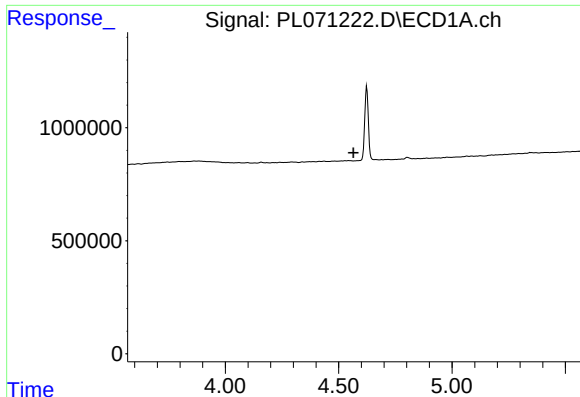

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

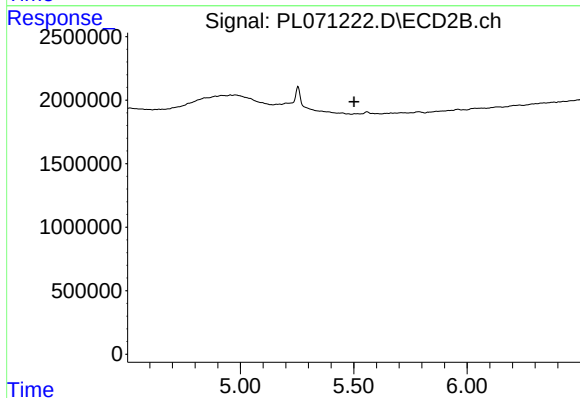


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.502 min
Response: 0
Conc: N.D.

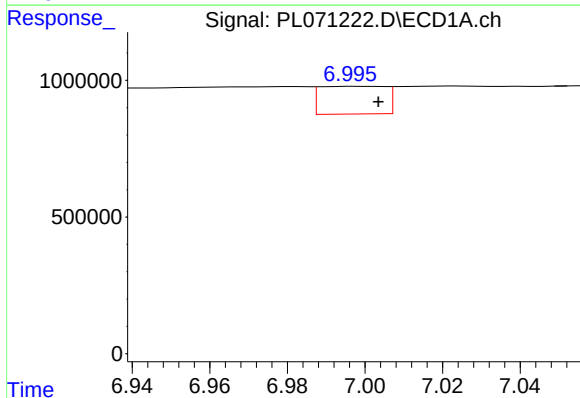


#8 Heptachlor epoxide

R.T.: 6.998 min
Delta R.T.: -0.005 min
Response: 1191252
Conc: 1.91 ng/ml

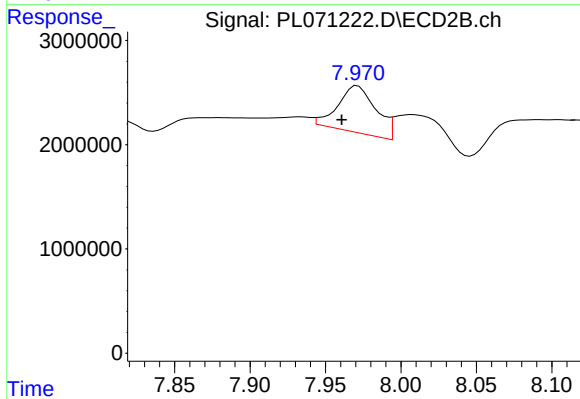

#8 Heptachlor epoxide


R.T.: 7.971 min
Delta R.T.: 0.010 min
Response: 7948340
Conc: 5.00 ng/ml

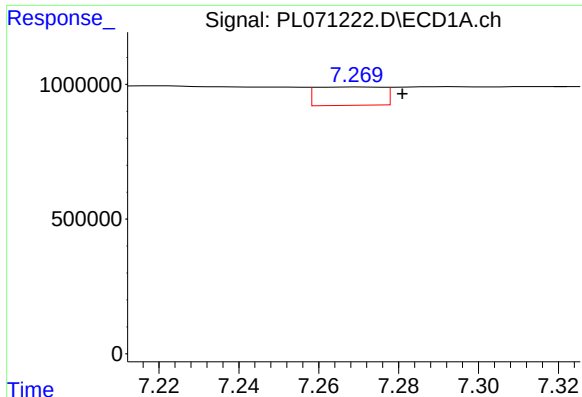

#10 gamma-Chlordane


R.T.: 7.271 min
Delta R.T.: -0.010 min
Response: 796845
Conc: 1.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

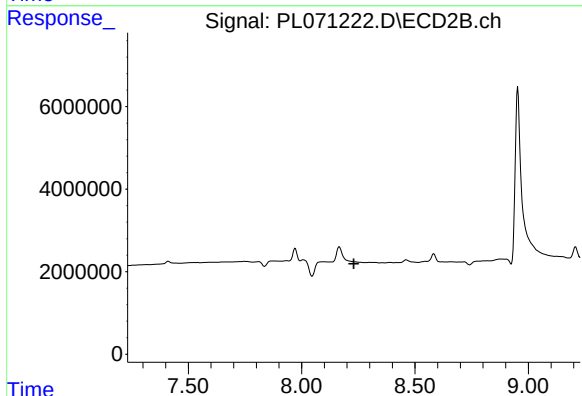


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.230 min
Response: 0
Conc: N.D.

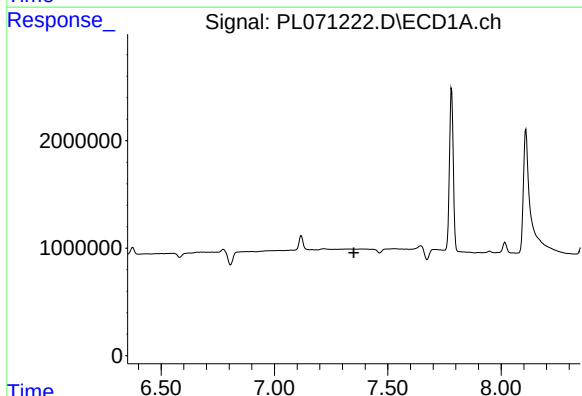


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.350 min
Response: 0
Conc: N.D.

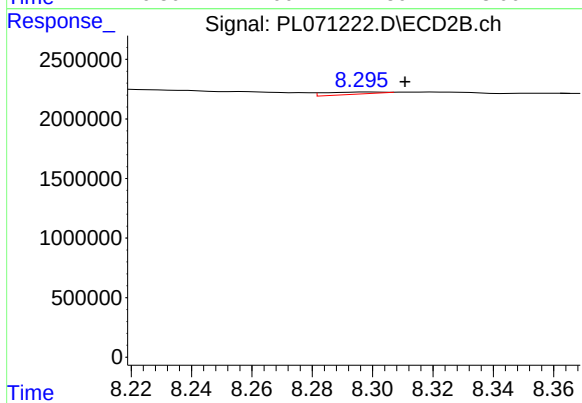

#11 alpha-Chlordane


R.T.: 8.298 min
Delta R.T.: -0.013 min
Response: 234123
Conc: 0.15 ng/ml

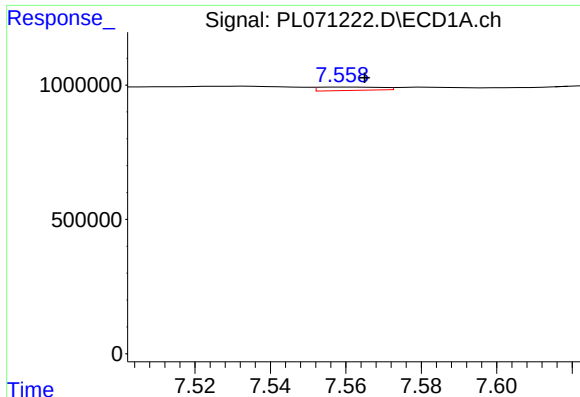

#12 4,4'-DDE


R.T.: 7.560 min
Delta R.T.: -0.005 min
Response: 144646
Conc: 0.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

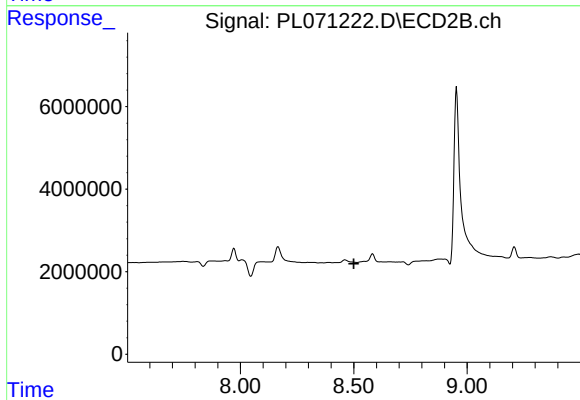


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 8.500 min
Response: 0
Conc: N.D.

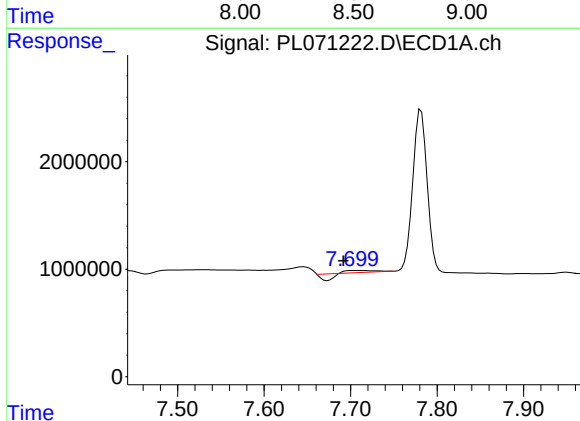


#13 Dieldrin

R.T.: 7.701 min
Delta R.T.: 0.009 min
Response: 70118
Conc: 0.12 ng/ml

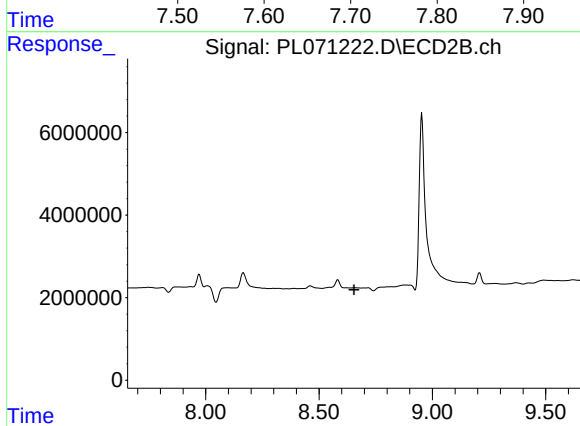

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 8.655 min
Response: 0
Conc: N.D.

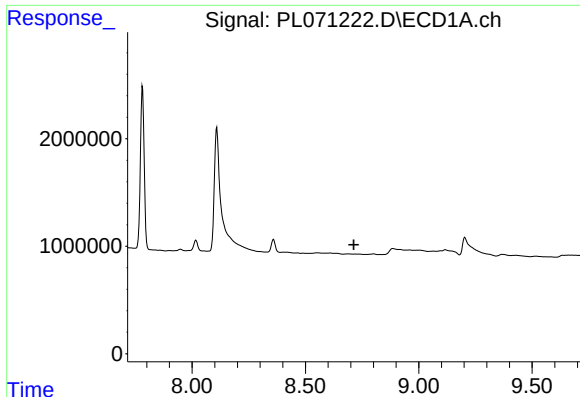

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 8.714 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

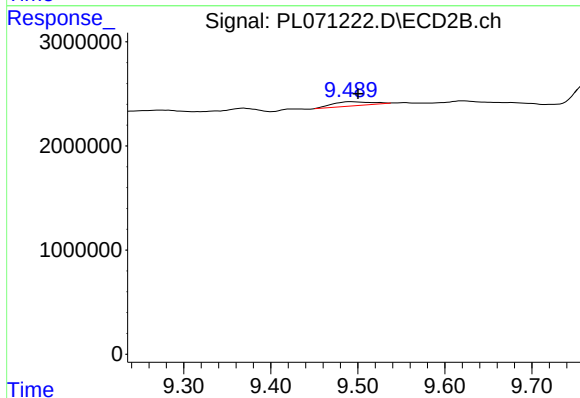


#19 Endosulfan Sulfate

R.T.: 9.491 min
Delta R.T.: -0.009 min
Response: 1211510
Conc: 0.93 ng/ml

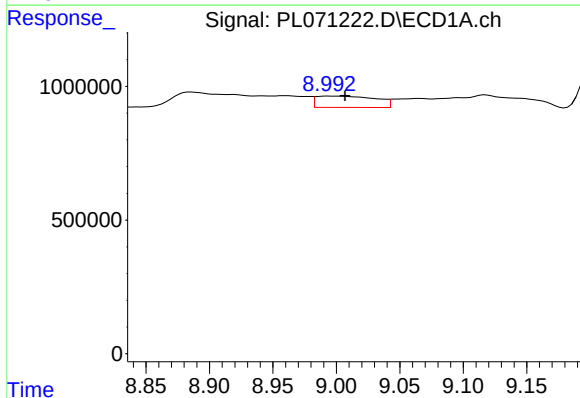


#20 Methoxychlor

R.T.: 8.994 min
Delta R.T.: -0.013 min
Response: 1378038
Conc: 3.81 ng/ml

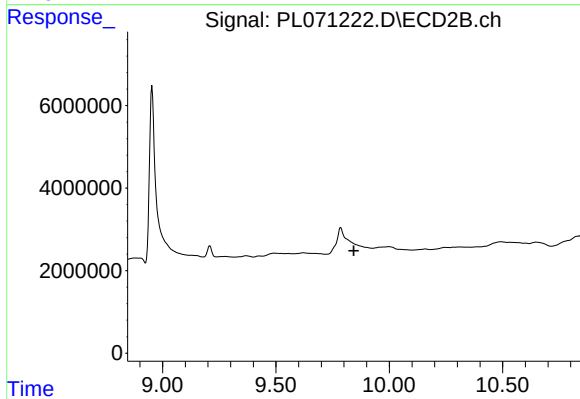

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 9.843 min
Response: 0
Conc: N.D.

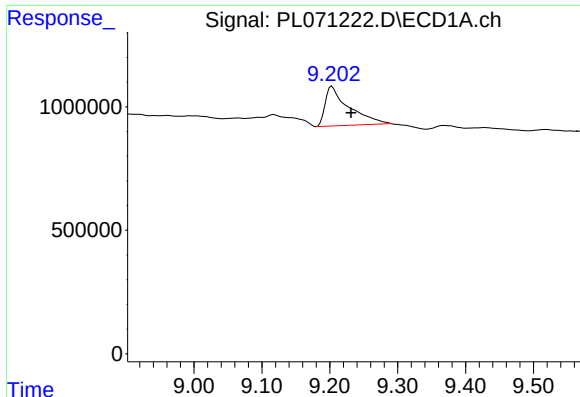

#21 Endrin ketone


R.T.: 9.203 min
Delta R.T.: -0.028 min
Response: 3867750
Conc: 5.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

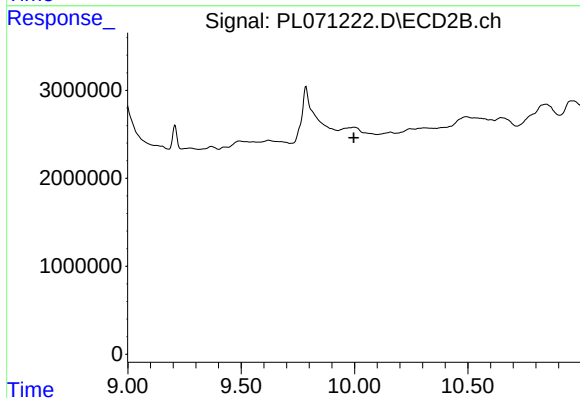


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.997 min
Response: 0
Conc: N.D.

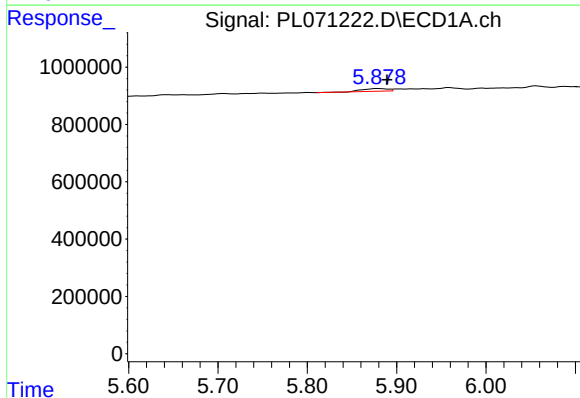


#23 Chlordane-1

R.T.: 5.879 min
Delta R.T.: -0.010 min
Response: 189939
Conc: 11.30 ng/ml

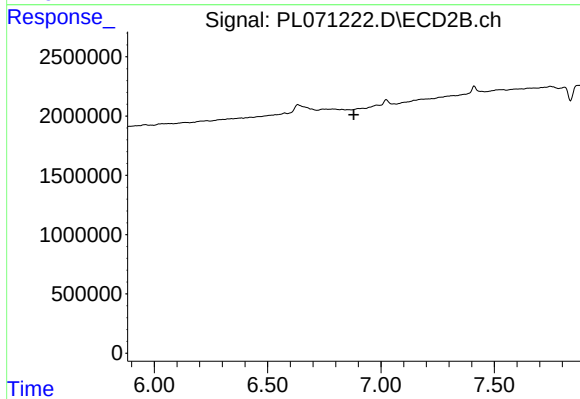

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 6.880 min
Response: 0
Conc: N.D.

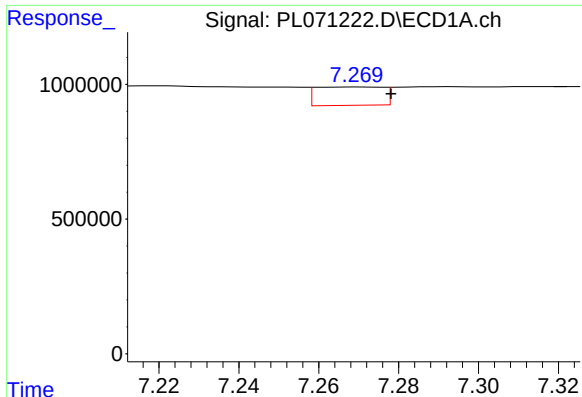

#25 Chlordane-3


R.T.: 7.271 min
Delta R.T.: -0.007 min
Response: 796845
Conc: 12.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

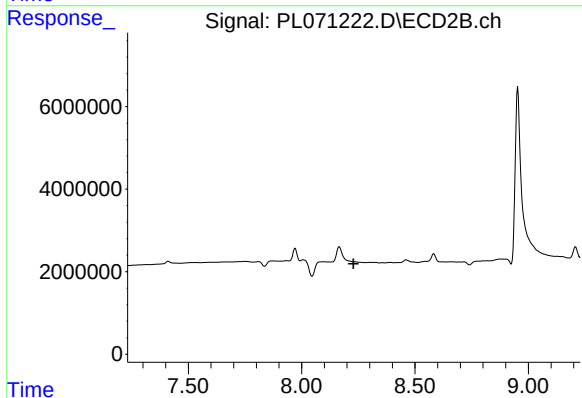


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 8.229 min
Response: 0
Conc: N.D.

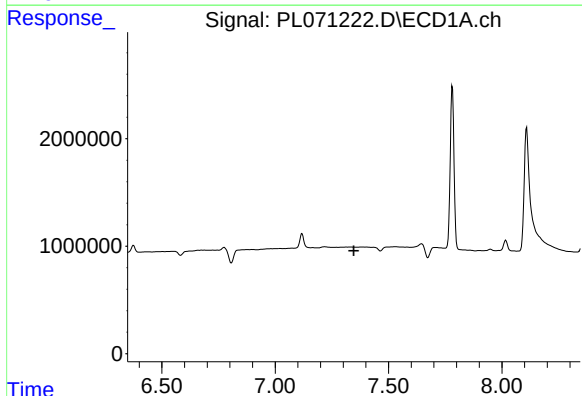


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.347 min
Response: 0
Conc: N.D.

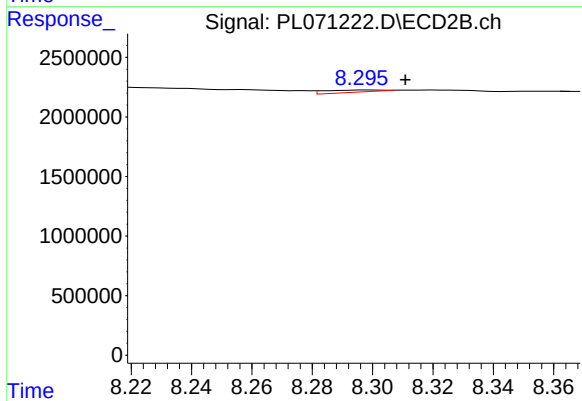

#26 Chlordane-4


R.T.: 8.298 min
Delta R.T.: -0.013 min
Response: 234123
Conc: 0.88 ng/ml

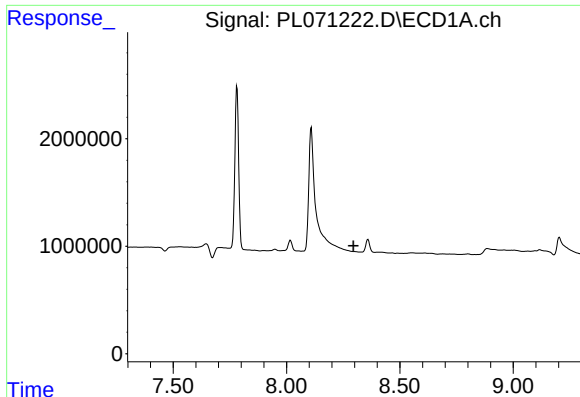

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.296 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

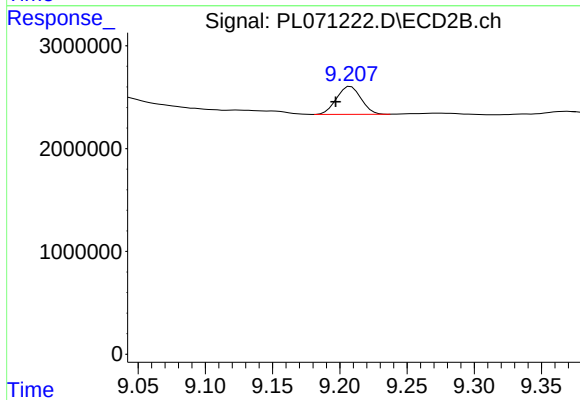


#27 Chlordane-5

R.T.: 9.208 min
Delta R.T.: 0.011 min
Response: 3435423
Conc: 72.87 ng/ml

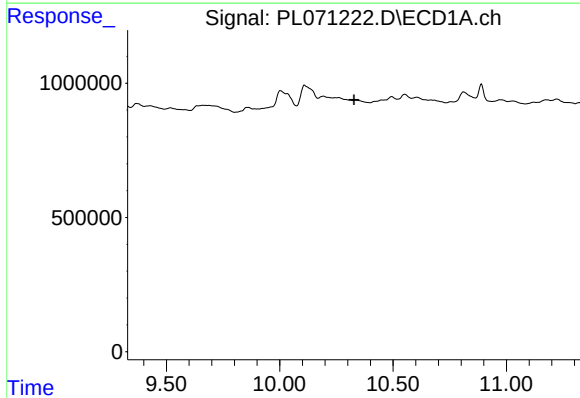

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 10.328 min
Response: 0
Conc: N.D.

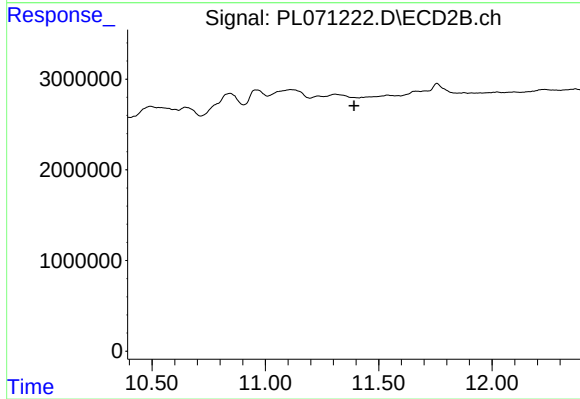

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 11.392 min
Response: 0
Conc: N.D.