

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120121\
 Data File : PL071228.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2021 13:11
 Operator : AR\AJ
 Sample : M4721-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 23:38:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.569	5.497	6205908	16834340	13.213	13.415
28)	SA Decachlor...	10.331	11.392	8884533	16824031	12.270	12.104
Target Compounds							
4)	MA Heptachlor	0.000	7.119	0	1298554	N.D.	0.708 #
6)	B beta-BHC	0.000	6.708f	0	13659615	N.D.	15.521 #
7)	B delta-BHC	0.000	7.020f	0	778112	N.D.	0.458 #
11)	B alpha-Chl...	7.322f	0.000	315534	0	0.493	N.D. #
12)	B 4,4'-DDE	7.568	8.498	372547	1143168	0.658	0.743
16)	A 4,4'-DDD	0.000	9.037	0	778133	N.D.	0.671 #
17)	MA 4,4'-DDT	8.409	0.000	248712	0	0.455	N.D. #
20)	A Methoxychlor	8.981f	0.000	439836	0	1.217	N.D. #
21)	B Endrin ke...	0.000	10.021f	0	555483	N.D.	0.379 #
26)	Chlordane-4	7.322f	0.000	315534	0	4.757	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120121\
Data File : PL071228.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2021 13:11
Operator : AR\AJ
Sample : M4721-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 23:38:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

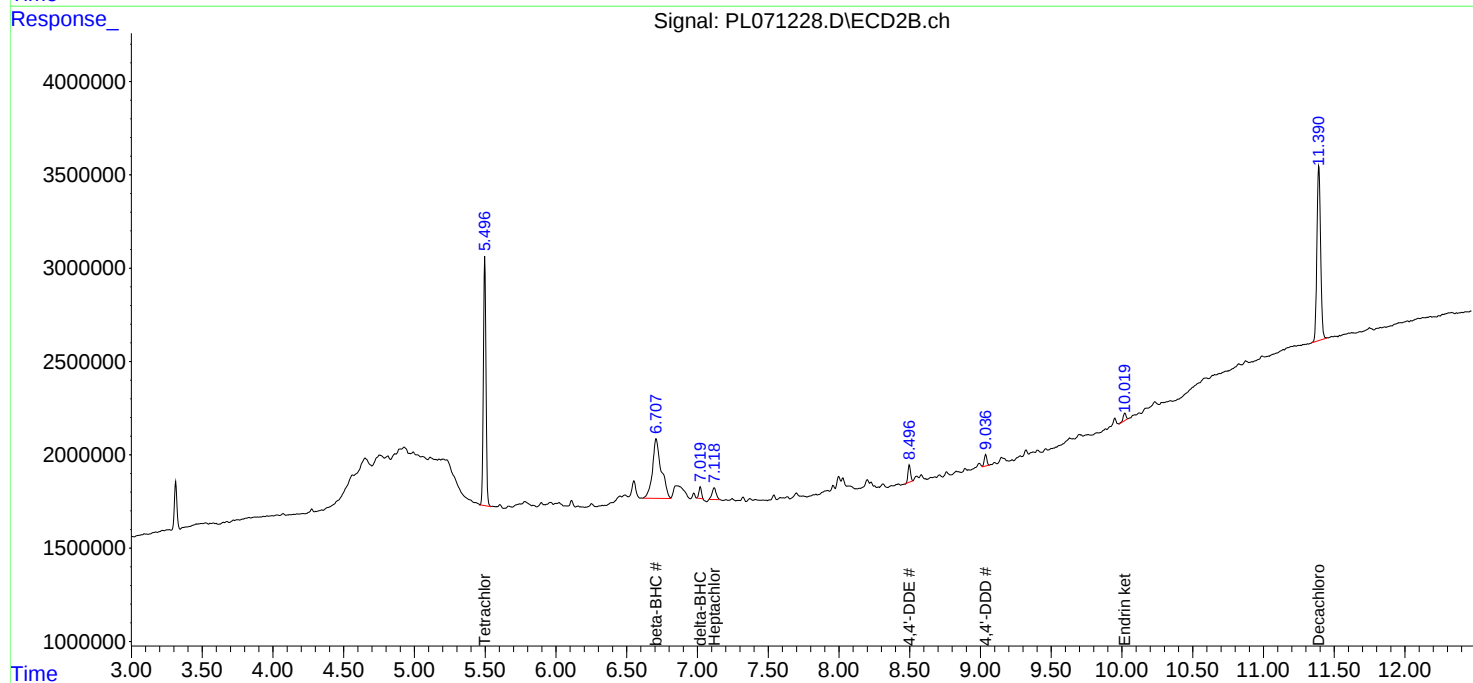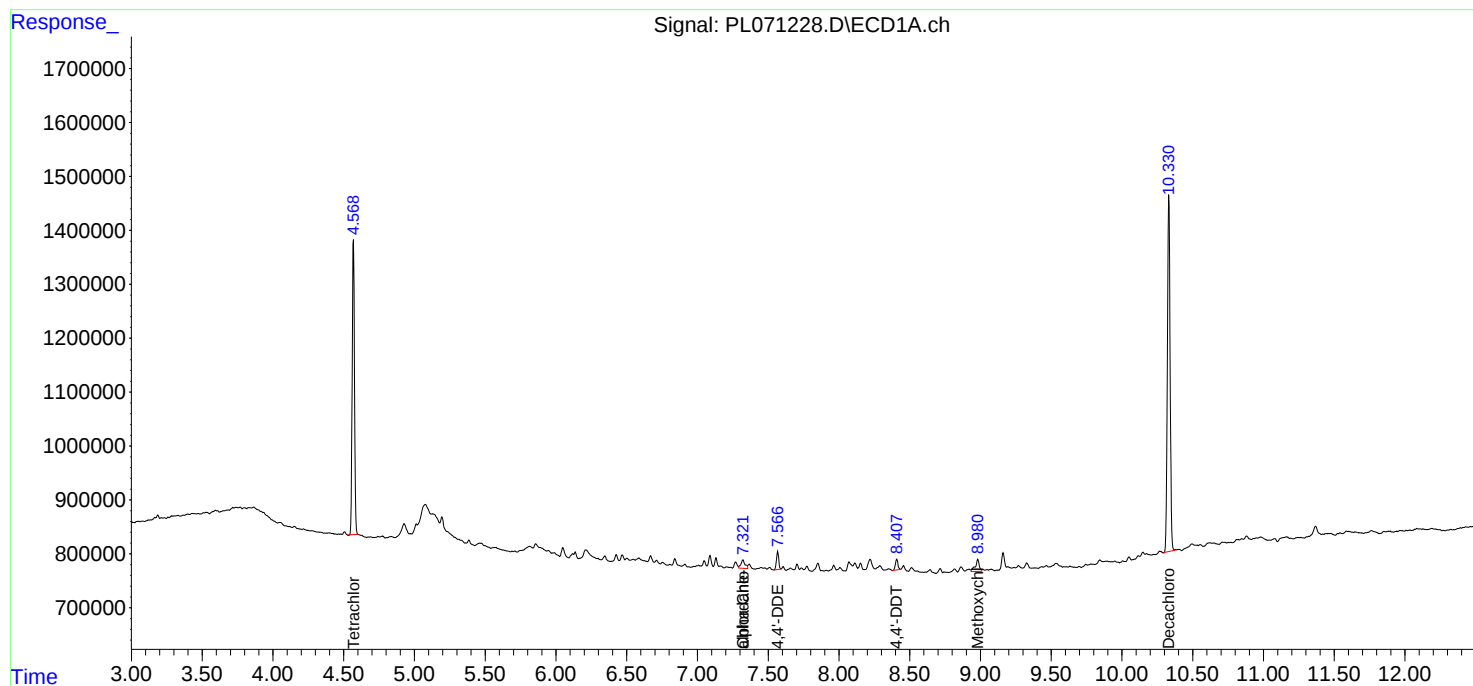


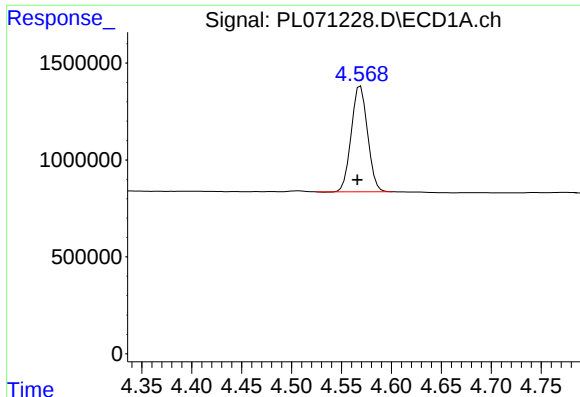

#1 Tetrachloro-m-xylene


R.T.: 4.569 min
Delta R.T.: 0.003 min
Response: 6205908
Conc: 13.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

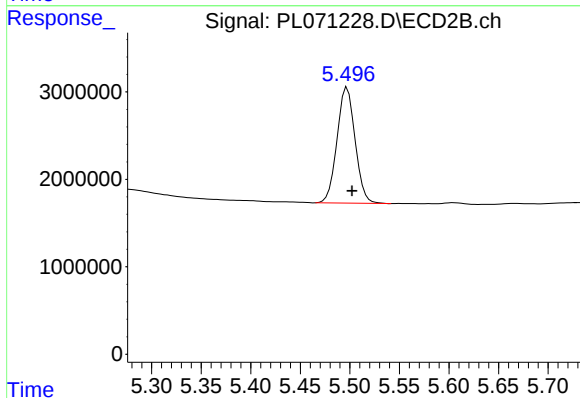


#1 Tetrachloro-m-xylene

R.T.: 5.497 min
Delta R.T.: -0.005 min
Response: 16834340
Conc: 13.41 ng/ml

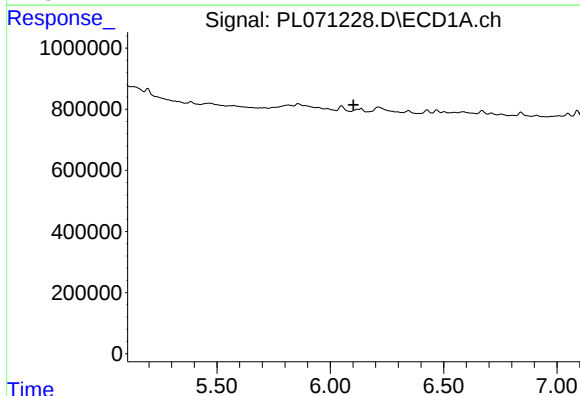


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 6.102 min
Response: 0
Conc: N.D.

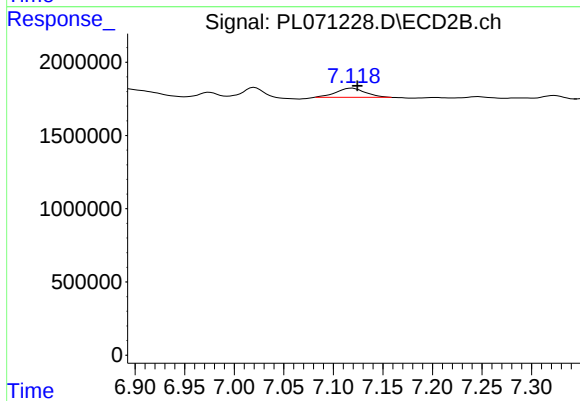

#4 Heptachlor


R.T.: 7.119 min
Delta R.T.: -0.005 min
Response: 1298554
Conc: 0.71 ng/ml

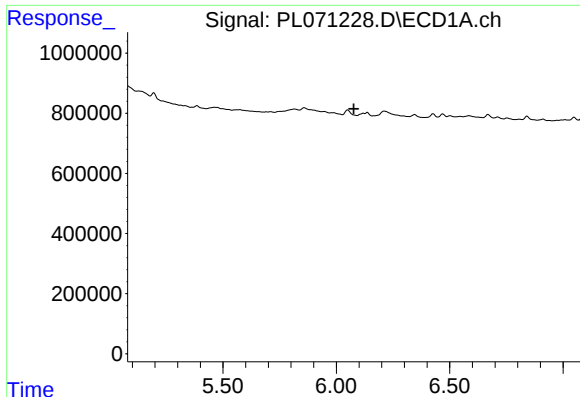

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.076 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

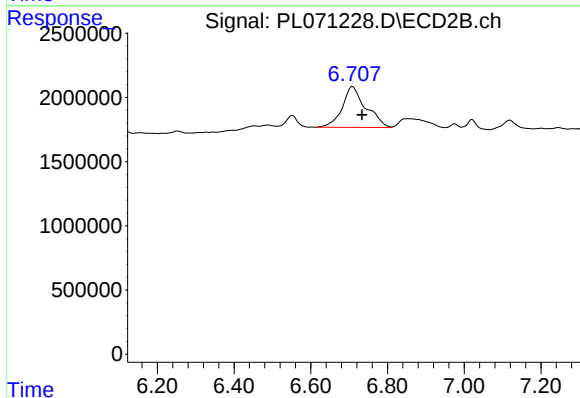


#6 beta-BHC

R.T.: 6.708 min
Delta R.T.: -0.026 min
Response: 13659615
Conc: 15.52 ng/ml

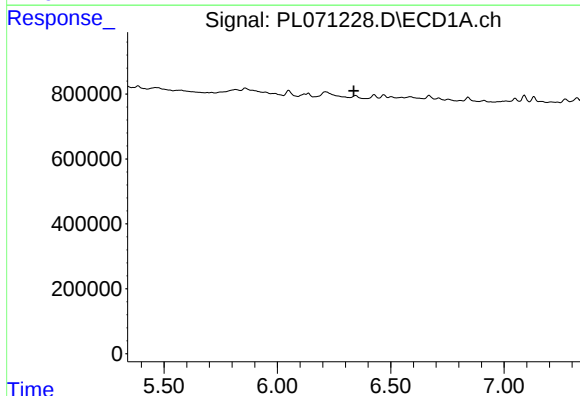


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.337 min
Response: 0
Conc: N.D.

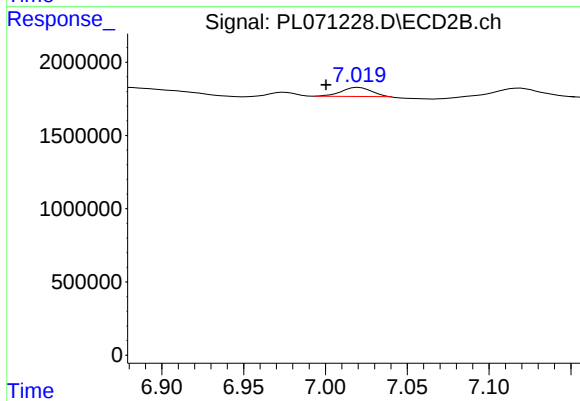

#7 delta-BHC


R.T.: 7.020 min
Delta R.T.: 0.020 min
Response: 778112
Conc: 0.46 ng/ml

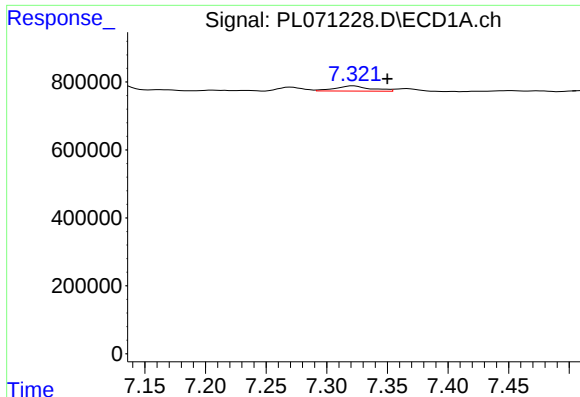

#11 alpha-Chlordane


R.T.: 7.322 min
Delta R.T.: -0.028 min
Response: 315534
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

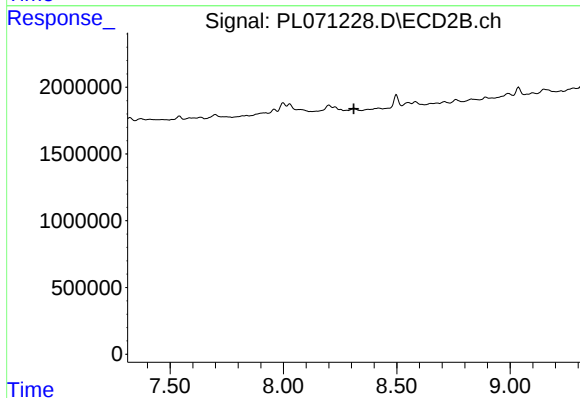


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.311 min
Response: 0
Conc: N.D.

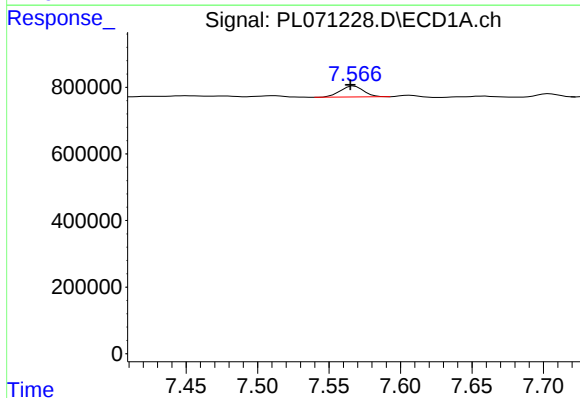


#12 4,4'-DDE

R.T.: 7.568 min
Delta R.T.: 0.003 min
Response: 372547
Conc: 0.66 ng/ml

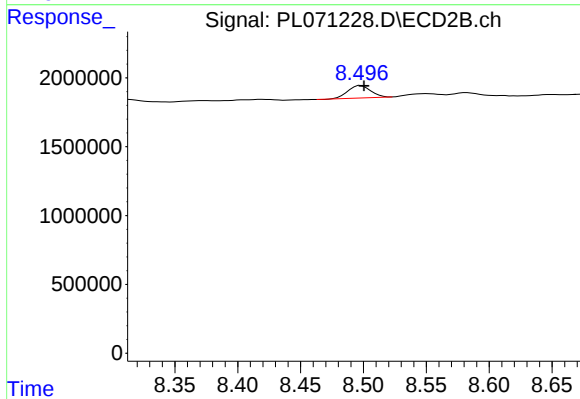

#12 4,4'-DDE


R.T.: 8.498 min
Delta R.T.: -0.003 min
Response: 1143168
Conc: 0.74 ng/ml

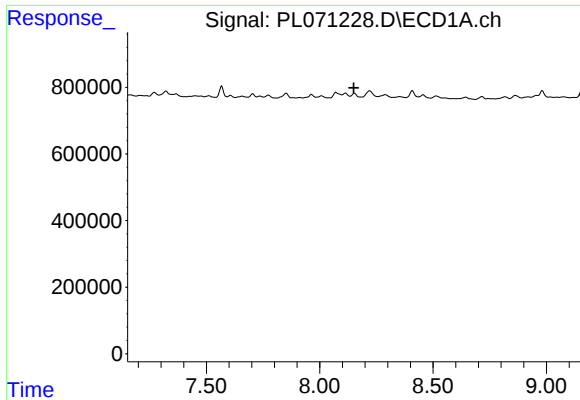

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

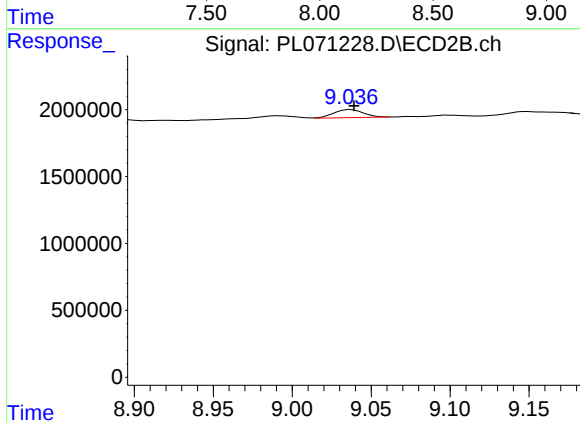


#16 4,4'-DDD

R.T.: 9.037 min
Delta R.T.: -0.002 min
Response: 778133
Conc: 0.67 ng/ml

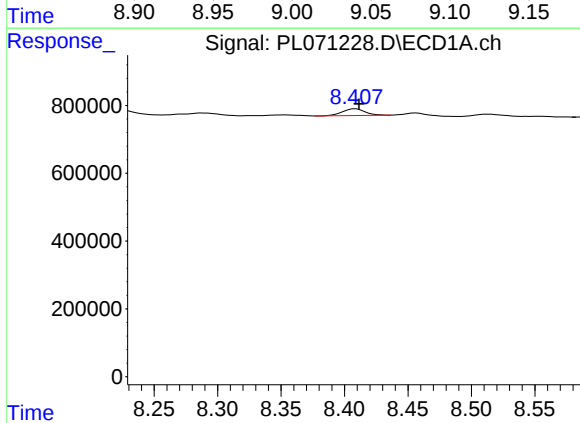


#17 4,4'-DDT

R.T.: 8.409 min
Delta R.T.: -0.003 min
Response: 248712
Conc: 0.45 ng/ml

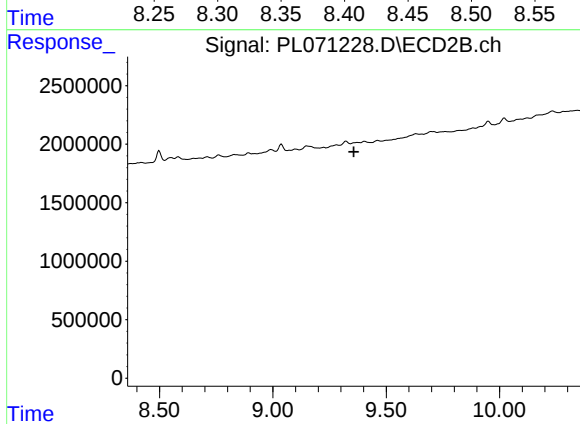

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.356 min
Response: 0
Conc: N.D.

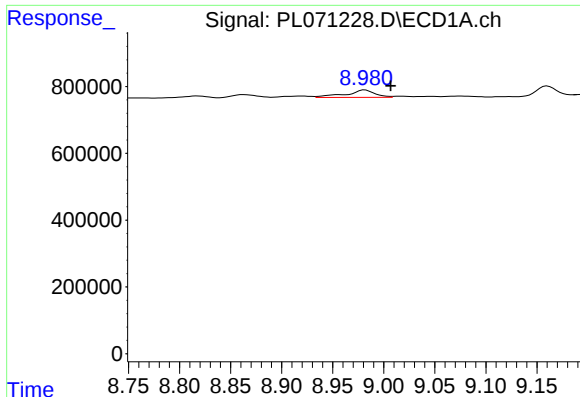

#20 Methoxychlor


R.T.: 8.981 min
Delta R.T.: -0.025 min
Response: 439836
Conc: 1.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

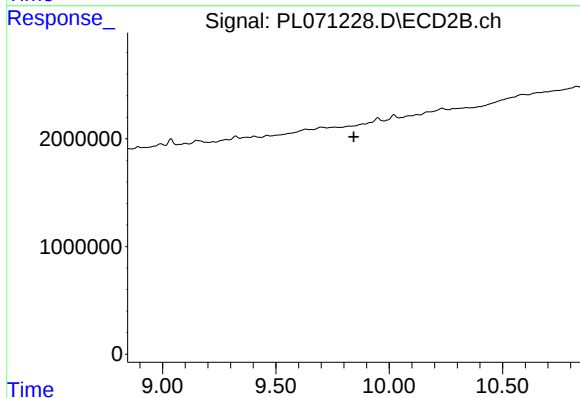


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.843 min
Response: 0
Conc: N.D.

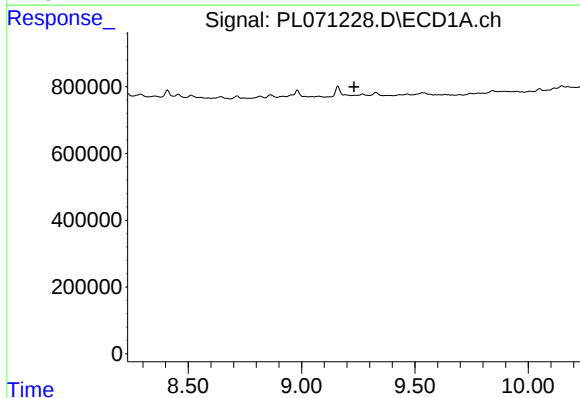


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.231 min
Response: 0
Conc: N.D.

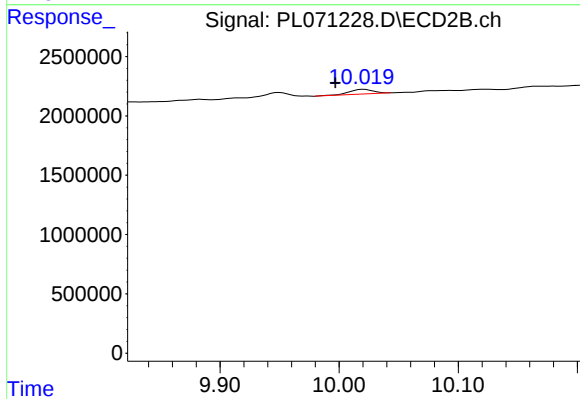

#21 Endrin ketone


R.T.: 10.021 min
Delta R.T.: 0.024 min
Response: 555483
Conc: 0.38 ng/ml

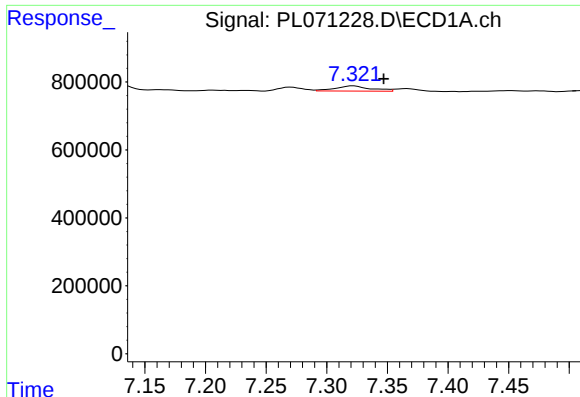

#26 Chlordane-4


R.T.: 7.322 min
Delta R.T.: -0.025 min
Response: 315534
Conc: 4.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

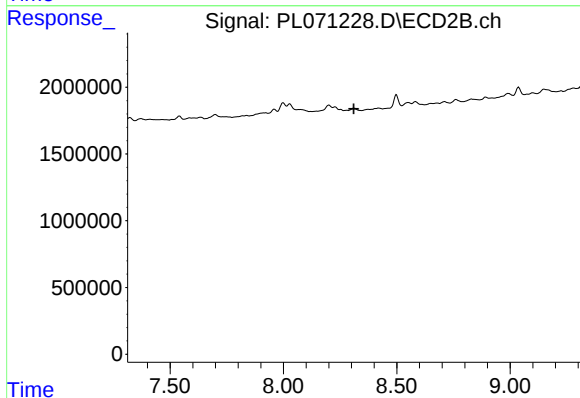


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.311 min
Response: 0
Conc: N.D.

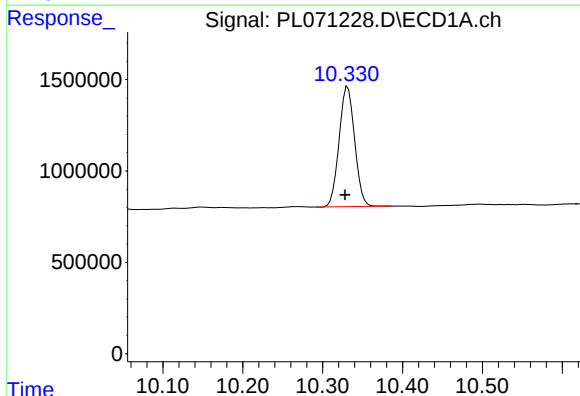

#28 Decachlorobiphenyl

R.T.: 10.331 min
Delta R.T.: 0.004 min
Response: 8884533
Conc: 12.27 ng/ml

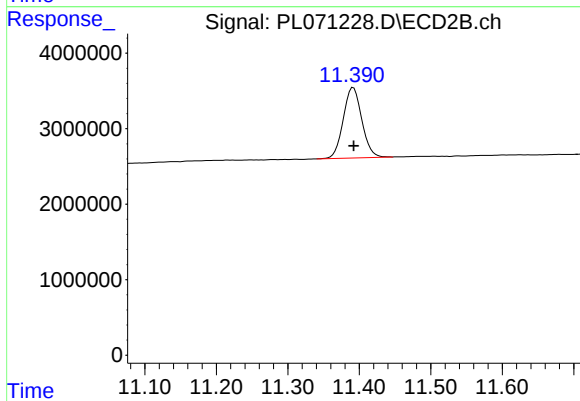

#28 Decachlorobiphenyl

R.T.: 11.392 min
Delta R.T.: 0.000 min
Response: 16824031
Conc: 12.10 ng/ml