

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120121\
 Data File : PL071226.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2021 12:27
 Operator : AR\AJ
 Sample : PB141093BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB141093BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/02/2021
 Supervised By : Ankita Jodhani 12/02/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 23:37:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.570	5.498	9426412	24597464	20.069m	19.601
2) SA Decachlor...	10.334	11.394	14435573	26141890	19.936	18.807

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120121\
Data File : PL071226.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2021 12:27
Operator : AR\AJ
Sample : PB141093BL
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB141093BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/02/2021
Supervised By : Ankita Jodhani 12/02/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 23:37:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

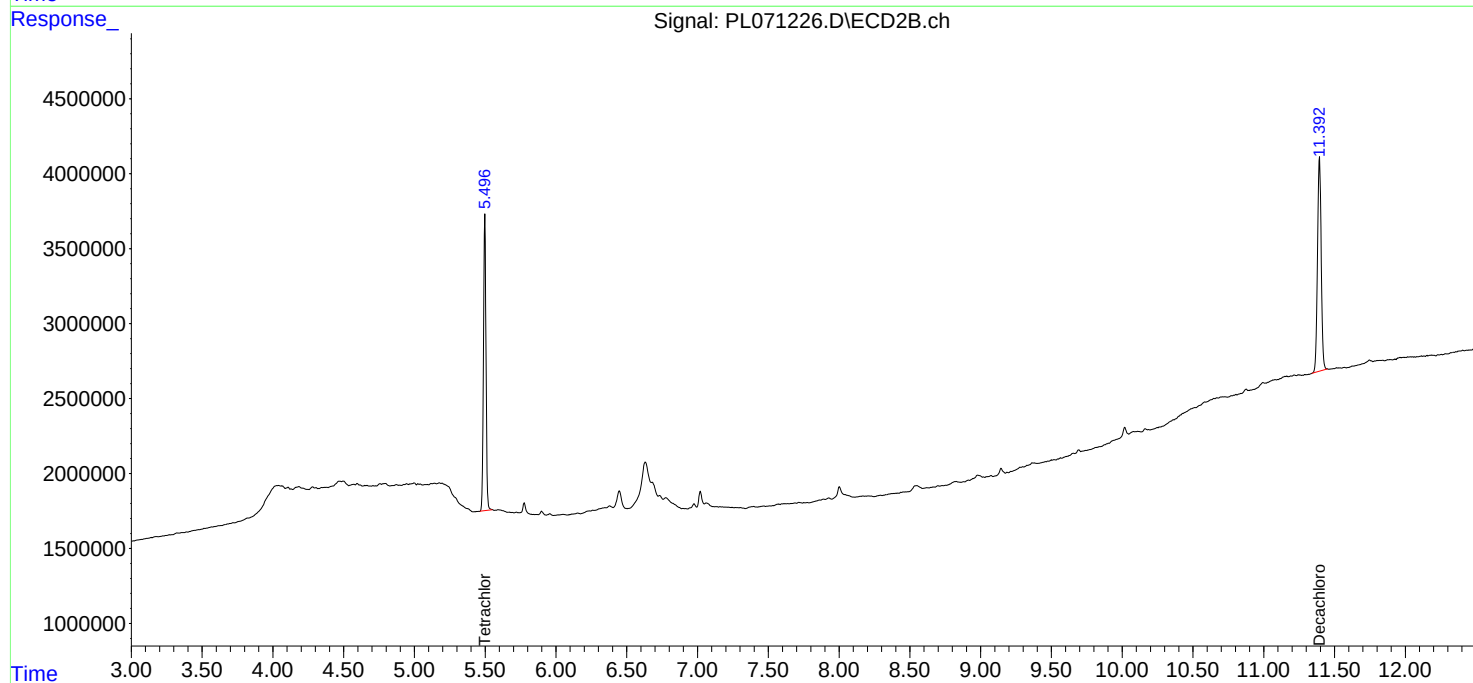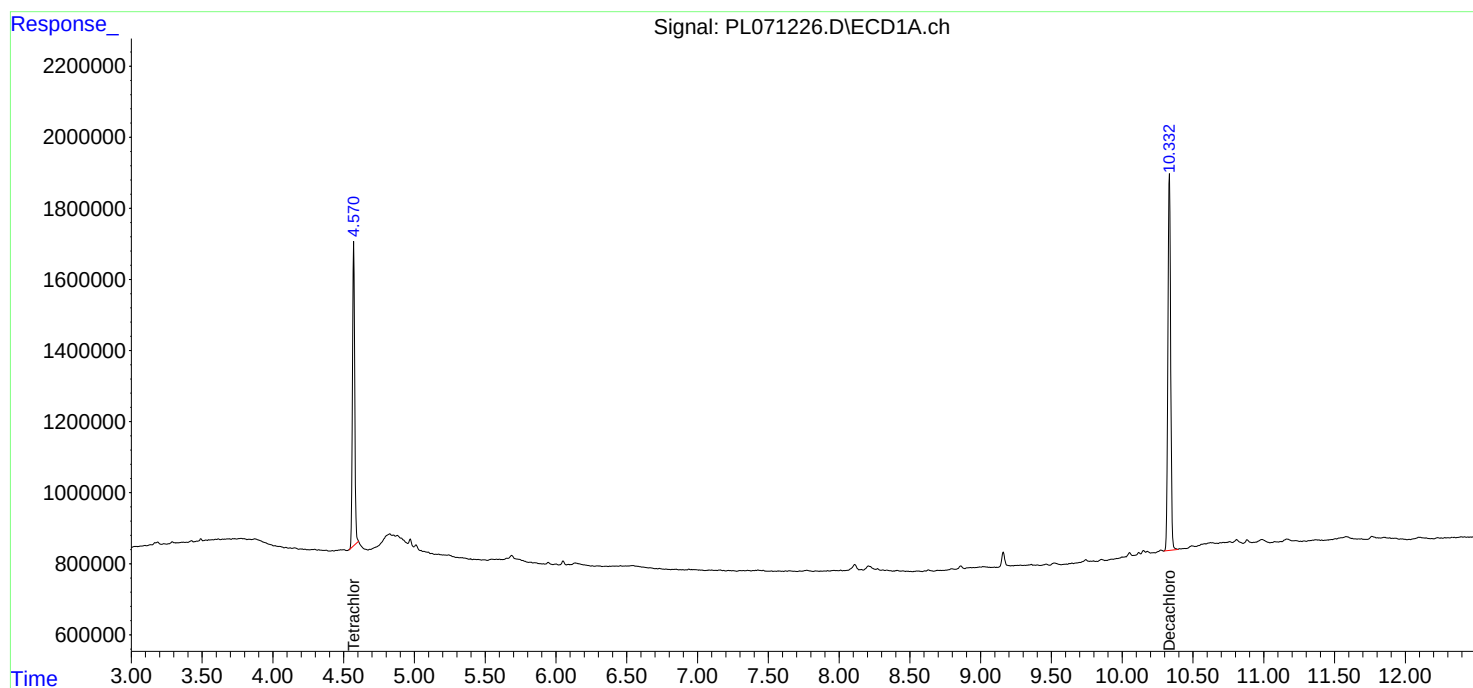

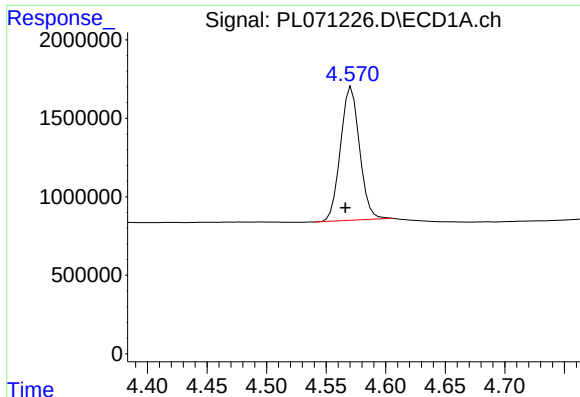

#1 Tetrachloro-m-xylene

R.T.: 4.570 min
Delta R.T.: 0.004 min
Response: 9426412
Conc: 20.07 ng/ml

Instrument :

ECD_L


ClientSampleId :

PB141093BL

Manual Integrations


APPROVED

Reviewed By :Abdul Mirza 12/02/2021
Supervised By :Ankita Jodhani 12/02/2021

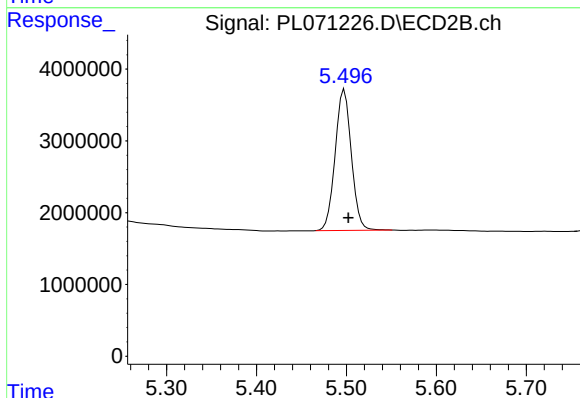


#1 Tetrachloro-m-xylene

R.T.: 5.498 min
Delta R.T.: -0.004 min
Response: 24597464
Conc: 19.60 ng/ml

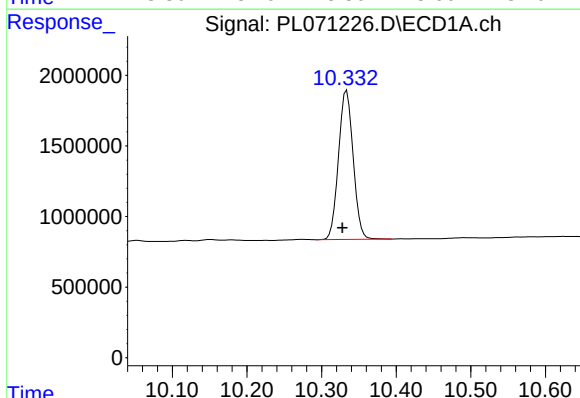

#28 Decachlorobiphenyl

R.T.: 10.334 min
Delta R.T.: 0.006 min
Response: 14435573
Conc: 19.94 ng/ml

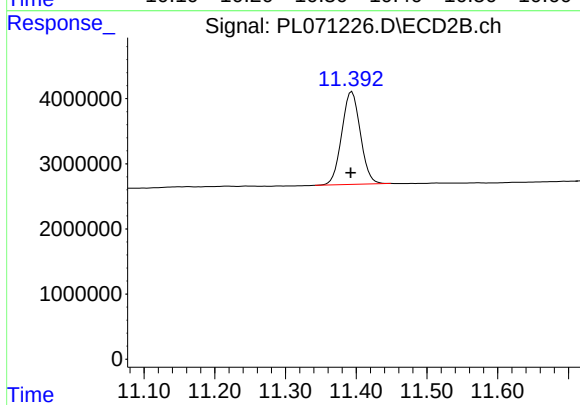

#28 Decachlorobiphenyl

R.T.: 11.394 min
Delta R.T.: 0.002 min
Response: 26141890
Conc: 18.81 ng/ml