

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120122\
 Data File : PL079532.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2022 14:31
 Operator : AR\AJ
 Sample : N5807-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 20:41:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 24 00:09:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	2.565	39093070	44406347	17.305	16.314
28)	SA Decachlor...	8.766	7.630	34421462	38158396	17.724	16.243
Target Compounds							
2)	A alpha-BHC	3.765	0.000	1147459	0	0.334	N.D. #
7)	B delta-BHC	4.539f	0.000	4213660	0	1.519	N.D. #
8)	B Heptachlo...	0.000	4.474	0	1064010	N.D.	0.315 #
9)	A Endosulfan I	5.840	0.000	50472	0	0.019	N.D. #
10)	B gamma-Chl...	5.702	0.000	301659	0	0.105	N.D. #
14)	MA Endrin	0.000	5.387f	0	794923	N.D.	0.263 #
15)	B Endosulfa...	6.548f	0.000	2737648	0	1.213	N.D. #
16)	A 4,4'-DDD	6.494	0.000	41829	0	0.021	N.D. #
17)	MA 4,4'-DDT	6.785f	0.000	254665	0	0.112	N.D. #
18)	B Endrin al...	0.000	5.864f	0	268935	N.D.	0.126 #
23)	Chlordane-1	0.000	3.515	0	2115719	N.D.	19.892 #
25)	Chlordane-3	5.702	0.000	301659	0	0.726	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120122\
Data File : PL079532.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2022 14:31
Operator : AR\AJ
Sample : N5807-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 20:41:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
Quant Title : GC Extractables
QLast Update : Thu Nov 24 00:09:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

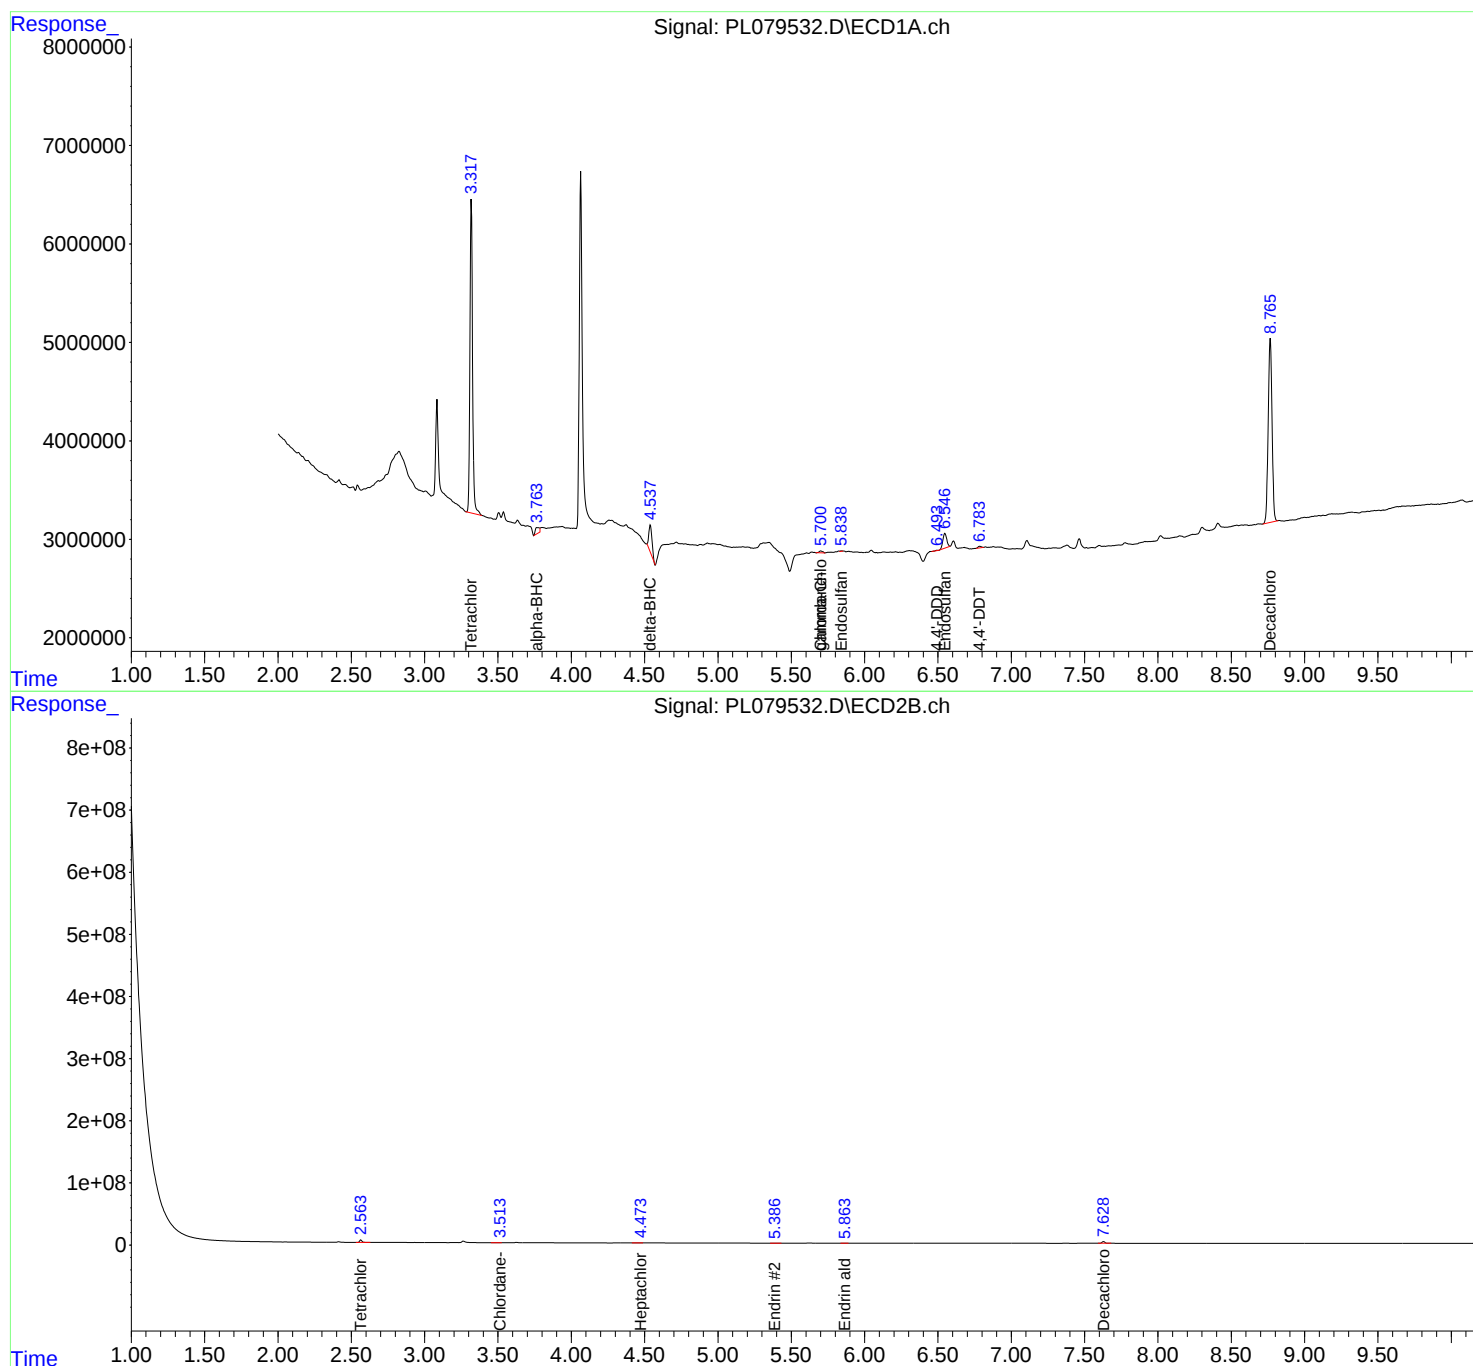


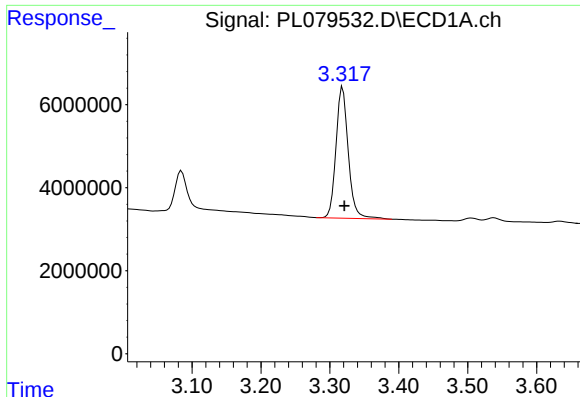

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: -0.002 min
Response: 39093070
Conc: 17.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

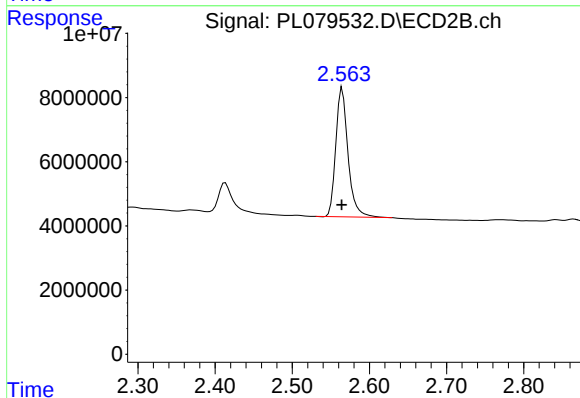


#1 Tetrachloro-m-xylene

R.T.: 2.565 min
Delta R.T.: 0.000 min
Response: 44406347
Conc: 16.31 ng/ml

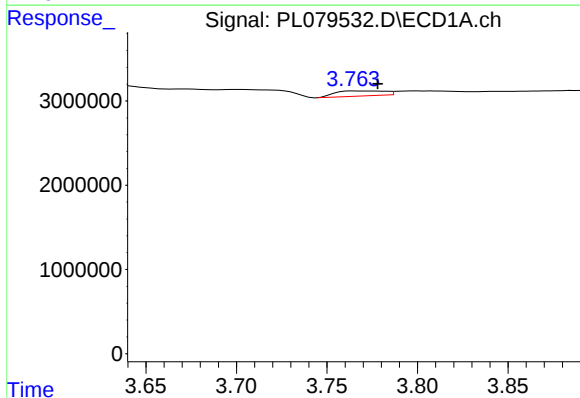


#2 alpha-BHC

R.T.: 3.765 min
Delta R.T.: -0.014 min
Response: 1147459
Conc: 0.33 ng/ml

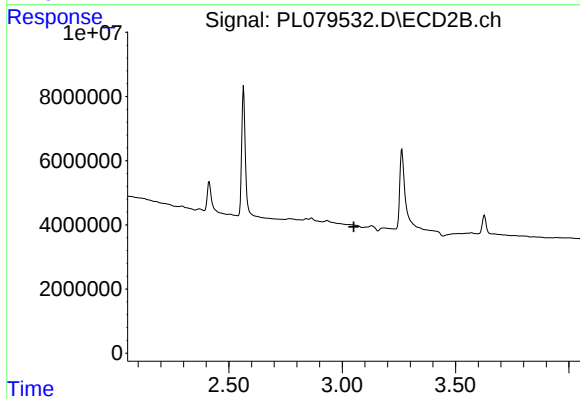

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 3.051 min
Response: 0
Conc: N.D.

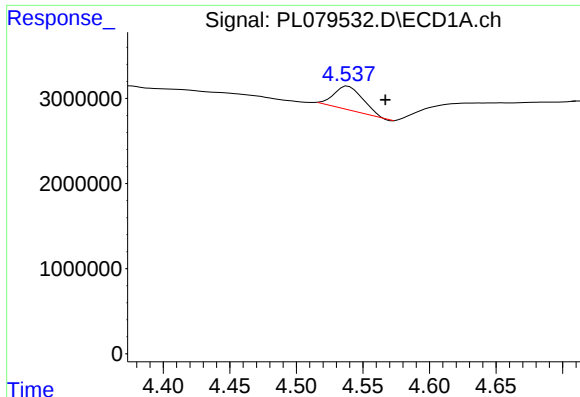

#7 delta-BHC


R.T.: 4.539 min
Delta R.T.: -0.028 min
Response: 4213660
Conc: 1.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

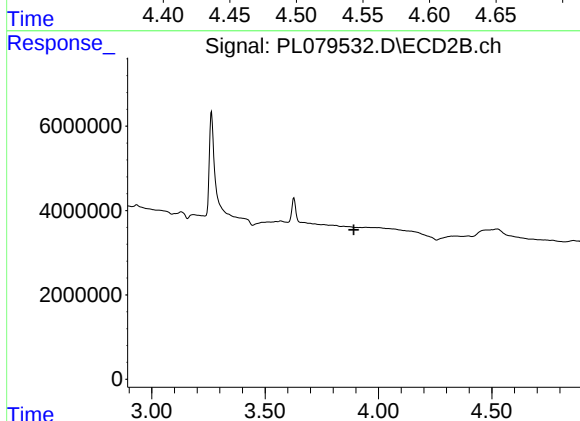


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 3.891 min
Response: 0
Conc: N.D.

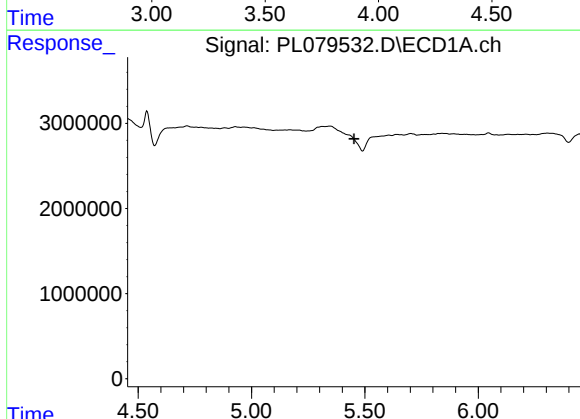


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.452 min
Response: 0
Conc: N.D.

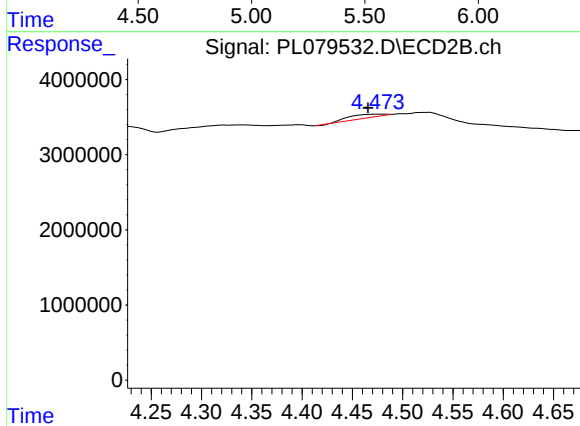

#8 Heptachlor epoxide


R.T.: 4.474 min
Delta R.T.: 0.008 min
Response: 1064010
Conc: 0.32 ng/ml

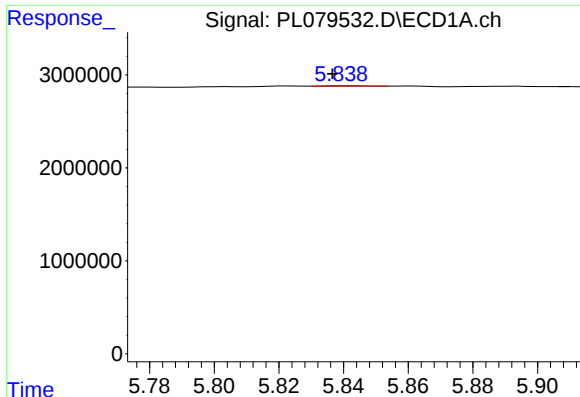

#9 Endosulfan I


R.T.: 5.840 min
Delta R.T.: 0.004 min
Response: 50472
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

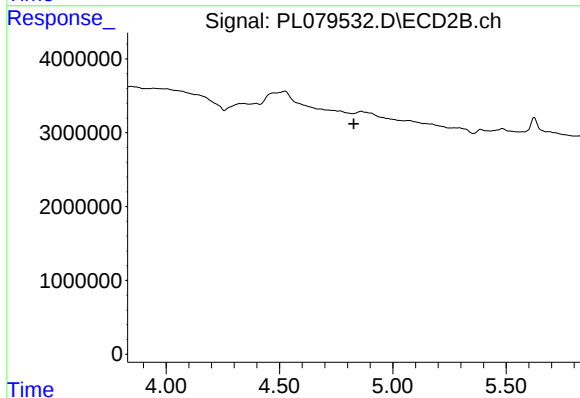


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 4.828 min
Response: 0
Conc: N.D.

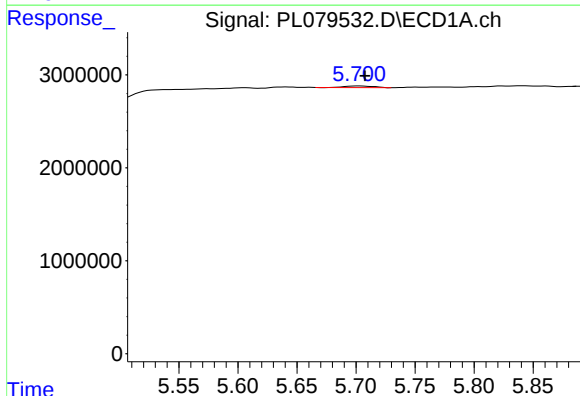


#10 gamma-Chlordane

R.T.: 5.702 min
Delta R.T.: -0.006 min
Response: 301659
Conc: 0.11 ng/ml

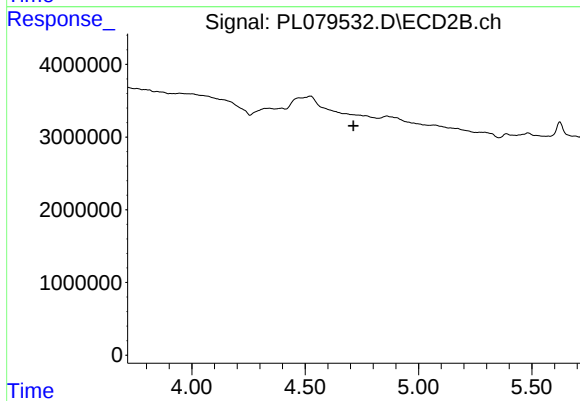

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 4.713 min
Response: 0
Conc: N.D.

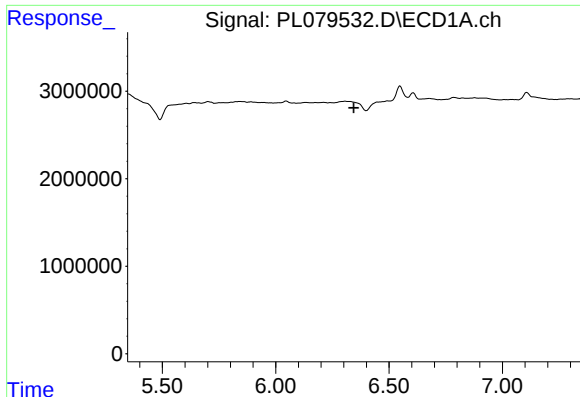

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.344 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

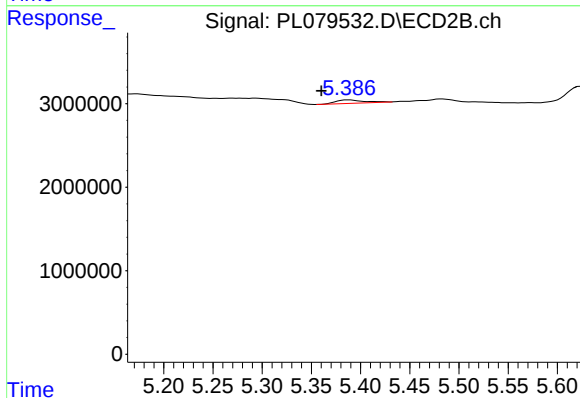


#14 Endrin

R.T.: 5.387 min
Delta R.T.: 0.027 min
Response: 794923
Conc: 0.26 ng/ml

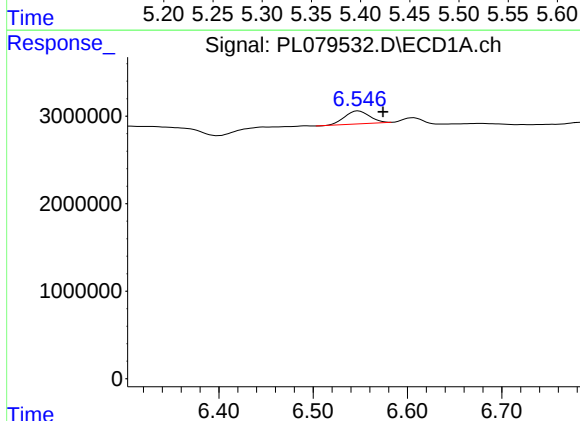


#15 Endosulfan II

R.T.: 6.548 min
Delta R.T.: -0.026 min
Response: 2737648
Conc: 1.21 ng/ml

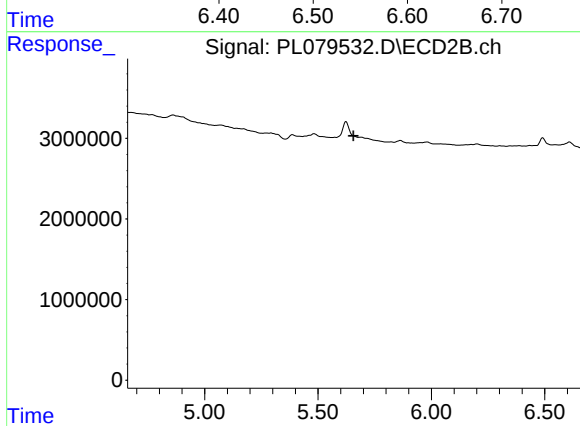

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.657 min
Response: 0
Conc: N.D.

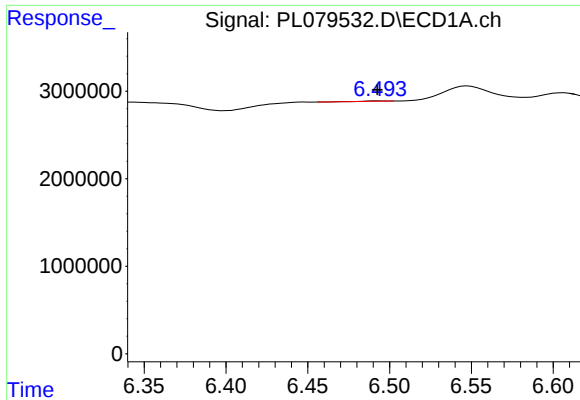

#16 4,4'-DDD


R.T.: 6.494 min
Delta R.T.: 0.002 min
Response: 41829
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

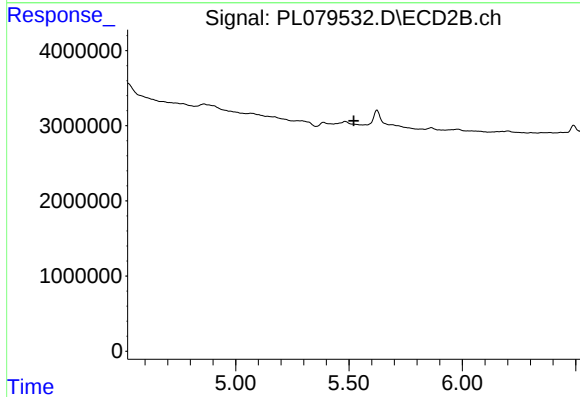


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.521 min
Response: 0
Conc: N.D.

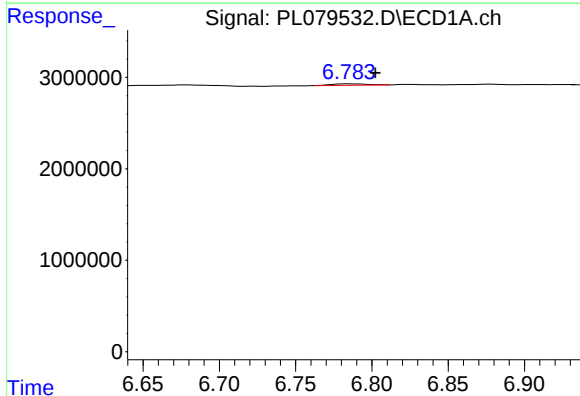


#17 4,4'-DDT

R.T.: 6.785 min
Delta R.T.: -0.017 min
Response: 254665
Conc: 0.11 ng/ml

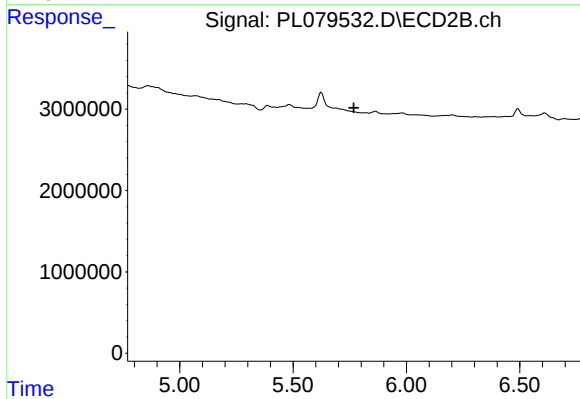

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 5.767 min
Response: 0
Conc: N.D.

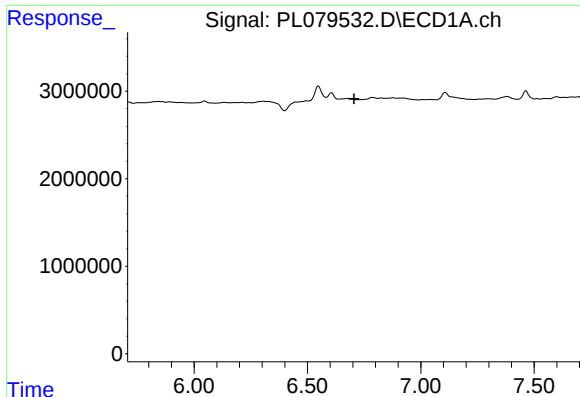

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

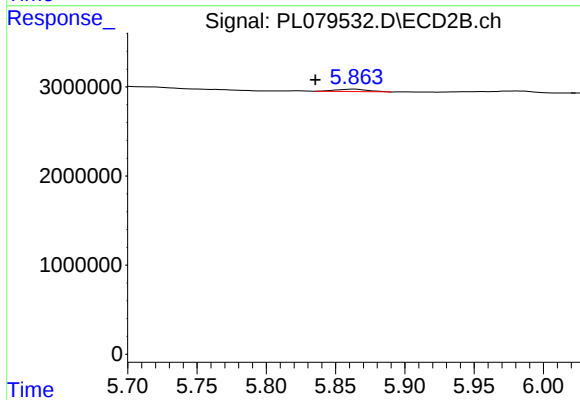


#18 Endrin aldehyde

R.T.: 5.864 min
Delta R.T.: 0.029 min
Response: 268935
Conc: 0.13 ng/ml

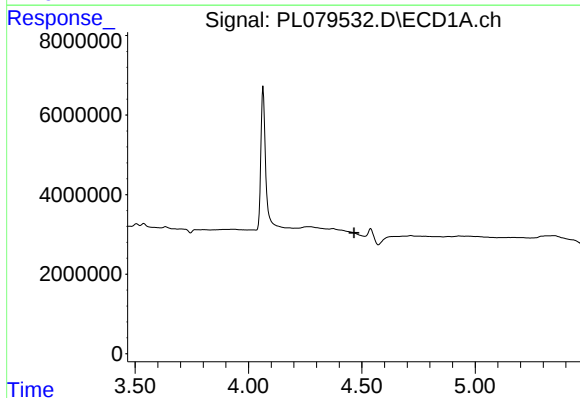


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.465 min
Response: 0
Conc: N.D.

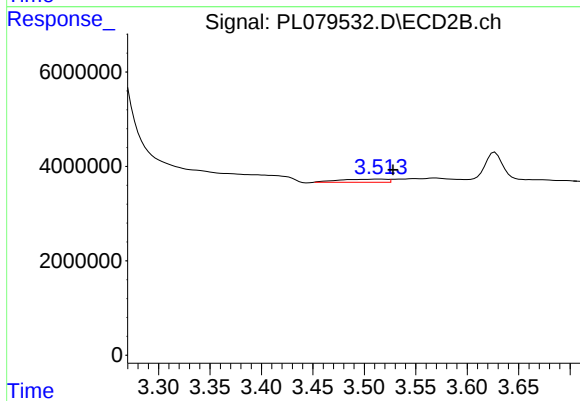

#23 Chlordane-1


R.T.: 3.515 min
Delta R.T.: -0.013 min
Response: 2115719
Conc: 19.89 ng/ml

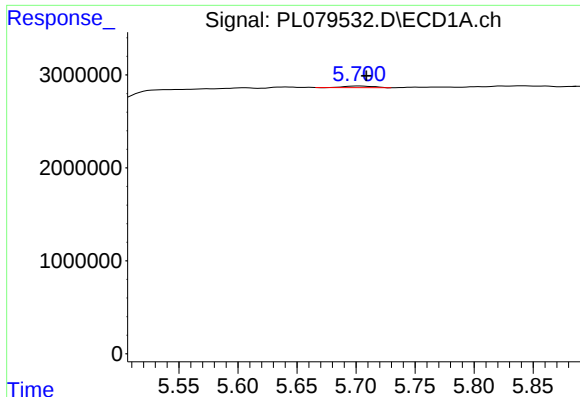

#25 Chlordane-3


R.T.: 5.702 min
Delta R.T.: -0.007 min
Response: 301659
Conc: 0.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

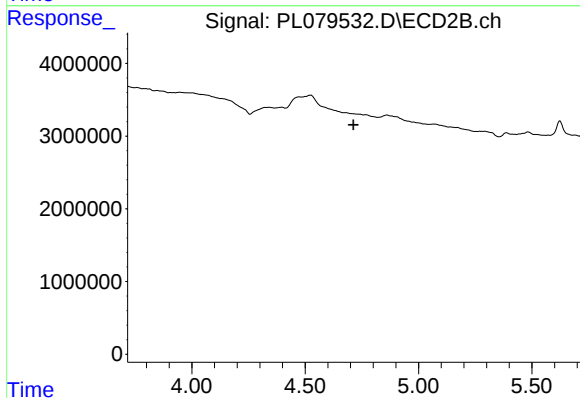


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 4.713 min
Response: 0
Conc: N.D.

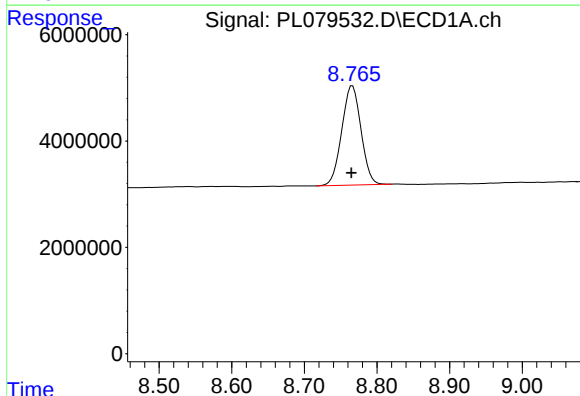

#28 Decachlorobiphenyl

R.T.: 8.766 min
Delta R.T.: 0.001 min
Response: 34421462
Conc: 17.72 ng/ml

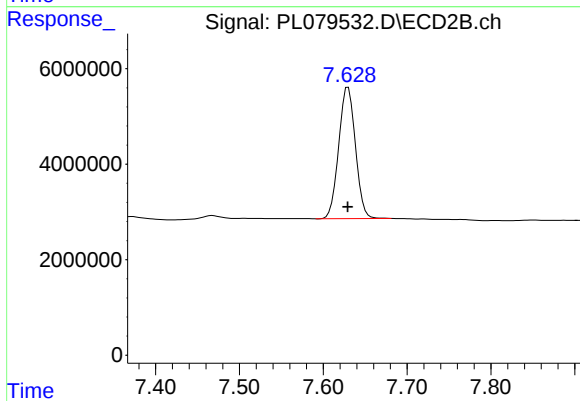

#28 Decachlorobiphenyl

R.T.: 7.630 min
Delta R.T.: 0.000 min
Response: 38158396
Conc: 16.24 ng/ml