

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120122\
 Data File : PL079525.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2022 12:40
 Operator : AR\AJ
 Sample : PB149365BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB149365BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/02/2022
 Supervised By : Ankita Jodhani 12/02/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 20:36:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 24 00:09:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.345f	2.562	40004377	46792367	17.709	17.190
2) SA Decachlor...	8.794f	7.632	35316217	41356368	18.185m	17.604

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120122\
Data File : PL079525.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2022 12:40
Operator : AR\AJ
Sample : PB149365BL
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB149365BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/02/2022
Supervised By : Ankita Jodhani 12/02/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 20:36:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
Quant Title : GC Extractables
QLast Update : Thu Nov 24 00:09:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

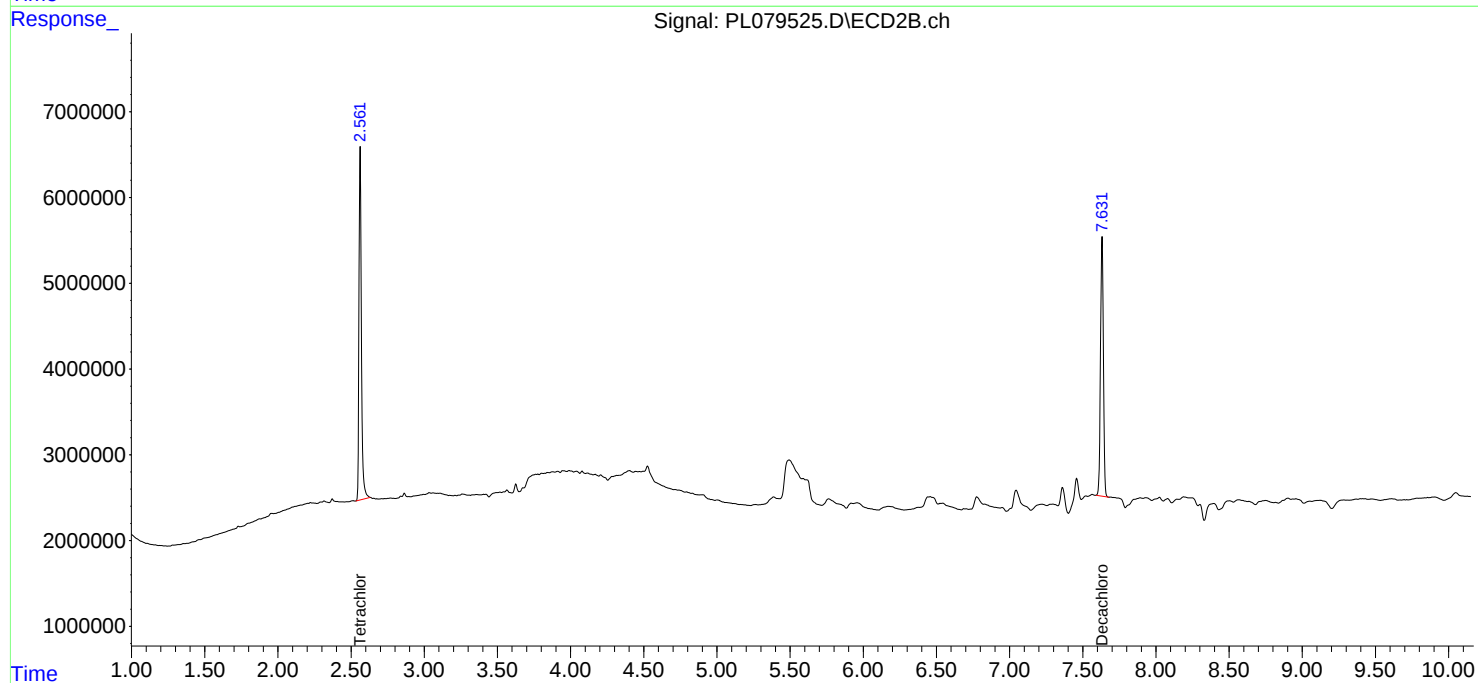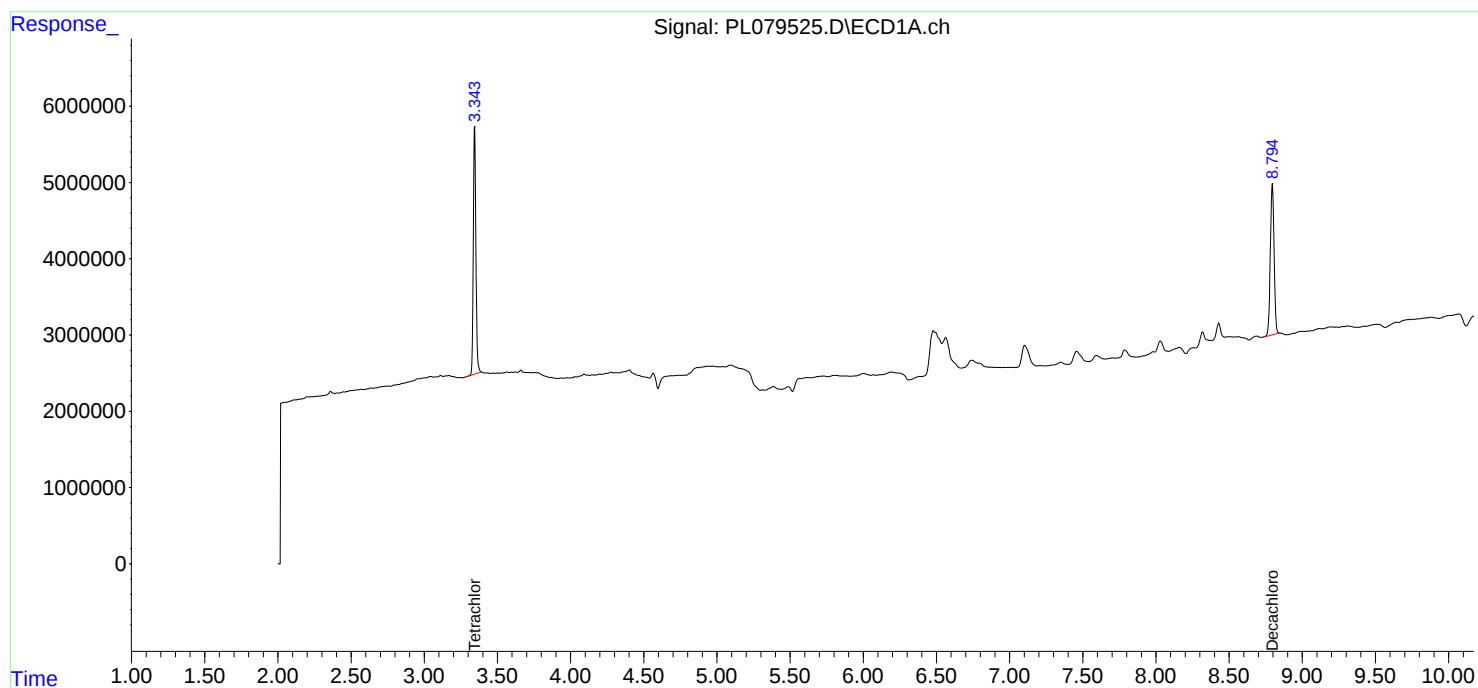

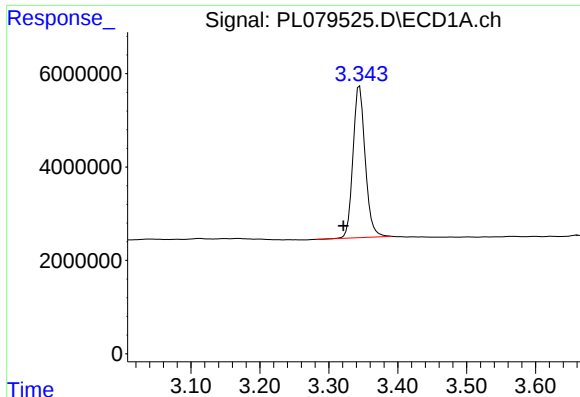


#1 Tetrachloro-m-xylene

R.T.: 3.345 min
Delta R.T.: 0.024 min
Response: 40004377
Conc: 17.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB149365BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/02/2022
Supervised By :Ankita Jodhani 12/02/2022

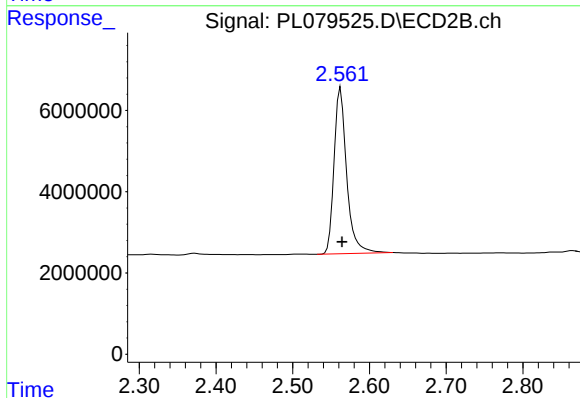


#1 Tetrachloro-m-xylene

R.T.: 2.562 min
Delta R.T.: -0.002 min
Response: 46792367
Conc: 17.19 ng/ml

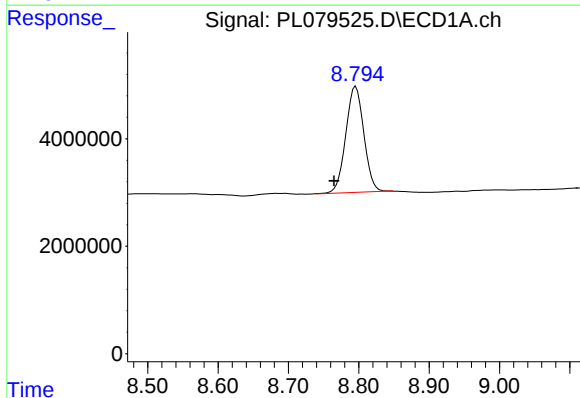

#28 Decachlorobiphenyl

R.T.: 8.794 min
Delta R.T.: 0.029 min
Response: 35316217
Conc: 18.18 ng/ml m

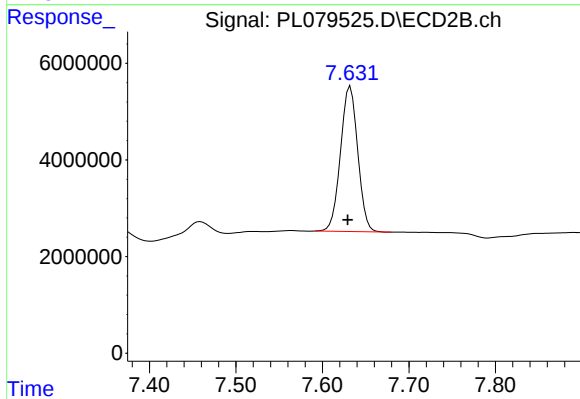

#28 Decachlorobiphenyl

R.T.: 7.632 min
Delta R.T.: 0.003 min
Response: 41356368
Conc: 17.60 ng/ml