

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120123\
 Data File : PL086909.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2023 14:17
 Operator : AR\AJ
 Sample : 05577-01 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EO-03-112923

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/01/2023
 Supervised By :Ankita Jodhani 12/01/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 22:00:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112923.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 29 06:35:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.341	2.610	4199991	1630748	1.314m	1.793 #
28)	SA Decachlor...	8.856	7.760	4550428	2585346	1.705m	2.345 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120123\
Data File : PL086909.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2023 14:17
Operator : AR\AJ
Sample : 05577-01 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
EO-03-112923


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/01/2023
Supervised By :Ankita Jodhani 12/01/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 22:00:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112923.M
Quant Title : GC Extractables
QLast Update : Wed Nov 29 06:35:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

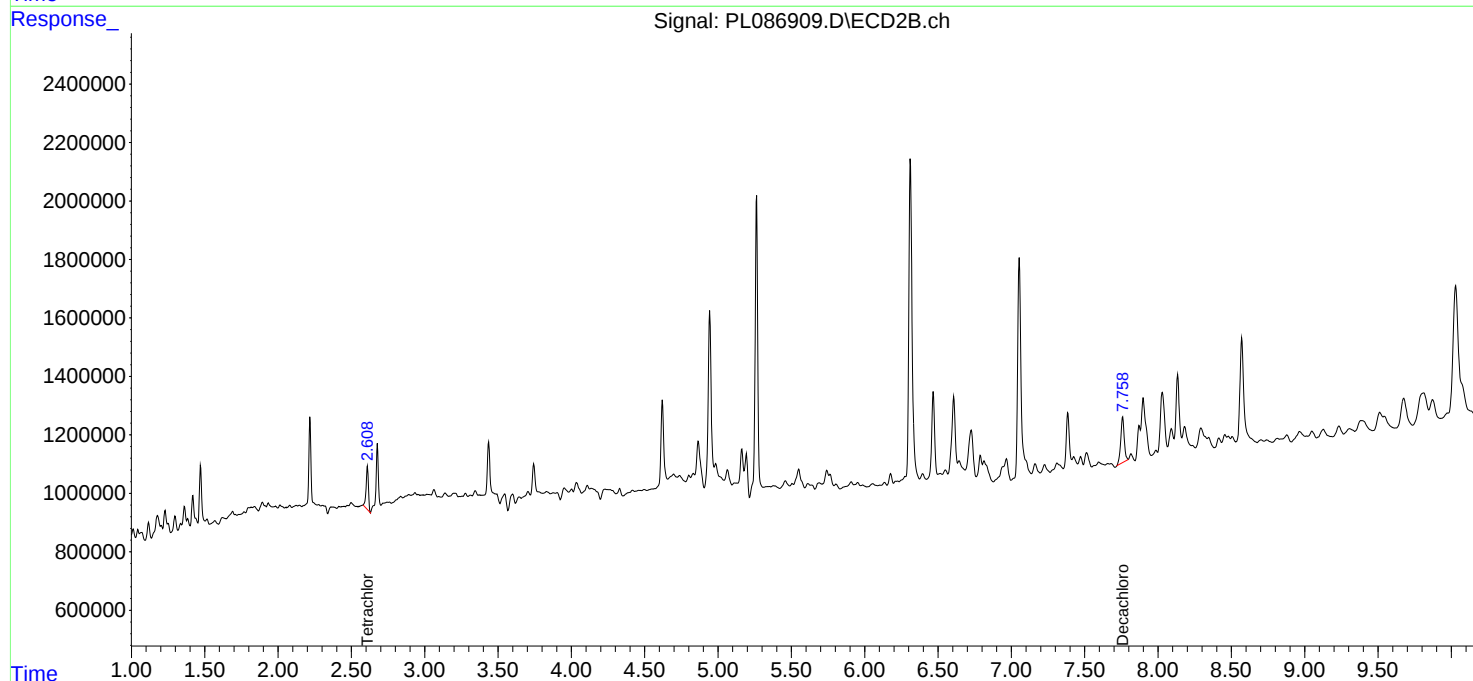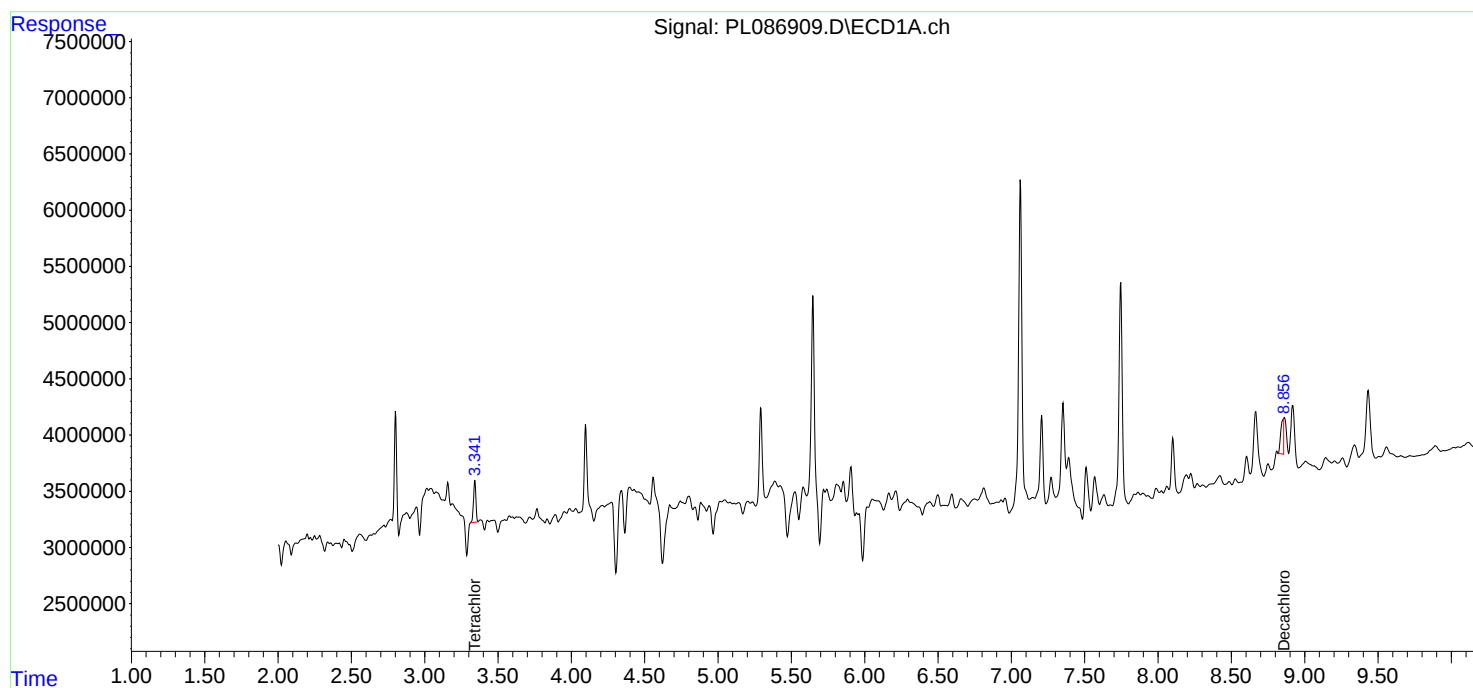

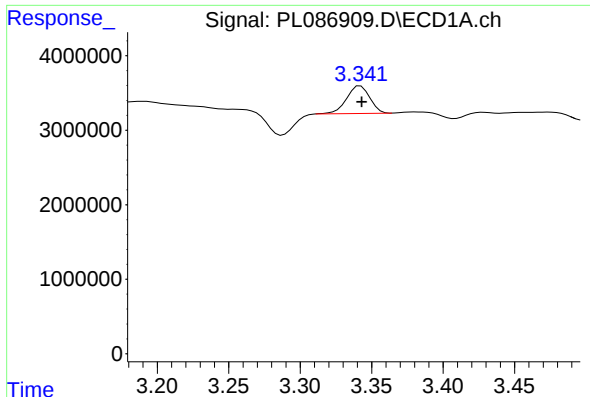


#1 Tetrachloro-m-xylene

R.T.: 3.341 min
Delta R.T.: -0.002 min
Response: 4199991
Conc: 1.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-03-112923


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/01/2023
Supervised By :Ankita Jodhani 12/01/2023

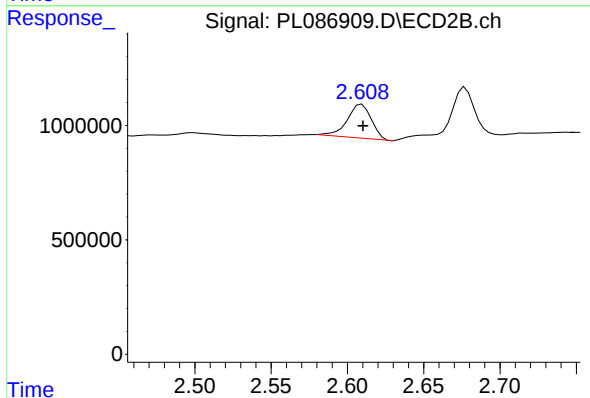


#1 Tetrachloro-m-xylene

R.T.: 2.610 min
Delta R.T.: 0.000 min
Response: 1630748
Conc: 1.79 ng/ml

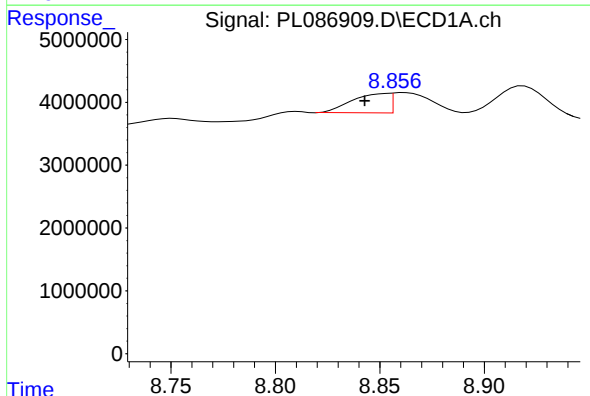

#28 Decachlorobiphenyl

R.T.: 8.856 min
Delta R.T.: 0.013 min
Response: 4550428
Conc: 1.70 ng/ml m

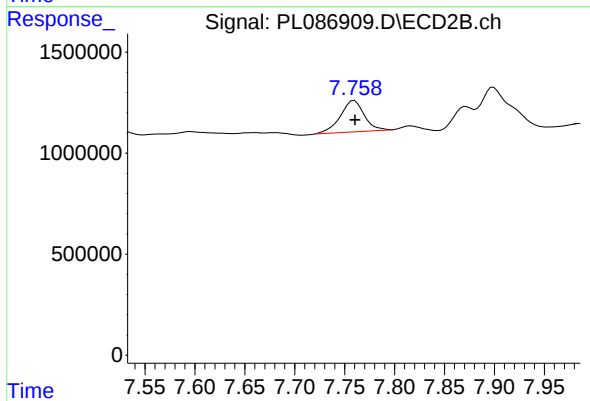

#28 Decachlorobiphenyl

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 2585346
Conc: 2.34 ng/ml