

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120223\
 Data File : PL086931.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2023 16:23
 Operator : AR\AJ
 Sample : 05592-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MW04S

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/04/2023
 Supervised By :Ankita Jodhani 12/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 21:34:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112923.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 29 06:35:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.341	2.609	46810907	16329735	14.642m	17.955
28)	SA Decachlor...	8.841	7.759	39406274	15079412	14.761	13.677

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120223\
Data File : PL086931.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2023 16:23
Operator : AR\AJ
Sample : 05592-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MW04S


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/04/2023
Supervised By :Ankita Jodhani 12/04/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 21:34:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112923.M
Quant Title : GC Extractables
QLast Update : Wed Nov 29 06:35:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

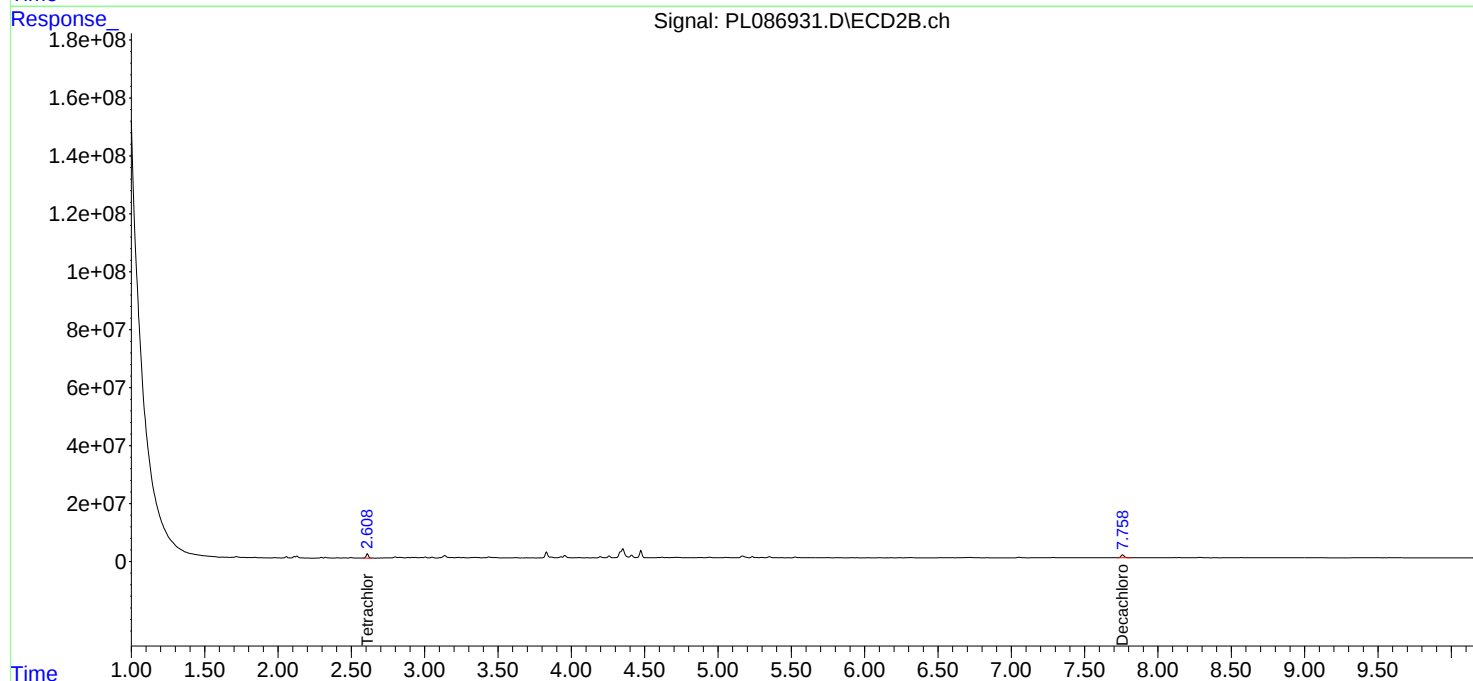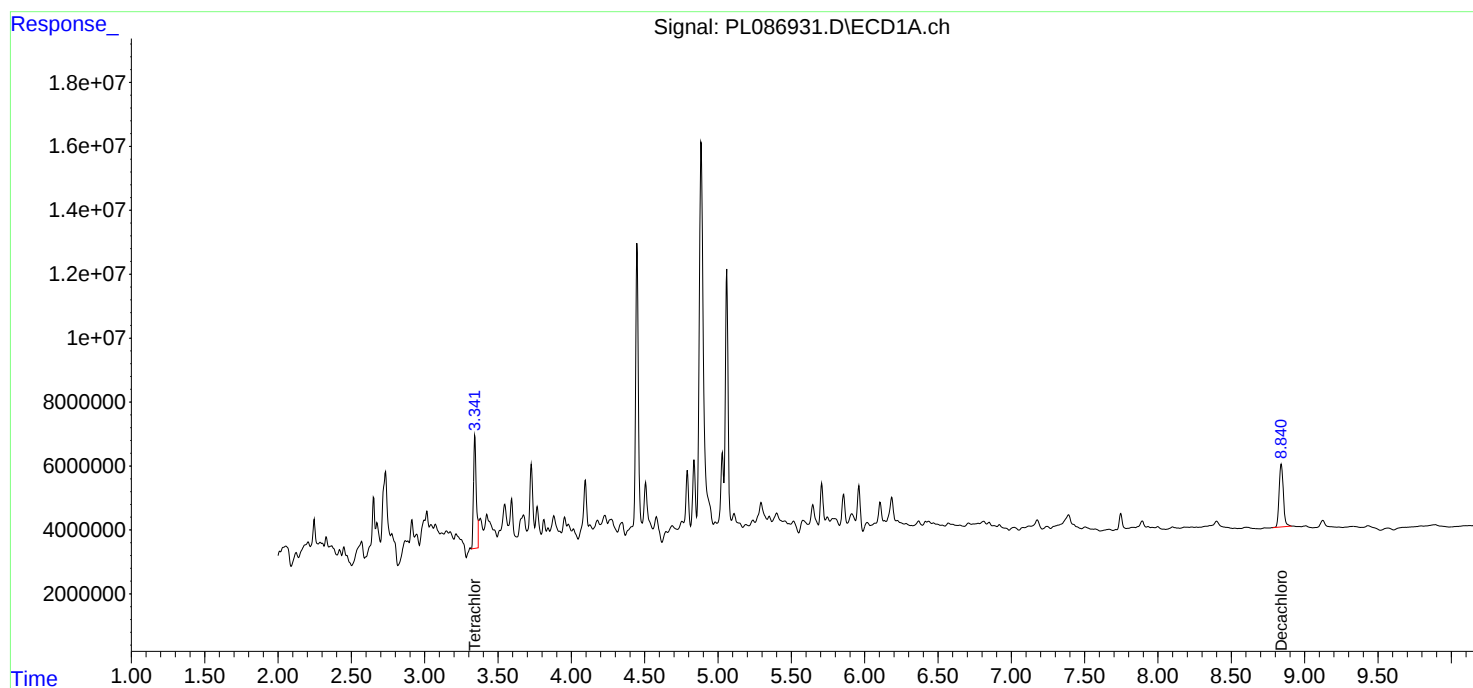

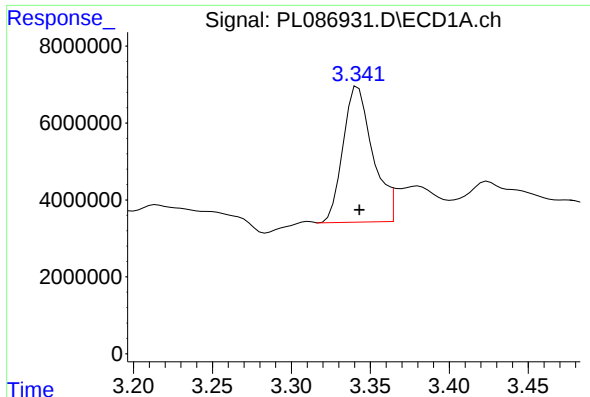


#1 Tetrachloro-m-xylene

R.T.: 3.341 min
Delta R.T.: -0.002 min
Response: 46810907
Conc: 14.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
MW04S


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/04/2023
Supervised By :Ankita Jodhani 12/04/2023

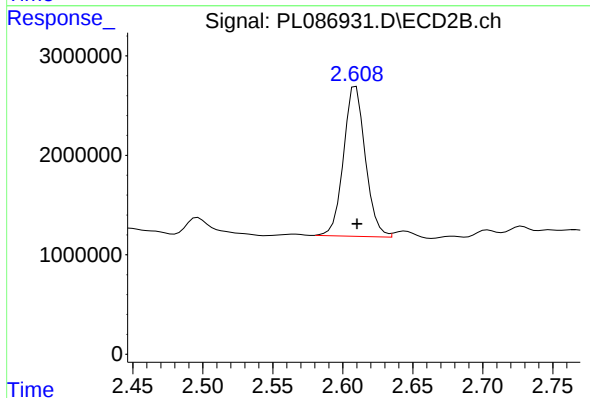


#1 Tetrachloro-m-xylene

R.T.: 2.609 min
Delta R.T.: 0.000 min
Response: 16329735
Conc: 17.95 ng/ml

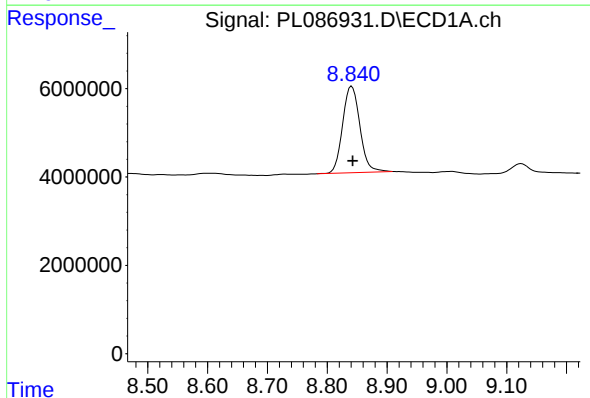

#28 Decachlorobiphenyl

R.T.: 8.841 min
Delta R.T.: -0.002 min
Response: 39406274
Conc: 14.76 ng/ml

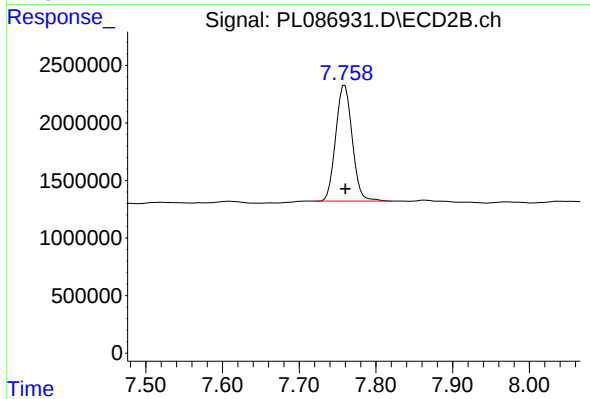

#28 Decachlorobiphenyl

R.T.: 7.759 min
Delta R.T.: -0.001 min
Response: 15079412
Conc: 13.68 ng/ml