

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120318\
 Data File : PL042678.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2018 10:06
 Operator : AJ\SJ
 Sample : J5770-16
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 23:56:32 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.102	148.9E6	76544153	25.304	26.614
28)	SA Decachlor...	8.206	9.235	142.2E6	60579143	22.562	25.117
Target Compounds							
3)	MA gamma-BHC...	4.198	4.832f	791407	2072361	0.096	0.524 #
5)	MB Aldrin	4.737	0.000	1513489	0	0.186	N.D. #
6)	B beta-BHC	4.401f	0.000	10306860	0	2.909	N.D. #
8)	B Heptachlo...	0.000	5.993	0	8683804	N.D.	2.422 #
13)	MA Dieldrin	5.739	0.000	1013724	0	0.138	N.D. #
14)	MA Endrin	6.021	6.784f	3740095	3302239	0.572	1.199 #
17)	MA 4,4'-DDT	6.394	0.000	1428837	0	0.257	N.D. #
18)	B Endrin al...	6.394f	0.000	1428837	0	0.275	N.D. #
23)	Chlordane-1	4.368	0.000	4515357	0	16.332	N.D. #
24)	Chlordane-2	4.865	0.000	1244040	0	4.427	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120318\
Data File : PL042678.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2018 10:06
Operator : AJ\SJ
Sample : J5770-16
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 23:56:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

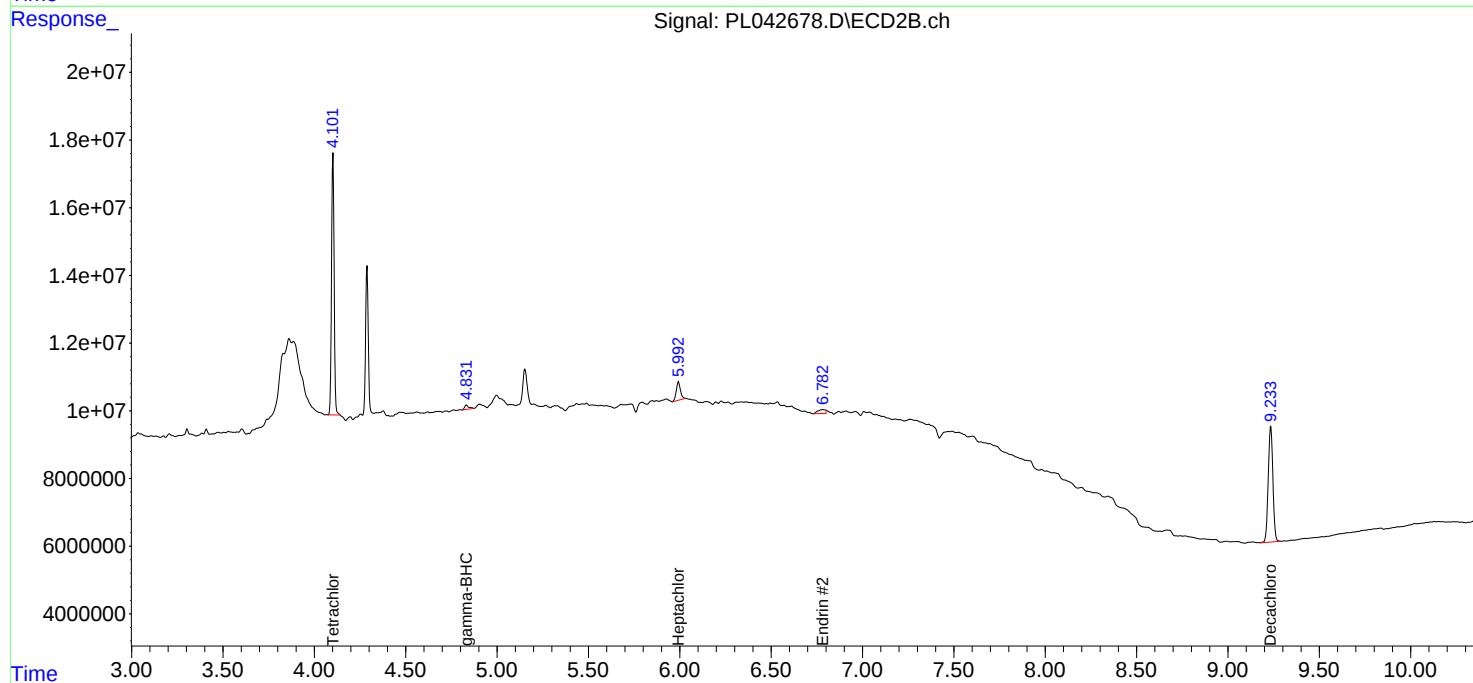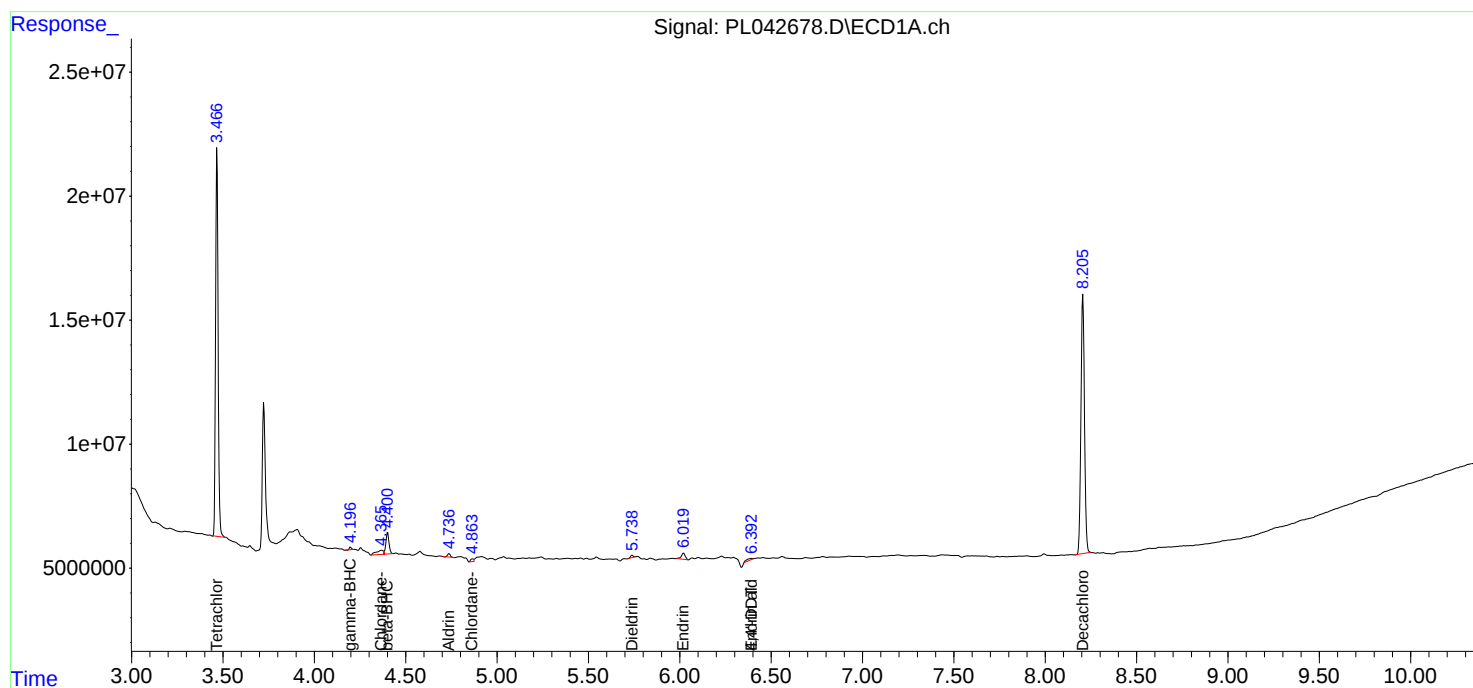


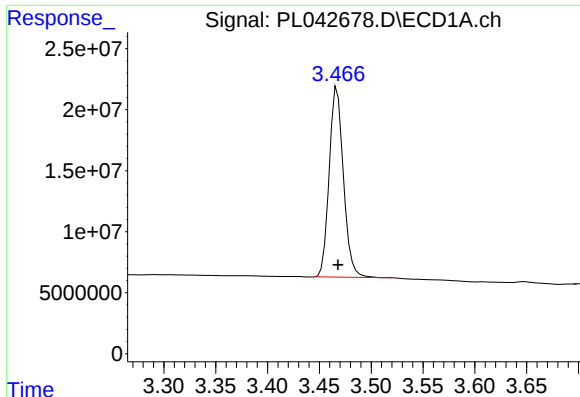

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 148877386
Conc: 25.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

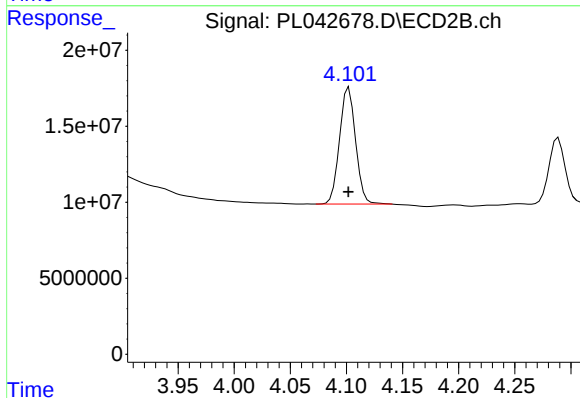


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 76544153
Conc: 26.61 ng/ml

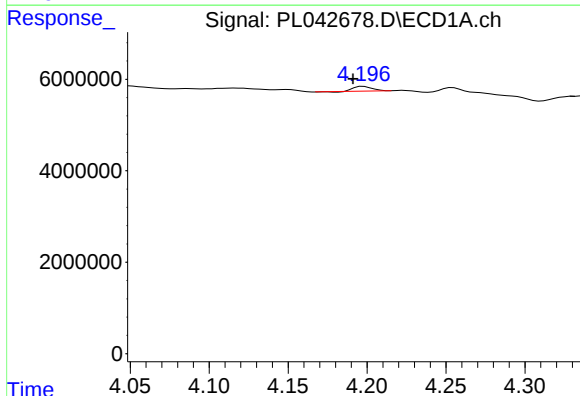


#3 gamma-BHC (Lindane)

R.T.: 4.198 min
Delta R.T.: 0.007 min
Response: 791407
Conc: 0.10 ng/ml

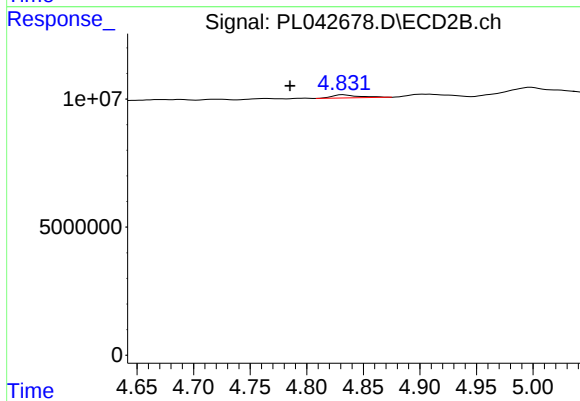

#3 gamma-BHC (Lindane)


R.T.: 4.832 min
Delta R.T.: 0.047 min
Response: 2072361
Conc: 0.52 ng/ml

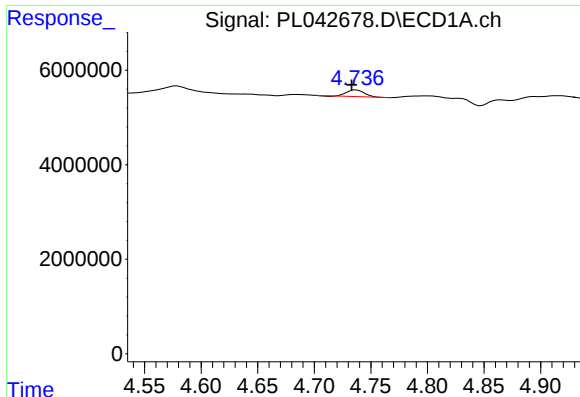

#5 Aldrin


R.T.: 4.737 min
Delta R.T.: 0.004 min
Response: 1513489
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

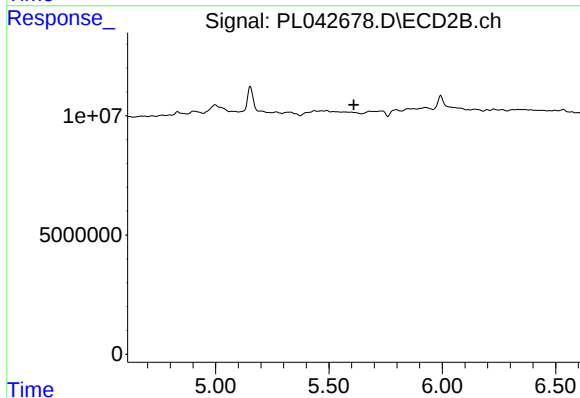


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.610 min
Response: 0
Conc: N.D.

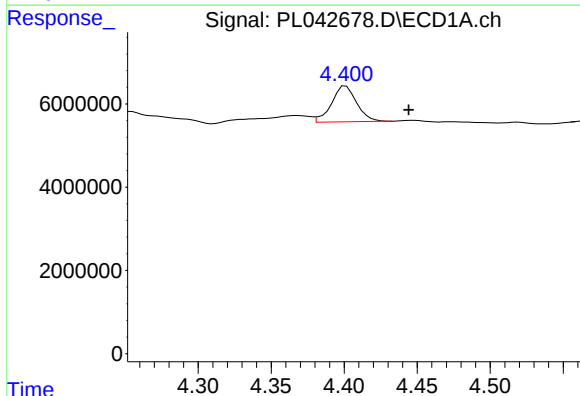


#6 beta-BHC

R.T.: 4.401 min
Delta R.T.: -0.043 min
Response: 10306860
Conc: 2.91 ng/ml

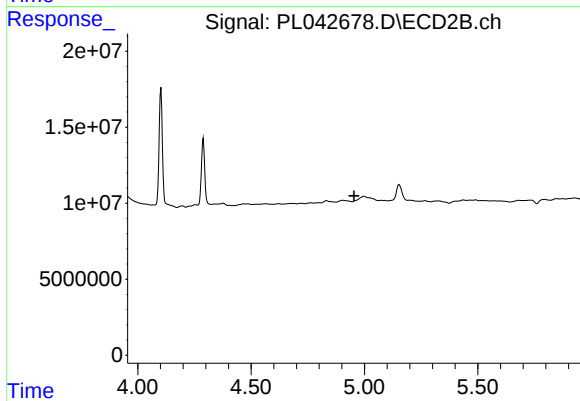

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

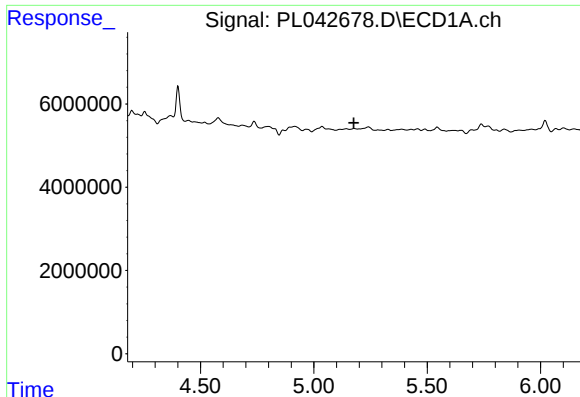

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

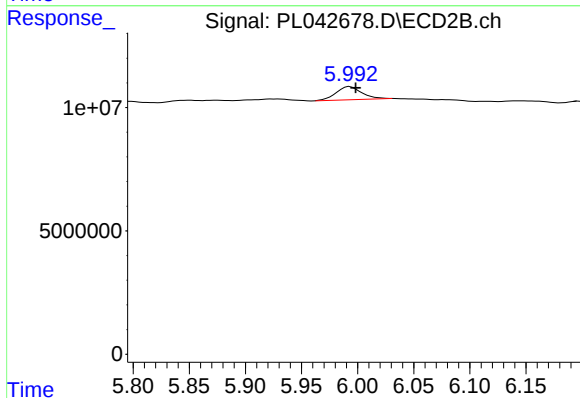


#8 Heptachlor epoxide

R.T.: 5.993 min
Delta R.T.: -0.005 min
Response: 8683804
Conc: 2.42 ng/ml

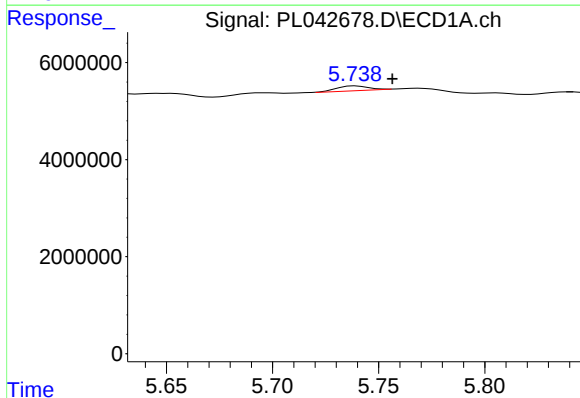


#13 Dieldrin

R.T.: 5.739 min
Delta R.T.: -0.017 min
Response: 1013724
Conc: 0.14 ng/ml

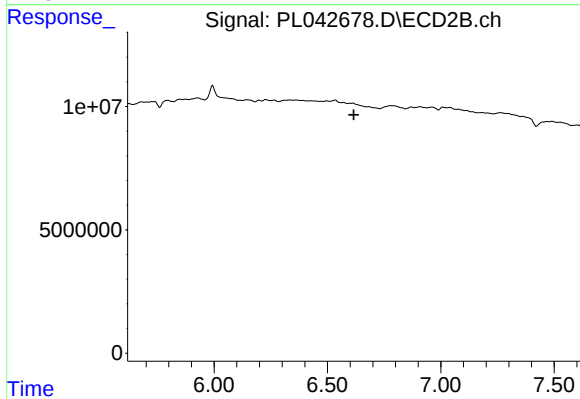

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.617 min
Response: 0
Conc: N.D.

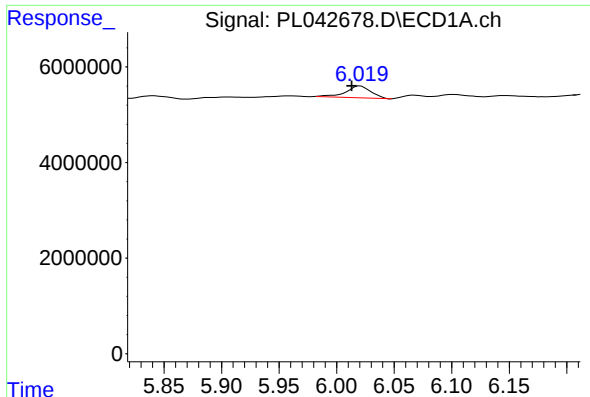

#14 Endrin


R.T.: 6.021 min
Delta R.T.: 0.008 min
Response: 3740095
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

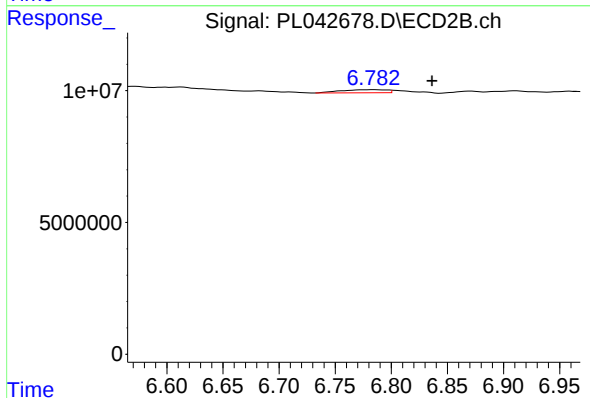


#14 Endrin

R.T.: 6.784 min
Delta R.T.: -0.053 min
Response: 3302239
Conc: 1.20 ng/ml

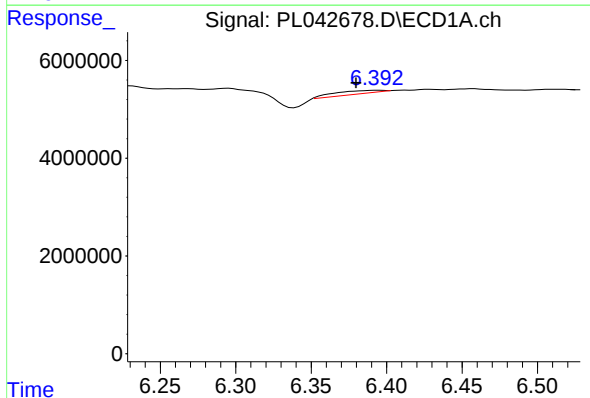


#17 4,4'-DDT

R.T.: 6.394 min
Delta R.T.: 0.014 min
Response: 1428837
Conc: 0.26 ng/ml

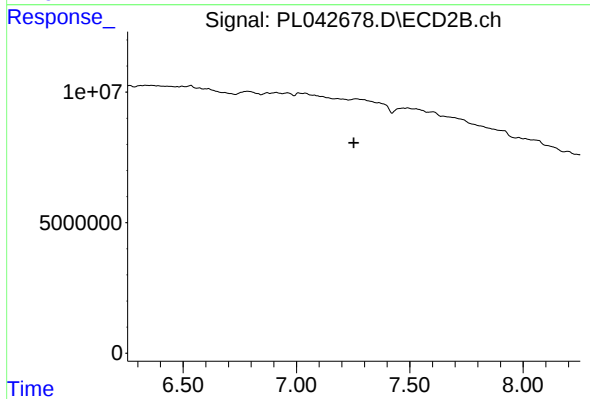

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.253 min
Response: 0
Conc: N.D.

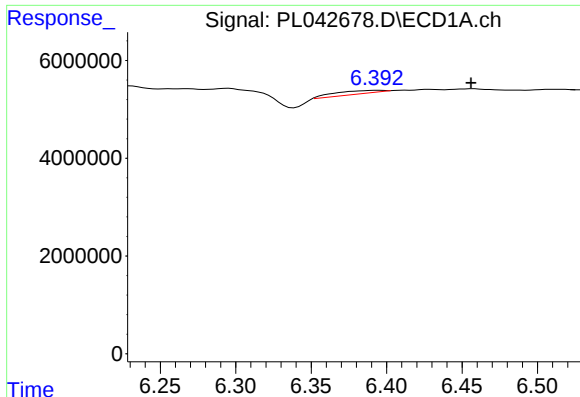

#18 Endrin aldehyde


R.T.: 6.394 min
Delta R.T.: -0.062 min
Response: 1428837
Conc: 0.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

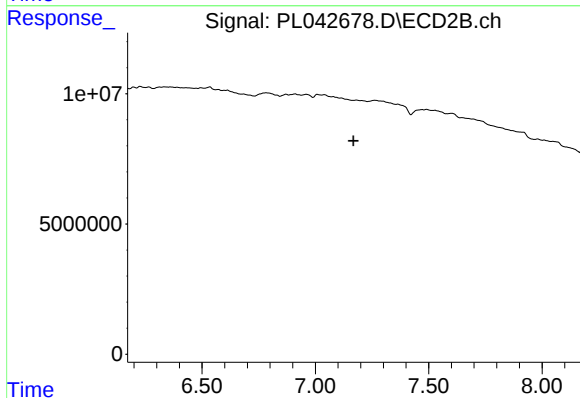


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.169 min
Response: 0
Conc: N.D.

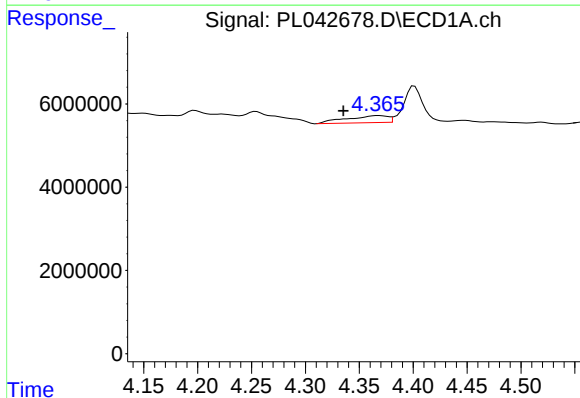


#23 Chlordane-1

R.T.: 4.368 min
Delta R.T.: 0.033 min
Response: 4515357
Conc: 16.33 ng/ml

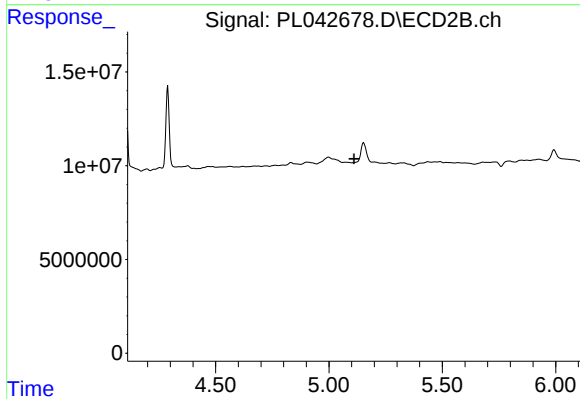

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

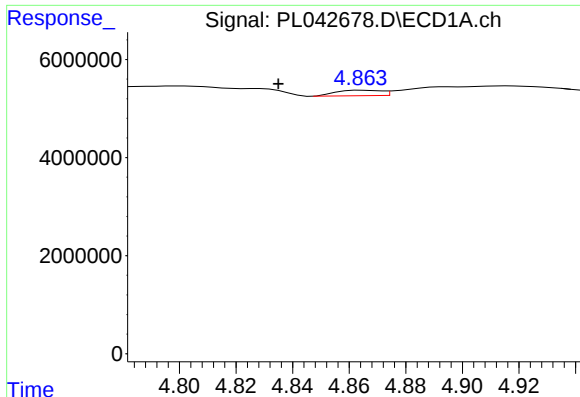

#24 Chlordane-2


R.T.: 4.865 min
Delta R.T.: 0.030 min
Response: 1244040
Conc: 4.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

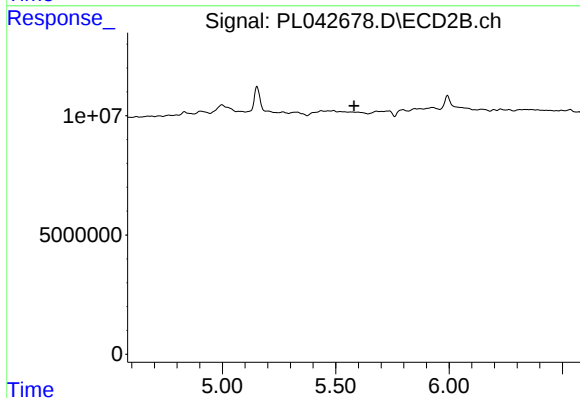


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.582 min
Response: 0
Conc: N.D.

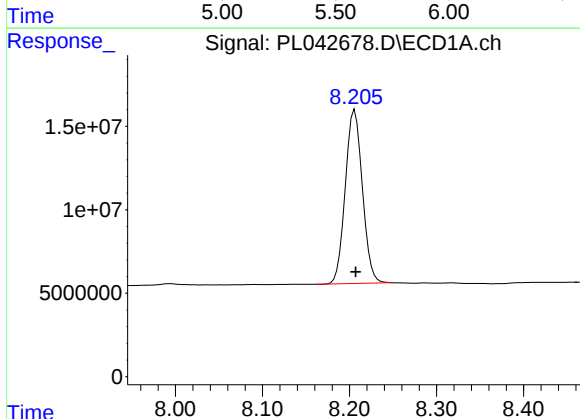

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 142187874
Conc: 22.56 ng/ml

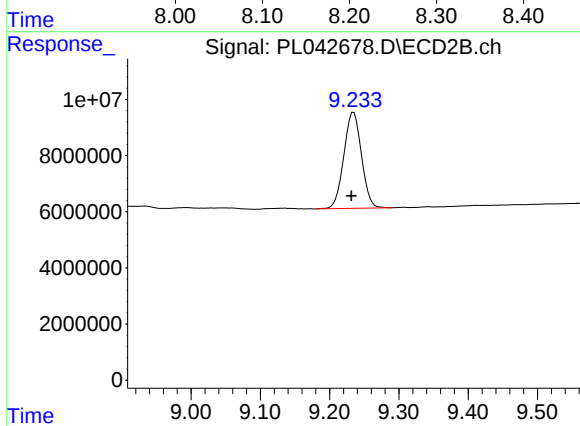

#28 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: 0.003 min
Response: 60579143
Conc: 25.12 ng/ml