

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120318\
 Data File : PL042681.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2018 10:48
 Operator : AJ\SJ
 Sample : J5771-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 23:56:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.102	152.0E6	77721603	25.843	27.023
28)	SA Decachlor...	8.206	9.233	159.4E6	68431309	25.300	28.373
Target Compounds							
6)	B beta-BHC	4.401f	4.905f	5686103	1742678	1.605	1.105 #
7)	B delta-BHC	0.000	5.158	0	1231708	N.D.	0.335 #
8)	B Heptachlo...	0.000	5.994	0	7835067	N.D.	2.185 #
13)	MA Dieldrin	5.739	0.000	926885	0	0.126	N.D. #
14)	MA Endrin	6.022	0.000	5431047	0	0.830	N.D. #
17)	MA 4,4'-DDT	6.395	0.000	1390305	0	0.250	N.D. #
18)	B Endrin al...	6.395f	0.000	1390305	0	0.267	N.D. #
19)	B Endosulfa...	6.676	0.000	1729596	0	0.277	N.D. #
23)	Chlordane-1	4.366	5.158	3787310	1231708	13.699	9.266 #
24)	Chlordane-2	4.864	0.000	1339606	0	4.767	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120318\
Data File : PL042681.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2018 10:48
Operator : AJ\SJ
Sample : J5771-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 23:56:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

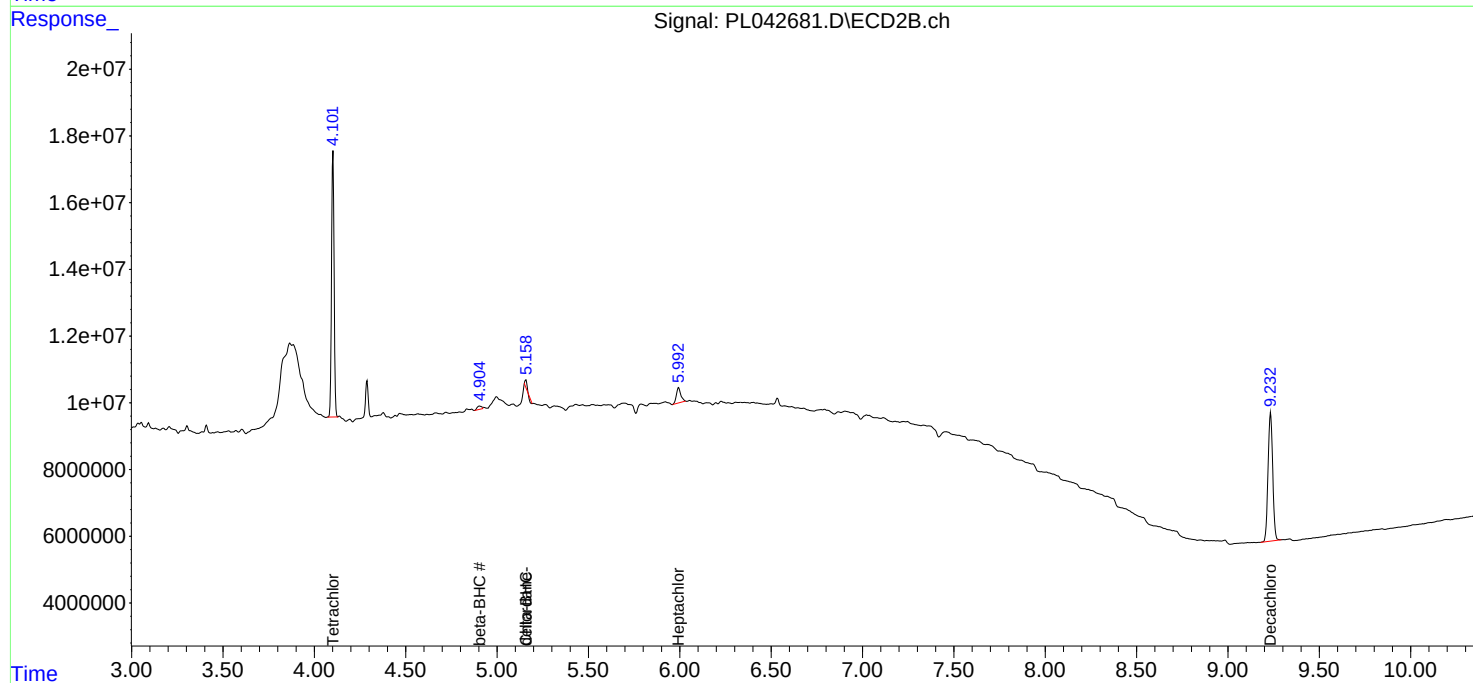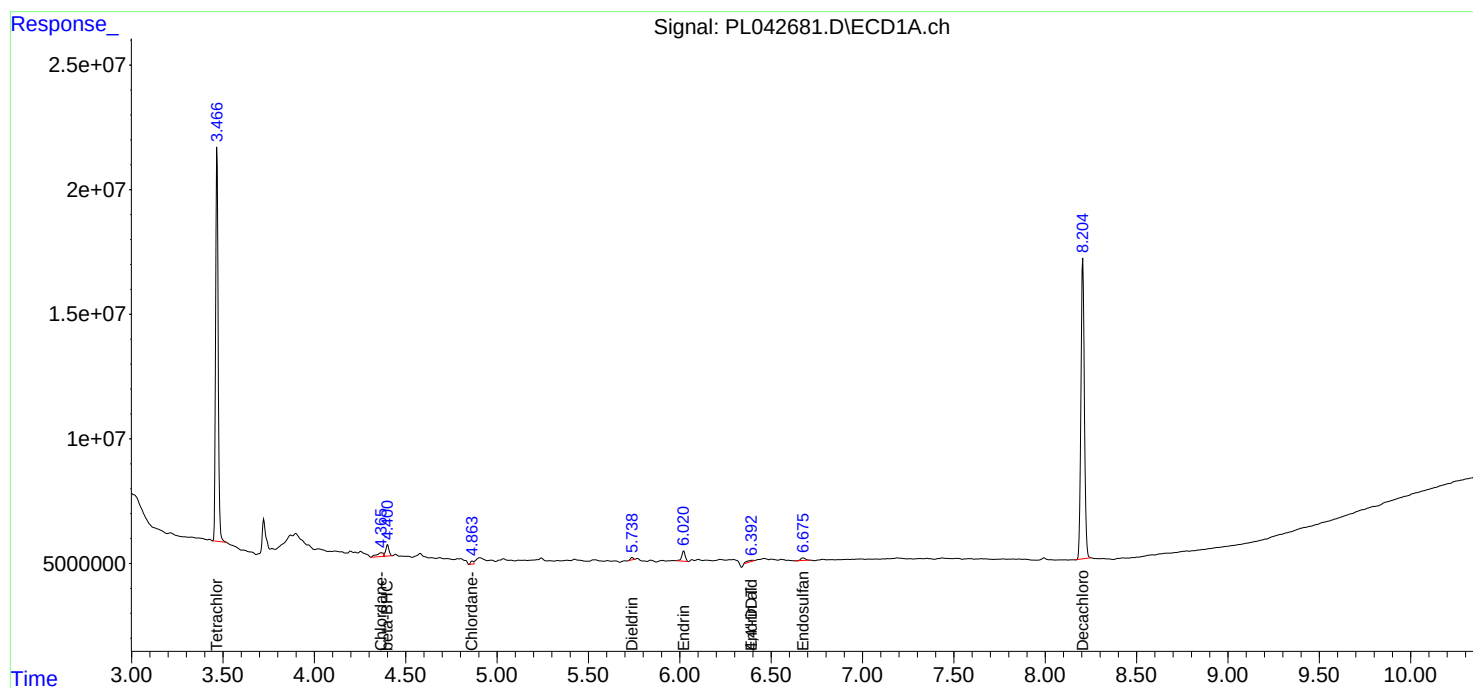


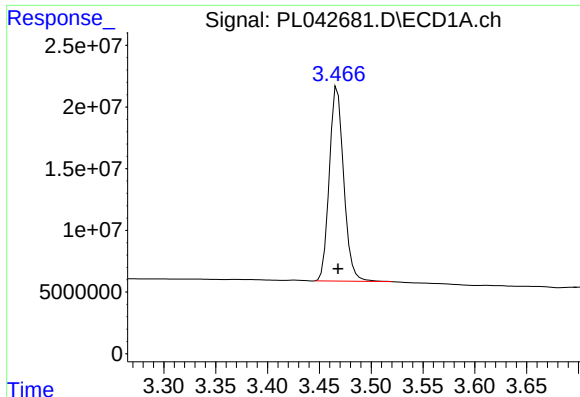

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 152048824
Conc: 25.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

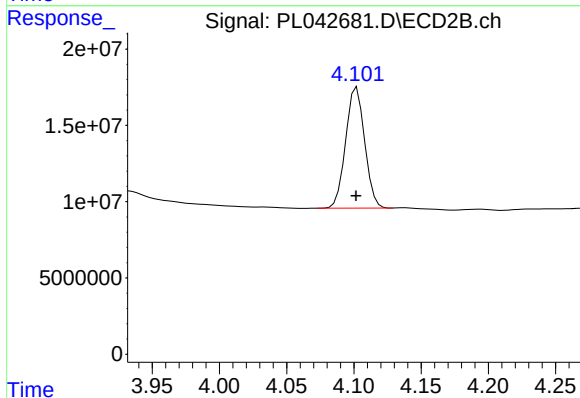


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 77721603
Conc: 27.02 ng/ml

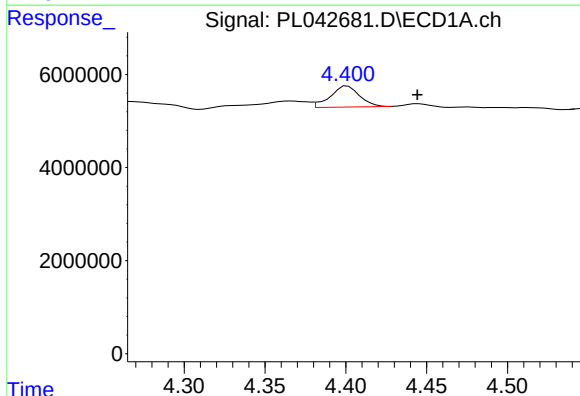


#6 beta-BHC

R.T.: 4.401 min
Delta R.T.: -0.043 min
Response: 5686103
Conc: 1.60 ng/ml

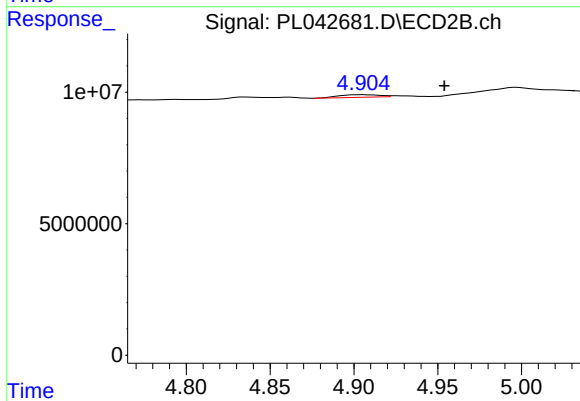

#6 beta-BHC


R.T.: 4.905 min
Delta R.T.: -0.049 min
Response: 1742678
Conc: 1.10 ng/ml

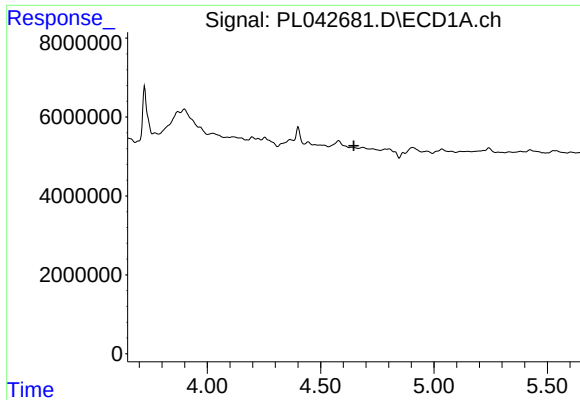

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.646 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

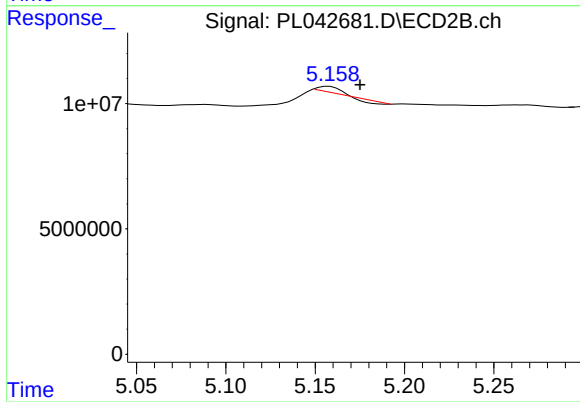


#7 delta-BHC

R.T.: 5.158 min
Delta R.T.: -0.017 min
Response: 1231708
Conc: 0.33 ng/ml

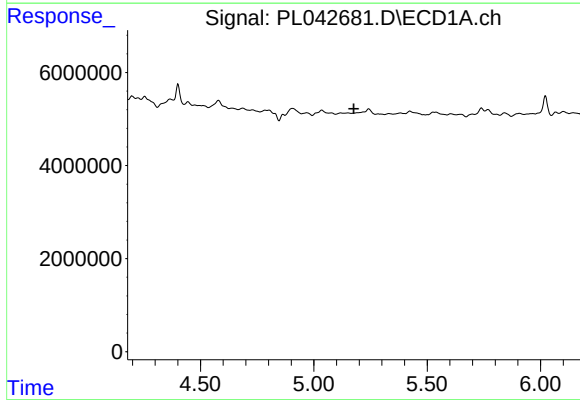


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.177 min
Response: 0
Conc: N.D.

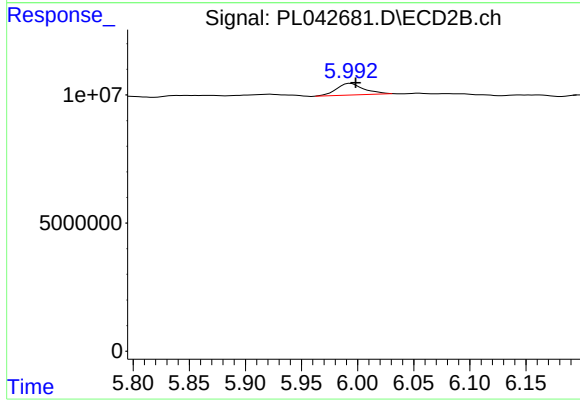

#8 Heptachlor epoxide


R.T.: 5.994 min
Delta R.T.: -0.005 min
Response: 7835067
Conc: 2.19 ng/ml

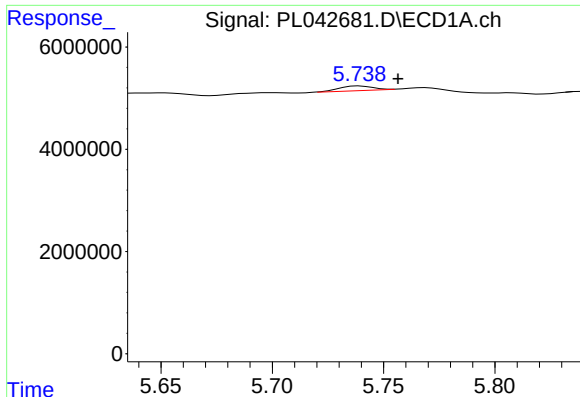

#13 Dieldrin


R.T.: 5.739 min
Delta R.T.: -0.017 min
Response: 926885
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

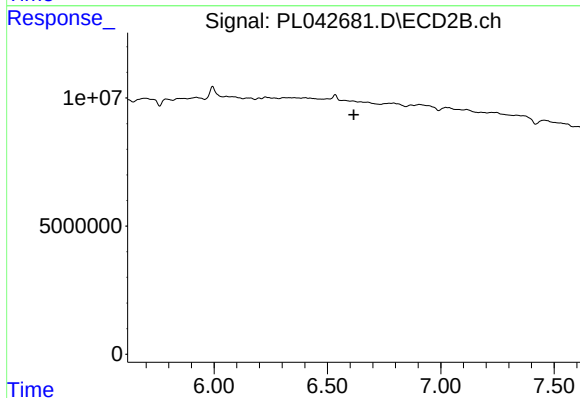


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.617 min
Response: 0
Conc: N.D.

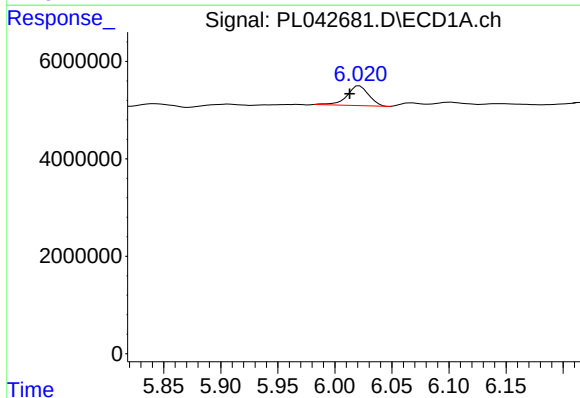


#14 Endrin

R.T.: 6.022 min
Delta R.T.: 0.009 min
Response: 5431047
Conc: 0.83 ng/ml

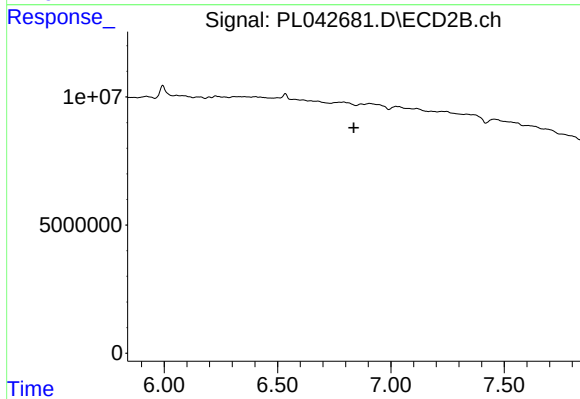

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.836 min
Response: 0
Conc: N.D.

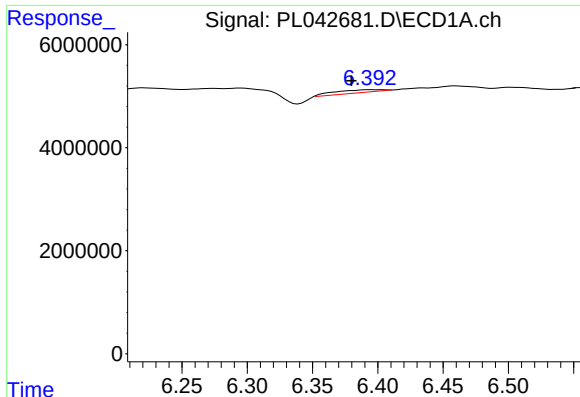

#17 4,4'-DDT


R.T.: 6.395 min
Delta R.T.: 0.015 min
Response: 1390305
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

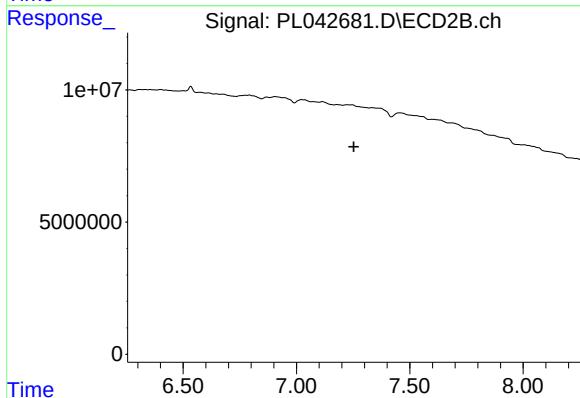


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.253 min
Response: 0
Conc: N.D.

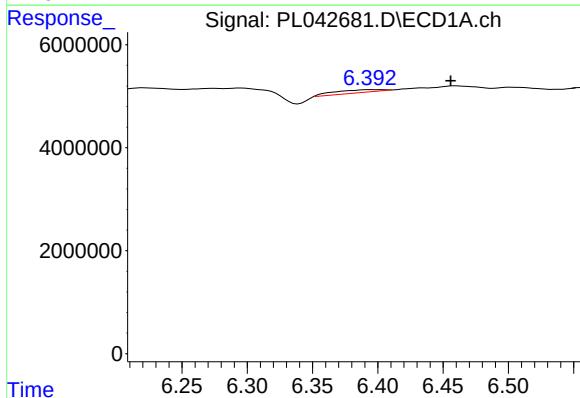


#18 Endrin aldehyde

R.T.: 6.395 min
Delta R.T.: -0.061 min
Response: 1390305
Conc: 0.27 ng/ml

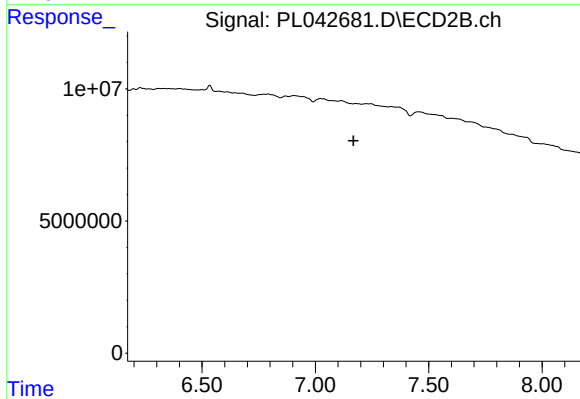

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.169 min
Response: 0
Conc: N.D.

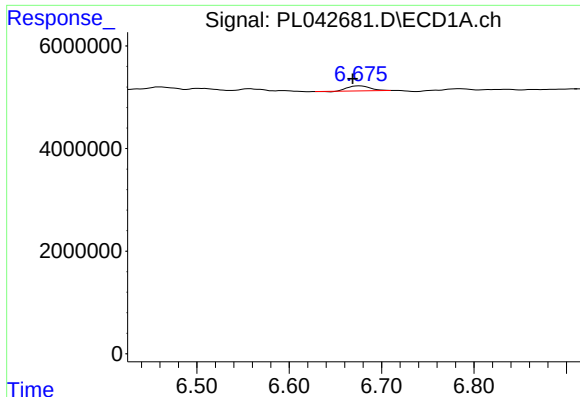

#19 Endosulfan Sulfate


R.T.: 6.676 min
Delta R.T.: 0.007 min
Response: 1729596
Conc: 0.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

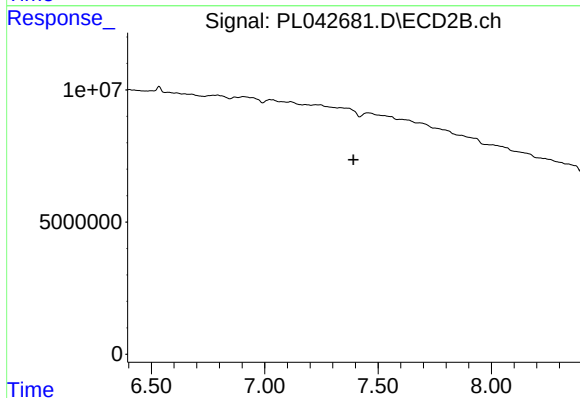


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

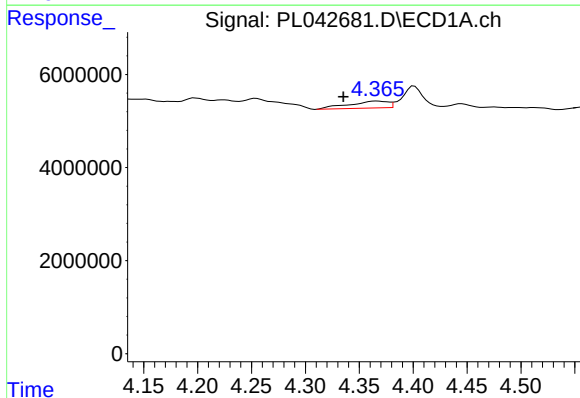


#23 Chlordane-1

R.T.: 4.366 min
Delta R.T.: 0.031 min
Response: 3787310
Conc: 13.70 ng/ml

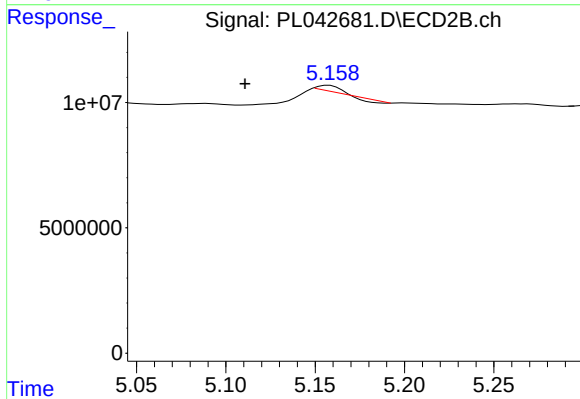

#23 Chlordane-1


R.T.: 5.158 min
Delta R.T.: 0.047 min
Response: 1231708
Conc: 9.27 ng/ml

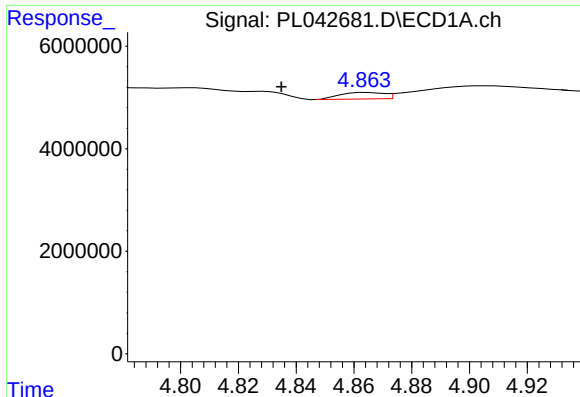

#24 Chlordane-2


R.T.: 4.864 min
Delta R.T.: 0.029 min
Response: 1339606
Conc: 4.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

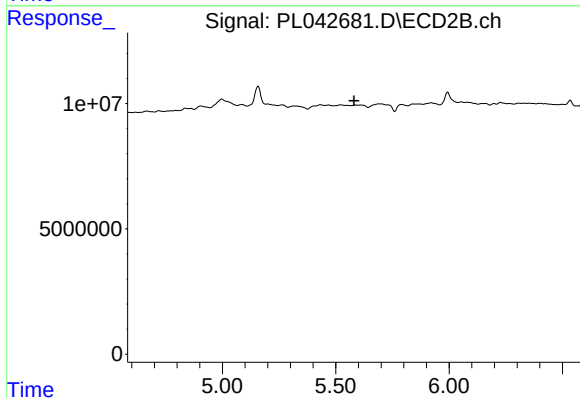


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.582 min
Response: 0
Conc: N.D.

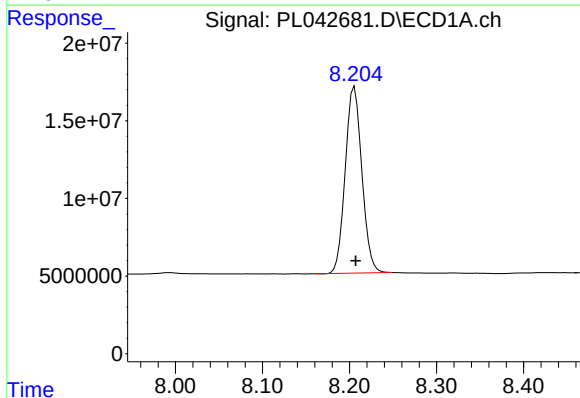

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.001 min
Response: 159444380
Conc: 25.30 ng/ml

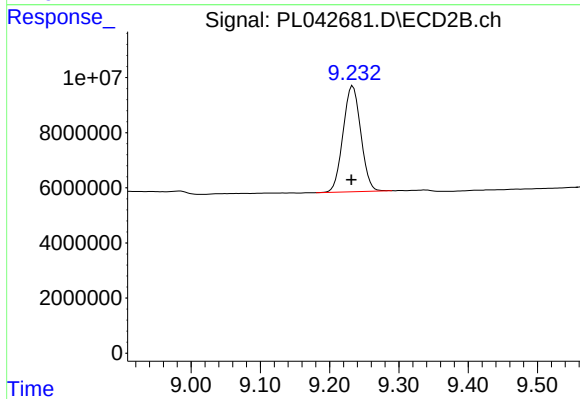

#28 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: 0.002 min
Response: 68431309
Conc: 28.37 ng/ml