

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120318\
 Data File : PL042689.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2018 13:09
 Operator : AJ\SJ
 Sample : PB115214BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 23:57:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.102	141.0E6	73934538	23.969	25.706
28)	SA Decachlor...	8.206	9.234	146.3E6	65201894	23.207	27.034
Target Compounds							
6)	B beta-BHC	4.401f	0.000	10160321	0	2.868	N.D. #
8)	B Heptachlo...	0.000	5.994	0	6223369	N.D.	1.736 #
9)	A Endosulfan I	0.000	6.353	0	1890197	N.D.	0.599 #
11)	B alpha-Chl...	0.000	6.306	0	4011555	N.D.	1.200 #
14)	MA Endrin	6.022	6.861	2611235	3183347	0.399	1.156 #
16)	A 4,4'-DDD	6.091f	0.000	1299115	0	0.245	N.D. #
23)	Chlordane-1	4.401	0.000	10160321	0	36.750	N.D. #
26)	Chlordane-4	0.000	6.306	0	4011555	N.D.	7.332 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120318\
Data File : PL042689.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2018 13:09
Operator : AJ\SJ
Sample : PB115214BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 23:57:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

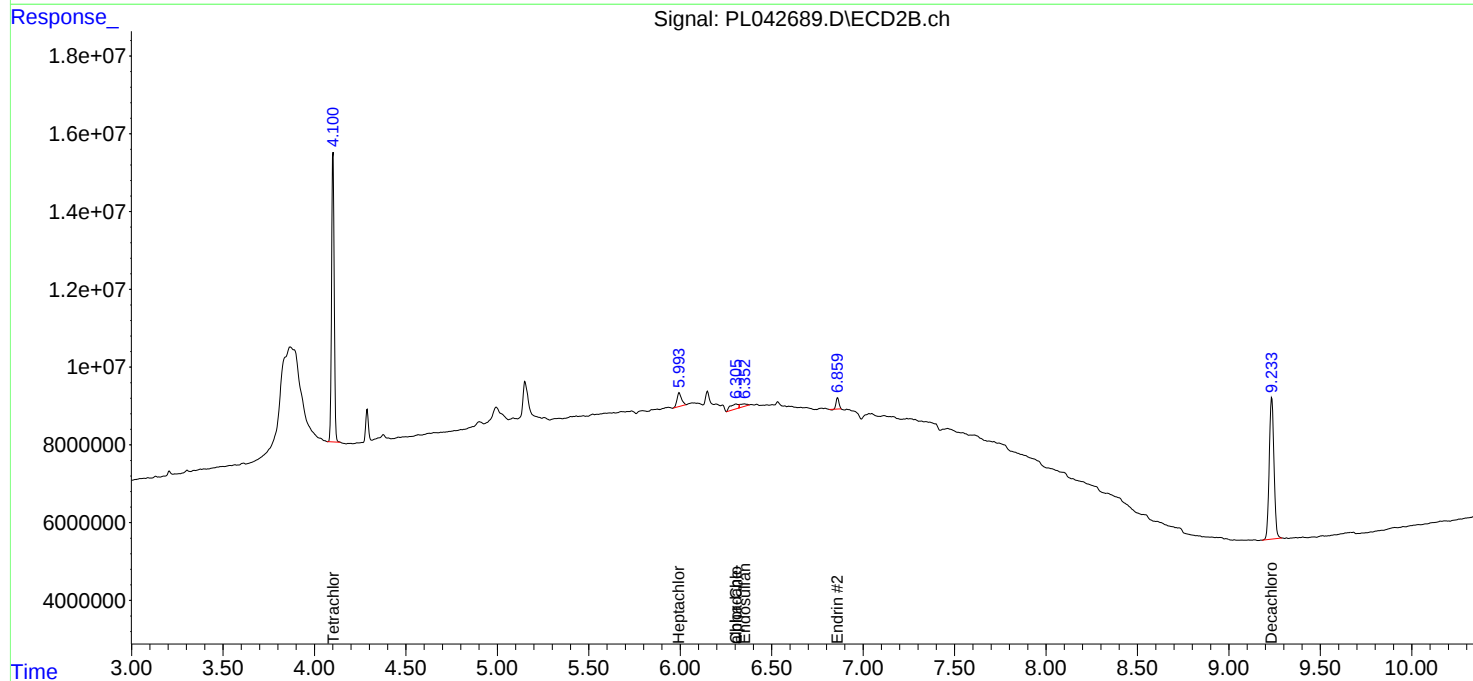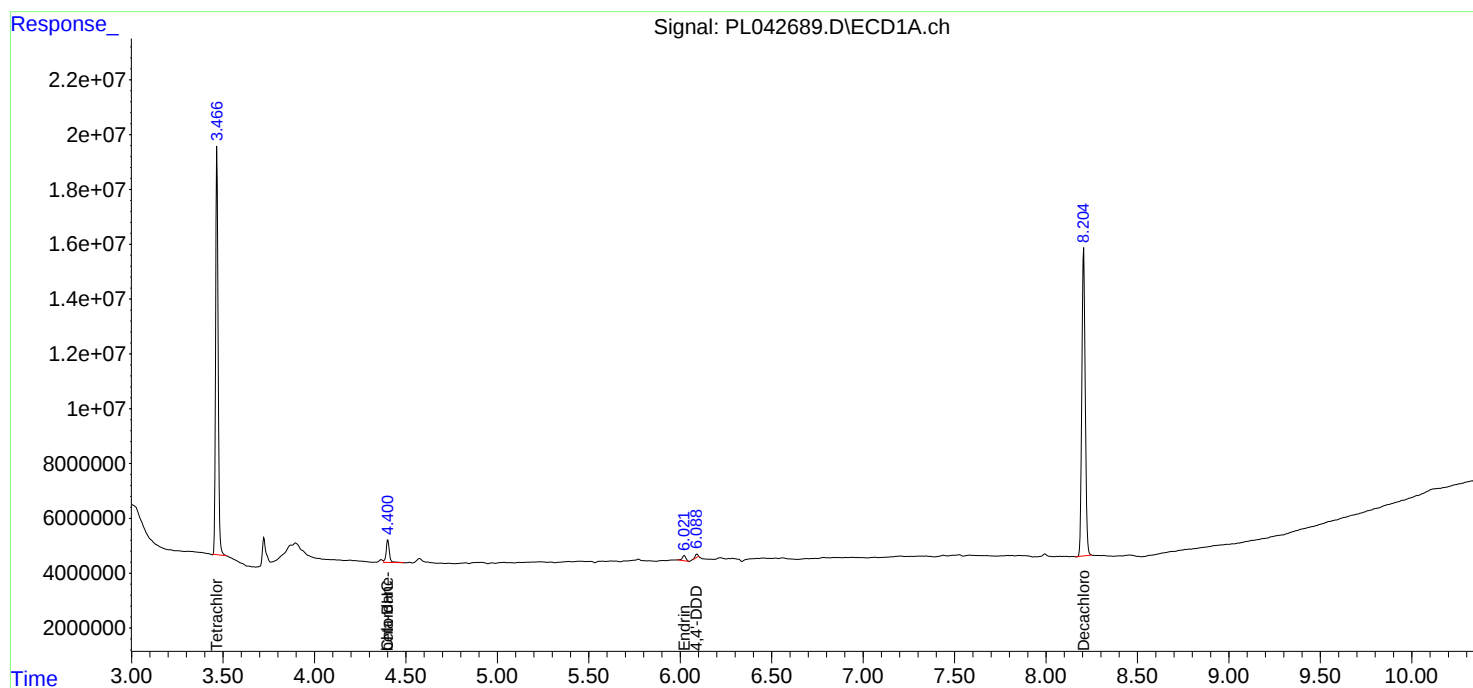


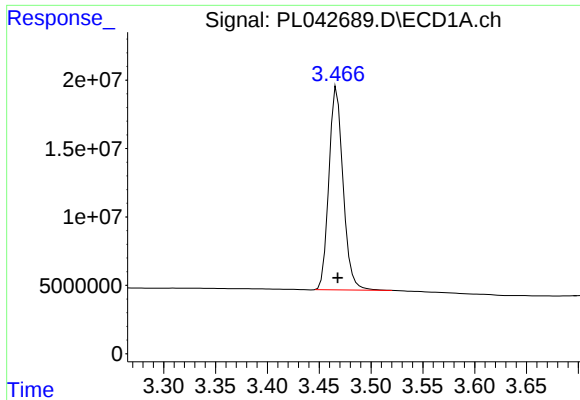

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 141022696
Conc: 23.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

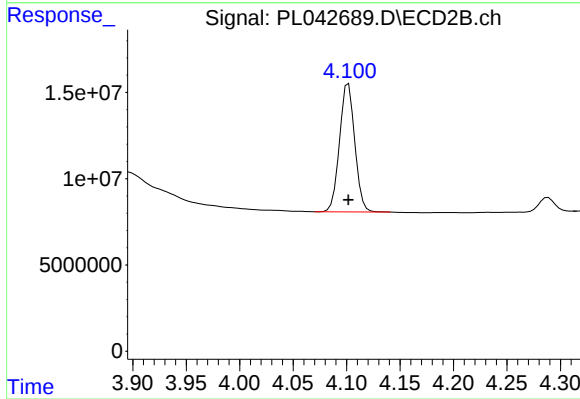


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 73934538
Conc: 25.71 ng/ml

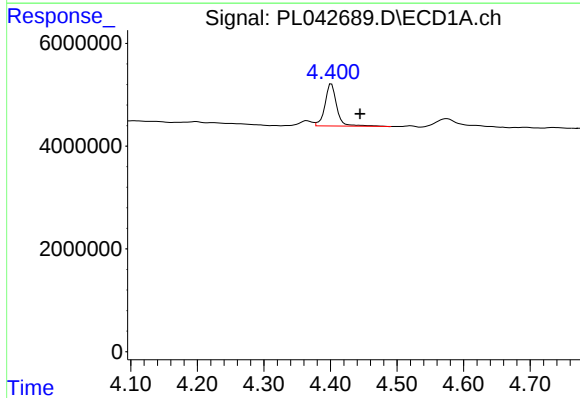


#6 beta-BHC

R.T.: 4.401 min
Delta R.T.: -0.043 min
Response: 10160321
Conc: 2.87 ng/ml

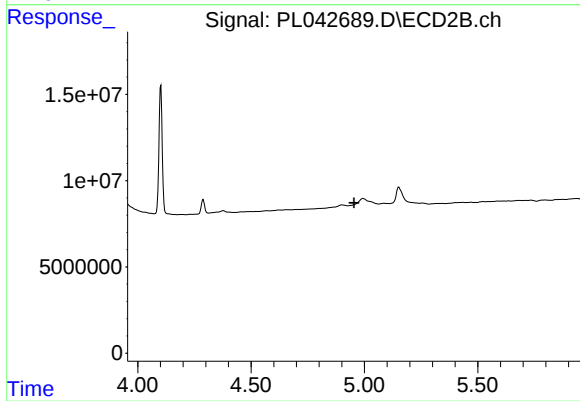

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

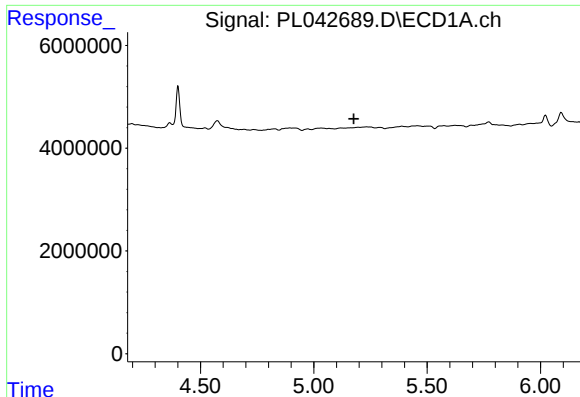

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

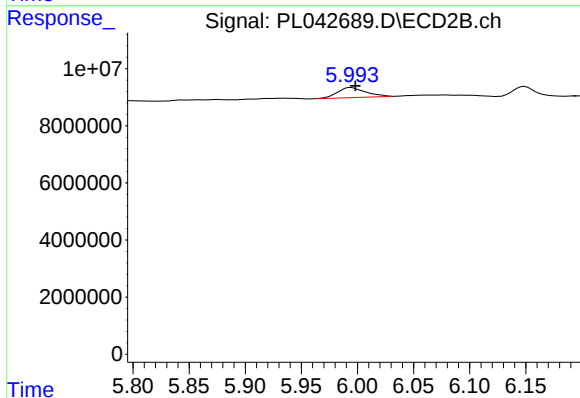


#8 Heptachlor epoxide

R.T.: 5.994 min
Delta R.T.: -0.004 min
Response: 6223369
Conc: 1.74 ng/ml

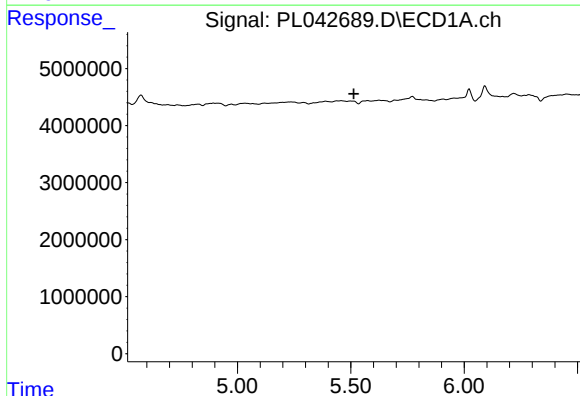


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.514 min
Response: 0
Conc: N.D.

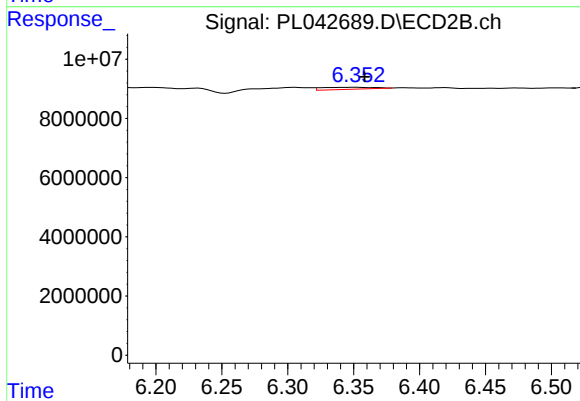

#9 Endosulfan I


R.T.: 6.353 min
Delta R.T.: -0.006 min
Response: 1890197
Conc: 0.60 ng/ml

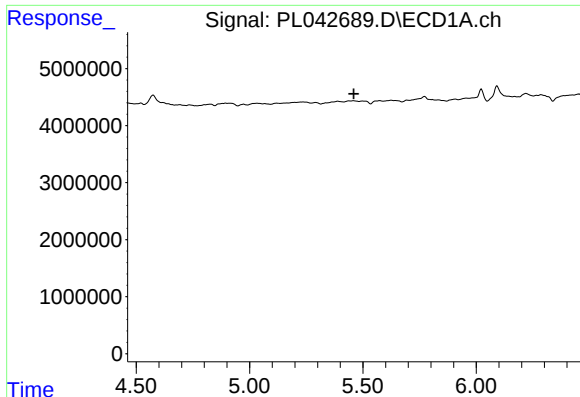

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

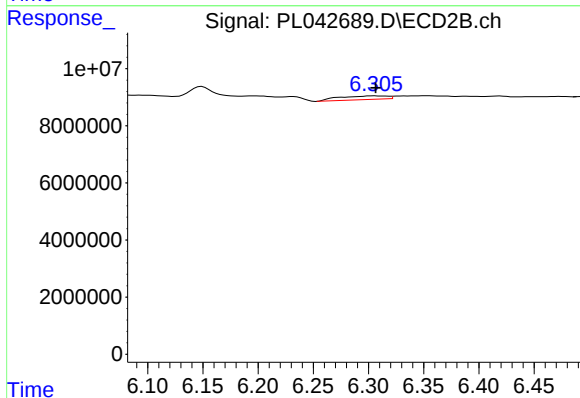


#11 alpha-Chlordane

R.T.: 6.306 min
Delta R.T.: -0.001 min
Response: 4011555
Conc: 1.20 ng/ml

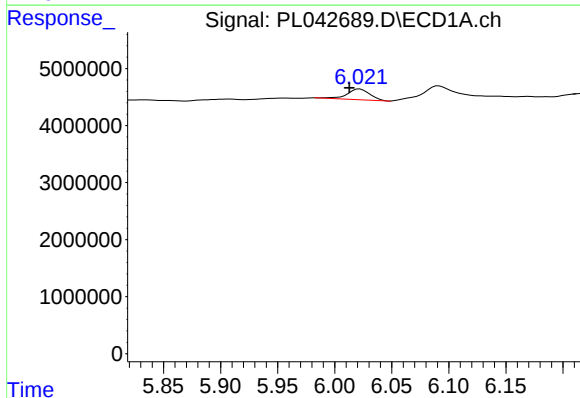


#14 Endrin

R.T.: 6.022 min
Delta R.T.: 0.009 min
Response: 2611235
Conc: 0.40 ng/ml

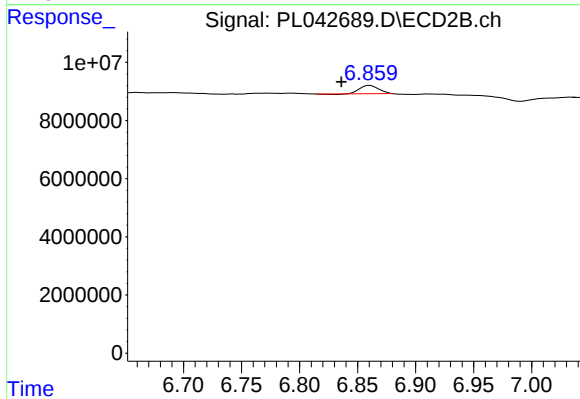

#14 Endrin


R.T.: 6.861 min
Delta R.T.: 0.024 min
Response: 3183347
Conc: 1.16 ng/ml

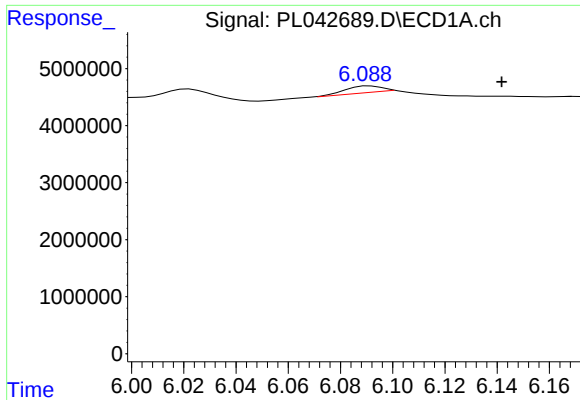

#16 4,4'-DDD


R.T.: 6.091 min
Delta R.T.: -0.050 min
Response: 1299115
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

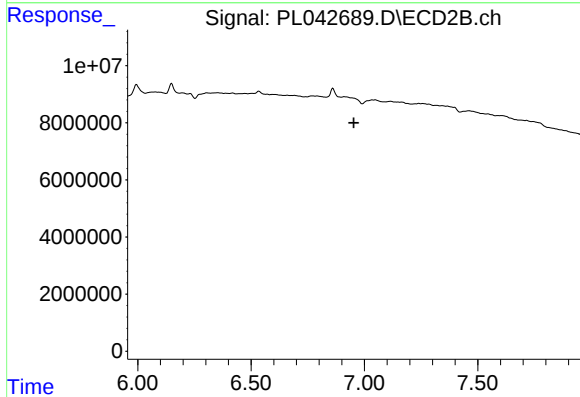


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.953 min
Response: 0
Conc: N.D.

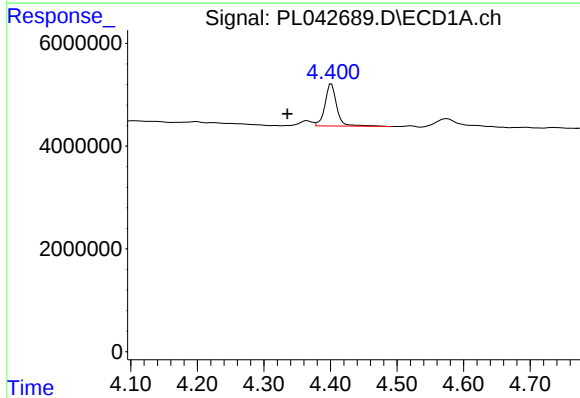


#23 Chlordane-1

R.T.: 4.401 min
Delta R.T.: 0.066 min
Response: 10160321
Conc: 36.75 ng/ml

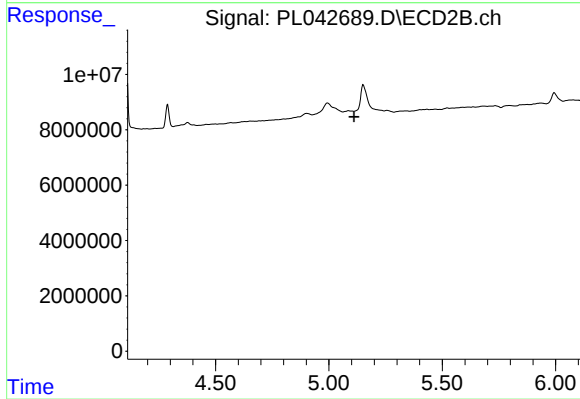

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

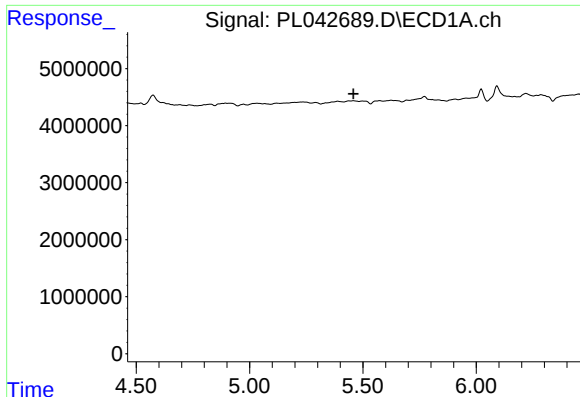

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

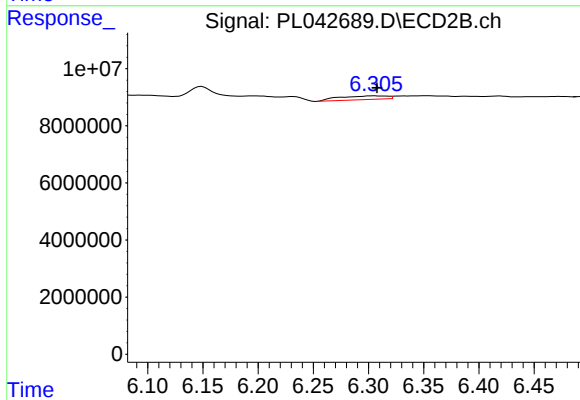


#26 Chlordane-4

R.T.: 6.306 min
Delta R.T.: -0.002 min
Response: 4011555
Conc: 7.33 ng/ml

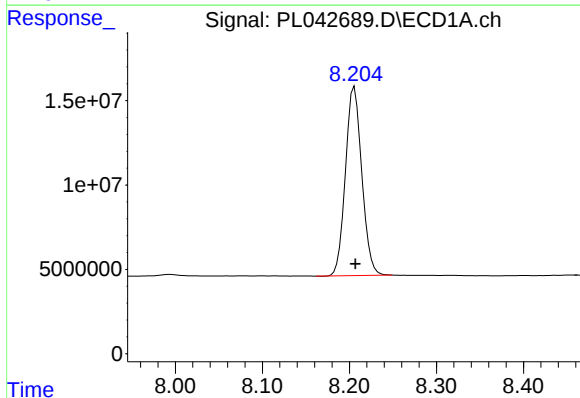

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.001 min
Response: 146253262
Conc: 23.21 ng/ml

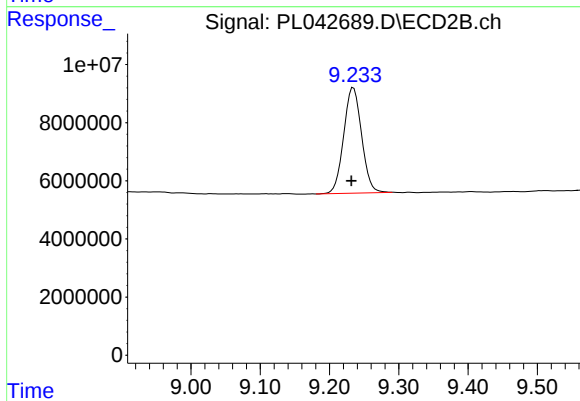

#28 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: 0.003 min
Response: 65201894
Conc: 27.03 ng/ml