

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120318\
 Data File : PL042710.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2018 20:48
 Operator : AJ\SJ
 Sample : J6179-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 23:59:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.102	107.2E6	57268530	18.219	19.912
28)	SA Decachlor...	8.206	9.235	91792779	38322932	14.565	15.889
Target Compounds							
6)	B beta-BHC	4.402f	0.000	5283447	0	1.491	N.D. #
7)	B delta-BHC	0.000	5.160	0	331997	N.D.	0.090 #
8)	B Heptachlo...	5.237f	5.995	4866376	5725531	0.642	1.597 #
9)	A Endosulfan I	5.542	6.310f	1292223	537908	0.187	0.170
10)	B gamma-Chl...	5.401	6.239	2680010	696249	0.351	0.205 #
11)	B alpha-Chl...	5.459	6.310	2889695	537908	0.385	0.161 #
15)	B Endosulfa...	6.222f	0.000	2033647	0	0.325	N.D. #
23)	Chlordane-1	4.360	5.160	2392899	331997	8.655	2.497 #
25)	Chlordane-3	5.401	6.239	2680010	696249	3.057	1.482 #
26)	Chlordane-4	5.459	6.310	2889695	537908	3.808	0.983 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120318\
Data File : PL042710.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2018 20:48
Operator : AJ\SJ
Sample : J6179-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 23:59:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

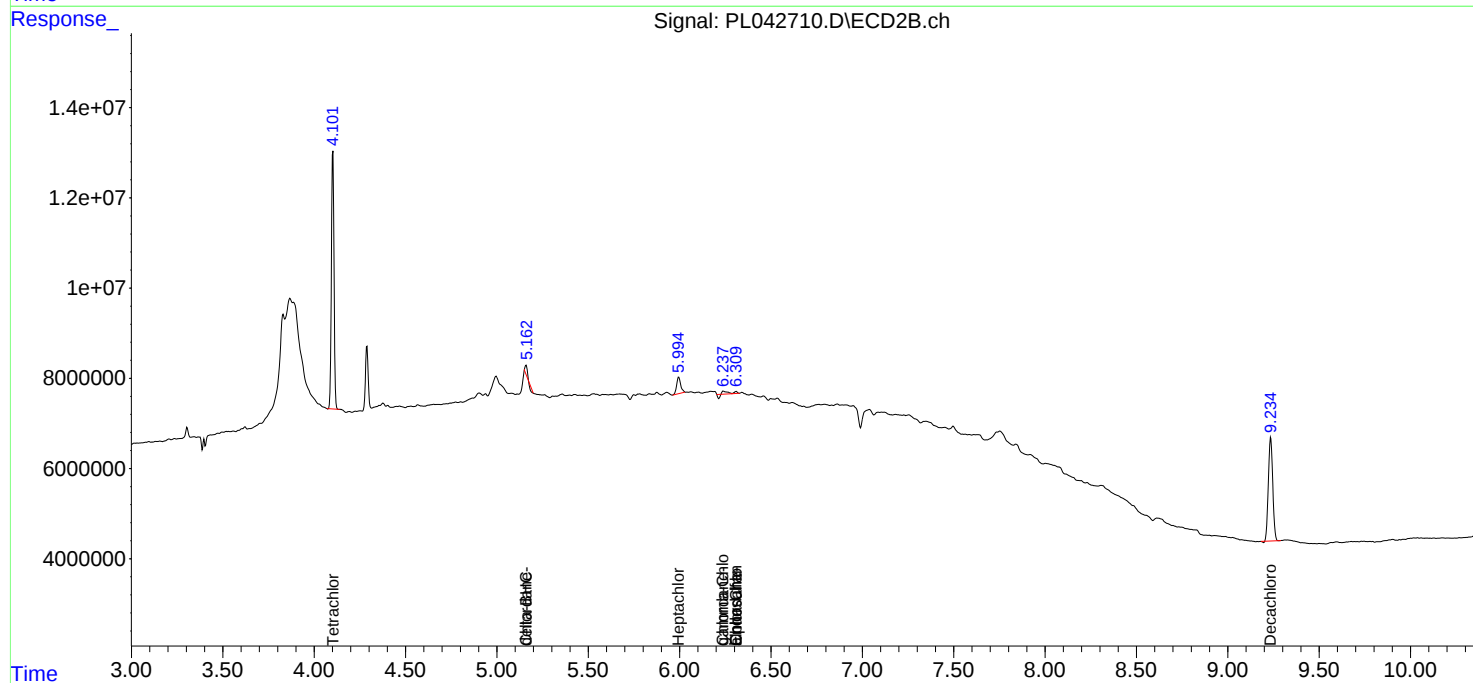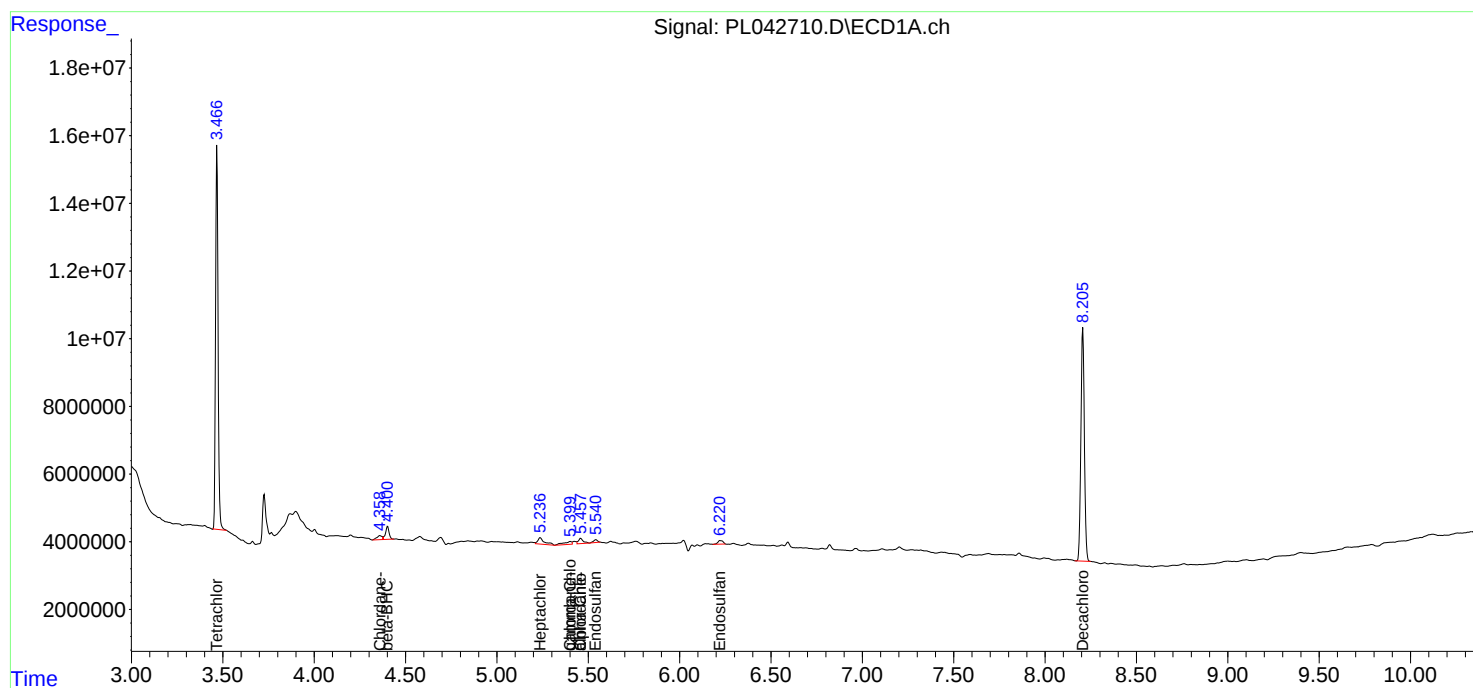


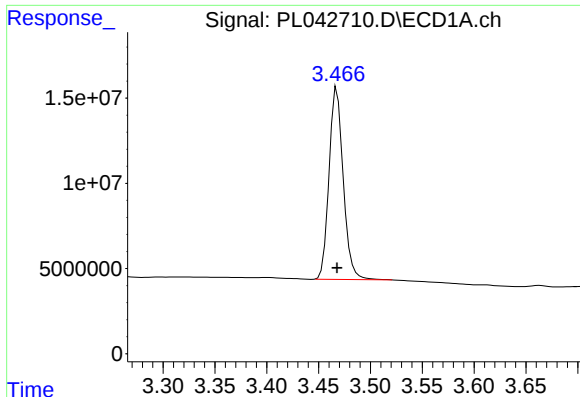

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: 0.000 min
Response: 107190756
Conc: 18.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

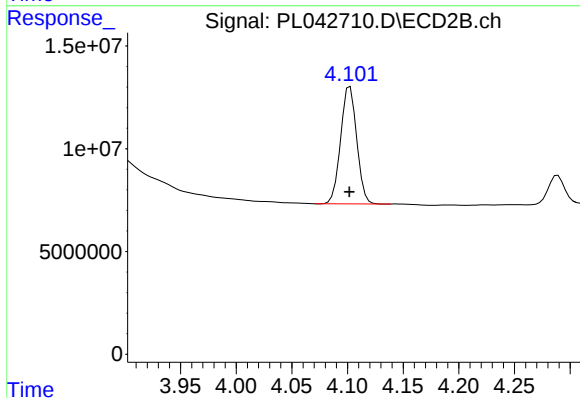


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 57268530
Conc: 19.91 ng/ml

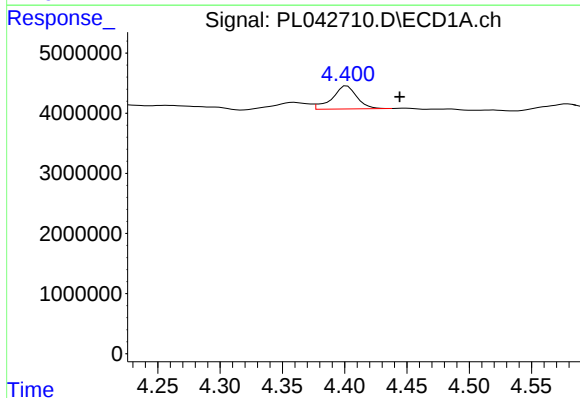


#6 beta-BHC

R.T.: 4.402 min
Delta R.T.: -0.042 min
Response: 5283447
Conc: 1.49 ng/ml

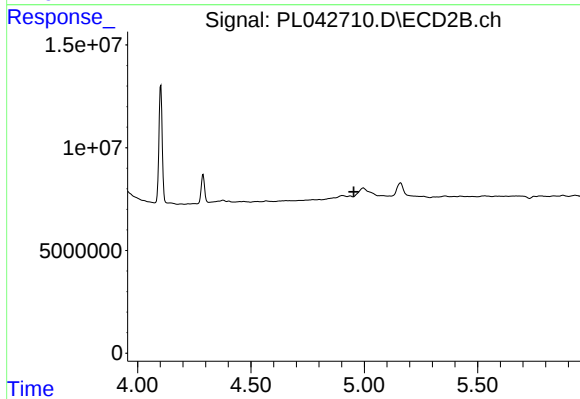

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

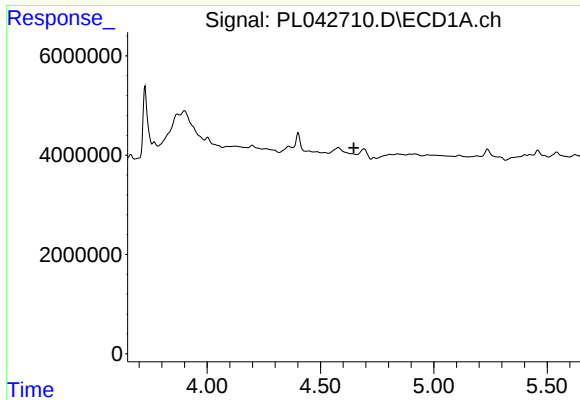

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.646 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

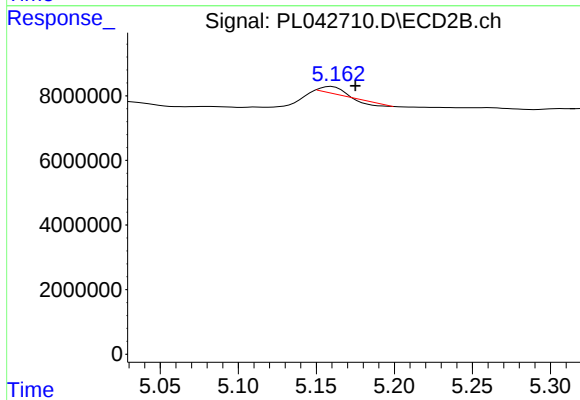


#7 delta-BHC

R.T.: 5.160 min
Delta R.T.: -0.015 min
Response: 331997
Conc: 0.09 ng/ml

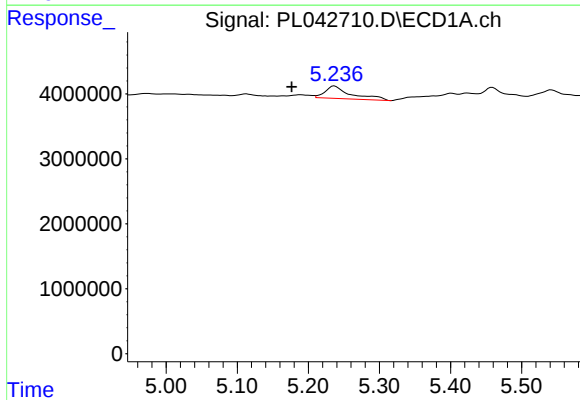


#8 Heptachlor epoxide

R.T.: 5.237 min
Delta R.T.: 0.060 min
Response: 4866376
Conc: 0.64 ng/ml

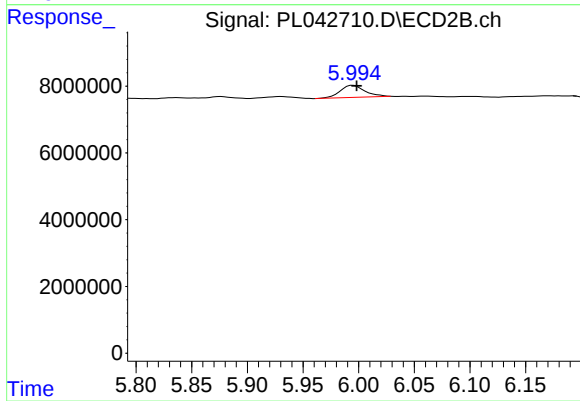

#8 Heptachlor epoxide


R.T.: 5.995 min
Delta R.T.: -0.003 min
Response: 5725531
Conc: 1.60 ng/ml

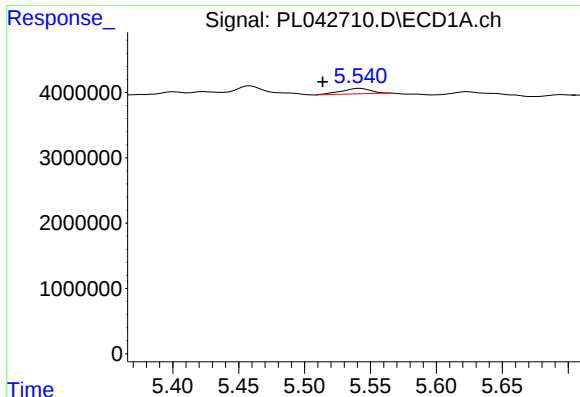

#9 Endosulfan I


R.T.: 5.542 min
Delta R.T.: 0.028 min
Response: 1292223
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

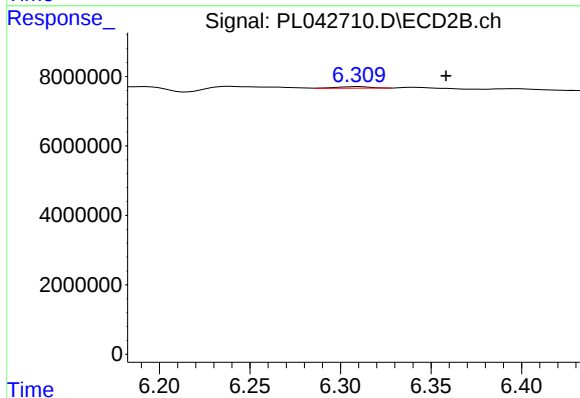


#9 Endosulfan I

R.T.: 6.310 min
Delta R.T.: -0.048 min
Response: 537908
Conc: 0.17 ng/ml

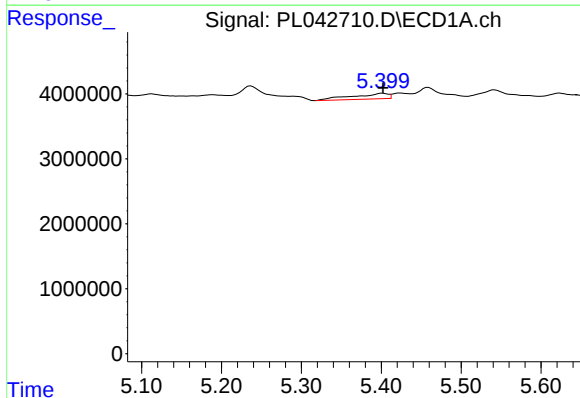


#10 gamma-Chlordane

R.T.: 5.401 min
Delta R.T.: 0.000 min
Response: 2680010
Conc: 0.35 ng/ml

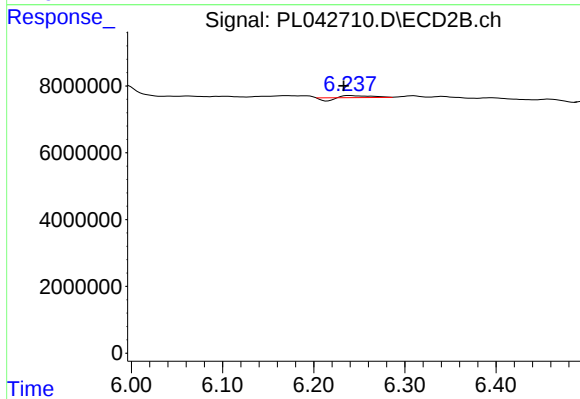

#10 gamma-Chlordane


R.T.: 6.239 min
Delta R.T.: 0.006 min
Response: 696249
Conc: 0.20 ng/ml

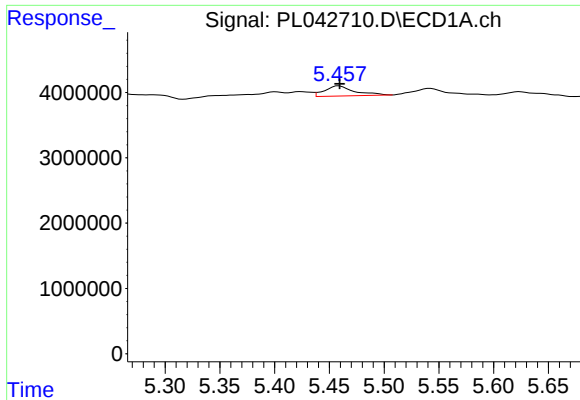

#11 alpha-Chlordane


R.T.: 5.459 min
Delta R.T.: 0.000 min
Response: 2889695
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

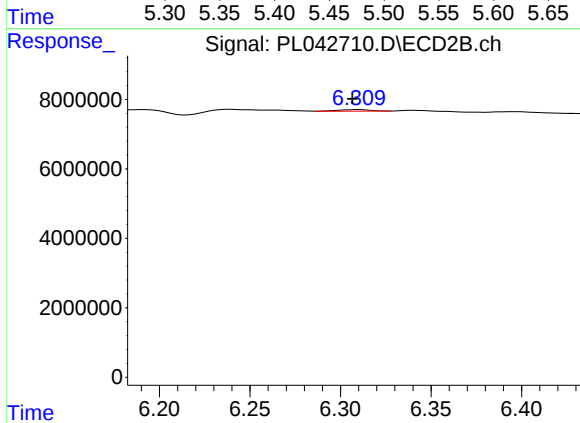


#11 alpha-Chlordane

R.T.: 6.310 min
Delta R.T.: 0.004 min
Response: 537908
Conc: 0.16 ng/ml

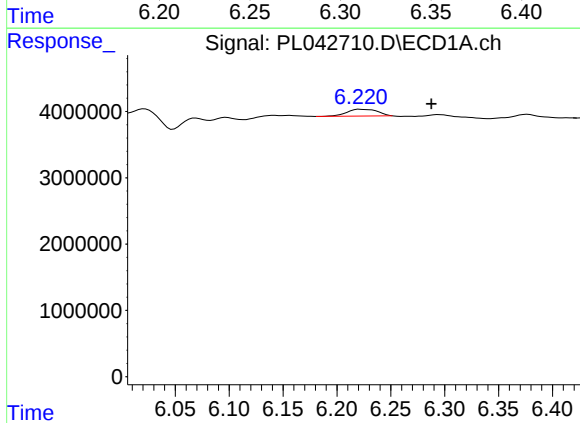


#15 Endosulfan II

R.T.: 6.222 min
Delta R.T.: -0.066 min
Response: 2033647
Conc: 0.33 ng/ml

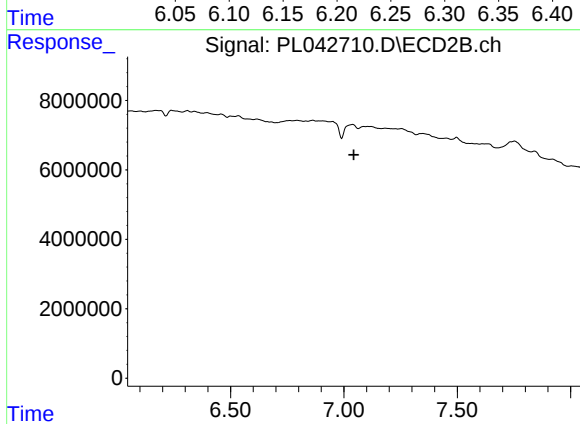

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 7.044 min
Response: 0
Conc: N.D.

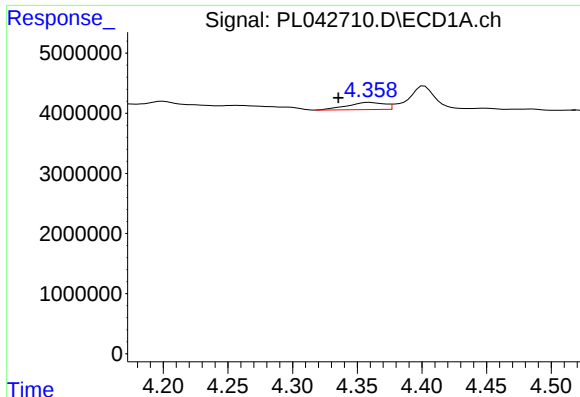

#23 Chlordane-1


R.T.: 4.360 min
Delta R.T.: 0.024 min
Response: 2392899
Conc: 8.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

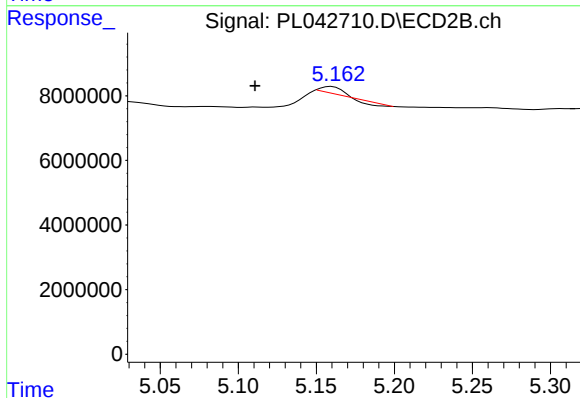


#23 Chlordane-1

R.T.: 5.160 min
Delta R.T.: 0.049 min
Response: 331997
Conc: 2.50 ng/ml

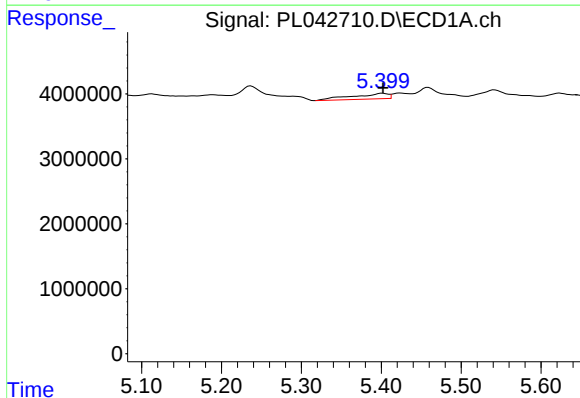


#25 Chlordane-3

R.T.: 5.401 min
Delta R.T.: 0.000 min
Response: 2680010
Conc: 3.06 ng/ml

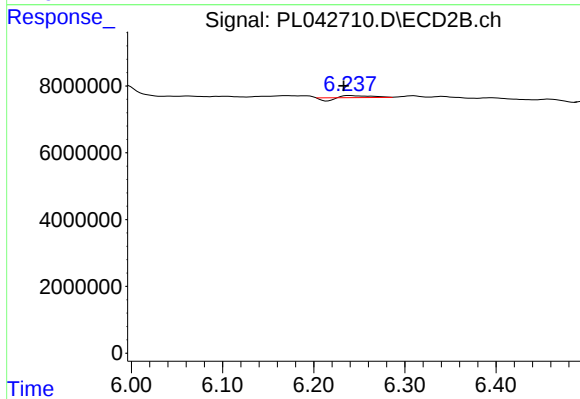

#25 Chlordane-3


R.T.: 6.239 min
Delta R.T.: 0.006 min
Response: 696249
Conc: 1.48 ng/ml

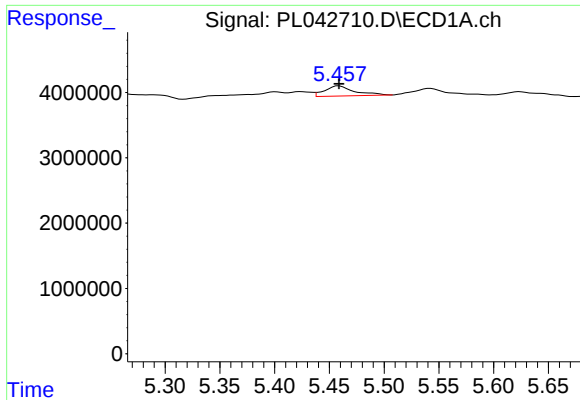

#26 Chlordane-4


R.T.: 5.459 min
Delta R.T.: 0.000 min
Response: 2889695
Conc: 3.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

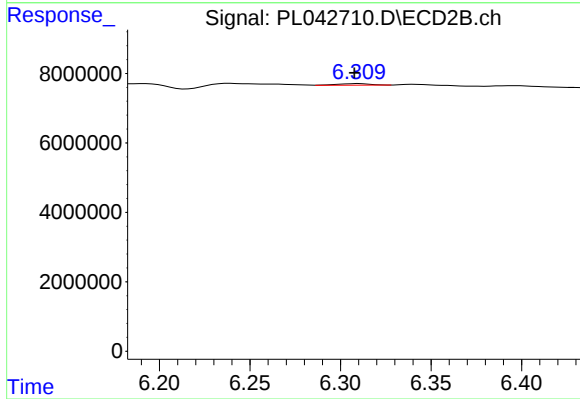


#26 Chlordane-4

R.T.: 6.310 min
Delta R.T.: 0.002 min
Response: 537908
Conc: 0.98 ng/ml

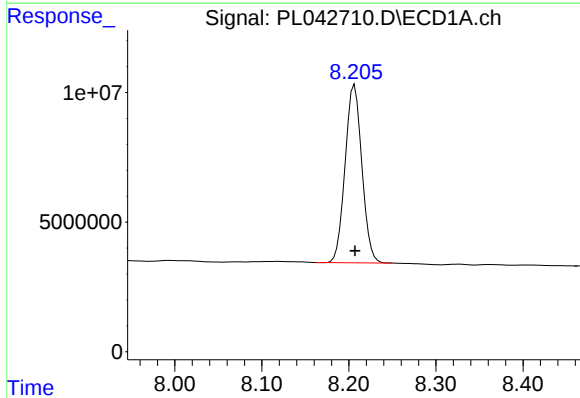

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 91792779
Conc: 14.57 ng/ml

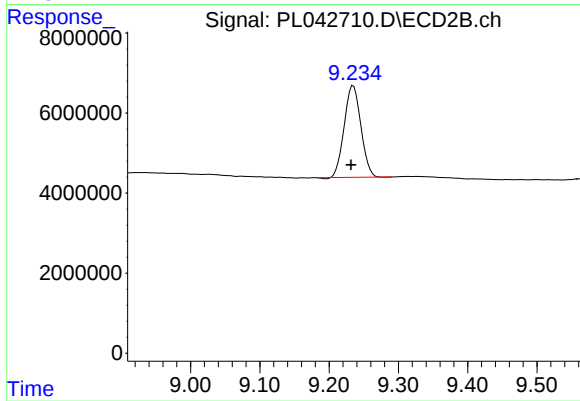

#28 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: 0.003 min
Response: 38322932
Conc: 15.89 ng/ml