

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120318\
 Data File : PL042718.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2018 22:40
 Operator : AJ\SJ
 Sample : J6179-10
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 00:00:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.102	103.6E6	55166153	17.605	19.181
28)	SA Decachlor...	8.206	9.235	74137324	31493903	11.764	13.058
Target Compounds							
6)	B beta-BHC	4.401f	0.000	3723565	0	1.051	N.D. #
7)	B delta-BHC	0.000	5.162	0	3982928	N.D.	1.082 #
8)	B Heptachlo...	5.237f	5.995	4083975	7453499	0.539	2.079 #
9)	A Endosulfan I	5.543	6.302f	1975887	1472295	0.286	0.466 #
10)	B gamma-Chl...	0.000	6.261	0	355995	N.D.	0.105 #
11)	B alpha-Chl...	0.000	6.302	0	1472295	N.D.	0.440 #
14)	MA Endrin	6.022	0.000	5456278	0	0.834	N.D. #
23)	Chlordane-1	4.355	5.162	2461001	3982928	8.901	29.962 #
25)	Chlordane-3	0.000	6.261	0	355995	N.D.	0.758 #
26)	Chlordane-4	0.000	6.302	0	1472295	N.D.	2.691 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120318\
Data File : PL042718.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2018 22:40
Operator : AJ\SJ
Sample : J6179-10
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 00:00:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

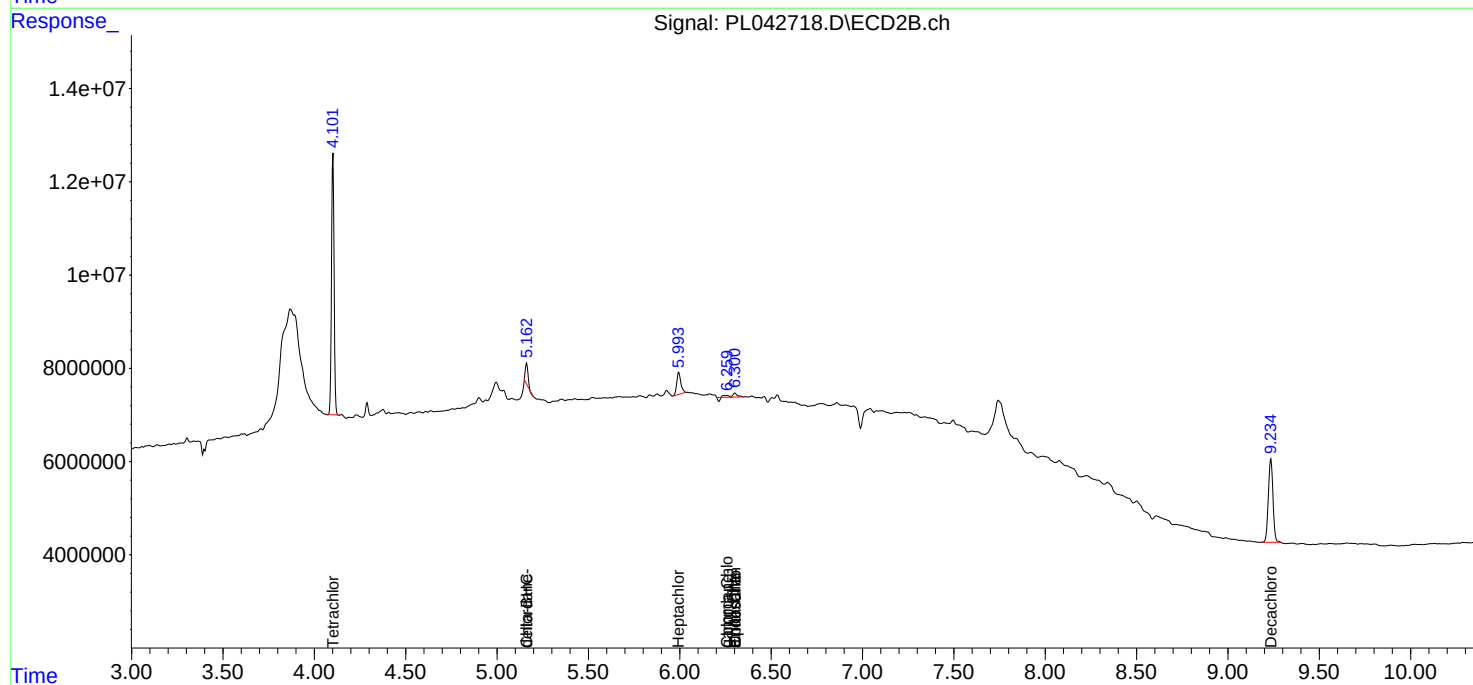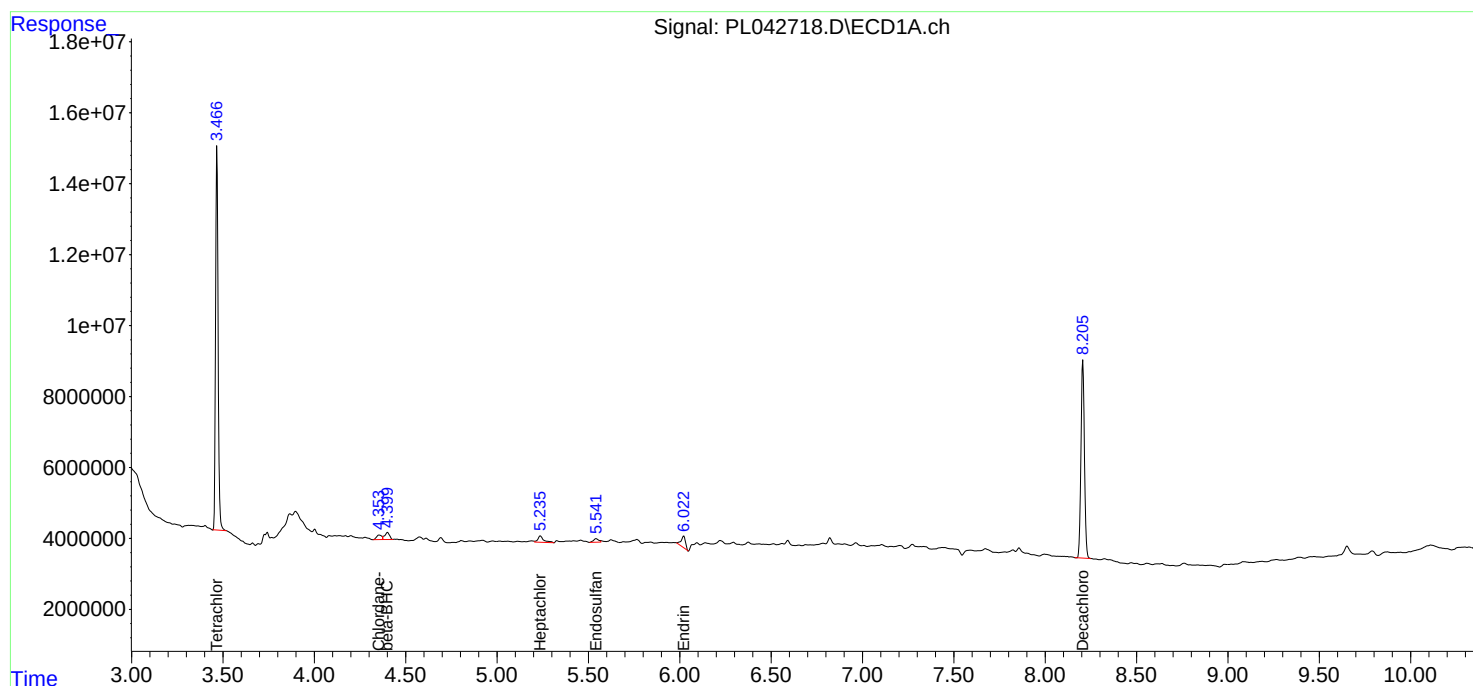


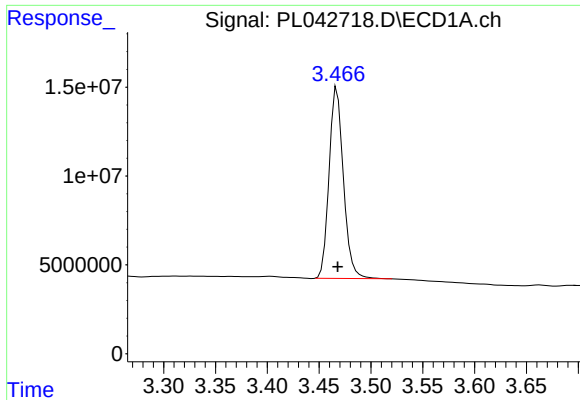

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 103576195
Conc: 17.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

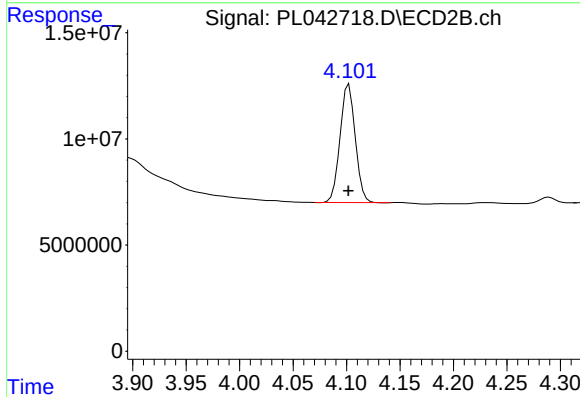


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 55166153
Conc: 19.18 ng/ml

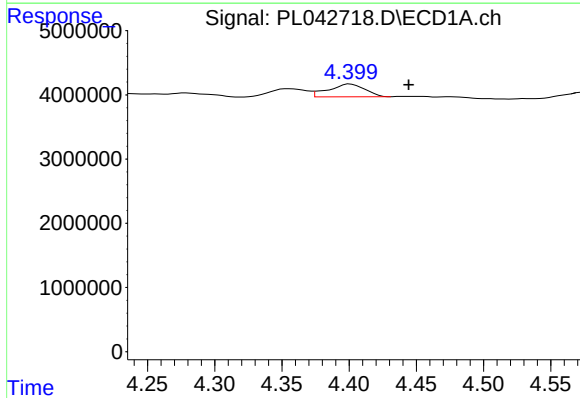


#6 beta-BHC

R.T.: 4.401 min
Delta R.T.: -0.043 min
Response: 3723565
Conc: 1.05 ng/ml

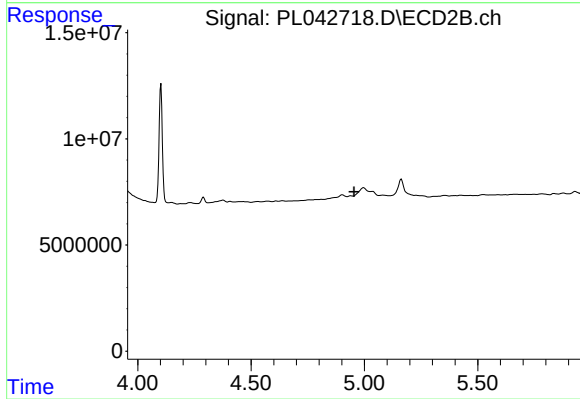

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

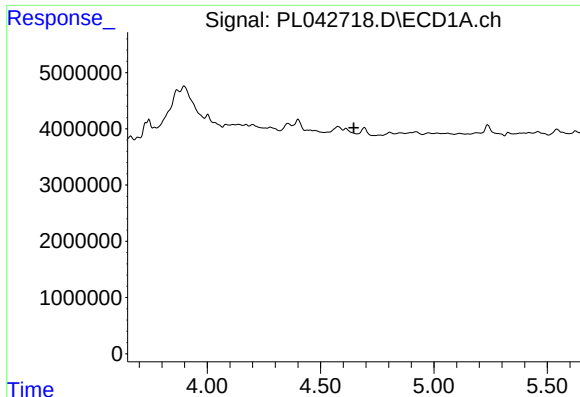

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.646 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

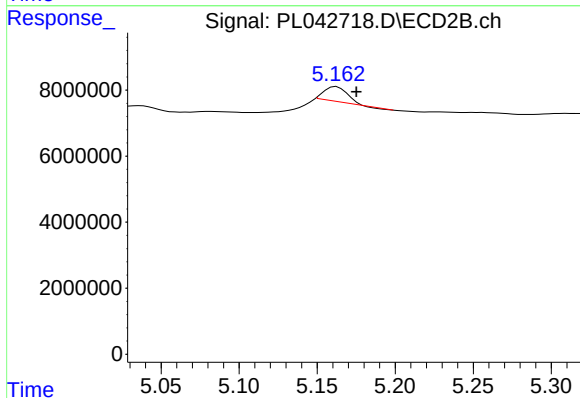


#7 delta-BHC

R.T.: 5.162 min
Delta R.T.: -0.013 min
Response: 3982928
Conc: 1.08 ng/ml

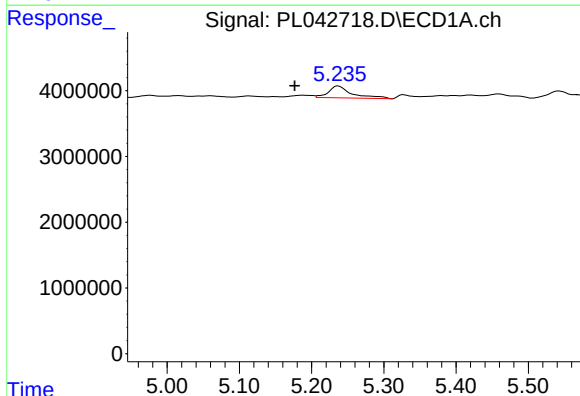


#8 Heptachlor epoxide

R.T.: 5.237 min
Delta R.T.: 0.060 min
Response: 4083975
Conc: 0.54 ng/ml

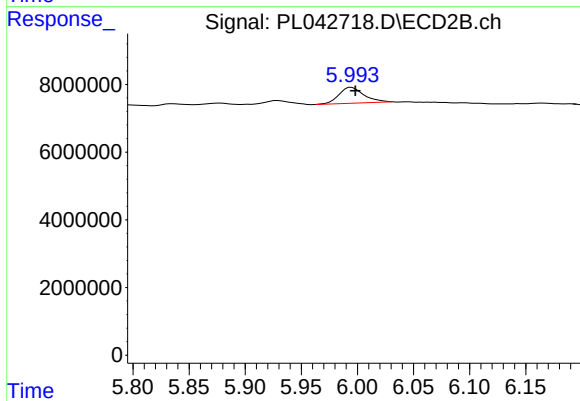

#8 Heptachlor epoxide


R.T.: 5.995 min
Delta R.T.: -0.003 min
Response: 7453499
Conc: 2.08 ng/ml

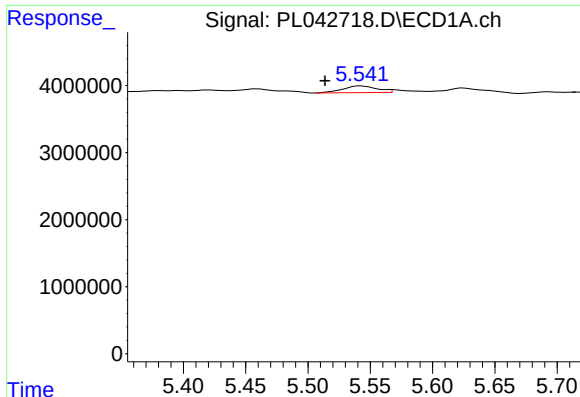

#9 Endosulfan I


R.T.: 5.543 min
Delta R.T.: 0.029 min
Response: 1975887
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

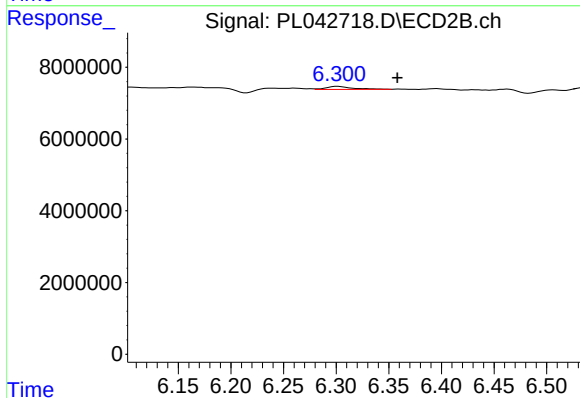


#9 Endosulfan I

R.T.: 6.302 min
Delta R.T.: -0.057 min
Response: 1472295
Conc: 0.47 ng/ml

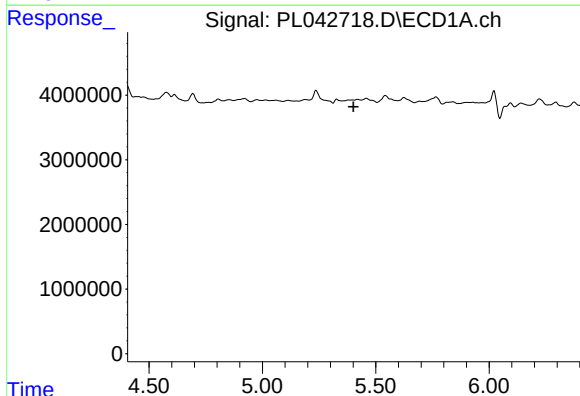


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

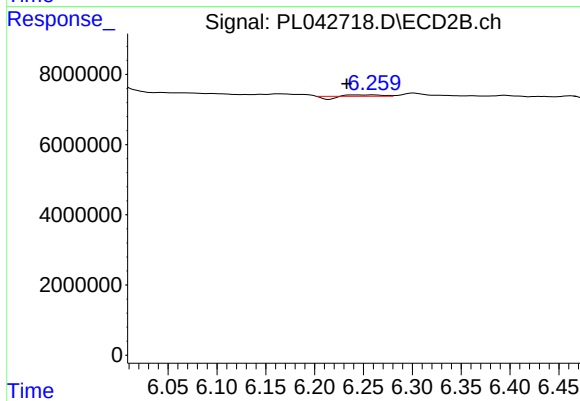

#10 gamma-Chlordane


R.T.: 6.261 min
Delta R.T.: 0.028 min
Response: 355995
Conc: 0.10 ng/ml

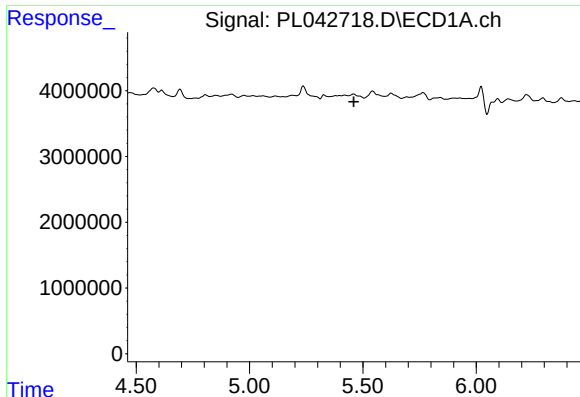

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

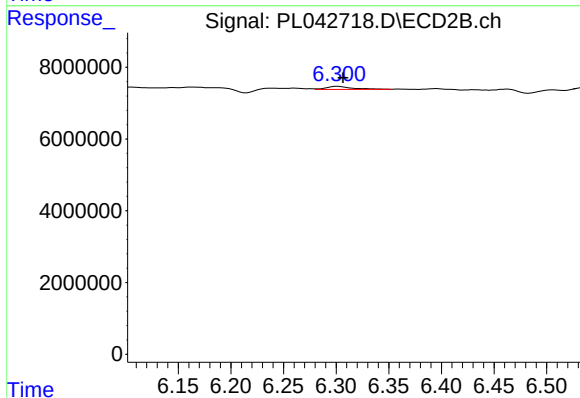


#11 alpha-Chlordane

R.T.: 6.302 min
Delta R.T.: -0.005 min
Response: 1472295
Conc: 0.44 ng/ml

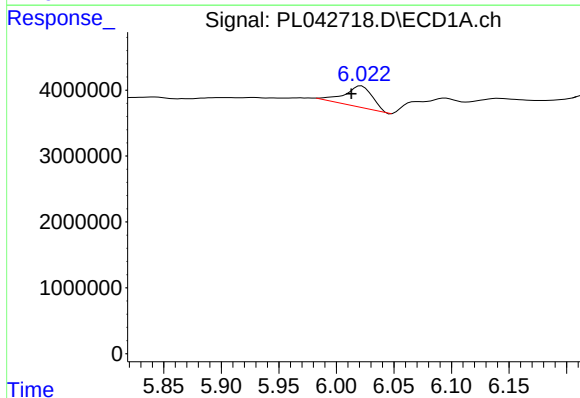


#14 Endrin

R.T.: 6.022 min
Delta R.T.: 0.009 min
Response: 5456278
Conc: 0.83 ng/ml

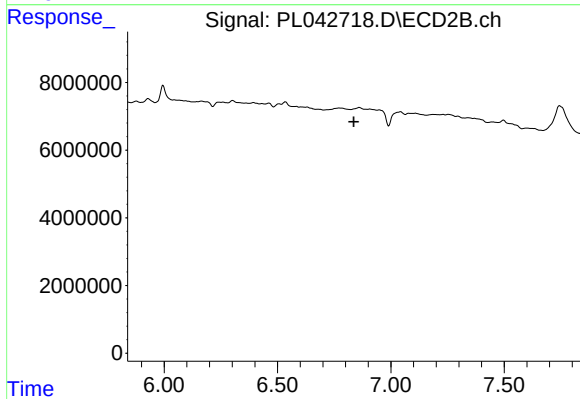

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.836 min
Response: 0
Conc: N.D.

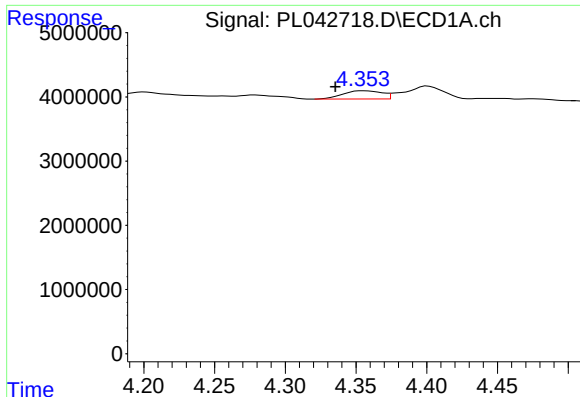

#23 Chlordane-1


R.T.: 4.355 min
Delta R.T.: 0.019 min
Response: 2461001
Conc: 8.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

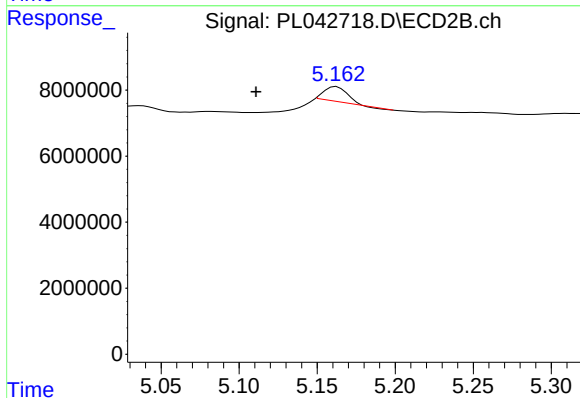


#23 Chlordane-1

R.T.: 5.162 min
Delta R.T.: 0.052 min
Response: 3982928
Conc: 29.96 ng/ml

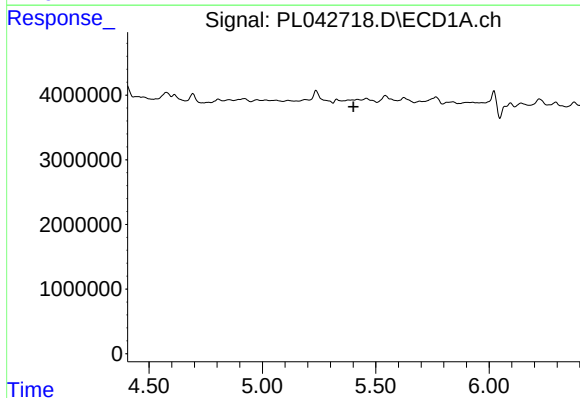


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

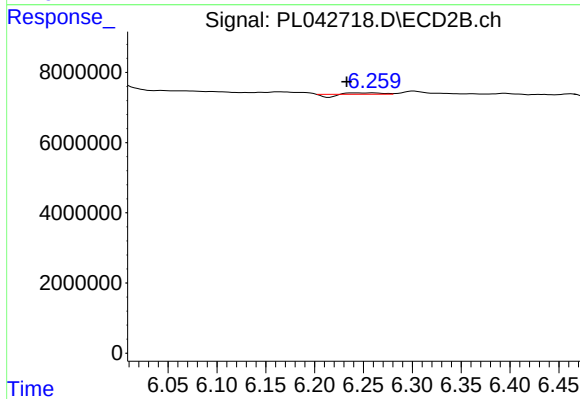

#25 Chlordane-3


R.T.: 6.261 min
Delta R.T.: 0.028 min
Response: 355995
Conc: 0.76 ng/ml

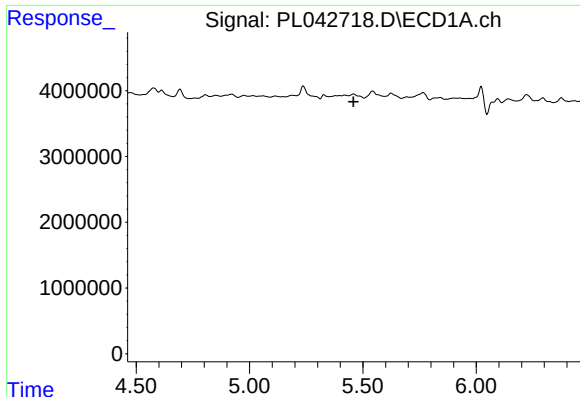

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

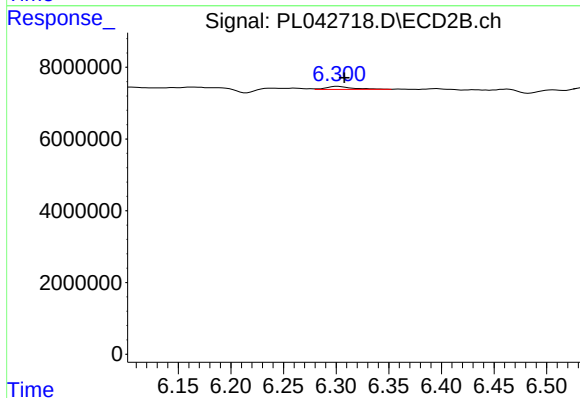


#26 Chlordane-4

R.T.: 6.302 min
Delta R.T.: -0.006 min
Response: 1472295
Conc: 2.69 ng/ml

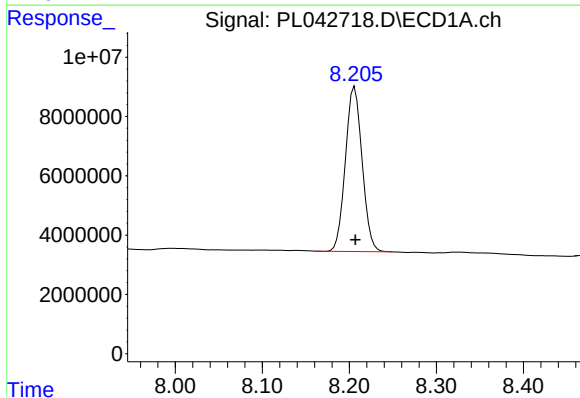

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 74137324
Conc: 11.76 ng/ml

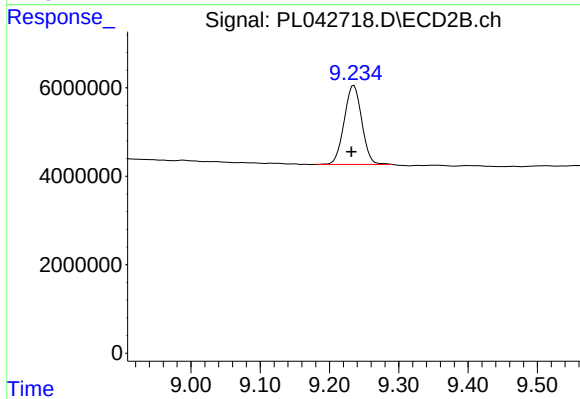

#28 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: 0.004 min
Response: 31493903
Conc: 13.06 ng/ml