

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120318\
 Data File : PL042722.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2018 23:37
 Operator : AJ\SJ
 Sample : PB115250BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 00:01:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.102	114.9E6	62219975	19.531	21.633
28)	SA Decachlor...	8.206	9.235	120.4E6	51591468	19.106	21.391
Target Compounds							
6)	B beta-BHC	4.405f	0.000	3322049	0	0.938	N.D. #
7)	B delta-BHC	0.000	5.162	0	3336423	N.D.	0.907 #
8)	B Heptachlo...	0.000	5.995	0	5287423	N.D.	1.475 #
23)	Chlordane-1	0.000	5.162	0	3336423	N.D.	25.099 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120318\
Data File : PL042722.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2018 23:37
Operator : AJ\SJ
Sample : PB115250BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 00:01:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

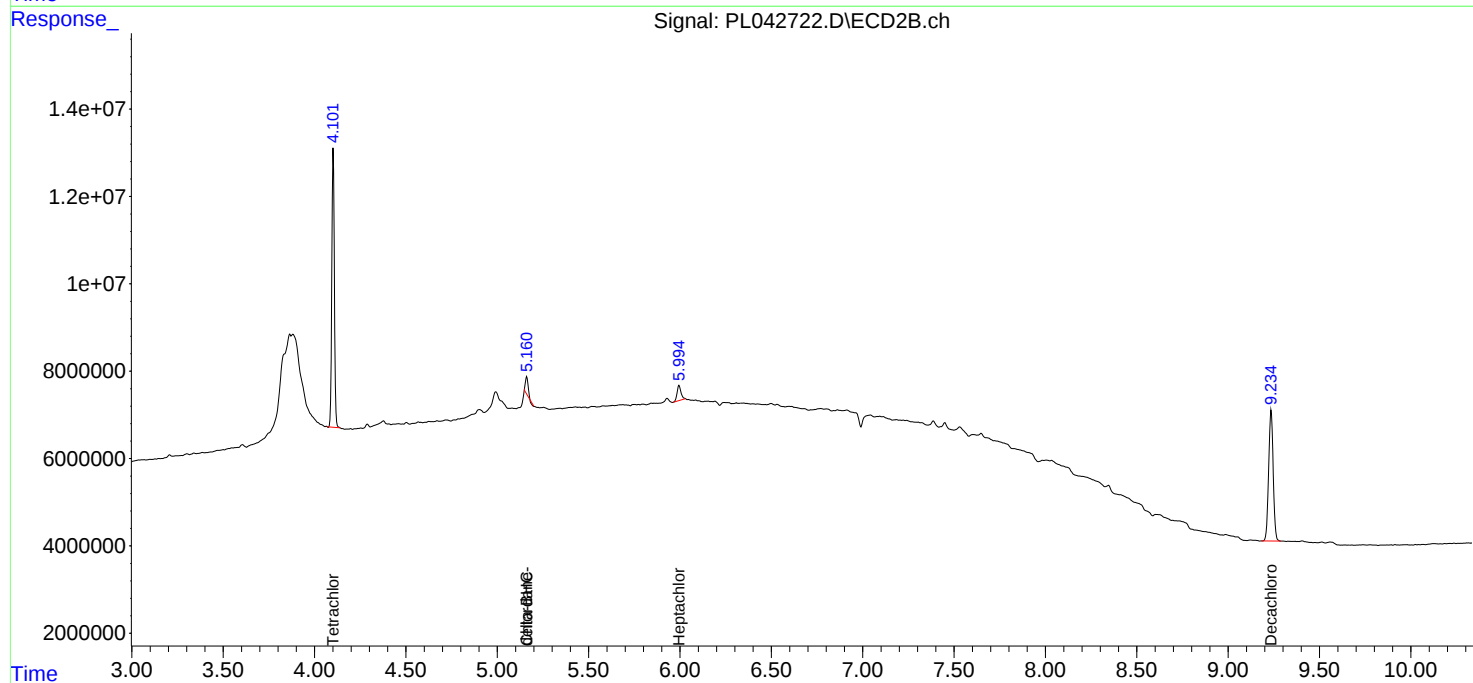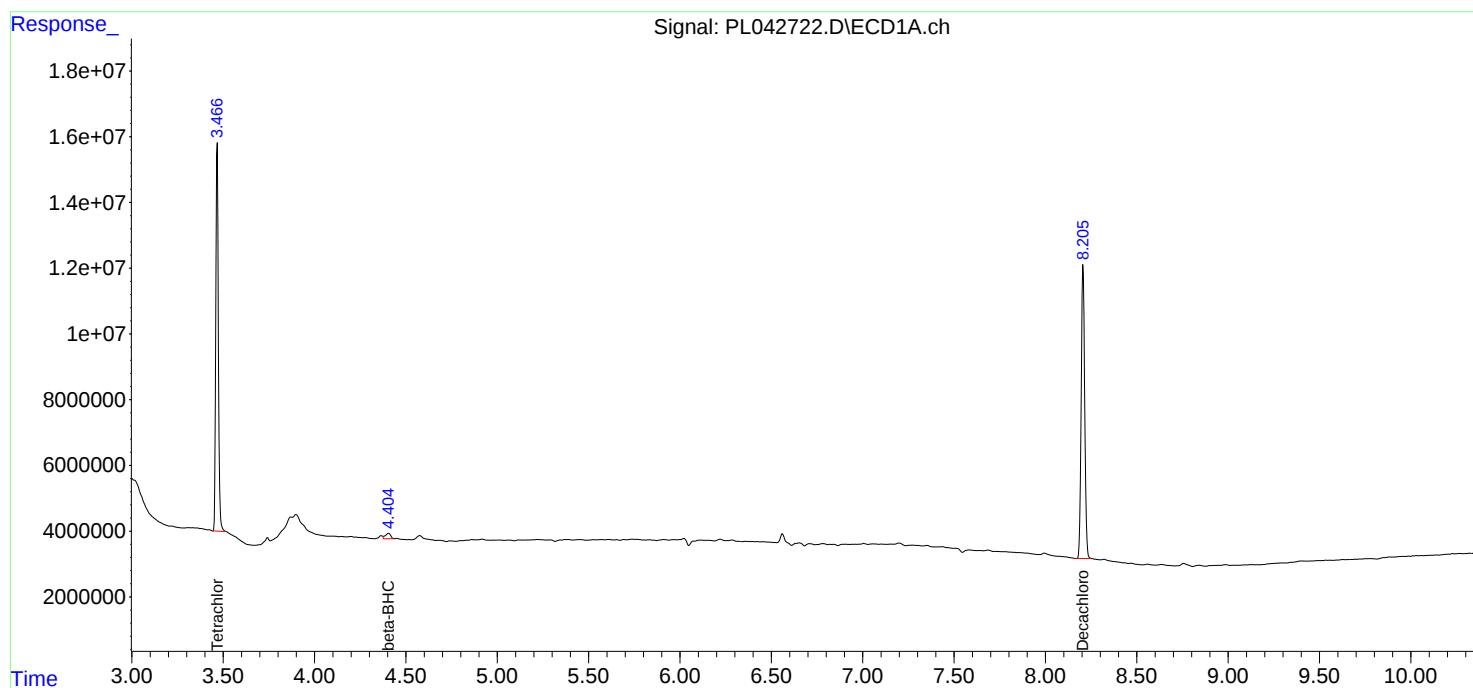


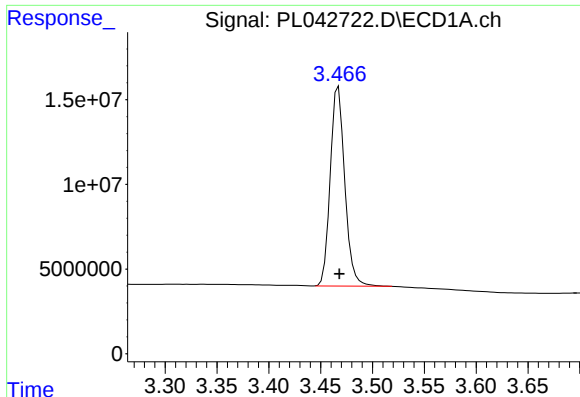

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 114909140
Conc: 19.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

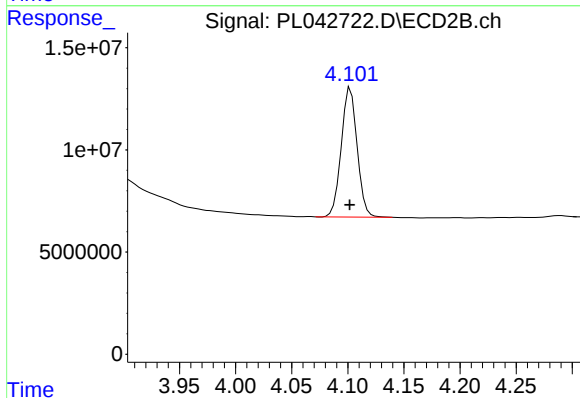


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 62219975
Conc: 21.63 ng/ml

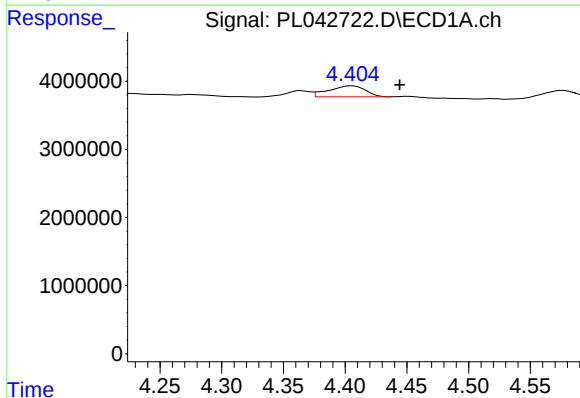


#6 beta-BHC

R.T.: 4.405 min
Delta R.T.: -0.039 min
Response: 3322049
Conc: 0.94 ng/ml

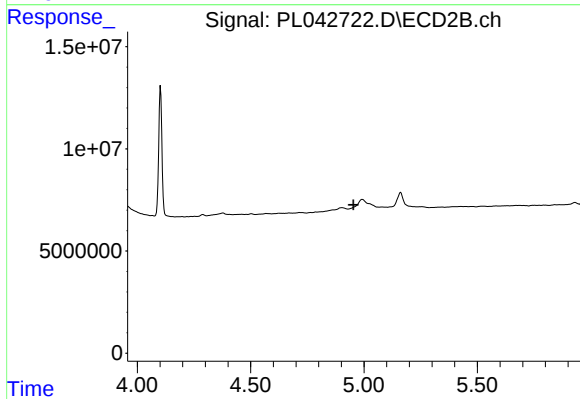

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

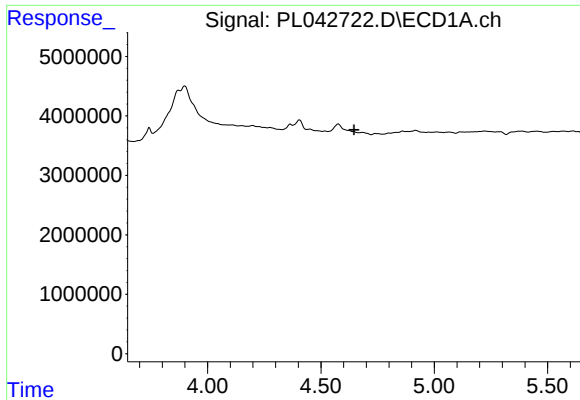

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.646 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

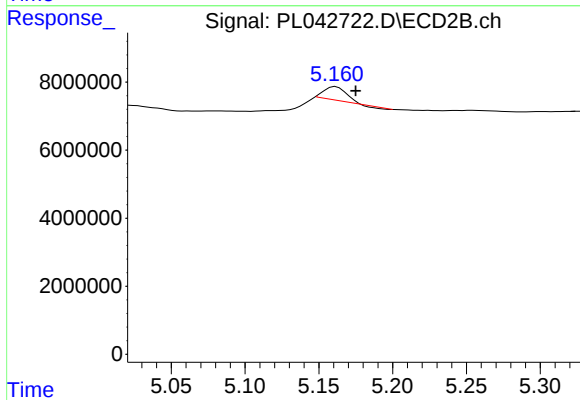


#7 delta-BHC

R.T.: 5.162 min
Delta R.T.: -0.013 min
Response: 3336423
Conc: 0.91 ng/ml

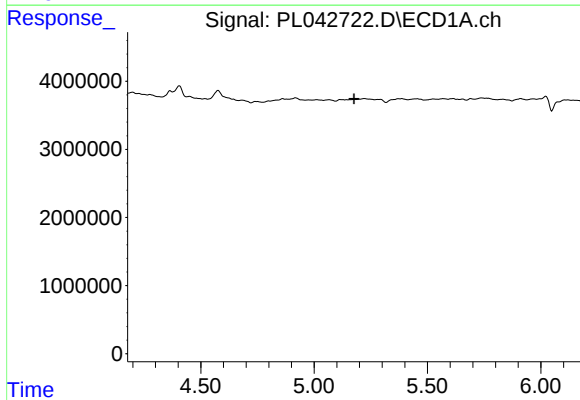


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.177 min
Response: 0
Conc: N.D.

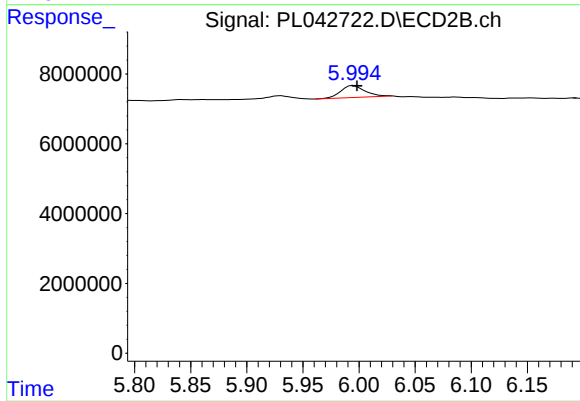

#8 Heptachlor epoxide

R.T.: 5.995 min
Delta R.T.: -0.003 min
Response: 5287423
Conc: 1.47 ng/ml

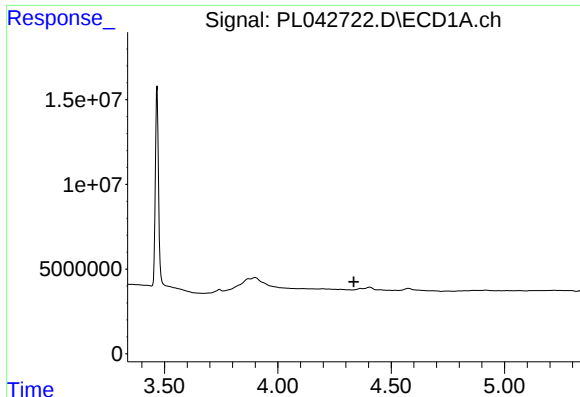

#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

#23 Chlordane-1

R.T.: 5.162 min
Delta R.T.: 0.051 min
Response: 3336423
Conc: 25.10 ng/ml

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 120405523
Conc: 19.11 ng/ml

#28 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: 0.004 min
Response: 51591468
Conc: 21.39 ng/ml