

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120318\
 Data File : PL042732.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2018 01:58
 Operator : AJ\SJ
 Sample : J5775-04
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 02:26:51 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.102	28490796	15274528	4.843	5.311
28)	SA Decachlor...	8.205	9.233	34748548	14810674	5.514	6.141
Target Compounds							
2)	A alpha-BHC	3.940f	4.489	1127442	2513653	0.125	0.587 #
3)	MA gamma-BHC...	0.000	4.832f	0	2570941	N.D.	0.651 #
4)	MA Heptachlor	4.447f	0.000	4903173	0	0.563	N.D. #
5)	MB Aldrin	0.000	5.638f	0	479834	N.D.	0.125 #
6)	B beta-BHC	4.447	4.905f	4903173	1164443	1.384	0.738 #
8)	B Heptachlo...	5.244f	5.994	2586805	5465888	0.341	1.524 #
18)	B Endrin al...	6.457	0.000	2142922	0	0.412	N.D. #
19)	B Endosulfa...	6.675	0.000	5072204	0	0.813	N.D. #
20)	A Methoxychlor	0.000	7.642f	0	4450501	N.D.	3.264 #
23)	Chlordane-1	4.342	0.000	2203237	0	7.969	N.D. #
24)	Chlordane-2	4.903	5.638	6485550	479834	23.078	3.441 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120318\
Data File : PL042732.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2018 01:58
Operator : AJ\SJ
Sample : J5775-04
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 02:26:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

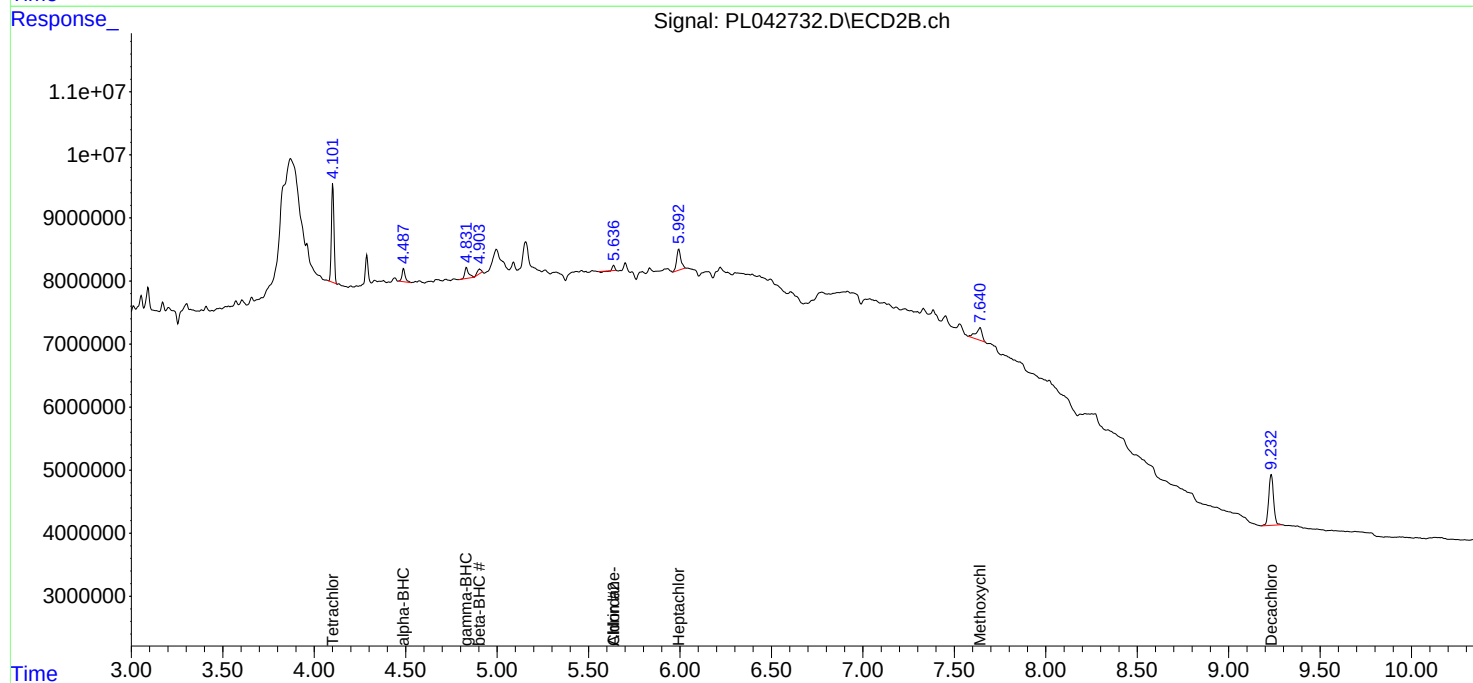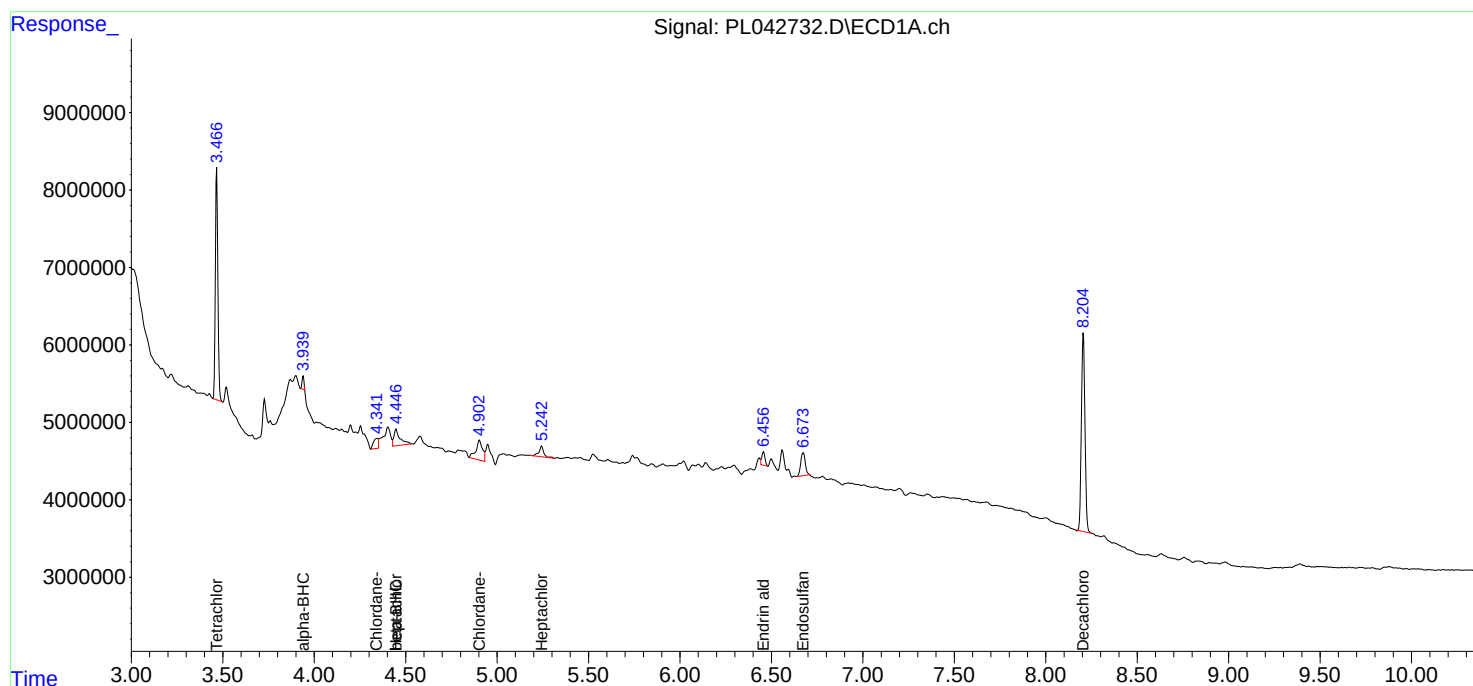


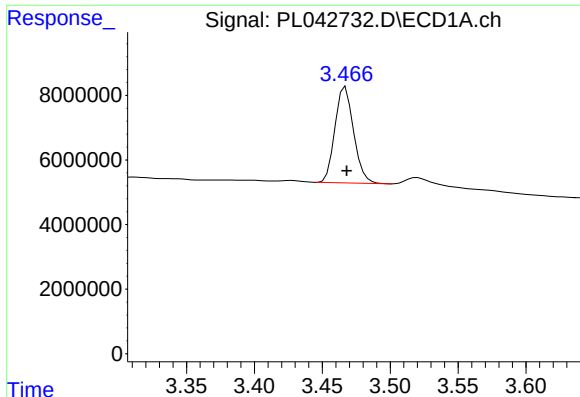

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 28490796
Conc: 4.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

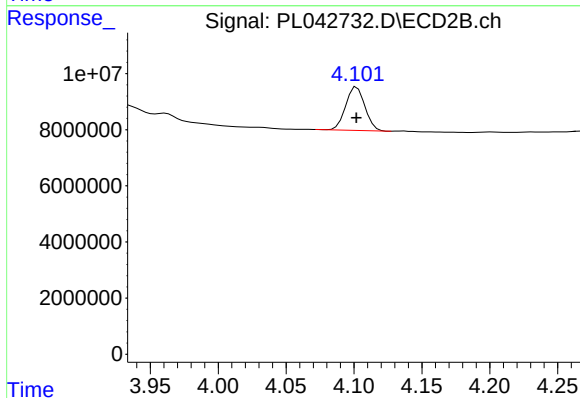


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 15274528
Conc: 5.31 ng/ml

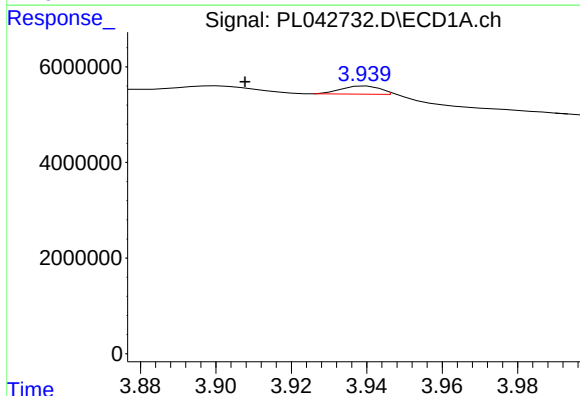


#2 alpha-BHC

R.T.: 3.940 min
Delta R.T.: 0.032 min
Response: 1127442
Conc: 0.12 ng/ml

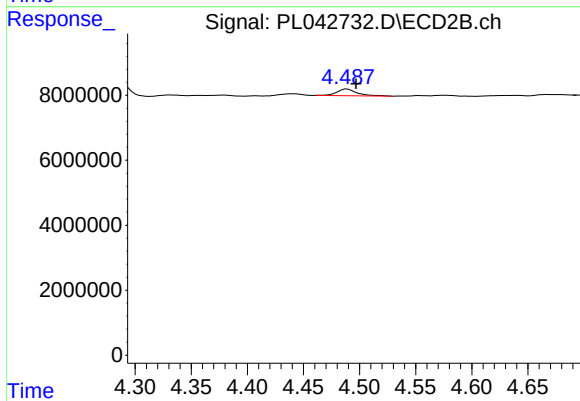

#2 alpha-BHC


R.T.: 4.489 min
Delta R.T.: -0.008 min
Response: 2513653
Conc: 0.59 ng/ml

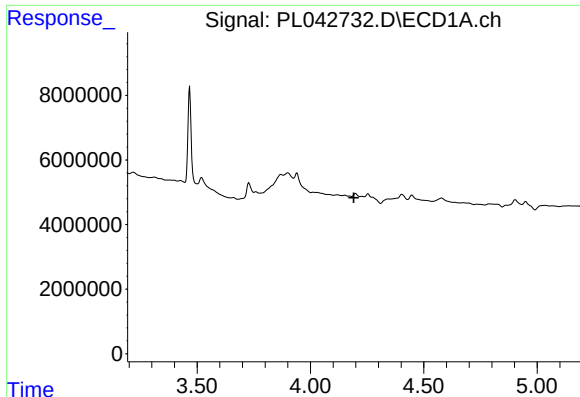

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

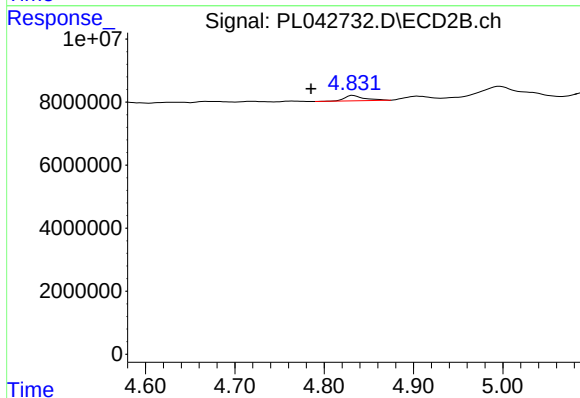


#3 gamma-BHC (Lindane)

R.T.: 4.832 min
Delta R.T.: 0.047 min
Response: 2570941
Conc: 0.65 ng/ml

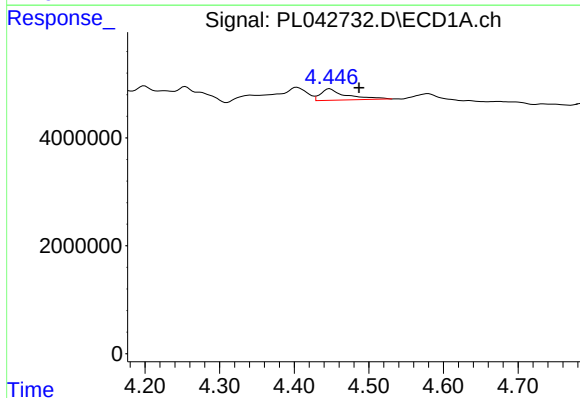


#4 Heptachlor

R.T.: 4.447 min
Delta R.T.: -0.039 min
Response: 4903173
Conc: 0.56 ng/ml

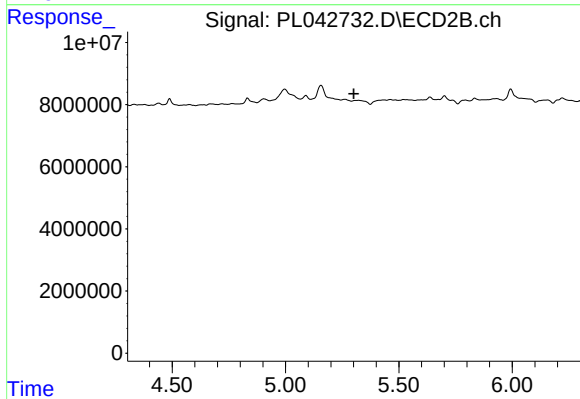

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.301 min
Response: 0
Conc: N.D.

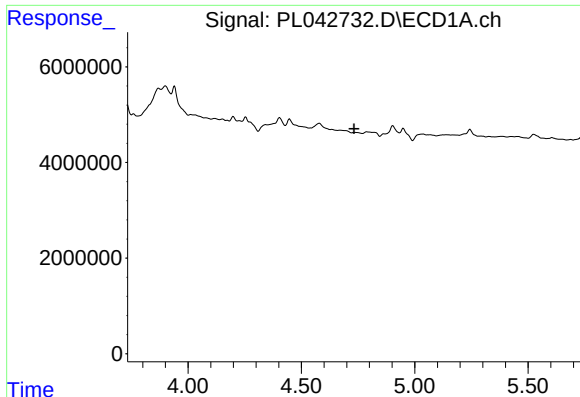

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.733 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

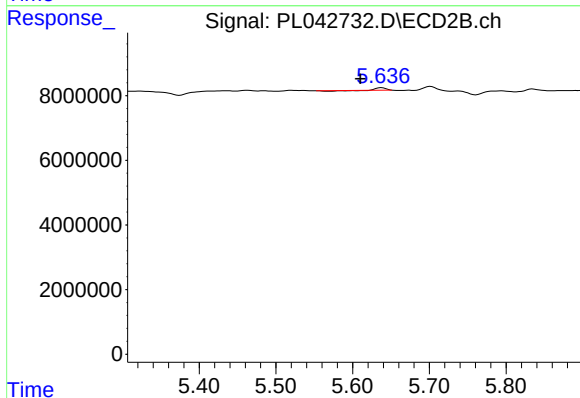


#5 Aldrin

R.T.: 5.638 min
Delta R.T.: 0.028 min
Response: 479834
Conc: 0.12 ng/ml

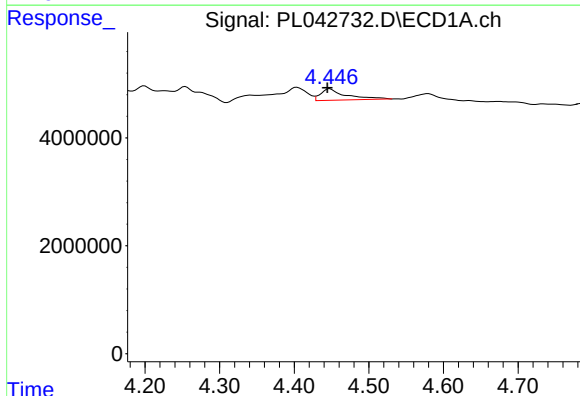


#6 beta-BHC

R.T.: 4.447 min
Delta R.T.: 0.003 min
Response: 4903173
Conc: 1.38 ng/ml

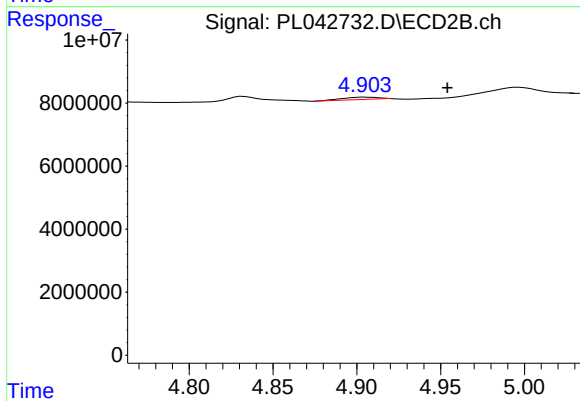

#6 beta-BHC


R.T.: 4.905 min
Delta R.T.: -0.049 min
Response: 1164443
Conc: 0.74 ng/ml

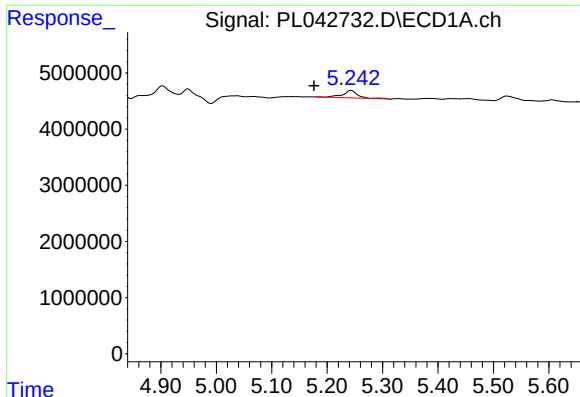

#8 Heptachlor epoxide


R.T.: 5.244 min
Delta R.T.: 0.067 min
Response: 2586805
Conc: 0.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

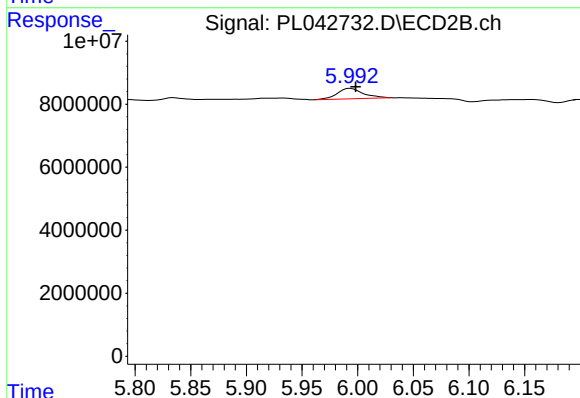


#8 Heptachlor epoxide

R.T.: 5.994 min
Delta R.T.: -0.005 min
Response: 5465888
Conc: 1.52 ng/ml

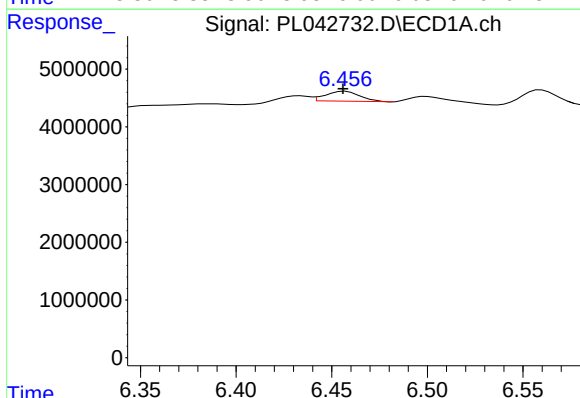


#18 Endrin aldehyde

R.T.: 6.457 min
Delta R.T.: 0.001 min
Response: 2142922
Conc: 0.41 ng/ml

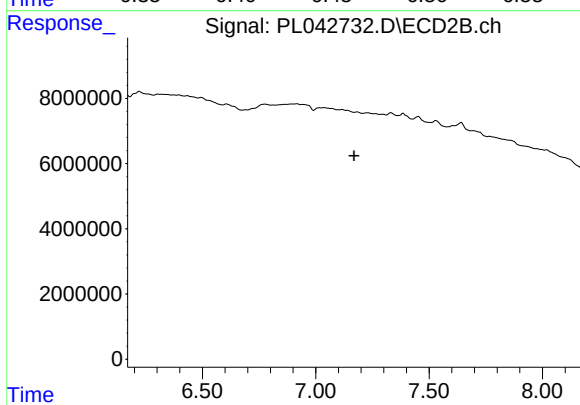

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 7.169 min
Response: 0
Conc: N.D.

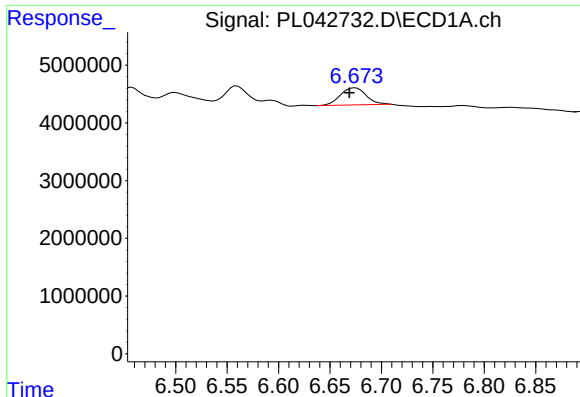

#19 Endosulfan Sulfate


R.T.: 6.675 min
Delta R.T.: 0.006 min
Response: 5072204
Conc: 0.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

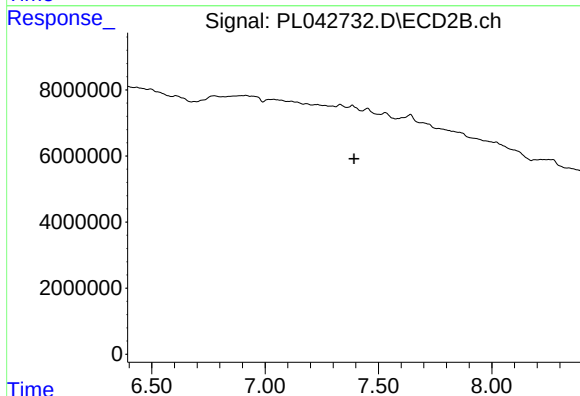


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

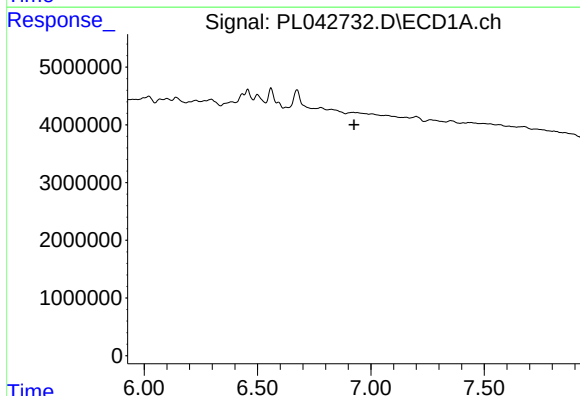


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.926 min
Response: 0
Conc: N.D.

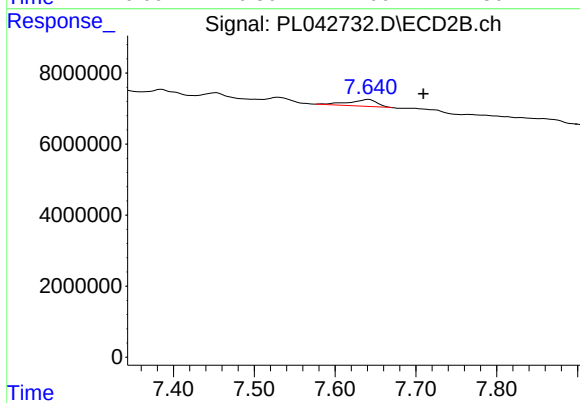

#20 Methoxychlor


R.T.: 7.642 min
Delta R.T.: -0.067 min
Response: 4450501
Conc: 3.26 ng/ml

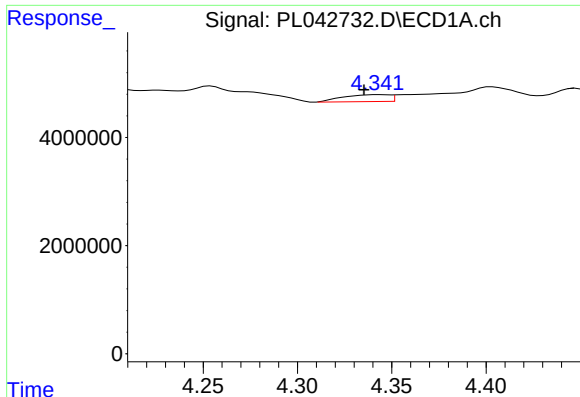

#23 Chlordane-1


R.T.: 4.342 min
Delta R.T.: 0.007 min
Response: 2203237
Conc: 7.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

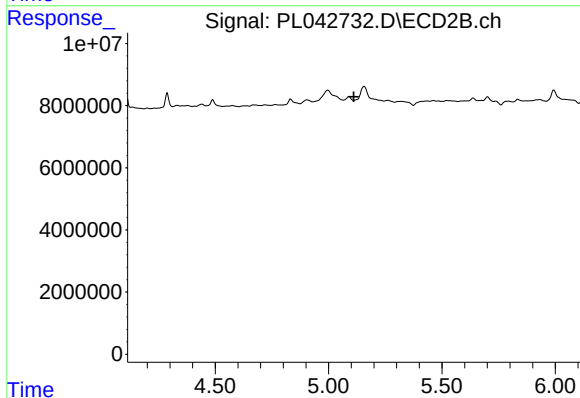


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

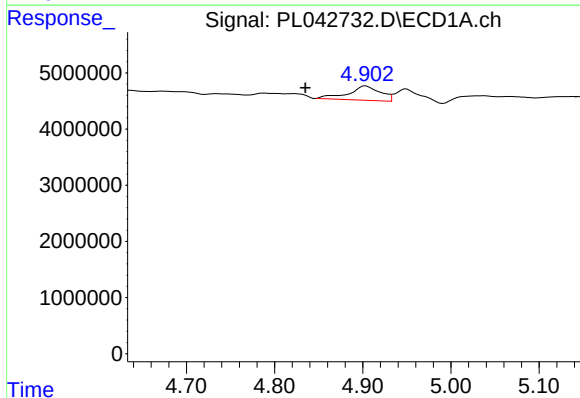


#24 Chlordane-2

R.T.: 4.903 min
Delta R.T.: 0.068 min
Response: 6485550
Conc: 23.08 ng/ml

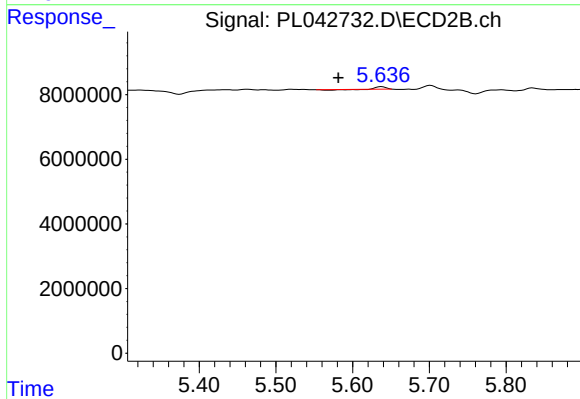

#24 Chlordane-2


R.T.: 5.638 min
Delta R.T.: 0.056 min
Response: 479834
Conc: 3.44 ng/ml

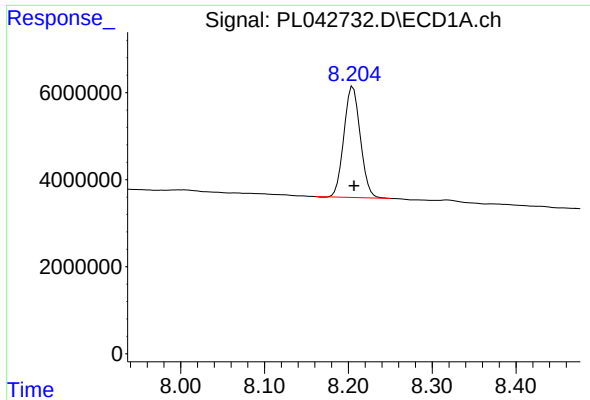

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.002 min
Response: 34748548
Conc: 5.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

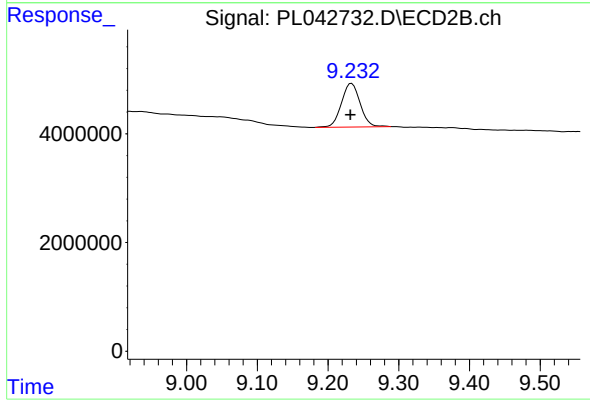

#28 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: 0.002 min
Response: 14810674
Conc: 6.14 ng/ml