

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120318\
 Data File : PL042764.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2018 09:31
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 12:02:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.102	117.4E6	61813769	19.952	21.492
28)	SA Decachlor...	8.204	9.231	126.9E6	52874230	20.134	21.923
Target Compounds							
2)	A alpha-BHC	3.903	0.000	4308770	0	0.478	N.D. #
6)	B beta-BHC	4.400f	4.906f	3928499	2223445	1.109	1.409 #
8)	B Heptachlo...	0.000	5.997	0	4640185	N.D.	1.294 #
13)	MA Dieldrin	5.698f	0.000	560276	0	0.076	N.D. #
14)	MA Endrin	6.019	0.000	2297964	0	0.351	N.D. #
23)	Chlordane-1	4.400	0.000	3928499	0	14.209	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120318\
Data File : PL042764.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2018 09:31
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 12:02:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

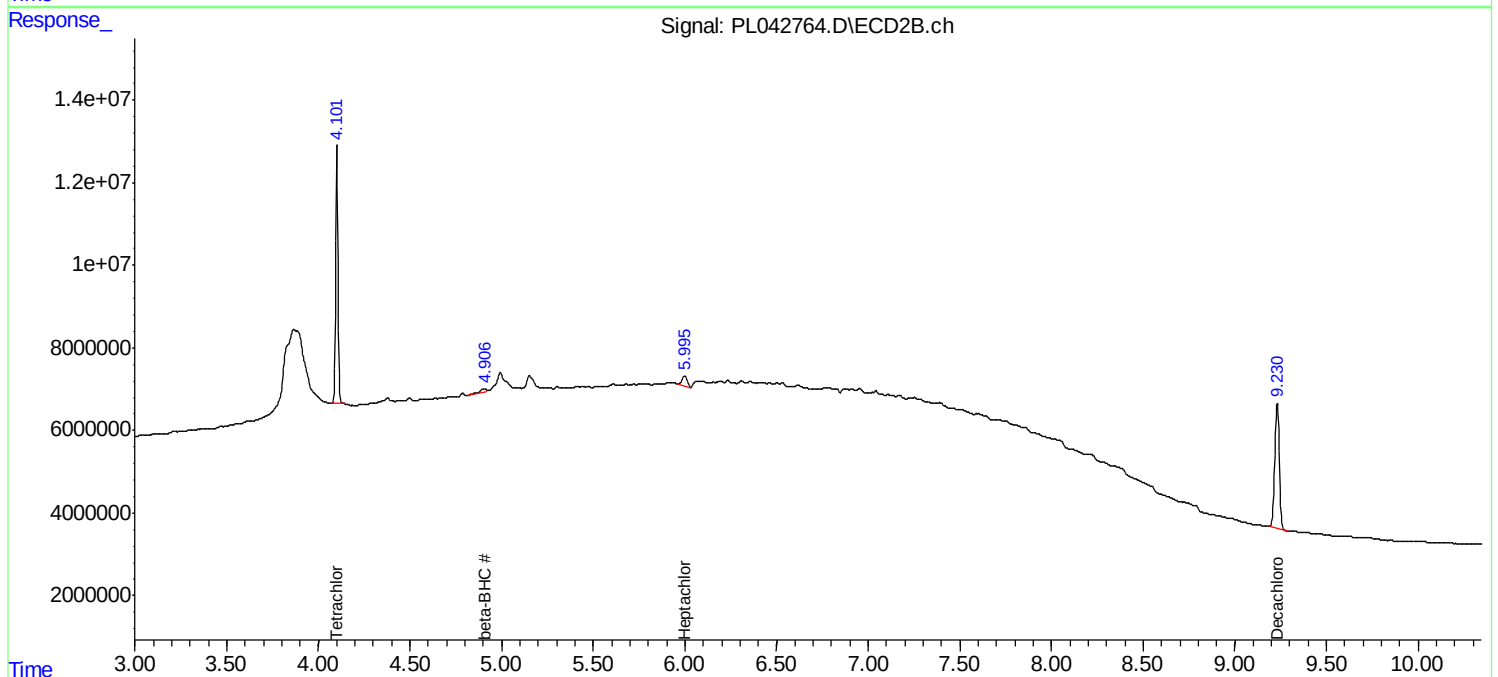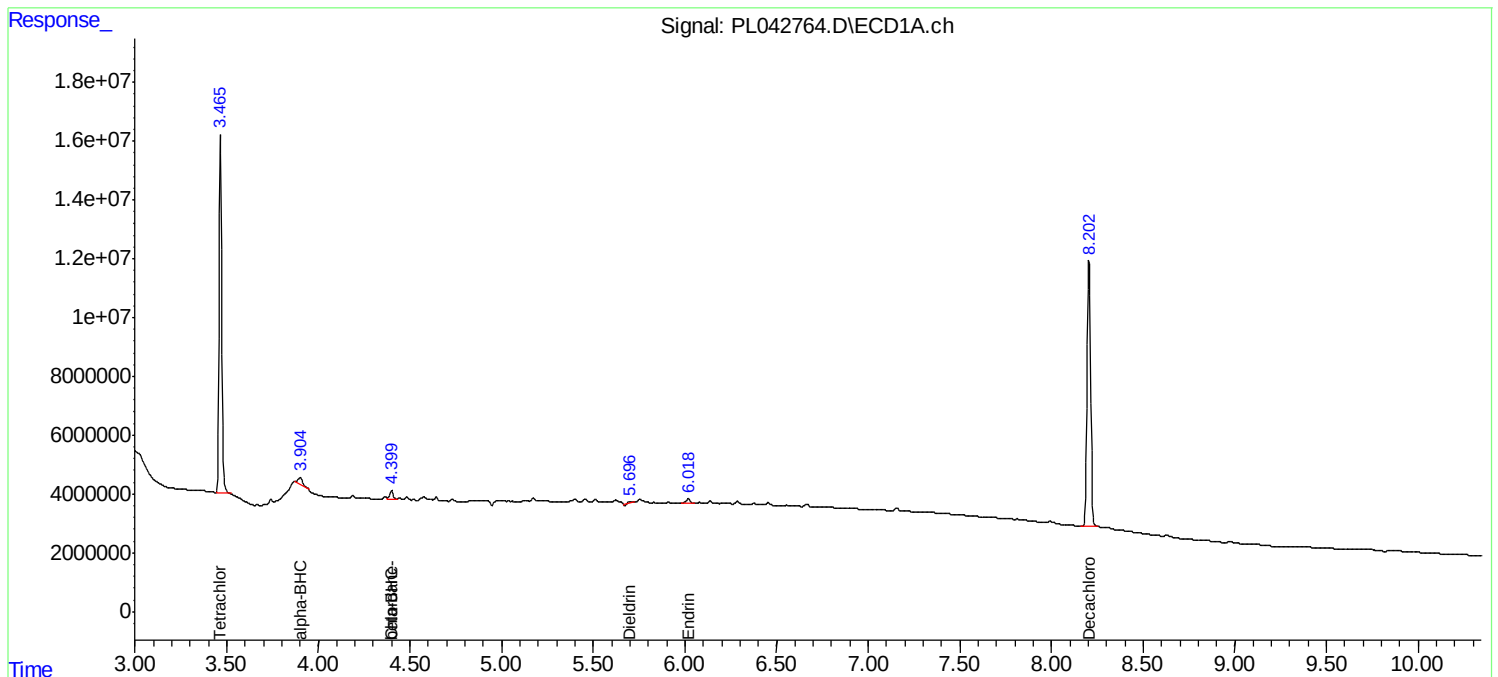


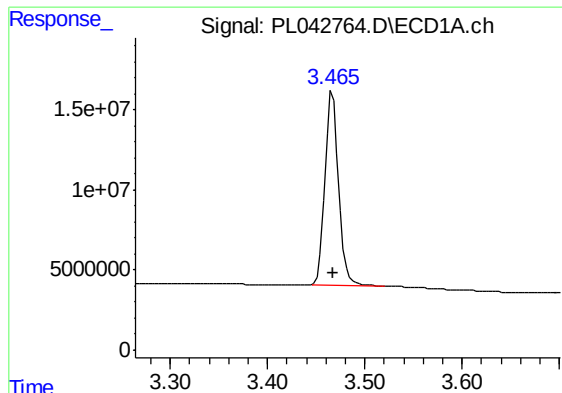

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: -0.001 min
Response: 117387102
Conc: 19.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

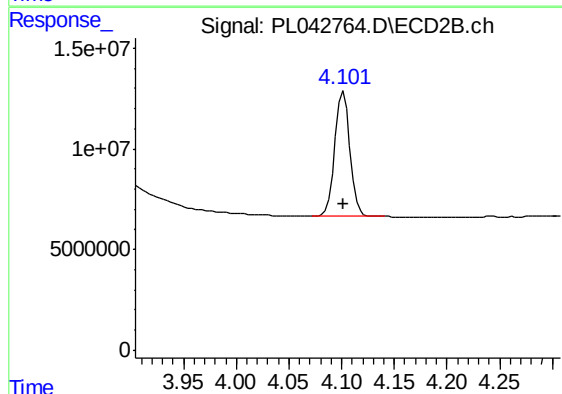


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 61813769
Conc: 21.49 ng/ml

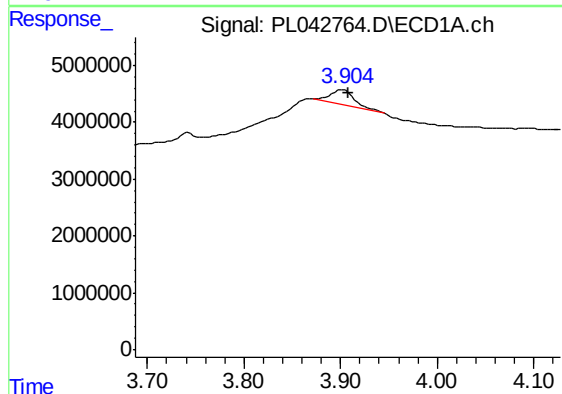


#2 alpha-BHC

R.T.: 3.903 min
Delta R.T.: -0.005 min
Response: 4308770
Conc: 0.48 ng/ml

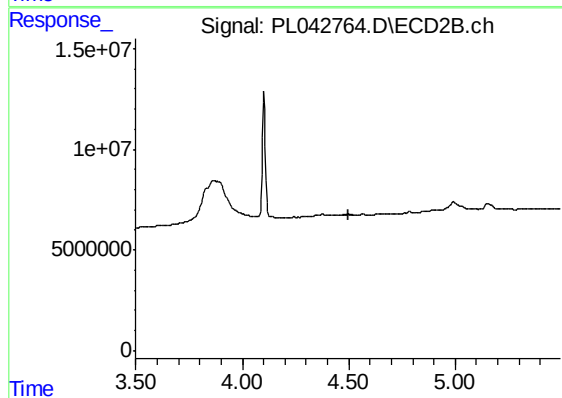

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.497 min
Response: 0
Conc: N.D.

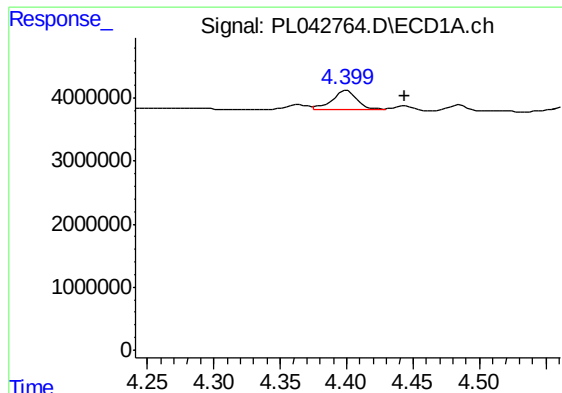

#6 beta-BHC


R.T.: 4.400 min
Delta R.T.: -0.044 min
Response: 3928499
Conc: 1.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

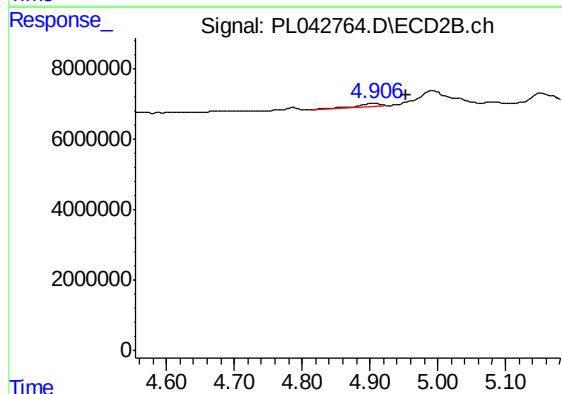


#6 beta-BHC

R.T.: 4.906 min
Delta R.T.: -0.048 min
Response: 2223445
Conc: 1.41 ng/ml

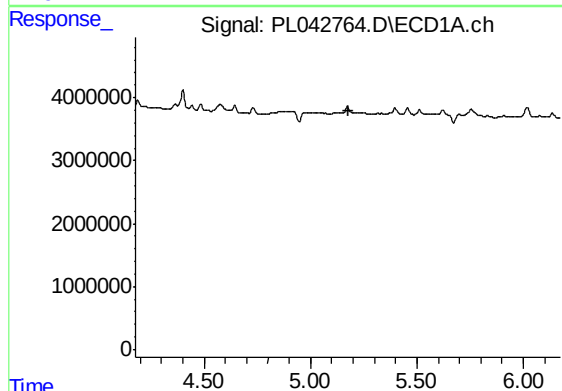


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.177 min
Response: 0
Conc: N.D.

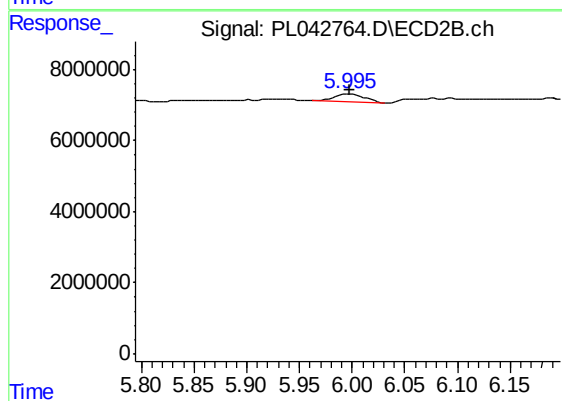

#8 Heptachlor epoxide


R.T.: 5.997 min
Delta R.T.: -0.002 min
Response: 4640185
Conc: 1.29 ng/ml

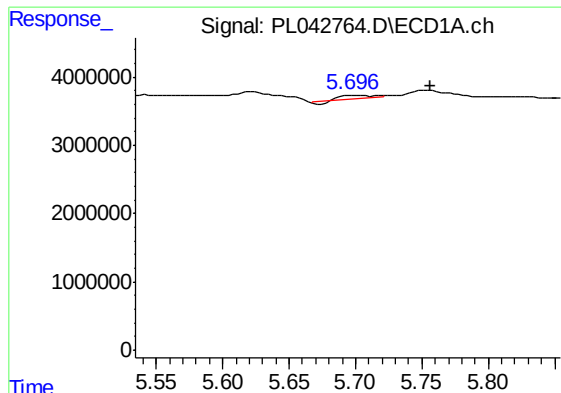

#13 Dielddrin


R.T.: 5.698 min
Delta R.T.: -0.058 min
Response: 560276
Conc: 0.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

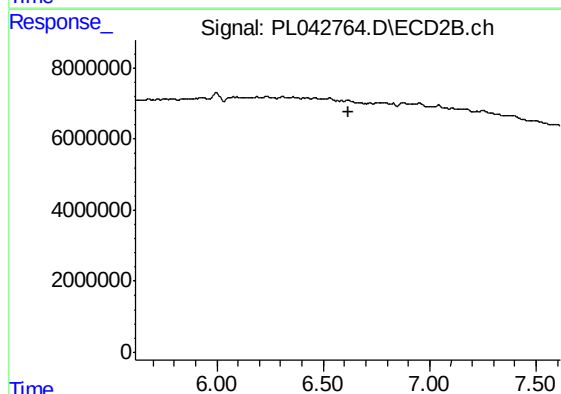


#13 Dielddrin

R.T.: 0.000 min
Exp R.T. : 6.617 min
Response: 0
Conc: N.D.

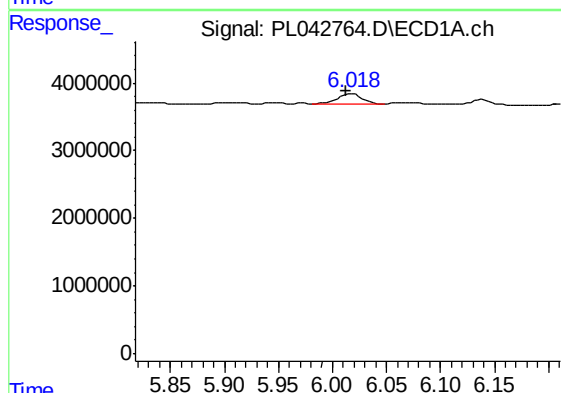


#14 Endrin

R.T.: 6.019 min
Delta R.T.: 0.006 min
Response: 2297964
Conc: 0.35 ng/ml

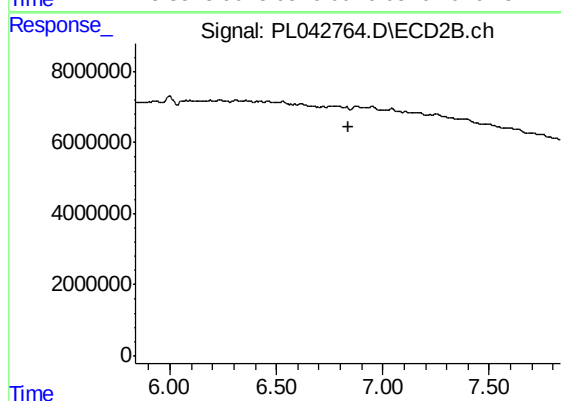

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.836 min
Response: 0
Conc: N.D.

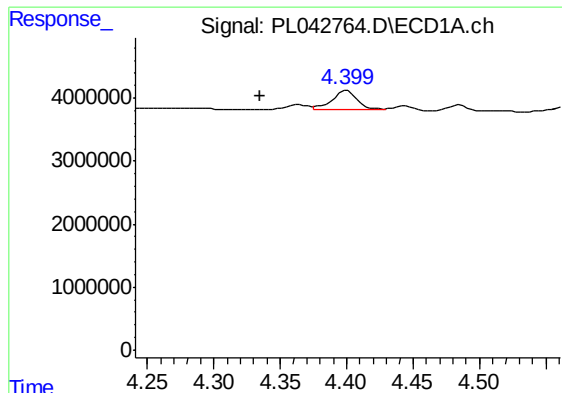

#23 Chlordane-1


R.T.: 4.400 min
Delta R.T.: 0.065 min
Response: 3928499
Conc: 14.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

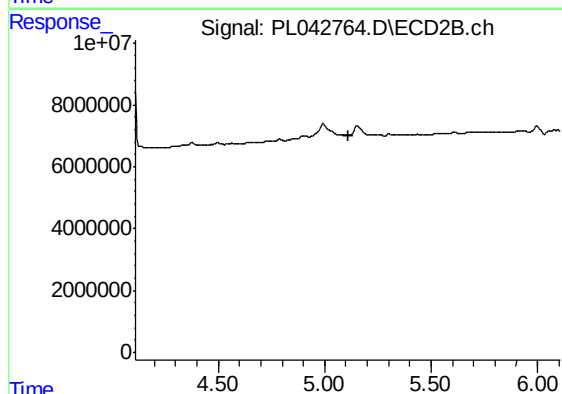


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

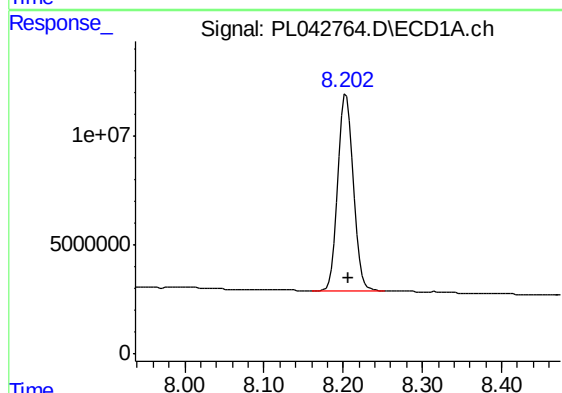

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.003 min
Response: 126886790
Conc: 20.13 ng/ml

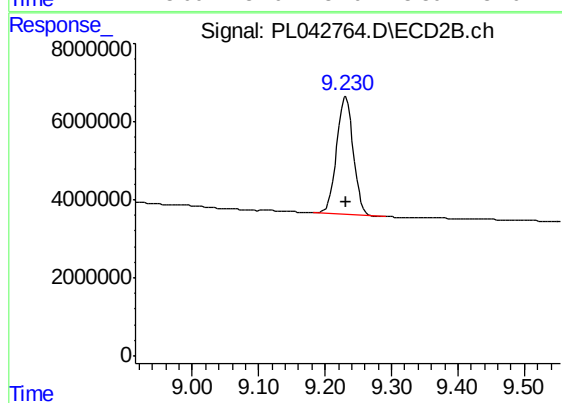

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.000 min
Response: 52874230
Conc: 21.92 ng/ml