

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120320\
 Data File : PL063321.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2020 11:30
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 05:18:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 24 01:53:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) B	Heptachlo...	0.000	5.806	0	132.5E6	N.D. 38.029 #
9) A	Endosulfan I	0.000	6.154	0	13189577	N.D. 3.907 #
14) MA	Endrin	5.931	0.000	14451474	0	8.605 N.D. #
17) MA	4,4'-DDT	0.000	7.060	0	16714789	N.D. 6.545 #
18) B	Endrin al...	6.376	0.000	8407606	0	5.642 N.D. #
20) A	Methoxychlor	6.840	0.000	7837861	0	9.148 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120320\
Data File : PL063321.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2020 11:30
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 05:18:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
Quant Title : GC Extractables
QLast Update : Tue Nov 24 01:53:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

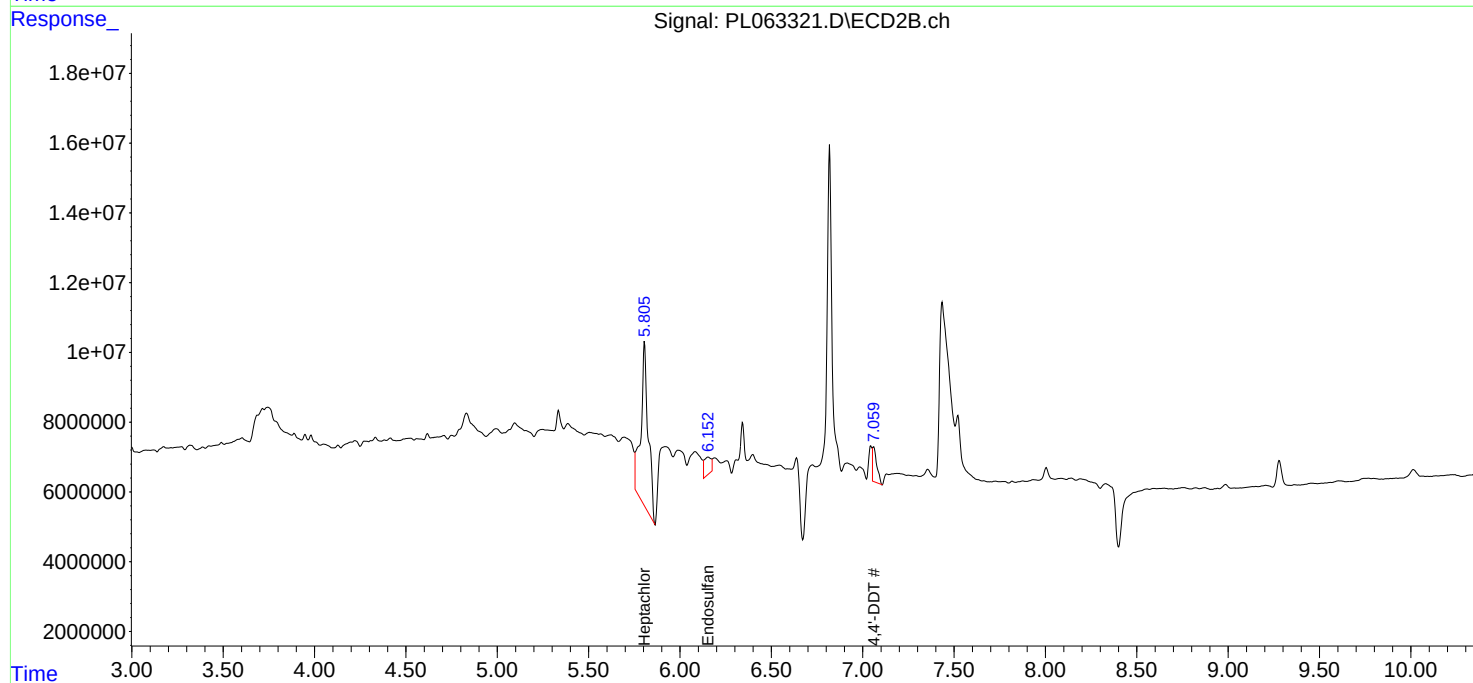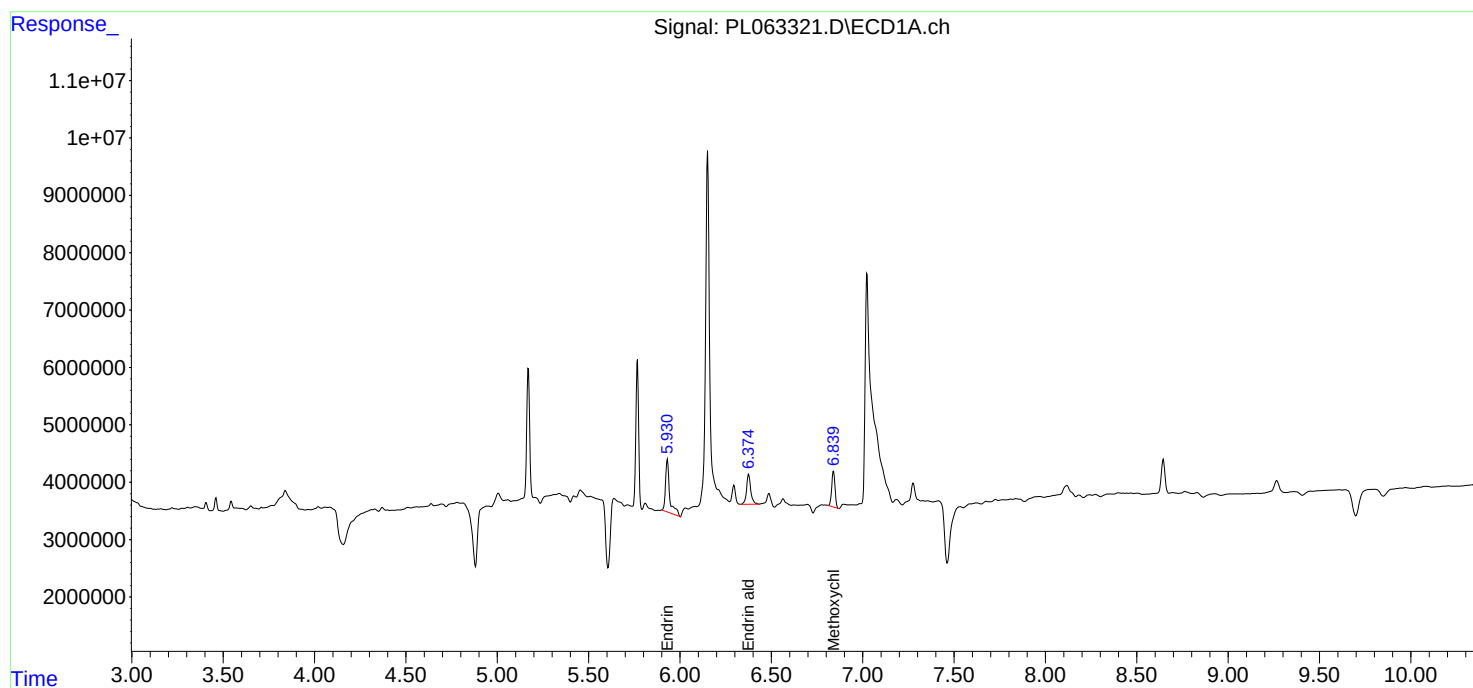


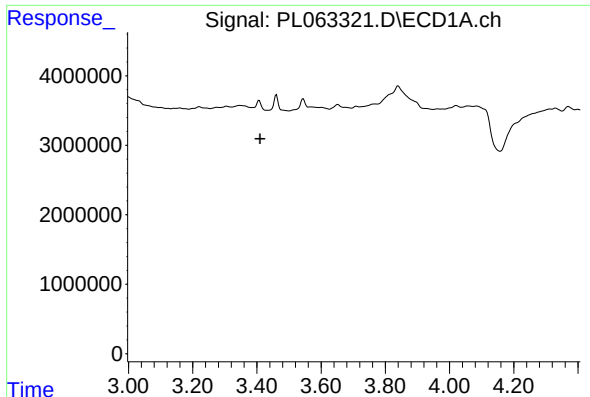

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.410 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

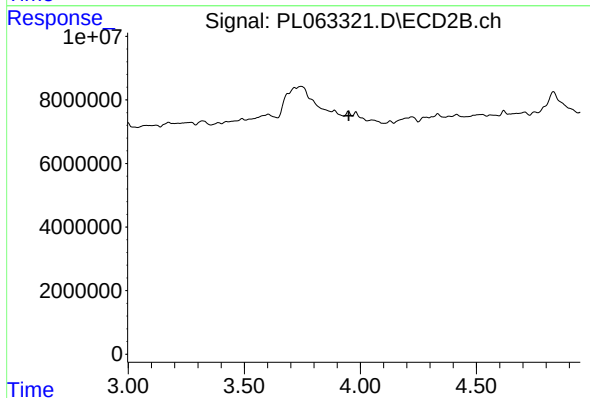


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.950 min
Response: 0
Conc: N.D.

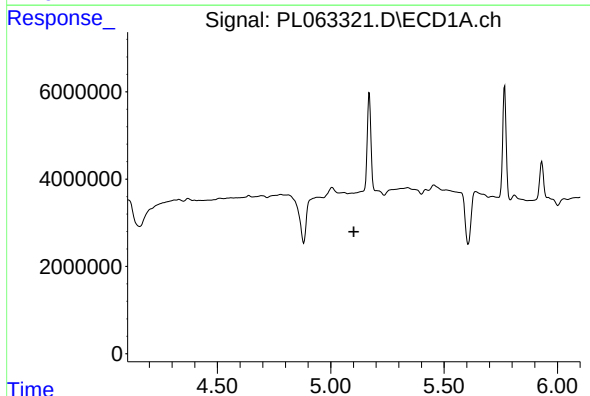


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.101 min
Response: 0
Conc: N.D.

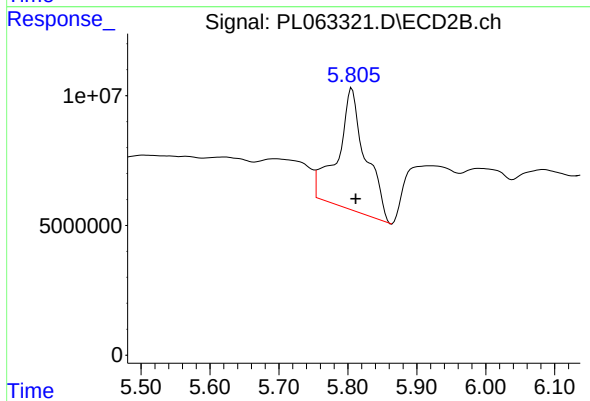

#8 Heptachlor epoxide


R.T.: 5.806 min
Delta R.T.: -0.006 min
Response: 132472329
Conc: 38.03 ng/ml

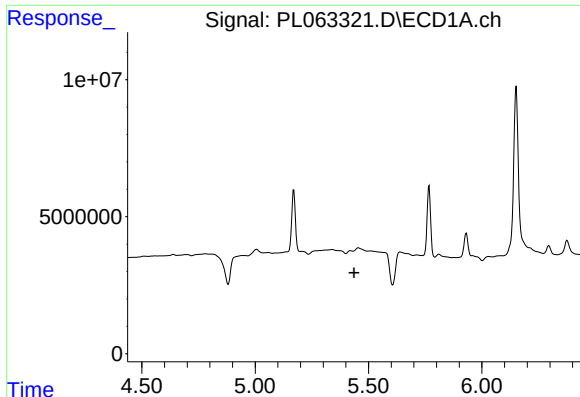

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.437 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

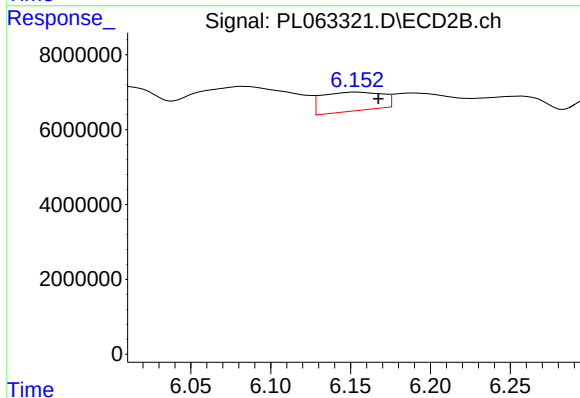


#9 Endosulfan I

R.T.: 6.154 min
Delta R.T.: -0.014 min
Response: 13189577
Conc: 3.91 ng/ml

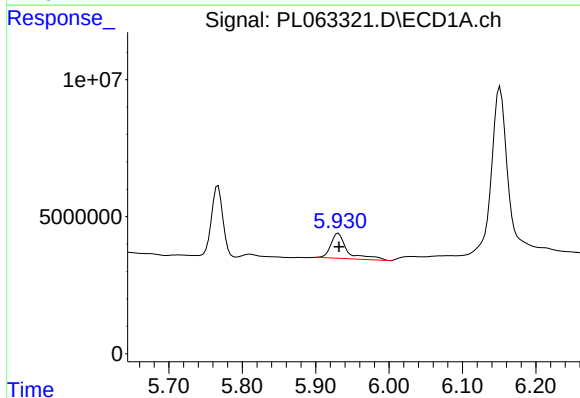


#14 Endrin

R.T.: 5.931 min
Delta R.T.: -0.001 min
Response: 14451474
Conc: 8.61 ng/ml

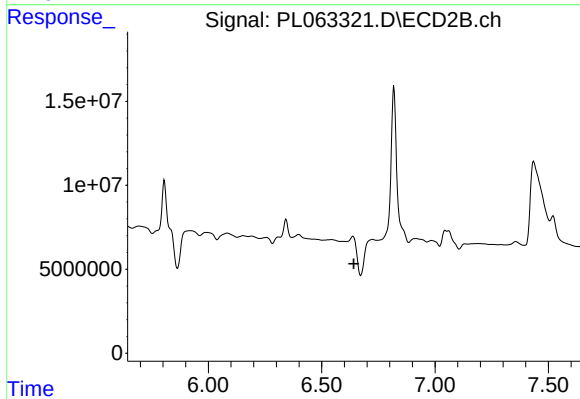

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.642 min
Response: 0
Conc: N.D.

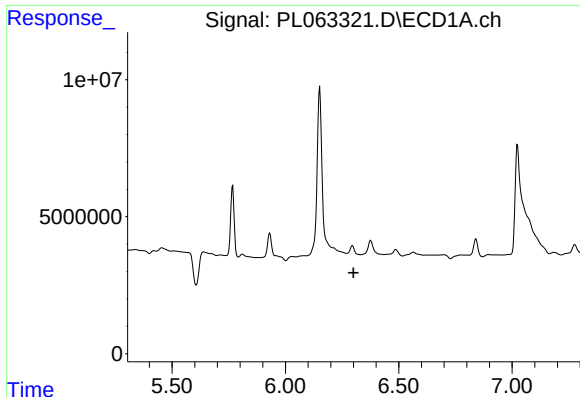

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.301 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

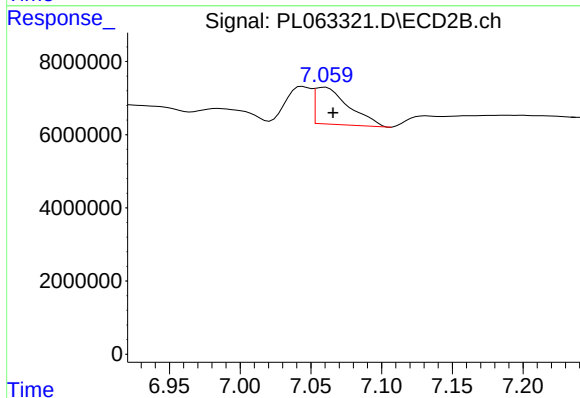


#17 4,4'-DDT

R.T.: 7.060 min
Delta R.T.: -0.006 min
Response: 16714789
Conc: 6.55 ng/ml

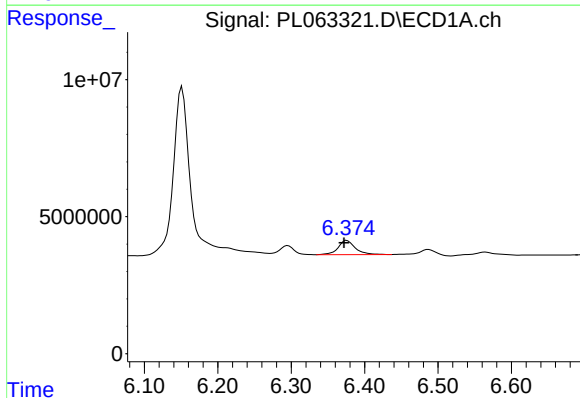


#18 Endrin aldehyde

R.T.: 6.376 min
Delta R.T.: 0.004 min
Response: 8407606
Conc: 5.64 ng/ml

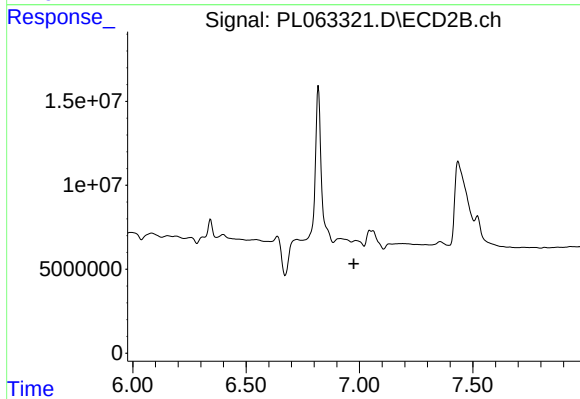

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.976 min
Response: 0
Conc: N.D.

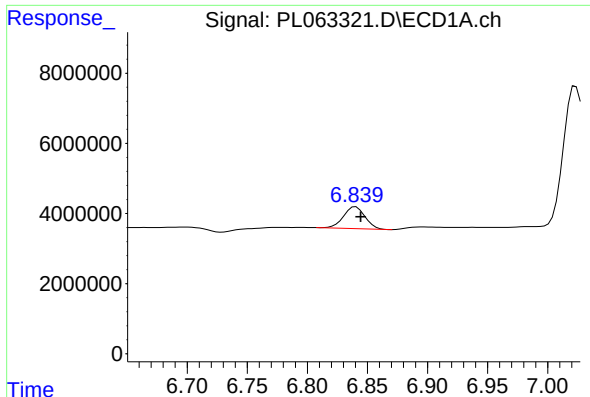

#20 Methoxychlor


R.T.: 6.840 min
Delta R.T.: -0.004 min
Response: 7837861
Conc: 9.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

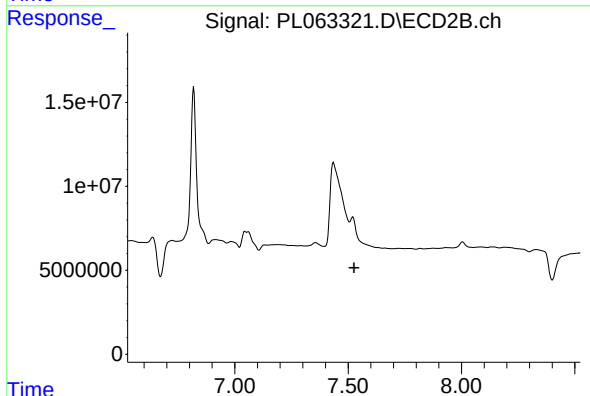


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.526 min
Response: 0
Conc: N.D.

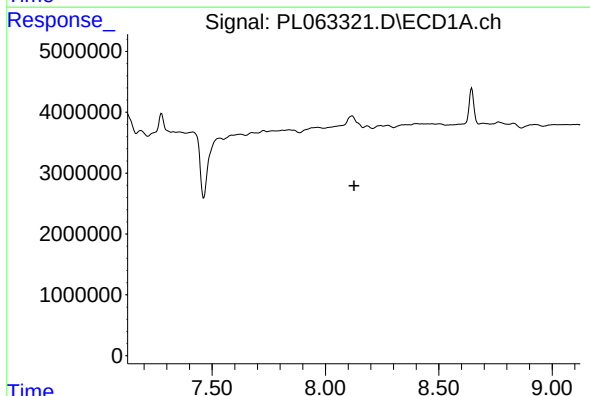

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.126 min
Response: 0
Conc: N.D.

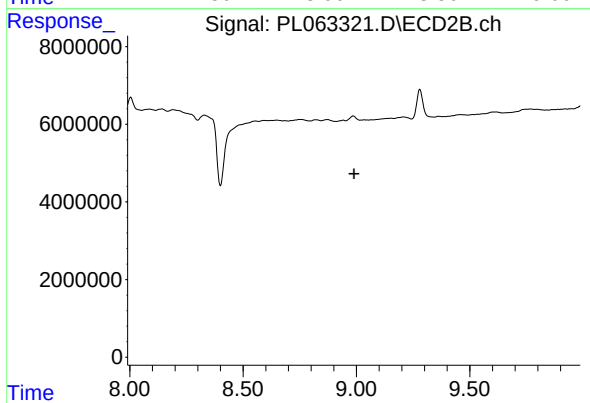

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.990 min
Response: 0
Conc: N.D.