

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120320\
 Data File : PL063327.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2020 13:06
 Operator : DD\AJ
 Sample : PB133367BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 05:19:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 24 01:53:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.950	33115883	63486861	19.445	19.452
28)	SA Decachlor...	8.125	8.990	36794513	46279303	19.703	19.451
Target Compounds							
17)	MA 4,4'-DDT	0.000	7.038f	0	12110932	N.D.	4.742 #
22)	Mirex	0.000	8.142f	0	10033076	N.D.	5.136 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120320\
Data File : PL063327.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2020 13:06
Operator : DD\AJ
Sample : PB133367BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 05:19:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
Quant Title : GC Extractables
QLast Update : Tue Nov 24 01:53:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

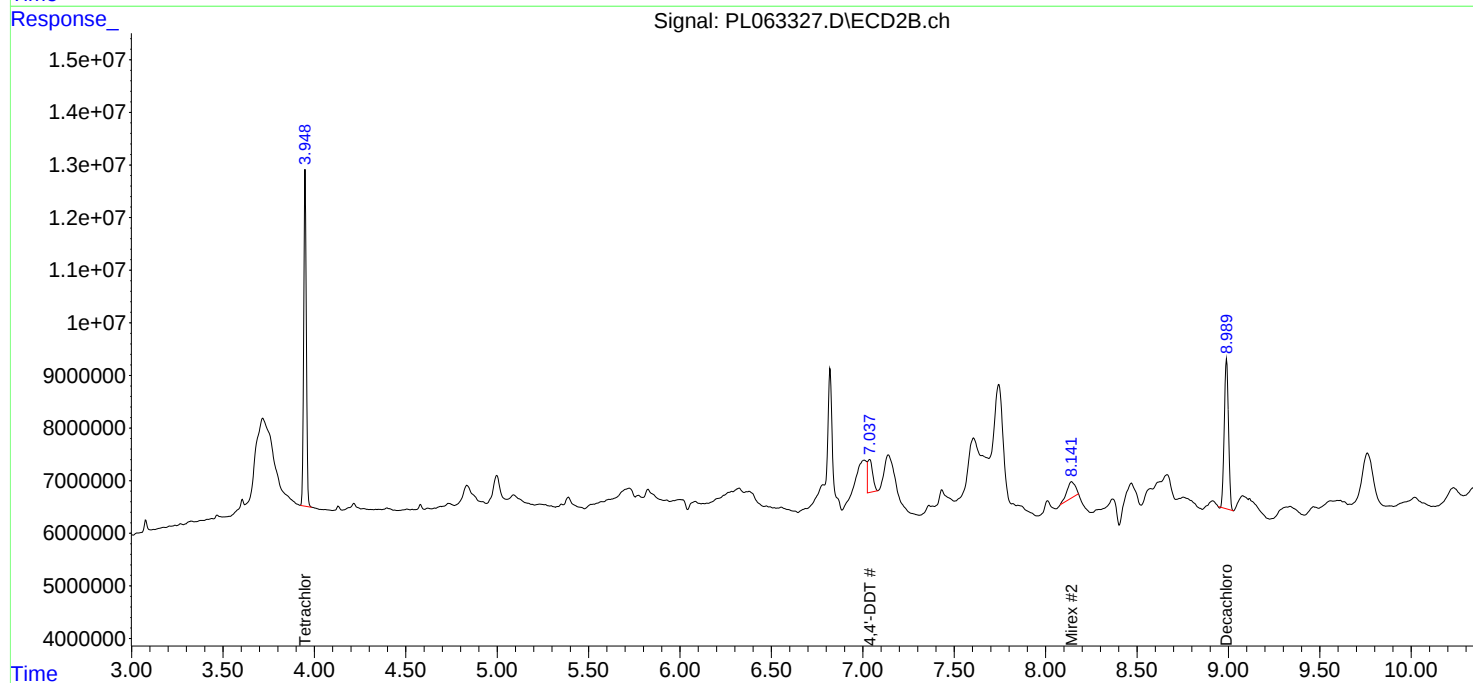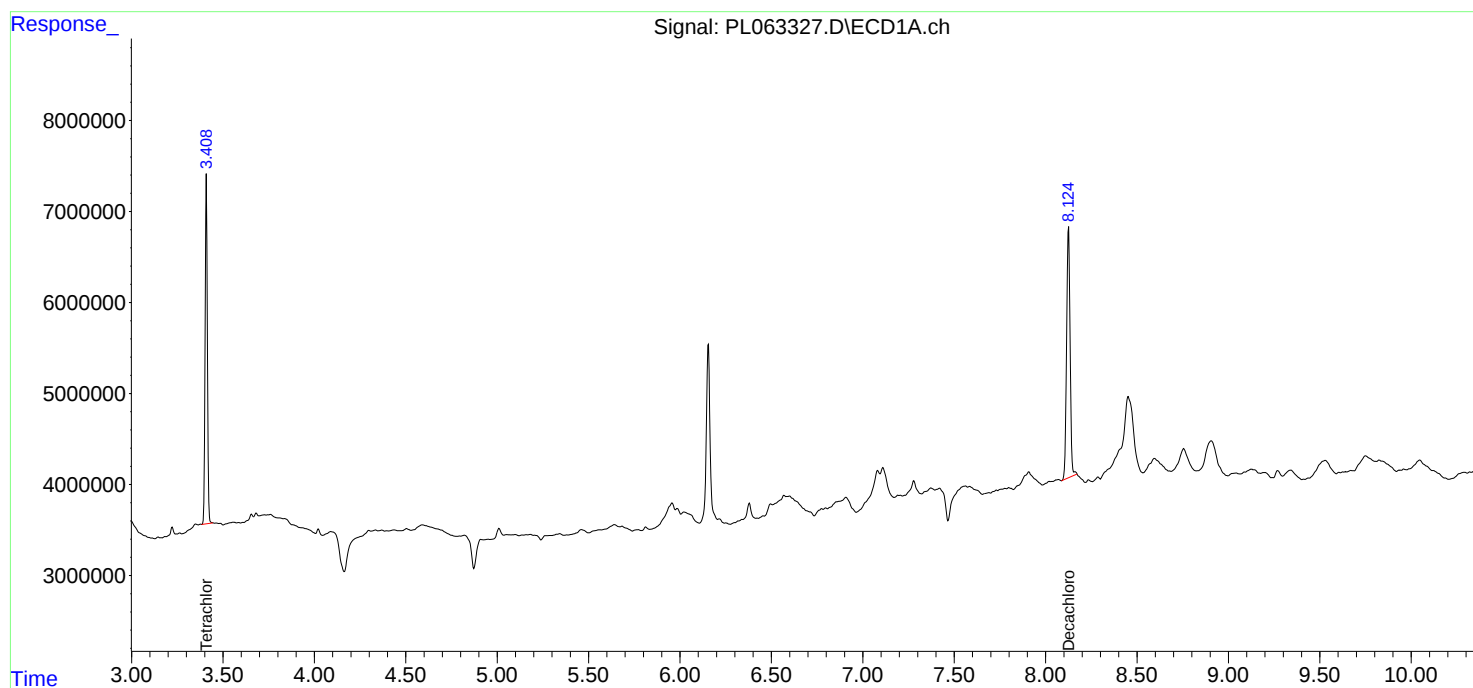


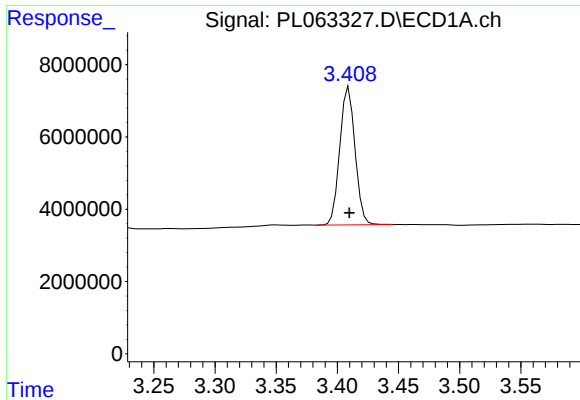

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 33115883
Conc: 19.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

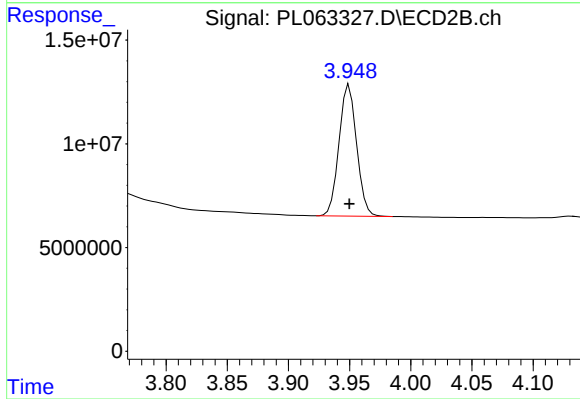


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 63486861
Conc: 19.45 ng/ml

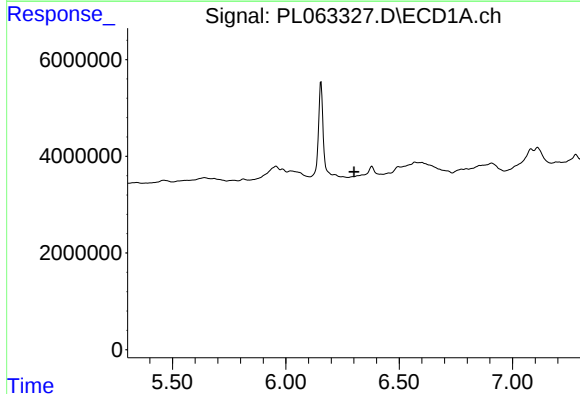


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.301 min
Response: 0
Conc: N.D.

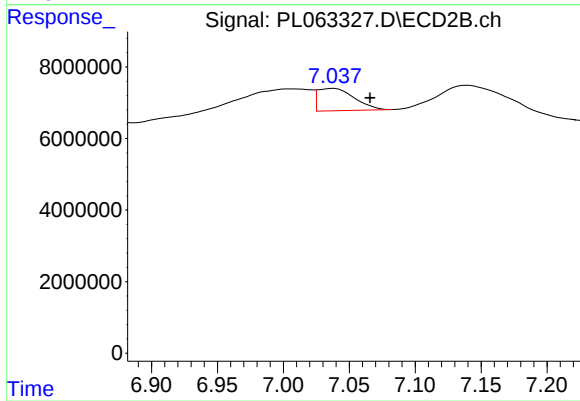

#17 4,4'-DDT


R.T.: 7.038 min
Delta R.T.: -0.027 min
Response: 12110932
Conc: 4.74 ng/ml

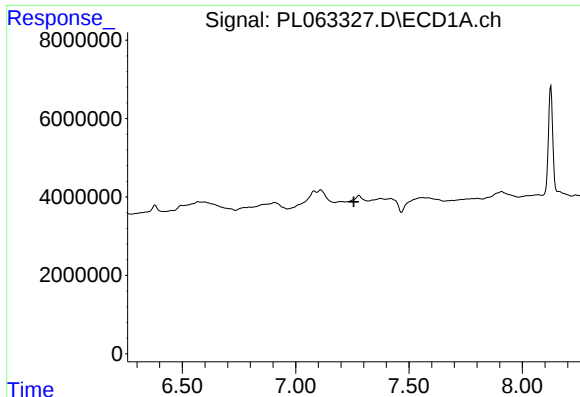

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.257 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

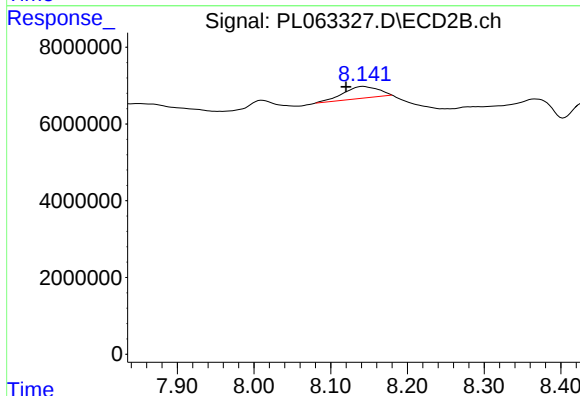


#22 Mirex

R.T.: 8.142 min
Delta R.T.: 0.022 min
Response: 10033076
Conc: 5.14 ng/ml

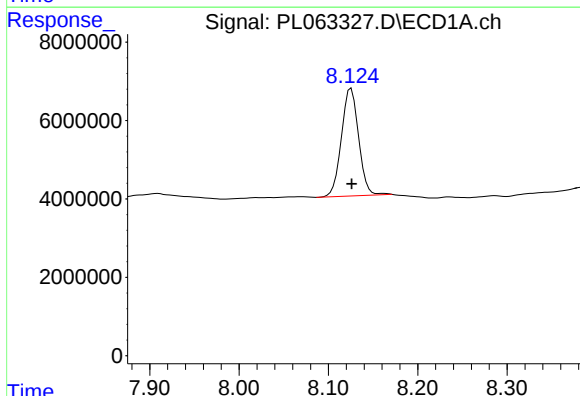

#28 Decachlorobiphenyl

R.T.: 8.125 min
Delta R.T.: 0.000 min
Response: 36794513
Conc: 19.70 ng/ml

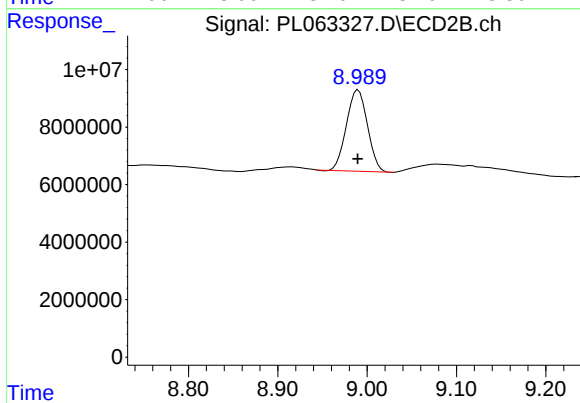

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.000 min
Response: 46279303
Conc: 19.45 ng/ml