

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120321\
 Data File : PL071253.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2021 08:37
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 00:31:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
6) B	beta-BHC	0.000	6.762f	0	259289	N.D. 0.295 #
7) B	delta-BHC	0.000	7.028f	0	668455	N.D. 0.393 #
8) B	Heptachlo...	7.032f	7.975	7084174	14197702	11.366 8.937
11) B	alpha-Chl...	0.000	8.336f	0	3002635	N.D. 1.889 #
12) B	4,4'-DDE	7.574	0.000	355330	0	0.628 N.D. #
20) A	Methoxychlor	9.008	0.000	322703	0	0.893 N.D. #
21) B	Endrin ke...	9.207f	0.000	17571533	0	24.656 N.D. #
22)	Mirex	0.000	10.460	0	840196	N.D. 0.770 #
23)	Chlordane-1	5.866f	0.000	54699	0	3.253 N.D. #
26)	Chlordane-4	0.000	8.336f	0	3002635	N.D. 11.316 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120321\
Data File : PL071253.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2021 08:37
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 00:31:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

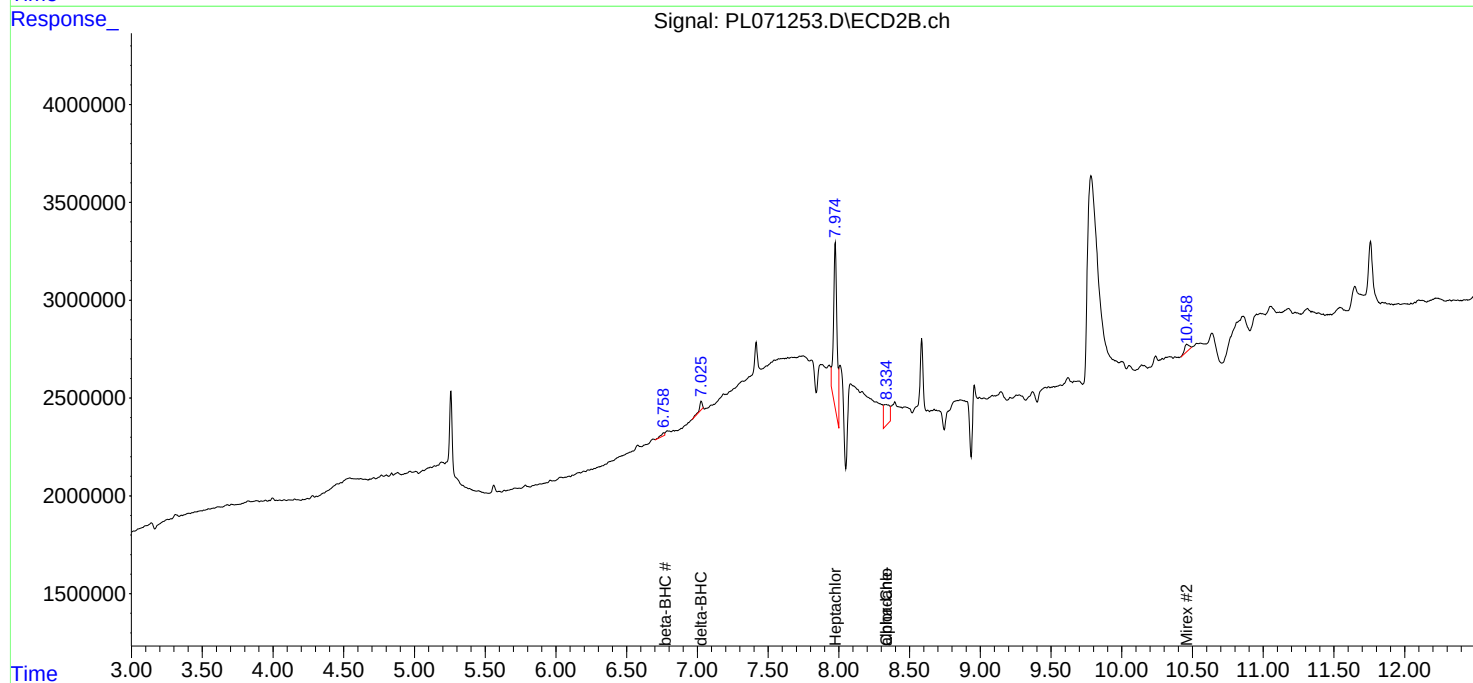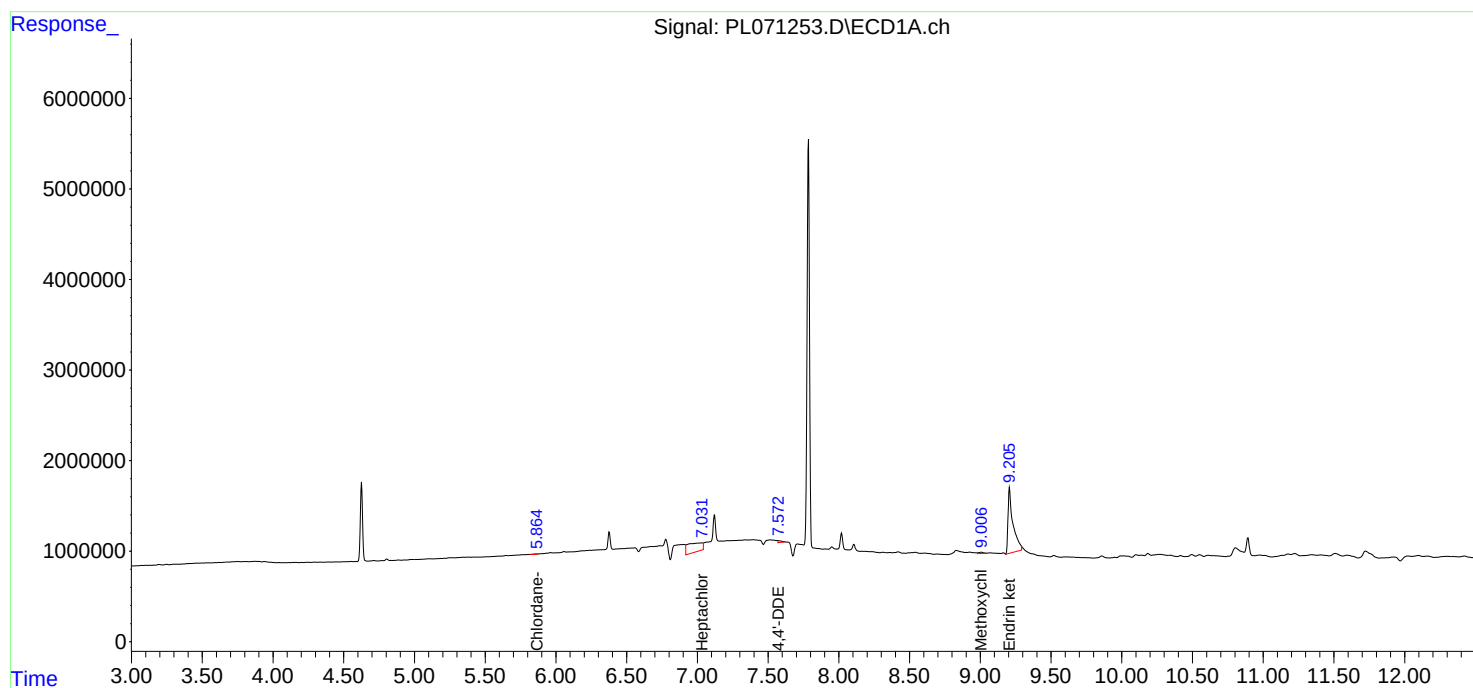


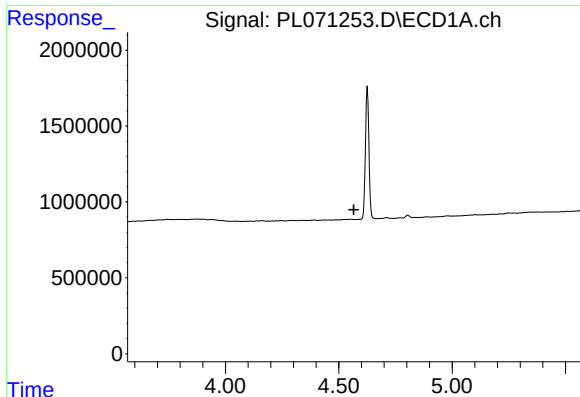

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

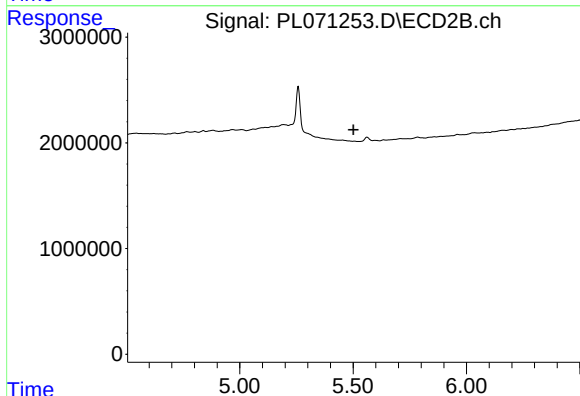


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.502 min
Response: 0
Conc: N.D.

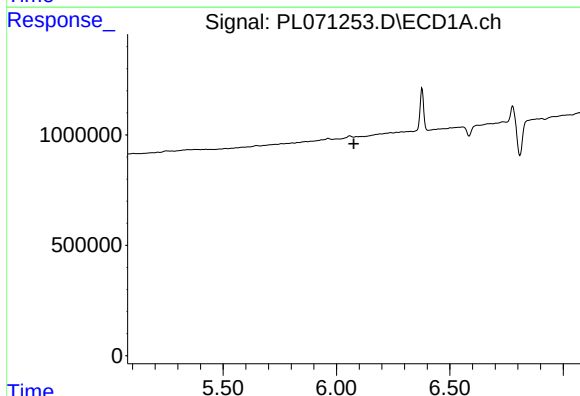


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.076 min
Response: 0
Conc: N.D.

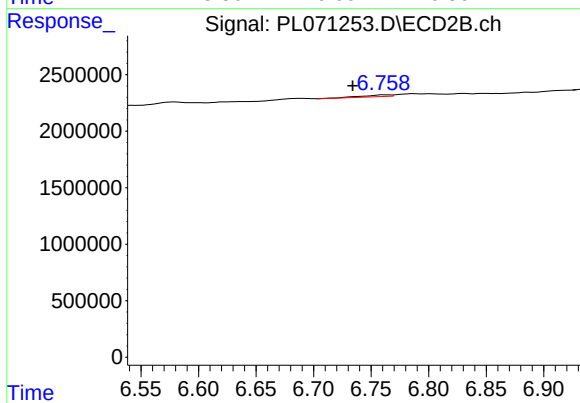

#6 beta-BHC


R.T.: 6.762 min
Delta R.T.: 0.028 min
Response: 259289
Conc: 0.29 ng/ml

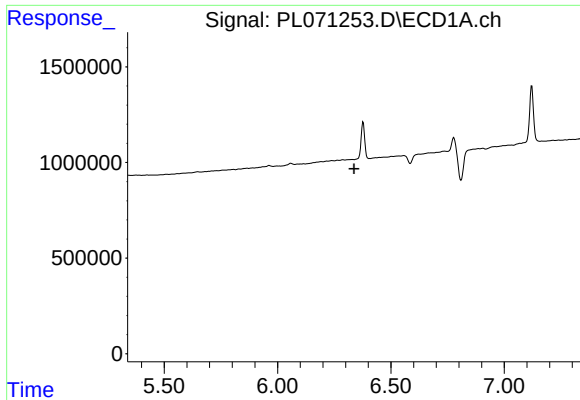

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.337 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

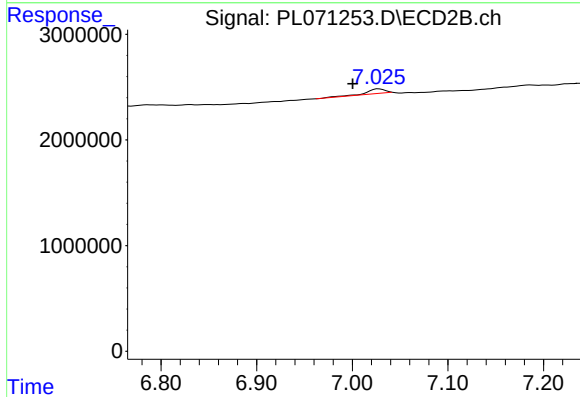


#7 delta-BHC

R.T.: 7.028 min
Delta R.T.: 0.027 min
Response: 668455
Conc: 0.39 ng/ml

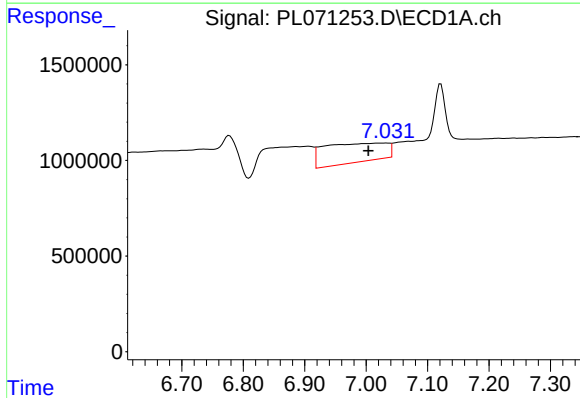


#8 Heptachlor epoxide

R.T.: 7.032 min
Delta R.T.: 0.029 min
Response: 7084174
Conc: 11.37 ng/ml

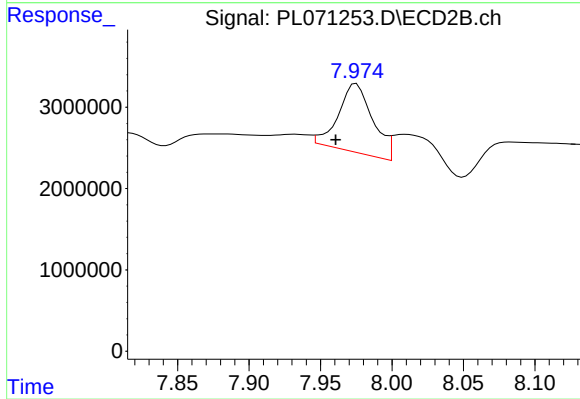

#8 Heptachlor epoxide


R.T.: 7.975 min
Delta R.T.: 0.014 min
Response: 14197702
Conc: 8.94 ng/ml

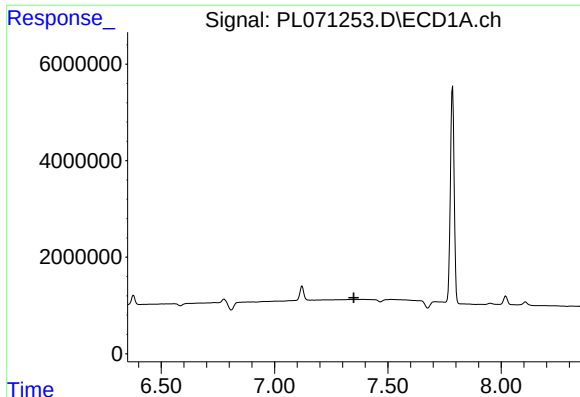

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

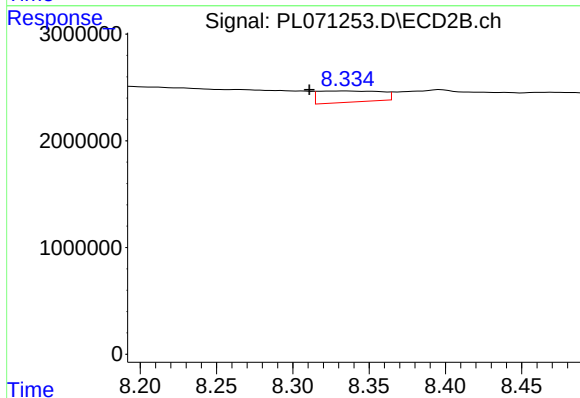


#11 alpha-Chlordane

R.T.: 8.336 min
Delta R.T.: 0.025 min
Response: 3002635
Conc: 1.89 ng/ml

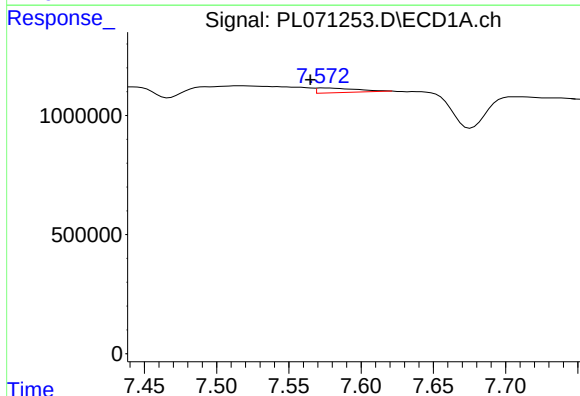


#12 4,4'-DDE

R.T.: 7.574 min
Delta R.T.: 0.009 min
Response: 355330
Conc: 0.63 ng/ml

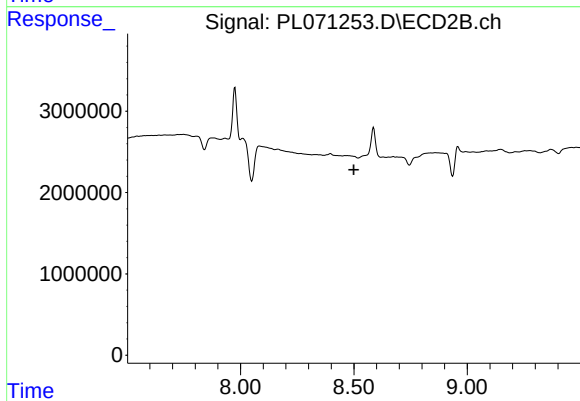

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 8.500 min
Response: 0
Conc: N.D.

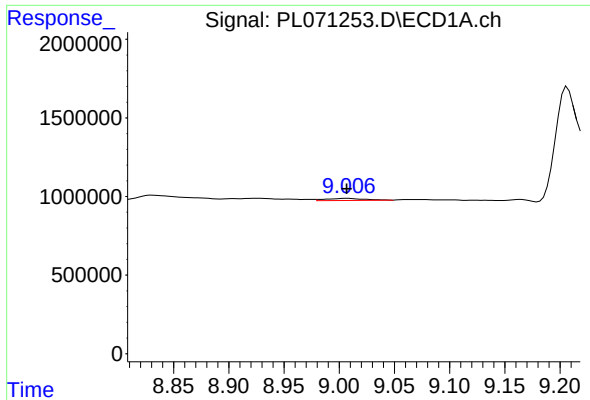

#20 Methoxychlor


R.T.: 9.008 min
Delta R.T.: 0.000 min
Response: 322703
Conc: 0.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

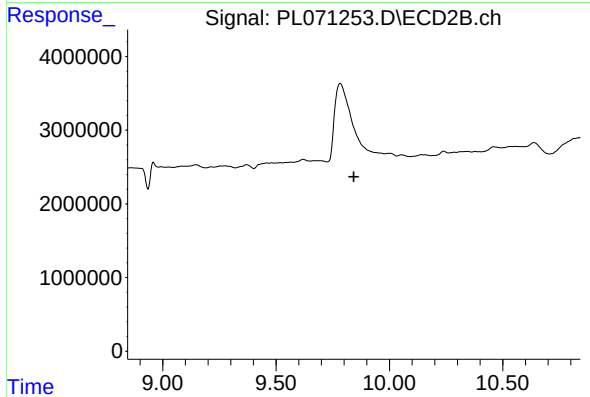


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.843 min
Response: 0
Conc: N.D.

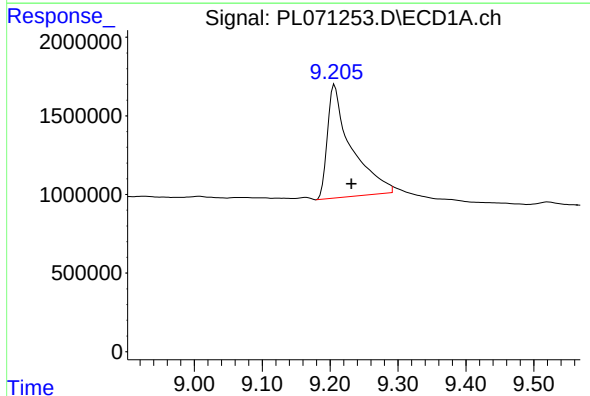


#21 Endrin ketone

R.T.: 9.207 min
Delta R.T.: -0.025 min
Response: 17571533
Conc: 24.66 ng/ml

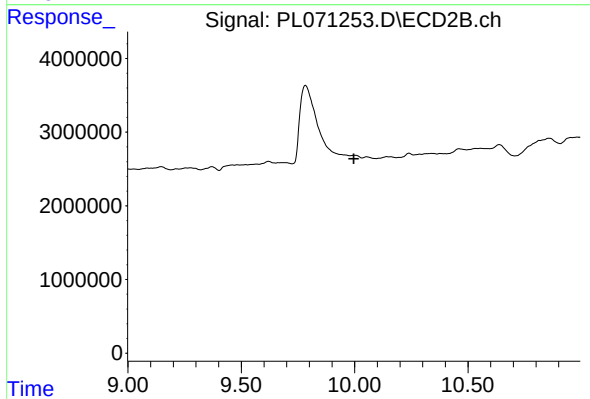

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.997 min
Response: 0
Conc: N.D.

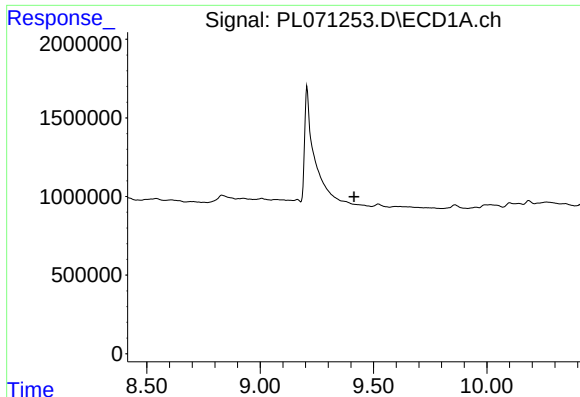

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.415 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

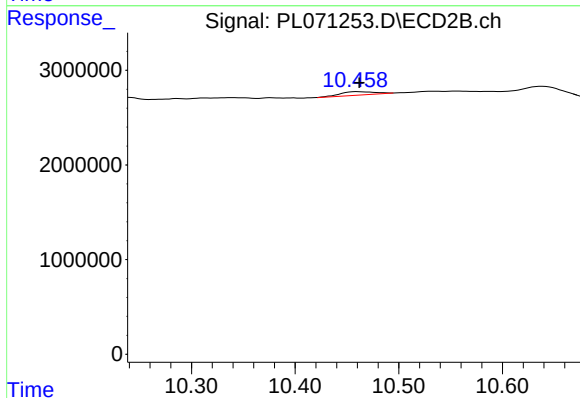


#22 Mirex

R.T.: 10.460 min
Delta R.T.: -0.002 min
Response: 840196
Conc: 0.77 ng/ml

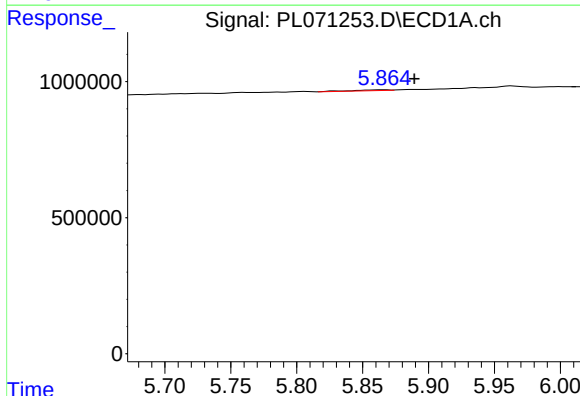


#23 Chlordane-1

R.T.: 5.866 min
Delta R.T.: -0.023 min
Response: 54699
Conc: 3.25 ng/ml

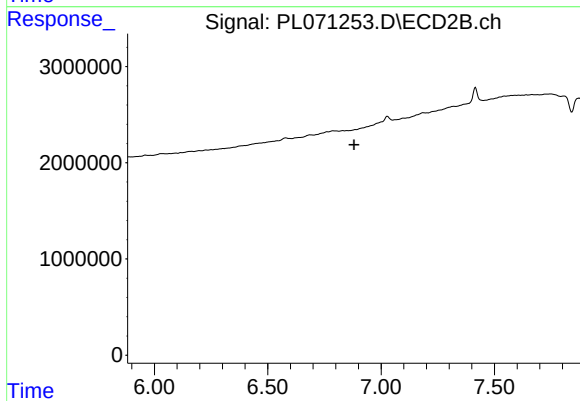

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 6.880 min
Response: 0
Conc: N.D.

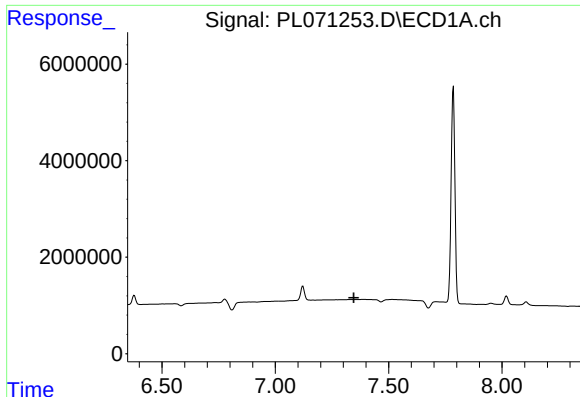

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.347 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

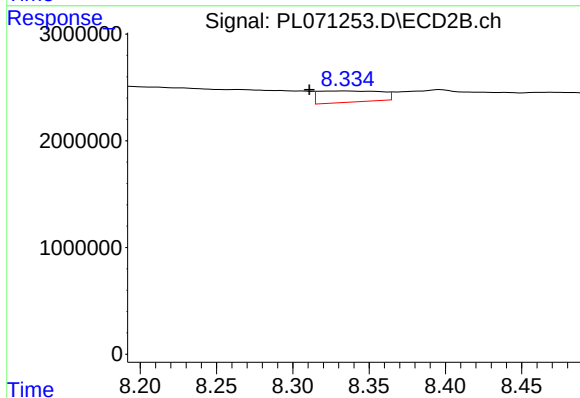


#26 Chlordane-4

R.T.: 8.336 min
Delta R.T.: 0.025 min
Response: 3002635
Conc: 11.32 ng/ml

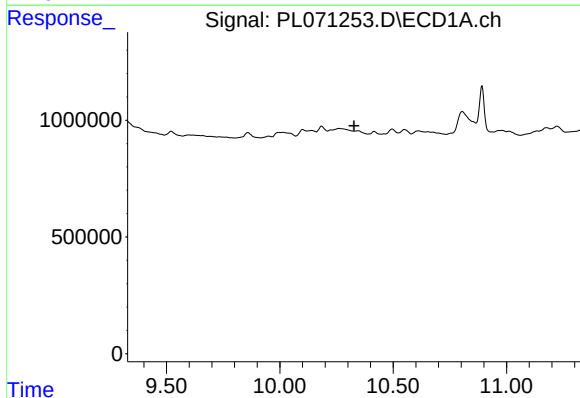

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 10.328 min
Response: 0
Conc: N.D.

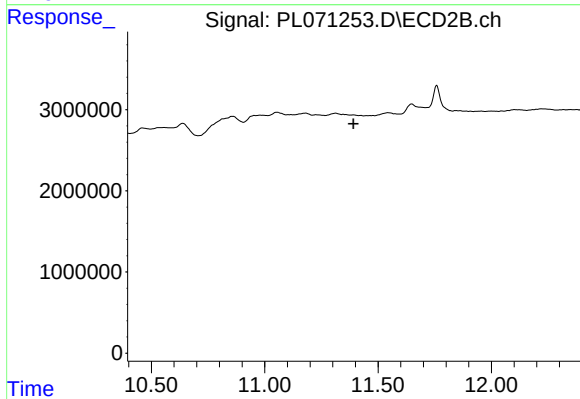

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 11.392 min
Response: 0
Conc: N.D.