

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120321\
 Data File : PL071263.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2021 14:09
 Operator : AR\AJ
 Sample : M4927-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 00:33:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.564	5.500	12213804	32477721	26.004	25.880
28)	SA Decachlor...	10.326	11.391	16621678	30531575	22.955	21.965
Target Compounds							
3)	MA gamma-BHC...	5.694	0.000	781393	0	1.224	N.D. #
7)	B delta-BHC	0.000	7.020f	0	416486	N.D.	0.245 #
11)	B alpha-Chl...	0.000	8.311	0	619650	N.D.	0.390 #
15)	B Endosulfa...	8.264f	9.150f	239765	944390	0.411	0.701 #
17)	MA 4,4'-DDT	0.000	9.355	0	184736	N.D.	0.133 #
20)	A Methoxychlor	8.984f	0.000	219024	0	0.606	N.D. #
21)	B Endrin ke...	0.000	9.975f	0	2253354	N.D.	1.539 #
23)	Chlordane-1	0.000	6.908f	0	505157	N.D.	9.520 #
26)	Chlordane-4	0.000	8.311	0	619650	N.D.	2.335 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120321\
Data File : PL071263.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2021 14:09
Operator : AR\AJ
Sample : M4927-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 00:33:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

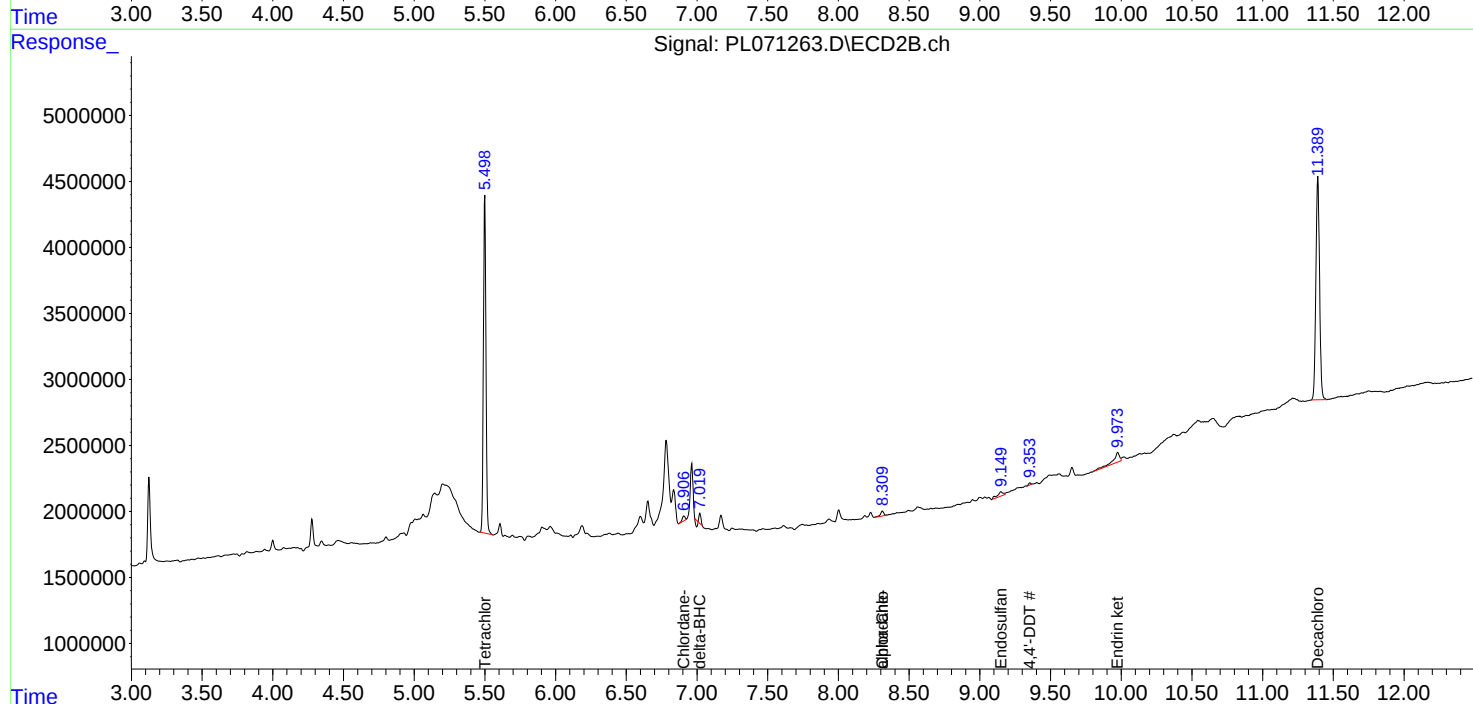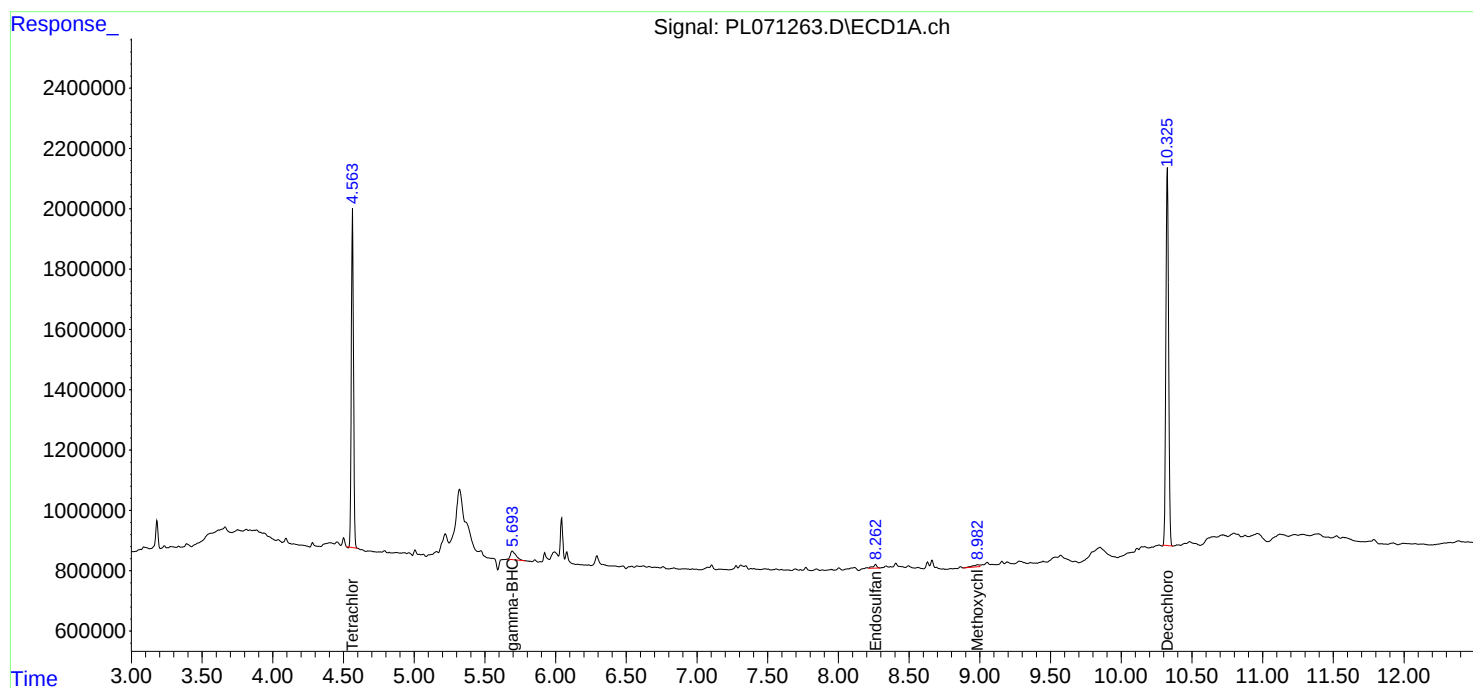


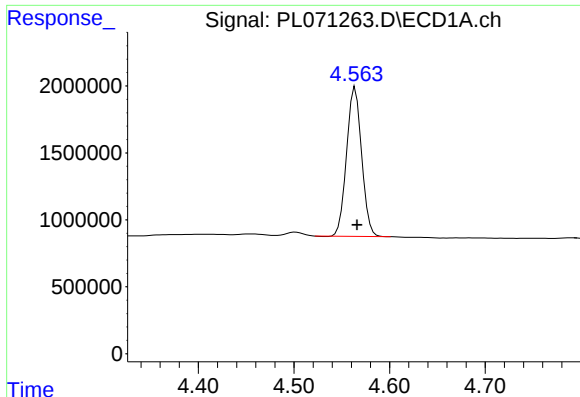

#1 Tetrachloro-m-xylene


R.T.: 4.564 min
Delta R.T.: -0.002 min
Response: 12213804
Conc: 26.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

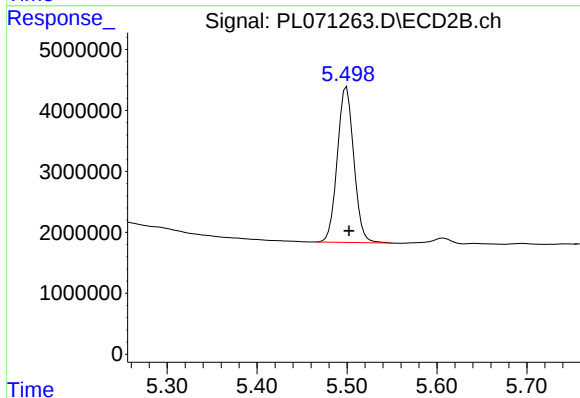


#1 Tetrachloro-m-xylene

R.T.: 5.500 min
Delta R.T.: -0.002 min
Response: 32477721
Conc: 25.88 ng/ml

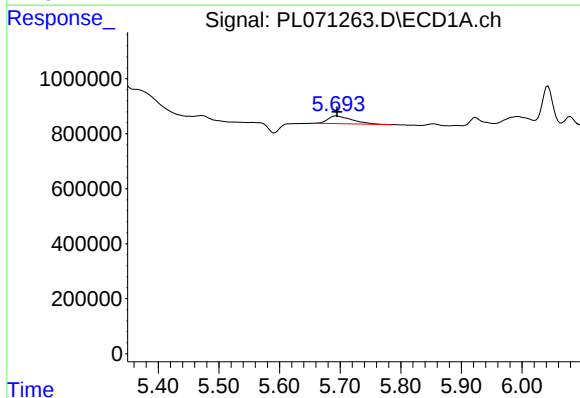


#3 gamma-BHC (Lindane)

R.T.: 5.694 min
Delta R.T.: -0.002 min
Response: 781393
Conc: 1.22 ng/ml

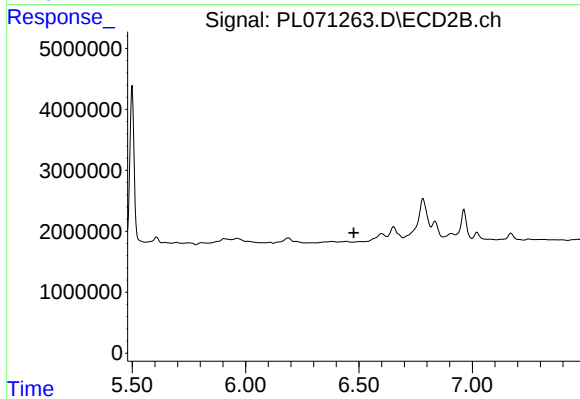

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 6.478 min
Response: 0
Conc: N.D.

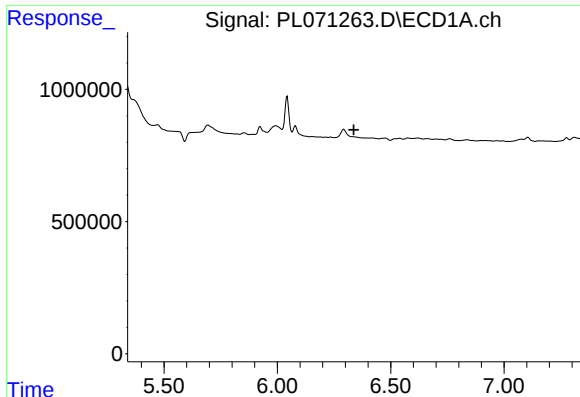

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.337 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

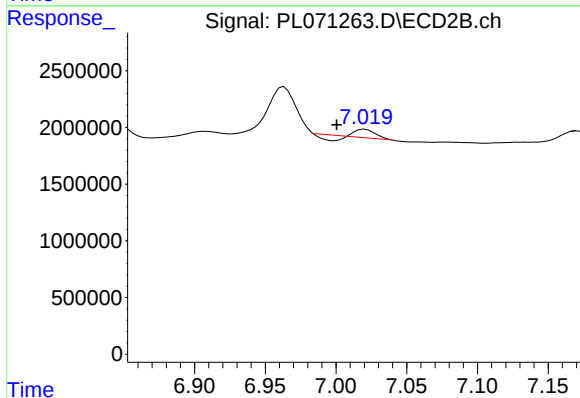


#7 delta-BHC

R.T.: 7.020 min
Delta R.T.: 0.020 min
Response: 416486
Conc: 0.24 ng/ml

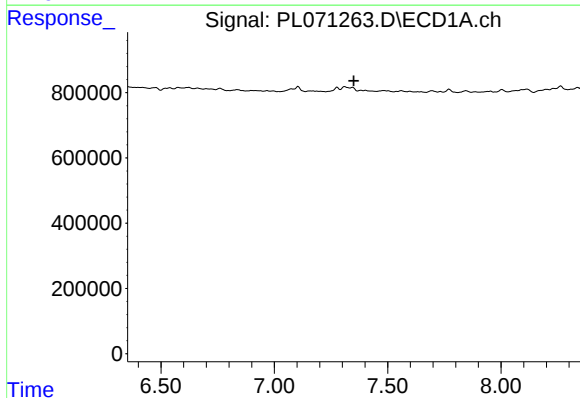


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.350 min
Response: 0
Conc: N.D.

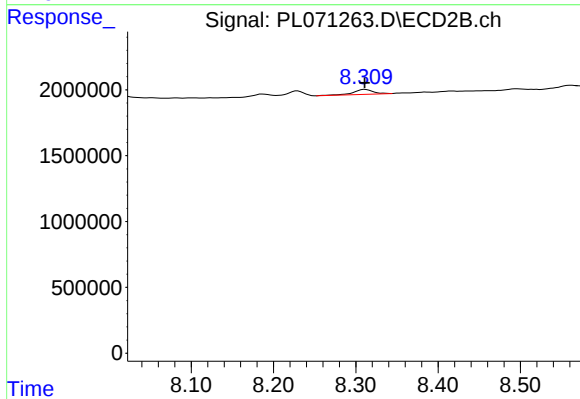

#11 alpha-Chlordane


R.T.: 8.311 min
Delta R.T.: 0.000 min
Response: 619650
Conc: 0.39 ng/ml

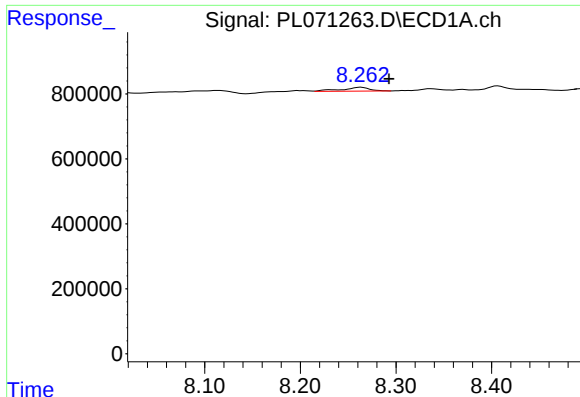

#15 Endosulfan II


R.T.: 8.264 min
Delta R.T.: -0.029 min
Response: 239765
Conc: 0.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

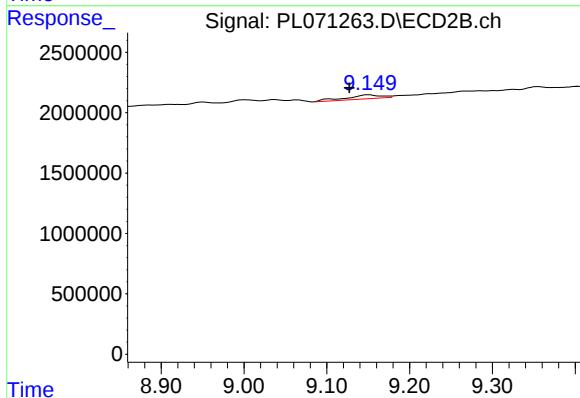


#15 Endosulfan II

R.T.: 9.150 min
Delta R.T.: 0.023 min
Response: 944390
Conc: 0.70 ng/ml

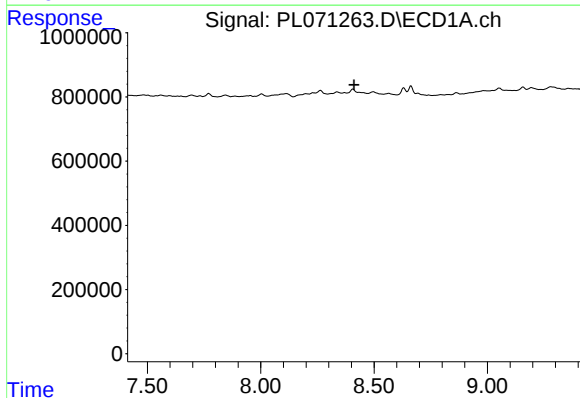


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 8.411 min
Response: 0
Conc: N.D.

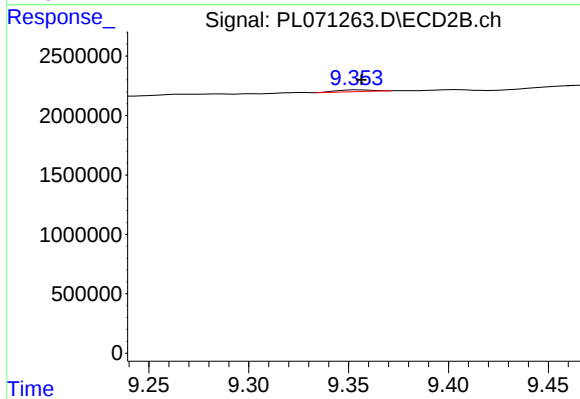

#17 4,4'-DDT


R.T.: 9.355 min
Delta R.T.: -0.002 min
Response: 184736
Conc: 0.13 ng/ml

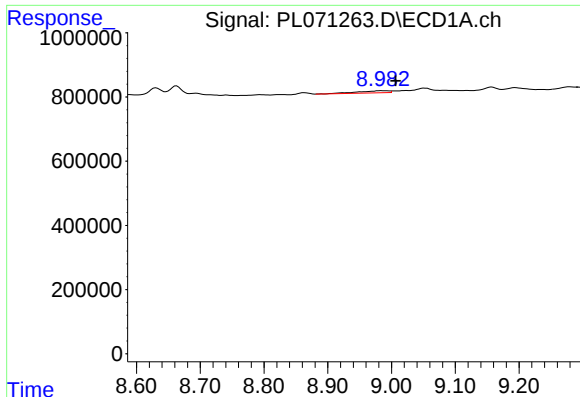

#20 Methoxychlor


R.T.: 8.984 min
Delta R.T.: -0.023 min
Response: 219024
Conc: 0.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

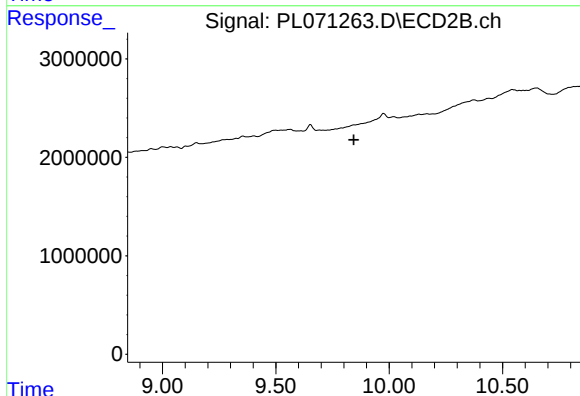


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.843 min
Response: 0
Conc: N.D.

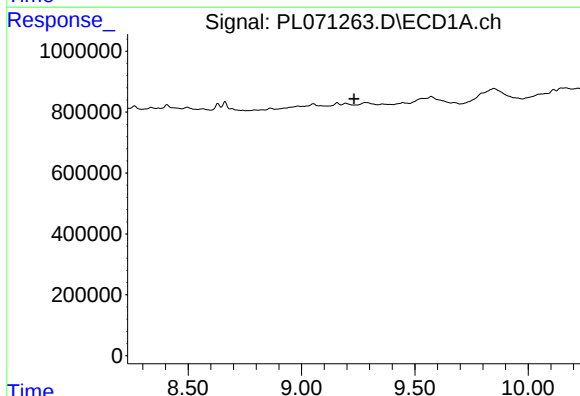


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.231 min
Response: 0
Conc: N.D.

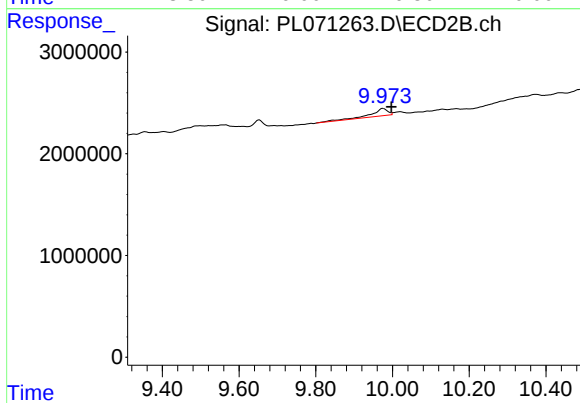

#21 Endrin ketone


R.T.: 9.975 min
Delta R.T.: -0.022 min
Response: 2253354
Conc: 1.54 ng/ml

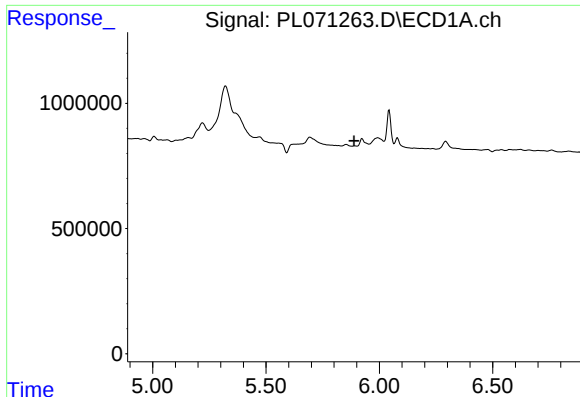

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.889 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

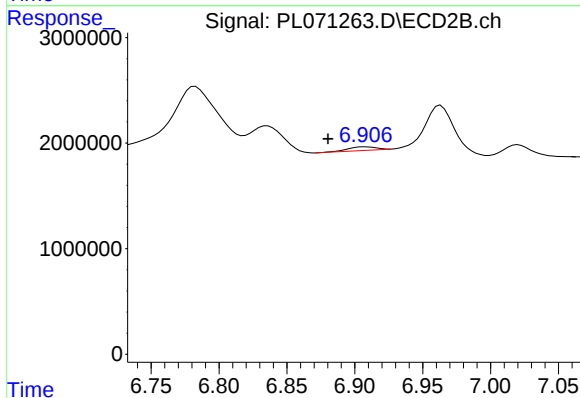


#23 Chlordane-1

R.T.: 6.908 min
Delta R.T.: 0.027 min
Response: 505157
Conc: 9.52 ng/ml

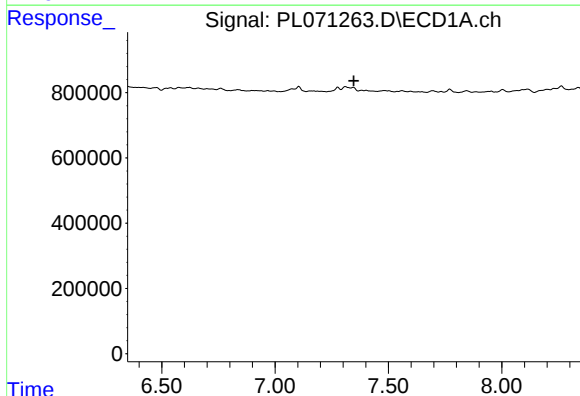


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.347 min
Response: 0
Conc: N.D.

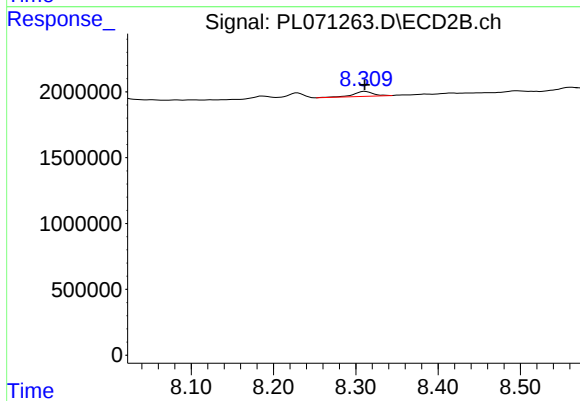

#26 Chlordane-4


R.T.: 8.311 min
Delta R.T.: 0.000 min
Response: 619650
Conc: 2.34 ng/ml

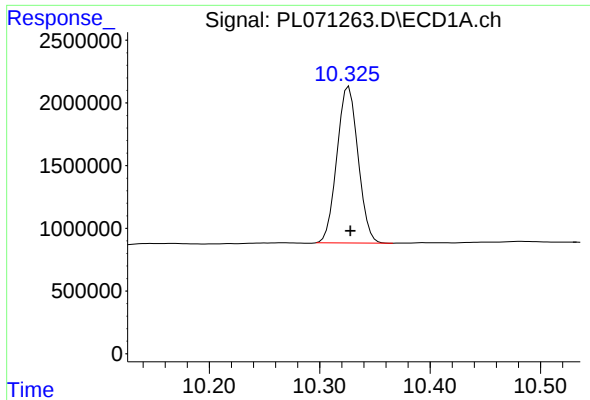

#28 Decachlorobiphenyl

R.T.: 10.326 min
Delta R.T.: -0.001 min
Response: 16621678
Conc: 22.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

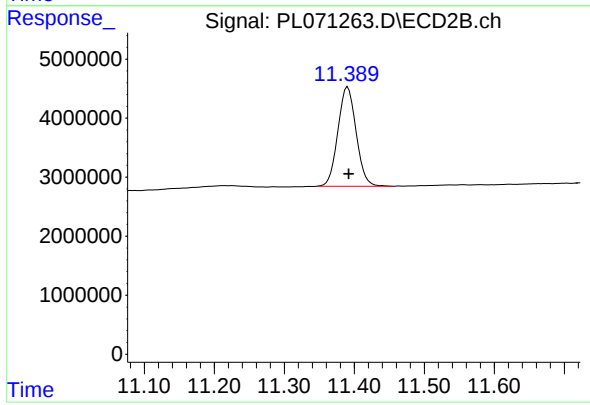

#28 Decachlorobiphenyl

R.T.: 11.391 min
Delta R.T.: -0.001 min
Response: 30531575
Conc: 21.97 ng/ml