

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120321\
 Data File : PL071277.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2021 18:55
 Operator : AR\AJ
 Sample : M4927-13
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 00:35:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.563	5.499	13112943	34493821	27.918	27.487
28)	SA Decachlor...	10.326	11.390	18588850	34604076	25.672	24.895
Target Compounds							
10)	B gamma-Chl...	7.276	8.228	295271	1303714	0.465	0.815 #
11)	B alpha-Chl...	7.345	8.310	290035	1041510	0.453	0.655 #
13)	MA Dieldrin	7.698	0.000	181945	0	0.301	N.D. #
14)	MA Endrin	8.003f	0.000	233365	0	0.413	N.D. #
17)	MA 4,4'-DDT	8.403	0.000	276467	0	0.505	N.D. #
20)	A Methoxychlor	8.978f	0.000	243880	0	0.675	N.D. #
21)	B Endrin ke...	0.000	9.978f	0	366613	N.D.	0.250 #
25)	Chlordane-3	7.276	8.228	295271	1303714	4.761	5.929
26)	Chlordane-4	7.345	8.310	290035	1041510	4.373	3.925



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120321\
Data File : PL071277.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2021 18:55
Operator : AR\AJ
Sample : M4927-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 00:35:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

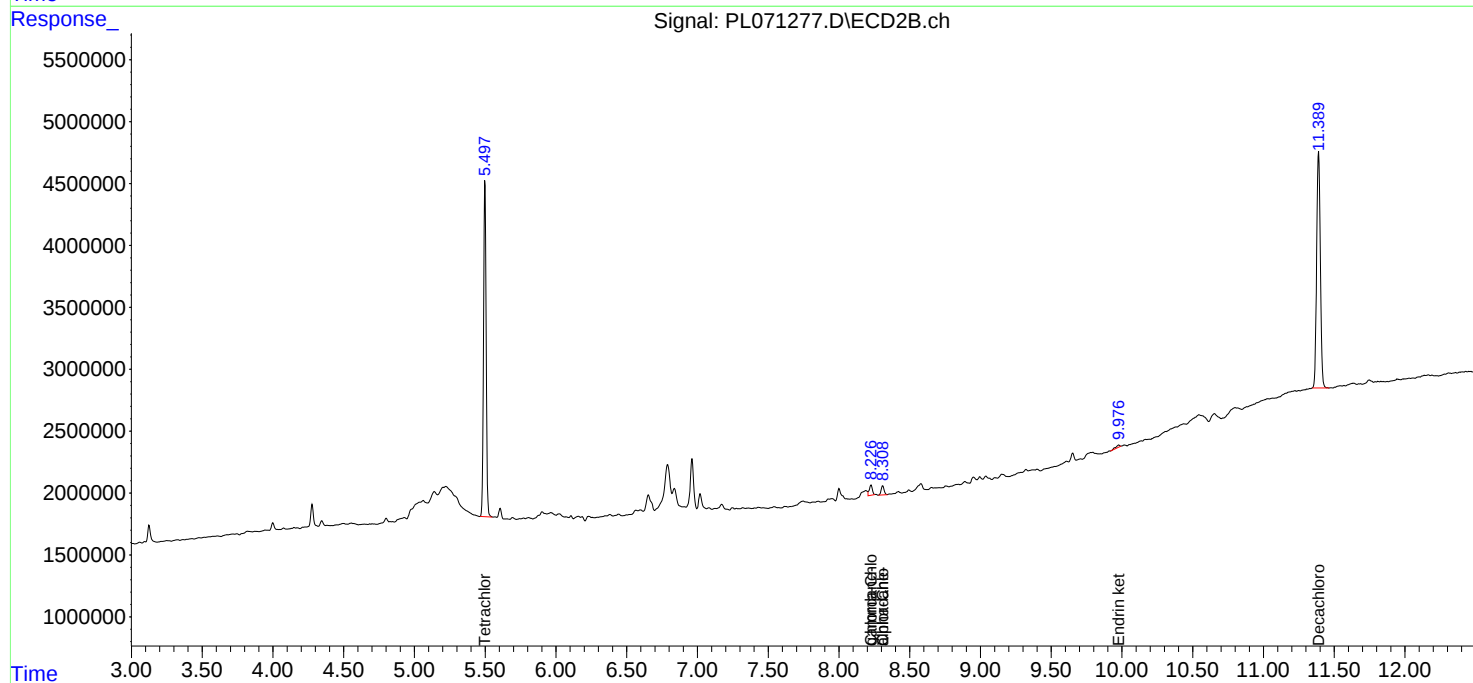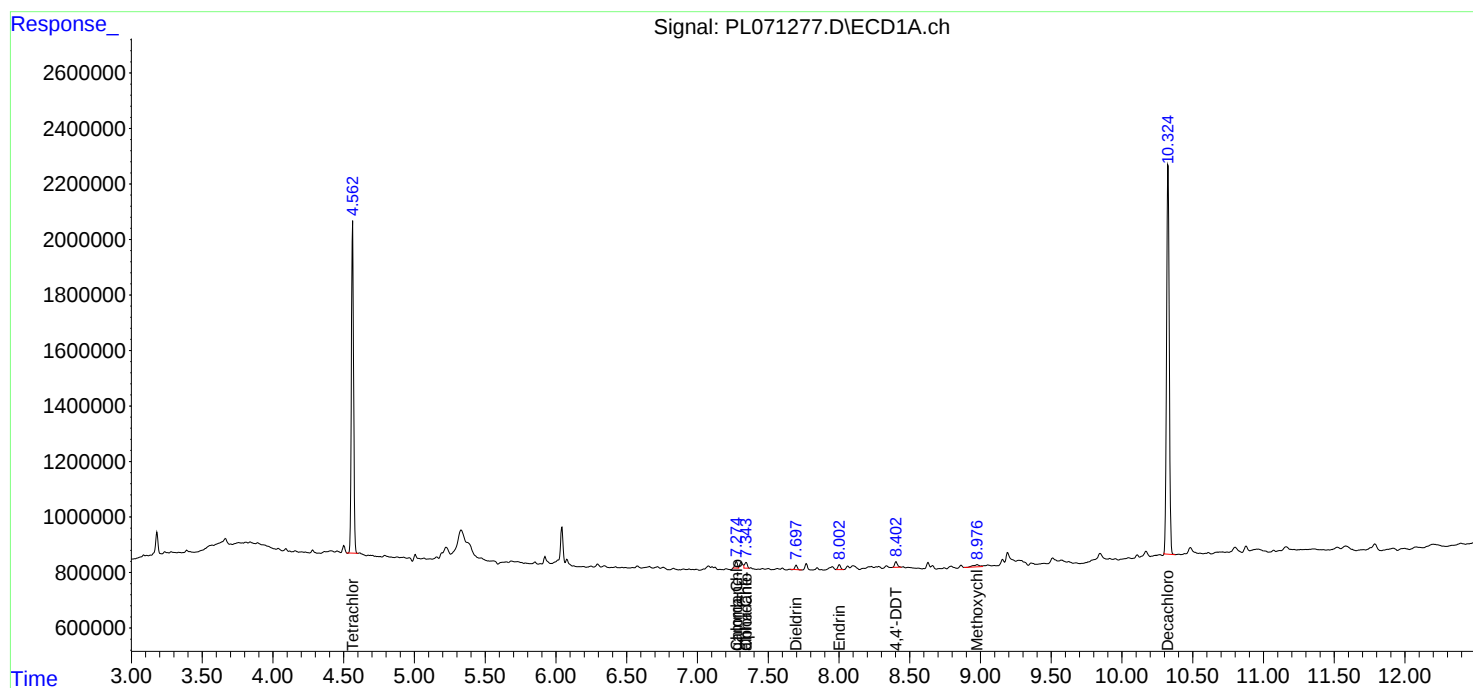


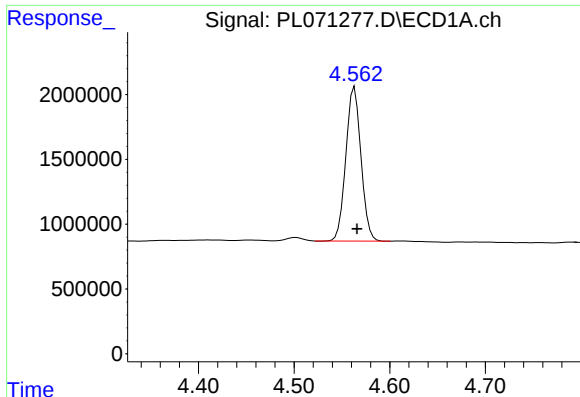

#1 Tetrachloro-m-xylene


R.T.: 4.563 min
Delta R.T.: -0.003 min
Response: 13112943
Conc: 27.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

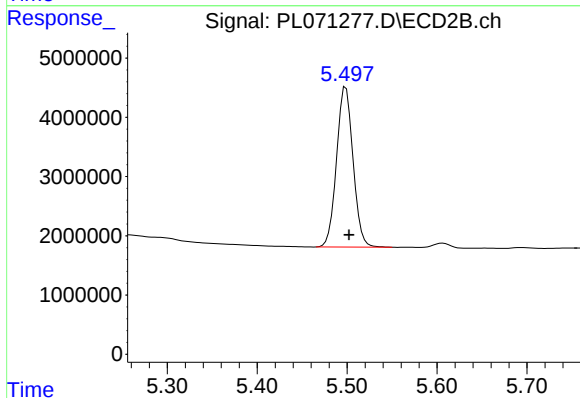


#1 Tetrachloro-m-xylene

R.T.: 5.499 min
Delta R.T.: -0.003 min
Response: 34493821
Conc: 27.49 ng/ml

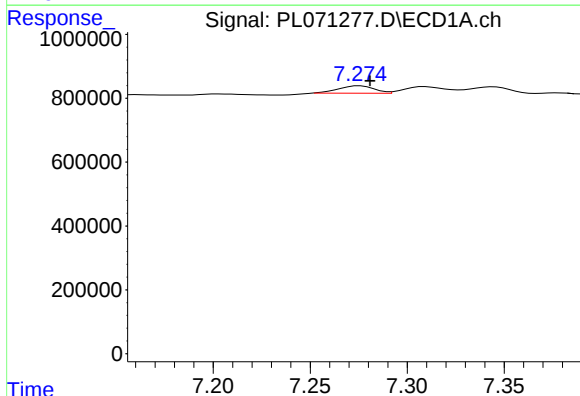


#10 gamma-Chlordane

R.T.: 7.276 min
Delta R.T.: -0.005 min
Response: 295271
Conc: 0.47 ng/ml

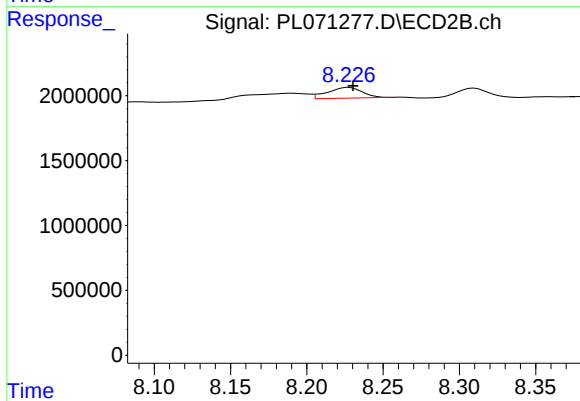

#10 gamma-Chlordane


R.T.: 8.228 min
Delta R.T.: -0.003 min
Response: 1303714
Conc: 0.82 ng/ml

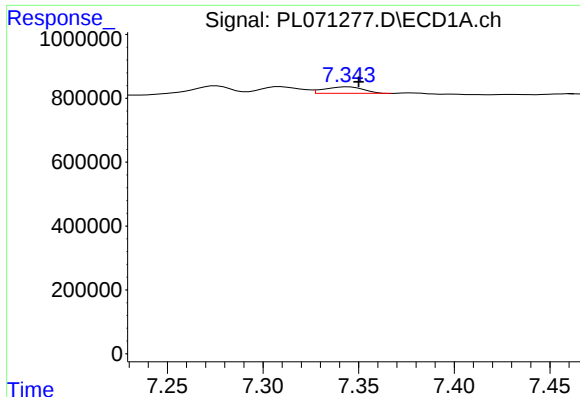

#11 alpha-Chlordane


R.T.: 7.345 min
Delta R.T.: -0.005 min
Response: 290035
Conc: 0.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

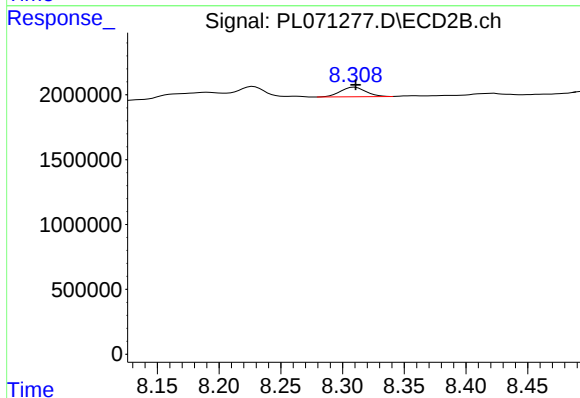


#11 alpha-Chlordane

R.T.: 8.310 min
Delta R.T.: 0.000 min
Response: 1041510
Conc: 0.66 ng/ml

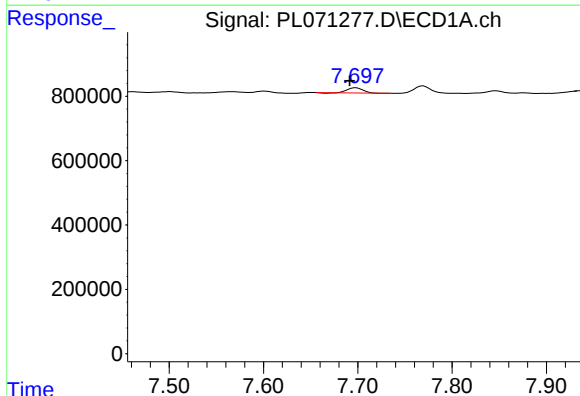


#13 Dieldrin

R.T.: 7.698 min
Delta R.T.: 0.006 min
Response: 181945
Conc: 0.30 ng/ml

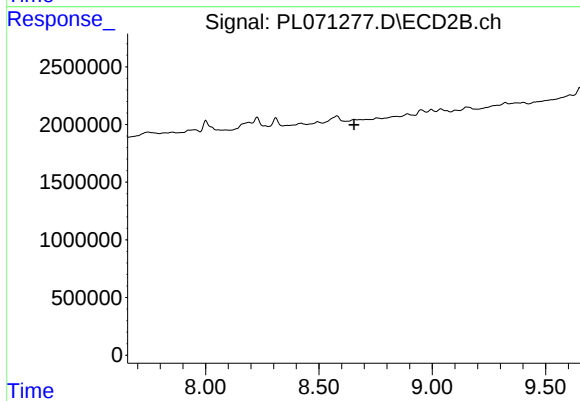

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.655 min
Response: 0
Conc: N.D.

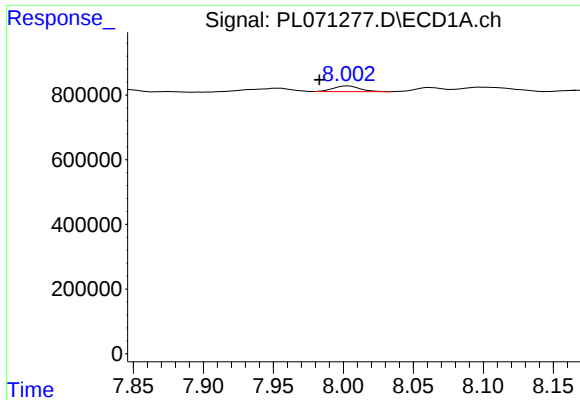

#14 Endrin


R.T.: 8.003 min
Delta R.T.: 0.021 min
Response: 233365
Conc: 0.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

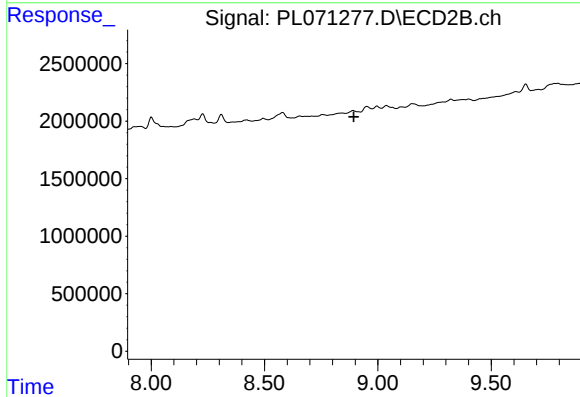


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.893 min
Response: 0
Conc: N.D.

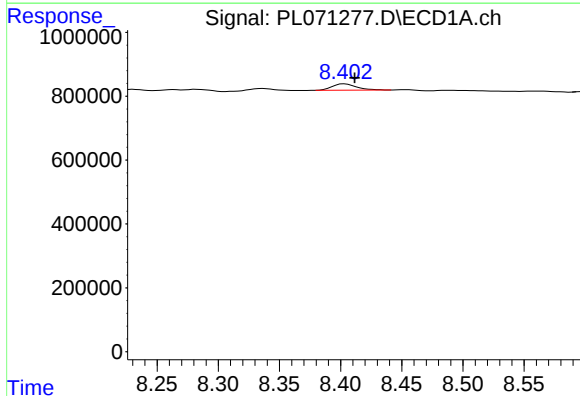


#17 4,4'-DDT

R.T.: 8.403 min
Delta R.T.: -0.008 min
Response: 276467
Conc: 0.51 ng/ml

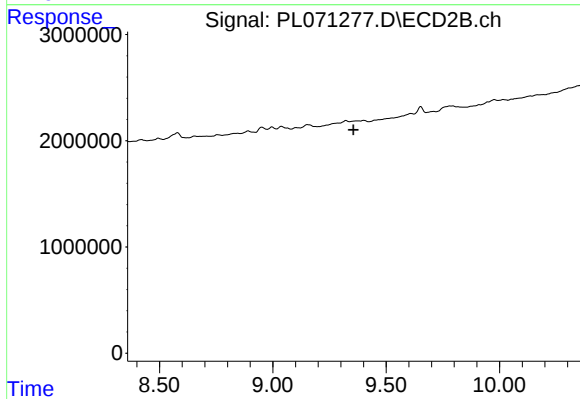

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 9.356 min
Response: 0
Conc: N.D.

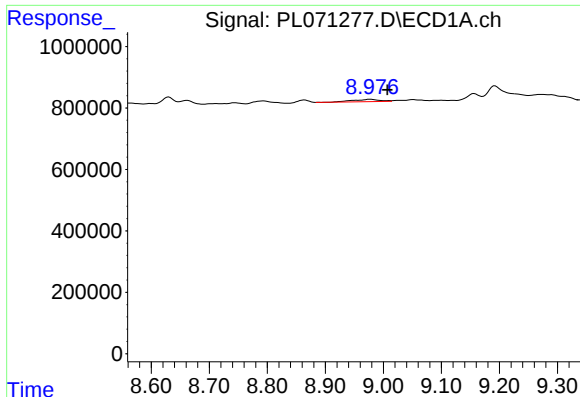

#20 Methoxychlor


R.T.: 8.978 min
Delta R.T.: -0.028 min
Response: 243880
Conc: 0.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

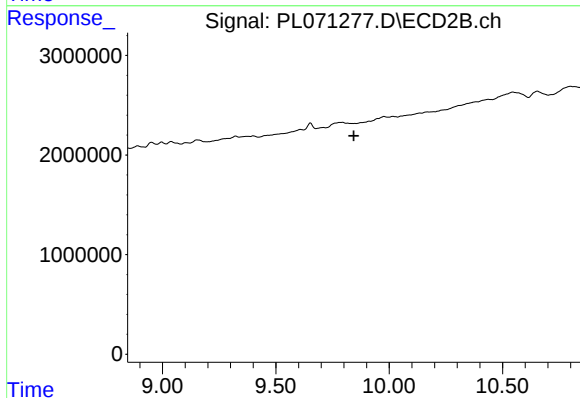


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.843 min
Response: 0
Conc: N.D.

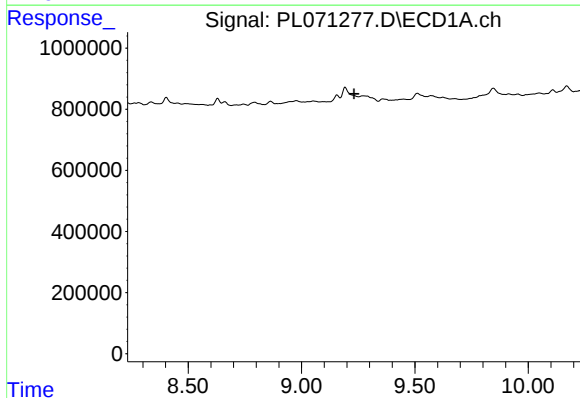


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.231 min
Response: 0
Conc: N.D.

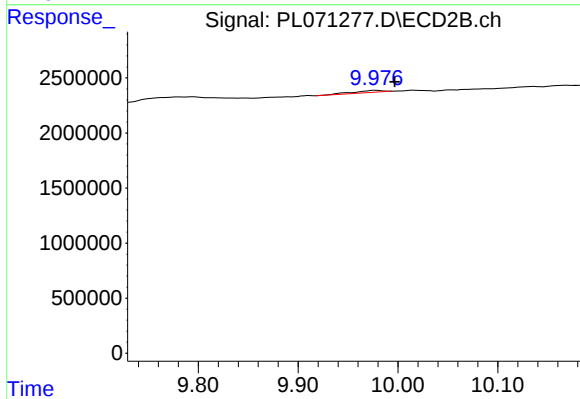

#21 Endrin ketone


R.T.: 9.978 min
Delta R.T.: -0.019 min
Response: 366613
Conc: 0.25 ng/ml

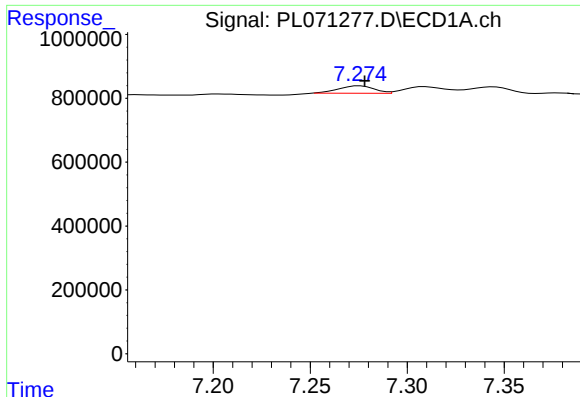

#25 Chlordane-3


R.T.: 7.276 min
Delta R.T.: -0.002 min
Response: 295271
Conc: 4.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

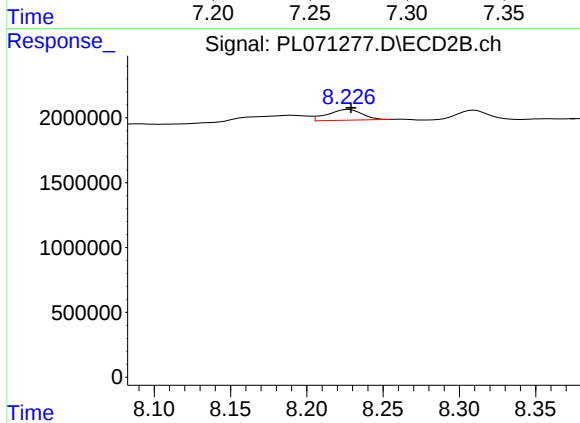


#25 Chlordane-3

R.T.: 8.228 min
Delta R.T.: -0.001 min
Response: 1303714
Conc: 5.93 ng/ml

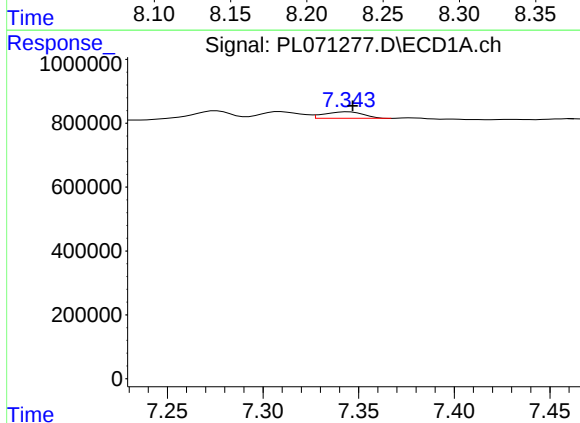


#26 Chlordane-4

R.T.: 7.345 min
Delta R.T.: -0.002 min
Response: 290035
Conc: 4.37 ng/ml

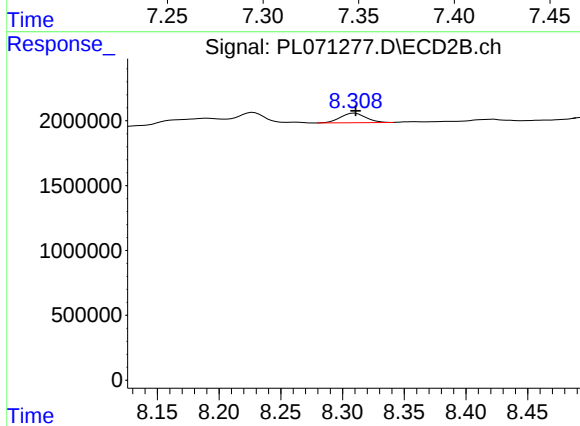

#26 Chlordane-4


R.T.: 8.310 min
Delta R.T.: -0.001 min
Response: 1041510
Conc: 3.93 ng/ml

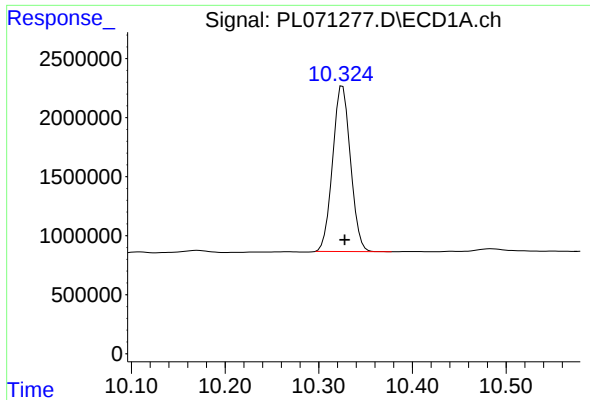

#28 Decachlorobiphenyl

R.T.: 10.326 min
Delta R.T.: -0.002 min
Response: 18588850
Conc: 25.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

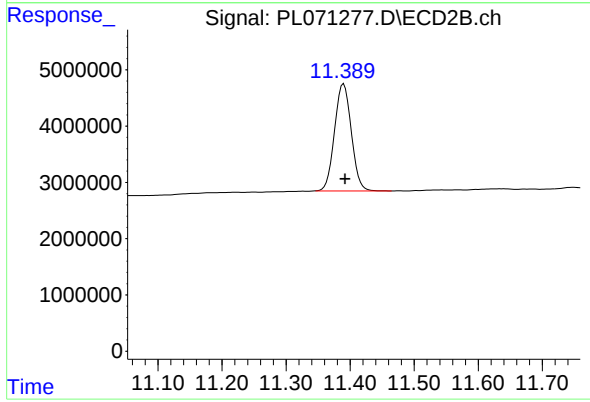

#28 Decachlorobiphenyl

R.T.: 11.390 min
Delta R.T.: -0.002 min
Response: 34604076
Conc: 24.89 ng/ml