

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120321\
 Data File : PL071281.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2021 00:25
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 03:28:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.570	5.500	10732062	27451685	22.849	21.875
28)	SA Decachlor...	10.334	11.396	15866738	28583148	21.913	20.563
Target Compounds							
2)	A alpha-BHC	5.256f	6.057f	345339	852098	0.528	0.460
3)	MA gamma-BHC...	0.000	6.494f	0	1097421	N.D.	0.623 #
6)	B beta-BHC	6.086	6.715f	-148356	2101607	N.D.	2.388
7)	B delta-BHC	0.000	7.022f	0	2144865	N.D.	1.261 #
15)	B Endosulfa...	8.275f	9.150f	201069	1290354	0.344	0.958 #
18)	B Endrin al...	0.000	9.284f	0	857169	N.D.	0.830 #
21)	B Endrin ke...	0.000	10.022f	0	910847	N.D.	0.622 #
27)	Chlordane-5	8.275f	0.000	201069	0	8.424	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120321\
Data File : PL071281.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2021 00:25
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 03:28:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

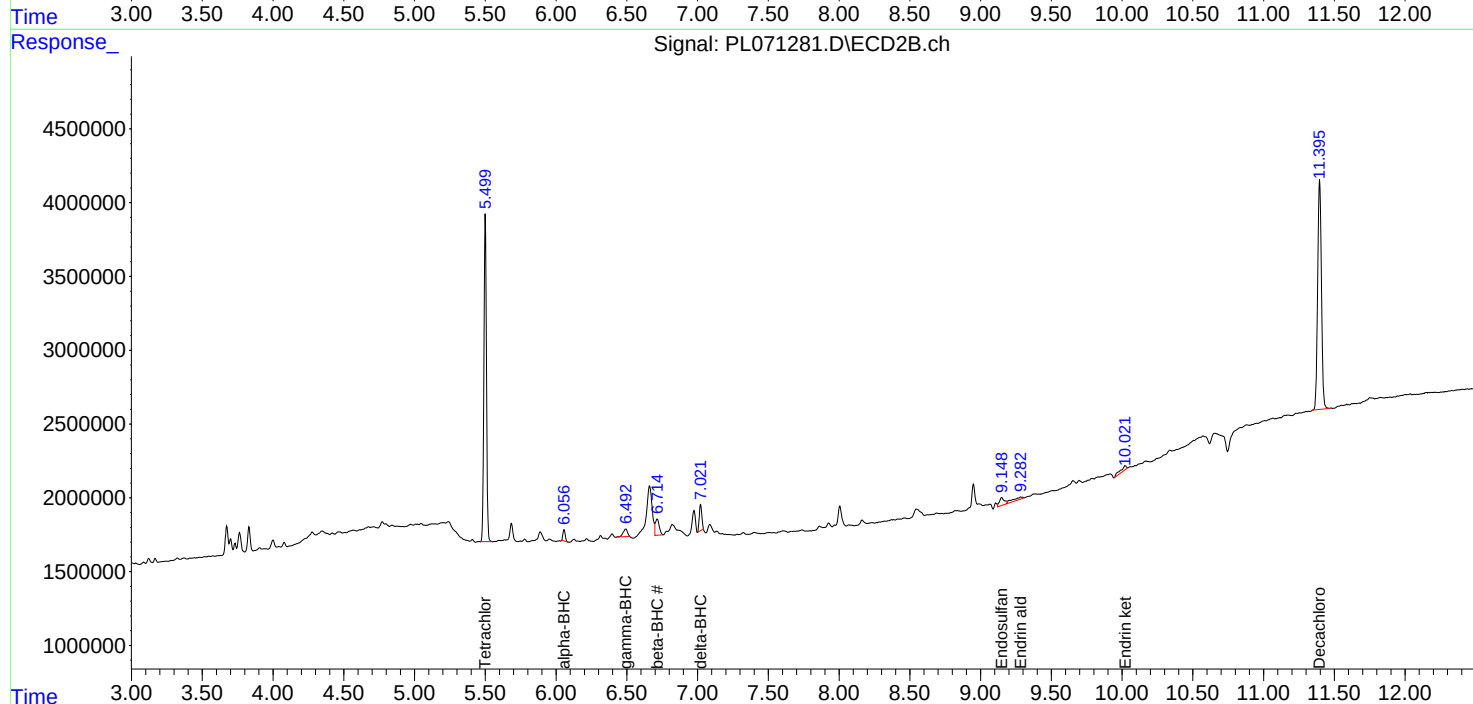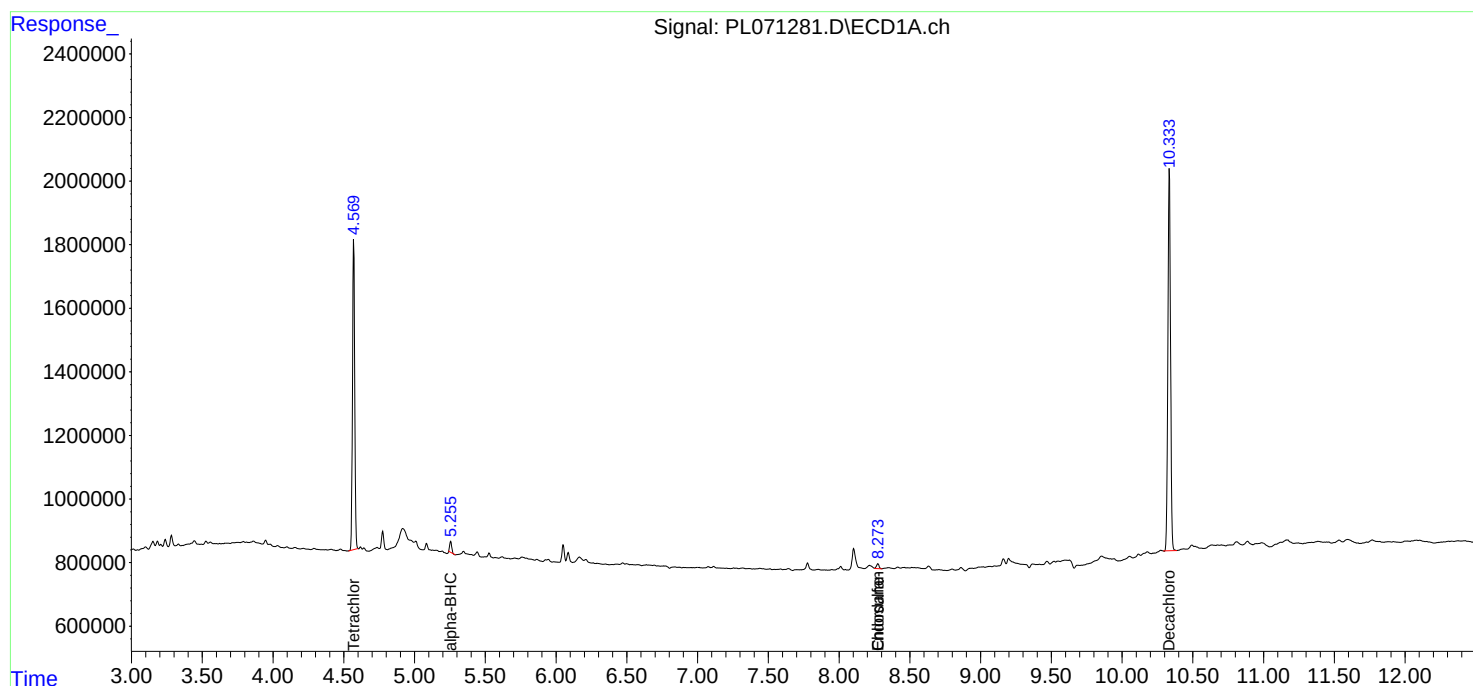


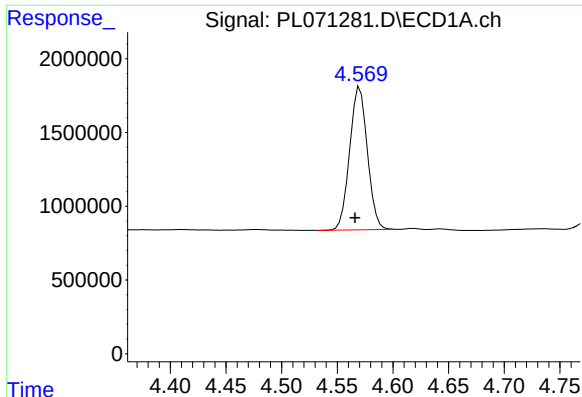

#1 Tetrachloro-m-xylene


R.T.: 4.570 min
Delta R.T.: 0.004 min
Response: 10732062
Conc: 22.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

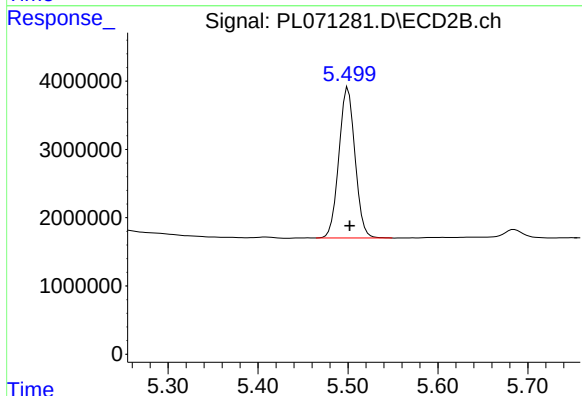


#1 Tetrachloro-m-xylene

R.T.: 5.500 min
Delta R.T.: -0.002 min
Response: 27451685
Conc: 21.88 ng/ml

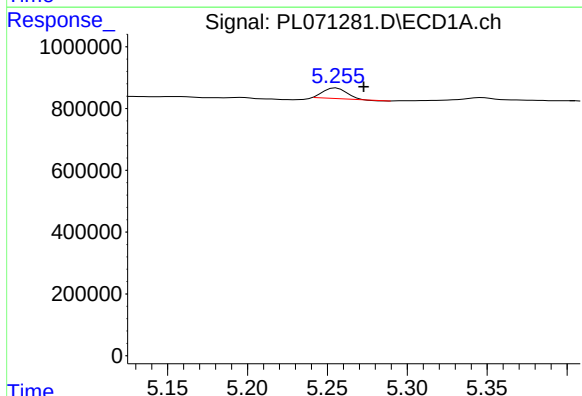


#2 alpha-BHC

R.T.: 5.256 min
Delta R.T.: -0.017 min
Response: 345339
Conc: 0.53 ng/ml

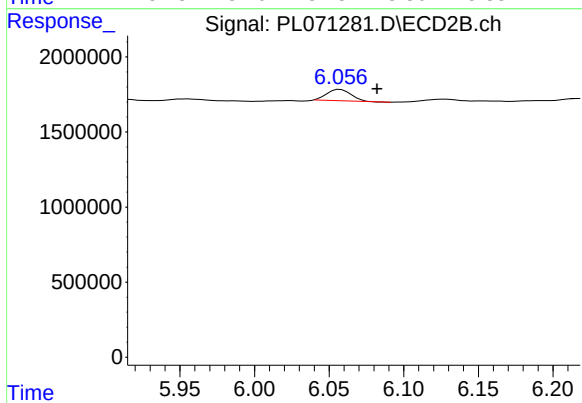

#2 alpha-BHC


R.T.: 6.057 min
Delta R.T.: -0.025 min
Response: 852098
Conc: 0.46 ng/ml

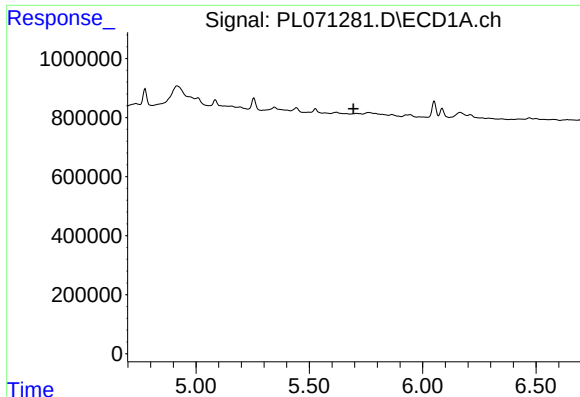

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 5.695 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

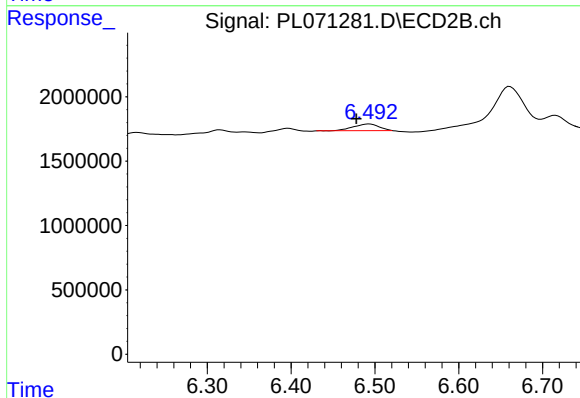


#3 gamma-BHC (Lindane)

R.T.: 6.494 min
Delta R.T.: 0.016 min
Response: 1097421
Conc: 0.62 ng/ml

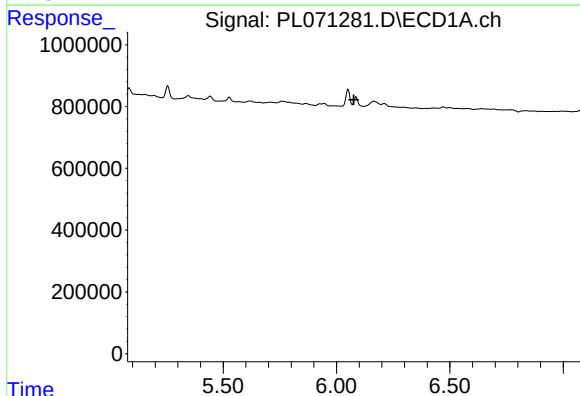


#6 beta-BHC

R.T.: 6.086 min
Delta R.T.: 0.010 min
Response: -148356
Conc: N.D.

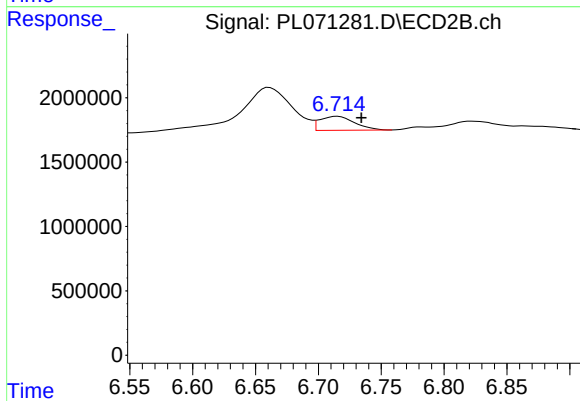

#6 beta-BHC


R.T.: 6.715 min
Delta R.T.: -0.019 min
Response: 2101607
Conc: 2.39 ng/ml

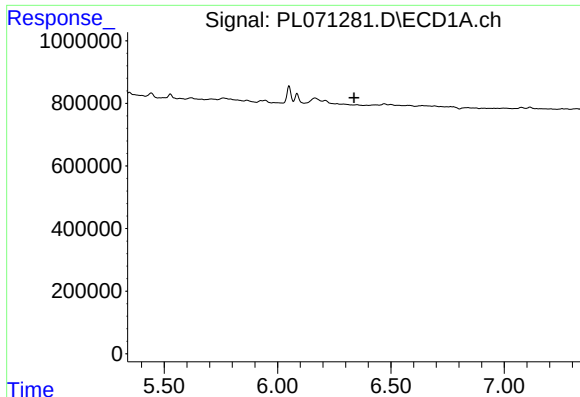

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.337 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

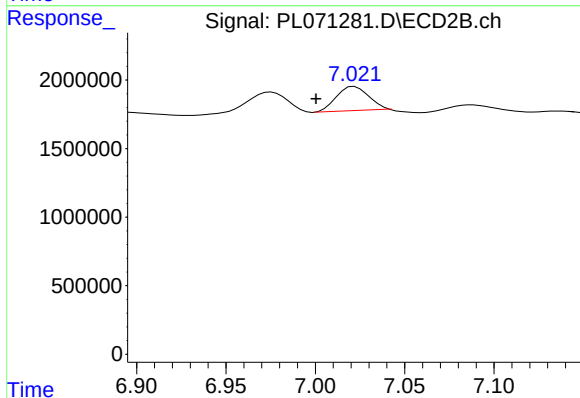


#7 delta-BHC

R.T.: 7.022 min
Delta R.T.: 0.021 min
Response: 2144865
Conc: 1.26 ng/ml

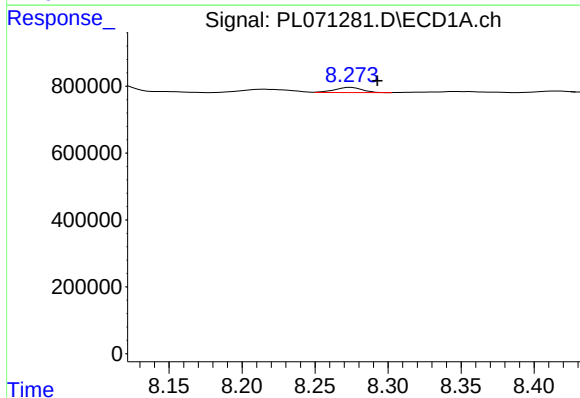


#15 Endosulfan II

R.T.: 8.275 min
Delta R.T.: -0.018 min
Response: 201069
Conc: 0.34 ng/ml

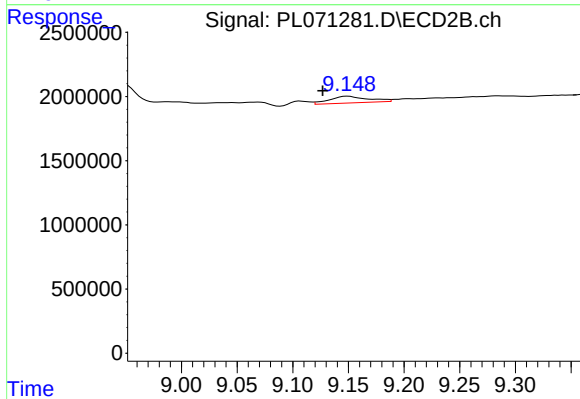

#15 Endosulfan II


R.T.: 9.150 min
Delta R.T.: 0.023 min
Response: 1290354
Conc: 0.96 ng/ml

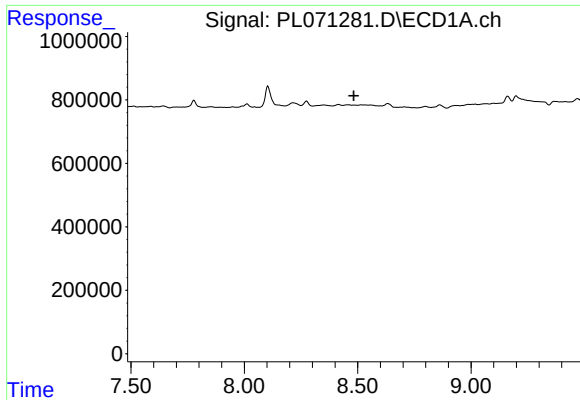

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 8.483 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

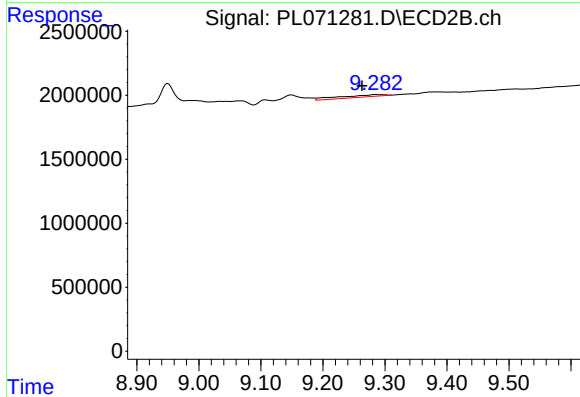


#18 Endrin aldehyde

R.T.: 9.284 min
Delta R.T.: 0.021 min
Response: 857169
Conc: 0.83 ng/ml

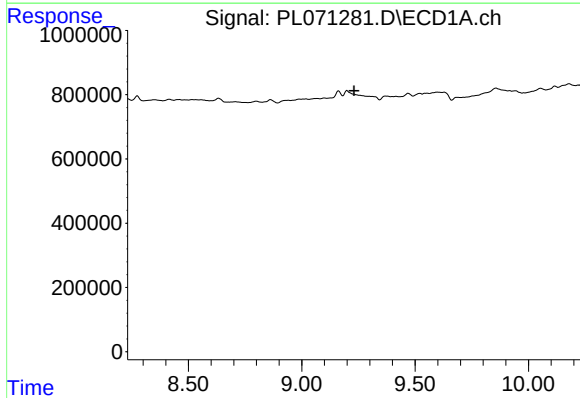


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.231 min
Response: 0
Conc: N.D.

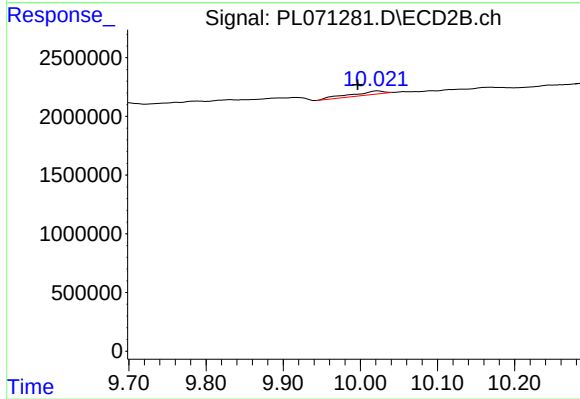

#21 Endrin ketone


R.T.: 10.022 min
Delta R.T.: 0.025 min
Response: 910847
Conc: 0.62 ng/ml

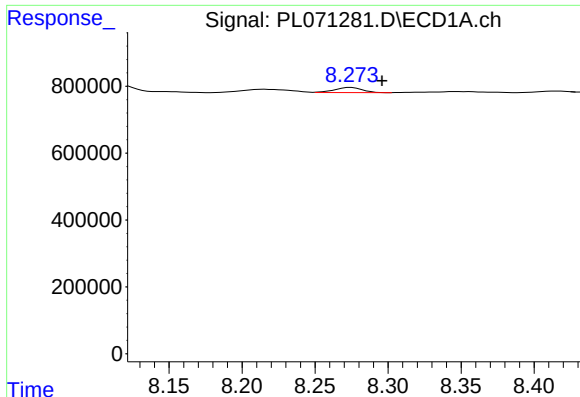

#27 Chlordane-5


R.T.: 8.275 min
Delta R.T.: -0.021 min
Response: 201069
Conc: 8.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

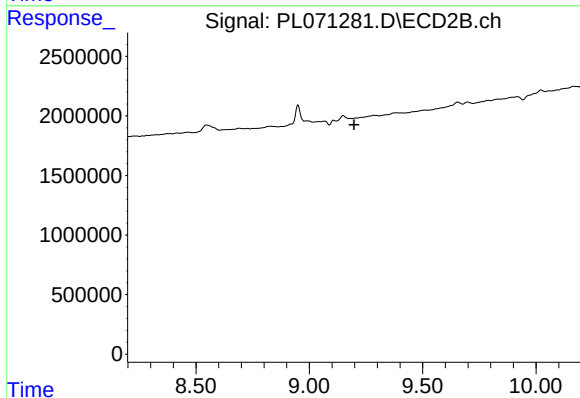


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.197 min
Response: 0
Conc: N.D.

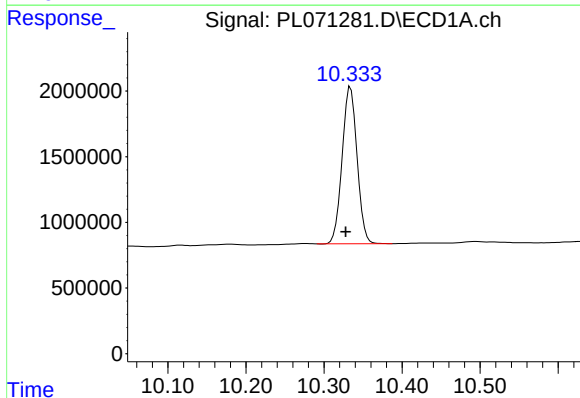

#28 Decachlorobiphenyl

R.T.: 10.334 min
Delta R.T.: 0.006 min
Response: 15866738
Conc: 21.91 ng/ml

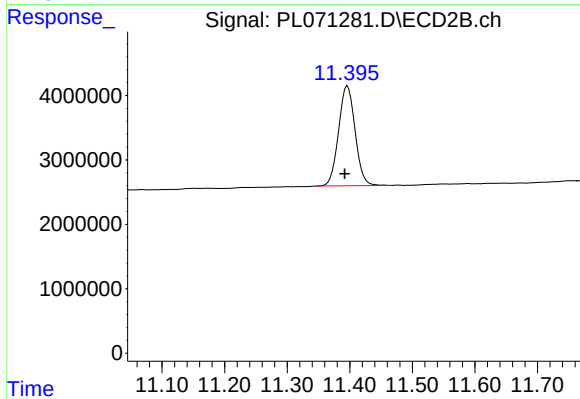

#28 Decachlorobiphenyl

R.T.: 11.396 min
Delta R.T.: 0.004 min
Response: 28583148
Conc: 20.56 ng/ml