

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120321\
 Data File : PL071257.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2021 12:27
 Operator : AR\AJ
 Sample : PB141144BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB141144BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/06/2021
 Supervised By : mohammad ahmed 12/06/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 00:32:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.575	5.502	10077982	24236671	21.456m	19.313
28)	SA Decachlor...	10.341	11.403	14733553	25408493	20.348	18.279

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120321\
Data File : PL071257.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2021 12:27
Operator : AR\AJ
Sample : PB141144BL
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB141144BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/06/2021
Supervised By : mohammad ahmed 12/06/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 00:32:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

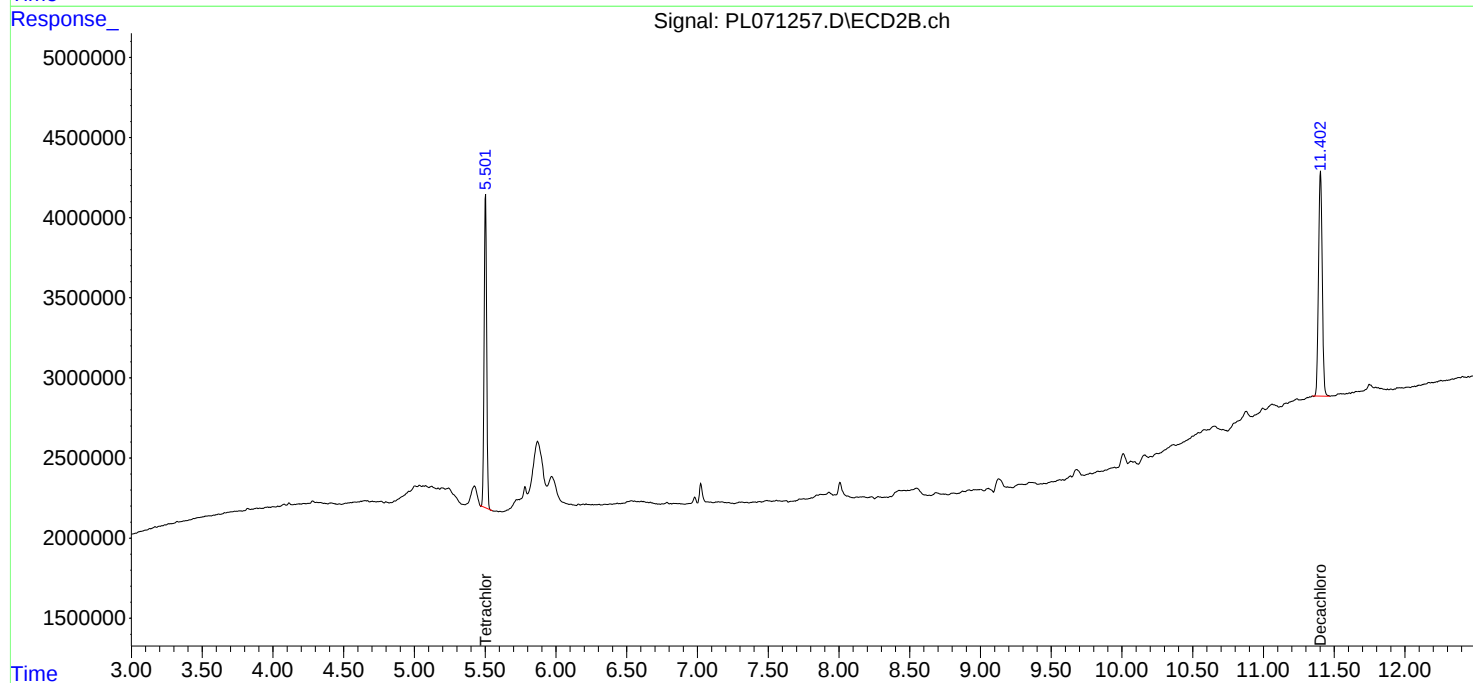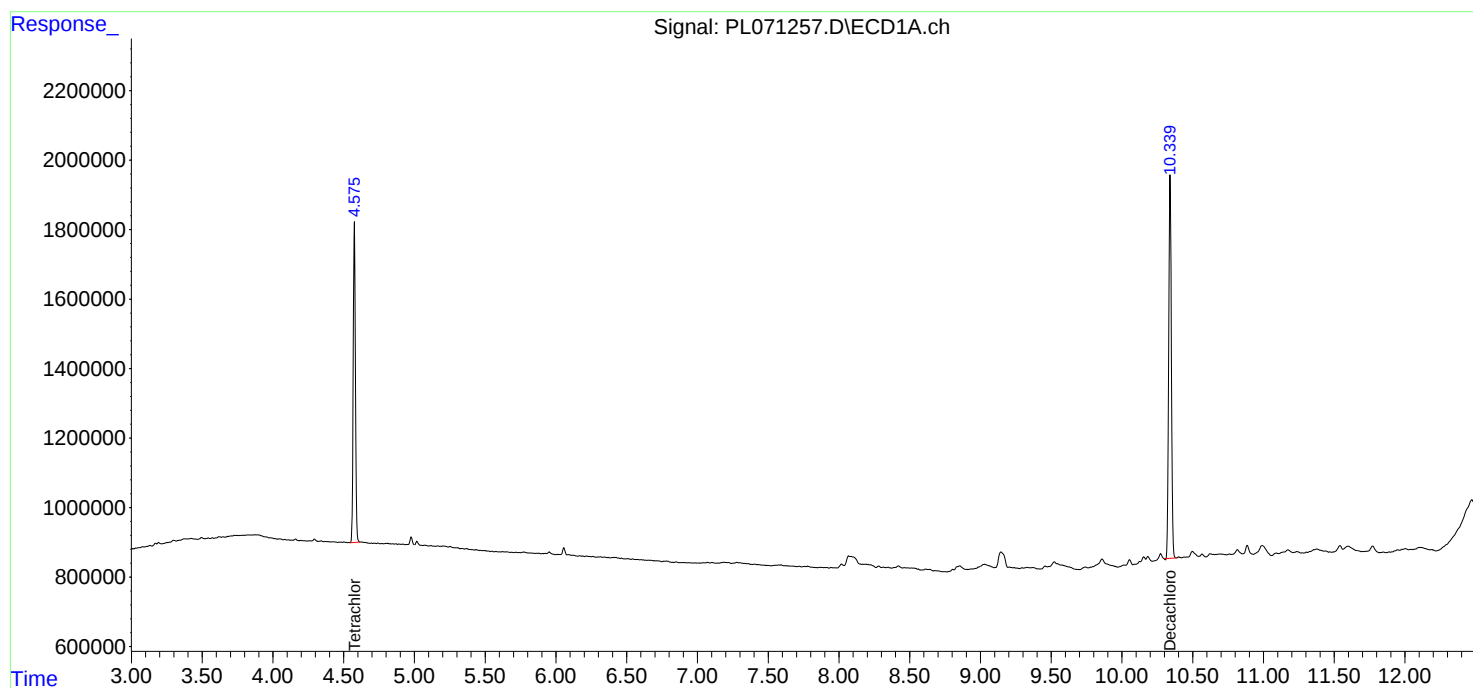

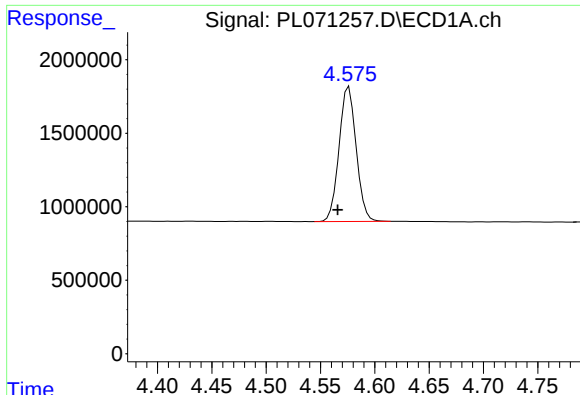


#1 Tetrachloro-m-xylene

R.T.: 4.575 min
Delta R.T.: 0.009 min
Response: 10077982
Conc: 21.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB141144BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/06/2021
Supervised By :mohammad ahmed 12/06/2021

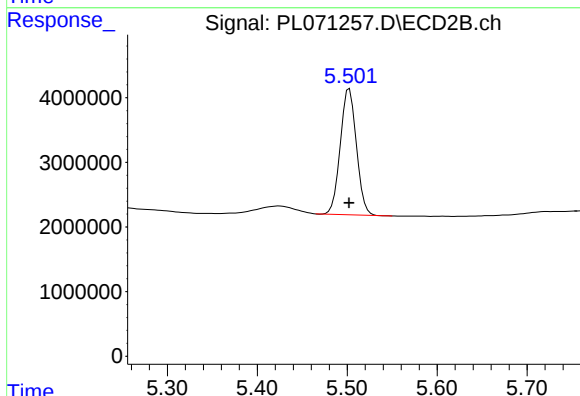


#1 Tetrachloro-m-xylene

R.T.: 5.502 min
Delta R.T.: 0.000 min
Response: 24236671
Conc: 19.31 ng/ml

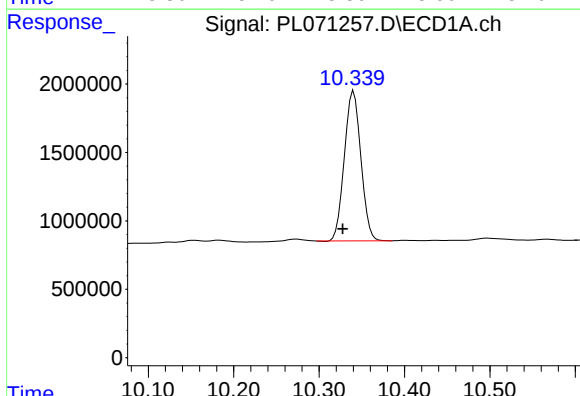

#28 Decachlorobiphenyl

R.T.: 10.341 min
Delta R.T.: 0.013 min
Response: 14733553
Conc: 20.35 ng/ml

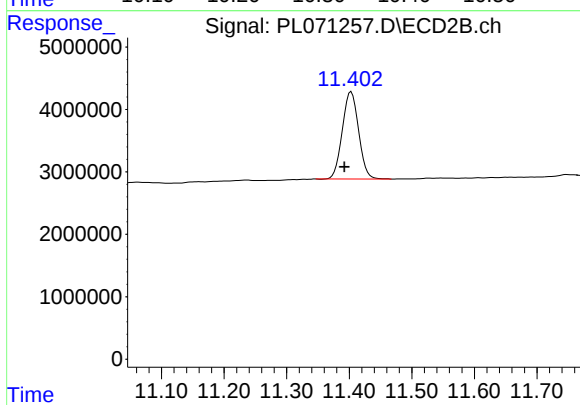

#28 Decachlorobiphenyl

R.T.: 11.403 min
Delta R.T.: 0.011 min
Response: 25408493
Conc: 18.28 ng/ml