

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120418\
 Data File : PL042799.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2018 23:22
 Operator : AJ\SJ
 Sample : J6206-11
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 00:11:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.102	103.6E6	54705784	17.609	19.021
28)	SA Decachlor...	8.204	9.232	79937168	40435265	12.684	16.765 #
Target Compounds							
2)	A alpha-BHC	3.899	0.000	4098771	0	0.454	N.D. #
7)	B delta-BHC	0.000	5.163	0	4034840	N.D.	1.096 #
8)	B Heptachlo...	5.233f	5.995	6172083	3988729	0.814	1.112 #
9)	A Endosulfan I	5.457f	6.358	951193	169476	0.137	0.054 #
10)	B gamma-Chl...	5.421	6.238	4207812	549103	0.552	0.161 #
11)	B alpha-Chl...	5.457	6.306	951193	1285190	0.127	0.384 #
19)	B Endosulfa...	6.643	0.000	1915524	0	0.307	N.D. #
23)	Chlordane-1	4.361	5.163	297321	4034840	1.075	30.353 #
25)	Chlordane-3	5.421	6.238	4207812	549103	4.800	1.168 #
26)	Chlordane-4	5.457	6.306	951193	1285190	1.253	2.349 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120418\
Data File : PL042799.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2018 23:22
Operator : AJ\SJ
Sample : J6206-11
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 00:11:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

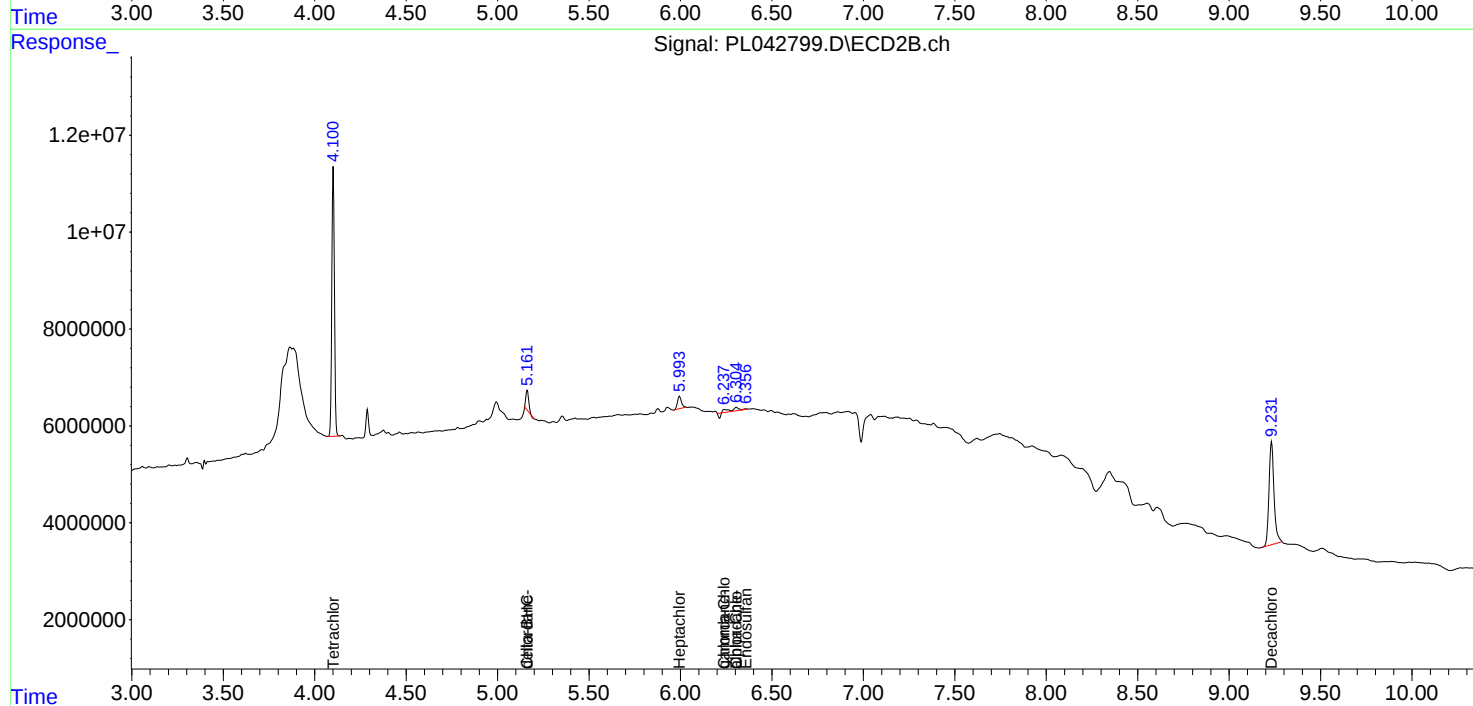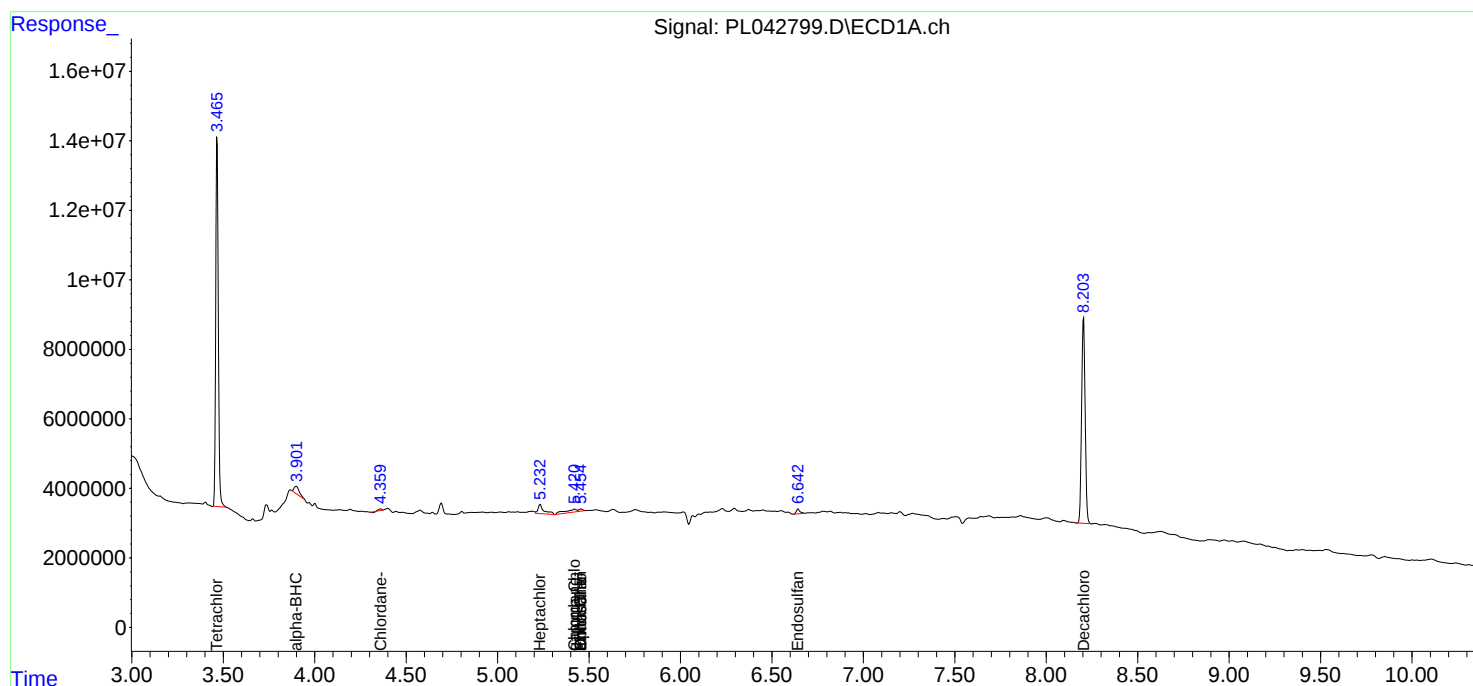


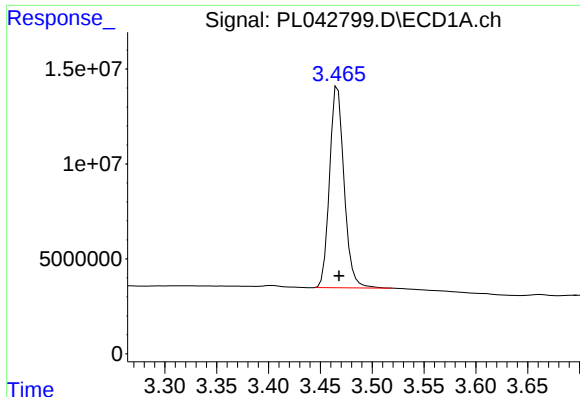

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: -0.001 min
Response: 103601749
Conc: 17.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

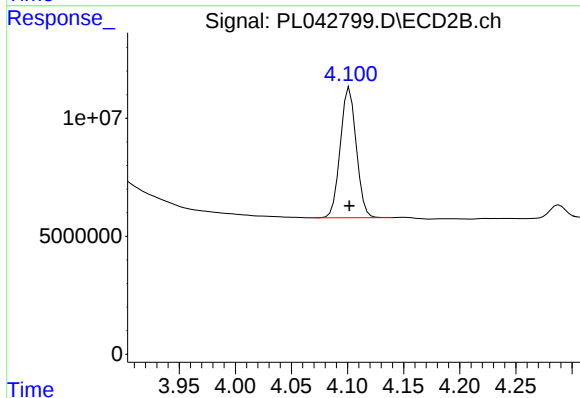


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 54705784
Conc: 19.02 ng/ml

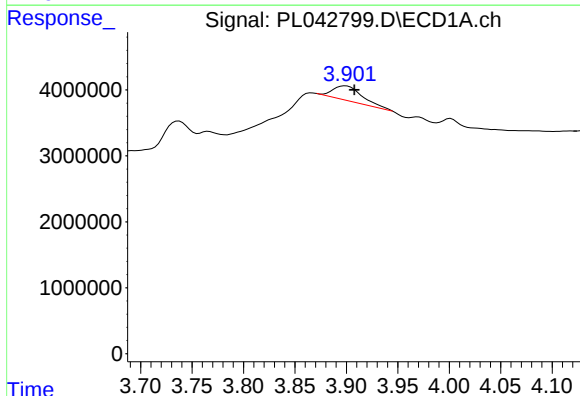


#2 alpha-BHC

R.T.: 3.899 min
Delta R.T.: -0.008 min
Response: 4098771
Conc: 0.45 ng/ml

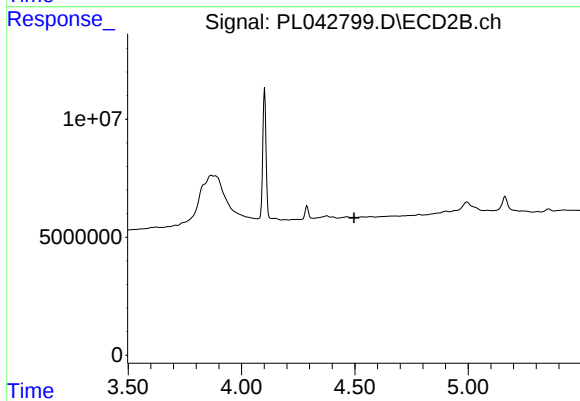

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.497 min
Response: 0
Conc: N.D.

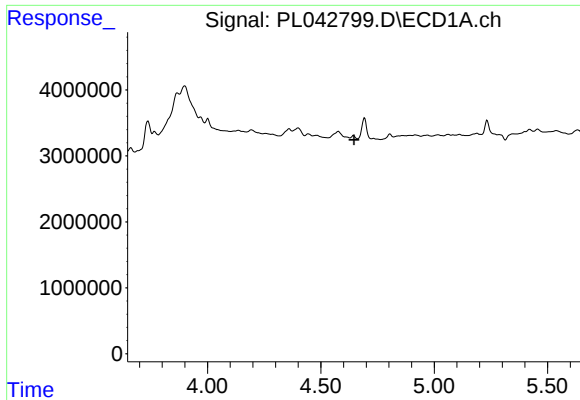

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.646 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

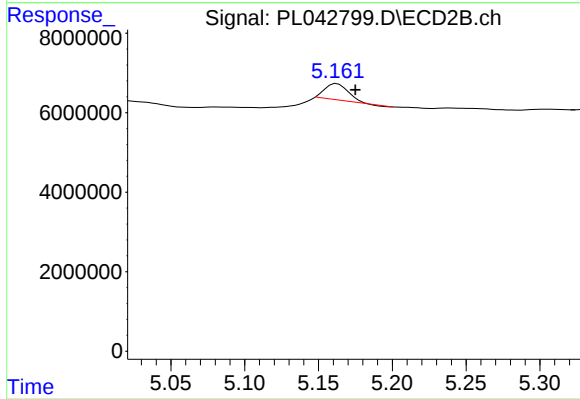


#7 delta-BHC

R.T.: 5.163 min
Delta R.T.: -0.012 min
Response: 4034840
Conc: 1.10 ng/ml

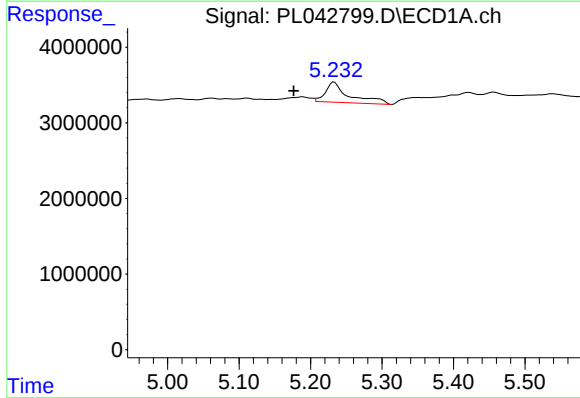


#8 Heptachlor epoxide

R.T.: 5.233 min
Delta R.T.: 0.057 min
Response: 6172083
Conc: 0.81 ng/ml

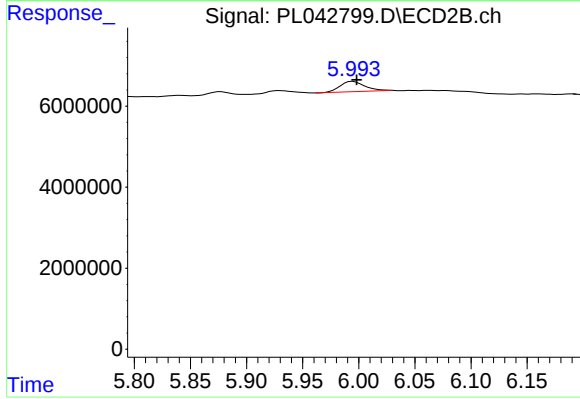

#8 Heptachlor epoxide


R.T.: 5.995 min
Delta R.T.: -0.004 min
Response: 3988729
Conc: 1.11 ng/ml

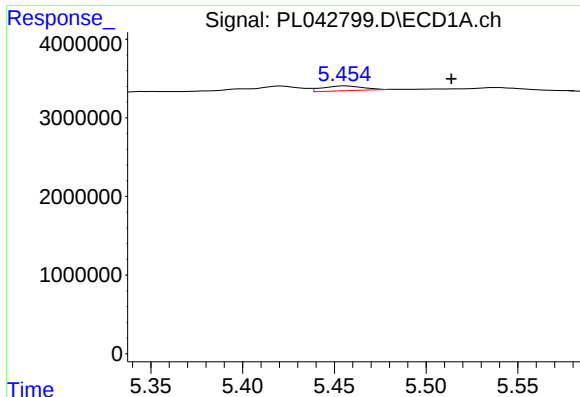

#9 Endosulfan I


R.T.: 5.457 min
Delta R.T.: -0.057 min
Response: 951193
Conc: 0.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

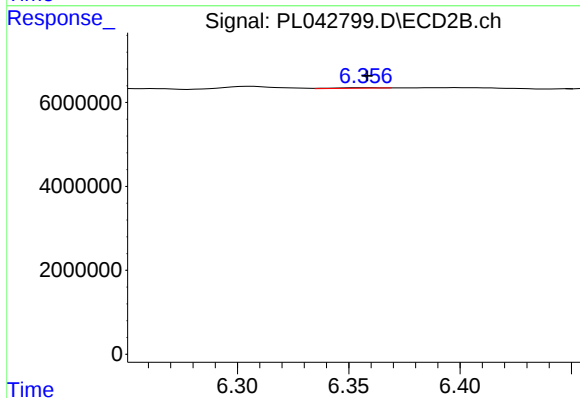


#9 Endosulfan I

R.T.: 6.358 min
Delta R.T.: 0.000 min
Response: 169476
Conc: 0.05 ng/ml

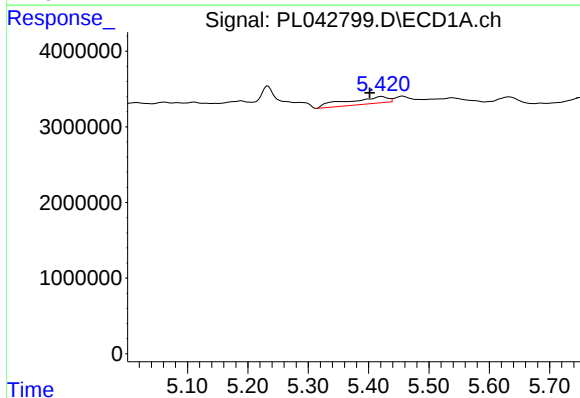


#10 gamma-Chlordane

R.T.: 5.421 min
Delta R.T.: 0.019 min
Response: 4207812
Conc: 0.55 ng/ml

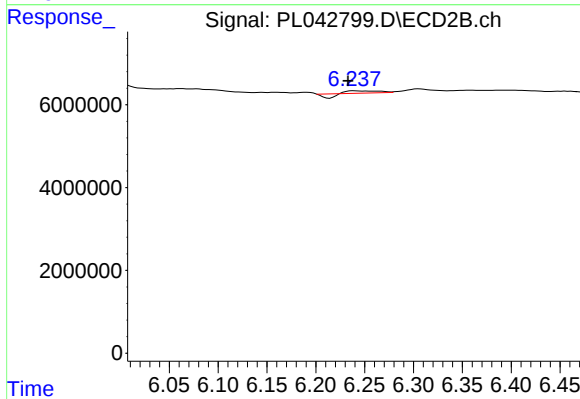

#10 gamma-Chlordane


R.T.: 6.238 min
Delta R.T.: 0.005 min
Response: 549103
Conc: 0.16 ng/ml

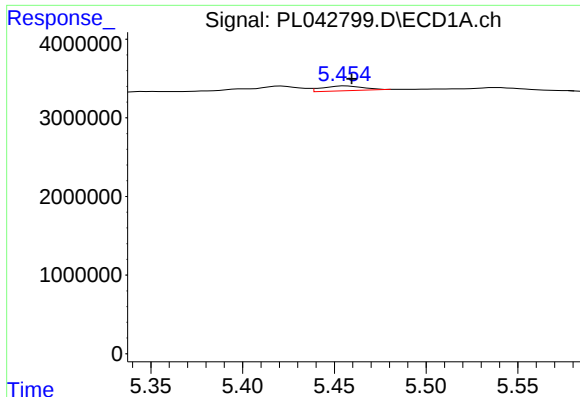

#11 alpha-Chlordane


R.T.: 5.457 min
Delta R.T.: -0.003 min
Response: 951193
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

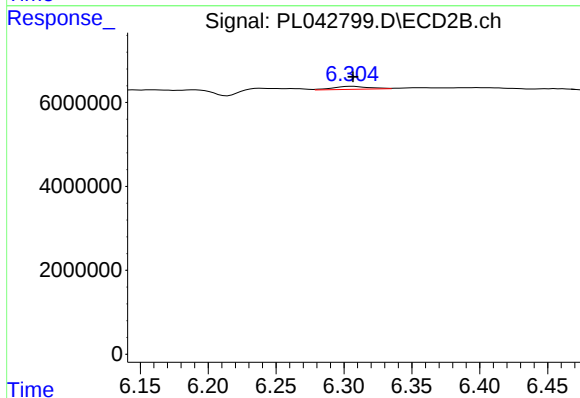


#11 alpha-Chlordane

R.T.: 6.306 min
Delta R.T.: 0.000 min
Response: 1285190
Conc: 0.38 ng/ml

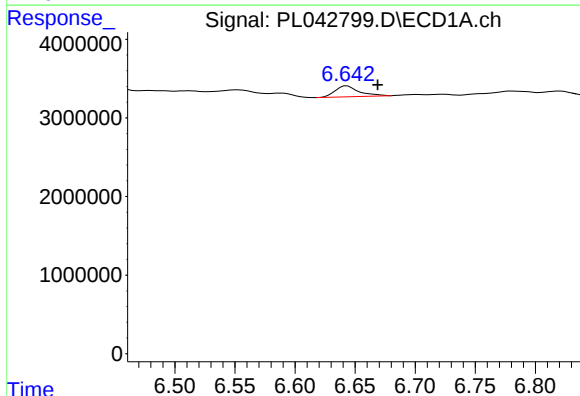


#19 Endosulfan Sulfate

R.T.: 6.643 min
Delta R.T.: -0.025 min
Response: 1915524
Conc: 0.31 ng/ml

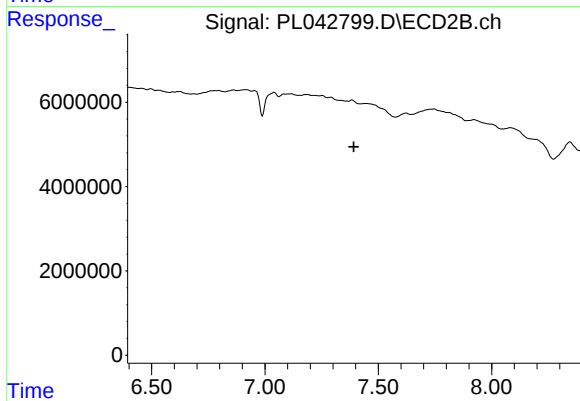

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.392 min
Response: 0
Conc: N.D.

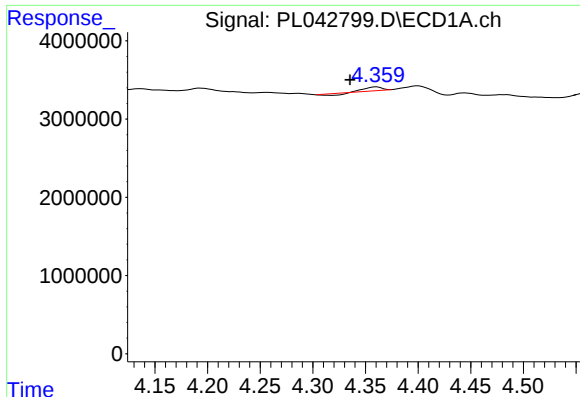

#23 Chlordane-1


R.T.: 4.361 min
Delta R.T.: 0.025 min
Response: 297321
Conc: 1.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

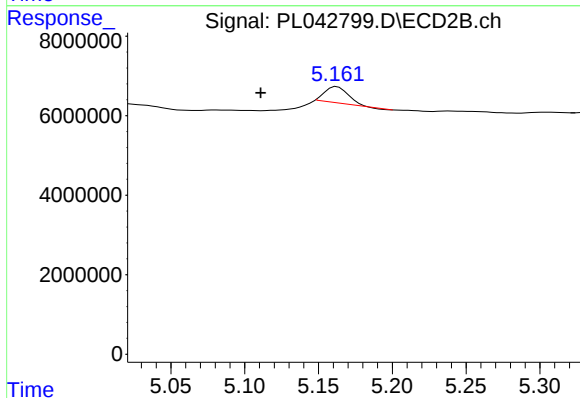


#23 Chlordane-1

R.T.: 5.163 min
Delta R.T.: 0.052 min
Response: 4034840
Conc: 30.35 ng/ml

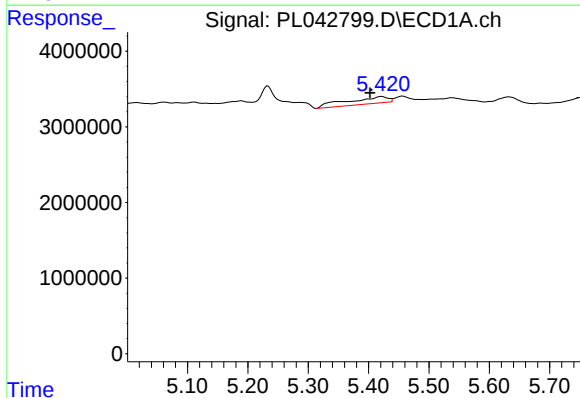


#25 Chlordane-3

R.T.: 5.421 min
Delta R.T.: 0.019 min
Response: 4207812
Conc: 4.80 ng/ml

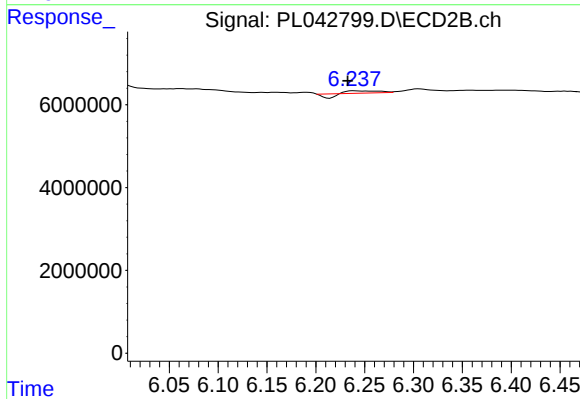

#25 Chlordane-3


R.T.: 6.238 min
Delta R.T.: 0.006 min
Response: 549103
Conc: 1.17 ng/ml

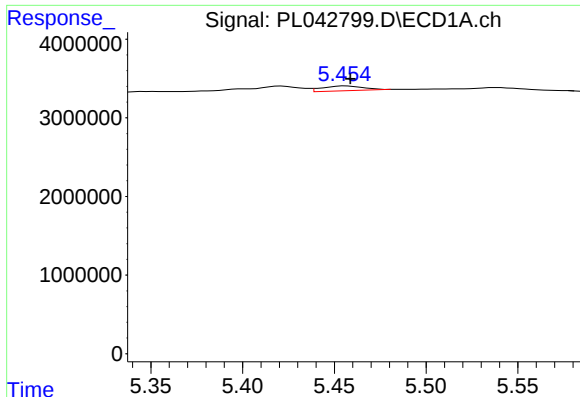

#26 Chlordane-4


R.T.: 5.457 min
Delta R.T.: -0.002 min
Response: 951193
Conc: 1.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

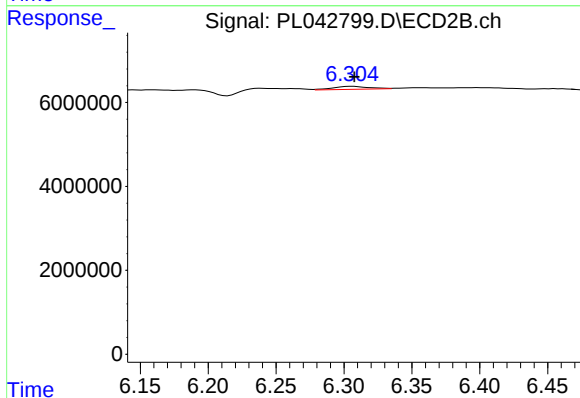


#26 Chlordane-4

R.T.: 6.306 min
Delta R.T.: -0.002 min
Response: 1285190
Conc: 2.35 ng/ml

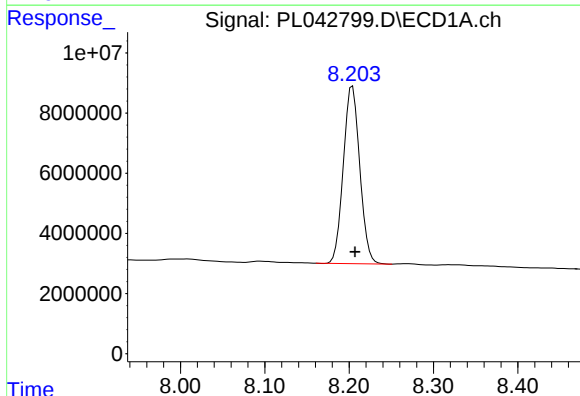

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.003 min
Response: 79937168
Conc: 12.68 ng/ml

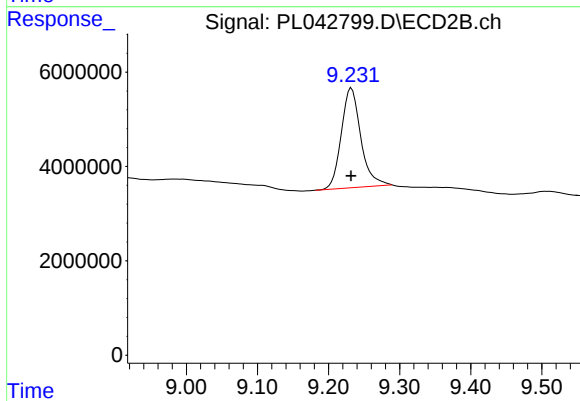

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.000 min
Response: 40435265
Conc: 16.77 ng/ml