

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120418\
 Data File : PL042786.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2018 20:18
 Operator : AJ\SJ
 Sample : J6204-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HLSP-SB-7A-(0-2)

Manual Integrations
 APPROVED

mohammad
 12/5/2018 4:43:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 00:10:30 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.467	4.102	120.0E6	60765835	20.390	21.128
28) SA Decachlor...	8.204	9.233	97196796	41779798	15.423	17.323
Target Compounds						
12) B 4,4'-DDE	5.622	6.460	3815887	4183454	0.583m	1.257 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120418\
Data File : PL042786.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2018 20:18
Operator : AJ\SJ
Sample : J6204-11
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HLSP-SB-7A-(0-2)


Manual Integrations
APPROVED

mohammad
12/5/2018 4:43:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 00:10:30 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

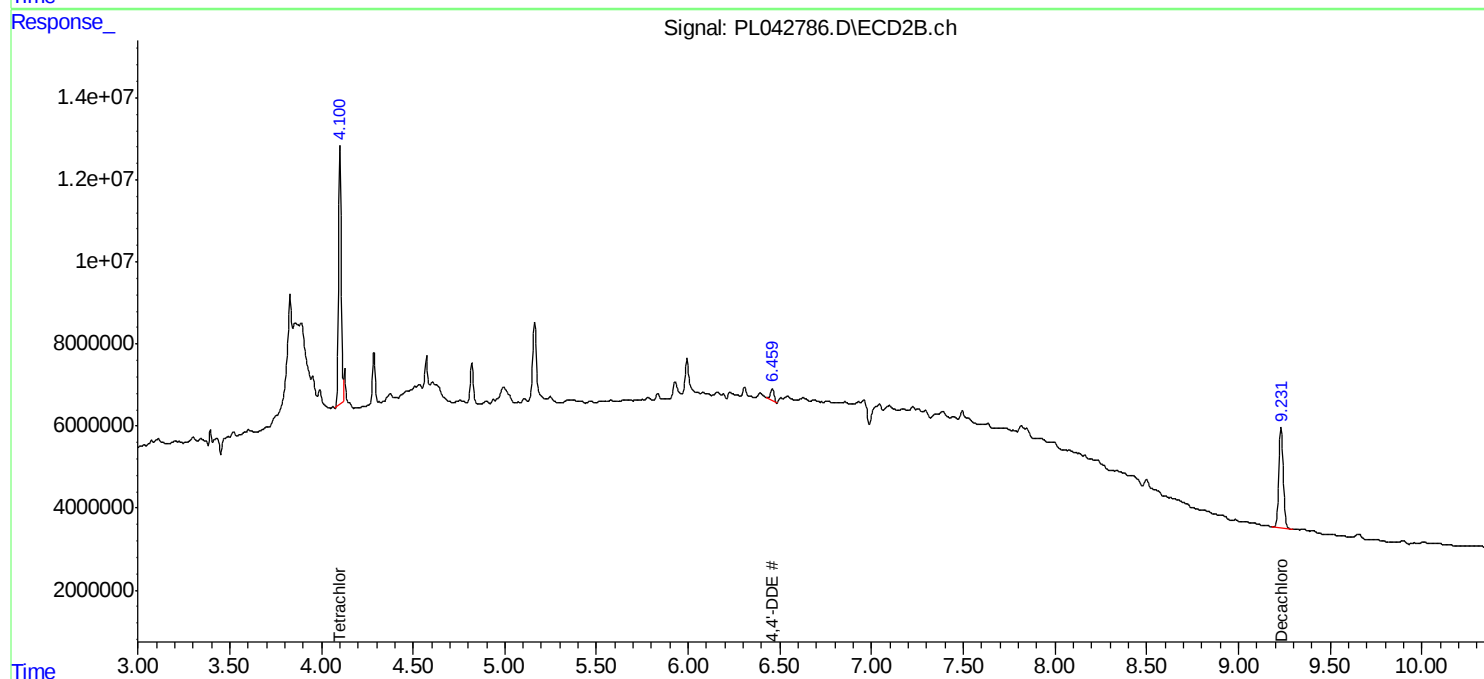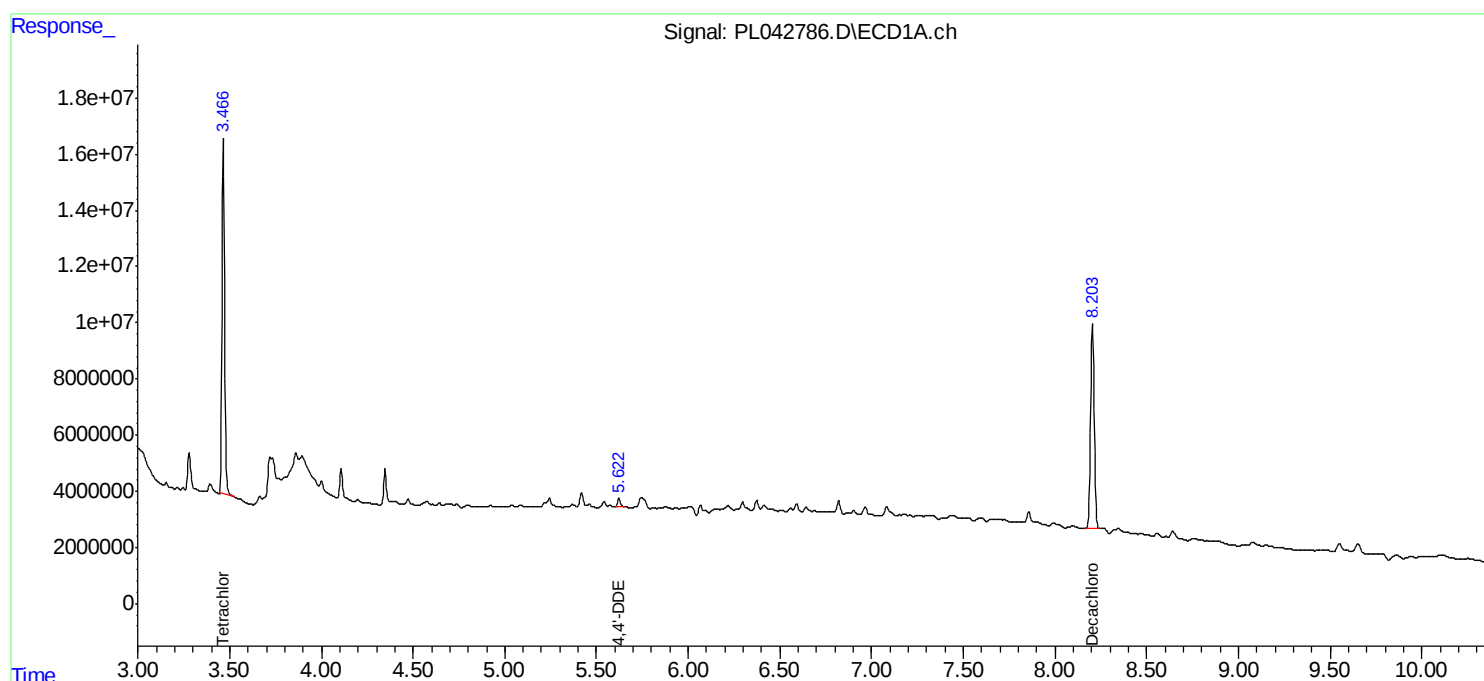

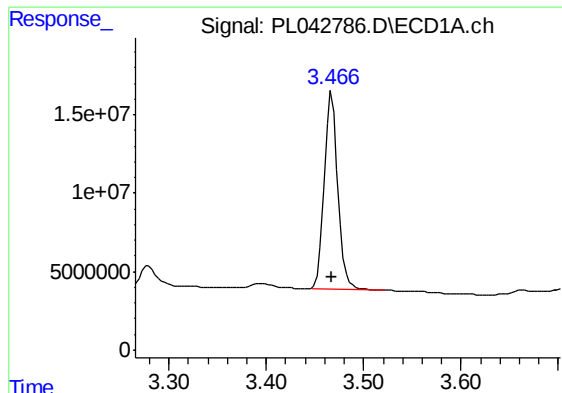


#1 Tetrachloro-m-xylene

R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 119964579
Conc: 20.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
HLSP-SB-7A-(0-2)


Manual Integrations
APPROVED

mohammad
12/5/2018 4:43:41 PM

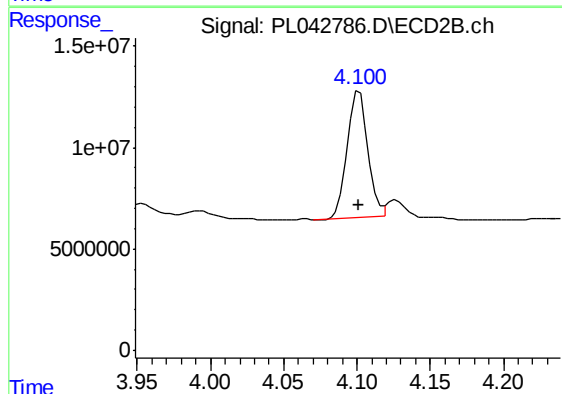


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 60765835
Conc: 21.13 ng/ml

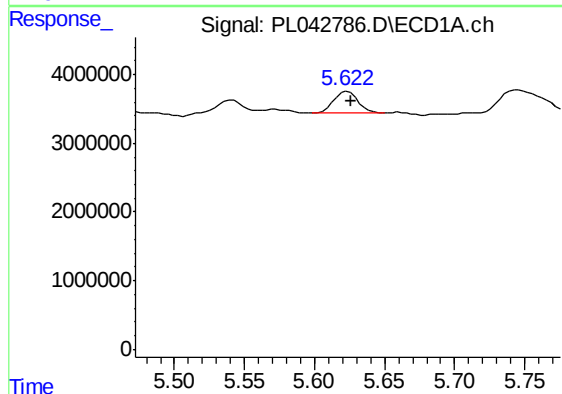


#12 4,4'-DDE

R.T.: 5.622 min
Delta R.T.: -0.004 min
Response: 3815887
Conc: 0.58 ng/ml m

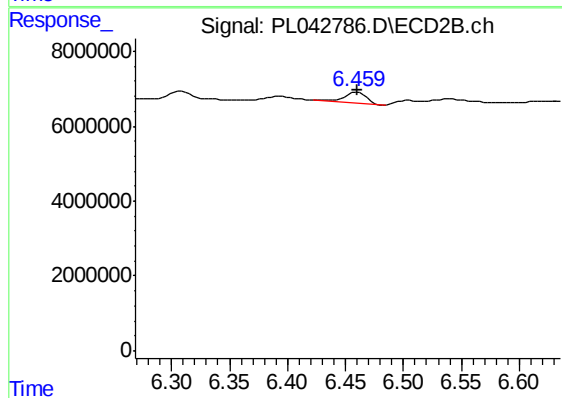

#12 4,4'-DDE

R.T.: 6.460 min
Delta R.T.: 0.000 min
Response: 4183454
Conc: 1.26 ng/ml

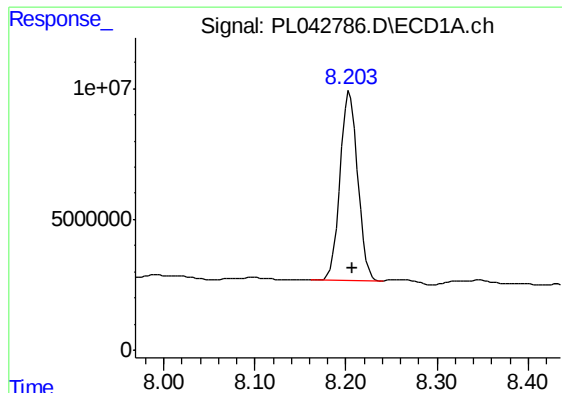


#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.003 min
Response: 97196796
Conc: 15.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
HLSP-SB-7A-(0-2)

Manual Integrations
APPROVED

mohammad
12/5/2018 4:43:41 PM

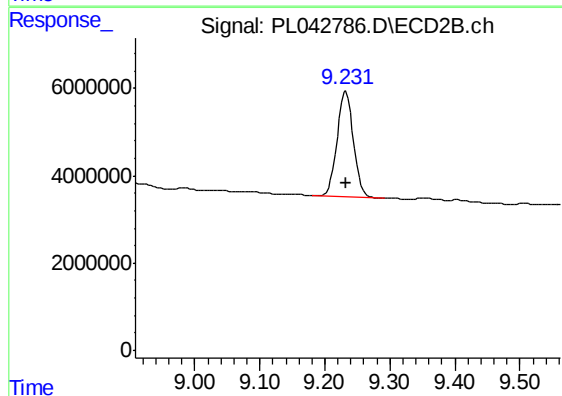

#28 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: 0.001 min
Response: 41779798
Conc: 17.32 ng/ml