

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120418\
 Data File : PL042791.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2018 21:29
 Operator : AJ\SJ
 Sample : J6206-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HLSP-SB-5A-(0-2)

Manual Integrations
 APPROVED

mohammad
 12/5/2018 4:43:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 00:11:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.102	97237770	51761259	16.527	17.997
28)	SA Decachlor...	8.204	9.231	74935127	31885939	11.890	13.221
Target Compounds							
17)	MA 4,4'-DDT	6.375	7.252	4884852	2347564	0.877	0.889m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120418\
Data File : PL042791.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2018 21:29
Operator : AJ\SJ
Sample : J6206-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HLSP-SB-5A-(0-2)


Manual Integrations
APPROVED

mohammad
12/5/2018 4:43:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 00:11:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

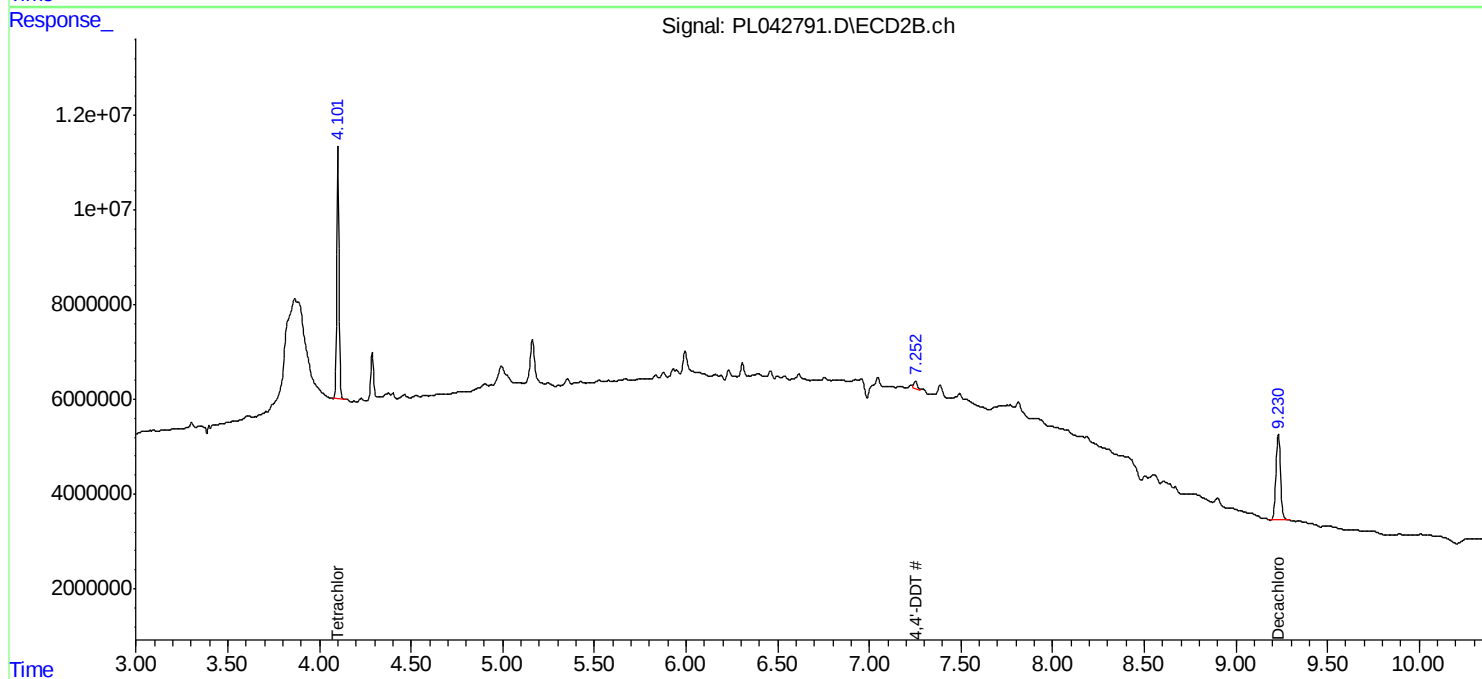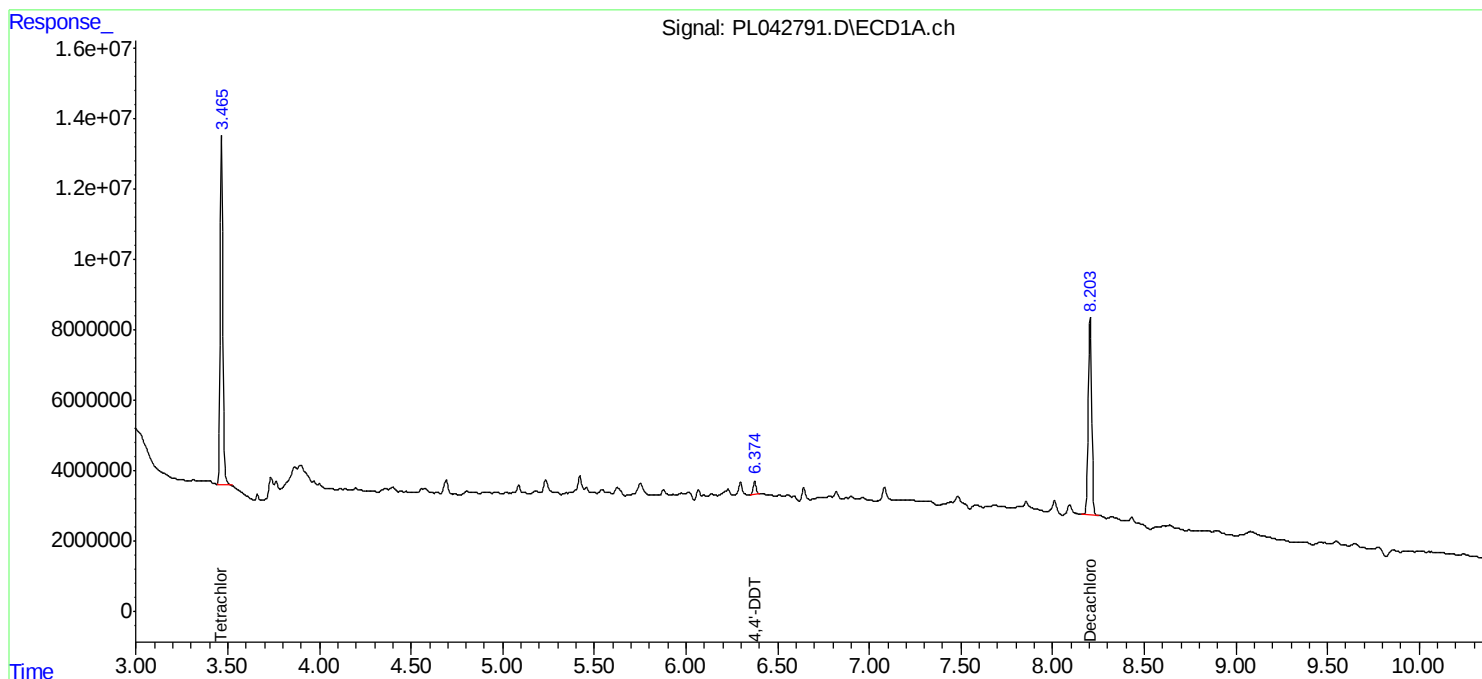

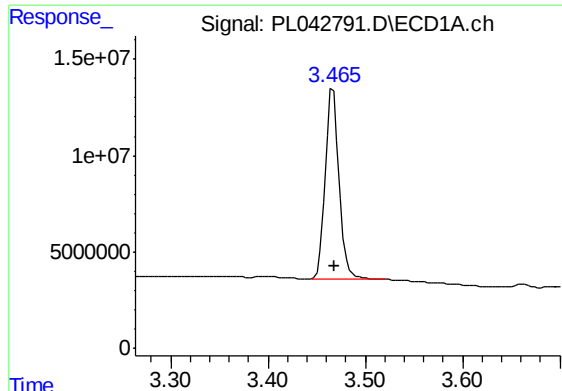


#1 Tetrachloro-m-xylene

R.T.: 3.467 min
Delta R.T.: -0.001 min
Response: 97237770
Conc: 16.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
HLSP-SB-5A-(0-2)


Manual Integrations
APPROVED

mohammad
12/5/2018 4:43:47 PM

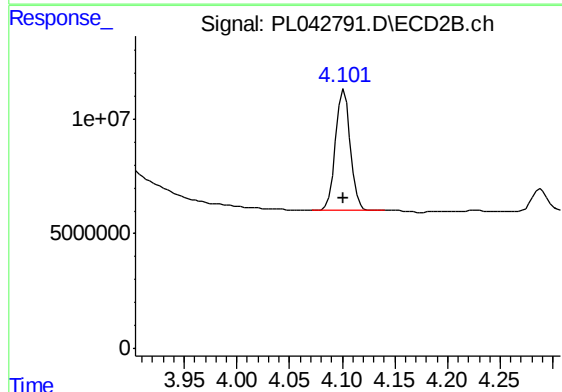


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 51761259
Conc: 18.00 ng/ml

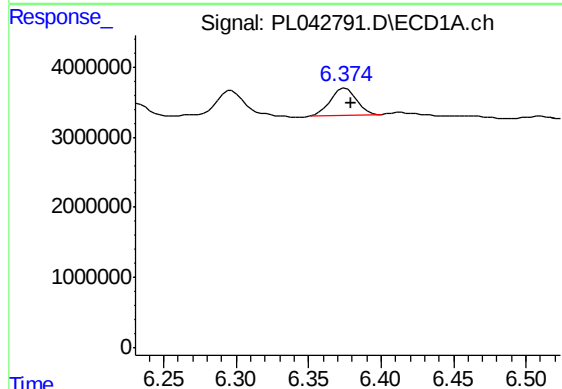


#17 4,4'-DDT

R.T.: 6.375 min
Delta R.T.: -0.004 min
Response: 4884852
Conc: 0.88 ng/ml

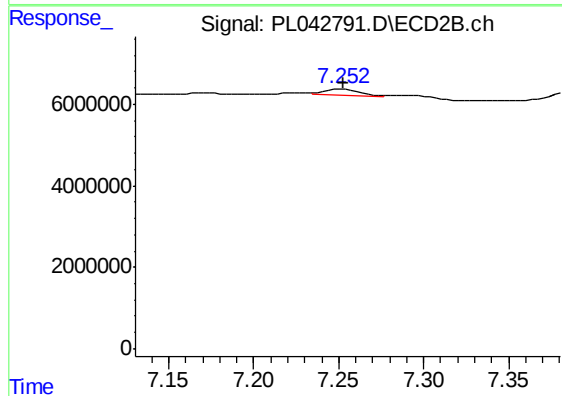

#17 4,4'-DDT

R.T.: 7.252 min
Delta R.T.: -0.001 min
Response: 2347564
Conc: 0.89 ng/ml m

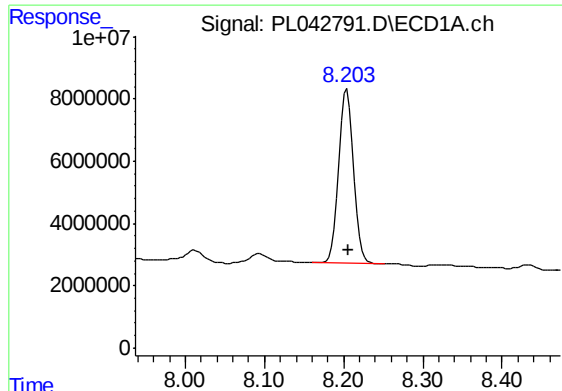


#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.003 min
Response: 74935127
Conc: 11.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
HLSP-SB-5A-(0-2)

Manual Integrations
APPROVED

mohammad
12/5/2018 4:43:47 PM

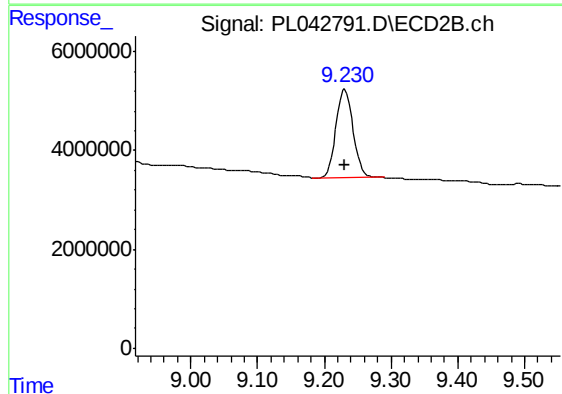

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.000 min
Response: 31885939
Conc: 13.22 ng/ml