

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120419\
 Data File : PL054751.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2019 14:35
 Operator : SG\AJ
 Sample : PB125230BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 00:12:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	4.052	191.3E6	50711693	16.439	19.873
28)	SA Decachlor...	8.332	9.162	188.7E6	49607959	19.701	20.692
Target Compounds							
6)	B beta-BHC	4.491f	0.000	4153426	0	0.560	N.D. #
8)	B Heptachlo...	5.275	0.000	23169545	0	1.532	N.D. #
10)	B gamma-Chl...	5.513	0.000	7121971	0	0.470	N.D. #
11)	B alpha-Chl...	5.549	0.000	18234544	0	1.237	N.D. #
12)	B 4,4'-DDE	5.699f	6.401	958971	431757	0.072	0.174 #
13)	MA Dieldrin	5.856	0.000	24027811	0	1.694	N.D. #
25)	Chlordane-3	5.513	0.000	7121971	0	5.546	N.D. #
26)	Chlordane-4	5.549	0.000	18234544	0	17.263	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120419\
Data File : PL054751.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2019 14:35
Operator : SG\AJ
Sample : PB125230BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 00:12:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

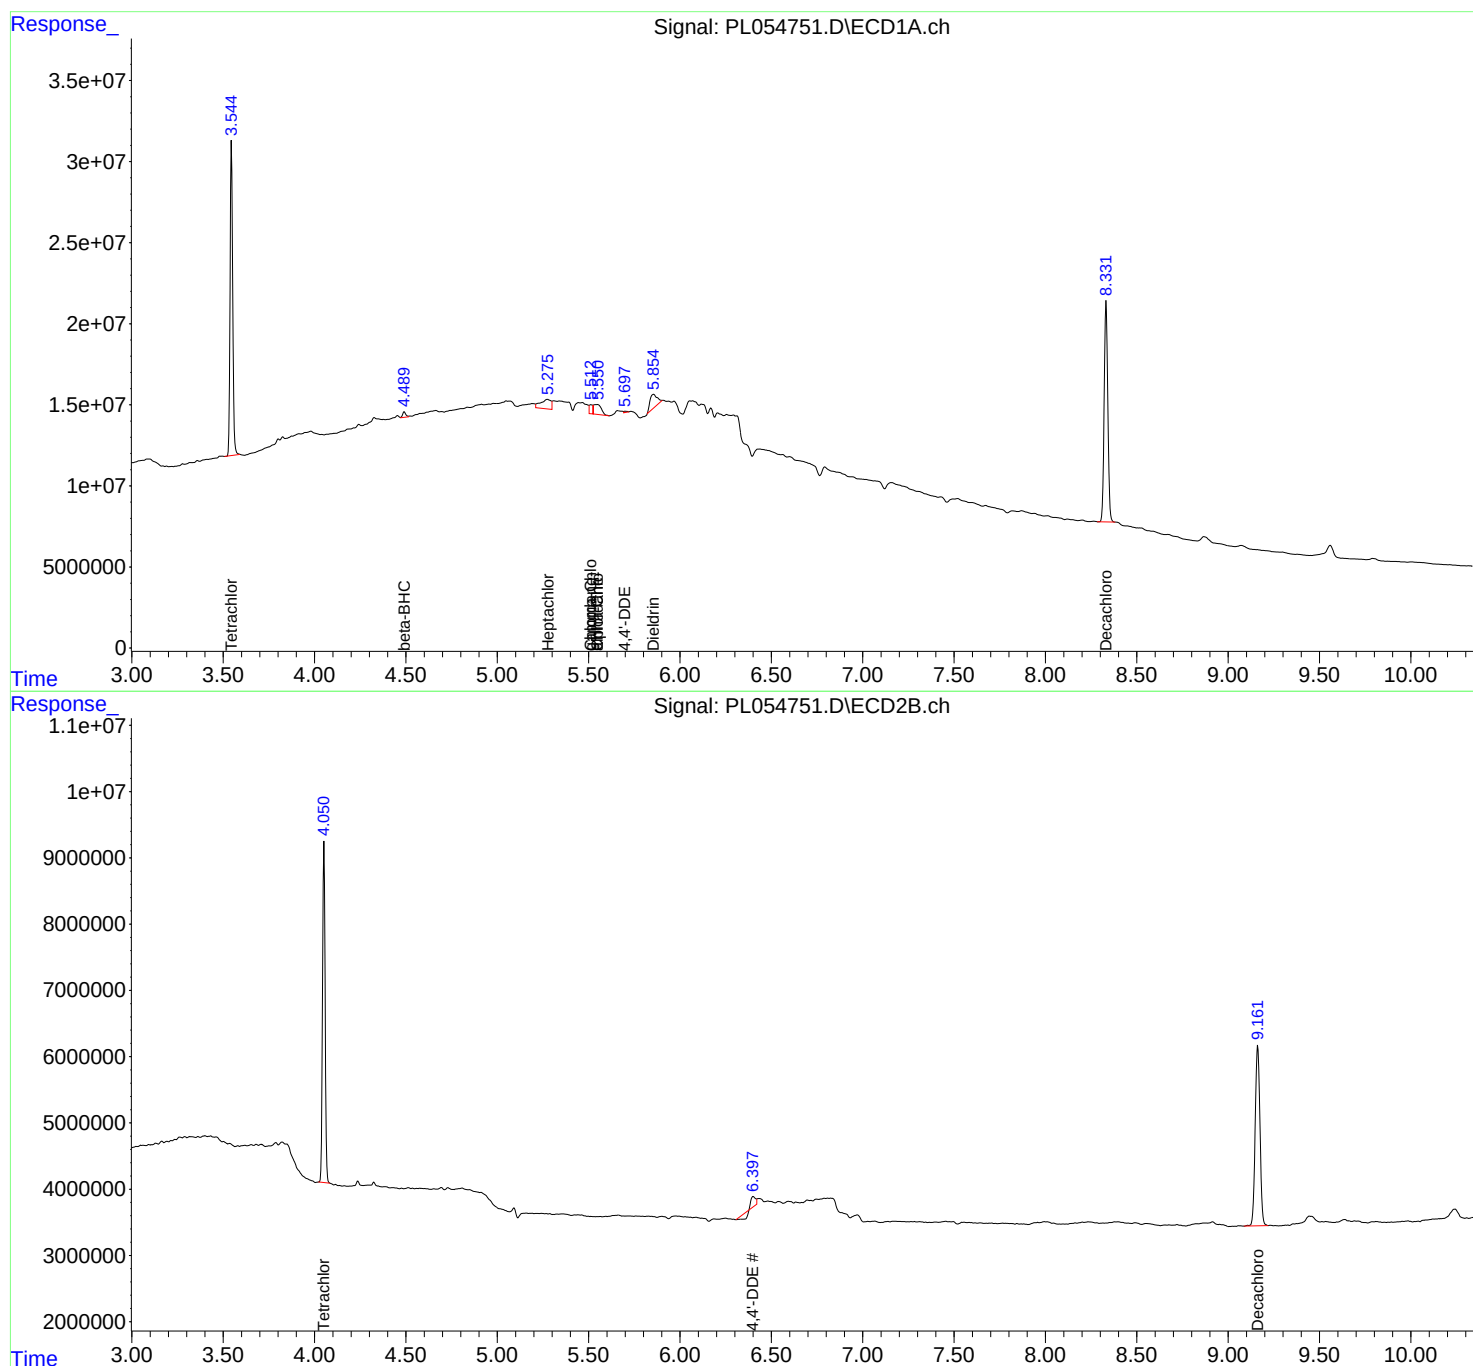


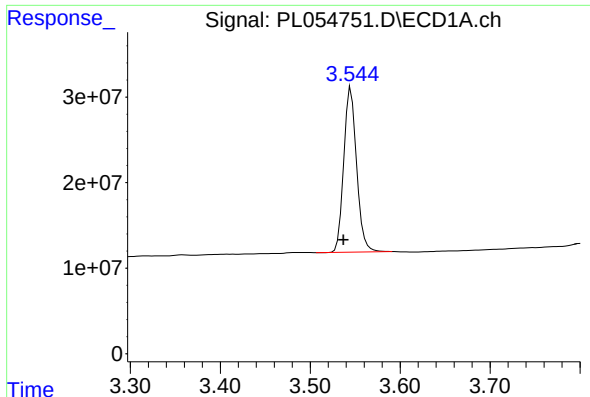

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: 0.008 min
Response: 191253643
Conc: 16.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

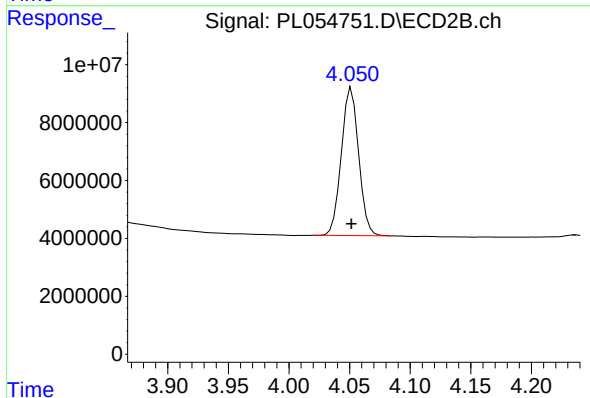


#1 Tetrachloro-m-xylene

R.T.: 4.052 min
Delta R.T.: 0.000 min
Response: 50711693
Conc: 19.87 ng/ml

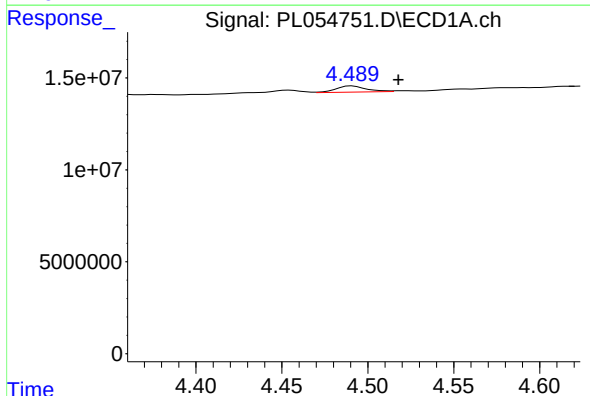


#6 beta-BHC

R.T.: 4.491 min
Delta R.T.: -0.027 min
Response: 4153426
Conc: 0.56 ng/ml

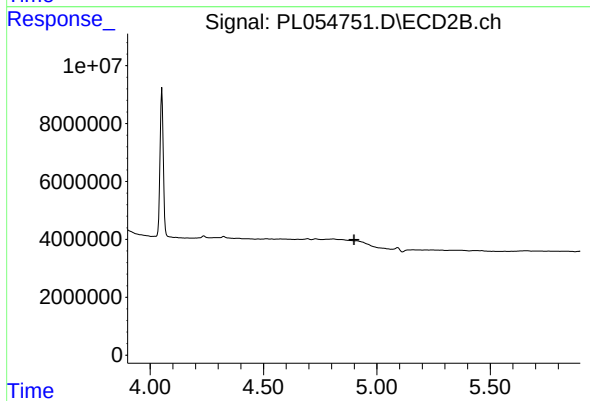

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.899 min
Response: 0
Conc: N.D.

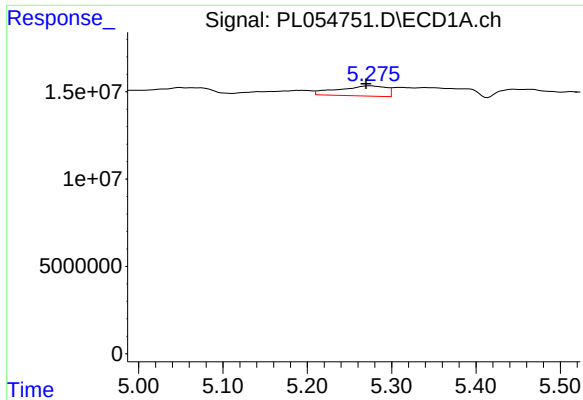

#8 Heptachlor epoxide


R.T.: 5.275 min
Delta R.T.: 0.006 min
Response: 23169545
Conc: 1.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

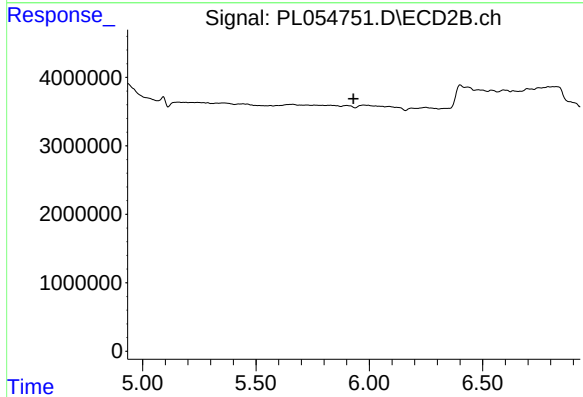


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.930 min
Response: 0
Conc: N.D.

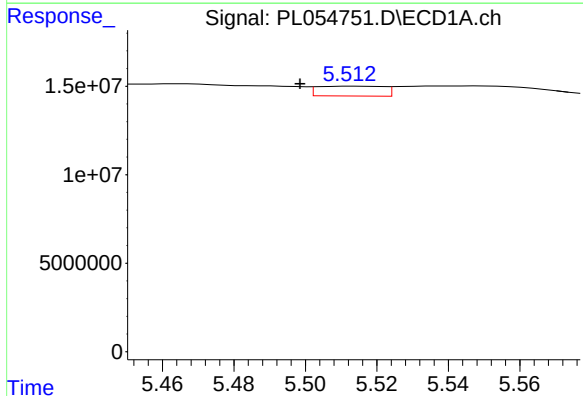


#10 gamma-Chlordane

R.T.: 5.513 min
Delta R.T.: 0.015 min
Response: 7121971
Conc: 0.47 ng/ml

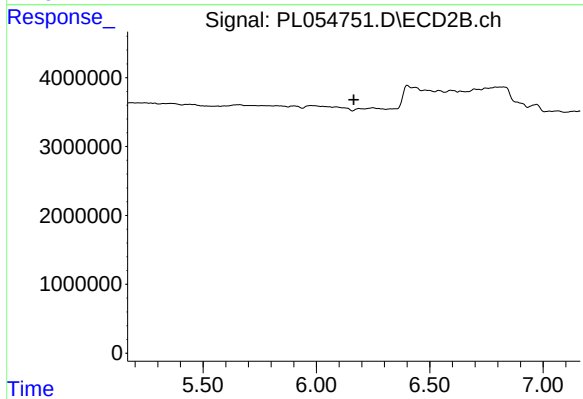

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.164 min
Response: 0
Conc: N.D.

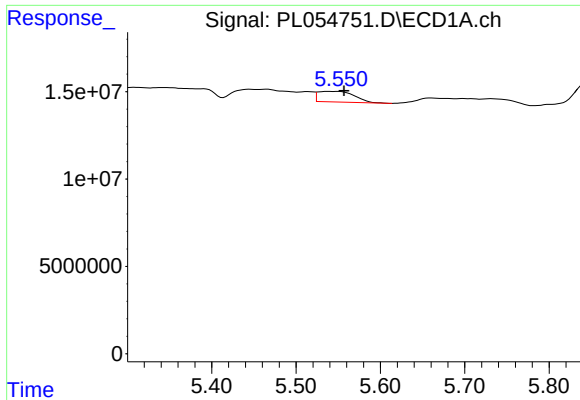

#11 alpha-Chlordane


R.T.: 5.549 min
Delta R.T.: -0.007 min
Response: 18234544
Conc: 1.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

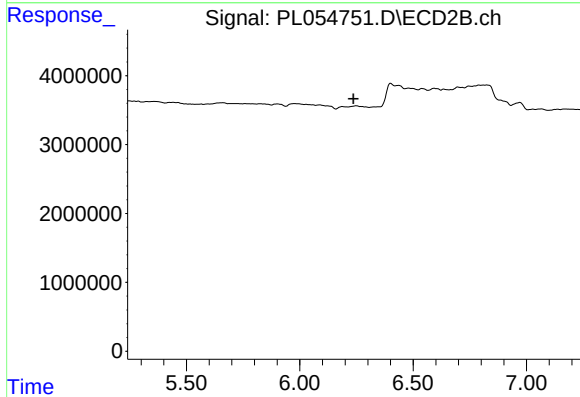


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

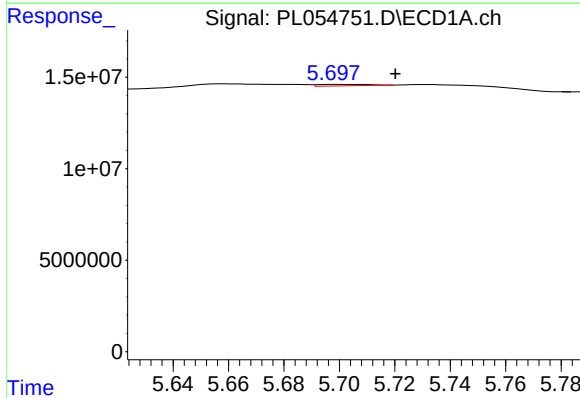


#12 4,4'-DDE

R.T.: 5.699 min
Delta R.T.: -0.021 min
Response: 958971
Conc: 0.07 ng/ml

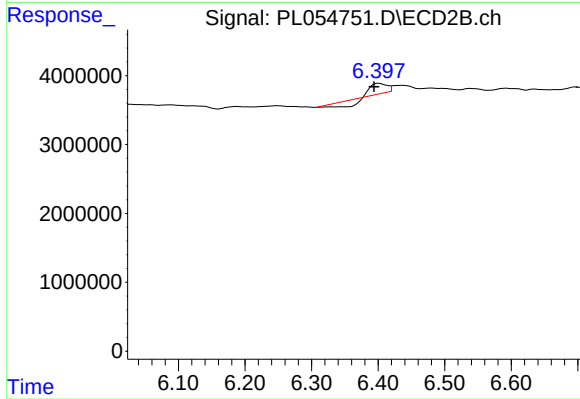

#12 4,4'-DDE


R.T.: 6.401 min
Delta R.T.: 0.007 min
Response: 431757
Conc: 0.17 ng/ml

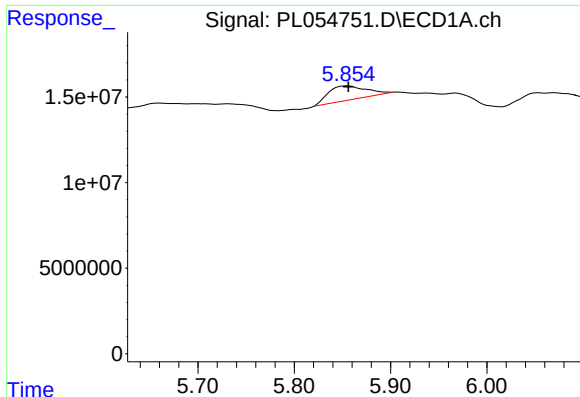

#13 Dieldrin


R.T.: 5.856 min
Delta R.T.: 0.000 min
Response: 24027811
Conc: 1.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

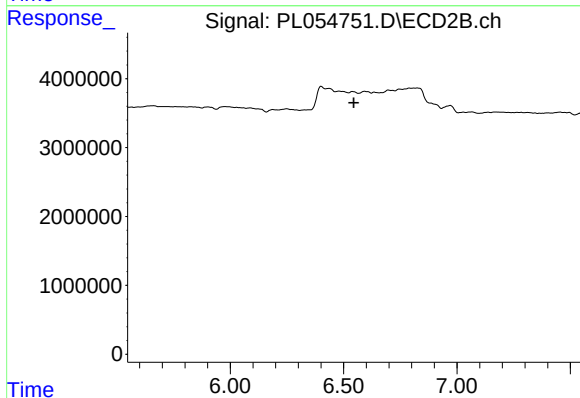


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.545 min
Response: 0
Conc: N.D.

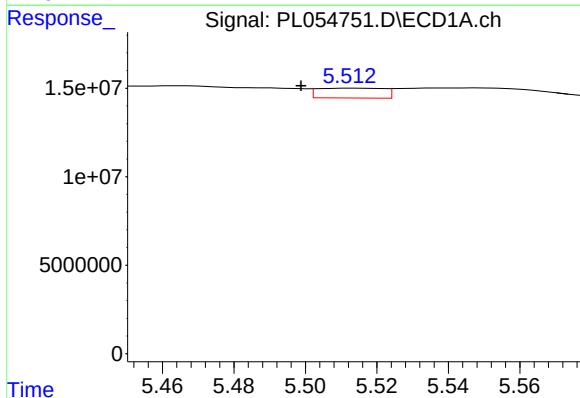


#25 Chlordane-3

R.T.: 5.513 min
Delta R.T.: 0.015 min
Response: 7121971
Conc: 5.55 ng/ml

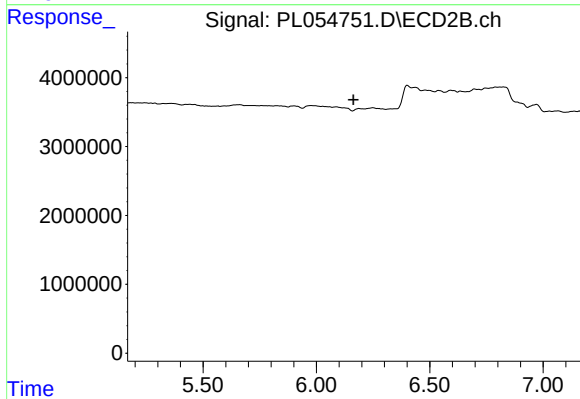

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.164 min
Response: 0
Conc: N.D.

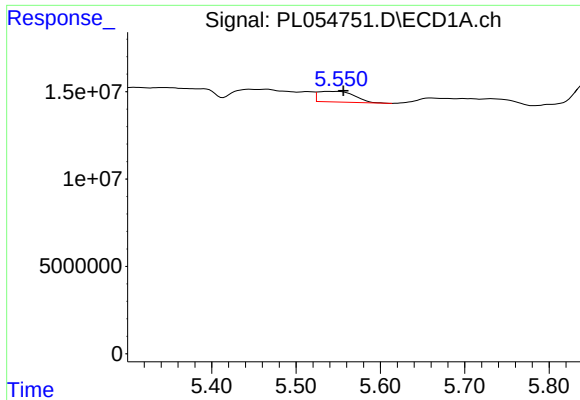

#26 Chlordane-4


R.T.: 5.549 min
Delta R.T.: -0.007 min
Response: 18234544
Conc: 17.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

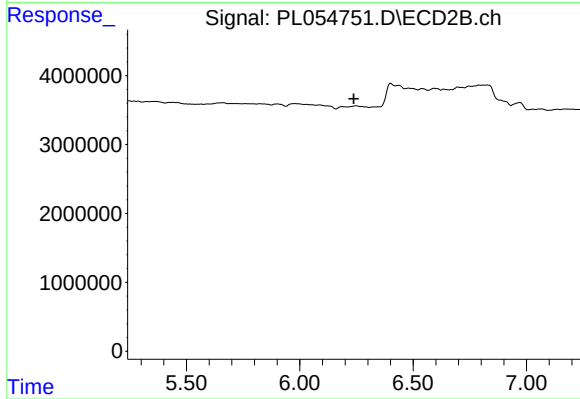


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.239 min
Response: 0
Conc: N.D.

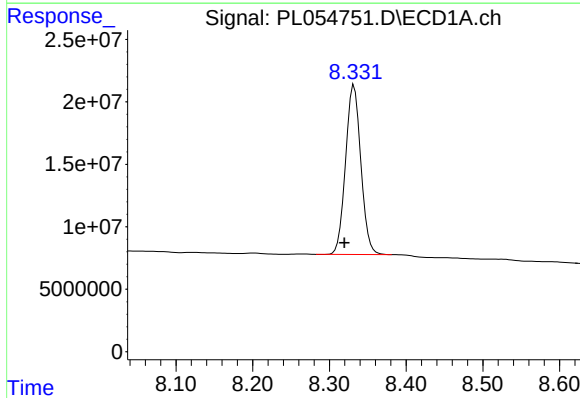

#28 Decachlorobiphenyl

R.T.: 8.332 min
Delta R.T.: 0.013 min
Response: 188661729
Conc: 19.70 ng/ml

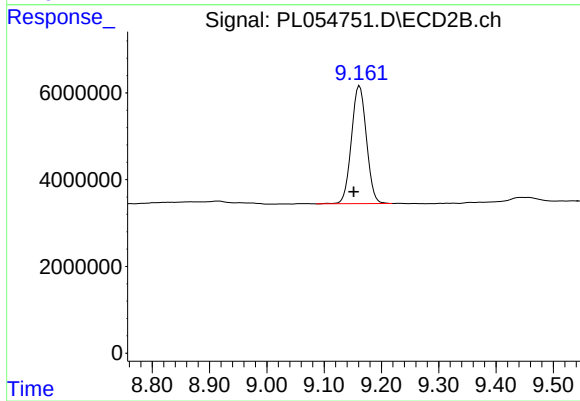

#28 Decachlorobiphenyl

R.T.: 9.162 min
Delta R.T.: 0.010 min
Response: 49607959
Conc: 20.69 ng/ml