

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120419\
 Data File : PL054772.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2019 19:55
 Operator : SG\AJ
 Sample : K6120-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 00:16:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	4.051	158.8E6	40292583	13.648	15.790
28)	SA Decachlor...	8.322	9.153	127.6E6	37552487	13.323	15.664
Target Compounds							
10)	B gamma-Chl...	5.497	0.000	2914303	0	0.192	N.D. #
11)	B alpha-Chl...	5.557	6.239	8882673	4882684	0.602	1.860 #
12)	B 4,4'-DDE	5.720	6.394	23671081	6396286	1.779	2.584 #
16)	A 4,4'-DDD	6.238	6.887	16643589	6536738	1.704	3.404 #
17)	MA 4,4'-DDT	6.480	7.186	254.0E6	60572923	24.244	30.572 #
20)	A Methoxychlor	7.011	0.000	3385183	0	0.675	N.D. #
23)	Chlordane-1	4.418	0.000	4155024	0	10.529	N.D. #
25)	Chlordane-3	5.497	0.000	2914303	0	2.269	N.D. #
26)	Chlordane-4	5.557	6.239	8882673	4882684	8.409	12.976 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120419\
Data File : PL054772.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2019 19:55
Operator : SG\AJ
Sample : K6120-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 00:16:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

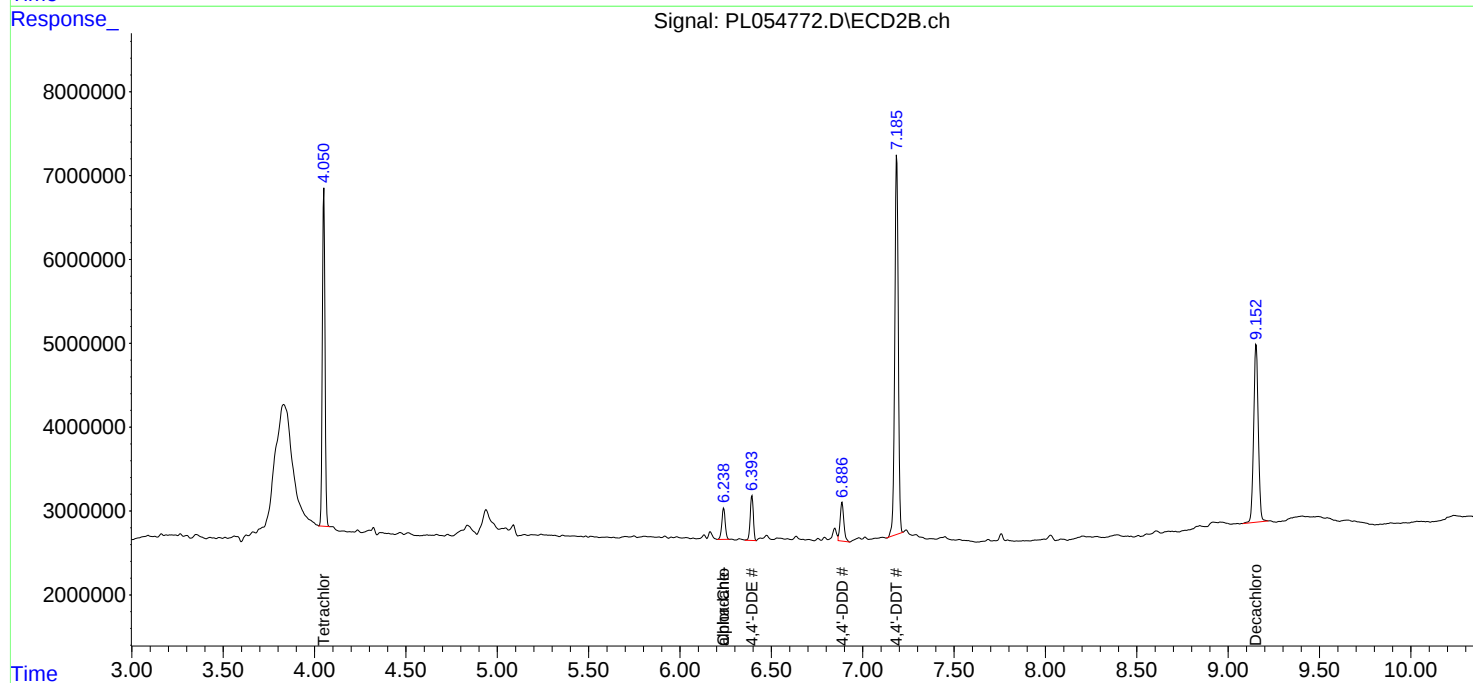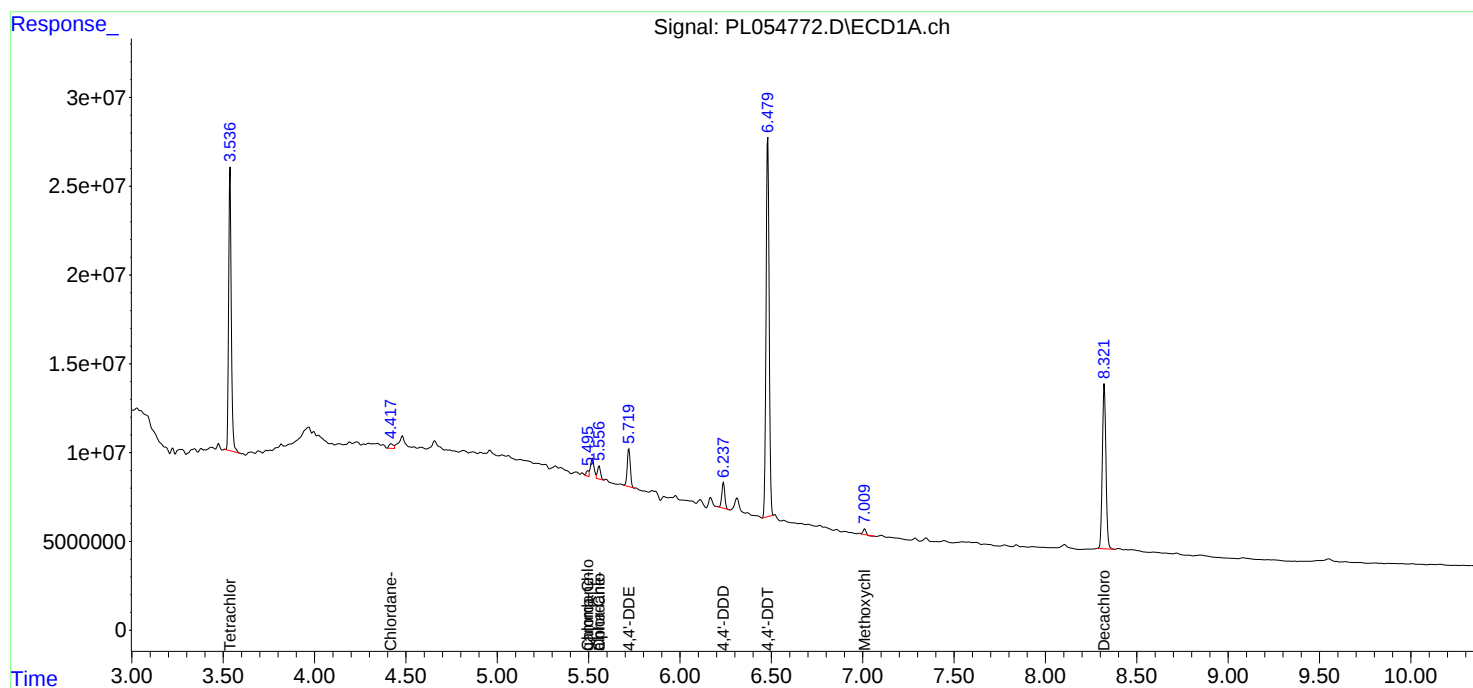


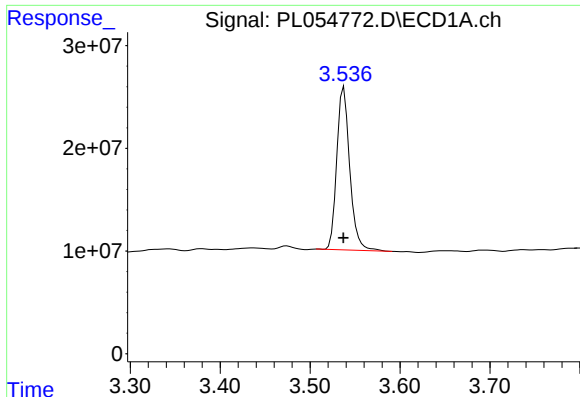

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 158778449
Conc: 13.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

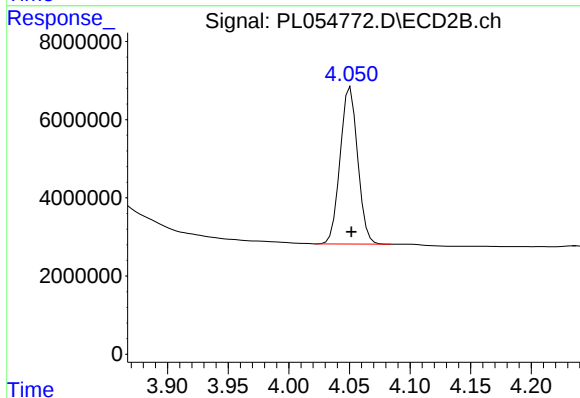


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 40292583
Conc: 15.79 ng/ml

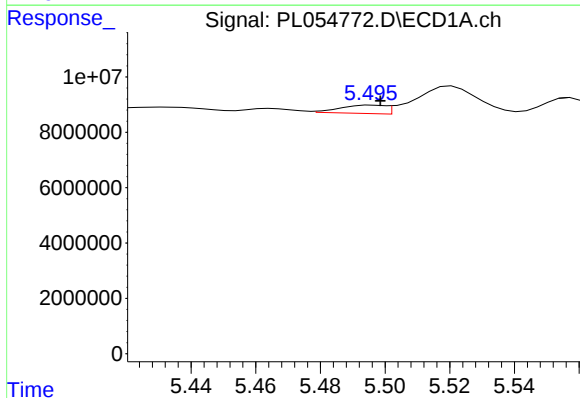


#10 gamma-Chlordane

R.T.: 5.497 min
Delta R.T.: -0.002 min
Response: 2914303
Conc: 0.19 ng/ml

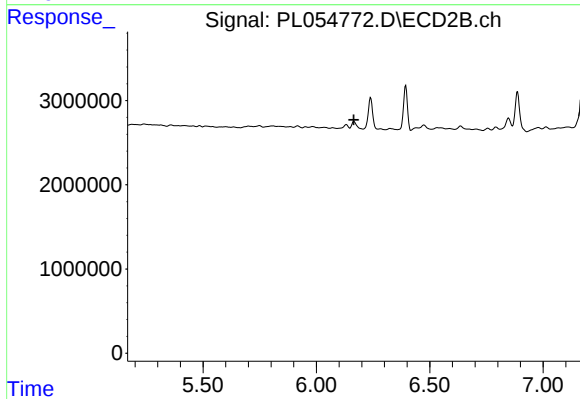

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.164 min
Response: 0
Conc: N.D.

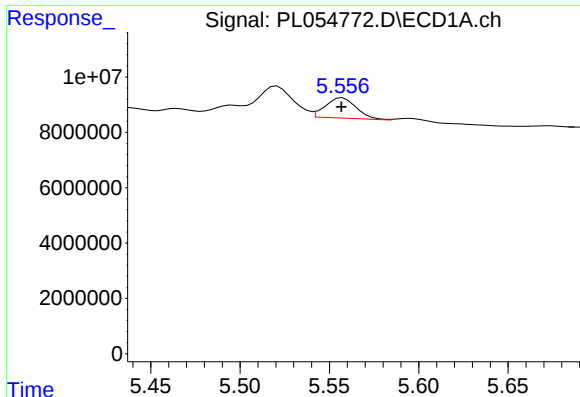

#11 alpha-Chlordane


R.T.: 5.557 min
Delta R.T.: 0.000 min
Response: 8882673
Conc: 0.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

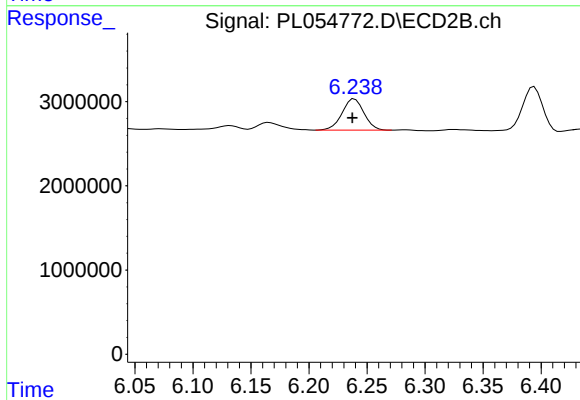


#11 alpha-Chlordane

R.T.: 6.239 min
Delta R.T.: 0.002 min
Response: 4882684
Conc: 1.86 ng/ml

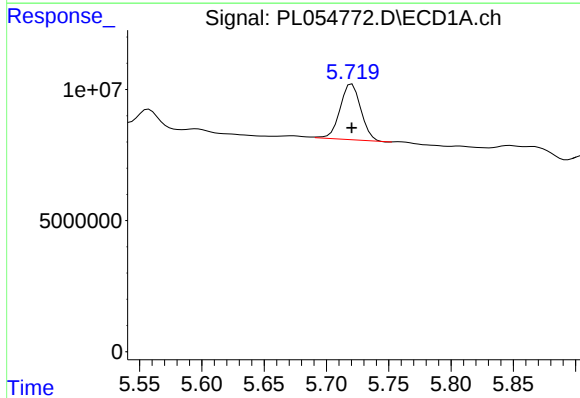


#12 4,4'-DDE

R.T.: 5.720 min
Delta R.T.: 0.000 min
Response: 23671081
Conc: 1.78 ng/ml

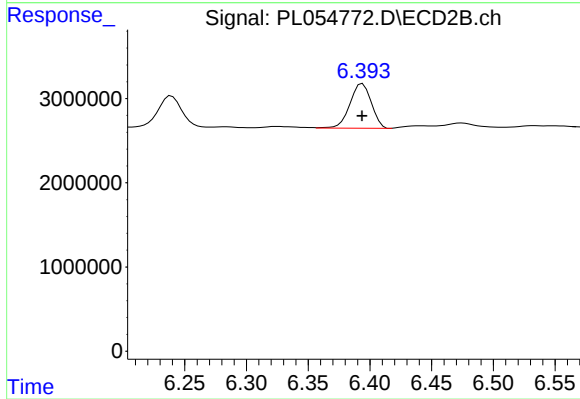

#12 4,4'-DDE


R.T.: 6.394 min
Delta R.T.: 0.000 min
Response: 6396286
Conc: 2.58 ng/ml

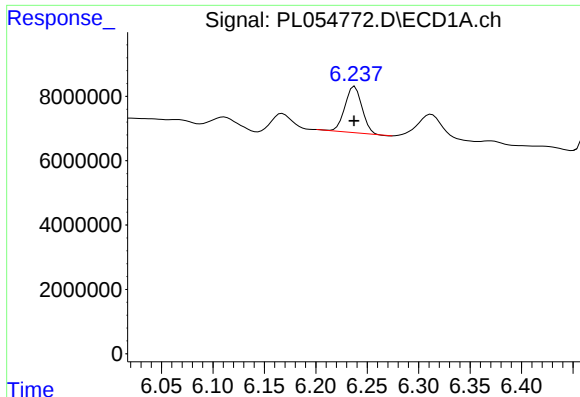

#16 4,4'-DDD


R.T.: 6.238 min
Delta R.T.: 0.000 min
Response: 16643589
Conc: 1.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

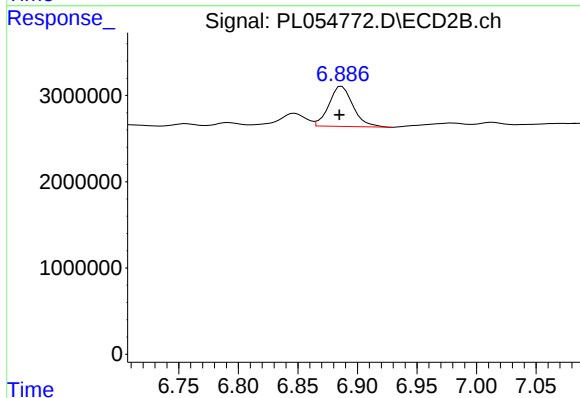


#16 4,4'-DDD

R.T.: 6.887 min
Delta R.T.: 0.002 min
Response: 6536738
Conc: 3.40 ng/ml

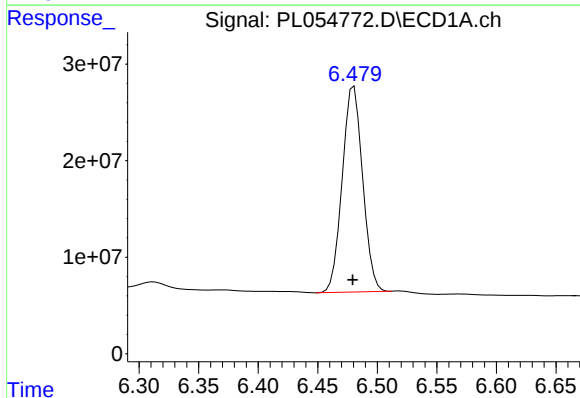


#17 4,4'-DDT

R.T.: 6.480 min
Delta R.T.: 0.001 min
Response: 253984031
Conc: 24.24 ng/ml

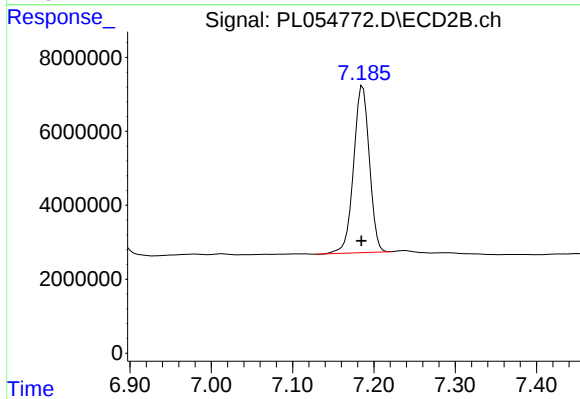

#17 4,4'-DDT


R.T.: 7.186 min
Delta R.T.: 0.002 min
Response: 60572923
Conc: 30.57 ng/ml

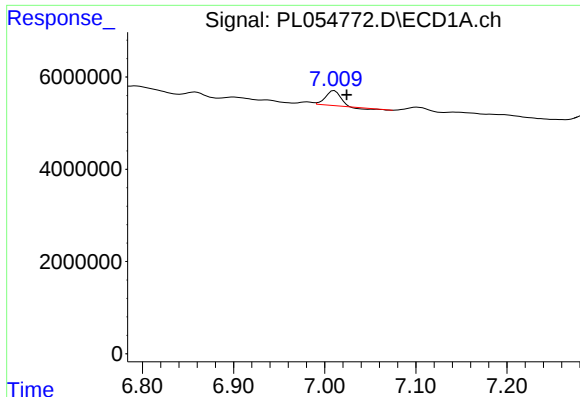

#20 Methoxychlor


R.T.: 7.011 min
Delta R.T.: -0.014 min
Response: 3385183
Conc: 0.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

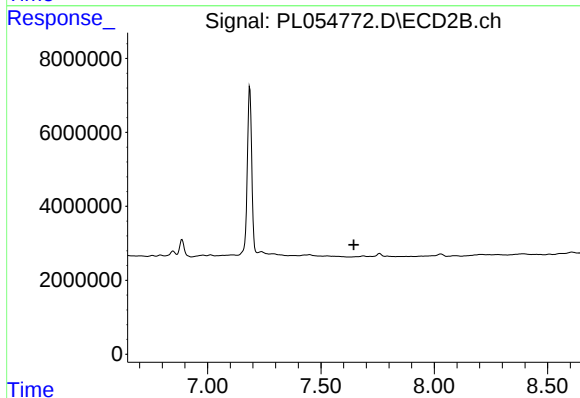


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.645 min
Response: 0
Conc: N.D.

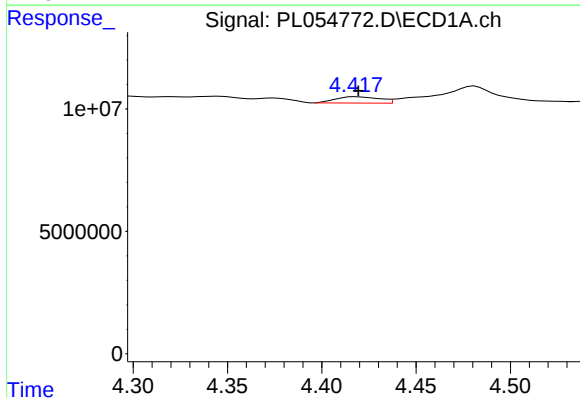


#23 Chlordane-1

R.T.: 4.418 min
Delta R.T.: -0.001 min
Response: 4155024
Conc: 10.53 ng/ml

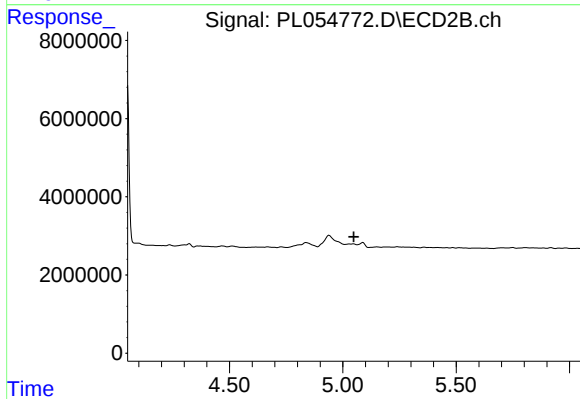

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.049 min
Response: 0
Conc: N.D.

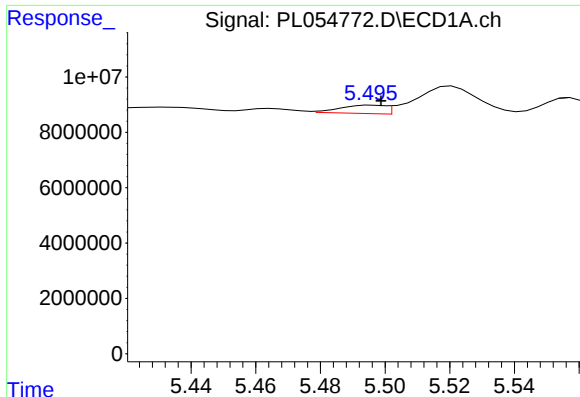

#25 Chlordane-3


R.T.: 5.497 min
Delta R.T.: -0.002 min
Response: 2914303
Conc: 2.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

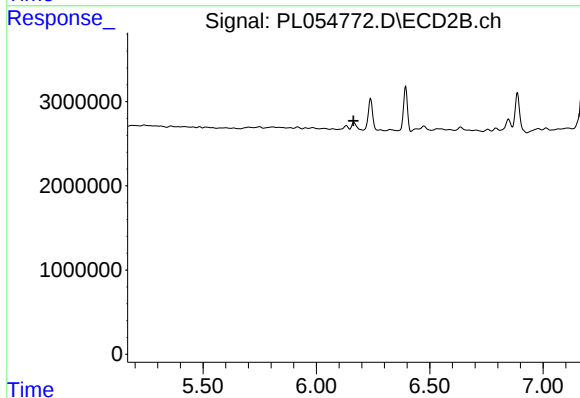


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.164 min
Response: 0
Conc: N.D.

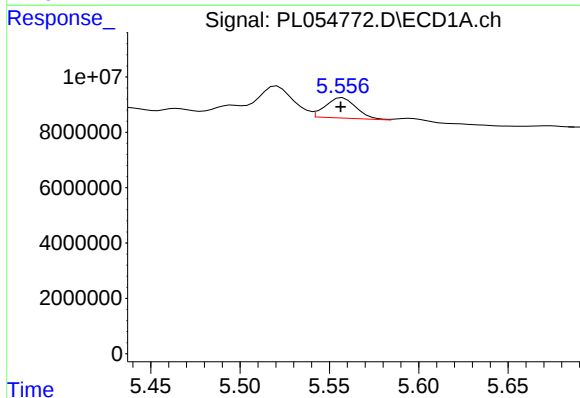


#26 Chlordane-4

R.T.: 5.557 min
Delta R.T.: 0.001 min
Response: 8882673
Conc: 8.41 ng/ml

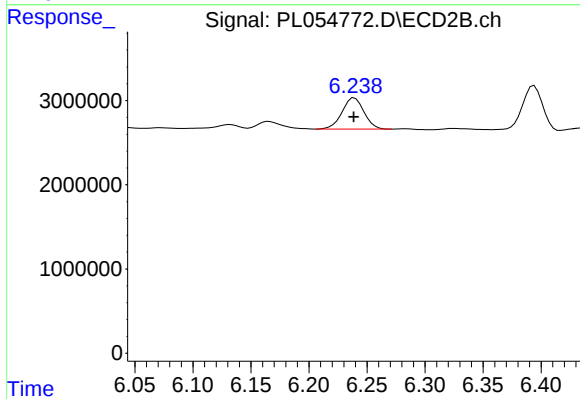

#26 Chlordane-4


R.T.: 6.239 min
Delta R.T.: 0.000 min
Response: 4882684
Conc: 12.98 ng/ml

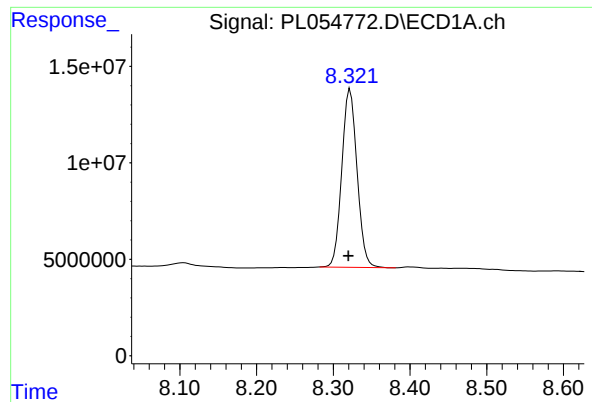

#28 Decachlorobiphenyl

R.T.: 8.322 min
Delta R.T.: 0.002 min
Response: 127580491
Conc: 13.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

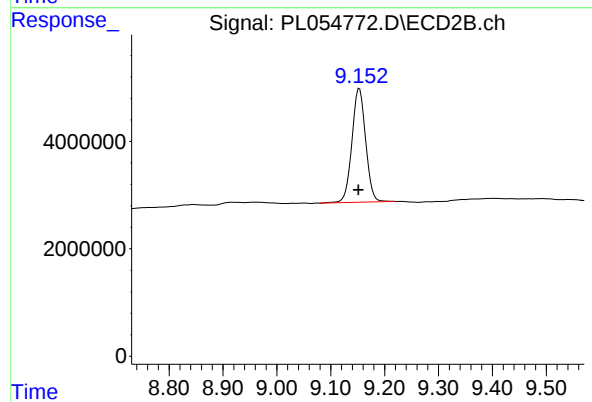

#28 Decachlorobiphenyl

R.T.: 9.153 min
Delta R.T.: 0.002 min
Response: 37552487
Conc: 15.66 ng/ml