

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120419\
 Data File : PL054774.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2019 20:23
 Operator : SG\AJ
 Sample : K6120-05
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 00:17:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	4.051	150.4E6	37560813	12.931	14.719
28)	SA Decachlor...	8.322	9.153	104.8E6	31420901	10.949	13.106
Target Compounds							
15)	B Endosulfa...	6.381	0.000	23241324	0	1.921	N.D. #
27)	Chlordane-5	6.381f	0.000	23241324	0	61.730	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120419\
Data File : PL054774.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2019 20:23
Operator : SG\AJ
Sample : K6120-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 00:17:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

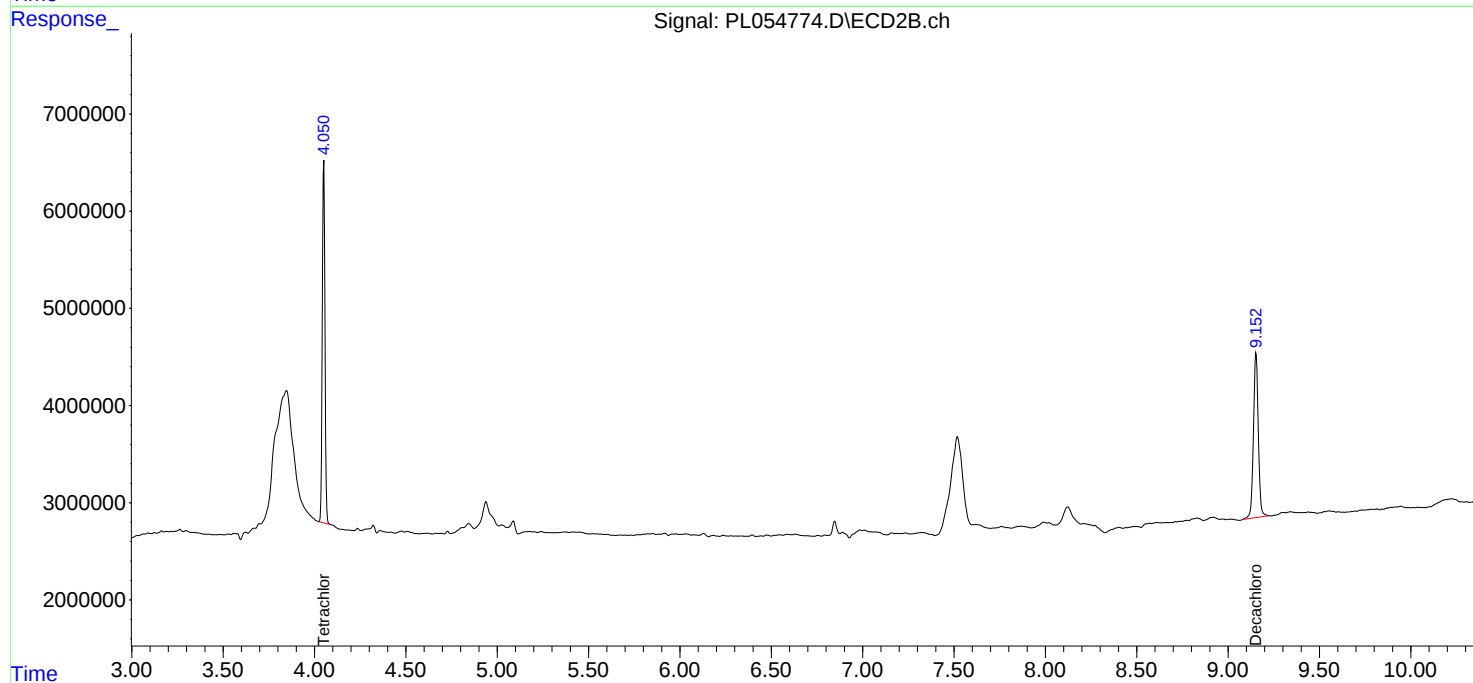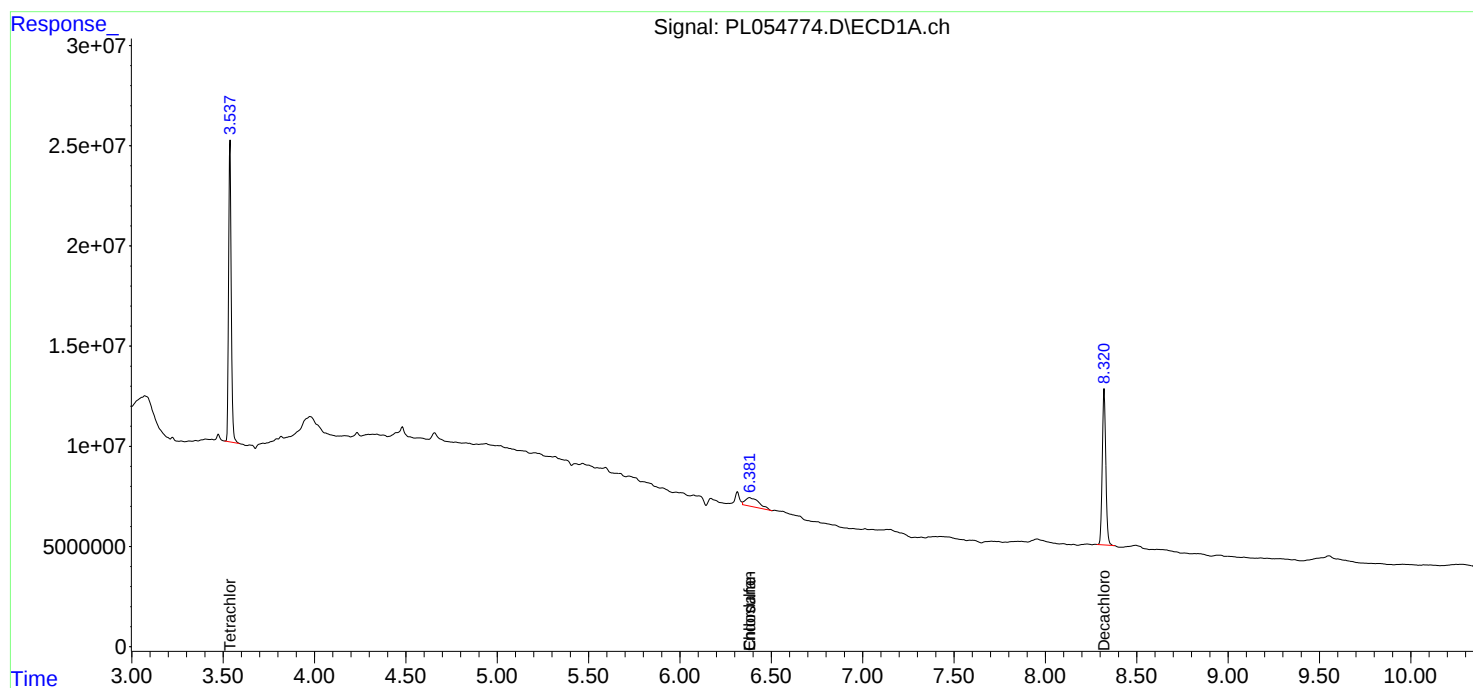


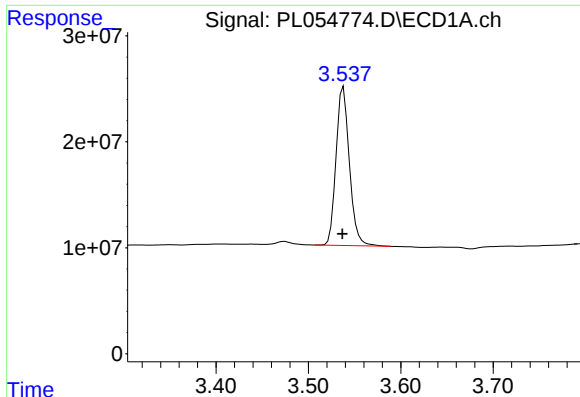

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 150437550
Conc: 12.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

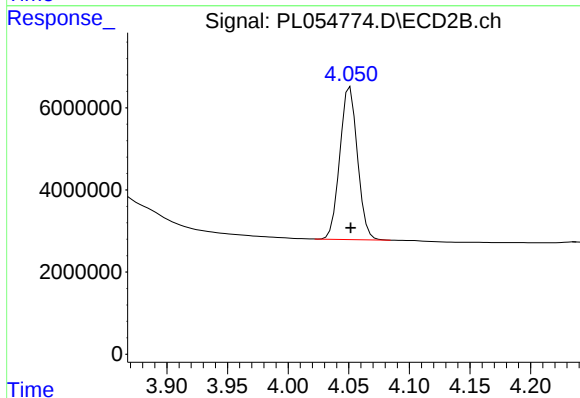


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 37560813
Conc: 14.72 ng/ml

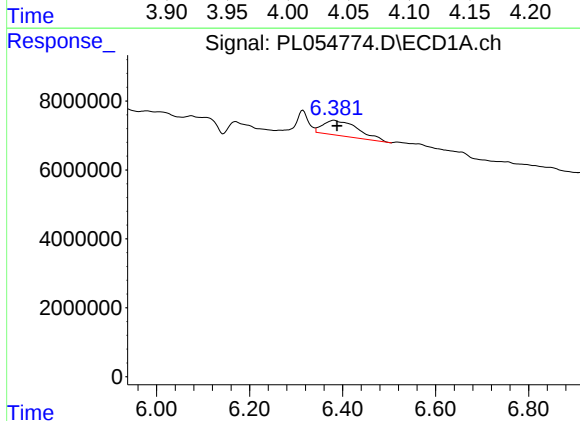


#15 Endosulfan II

R.T.: 6.381 min
Delta R.T.: -0.006 min
Response: 23241324
Conc: 1.92 ng/ml

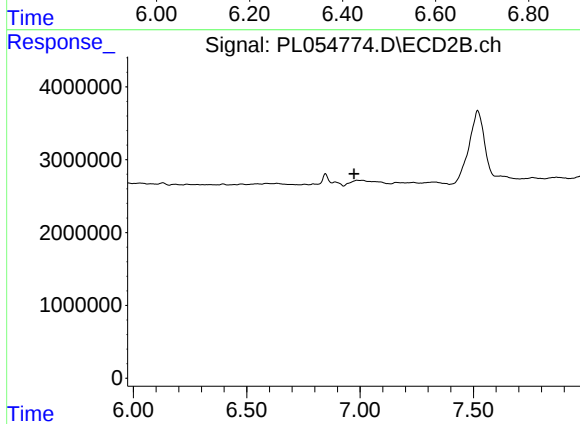

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.974 min
Response: 0
Conc: N.D.

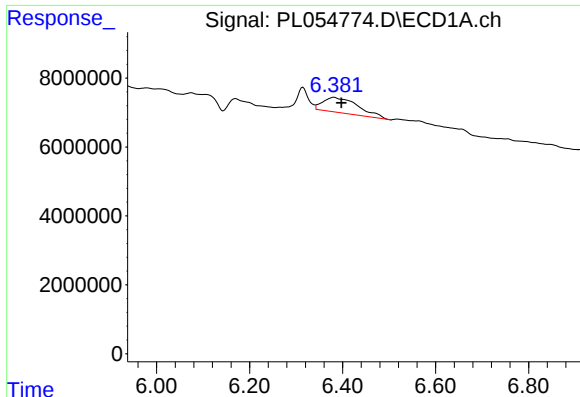

#27 Chlordane-5


R.T.: 6.381 min
Delta R.T.: -0.016 min
Response: 23241324
Conc: 61.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

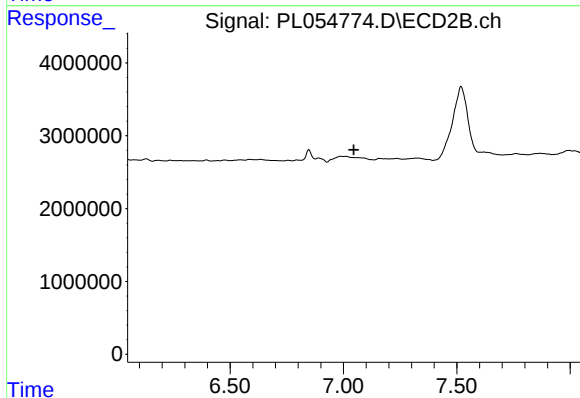


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.045 min
Response: 0
Conc: N.D.

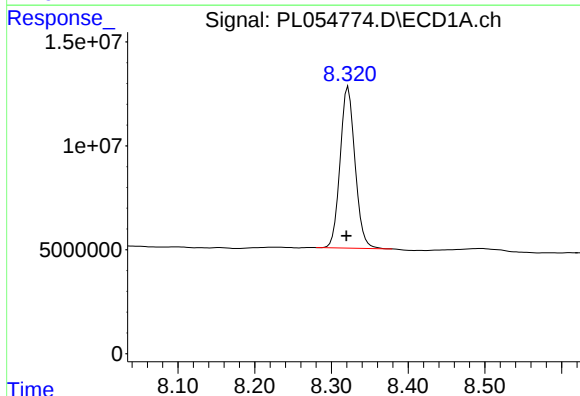

#28 Decachlorobiphenyl

R.T.: 8.322 min
Delta R.T.: 0.002 min
Response: 104847497
Conc: 10.95 ng/ml

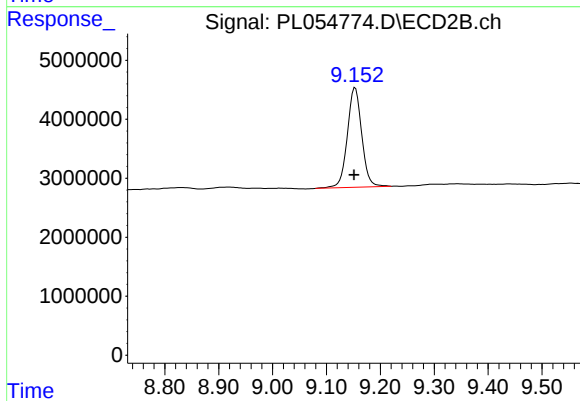

#28 Decachlorobiphenyl

R.T.: 9.153 min
Delta R.T.: 0.002 min
Response: 31420901
Conc: 13.11 ng/ml