

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120420\
 Data File : PL063358.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2020 18:38
 Operator : DD\AJ
 Sample : L4950-01 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 00:15:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 24 01:53:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	3.950	0	4487927	N.D.	1.375 #
Target Compounds							
6)	B beta-BHC	0.000	4.801	0	26998097	N.D.	13.241 #
8)	B Heptachlo...	0.000	5.827f	0	22512203	N.D.	6.463 #
9)	A Endosulfan I	5.458f	0.000	13008924	0	7.685	N.D. #
10)	B gamma-Chl...	0.000	6.039	0	14841549	N.D.	4.195 #
11)	B alpha-Chl...	0.000	6.118	0	23444329	N.D.	6.497 #
13)	MA Dieldrin	5.678	6.425	33014602	54473713	18.624	15.851
18)	B Endrin al...	6.384	0.000	4870434	0	3.269	N.D. #
19)	B Endosulfa...	6.599f	7.208	25273990	4400455	15.355	1.616 #
24)	Chlordane-2	4.777	0.000	11100594	0	199.670	N.D. #
25)	Chlordane-3	0.000	6.039	0	14841549	N.D.	33.466 #
26)	Chlordane-4	0.000	6.118	0	23444329	N.D.	43.711 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120420\
Data File : PL063358.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2020 18:38
Operator : DD\AJ
Sample : L4950-01 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 00:15:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
Quant Title : GC Extractables
QLast Update : Tue Nov 24 01:53:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

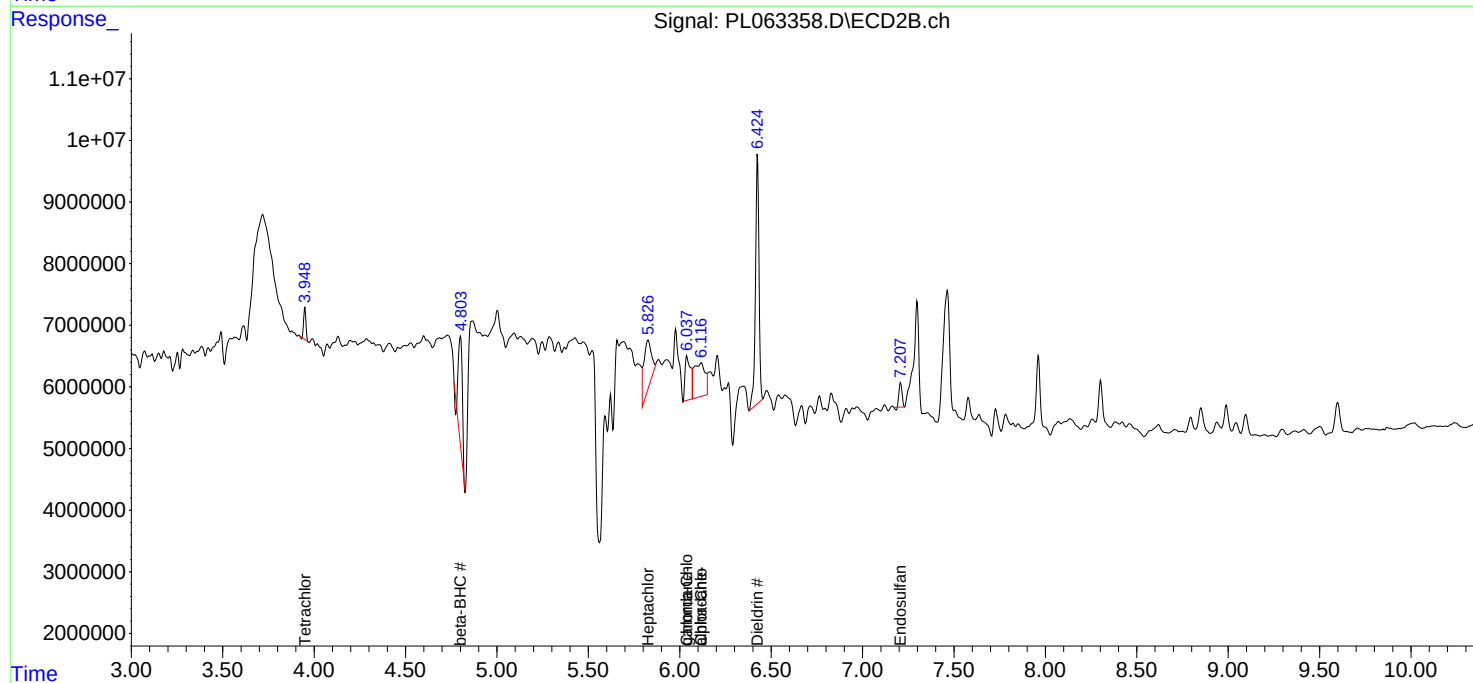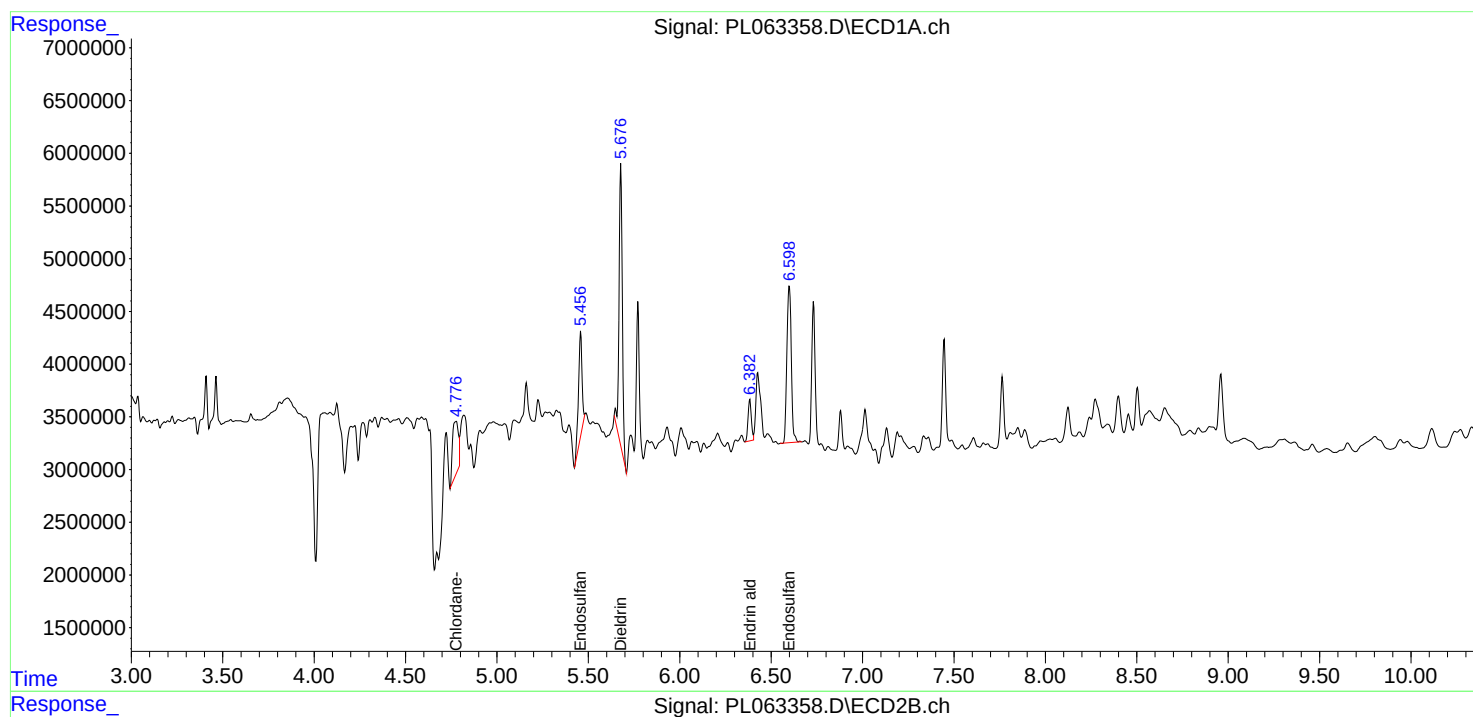


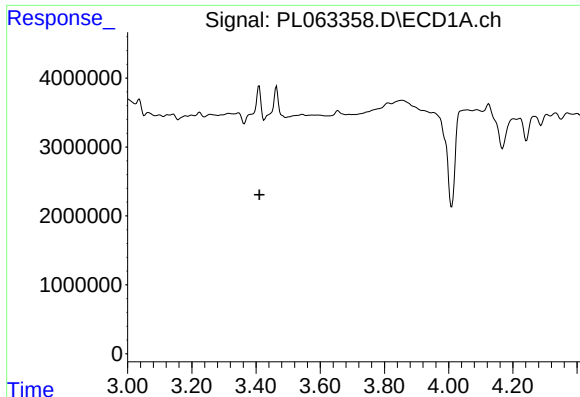

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.410 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

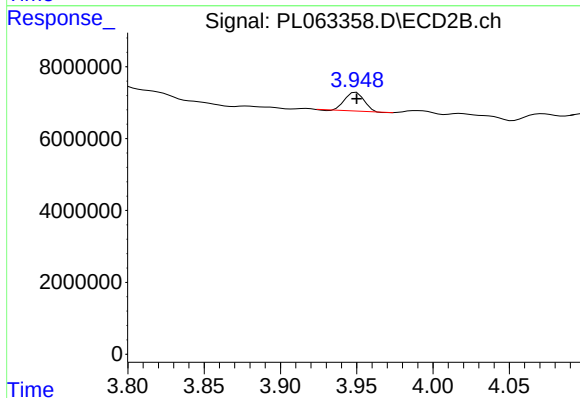


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 4487927
Conc: 1.38 ng/ml

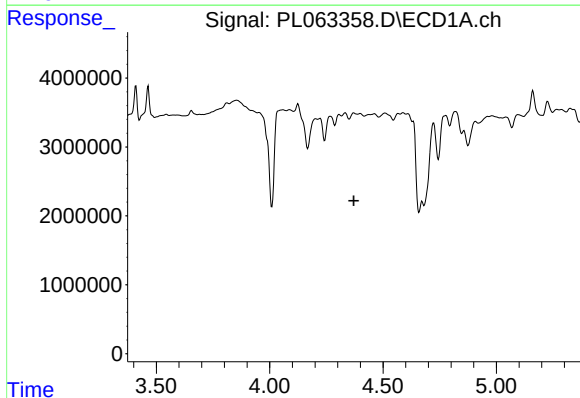


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.371 min
Response: 0
Conc: N.D.

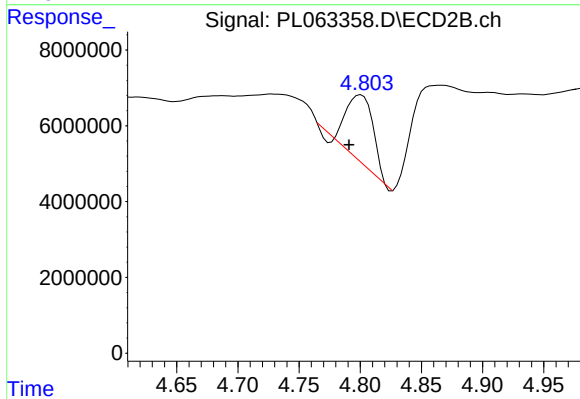

#6 beta-BHC


R.T.: 4.801 min
Delta R.T.: 0.010 min
Response: 26998097
Conc: 13.24 ng/ml

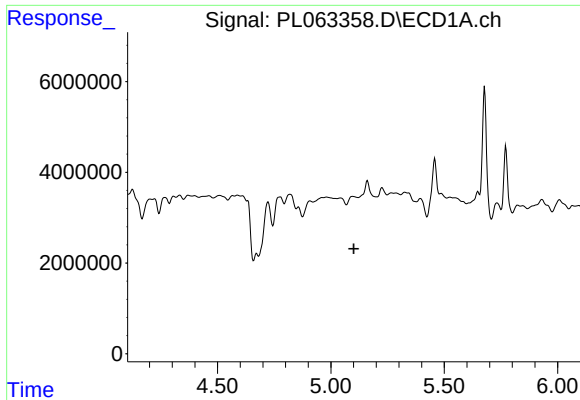

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.101 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

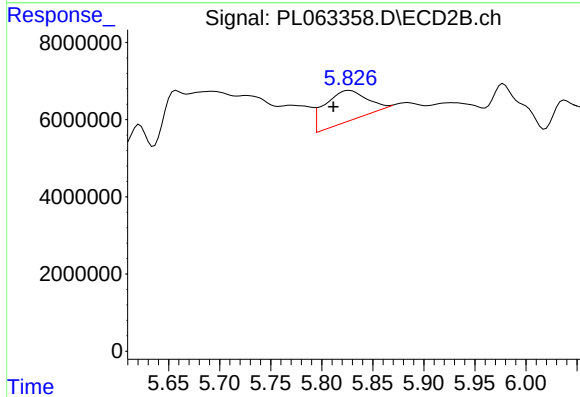


#8 Heptachlor epoxide

R.T.: 5.827 min
Delta R.T.: 0.016 min
Response: 22512203
Conc: 6.46 ng/ml

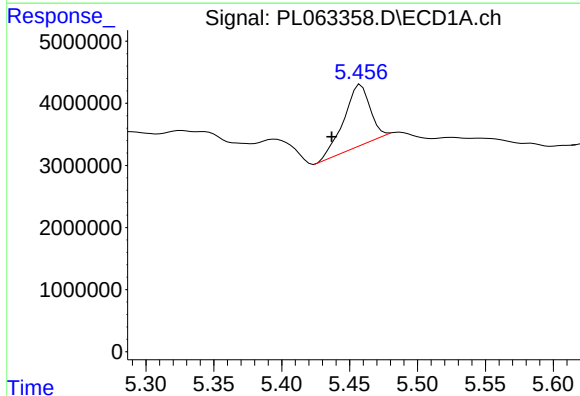


#9 Endosulfan I

R.T.: 5.458 min
Delta R.T.: 0.021 min
Response: 13008924
Conc: 7.68 ng/ml

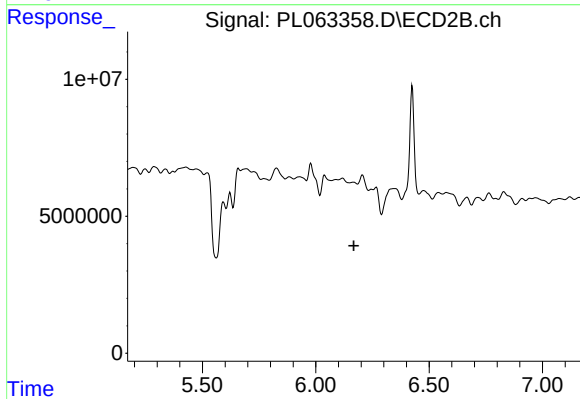

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.167 min
Response: 0
Conc: N.D.

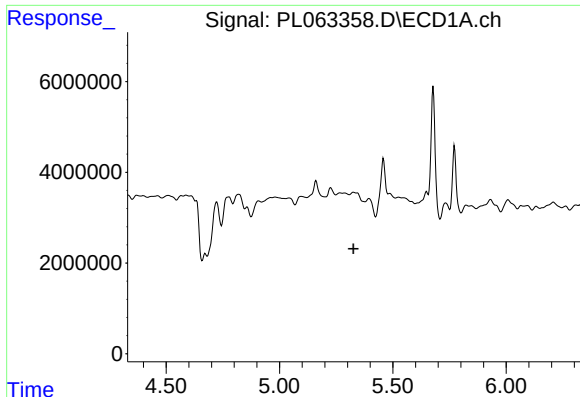

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.327 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

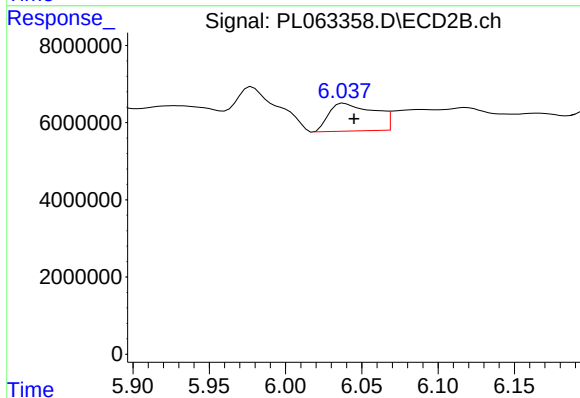


#10 gamma-Chlordane

R.T.: 6.039 min
Delta R.T.: -0.006 min
Response: 14841549
Conc: 4.19 ng/ml

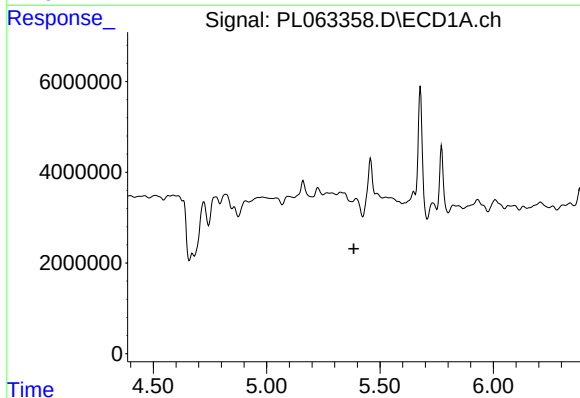


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.384 min
Response: 0
Conc: N.D.

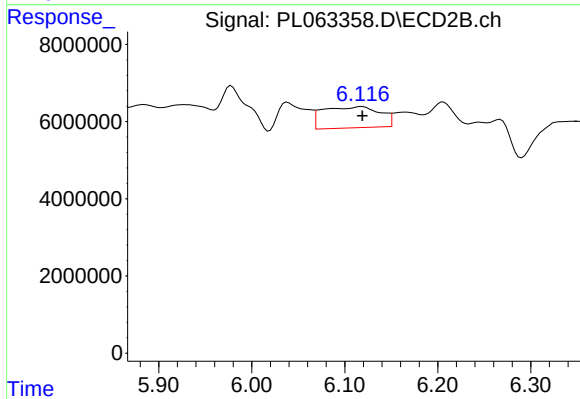

#11 alpha-Chlordane


R.T.: 6.118 min
Delta R.T.: 0.000 min
Response: 23444329
Conc: 6.50 ng/ml

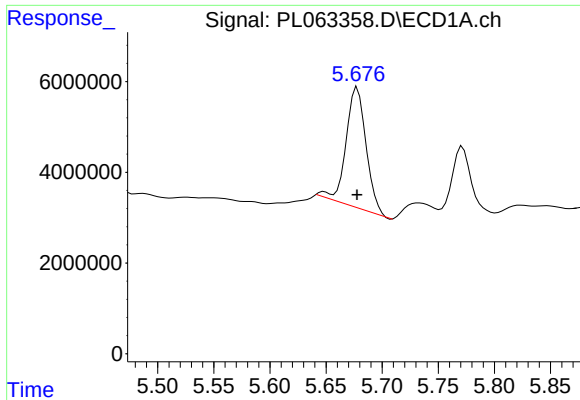

#13 Dieldrin


R.T.: 5.678 min
Delta R.T.: 0.000 min
Response: 33014602
Conc: 18.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

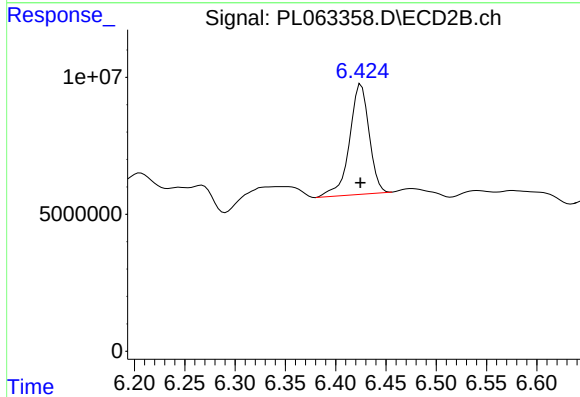


#13 Dieldrin

R.T.: 6.425 min
Delta R.T.: 0.000 min
Response: 54473713
Conc: 15.85 ng/ml

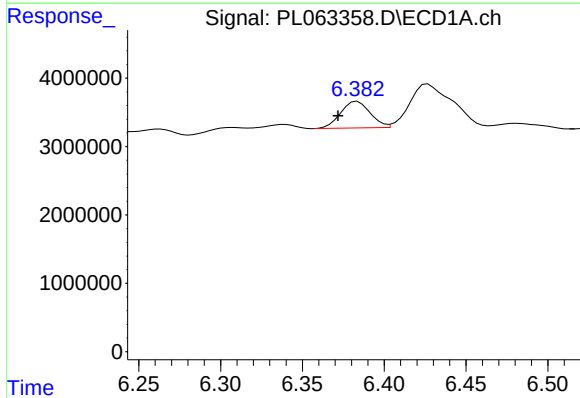


#18 Endrin aldehyde

R.T.: 6.384 min
Delta R.T.: 0.012 min
Response: 4870434
Conc: 3.27 ng/ml

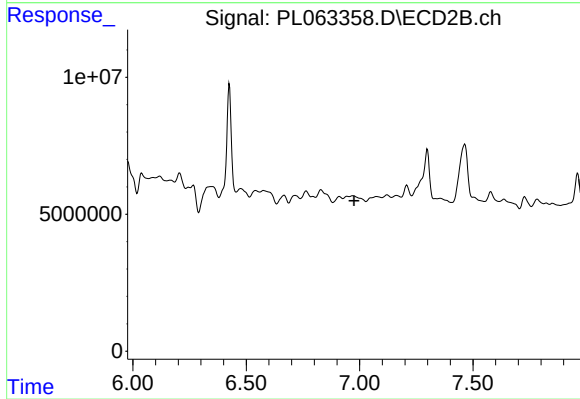

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.976 min
Response: 0
Conc: N.D.

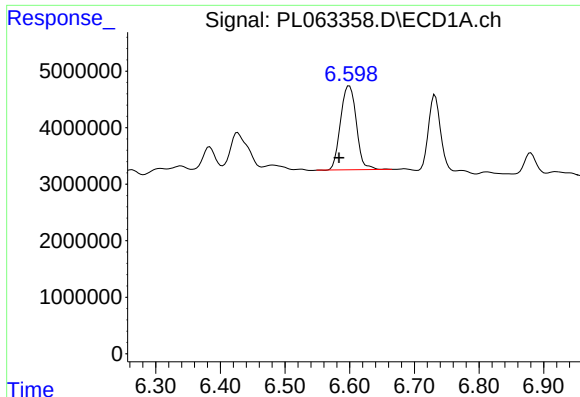

#19 Endosulfan Sulfate


R.T.: 6.599 min
Delta R.T.: 0.016 min
Response: 25273990
Conc: 15.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

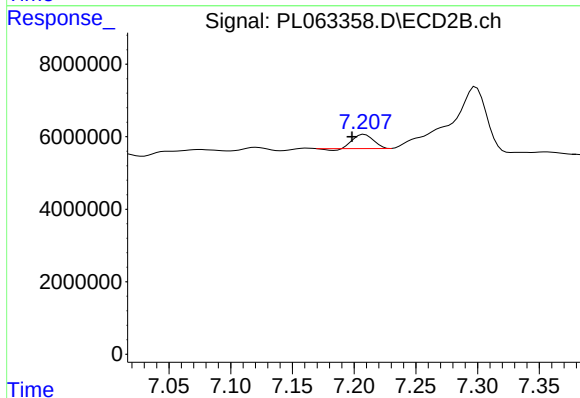


#19 Endosulfan Sulfate

R.T.: 7.208 min
Delta R.T.: 0.010 min
Response: 4400455
Conc: 1.62 ng/ml

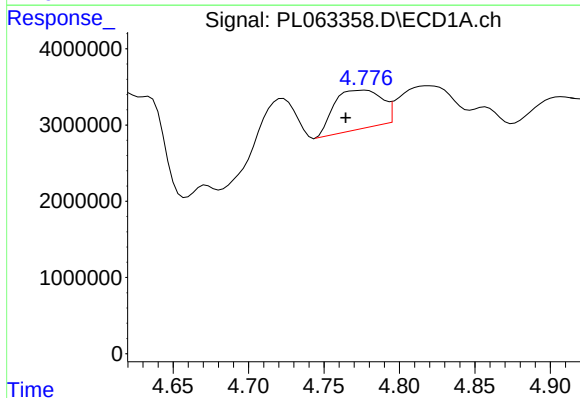


#24 Chlordane-2

R.T.: 4.777 min
Delta R.T.: 0.013 min
Response: 11100594
Conc: 199.67 ng/ml

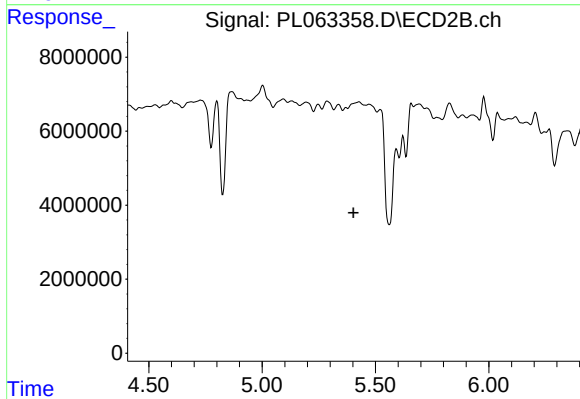

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.403 min
Response: 0
Conc: N.D.

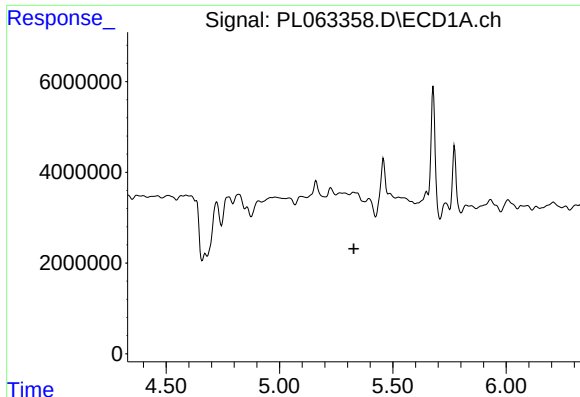

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

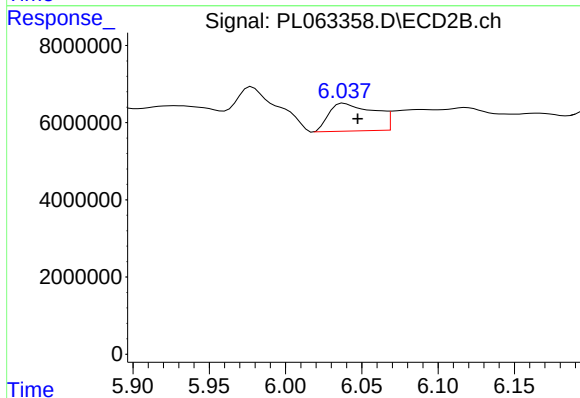


#25 Chlordane-3

R.T.: 6.039 min
Delta R.T.: -0.009 min
Response: 14841549
Conc: 33.47 ng/ml

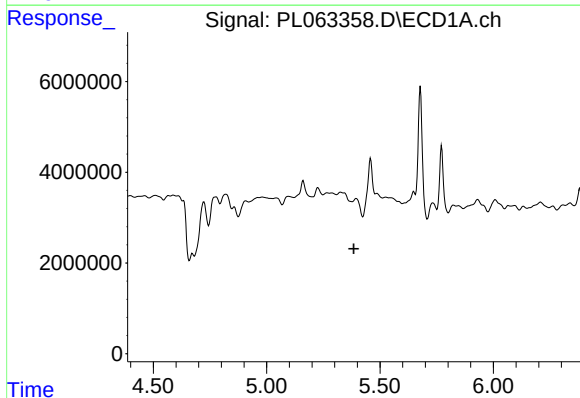


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.385 min
Response: 0
Conc: N.D.

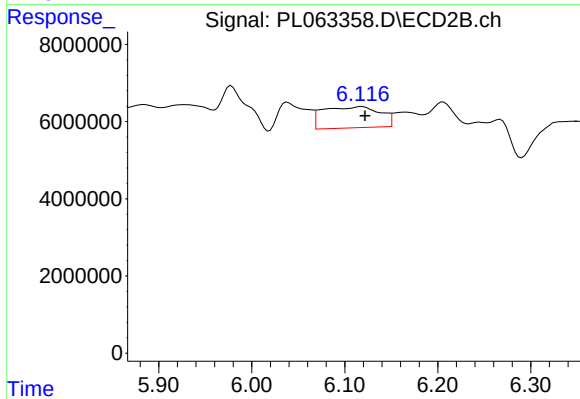

#26 Chlordane-4


R.T.: 6.118 min
Delta R.T.: -0.003 min
Response: 23444329
Conc: 43.71 ng/ml

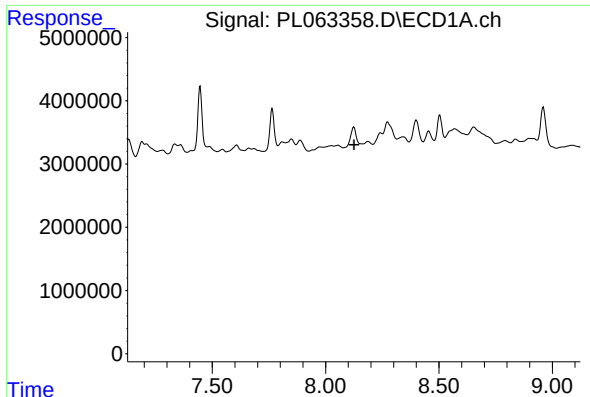

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.126 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

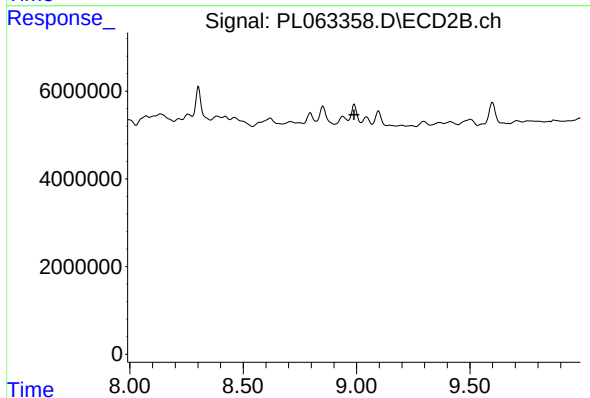

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.990 min
Response: 0
Conc: N.D.