

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120420\
 Data File : PL063354.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2020 17:26
 Operator : DD\AJ
 Sample : L4939-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EO-02-12320

Manual Integrations
 APPROVED

Ankita
 12/7/2020 1:34:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 00:15:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 24 01:53:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.950	23464128	41105696	13.777	12.595
28)	SA Decachlor...	8.127	8.991	26022764	35601484	13.935	14.963
Target Compounds							
12)	B 4,4'-DDE	5.549	6.271	2656053	4756148	1.603m	1.356m
17)	MA 4,4'-DDT	6.298	7.066	1013375	1534186	0.753m	0.601m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120420\
Data File : PL063354.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2020 17:26
Operator : DD\AJ
Sample : L4939-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
EO-02-12320


Manual Integrations
APPROVED

Ankita
12/7/2020 1:34:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 00:15:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
Quant Title : GC Extractables
QLast Update : Tue Nov 24 01:53:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

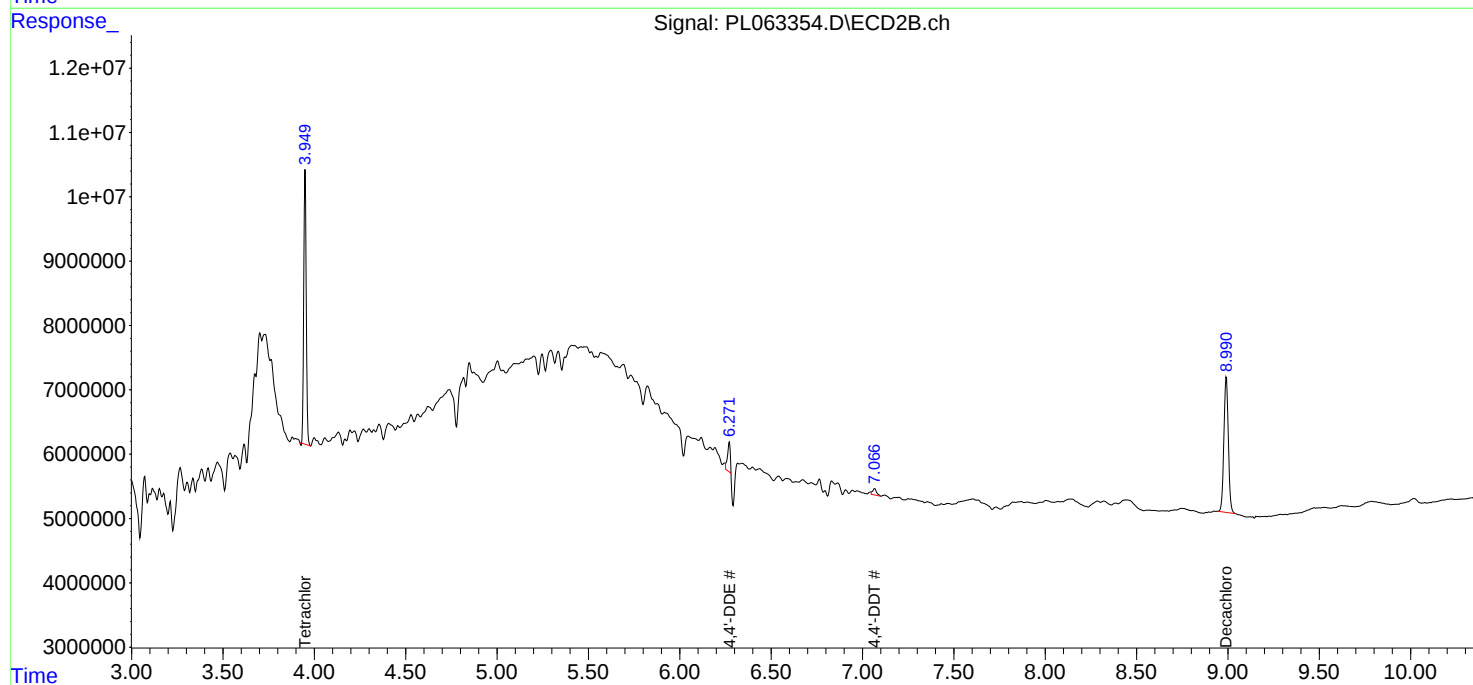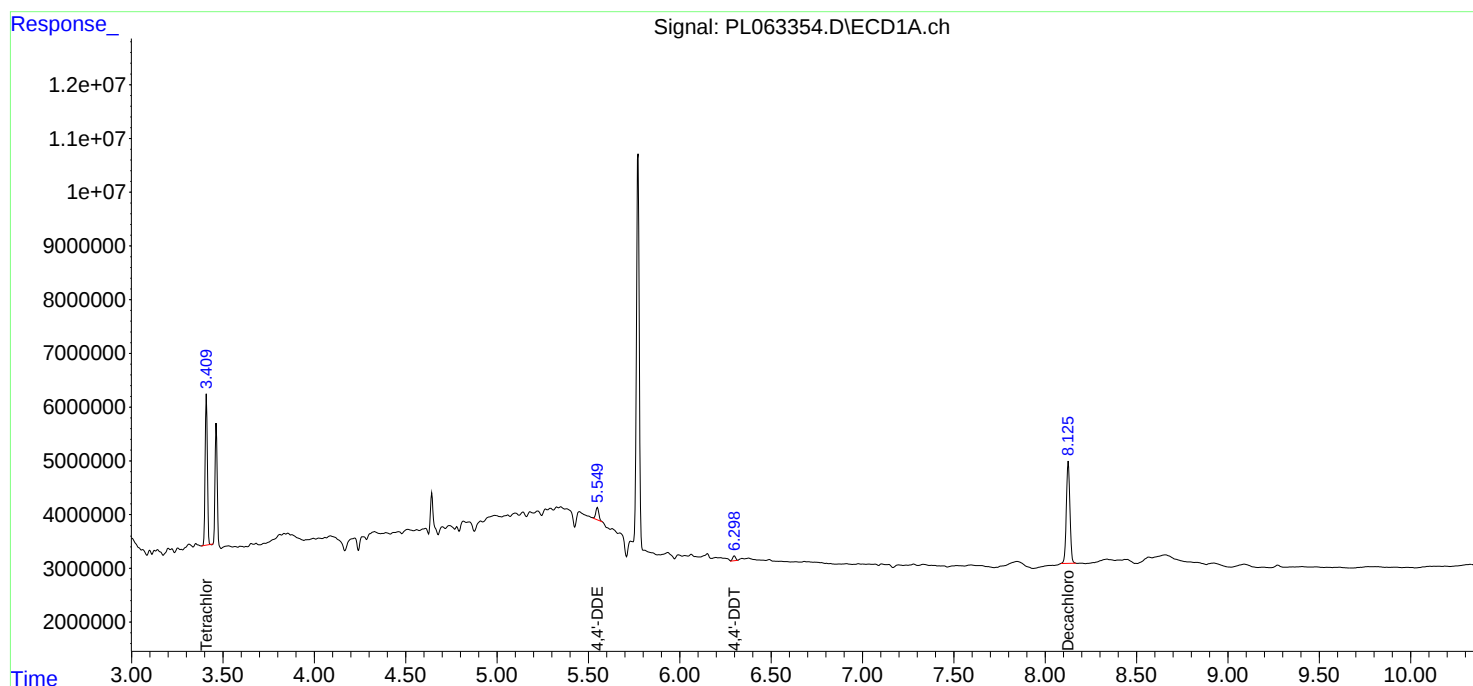

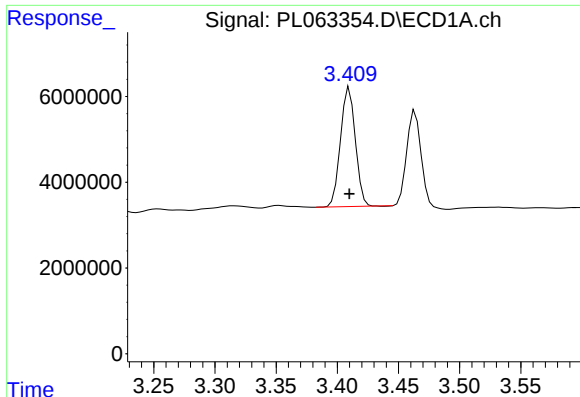


#1 Tetrachloro-m-xylene

R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 23464128
Conc: 13.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-12320


Manual Integrations
APPROVED

Ankita
12/7/2020 1:34:12 PM

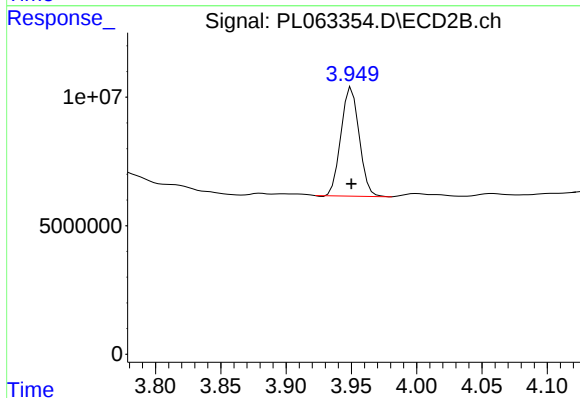


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 41105696
Conc: 12.59 ng/ml

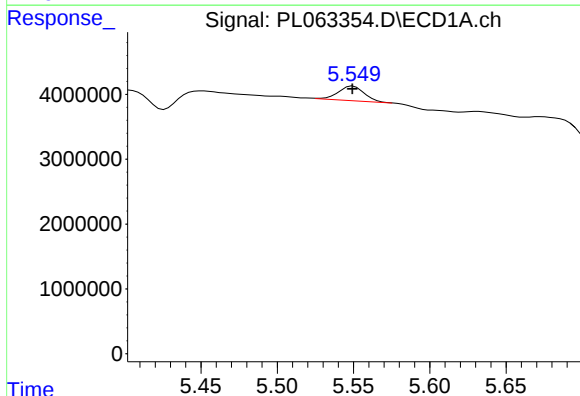


#12 4,4'-DDE

R.T.: 5.549 min
Delta R.T.: 0.000 min
Response: 2656053
Conc: 1.60 ng/ml m

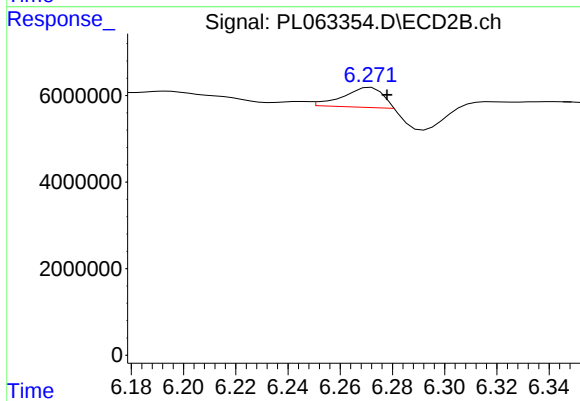

#12 4,4'-DDE

R.T.: 6.271 min
Delta R.T.: -0.007 min
Response: 4756148
Conc: 1.36 ng/ml m

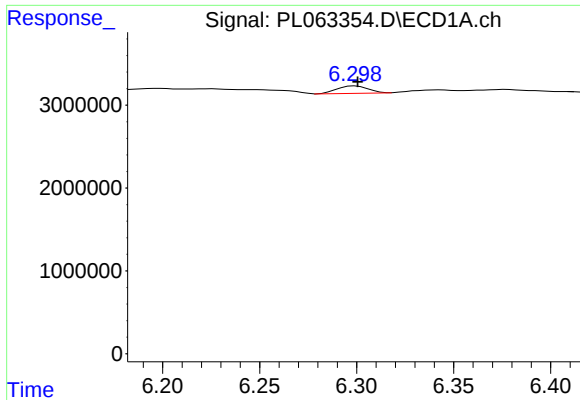


#17 4,4'-DDT

R.T.: 6.298 min
Delta R.T.: -0.003 min
Response: 1013375
Conc: 0.75 ng/ml m

Instrument :
ECD_L
ClientSampleId :
EO-02-12320


Manual Integrations
APPROVED

Ankita
12/7/2020 1:34:12 PM

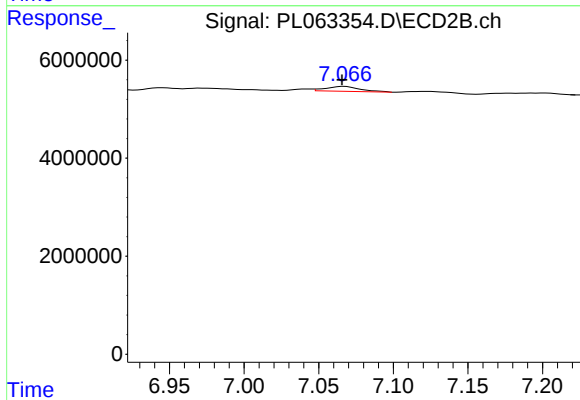


#17 4,4'-DDT

R.T.: 7.066 min
Delta R.T.: 0.000 min
Response: 1534186
Conc: 0.60 ng/ml m

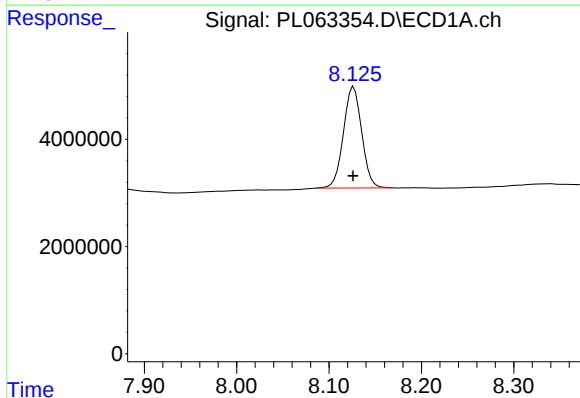

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 26022764
Conc: 13.93 ng/ml

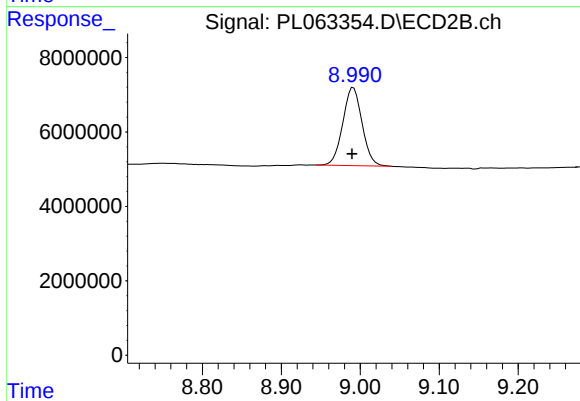

#28 Decachlorobiphenyl

R.T.: 8.991 min
Delta R.T.: 0.002 min
Response: 35601484
Conc: 14.96 ng/ml