

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120423\
 Data File : PL086947.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2023 14:16
 Operator : AR\AJ
 Sample : 05599-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LKWD-BACKFILL-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 20:28:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112923.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 29 06:35:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.342	2.610	67963187	18584696	21.258	20.434
28)	SA Decachlor...	8.843	7.760	62523658	24652038	23.420	22.359

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120423\
Data File : PL086947.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2023 14:16
Operator : AR\AJ
Sample : 05599-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
LKWD-BACKFILL-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 20:28:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112923.M
Quant Title : GC Extractables
QLast Update : Wed Nov 29 06:35:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

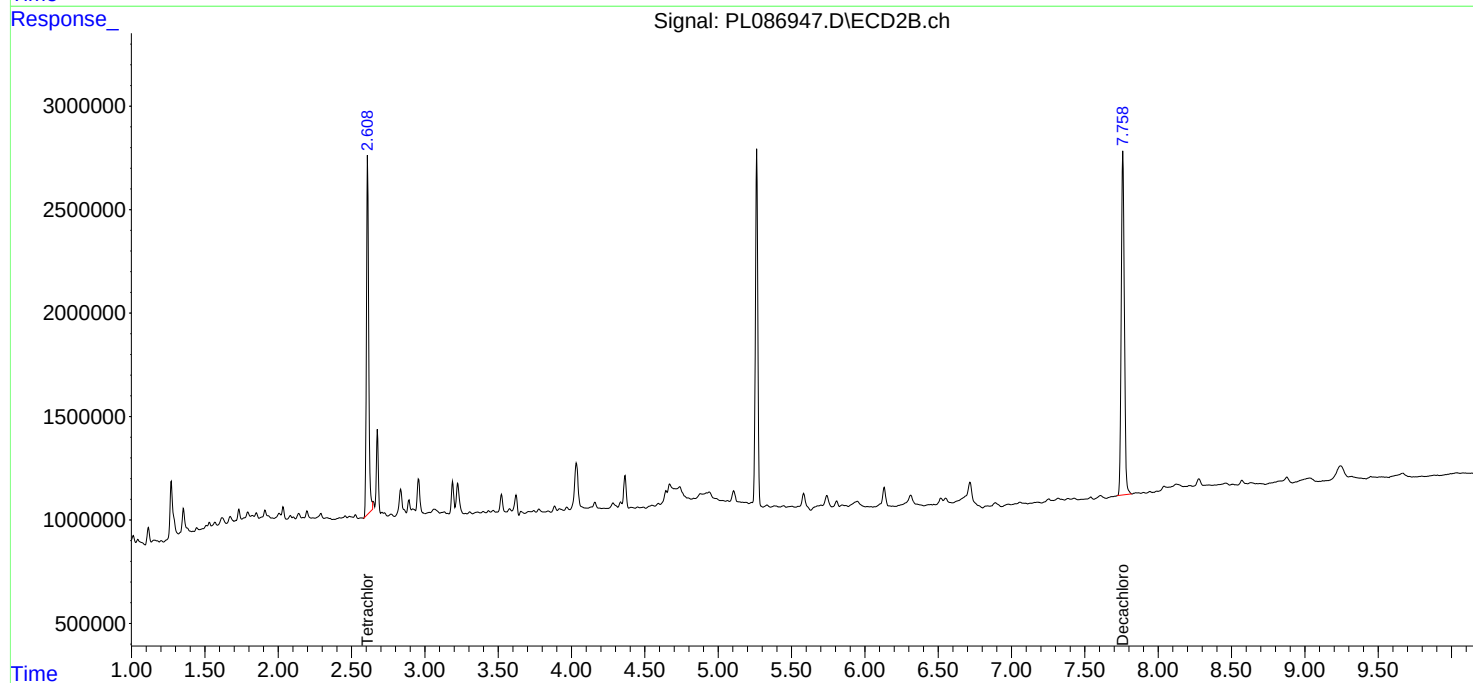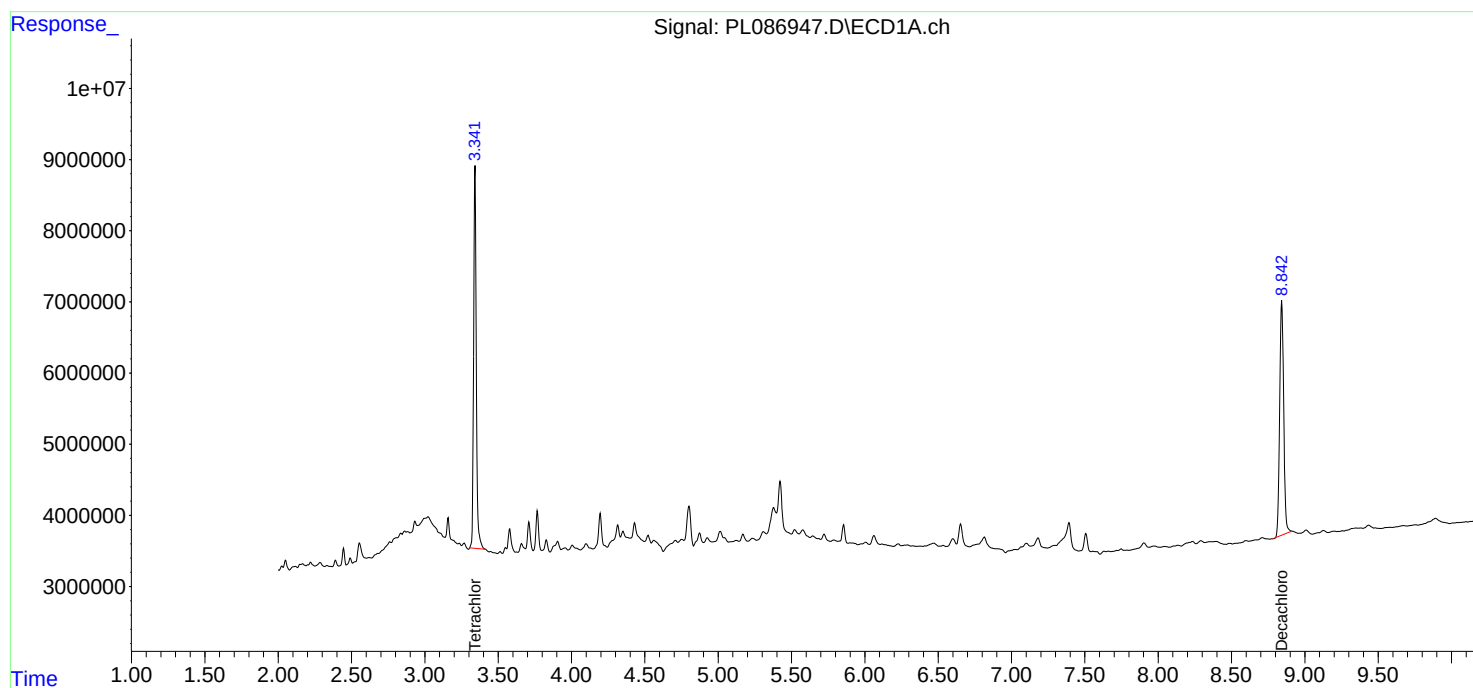


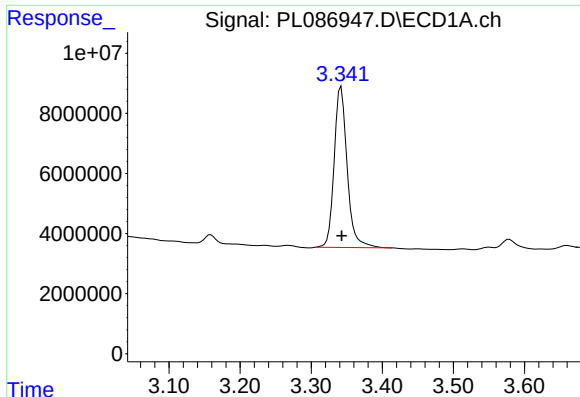

#1 Tetrachloro-m-xylene


R.T.: 3.342 min
Delta R.T.: 0.000 min
Response: 67963187
Conc: 21.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
LKWD-BACKFILL-03

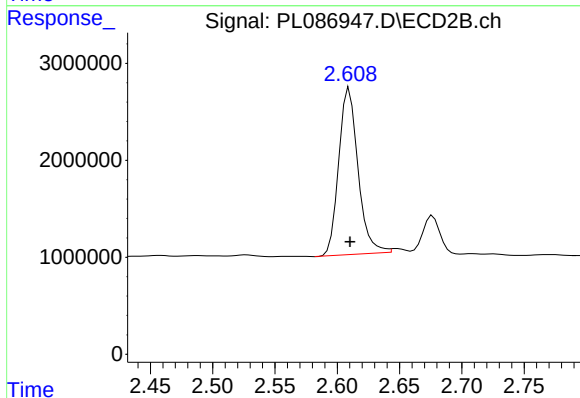


#1 Tetrachloro-m-xylene

R.T.: 2.610 min
Delta R.T.: 0.000 min
Response: 18584696
Conc: 20.43 ng/ml

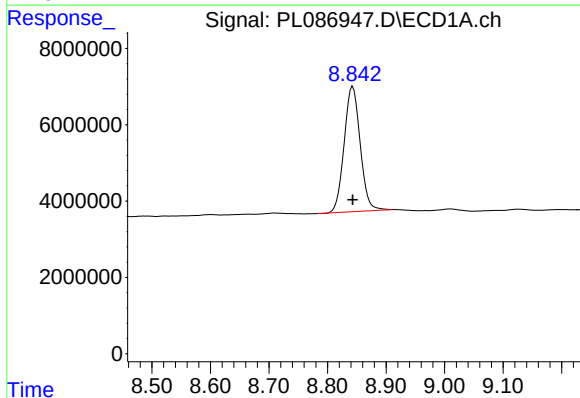

#28 Decachlorobiphenyl

R.T.: 8.843 min
Delta R.T.: 0.000 min
Response: 62523658
Conc: 23.42 ng/ml

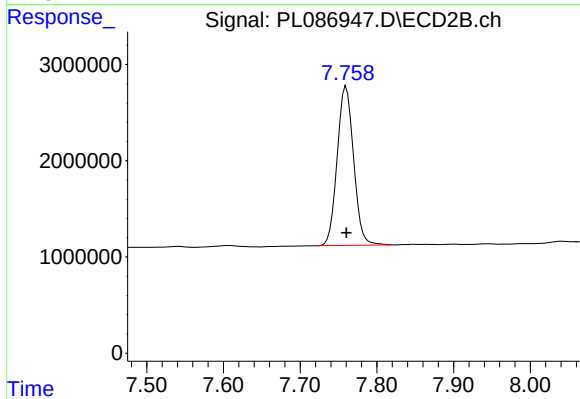

#28 Decachlorobiphenyl

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 24652038
Conc: 22.36 ng/ml