

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120423\
 Data File : PL086958.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2023 17:04
 Operator : AR\AJ
 Sample : 05599-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LKWD-BACKFILL-08

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 20:34:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112923.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 29 06:35:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.342	2.610	63631984	17934630	19.903	19.720
28)	SA Decachlor...	8.844	7.760	60511428	23961308	22.667	21.732

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120423\
Data File : PL086958.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2023 17:04
Operator : AR\AJ
Sample : 05599-15
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
LKWD-BACKFILL-08

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 20:34:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112923.M
Quant Title : GC Extractables
QLast Update : Wed Nov 29 06:35:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

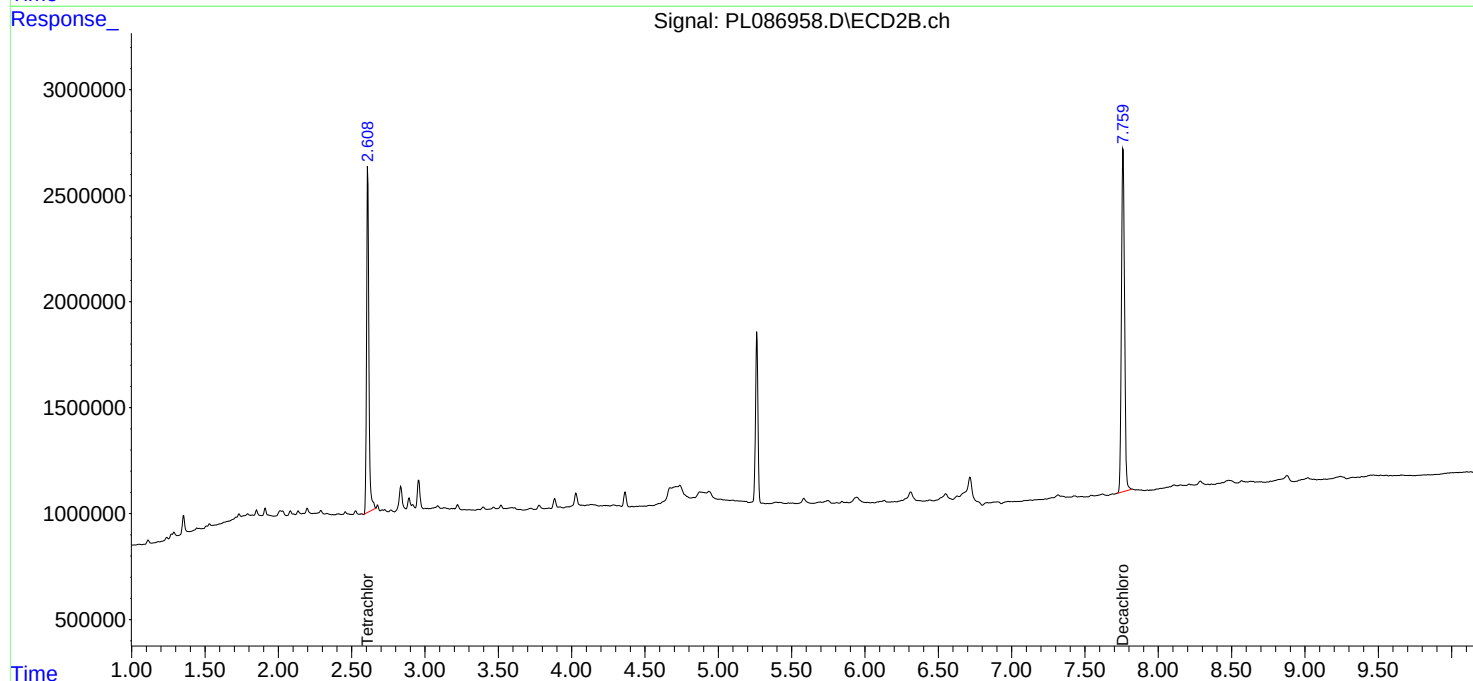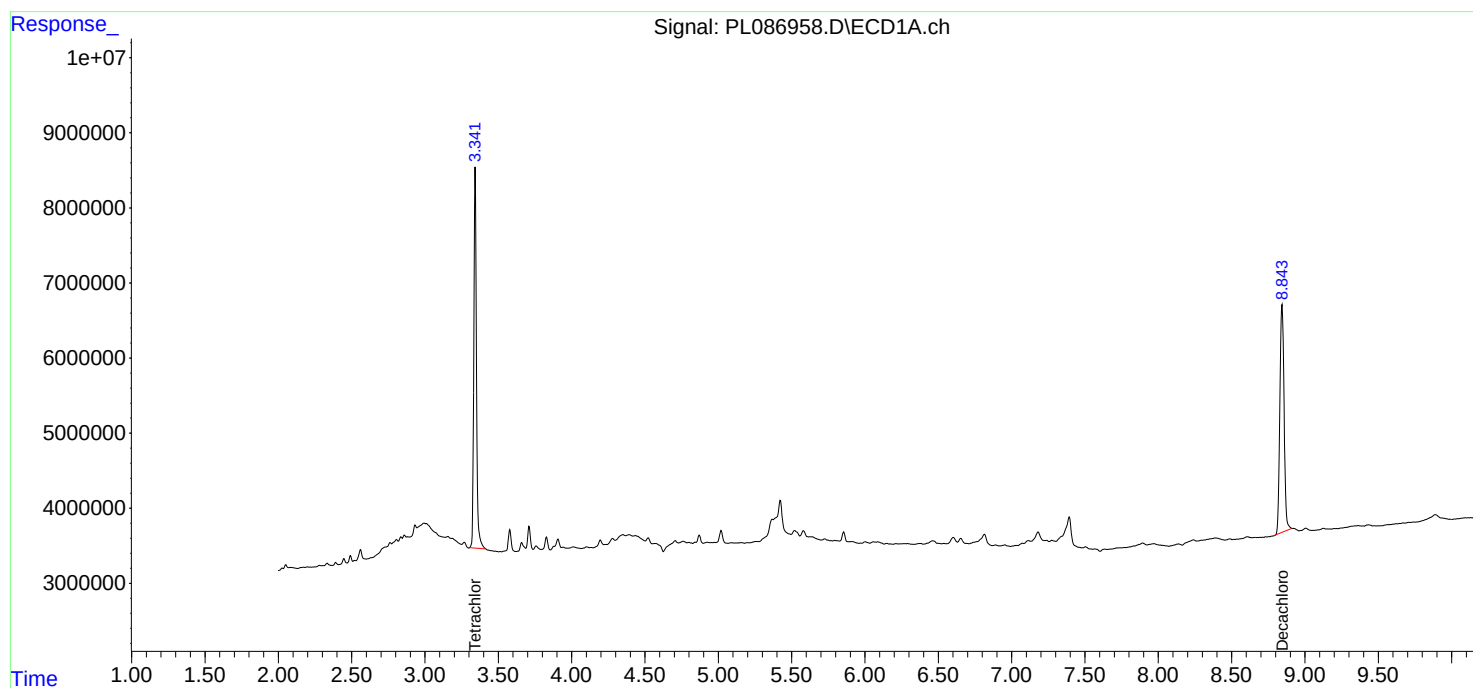


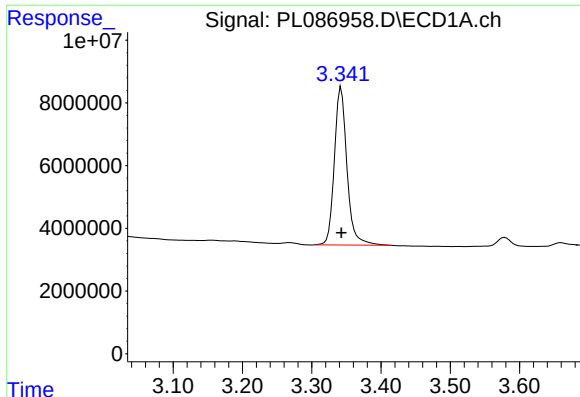

#1 Tetrachloro-m-xylene


R.T.: 3.342 min
Delta R.T.: 0.000 min
Response: 63631984
Conc: 19.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
LKWD-BACKFILL-08

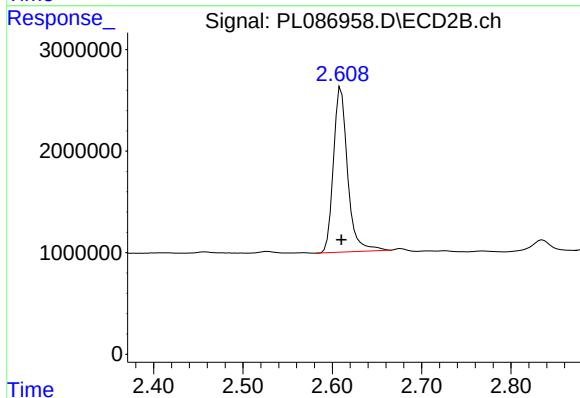


#1 Tetrachloro-m-xylene

R.T.: 2.610 min
Delta R.T.: 0.000 min
Response: 17934630
Conc: 19.72 ng/ml

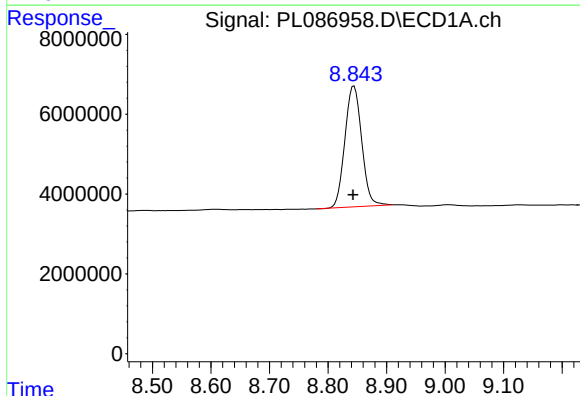

#28 Decachlorobiphenyl

R.T.: 8.844 min
Delta R.T.: 0.002 min
Response: 60511428
Conc: 22.67 ng/ml

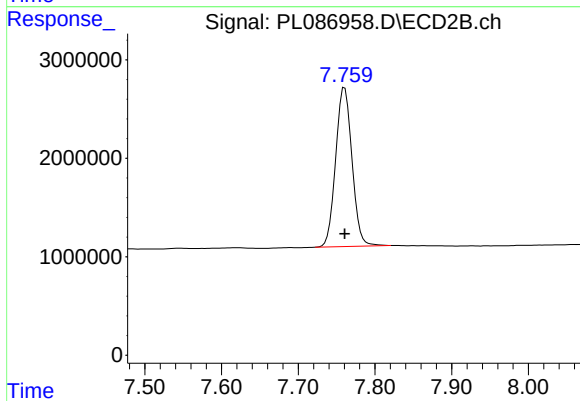

#28 Decachlorobiphenyl

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 23961308
Conc: 21.73 ng/ml