

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120423\
 Data File : PL086977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2023 22:12
 Operator : AR\AJ
 Sample : 05612-05
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MW-06S

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/05/2023
 Supervised By :Ankita Jodhani 12/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 00:41:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112923.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 29 06:35:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.342	2.609	42283416	15829466	13.225	17.405m#
28) SA Decachlor...	8.843	7.761	48917125	19794974	18.324	17.953

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120423\
Data File : PL086977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2023 22:12
Operator : AR\AJ
Sample : 05612-05
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MW-06S


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/05/2023
Supervised By :Ankita Jodhani 12/05/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 00:41:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112923.M
Quant Title : GC Extractables
QLast Update : Wed Nov 29 06:35:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

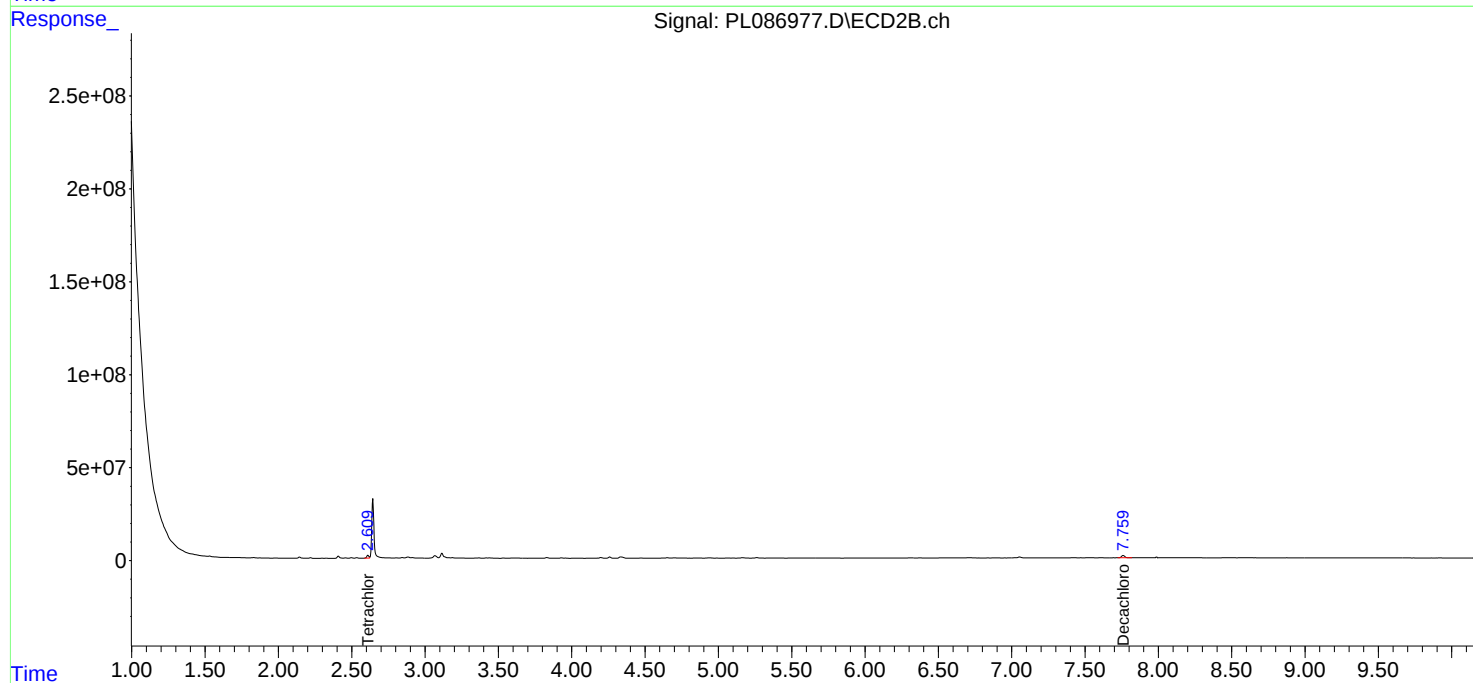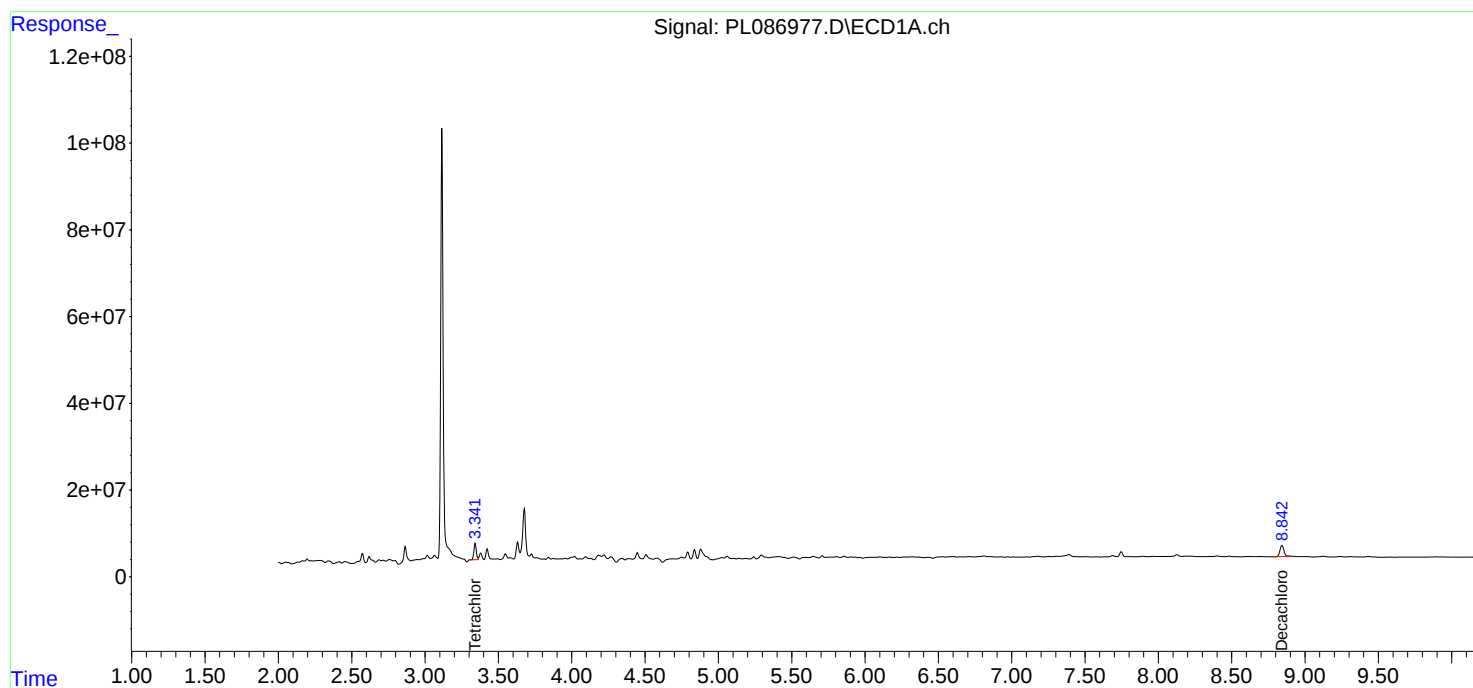

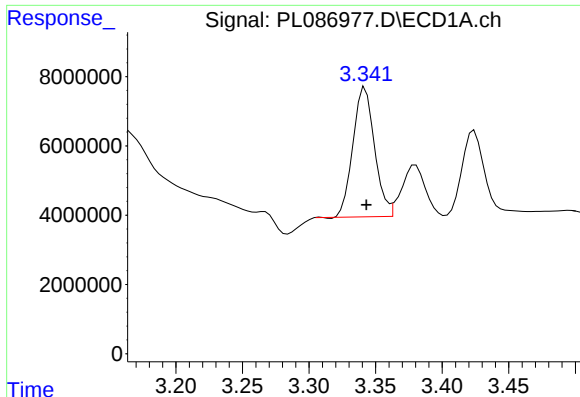


#1 Tetrachloro-m-xylene

R.T.: 3.342 min
Delta R.T.: 0.000 min
Response: 42283416
Conc: 13.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
MW-06S


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/05/2023
Supervised By :Ankita Jodhani 12/05/2023

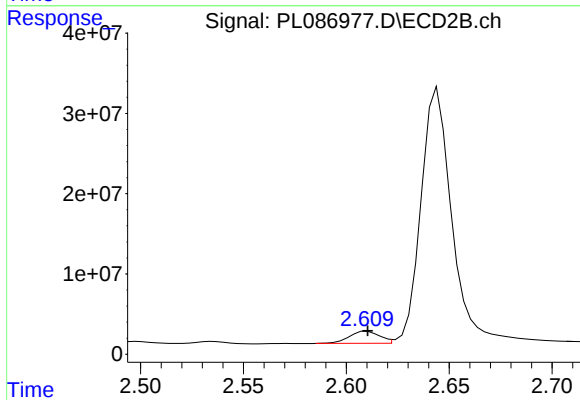


#1 Tetrachloro-m-xylene

R.T.: 2.609 min
Delta R.T.: -0.002 min
Response: 15829466
Conc: 17.40 ng/ml m

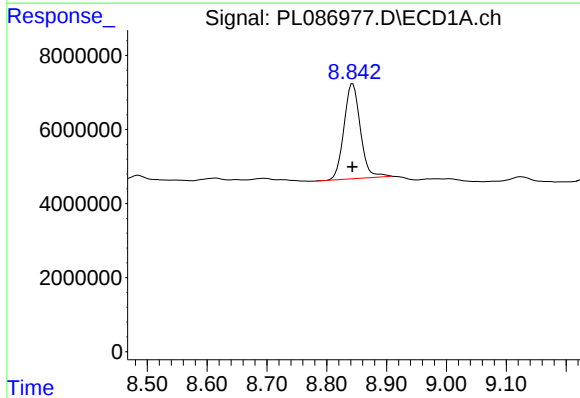

#28 Decachlorobiphenyl

R.T.: 8.843 min
Delta R.T.: 0.000 min
Response: 48917125
Conc: 18.32 ng/ml

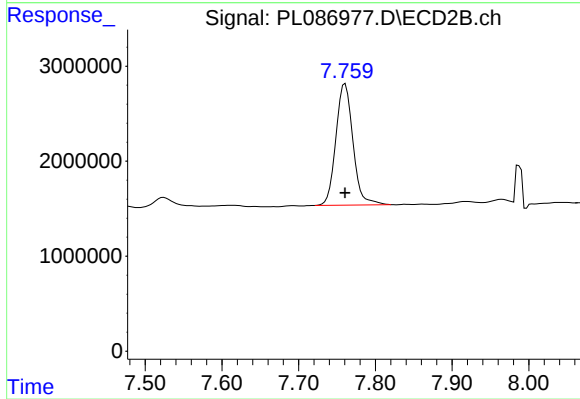

#28 Decachlorobiphenyl

R.T.: 7.761 min
Delta R.T.: 0.000 min
Response: 19794974
Conc: 17.95 ng/ml