

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120423\
 Data File : PL086978.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2023 22:26
 Operator : AR\AJ
 Sample : 05612-07
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DUP-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/05/2023
 Supervised By :Ankita Jodhani 12/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 00:41:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112923.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 29 06:35:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.343	2.609	43958567	16688494	13.749	18.349m#
28) SA Decachlor...	8.842	7.761	56702471	22861601	21.240	20.735

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120423\
Data File : PL086978.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2023 22:26
Operator : AR\AJ
Sample : 05612-07
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
DUP-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/05/2023
Supervised By :Ankita Jodhani 12/05/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 00:41:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112923.M
Quant Title : GC Extractables
QLast Update : Wed Nov 29 06:35:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

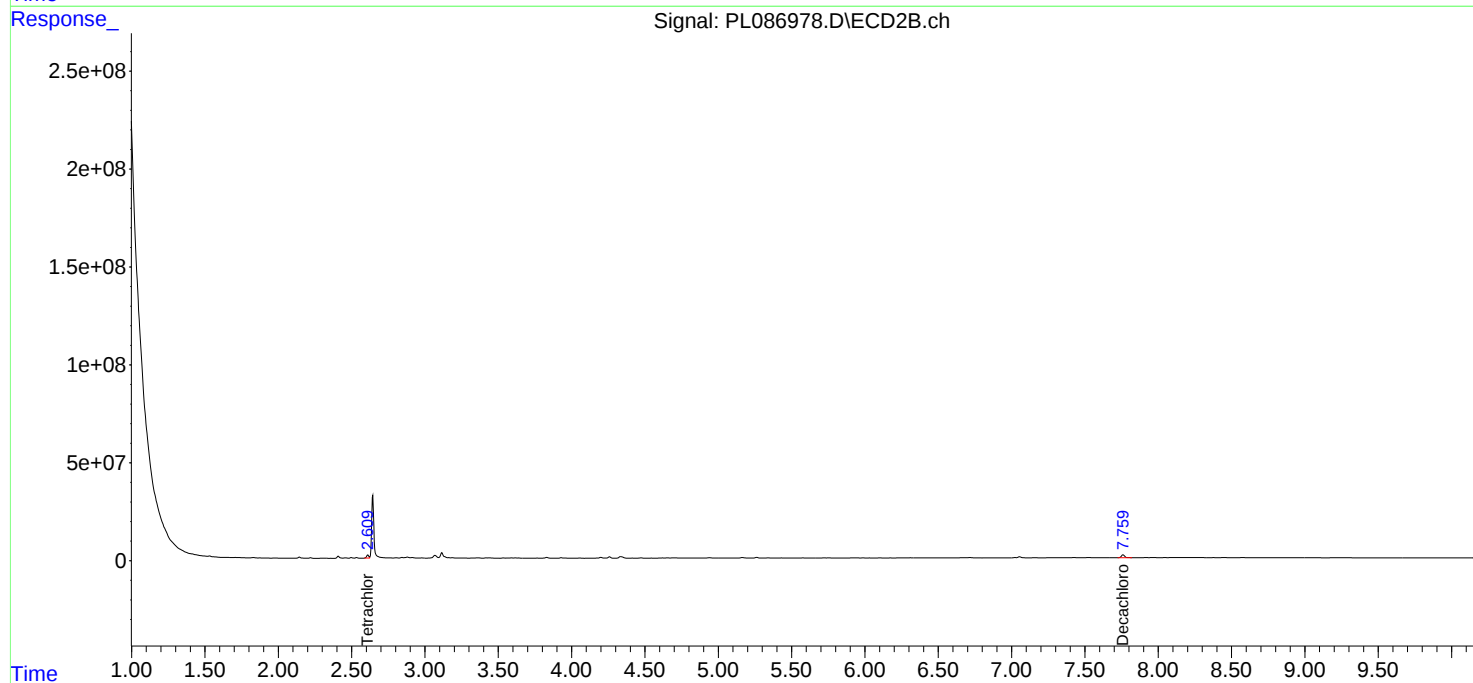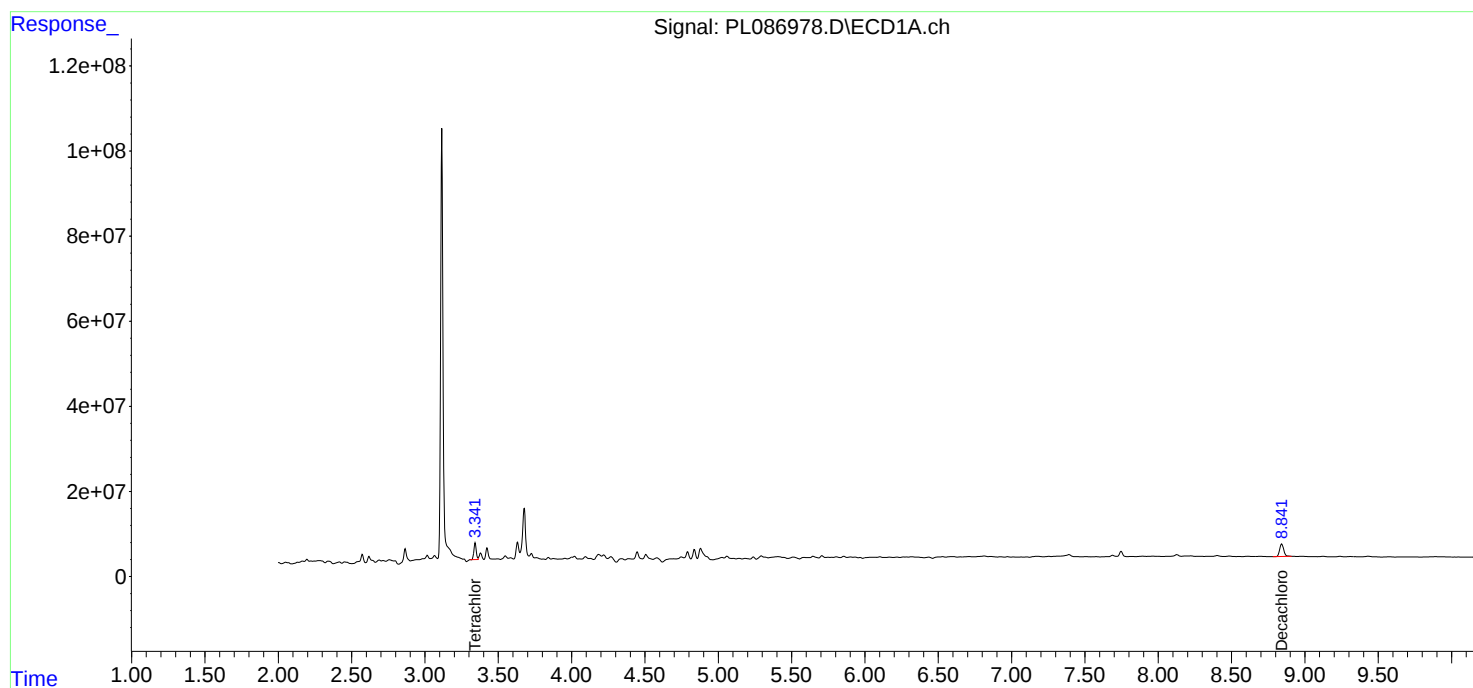

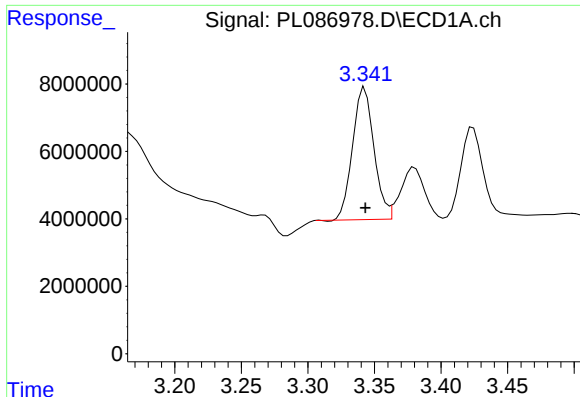


#1 Tetrachloro-m-xylene

R.T.: 3.343 min
Delta R.T.: 0.000 min
Response: 43958567
Conc: 13.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
DUP-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/05/2023
Supervised By :Ankita Jodhani 12/05/2023

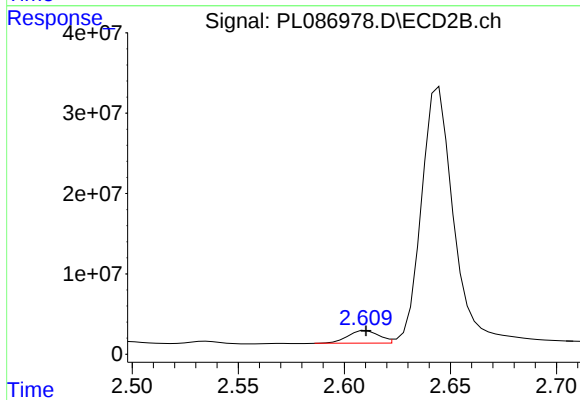


#1 Tetrachloro-m-xylene

R.T.: 2.609 min
Delta R.T.: -0.002 min
Response: 16688494
Conc: 18.35 ng/ml m

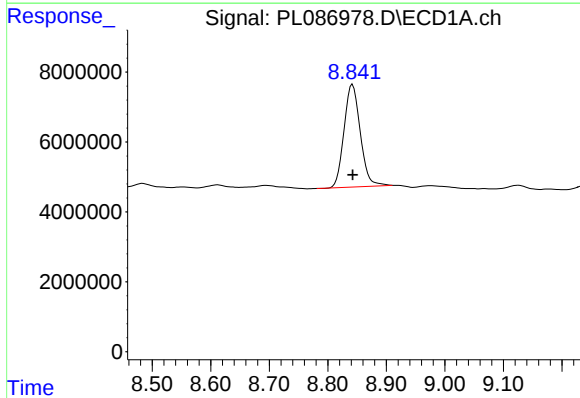

#28 Decachlorobiphenyl

R.T.: 8.842 min
Delta R.T.: 0.000 min
Response: 56702471
Conc: 21.24 ng/ml

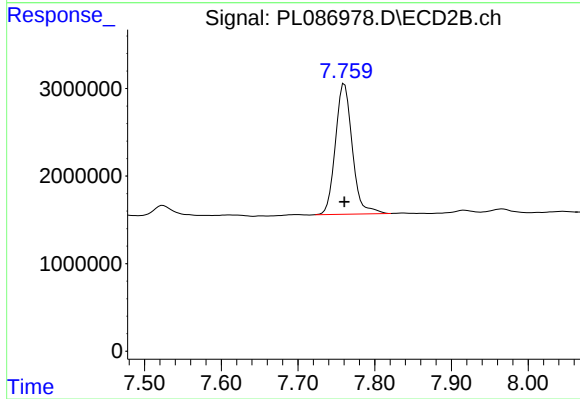

#28 Decachlorobiphenyl

R.T.: 7.761 min
Delta R.T.: 0.000 min
Response: 22861601
Conc: 20.73 ng/ml